

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
 Data File : VX029620.D
 Acq On : 20 Jun 2022 14:06
 Operator : JC/MD
 Sample : N3290-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-10DL

Quant Time: Jun 21 01:50:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	270003	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	458778	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	395214	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	172251	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	155817	43.596	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.200%
35) Dibromofluoromethane	5.391	113	135823	45.429	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.860%
50) Toluene-d8	8.653	98	516287	47.269	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.540%
62) 4-Bromofluorobenzene	11.079	95	188088	45.664	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.320%

Target Compounds			Qvalue			
3) Chloromethane	1.295	50	945	0.268	ug/l #	80
5) Bromomethane	1.618	94	705	0.426	ug/l #	62
6) Chloroethane	1.709	64	282	1.401	ug/l #	43
10) Methyl Iodide	2.459	142	553	3.178	ug/l #	84
11) Tert butyl alcohol	2.965	59	45314	50.806	ug/l	96
13) Acrolein	2.221	56	248	1.260	ug/l #	1
14) Allyl chloride	2.764	41	986	0.223	ug/l #	1
16) Acetone	2.380	43	2326	1.633	ug/l #	86
19) Methyl tert-butyl Ether	3.117	73	33789	3.558	ug/l	92
22) Diisopropyl ether	3.764	45	2700	0.309	ug/l #	94
23) Vinyl Acetate	3.764	43	1551	0.213	ug/l #	66
25) 2-Butanone	4.593	43	1306	0.580	ug/l #	78
31) Cyclohexane	5.471	56	9783	2.039	ug/l	96
36) 1,1-Dichloropropene	5.556	75	20105	4.968	ug/l #	50
38) Carbon Tetrachloride	5.556	117	28872	7.256	ug/l #	16
39) Methylcyclohexane	7.385	83	3332	0.660	ug/l	92
40) Benzene	6.044	78	390333	32.542	ug/l	99
42) 1,2-Dichloroethane	6.044	62	3546	0.860	ug/l #	73
44) Trichloroethene	7.135	130	2156	Below Cal		93
52) Toluene	8.720	92	24555	3.197	ug/l	99
59) 2-Hexanone	9.452	43	2091	0.664	ug/l	94
67) Ethyl Benzene	10.195	91	36460	2.614	ug/l	96
68) m/p-Xylenes	10.299	106	248857	45.743	ug/l	95
69) o-Xylene	10.647	106	18536	3.449	ug/l	98
73) Isopropylbenzene	10.964	105	51192	3.964	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	89761	23.920	ug/l #	38
78) n-propylbenzene	11.305	91	139262	9.574	ug/l	100
79) 2-Chlorotoluene	11.402	91	4397	0.488	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	29200	2.685	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	89761	79.577	ug/l #	15
82) 4-Chlorotoluene	11.402	91	4397	0.428	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.756	105	53899	4.969	ug/l	98
85) sec-Butylbenzene	11.890	105	4964	0.378	ug/l	96
89) n-Butylbenzene	12.335	91	6568	0.707	ug/l #	61
90) Hexachloroethane	12.646	117	6779	4.302	ug/l #	10
95) Naphthalene	13.774	128	158421	13.112	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
Data File : VX029620.D
Acq On : 20 Jun 2022 14:06
Operator : JC/MD
Sample : N3290-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10DL

Quant Time: Jun 21 01:50:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
Data File : VX029620.D
Acq On : 20 Jun 2022 14:06
Operator : JC/MD
Sample : N3290-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10DL

Quant Time: Jun 21 01:50:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




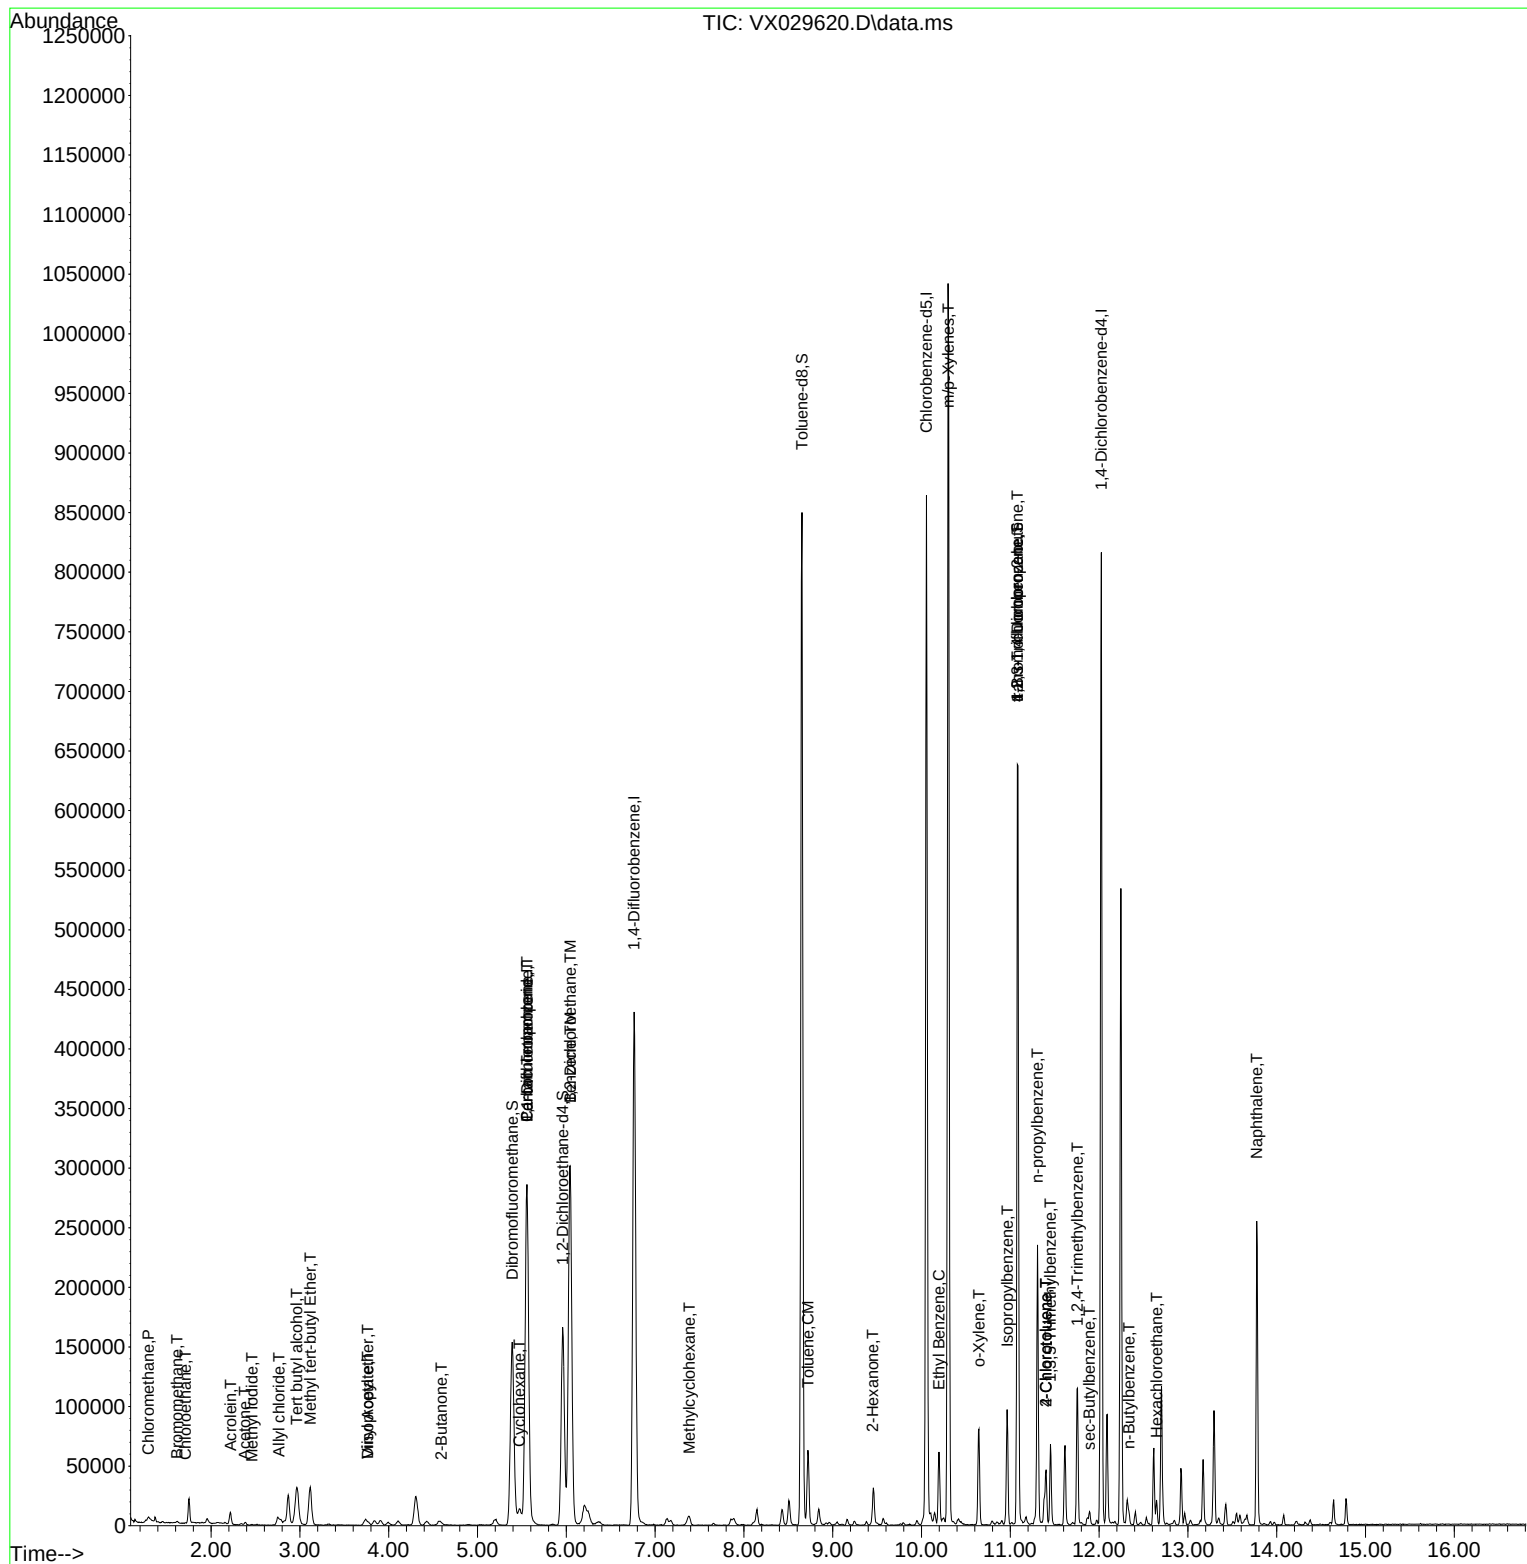




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion:168 Resp: 270003
Ion Ratio Lower Upper
168 100
99 58.2 41.7 62.5



#3
Chloromethane
Concen: 0.268 ug/l
RT: 1.295 min Scan# 34
Delta R.T. 0.007 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 50 Resp: 945
Ion Ratio Lower Upper
50 100
52 21.5 26.4 39.6#


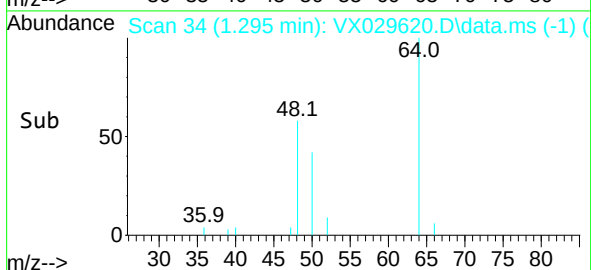

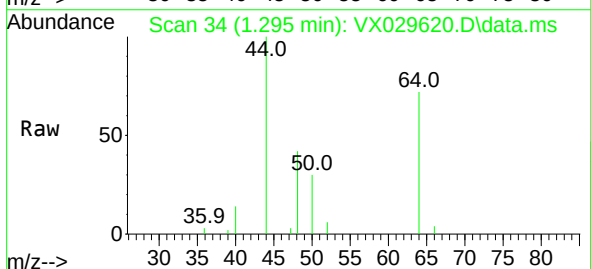


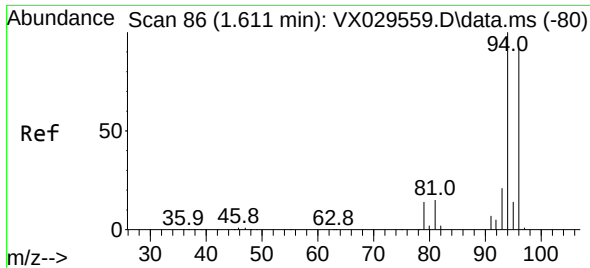

#5
Bromomethane
Concen: 0.426 ug/l
RT: 1.618 min Scan# 81
Delta R.T. 0.007 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 94 Resp: 705
Ion Ratio Lower Upper
94 100
96 131.2 75.3 112.9#

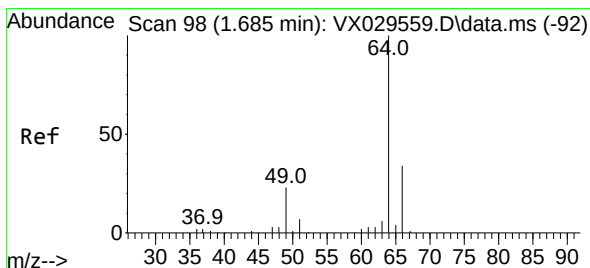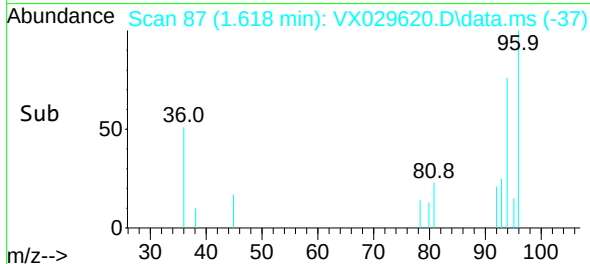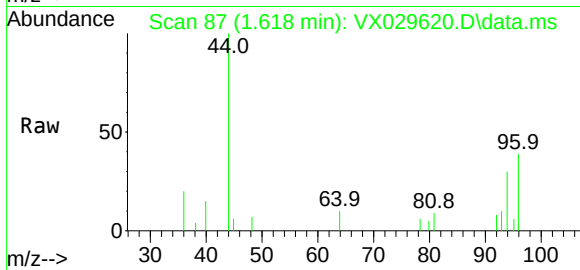

#6
Chloroethane
Concen: 1.401 ug/l
RT: 1.709 min Scan# 102
Delta R.T. 0.024 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 64 Resp: 282
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#


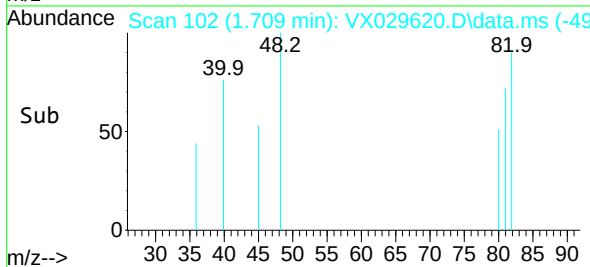

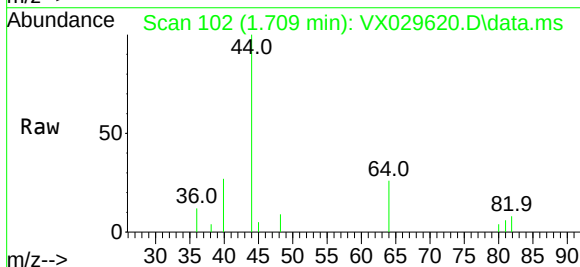


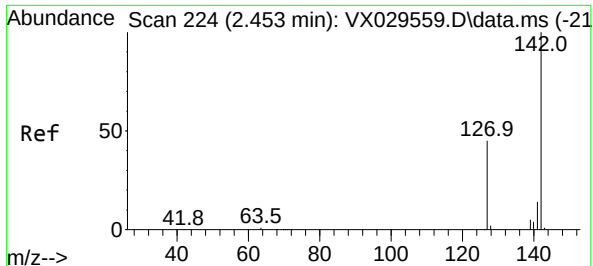

#10
Methyl Iodide
Concen: 3.178 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion:142 Resp: 553
Ion Ratio Lower Upper
142 100
127 51.5 33.9 50.9#
141 5.1 11.4 17.2#

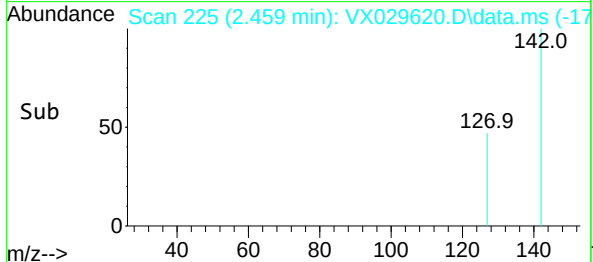

#11
Tert butyl alcohol
Concen: 50.806 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.018 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 59 Resp: 45314
Ion Ratio Lower Upper
59 100
57 8.9 8.3 12.5

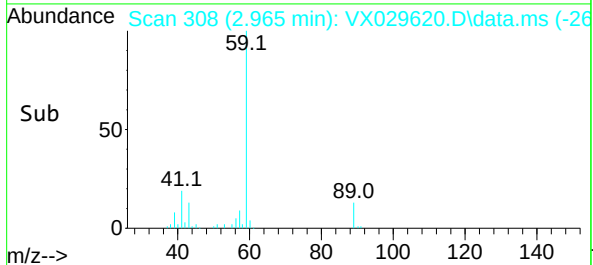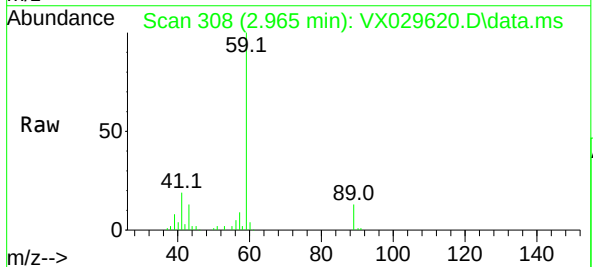

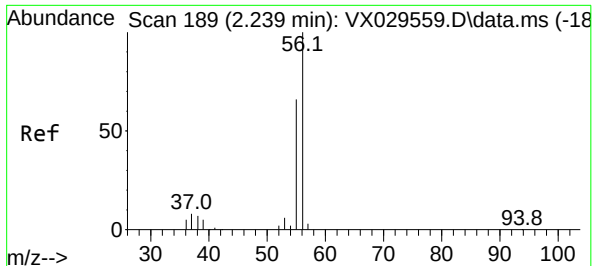

#13

Acrolein

Concen: 1.260 ug/l

RT: 2.221 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06

Instrument :

MSVOA_X

ClientSampleId :





MW-10DL

Tgt Ion: 56 Resp: 248

Ion Ratio Lower Upper

56 100

55 2248.8 55.0 82.6#

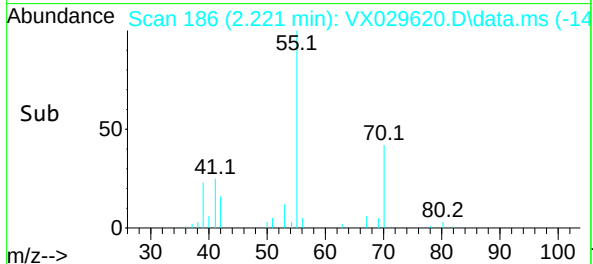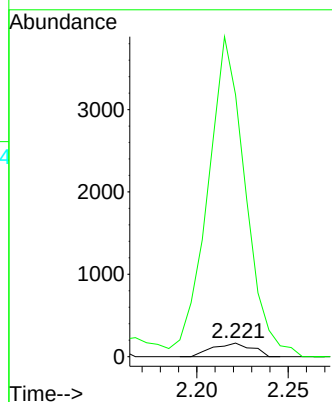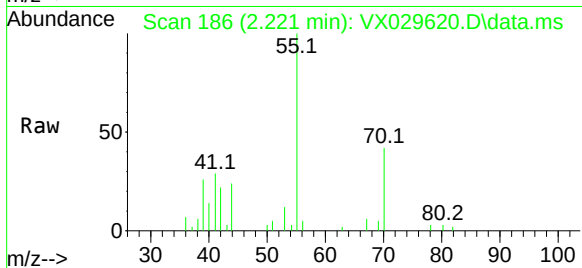

#14

Allyl chloride

Concen: 0.223 ug/l

RT: 2.764 min Scan# 275

Delta R.T. 0.098 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06




Tgt Ion: 41 Resp: 986


Ion Ratio Lower Upper

41 100

39 161.1 50.4 75.6#

76 0.0 32.7 49.1#


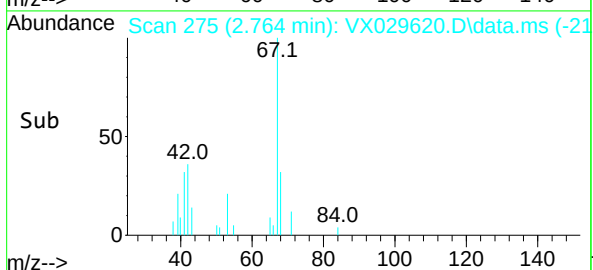

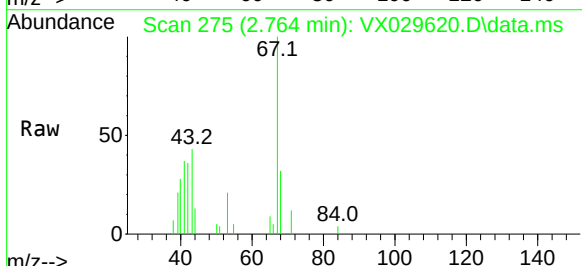




#16
Acetone
Concen: 1.633 ug/l
RT: 2.380 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 43 Resp: 2326
Ion Ratio Lower Upper
43 100
58 27.7 28.8 43.2#

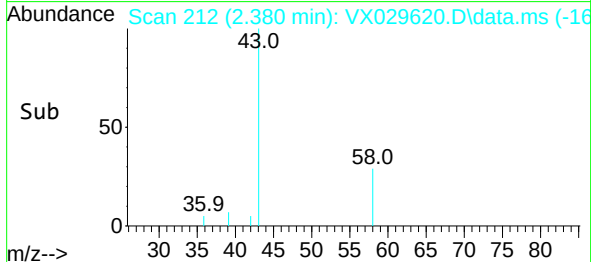

#19
Methyl tert-butyl Ether
Concen: 3.558 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 73 Resp: 33789
Ion Ratio Lower Upper
73 100
57 24.5 16.8 25.2


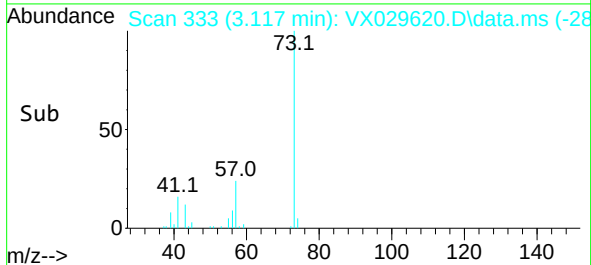

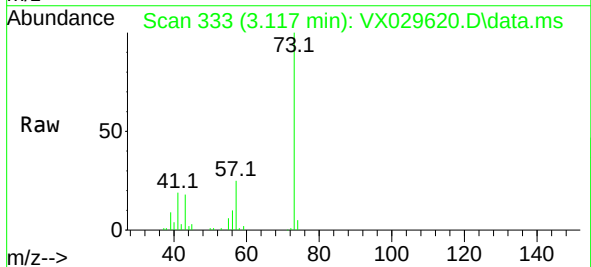




#22
Diisopropyl ether
Concen: 0.309 ug/l
RT: 3.764 min Scan# 41
Delta R.T. 0.001 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 45 Resp: 2700
Ion Ratio Lower Upper
45 100
43 60.3 50.8 76.2
87 28.9 26.6 39.8
59 16.7 10.5 15.7#

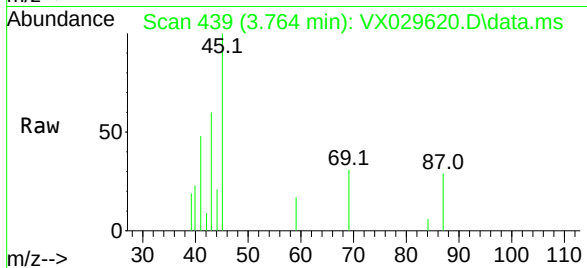

#23
Vinyl Acetate
Concen: 0.213 ug/l
RT: 3.764 min Scan# 439
Delta R.T. 0.037 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 43 Resp: 1551
Ion Ratio Lower Upper
43 100
86 0.0 10.8 16.2#


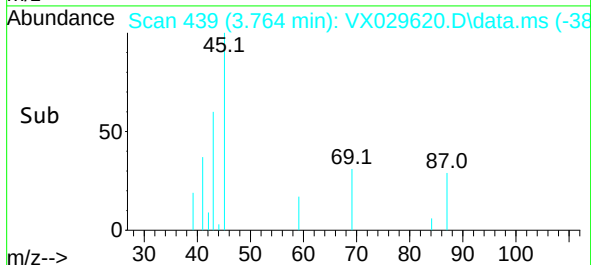

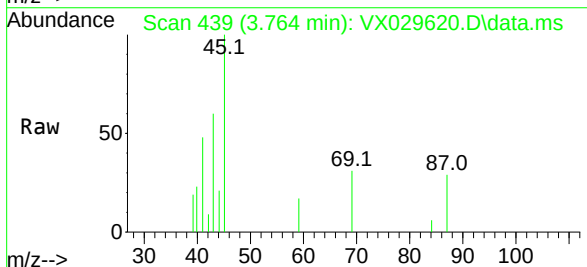




#25
2-Butanone
Concen: 0.580 ug/l
RT: 4.593 min Scan# 51
Delta R.T. 0.031 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 43 Resp: 1306
Ion Ratio Lower Upper
43 100
72 18.6 24.4 36.6#

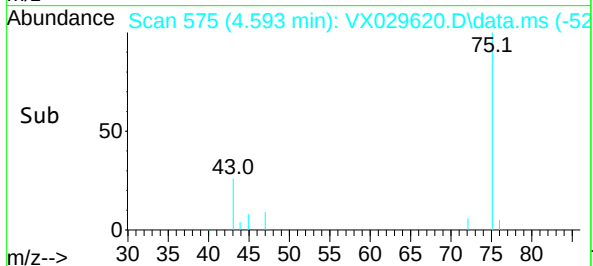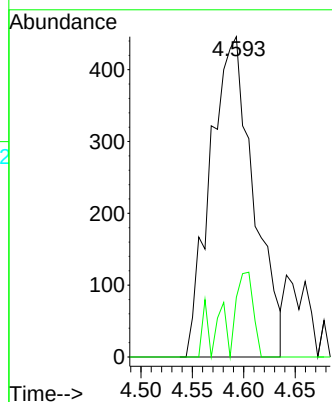

#31
Cyclohexane
Concen: 2.039 ug/l
RT: 5.471 min Scan# 719
Delta R.T. -0.006 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 56 Resp: 9783
Ion Ratio Lower Upper
56 100
69 29.9 26.7 40.1
84 100.1 77.2 115.8

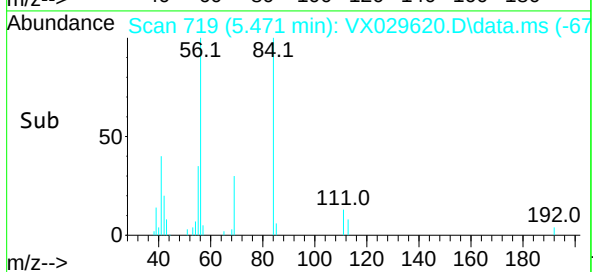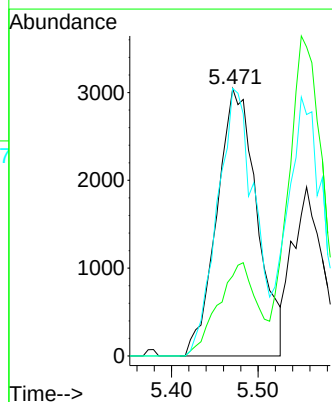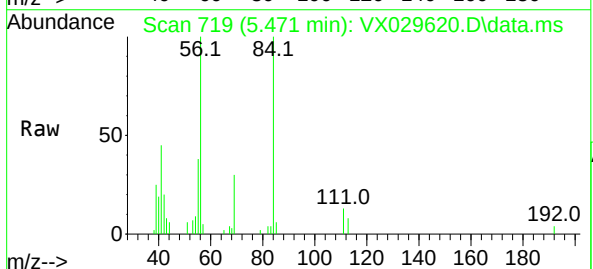

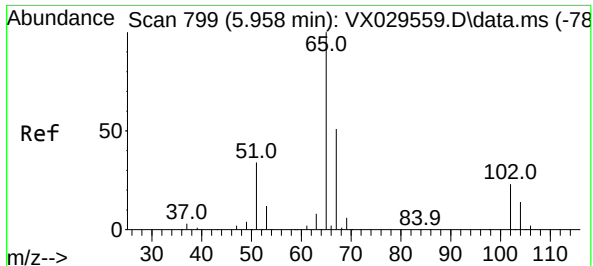

#33

1,2-Dichloroethane-d4

Concen: 43.596 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06

Instrument :

MSVOA_X

ClientSampleId :





MW-10DL

Tgt Ion: 65 Resp: 155817

Ion Ratio Lower Upper

65 100

67 52.7 0.0 107.4

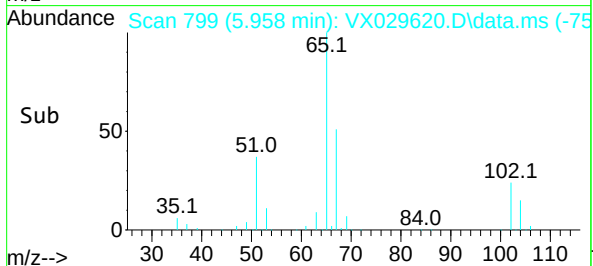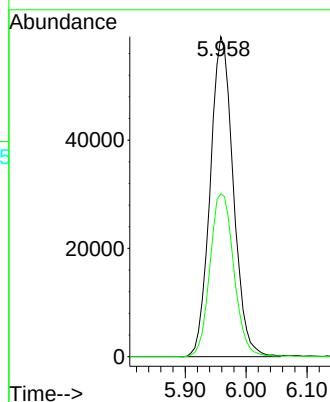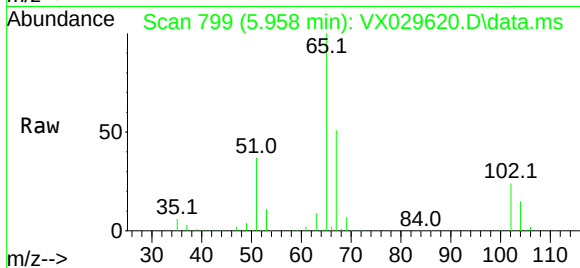

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06




Tgt Ion: 114 Resp: 458778


Ion Ratio Lower Upper

114 100

63 19.3 0.0 36.8

88 17.5 0.0 32.4

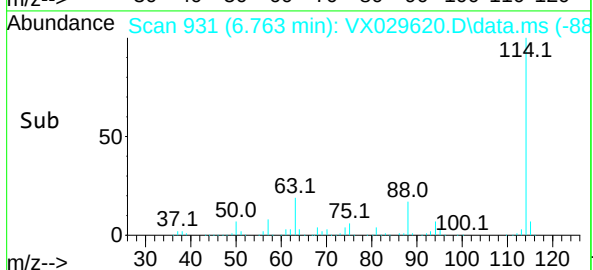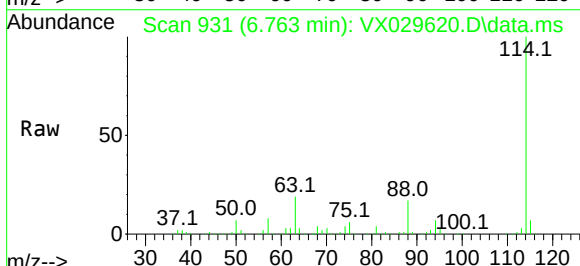

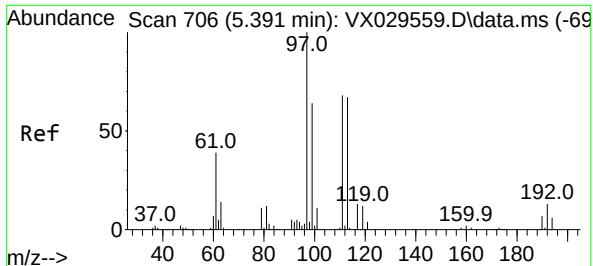

#35

Dibromofluoromethane

Concen: 45.429 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06

Instrument :

MSVOA_X

ClientSampleId :

MW-10DL





Tgt Ion:113 Resp: 135823

Ion Ratio Lower Upper

113 100

111 104.0 82.8 124.2

192 18.6 16.9 25.3

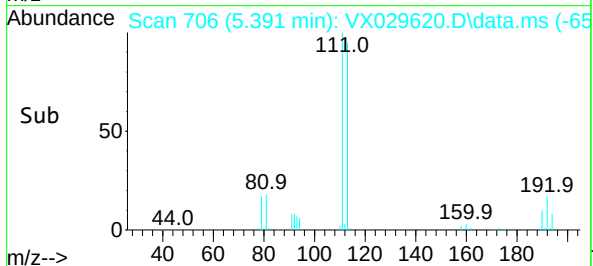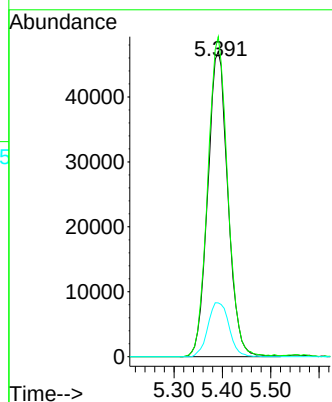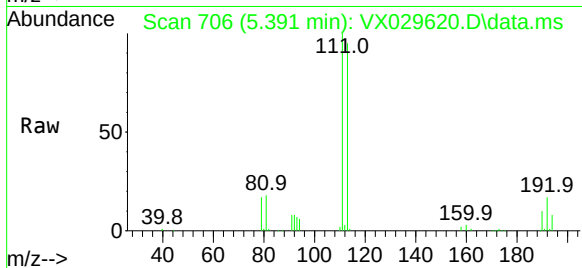

#36

1,1-Dichloropropene

Concen: 4.968 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06




Tgt Ion: 75 Resp: 20105


Ion Ratio Lower Upper

75 100

110 10.5 18.3 54.8#


77 0.0 24.8 37.2#

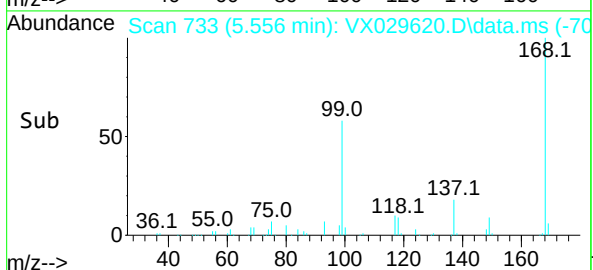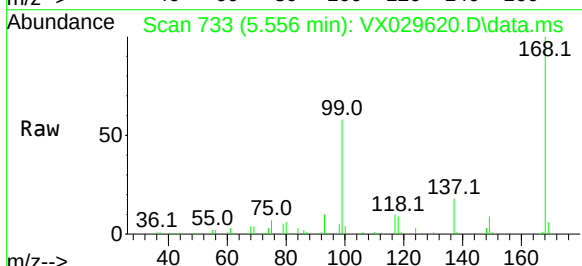






#38
Carbon Tetrachloride
Concen: 7.256 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Instrument :
MSVOA_X
ClientSampleId :
MW-10DL



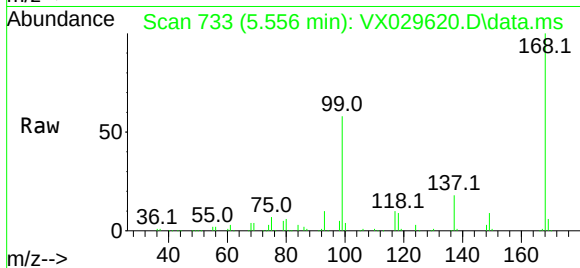



Tgt Ion:117 Resp: 28872
Ion Ratio Lower Upper
117 100
119 5.2 77.3 115.9#
121 0.0 24.2 36.2#

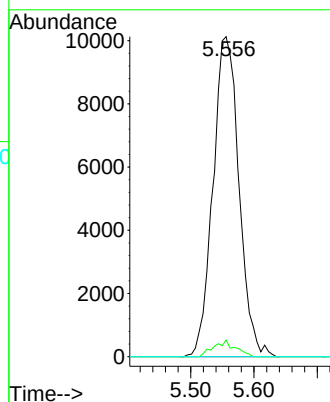

#39
Methylcyclohexane
Concen: 0.660 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 83 Resp: 3332
Ion Ratio Lower Upper
83 100
55 76.2 54.6 81.8
98 50.1 37.4 56.2


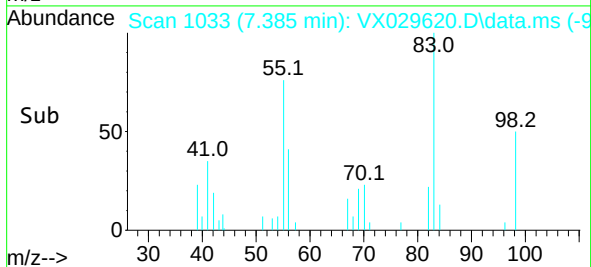

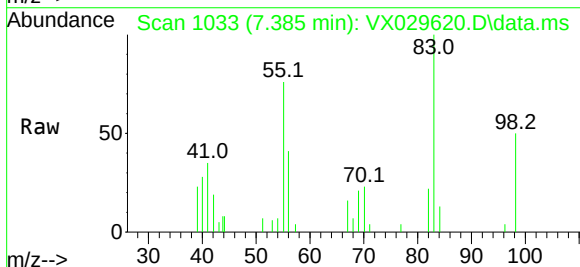




#40
Benzene
Concen: 32.542 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 78 Resp: 390333
Ion Ratio Lower Upper
78 100
77 23.6 19.3 28.9

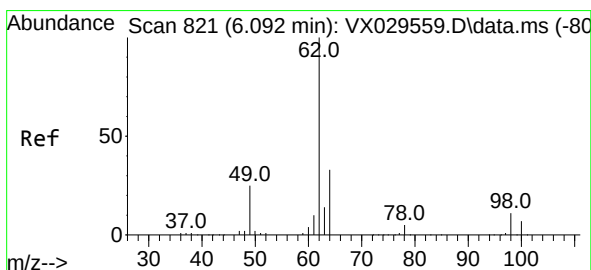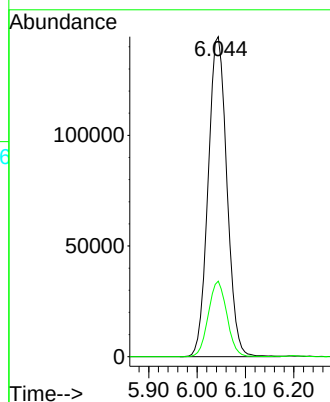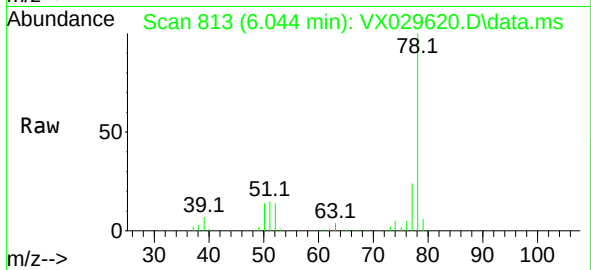

#42
1,2-Dichloroethane
Concen: 0.860 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.048 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 62 Resp: 3546
Ion Ratio Lower Upper
62 100
98 0.0 0.0 20.4


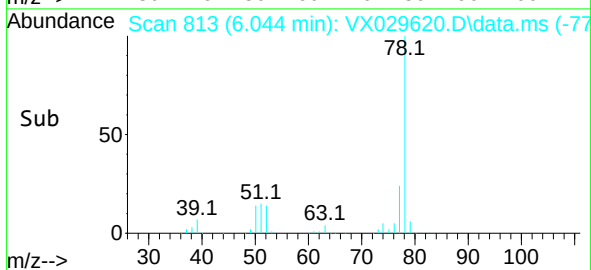
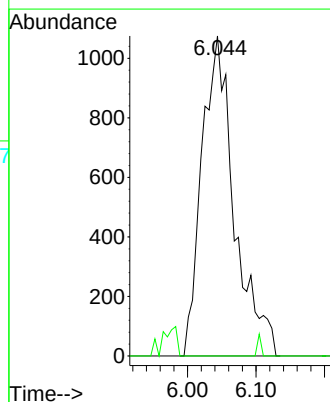
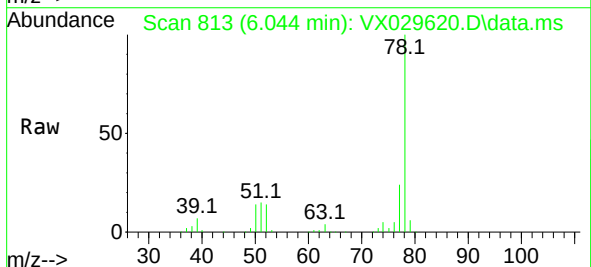


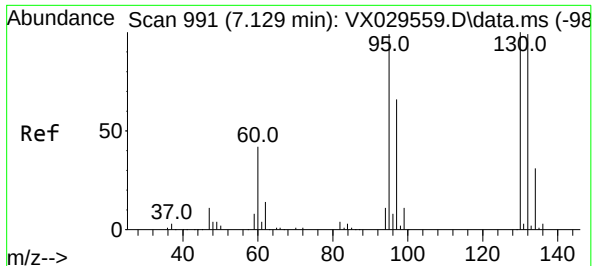

#44
Trichloroethene
Concen: Below Cal
RT: 7.135 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion:130 Resp: 2156
Ion Ratio Lower Upper
130 100
95 87.3 0.0 188.8

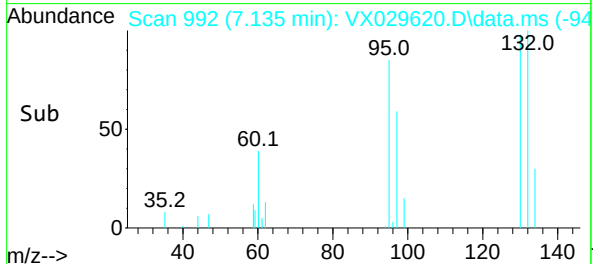

#50
Toluene-d8
Concen: 47.269 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 98 Resp: 516287
Ion Ratio Lower Upper
98 100
100 67.7 52.6 78.8


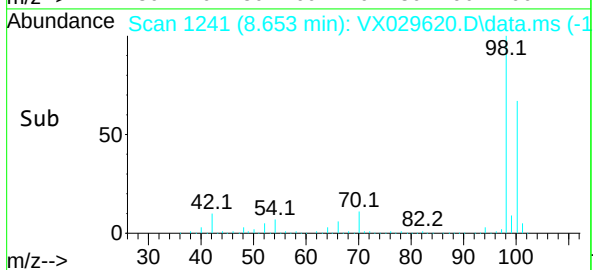

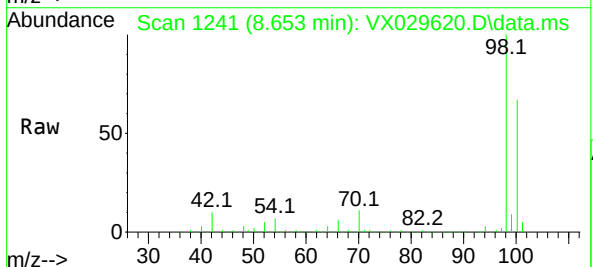




#52
Toluene
Concen: 3.197 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 92 Resp: 24555
Ion Ratio Lower Upper
92 100
91 170.8 137.5 206.3



#59
2-Hexanone
Concen: 0.664 ug/l
RT: 9.452 min Scan# 1372
Delta R.T. 0.019 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 43 Resp: 2091
Ion Ratio Lower Upper
43 100
58 59.3 31.9 95.7

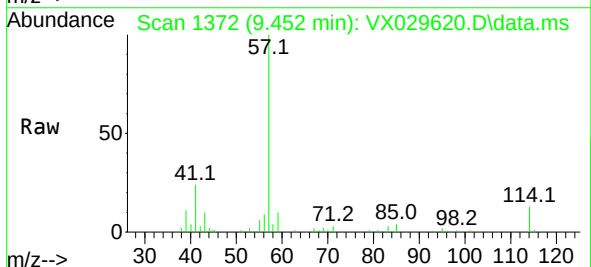



#62

4-Bromofluorobenzene

Concen: 45.664 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06

Instrument :

MSVOA_X

ClientSampleId :

MW-10DL





Tgt Ion: 95 Resp: 188088

Ion Ratio Lower Upper

95 100

174 72.3 0.0 163.0

176 70.4 0.0 155.0

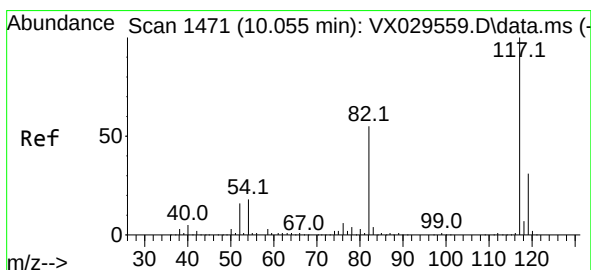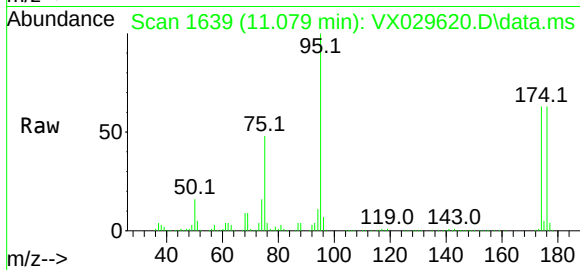

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX029620.D

Acq: 20 Jun 2022 14:06




Tgt Ion: 117 Resp: 395214


Ion Ratio Lower Upper

117 100

82 55.2 41.8 62.8

119 32.0 24.8 37.2


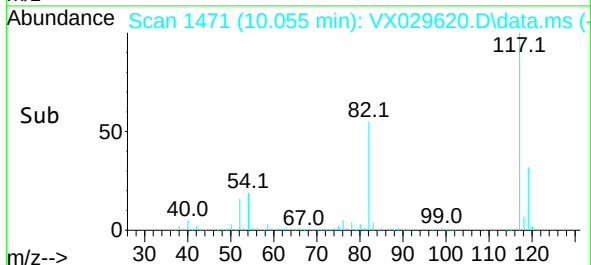

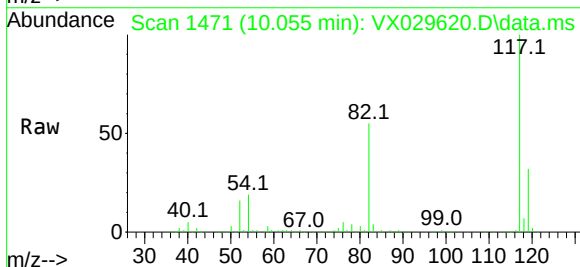




#67
Ethyl Benzene
Concen: 2.614 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 91 Resp: 36460
Ion Ratio Lower Upper
91 100
106 32.9 24.6 36.8

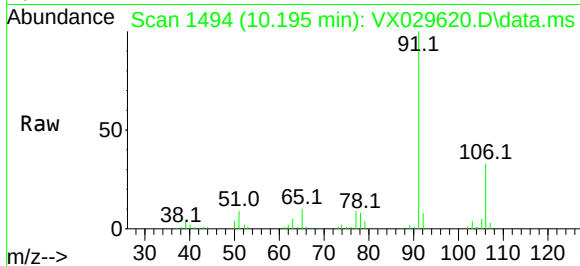

#68
m/p-Xylenes
Concen: 45.743 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 106 Resp: 248857
Ion Ratio Lower Upper
106 100
91 207.9 160.4 240.6


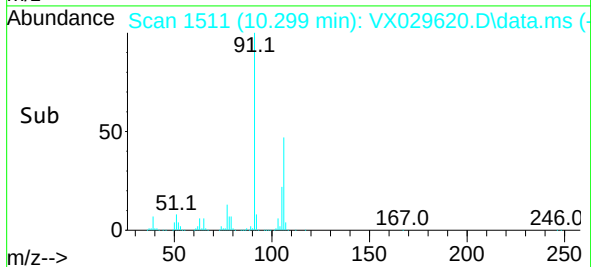

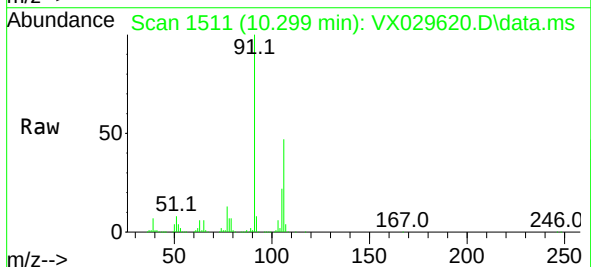




#69
o-Xylene
Concen: 3.449 ug/l
RT: 10.647 min Scan# 11
Delta R.T. 0.001 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion:106 Resp: 18536
Ion Ratio Lower Upper
106 100
91 215.3 106.1 318.1

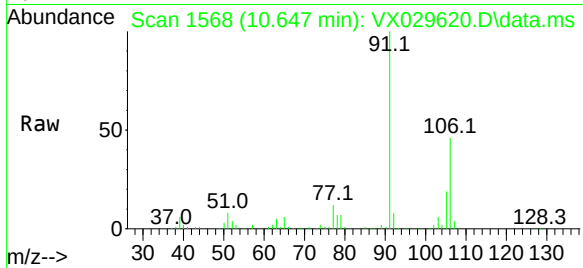

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion:152 Resp: 172251
Ion Ratio Lower Upper
152 100
115 63.6 37.5 112.7
150 157.9 0.0 338.2


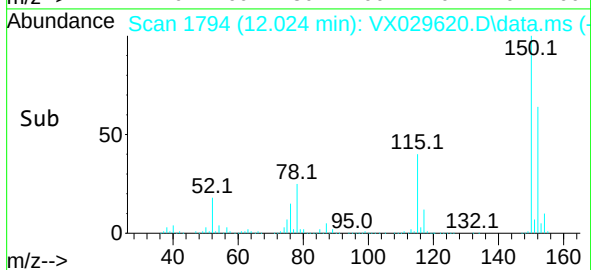

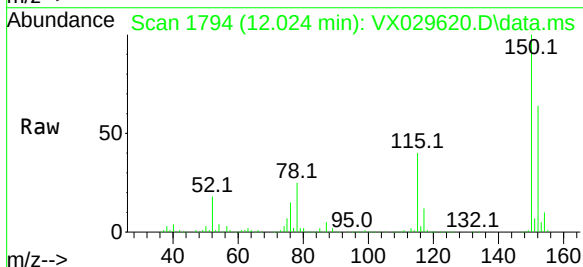




#73
Isopropylbenzene
Concen: 3.964 ug/l
RT: 10.964 min Scan# 1639
Delta R.T. 0.001 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion:105 Resp: 51192
Ion Ratio Lower Upper
105 100
120 26.3 13.5 40.5

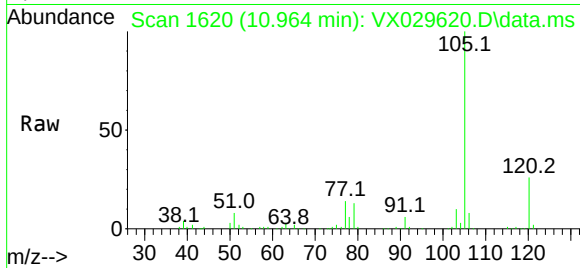

#76
1,2,3-Trichloropropane
Concen: 23.920 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 75 Resp: 89761
Ion Ratio Lower Upper
75 100
77 1.3 19.4 58.2#



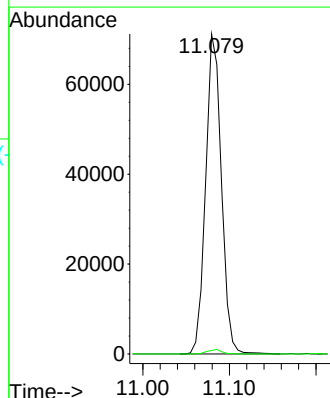
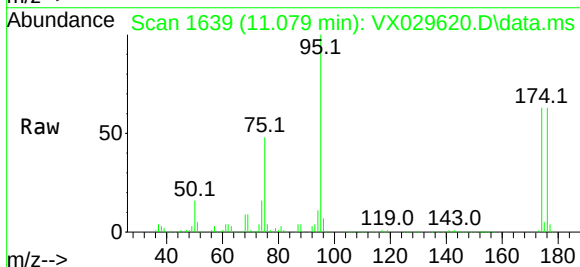


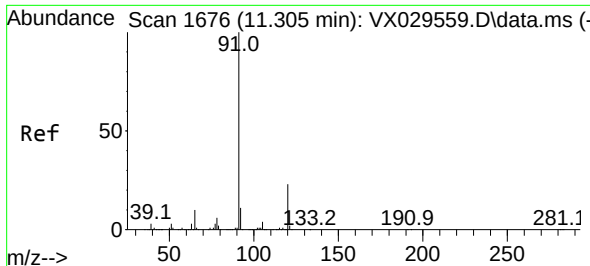

#78
n-propylbenzene
Concen: 9.574 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 91 Resp: 139262
Ion Ratio Lower Upper
91 100
120 23.2 11.6 34.8

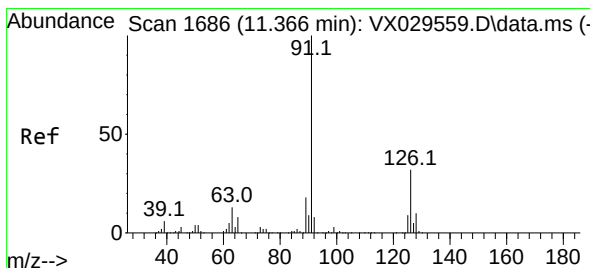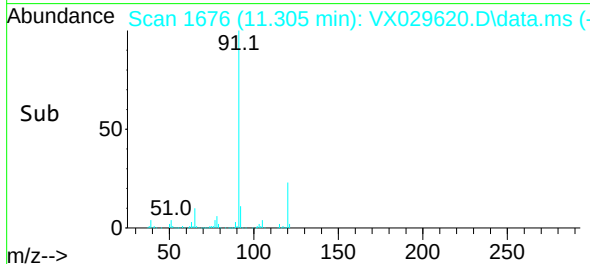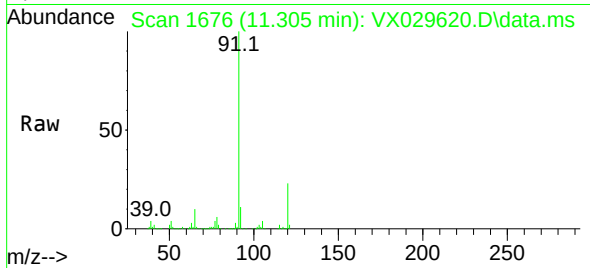

#79
2-Chlorotoluene
Concen: 0.488 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. 0.036 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 91 Resp: 4397
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#


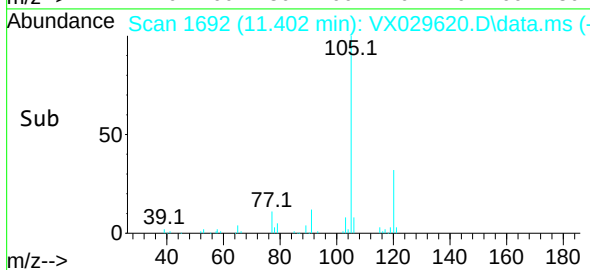

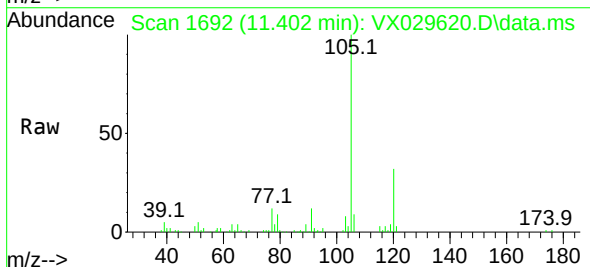




#80
1,3,5-Trimethylbenzene
Concen: 2.685 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion:105 Resp: 29200
Ion Ratio Lower Upper
105 100
120 47.0 24.3 72.9

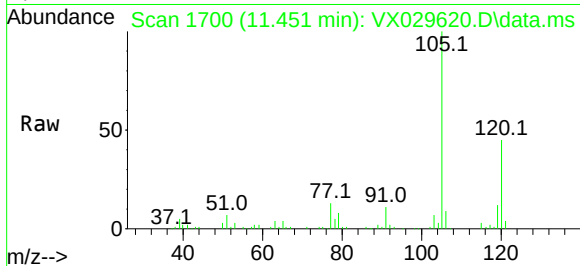

#81
trans-1,4-Dichloro-2-butene
Concen: 79.577 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 75 Resp: 89761
Ion Ratio Lower Upper
75 100
53 0.1 69.0 103.4#
89 0.0 37.0 55.6#


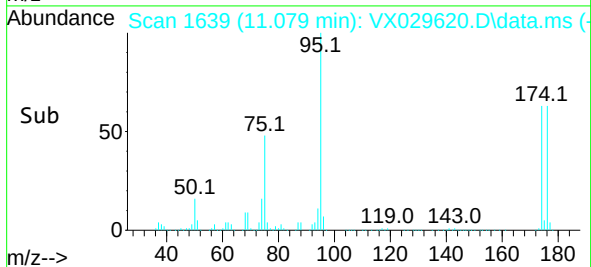

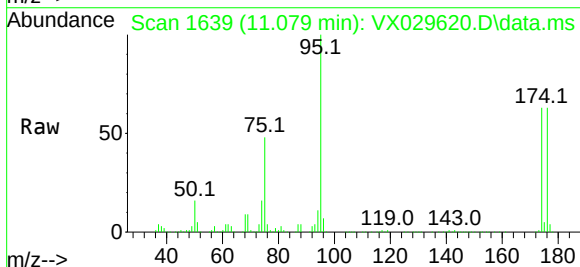




#82
4-Chlorotoluene
Concen: 0.428 ug/l
RT: 11.402 min Scan# 11
Delta R.T. -0.055 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06




Instrument :
MSVOA_X
ClientSampleId :
MW-10DL


Tgt Ion: 91 Resp: 4397
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

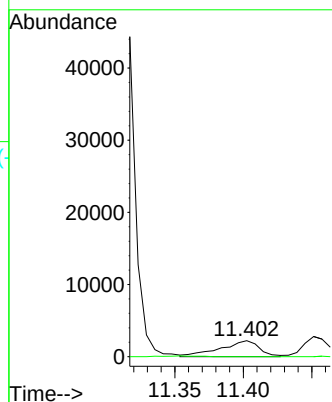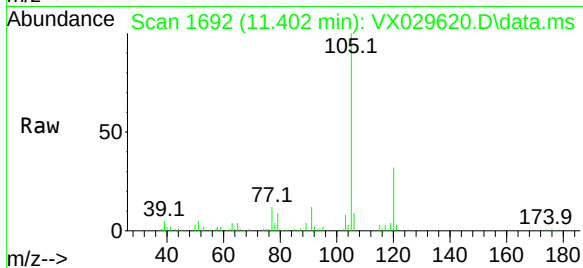

#84
1,2,4-Trimethylbenzene
Concen: 4.969 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion: 105 Resp: 53899
Ion Ratio Lower Upper
105 100
120 46.3 22.6 67.8


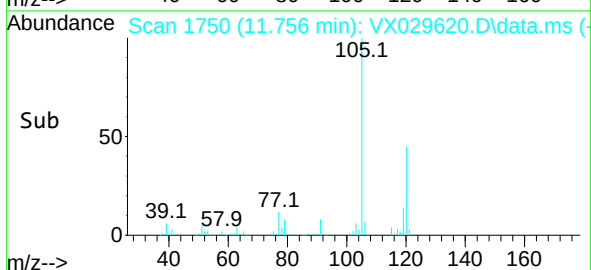

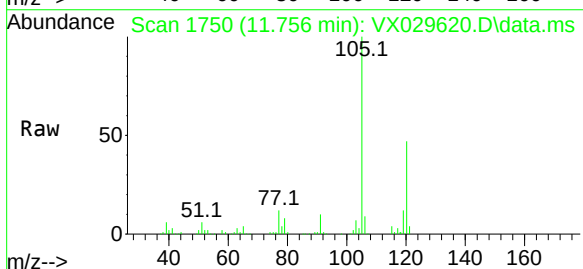




#85
 sec-Butylbenzene
 Concen: 0.378 ug/l
 RT: 11.890 min Scan# 11772
 Delta R.T. 0.000 min
 Lab File: VX029620.D
 Acq: 20 Jun 2022 14:06




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-10DL


Tgt Ion:105 Resp: 4964
 Ion Ratio Lower Upper
 105 100
 134 18.4 10.2 30.4

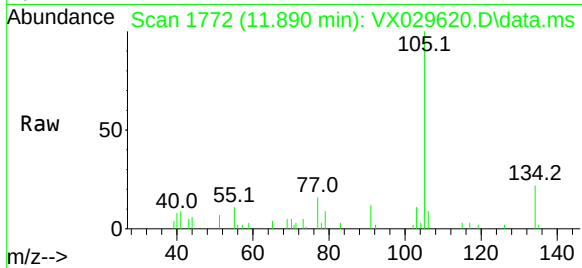

#89
 n-Butylbenzene
 Concen: 0.707 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX029620.D
 Acq: 20 Jun 2022 14:06

Tgt Ion: 91 Resp: 6568
 Ion Ratio Lower Upper
 91 100
 92 35.6 27.8 83.3
 134 58.3 13.3 39.8#


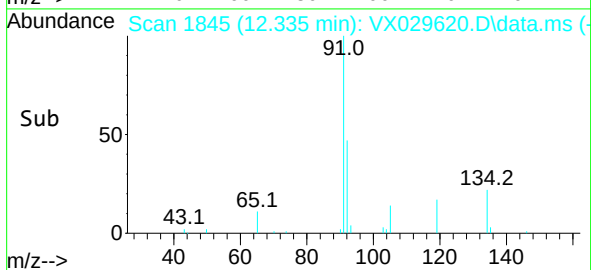

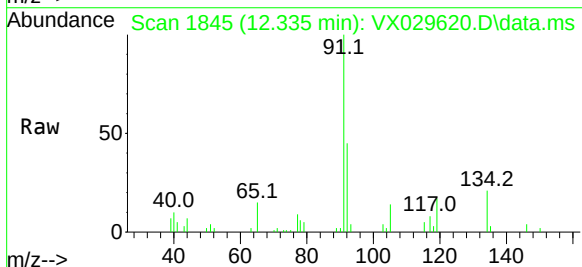




#90
Hexachloroethane
Concen: 4.302 ug/l
RT: 12.646 min Scan# 1879
Delta R.T. 0.104 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Instrument :
MSVOA_X
ClientSampleId :
MW-10DL

Tgt Ion:117 Resp: 6779
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

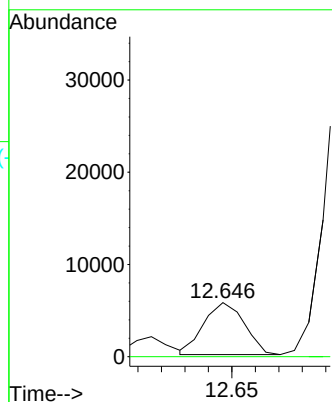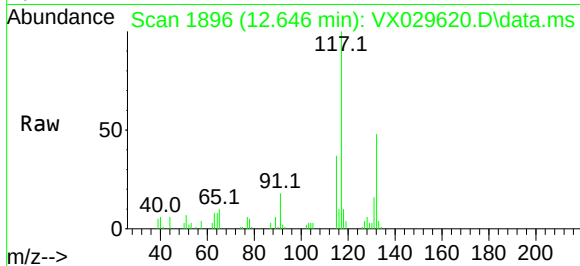

#95
Naphthalene
Concen: 13.112 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX029620.D
Acq: 20 Jun 2022 14:06

Tgt Ion:128 Resp: 158421
Ion Ratio Lower Upper
128 100
127 12.4 10.2 15.4
129 11.0 8.7 13.1

