

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
 Data File : VX029627.D
 Acq On : 20 Jun 2022 16:49
 Operator : JC/MD
 Sample : N3391-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 M15848

Quant Time: Jun 21 01:52:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	252970	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	421375	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	366985	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	161080	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	5.958	65	145769	43.531	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.060%
35) Dibromofluoromethane	5.391	113	126249	45.975	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.940%
50) Toluene-d8	8.653	98	484081	48.255	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.500%
62) 4-Bromofluorobenzene	11.079	95	174507	46.128	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.260%

Target Compounds


						Qvalue
3) Chloromethane	1.288	50	2221	0.673	ug/l #	82
5) Bromomethane	1.611	94	734	0.473	ug/l #	69
6) Chloroethane	1.691	64	1730	2.001	ug/l	98
10) Methyl Iodide	2.459	142	503	3.174	ug/l #	84
11) Tert butyl alcohol	2.971	59	71002	91.429	ug/l	97
13) Acrolein	2.239	56	1184	6.419	ug/l #	56
14) Allyl chloride	2.642	41	938	0.227	ug/l #	25
15) Acrylonitrile	2.971	53	782	0.499	ug/l #	16
16) Acetone	2.379	43	313463	234.851	ug/l	99
18) Methyl Acetate	2.556	43	16172	4.583	ug/l #	46
25) 2-Butanone	4.562	43	109471	51.888	ug/l	98
29) Tetrahydrofuran	5.019	42	2110	1.501	ug/l	89
31) Cyclohexane	5.556	56	4698	1.045	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	18692	5.029	ug/l #	49
37) Ethyl Acetate	4.562	43	109471	28.735	ug/l #	65
38) Carbon Tetrachloride	5.556	117	26010	7.117	ug/l #	15
40) Benzene	6.043	78	2965	0.269	ug/l	98
42) 1,2-Dichloroethane	6.110	62	1208	0.319	ug/l	91
43) Isopropyl Acetate	6.245	43	4848	0.818	ug/l #	56
44) Trichloroethene	7.129	130	1741	Below Cal		98
48) Methyl methacrylate	7.592	41	2279	0.785	ug/l #	29
49) 1,4-Dioxane	7.482	88	372	4.967	ug/l #	25
51) 4-Methyl-2-Pentanone	8.573	43	70650	18.503	ug/l	96
59) 2-Hexanone	9.433	43	44901	15.529	ug/l	89
65) Chlorobenzene	10.274	112	4125	0.573	ug/l #	46
68) m/p-Xylenes	10.305	106	1093	0.216	ug/l	75
74) N-amyl acetate	10.890	43	18283	4.359	ug/l #	64
76) 1,2,3-Trichloropropane	11.079	75	83570	23.815	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	83570	79.227	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	2721	0.268	ug/l	75
92) 1,2-Dibromo-3-Chloropr...	12.804	75	1182	1.366	ug/l #	1
95) Naphthalene	13.780	128	3459	0.306	ug/l #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
Data File : VX029627.D
Acq On : 20 Jun 2022 16:49
Operator : JC/MD
Sample : N3391-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
M15848

Quant Time: Jun 21 01:52:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




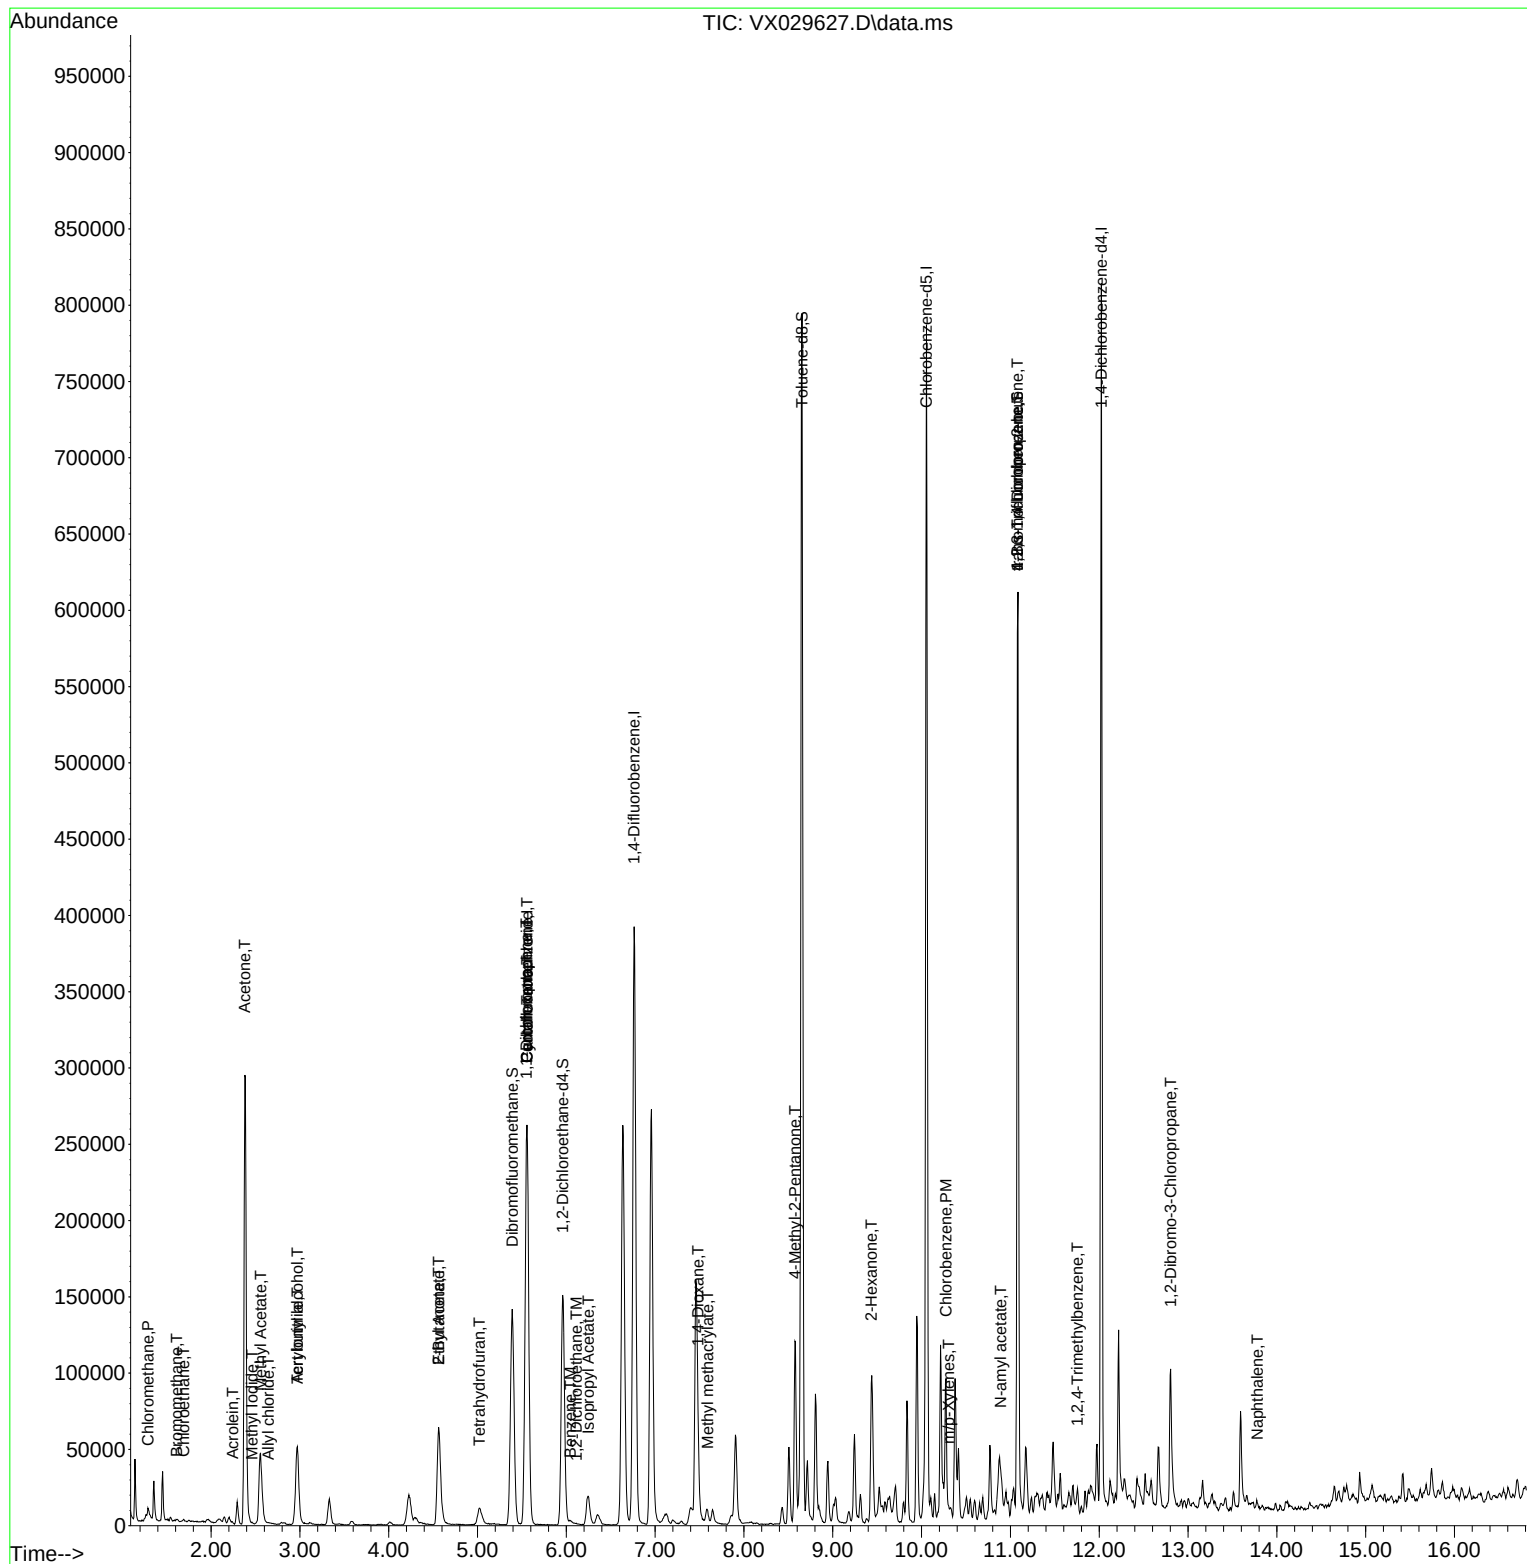




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion:168 Resp: 252970
Ion Ratio Lower Upper
168 100
99 59.7 41.7 62.5

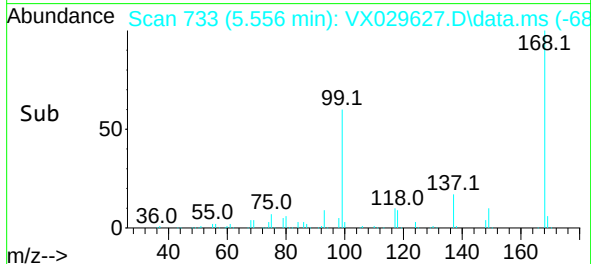

#3
Chloromethane
Concen: 0.673 ug/l
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 50 Resp: 2221
Ion Ratio Lower Upper
50 100
52 43.1 26.4 39.6#




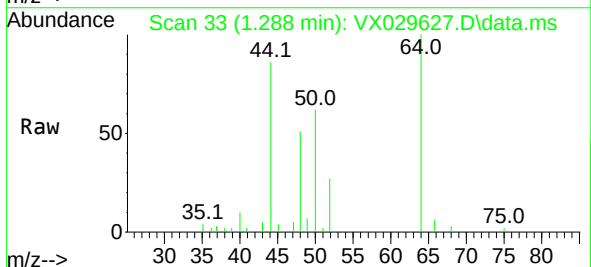


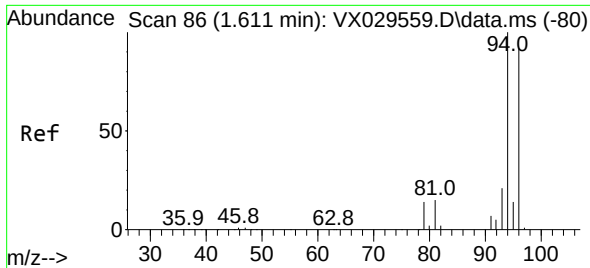

#5
Bromomethane
Concen: 0.473 ug/l
RT: 1.611 min Scan# 80
Delta R.T. 0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 94 Resp: 734
Ion Ratio Lower Upper
94 100
96 64.0 75.3 112.9#

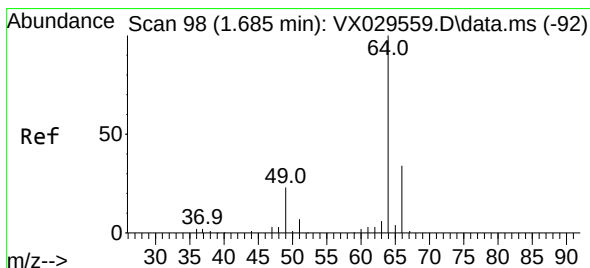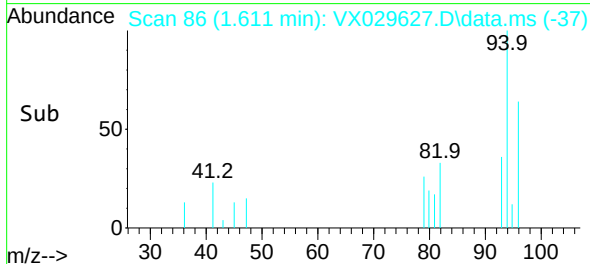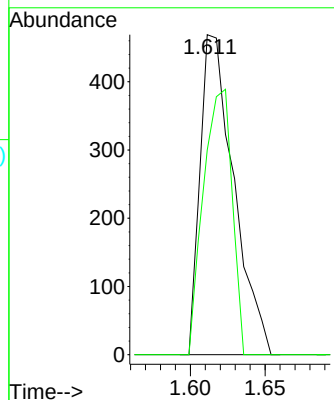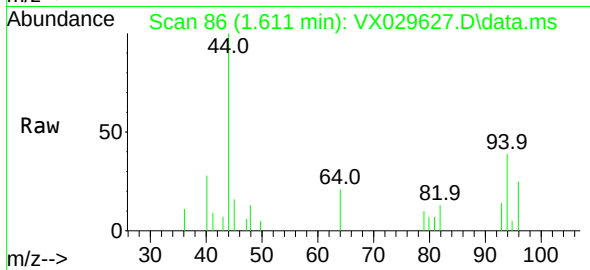

#6
Chloroethane
Concen: 2.001 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 64 Resp: 1730
Ion Ratio Lower Upper
64 100
66 30.6 25.3 37.9


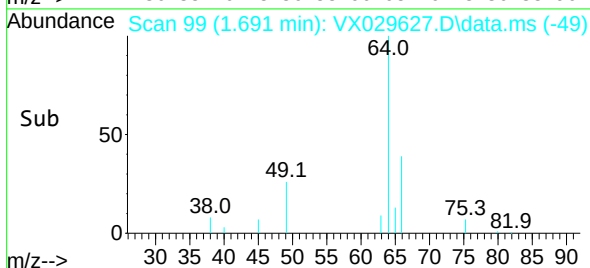
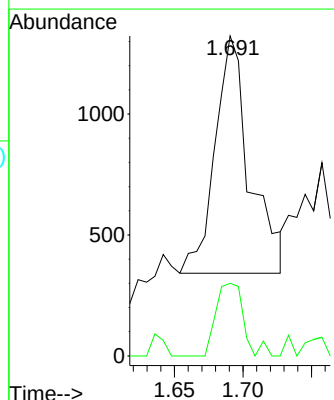
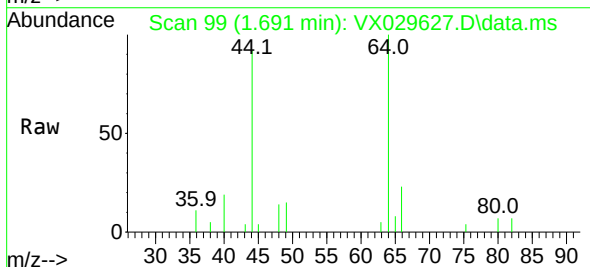


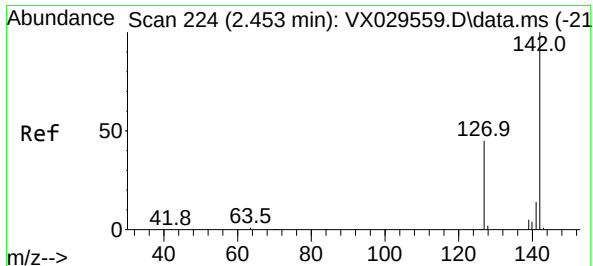

#10
Methyl Iodide
Concen: 3.174 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion:142 Resp: 503
Ion Ratio Lower Upper
142 100
127 36.4 33.9 50.9
141 0.0 11.4 17.2#

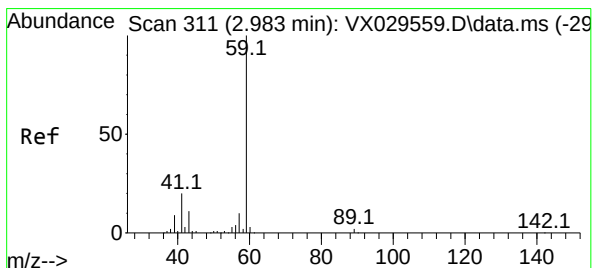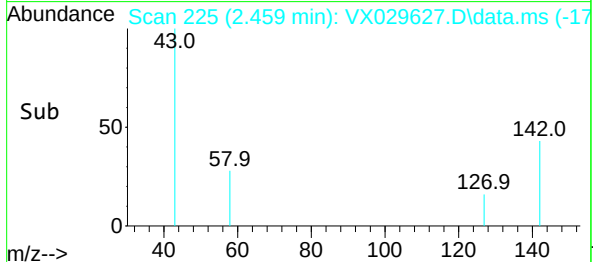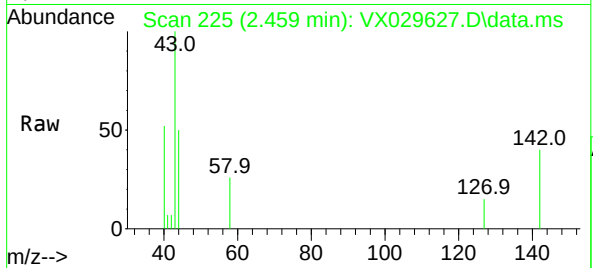

#11
Tert butyl alcohol
Concen: 91.429 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 59 Resp: 71002
Ion Ratio Lower Upper
59 100
57 9.4 8.3 12.5

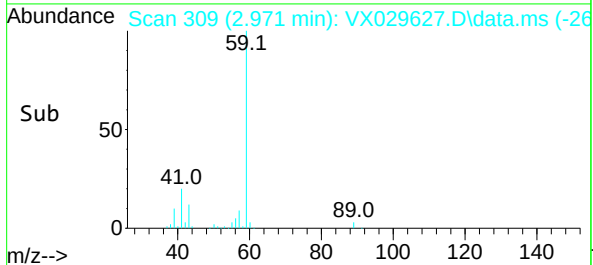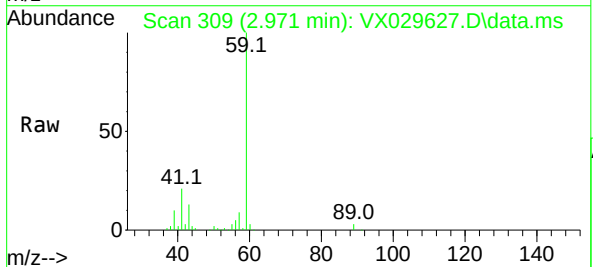

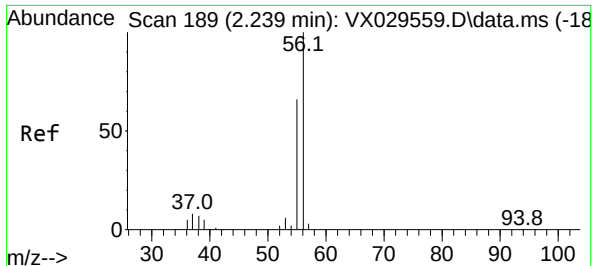

#13

Acrolein

Concen: 6.419 ug/l

RT: 2.239 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :





M15848

Tgt Ion: 56 Resp: 1184

Ion Ratio Lower Upper

56 100

55 104.9 55.0 82.6#

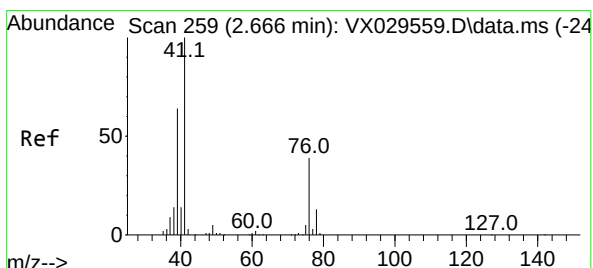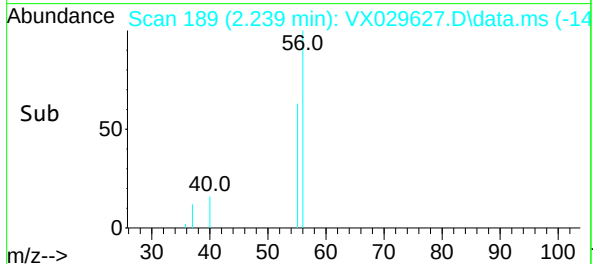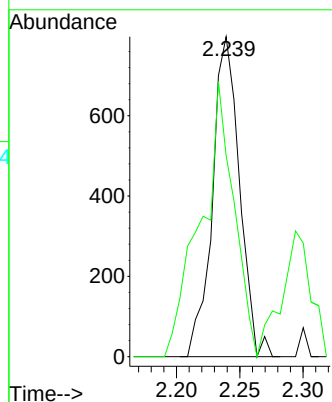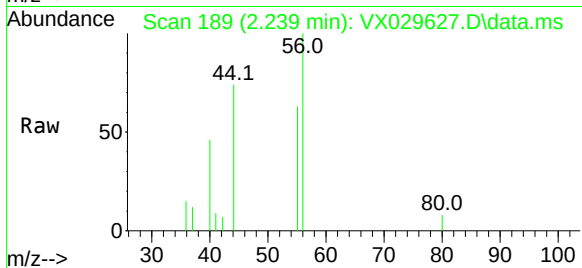

#14

Allyl chloride

Concen: 0.227 ug/l

RT: 2.642 min Scan# 255

Delta R.T. -0.024 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 41 Resp: 938


Ion Ratio Lower Upper

41 100

39 0.0 50.4 75.6#

76 0.0 32.7 49.1#


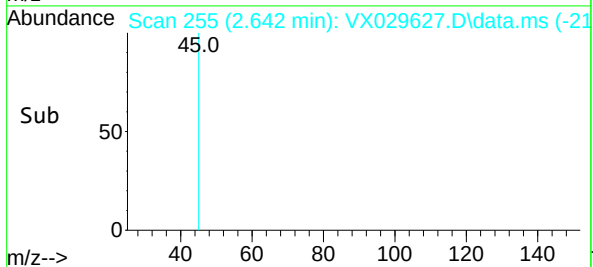
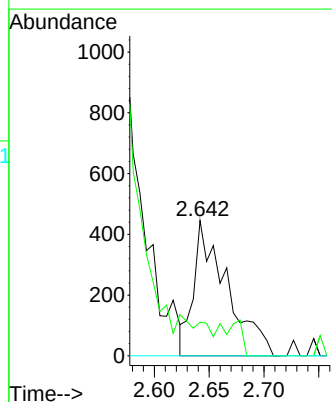
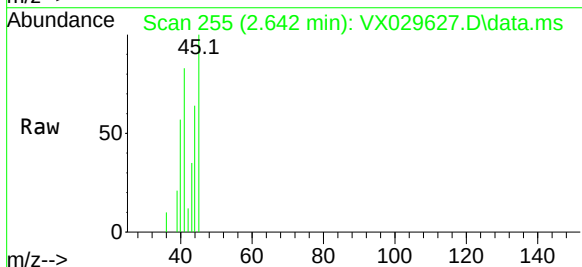




#15
Acrylonitrile
Concen: 0.499 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.097 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 53 Resp: 782
Ion Ratio Lower Upper
53 100
52 9.5 65.7 98.5#
51 87.9 28.4 42.6#

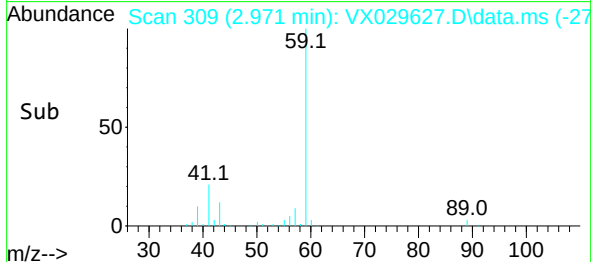

#16
Acetone
Concen: 234.851 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.007 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 43 Resp: 313463
Ion Ratio Lower Upper
43 100
58 35.2 28.8 43.2

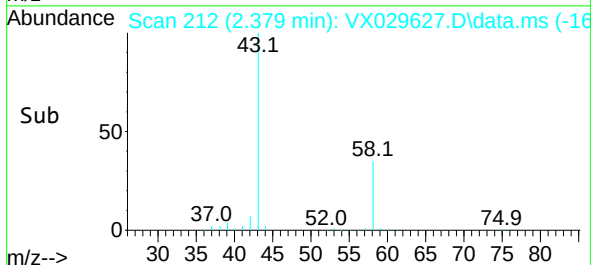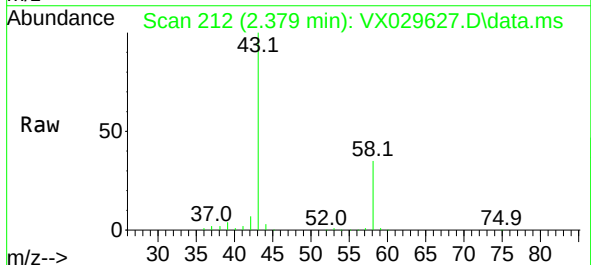

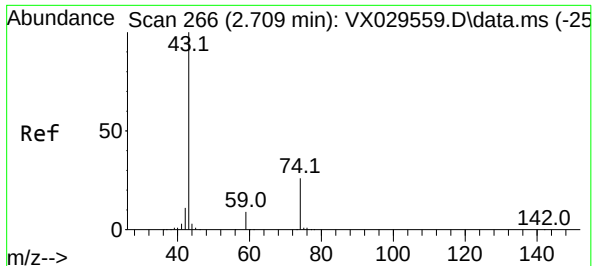

#18

Methyl Acetate

Concen: 4.583 ug/l

RT: 2.556 min Scan# 241

Delta R.T. -0.153 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :





M15848

Tgt Ion: 43 Resp: 16172

Ion Ratio Lower Upper

43 100

74 0.0 22.8 34.2#

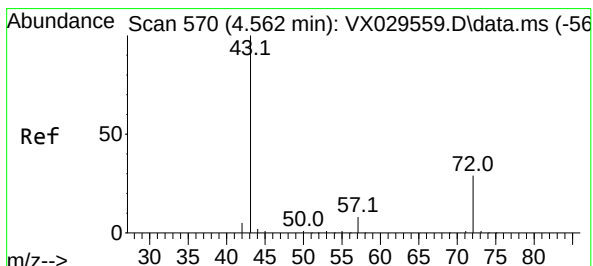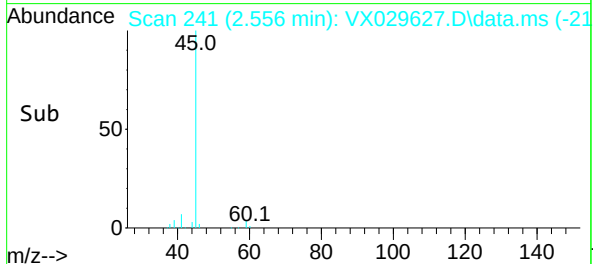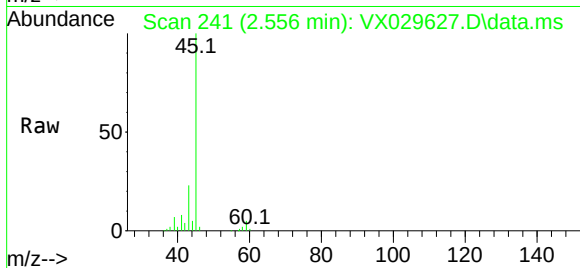

#25

2-Butanone

Concen: 51.888 ug/l

RT: 4.562 min Scan# 570

Delta R.T. -0.000 min

Lab File: VX029627.D




Acq: 20 Jun 2022 16:49


Tgt Ion: 43 Resp: 109471

Ion Ratio Lower Upper

43 100

72 29.5 24.4 36.6

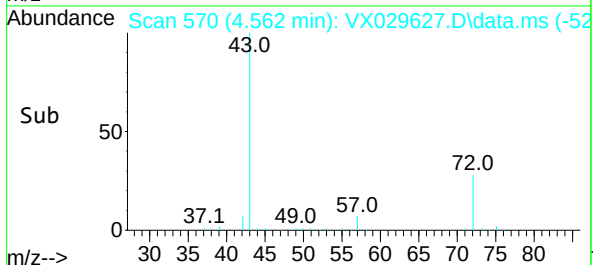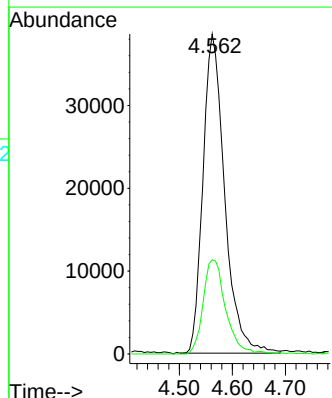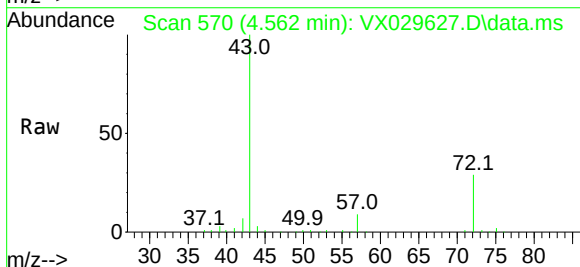



#29

Tetrahydrofuran

Concen: 1.501 ug/l

RT: 5.019 min Scan# 644

Delta R.T. 0.006 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :

M15848





Tgt Ion: 42 Resp: 2110

Ion Ratio Lower Upper

42 100

72 61.2 44.1 66.1

71 40.6 40.5 60.7

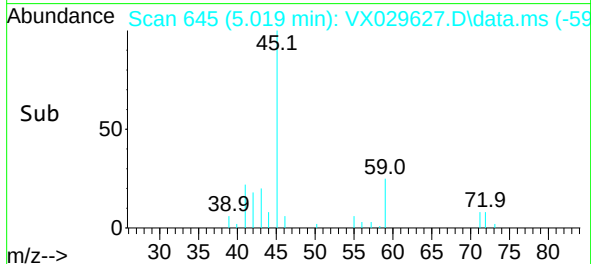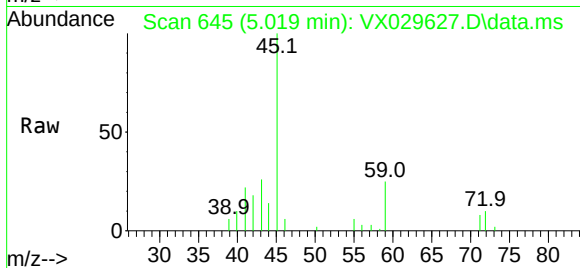

#31

Cyclohexane

Concen: 1.045 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.079 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 56 Resp: 4698


Ion Ratio Lower Upper

56 100

69 196.6 26.7 40.1#

84 146.3 77.2 115.8#

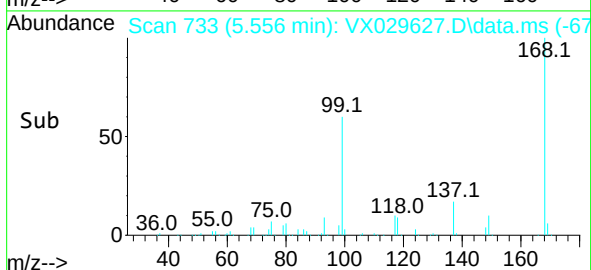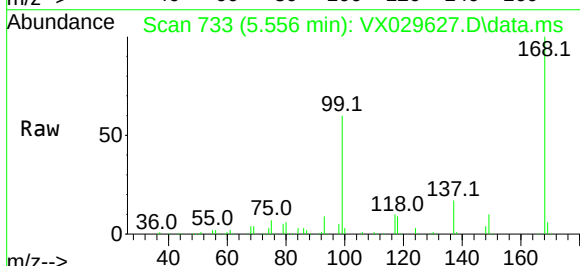

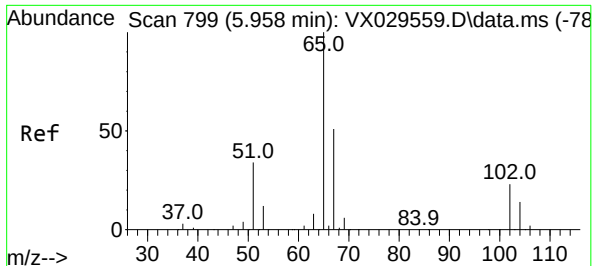

#33

1,2-Dichloroethane-d4

Concen: 43.531 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :





M15848

Tgt Ion: 65 Resp: 145769

Ion Ratio Lower Upper

65 100

67 52.8 0.0 107.4

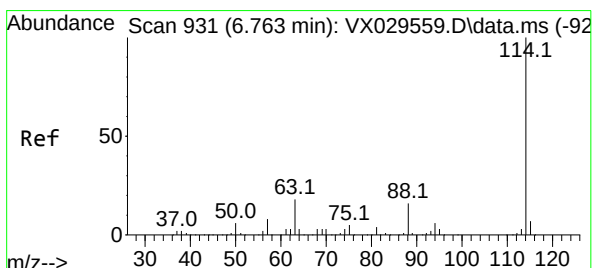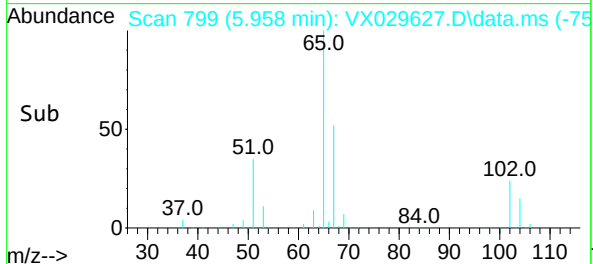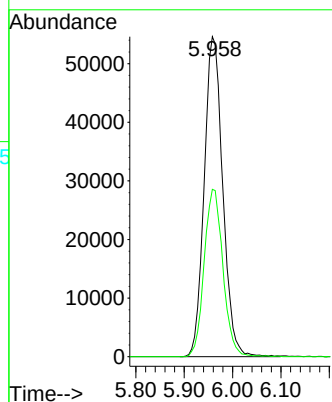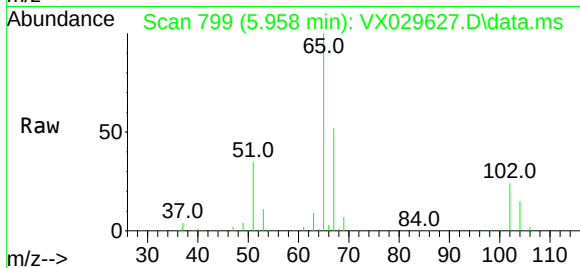

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 114 Resp: 421375


Ion Ratio Lower Upper

114 100

63 19.8 0.0 36.8

88 15.9 0.0 32.4

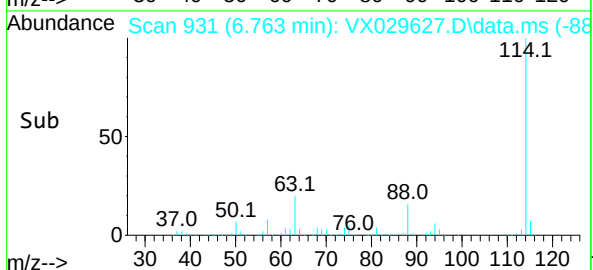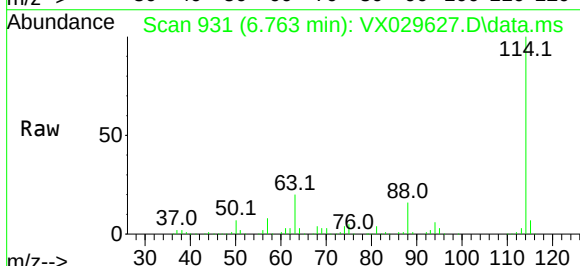

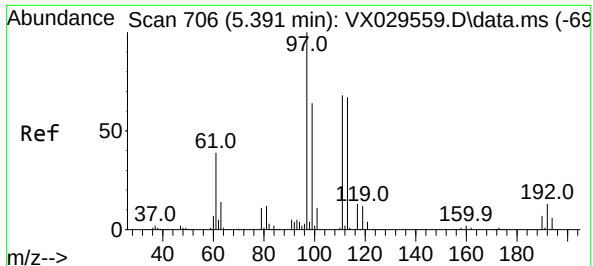

#35

Dibromofluoromethane

Concen: 45.975 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :

M15848





Tgt Ion:113 Resp: 126249

Ion Ratio Lower Upper

113 100

111 101.7 82.8 124.2

192 18.6 16.9 25.3

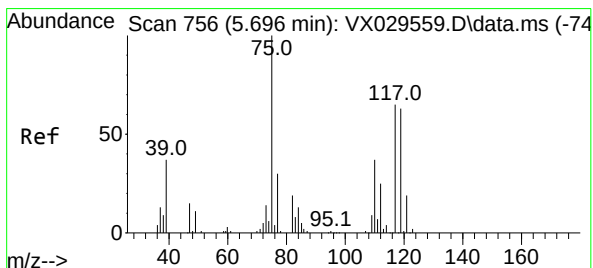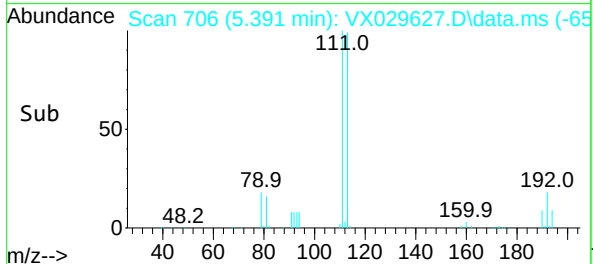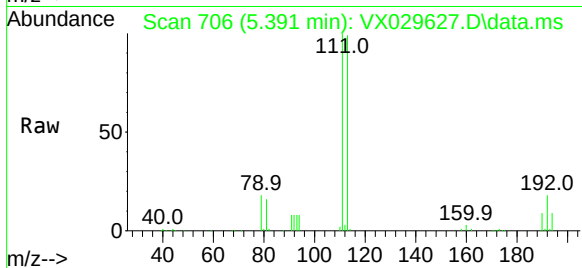

#36

1,1-Dichloropropene

Concen: 5.029 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 75 Resp: 18692


Ion Ratio Lower Upper

75 100

110 9.4 18.3 54.8#

77 0.0 24.8 37.2#

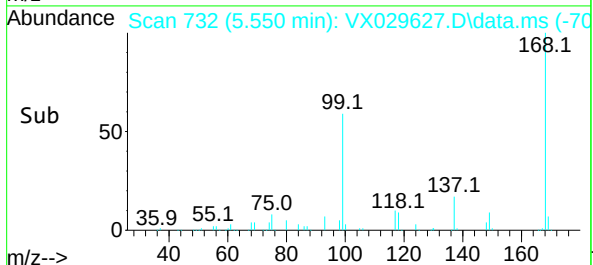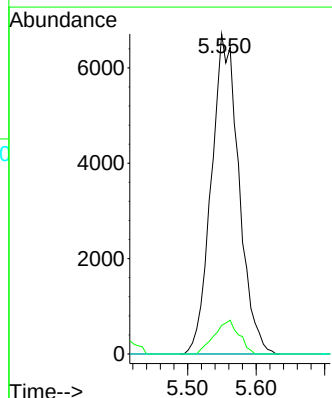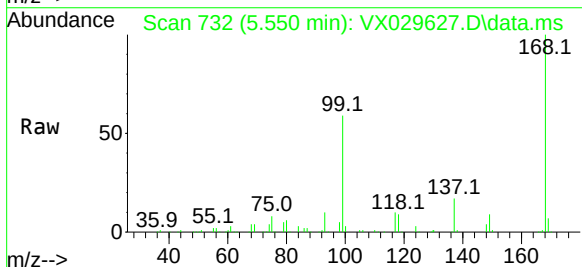



#37

Ethyl Acetate

Concen: 28.735 ug/l

RT: 4.562 min Scan# 51

Delta R.T. -0.159 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :

M15848





Tgt Ion: 43 Resp: 109471

Ion Ratio Lower Upper

43 100

61 0.0 12.6 19.0#

70 0.0 10.2 15.2#

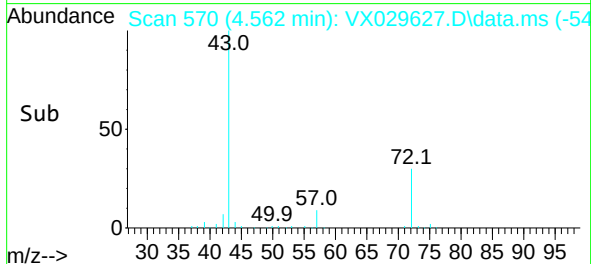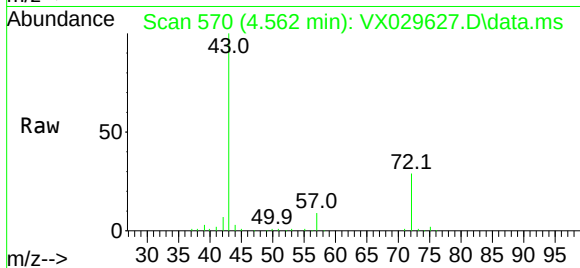

#38

Carbon Tetrachloride

Concen: 7.117 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 117 Resp: 26010


Ion Ratio Lower Upper

117 100

119 4.0 77.3 115.9#

121 0.0 24.2 36.2#


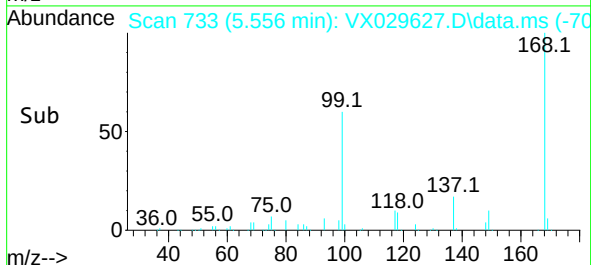
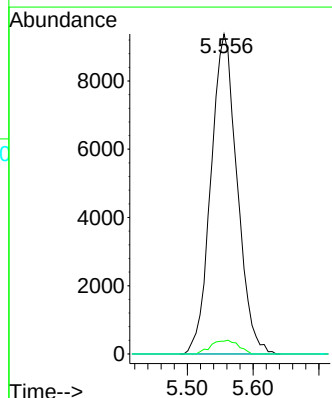
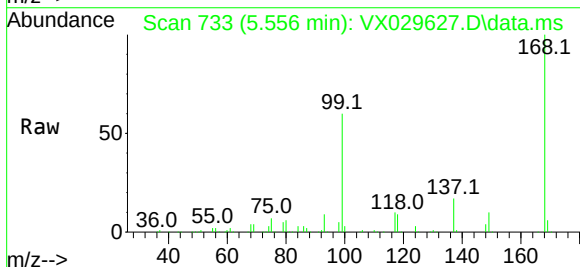


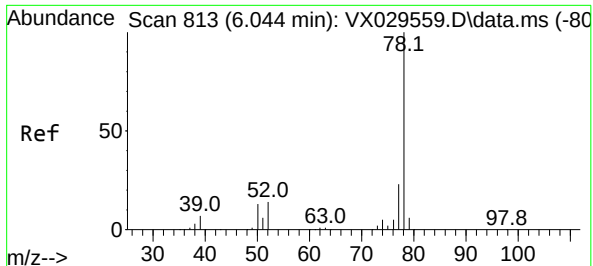

#40
Benzene
Concen: 0.269 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 78 Resp: 2965
Ion Ratio Lower Upper
78 100
77 23.1 19.3 28.9

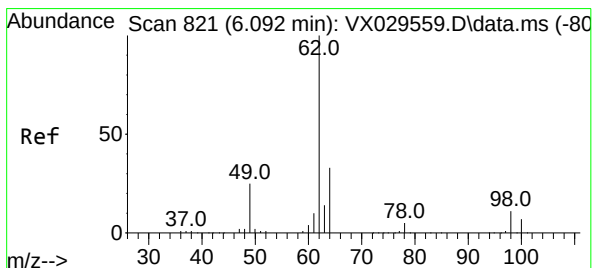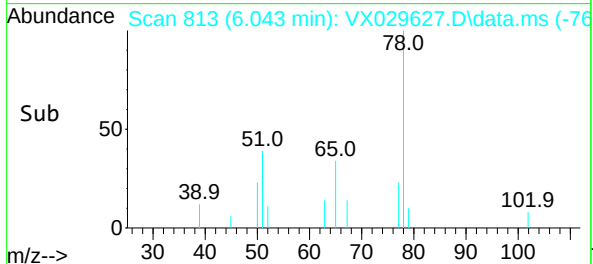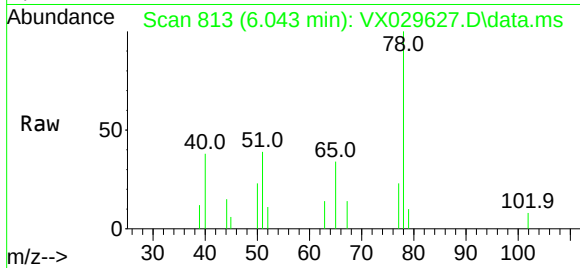

#42
1,2-Dichloroethane
Concen: 0.319 ug/l
RT: 6.110 min Scan# 824
Delta R.T. 0.018 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 62 Resp: 1208
Ion Ratio Lower Upper
62 100
98 6.8 0.0 20.4


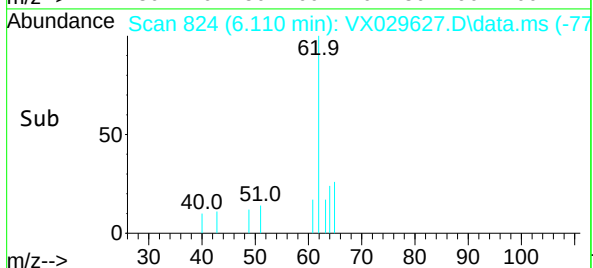

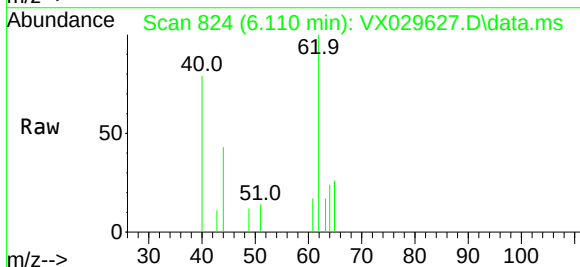




#43
Isopropyl Acetate
Concen: 0.818 ug/l
RT: 6.245 min Scan# 84
Delta R.T. -0.097 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 43 Resp: 4848
Ion Ratio Lower Upper
43 100
61 0.0 18.5 27.7#
87 0.0 13.0 19.6#

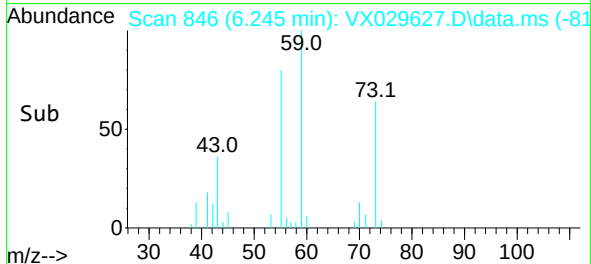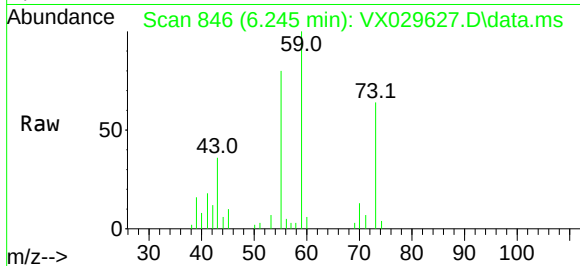

#44
Trichloroethene
Concen: Below Cal
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion:130 Resp: 1741
Ion Ratio Lower Upper
130 100
95 95.9 0.0 188.8

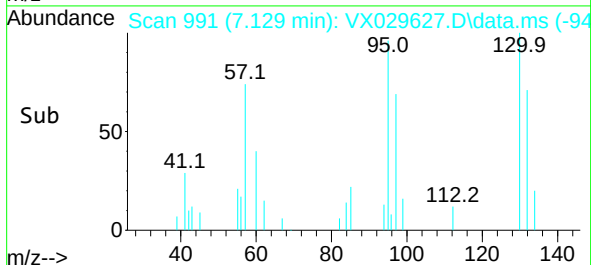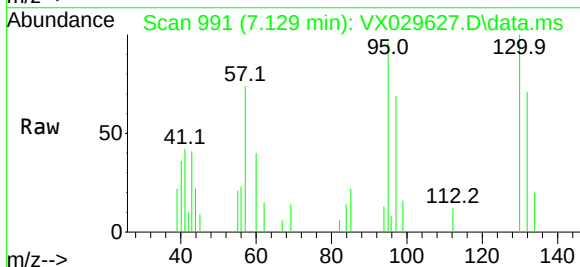

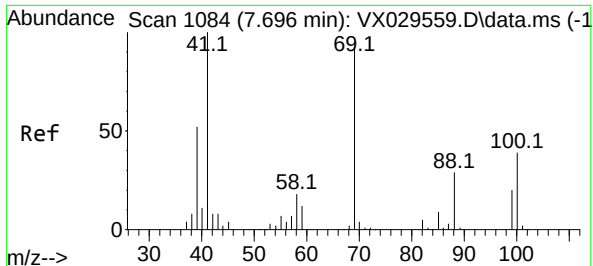

#48

Methyl methacrylate

Concen: 0.785 ug/l

RT: 7.592 min Scan# 1067

Delta R.T. -0.104 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :

M15848





Tgt Ion: 41 Resp: 2279

Ion Ratio Lower Upper

41 100

69 0.0 82.5 123.7#

39 44.8 43.8 65.8

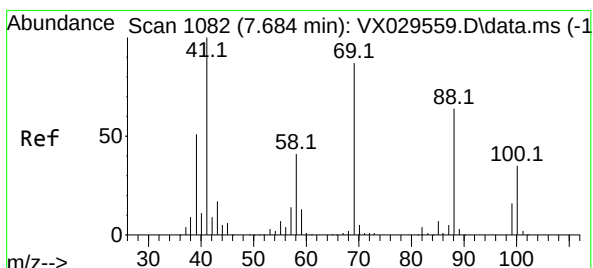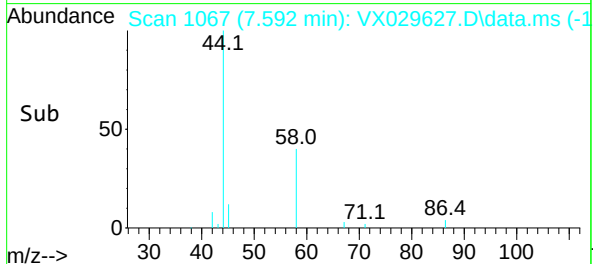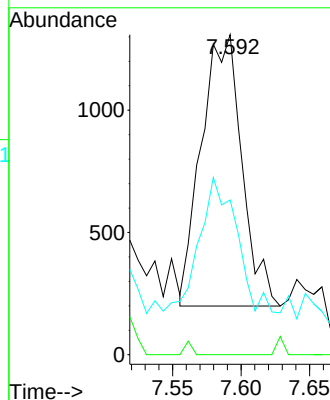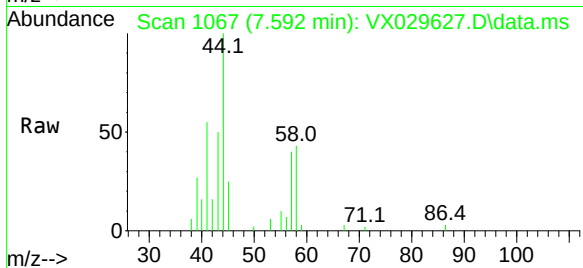

#49

1,4-Dioxane

Concen: 4.967 ug/l

RT: 7.482 min Scan# 1049

Delta R.T. -0.202 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 88 Resp: 372


Ion Ratio Lower Upper

88 100

43 0.0 21.9 32.9#

58 0.0 53.7 80.5#


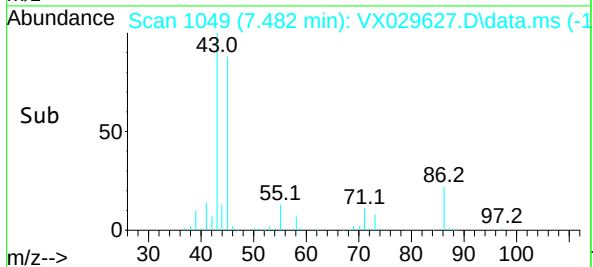
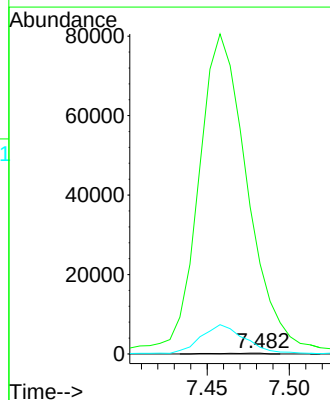
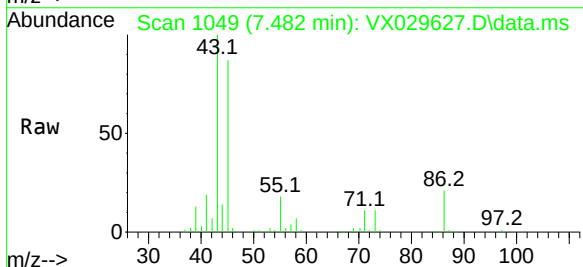




#50
Toluene-d8
Concen: 48.255 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 98 Resp: 484081
Ion Ratio Lower Upper
98 100
100 66.1 52.6 78.8

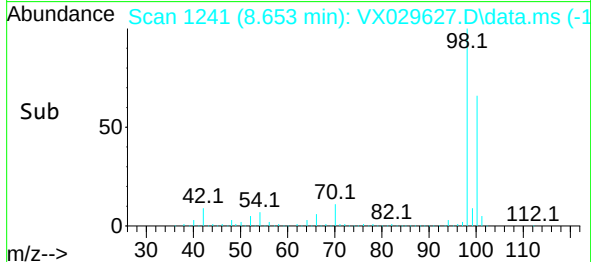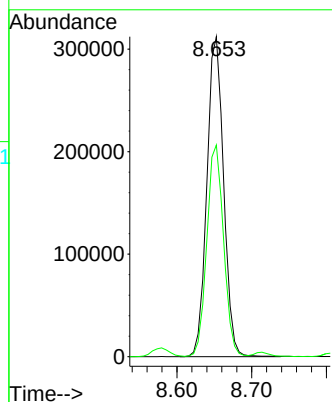

#51
4-Methyl-2-Pentanone
Concen: 18.503 ug/l
RT: 8.573 min Scan# 1228
Delta R.T. -0.001 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 43 Resp: 70650
Ion Ratio Lower Upper
43 100
58 42.4 36.1 54.1

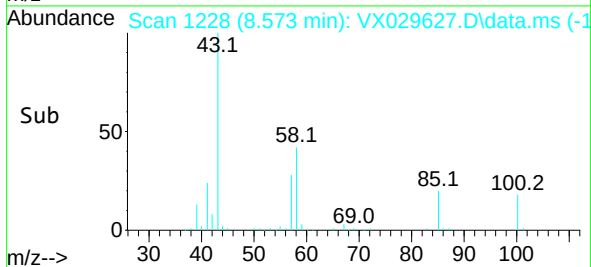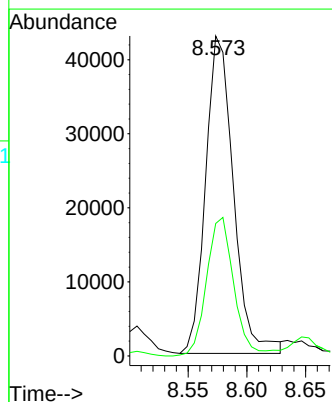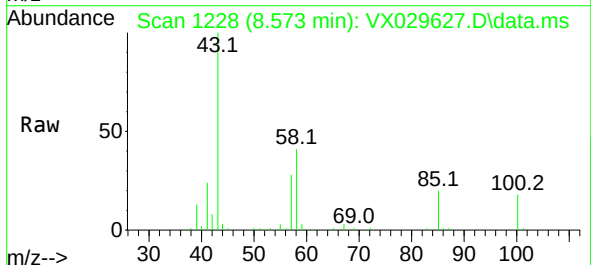



#59

2-Hexanone

Concen: 15.529 ug/l

RT: 9.433 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49

Instrument :

MSVOA_X

ClientSampleId :





M15848

Tgt Ion: 43 Resp: 44901

Ion Ratio Lower Upper

43 100

58 55.0 31.9 95.7

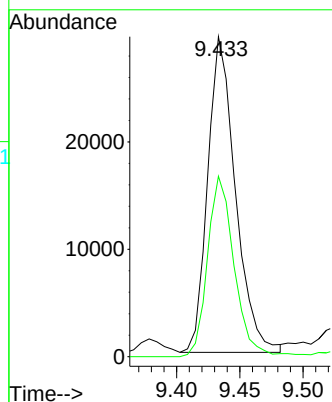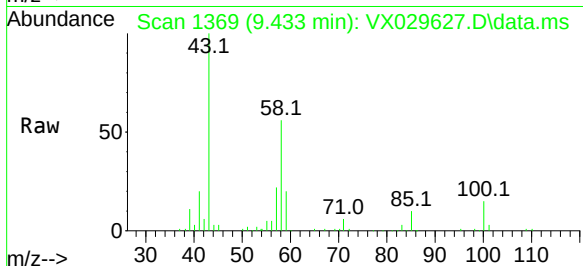

#62

4-Bromofluorobenzene

Concen: 46.128 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX029627.D

Acq: 20 Jun 2022 16:49




Tgt Ion: 95 Resp: 174507


Ion Ratio Lower Upper

95 100

174 71.9 0.0 163.0

176 70.1 0.0 155.0


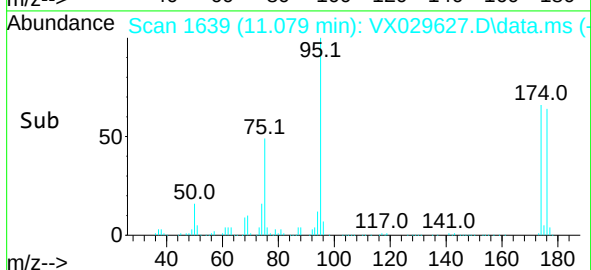

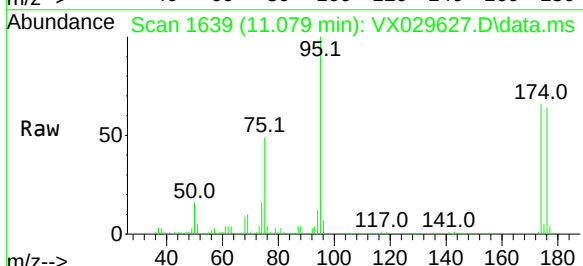




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion:117 Resp: 366985
Ion Ratio Lower Upper
117 100
82 54.3 41.8 62.8
119 31.3 24.8 37.2

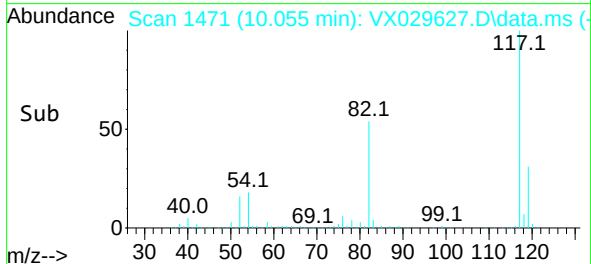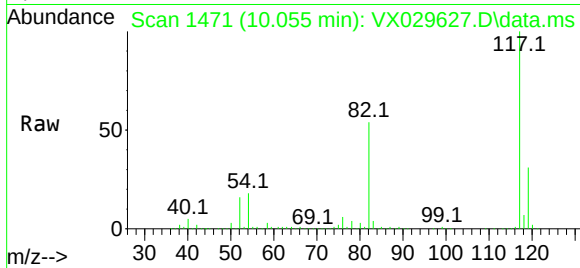

#65
Chlorobenzene
Concen: 0.573 ug/l
RT: 10.274 min Scan# 1507
Delta R.T. 0.195 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion:112 Resp: 4125
Ion Ratio Lower Upper
112 100
114 1.8 25.8 38.8#


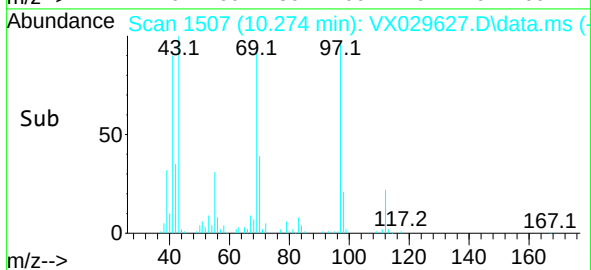
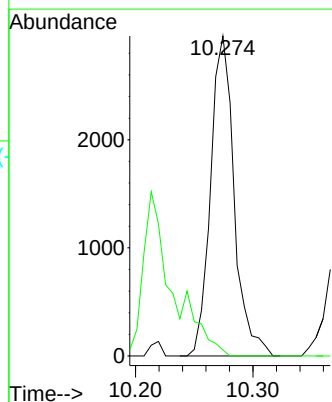
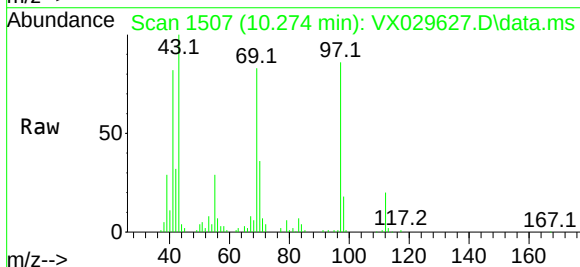


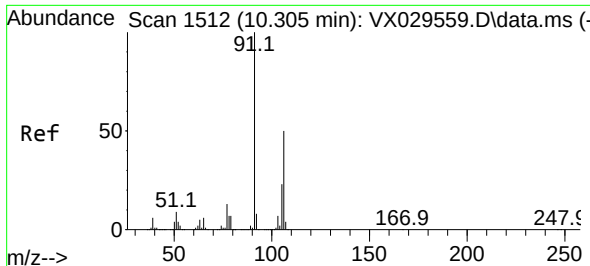

#68
m/p-Xylenes
Concen: 0.216 ug/l
RT: 10.305 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion:106 Resp: 1093
Ion Ratio Lower Upper
106 100
91 237.8 160.4 240.6

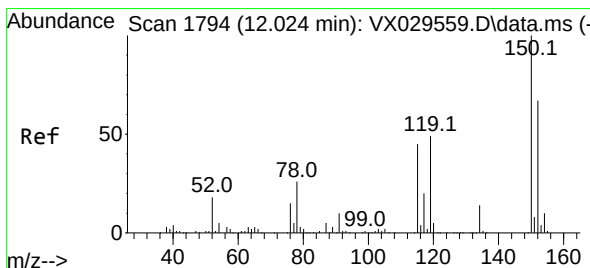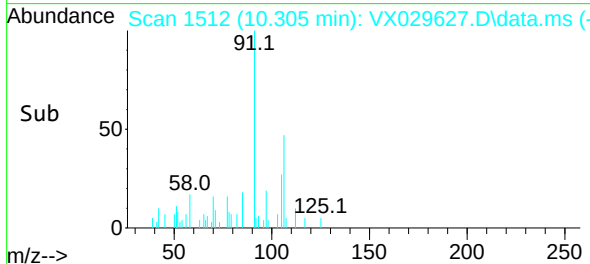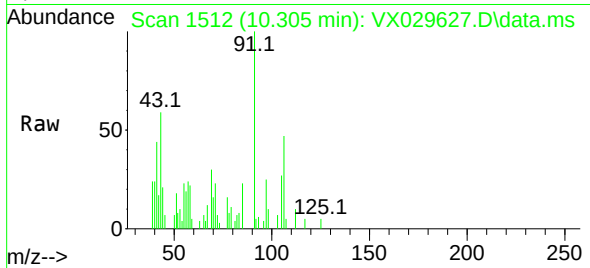

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion:152 Resp: 161080
Ion Ratio Lower Upper
152 100
115 62.9 37.5 112.7
150 159.0 0.0 338.2


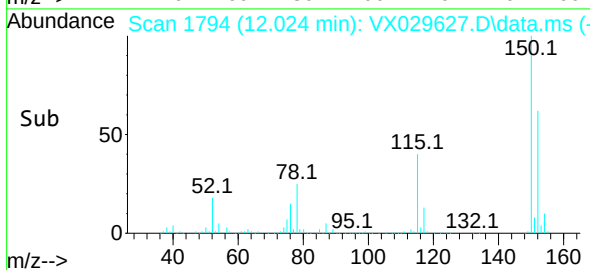

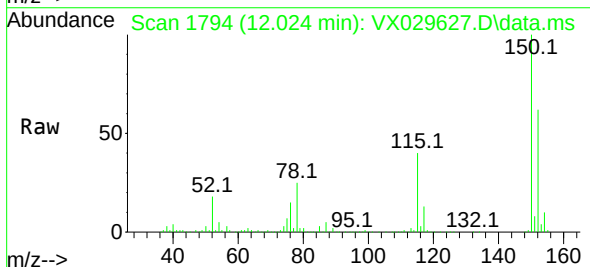




#74
N-amy1 acetate
Concen: 4.359 ug/l
RT: 10.890 min Scan# 1608
Delta R.T. 0.042 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 43	Resp: 18283
Ion Ratio	Lower Upper
43 100	
70 27.9	42.5 63.7#
55 39.9	23.1 34.7#
61 0.0	22.8 34.2#

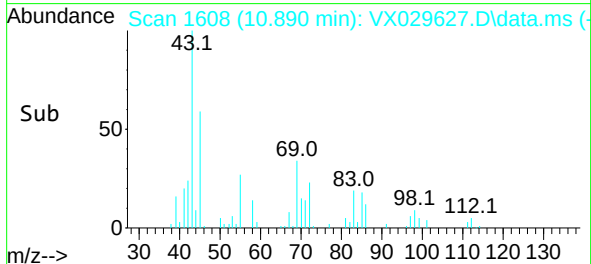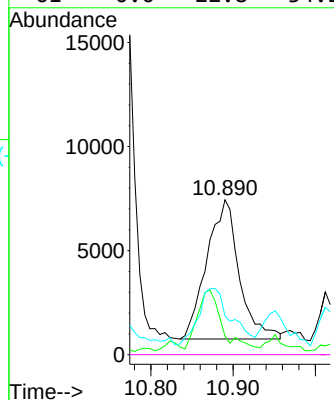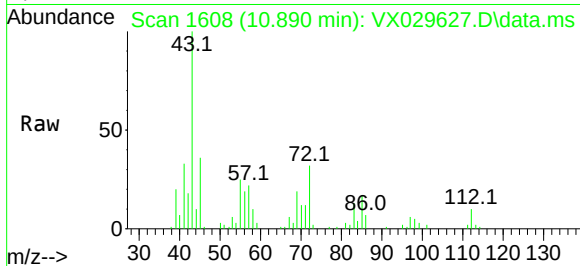

#76
1,2,3-Trichloropropane
Concen: 23.815 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 75	Resp: 83570
Ion Ratio	Lower Upper
75 100	
77 1.7	19.4 58.2#


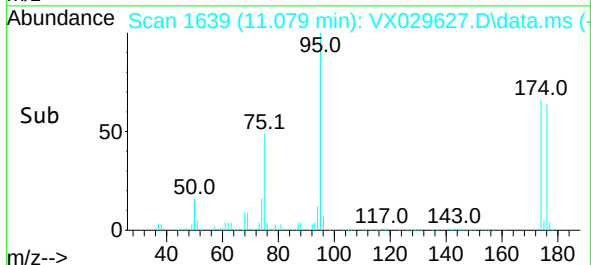
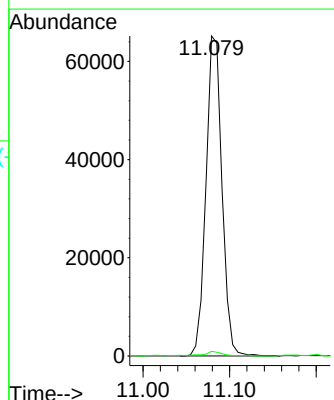
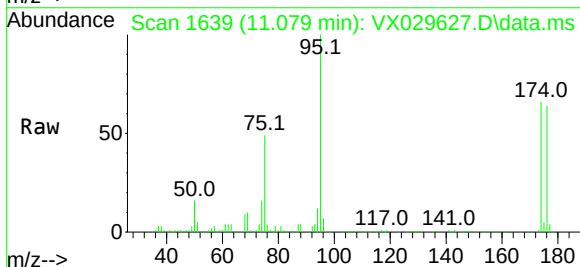




#81
trans-1,4-Dichloro-2-butene
Concen: 79.227 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49




Instrument :
MSVOA_X
ClientSampleId :
M15848


Tgt Ion: 75 Resp: 83570
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

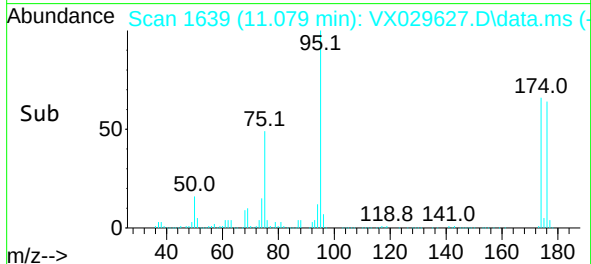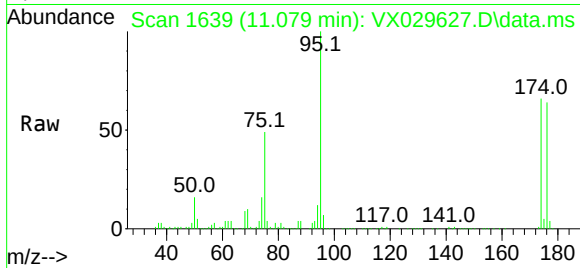

#84
1,2,4-Trimethylbenzene
Concen: 0.268 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 105 Resp: 2721
Ion Ratio Lower Upper
105 100
120 29.0 22.6 67.8


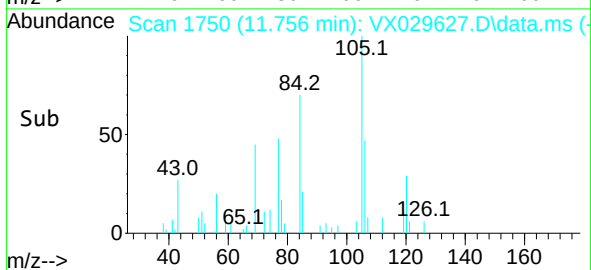

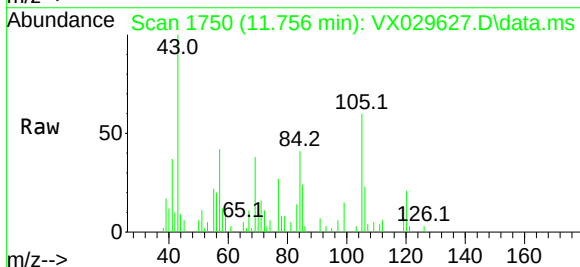




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.366 ug/l
RT: 12.804 min Scan# 1945
Delta R.T. -0.141 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Instrument :
MSVOA_X
ClientSampleId :
M15848

Tgt Ion: 75 Resp: 1182
Ion Ratio Lower Upper
75 100
155 0.0 47.0 141.2#
157 0.0 57.9 173.6#

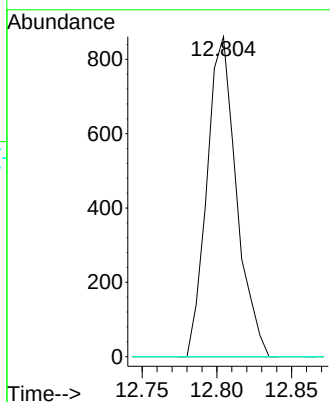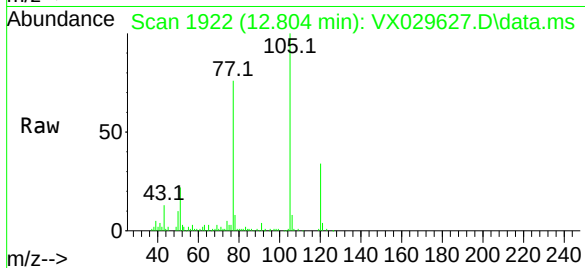

#95
Naphthalene
Concen: 0.306 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX029627.D
Acq: 20 Jun 2022 16:49

Tgt Ion: 128 Resp: 3459
Ion Ratio Lower Upper
128 100
127 17.5 10.2 15.4#
129 14.0 8.7 13.1#

