

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
 Data File : VX029631.D
 Acq On : 20 Jun 2022 18:23
 Operator : JC/MD
 Sample : N3339-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-GW-20220613

Quant Time: Jun 21 01:52:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	260676	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	435384	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	378396	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	160985	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	148233	42.958	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	85.920%		
35) Dibromofluoromethane	5.391	113	77381	27.272	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	54.540%#		
50) Toluene-d8	8.652	98	494097	47.668	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.340%		
62) 4-Bromofluorobenzene	11.085	95	174932	44.752	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	89.500%		
Target Compounds					Qvalue	
3) Chloromethane	1.294	50	883	0.260	ug/l	94
5) Bromomethane	1.617	94	556	0.348	ug/l #	59
6) Chloroethane	1.684	64	129	1.344	ug/l #	43
10) Methyl Iodide	2.458	142	274	3.100	ug/l #	75
11) Tert butyl alcohol	2.971	59	1081	Below Cal	#	72
13) Acrolein	2.239	56	174	0.915	ug/l #	1
14) Allyl chloride	2.654	41	1092	0.256	ug/l #	44
16) Acetone	2.385	43	40581	29.505	ug/l	100
17) Carbon Disulfide	2.513	76	1564	0.228	ug/l #	95
20) Methylene Chloride	2.794	84	3798	1.240	ug/l	97
25) 2-Butanone	4.580	43	8406	3.867	ug/l	94
28) Bromochloromethane	5.098	49	2632	1.358	ug/l #	7
30) Chloroform	5.104	83	40382	7.522	ug/l	97
36) 1,1-Dichloropropene	5.556	75	19706	5.132	ug/l #	50
37) Ethyl Acetate	4.580	43	8406	2.136	ug/l #	65
38) Carbon Tetrachloride	5.556	117	26687	7.067	ug/l #	15
40) Benzene	6.043	78	7600	0.668	ug/l	100
44) Trichloroethene	7.128	130	2258	Below Cal		82
51) 4-Methyl-2-Pentanone	8.585	43	3078	0.780	ug/l	100
52) Toluene	8.720	92	22993	3.154	ug/l	100
59) 2-Hexanone	9.439	43	1431	0.479	ug/l	96
67) Ethyl Benzene	10.195	91	14181	1.062	ug/l	99
68) m/p-Xylenes	10.305	106	20842	4.001	ug/l	93
69) o-Xylene	10.646	106	13843	2.690	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	85243	24.306	ug/l #	38
80) 1,3,5-Trimethylbenzene	11.457	105	5011	0.493	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	85243	80.861	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	14337	1.414	ug/l	94
85) sec-Butylbenzene	11.756	105	14337	1.167	ug/l #	56
95) Naphthalene	13.780	128	24340	2.155	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
Data File : VX029631.D
Acq On : 20 Jun 2022 18:23
Operator : JC/MD
Sample : N3339-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613

Quant Time: Jun 21 01:52:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




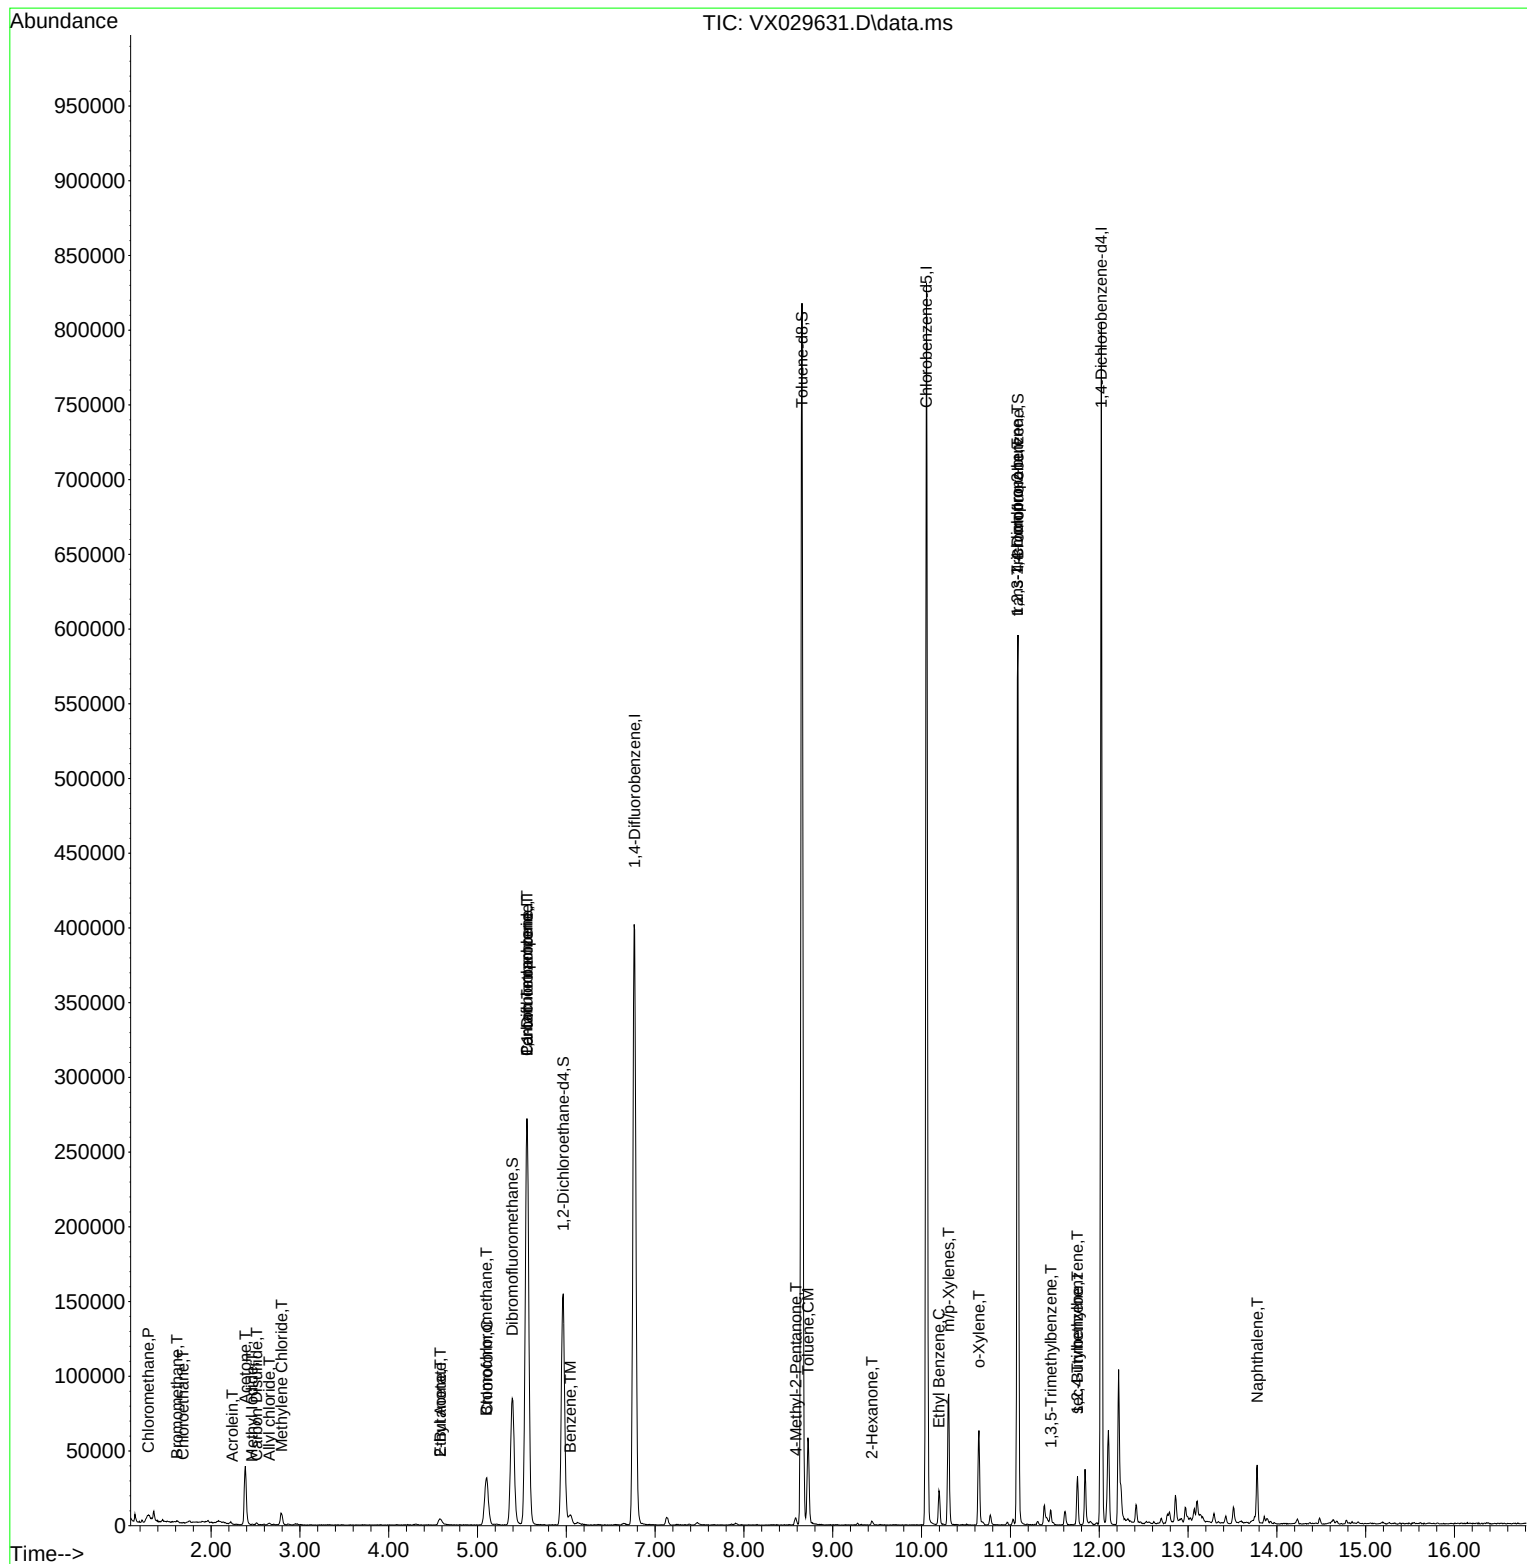


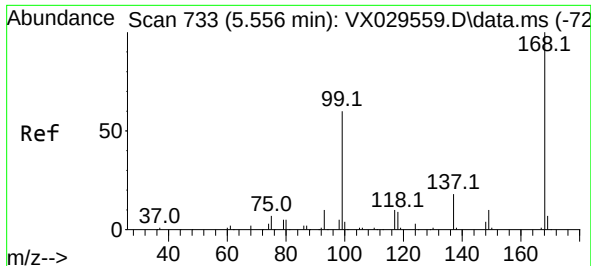

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion:168 Resp: 260676
Ion Ratio Lower Upper
168 100
99 61.2 41.7 62.5



#3
Chloromethane
Concen: 0.260 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 50 Resp: 883
Ion Ratio Lower Upper
50 100
52 29.3 26.4 39.6







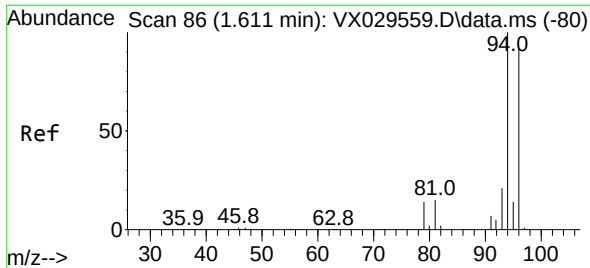

#5
Bromomethane
Concen: 0.348 ug/l
RT: 1.617 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 94 Resp: 556
Ion Ratio Lower Upper
94 100
96 54.1 75.3 112.9#

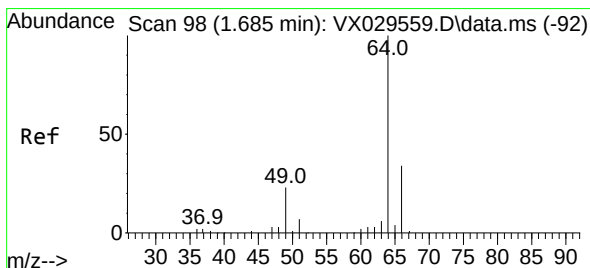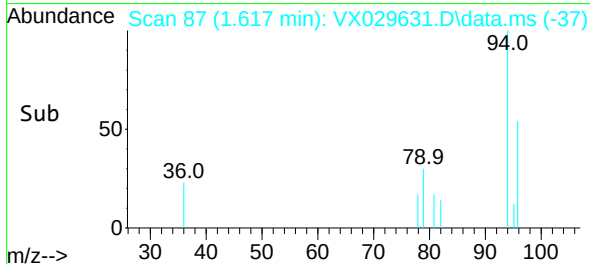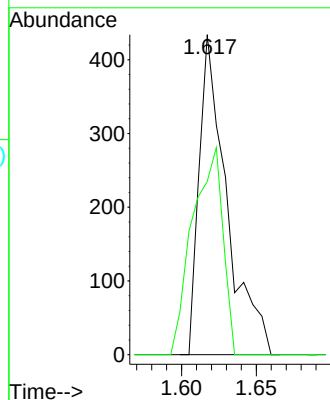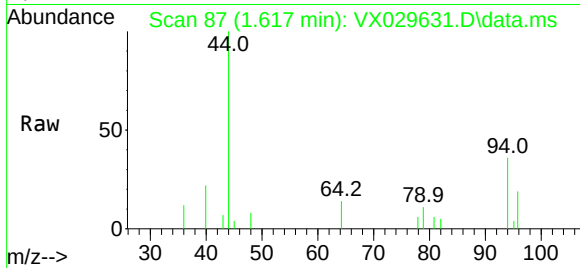

#6
Chloroethane
Concen: 1.344 ug/l
RT: 1.684 min Scan# 98
Delta R.T. -0.001 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 64 Resp: 129
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#


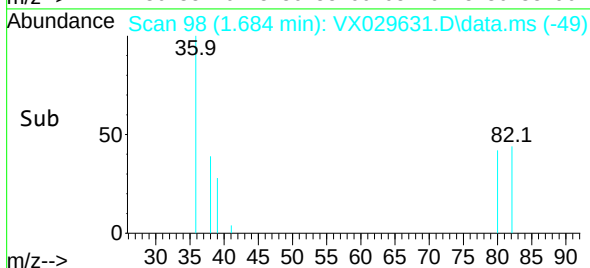
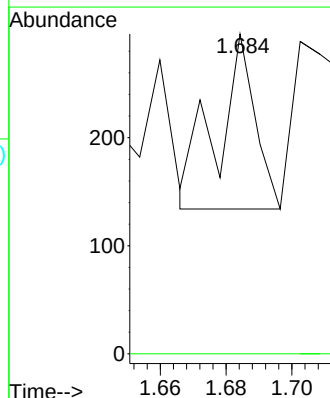
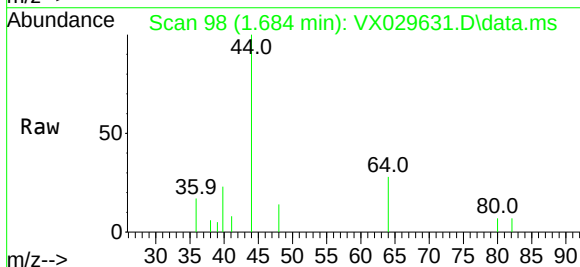


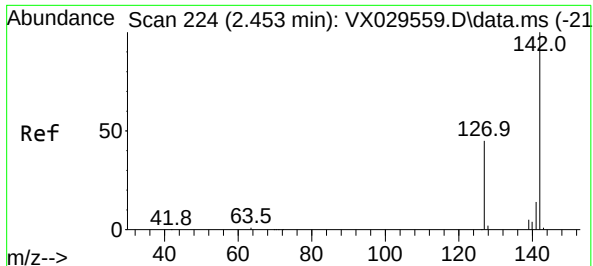

#10
Methyl Iodide
Concen: 3.100 ug/l
RT: 2.458 min Scan# 21
Delta R.T. 0.005 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion:142 Resp: 274
Ion Ratio Lower Upper
142 100
127 28.5 33.9 50.9#
141 0.0 11.4 17.2#

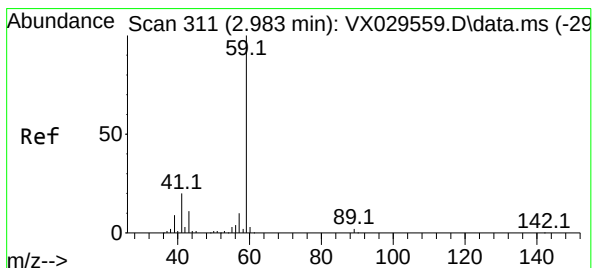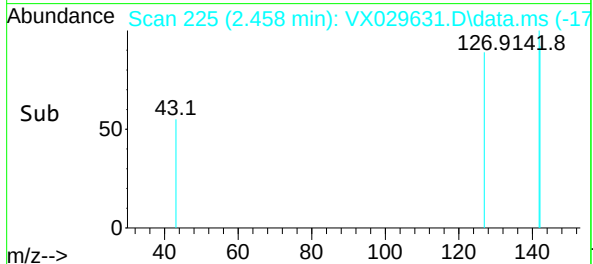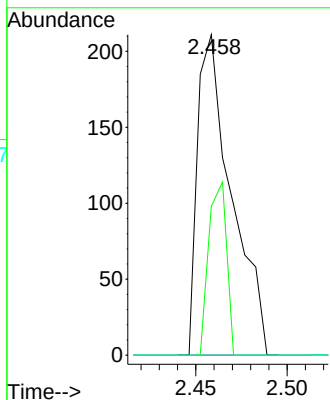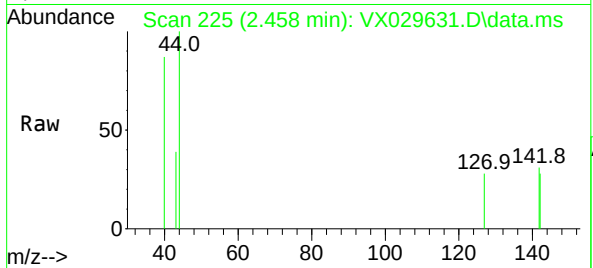

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 59 Resp: 1081
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

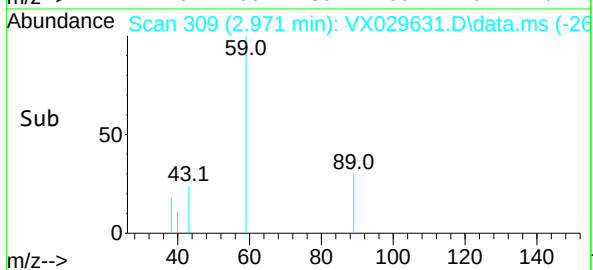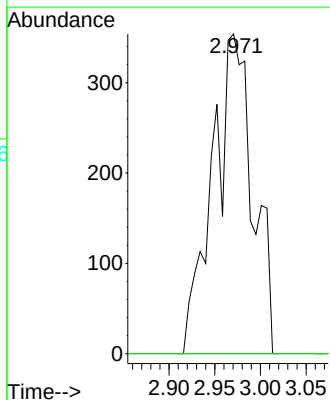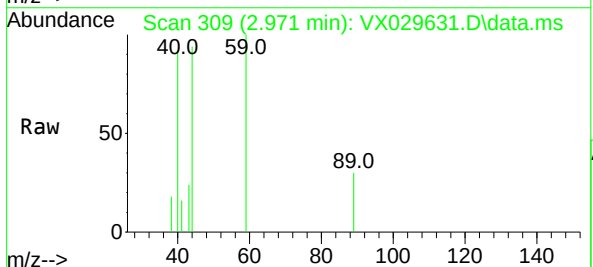

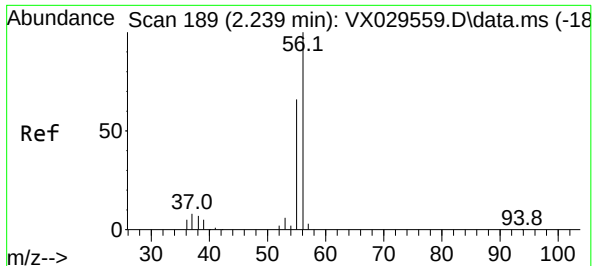

#13

Acrolein

Concen: 0.915 ug/l

RT: 2.239 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :





WC-GW-20220613

Tgt Ion: 56 Resp: 174

Ion Ratio Lower Upper

56 100

55 458.6 55.0 82.6#

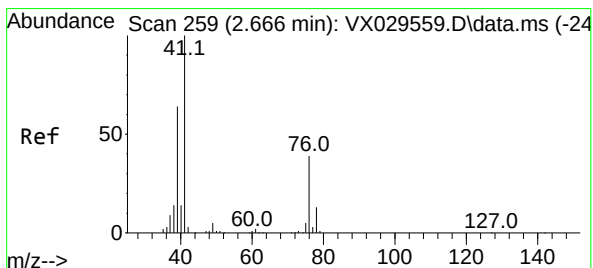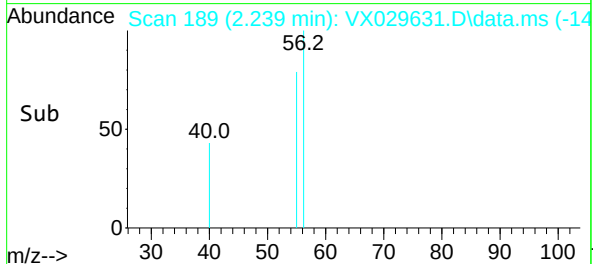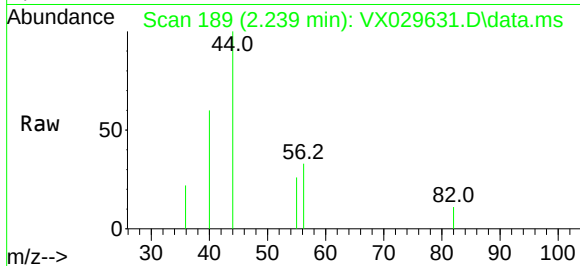

#14

Allyl chloride

Concen: 0.256 ug/l

RT: 2.654 min Scan# 257

Delta R.T. -0.012 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23




Tgt Ion: 41 Resp: 1092


Ion Ratio Lower Upper

41 100

39 23.7 50.4 75.6#

76 0.0 32.7 49.1#


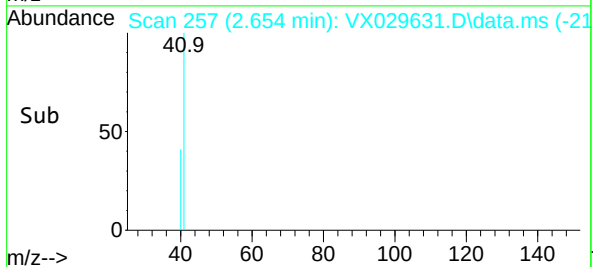

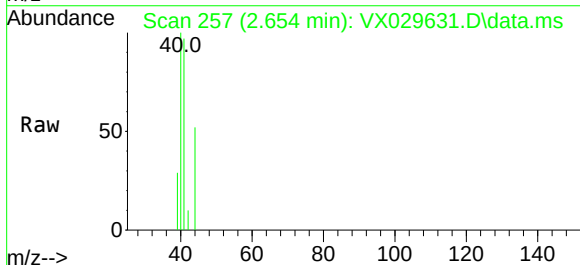




#16
Acetone
Concen: 29.505 ug/l
RT: 2.385 min Scan# 213
Delta R.T. -0.001 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 43 Resp: 40581
Ion Ratio Lower Upper
43 100
58 35.8 28.8 43.2



#17
Carbon Disulfide
Concen: 0.228 ug/l
RT: 2.513 min Scan# 234
Delta R.T. -0.001 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 76 Resp: 1564
Ion Ratio Lower Upper
76 100
78 10.8 7.2 10.8#



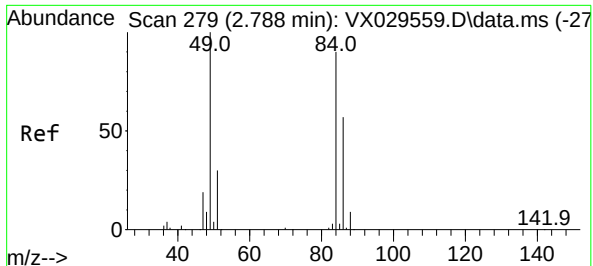

#20

Methylene Chloride

Concen: 1.240 ug/l

RT: 2.794 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX029631.D


Acq: 20 Jun 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :

WC-GW-20220613

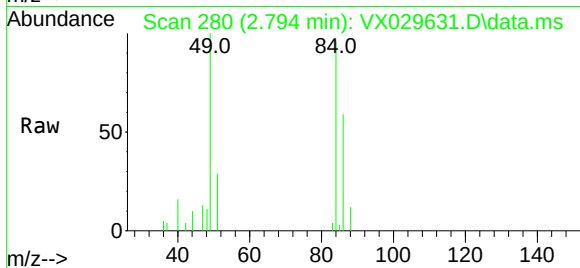

Tgt Ion: 84 Resp: 3798




Ion Ratio Lower Upper

84 100

49 104.2 85.5 128.3

51 30.6 26.6 39.8

86 61.1 51.5 77.3

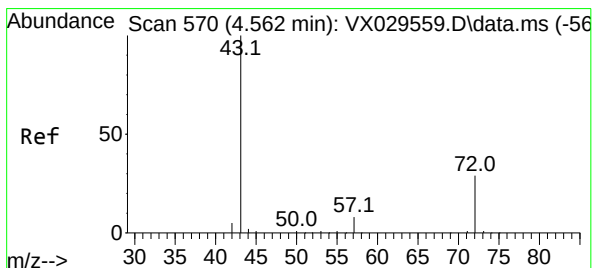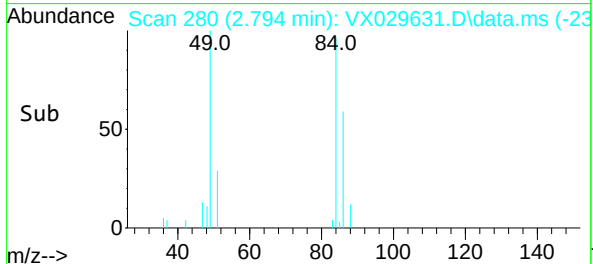

#25

2-Butanone

Concen: 3.867 ug/l

RT: 4.580 min Scan# 573

Delta R.T. 0.018 min

Lab File: VX029631.D




Acq: 20 Jun 2022 18:23


Tgt Ion: 43 Resp: 8406

Ion Ratio Lower Upper

43 100

72 27.1 24.4 36.6


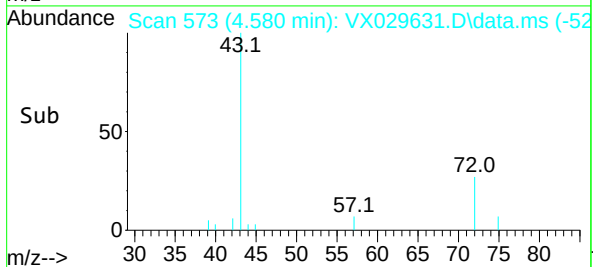

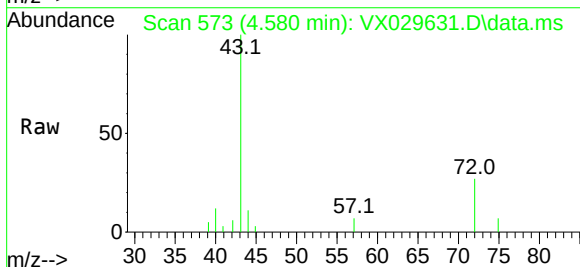


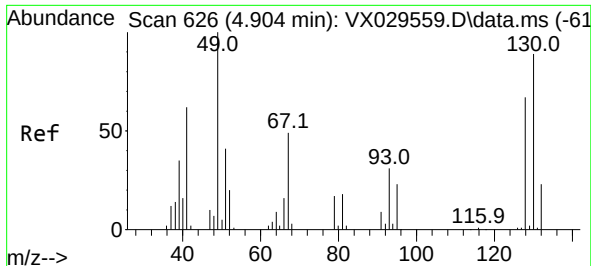

#28
Bromochloromethane
Concen: 1.358 ug/l
RT: 5.098 min Scan# 61
Delta R.T. 0.194 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 49 Resp: 2632
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.4
130 0.0 70.7 106.1#

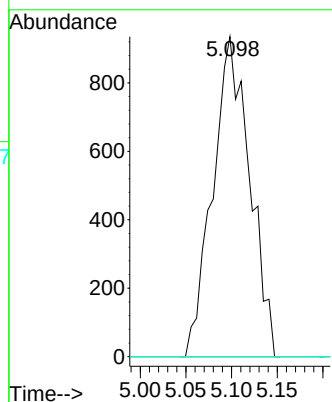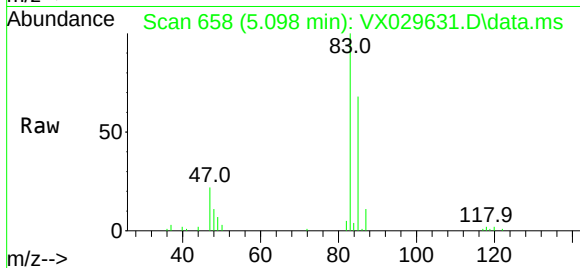

#30
Chloroform
Concen: 7.522 ug/l
RT: 5.104 min Scan# 659
Delta R.T. 0.005 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 83 Resp: 40382
Ion Ratio Lower Upper
83 100
85 63.5 52.7 79.1

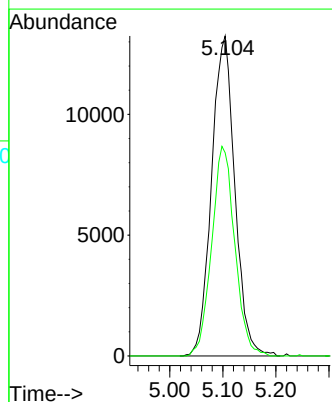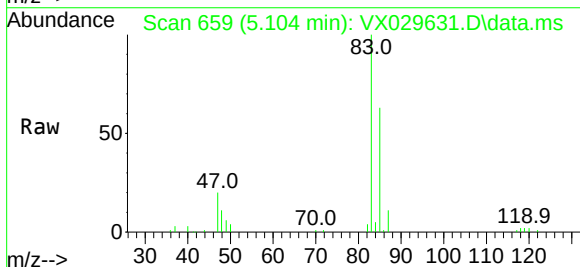

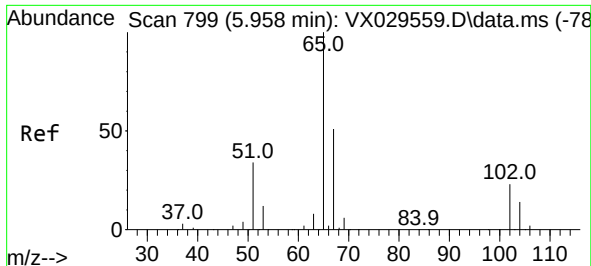

#33

1,2-Dichloroethane-d4

Concen: 42.958 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :





WC-GW-20220613

Tgt Ion: 65 Resp: 148233

Ion Ratio Lower Upper

65 100

67 53.3 0.0 107.4

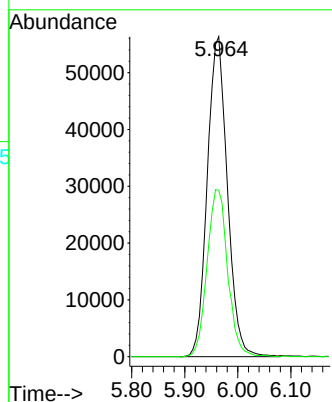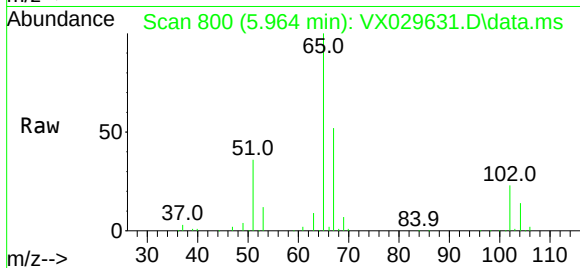

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23




Tgt Ion: 114 Resp: 435384


Ion Ratio Lower Upper

114 100

63 19.1 0.0 36.8

88 16.3 0.0 32.4

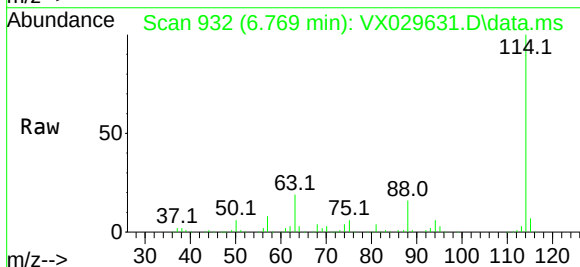

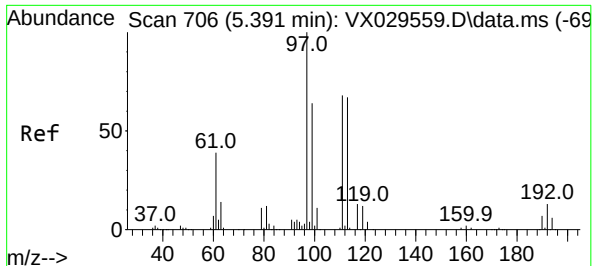

#35

Dibromofluoromethane

Concen: 27.272 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX029631.D


Acq: 20 Jun 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :

WC-GW-20220613

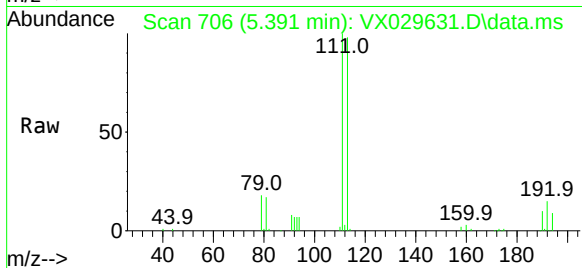




Tgt Ion:113 Resp: 77381

Ion Ratio Lower Upper

113 100

111 104.2 82.8 124.2

192 18.1 16.9 25.3

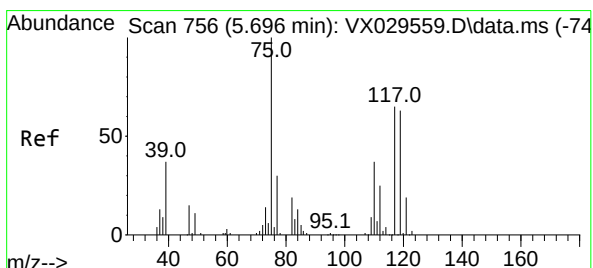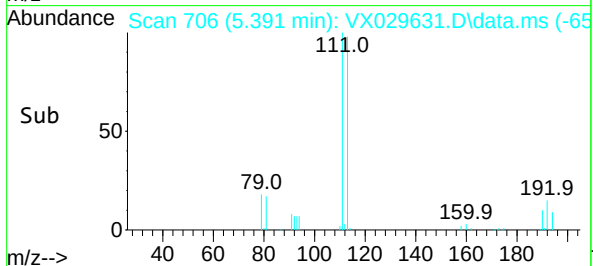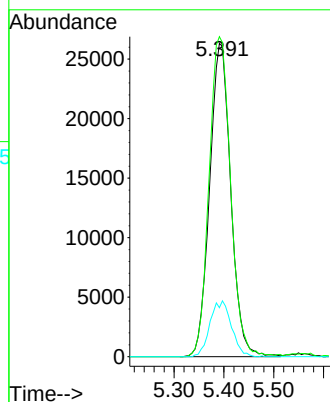

#36

1,1-Dichloropropene

Concen: 5.132 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23




Tgt Ion: 75 Resp: 19706


Ion Ratio Lower Upper

75 100

110 9.8 18.3 54.8#

77 0.0 24.8 37.2#

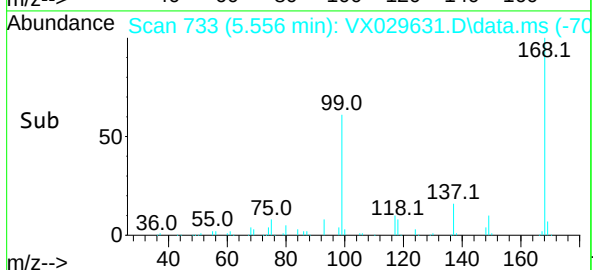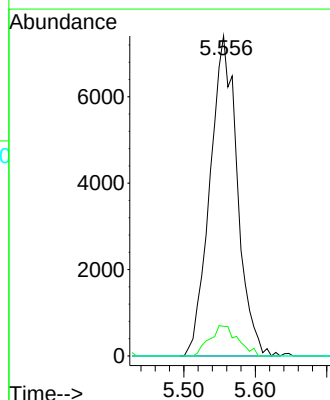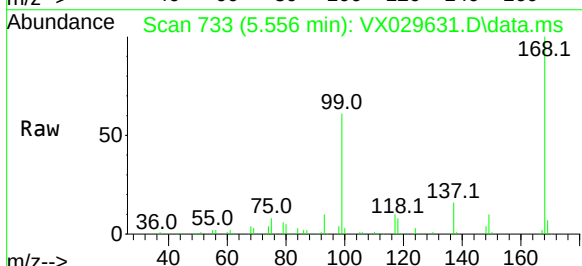

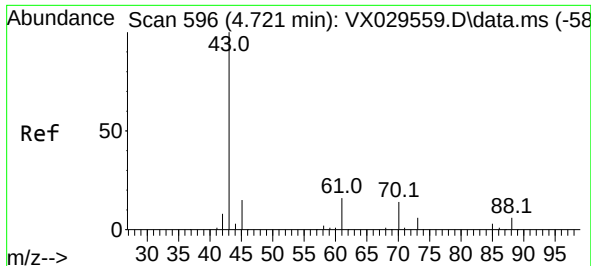

#37

Ethyl Acetate

Concen: 2.136 ug/l

RT: 4.580 min Scan# 51

Delta R.T. -0.141 min

Lab File: VX029631.D


Acq: 20 Jun 2022 18:23

Instrument :




MSVOA_X

ClientSampleId :

WC-GW-20220613

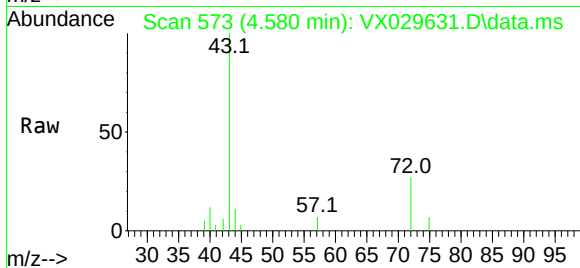

Tgt Ion: 43	Resp: 8406
Ion Ratio	Lower Upper
43	100
61	0.0 12.6 19.0#
70	0.0 10.2 15.2#

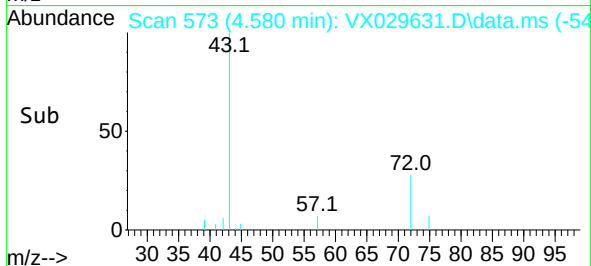

#38

Carbon Tetrachloride

Concen: 7.067 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.128 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23

Tgt Ion: 117	Resp: 26687
Ion Ratio	Lower Upper
117	100
119	4.8 77.3 115.9#
121	0.0 24.2 36.2#


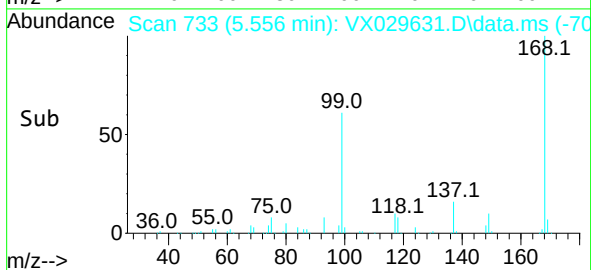

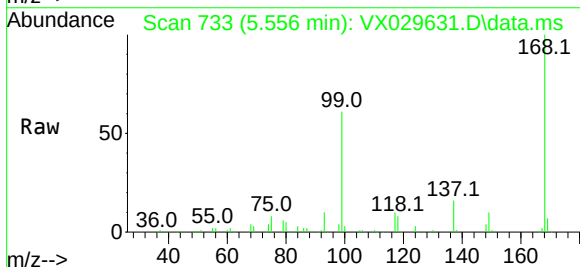


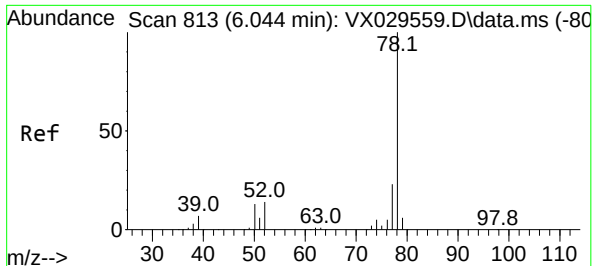

#40
Benzene
Concen: 0.668 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 78 Resp: 7600
Ion Ratio Lower Upper
78 100
77 23.9 19.3 28.9

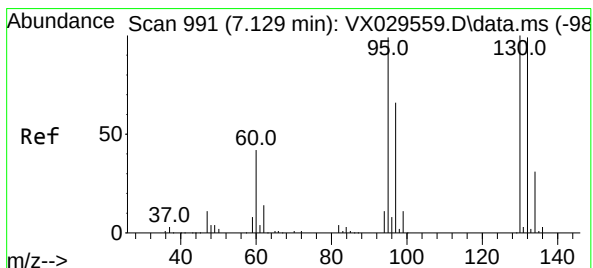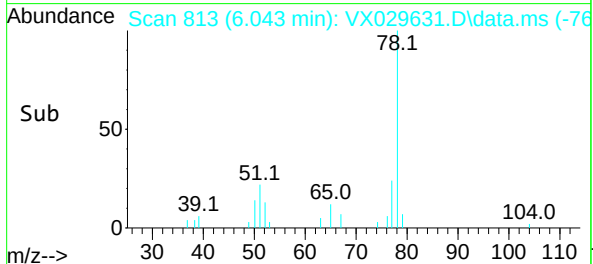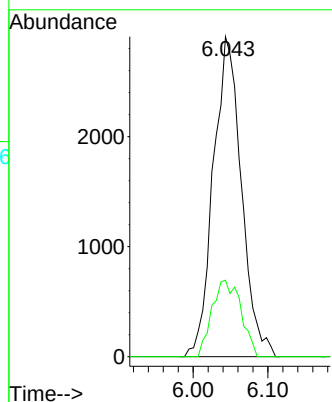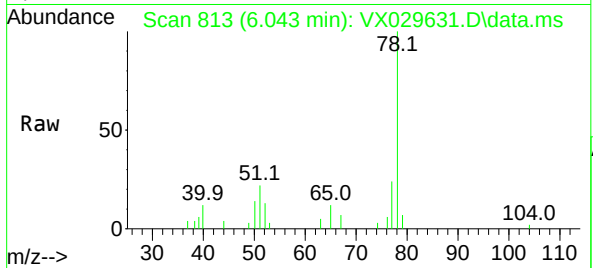

#44
Trichloroethene
Concen: Below Cal
RT: 7.128 min Scan# 991
Delta R.T. -0.001 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion:130 Resp: 2258
Ion Ratio Lower Upper
130 100
95 111.5 0.0 188.8


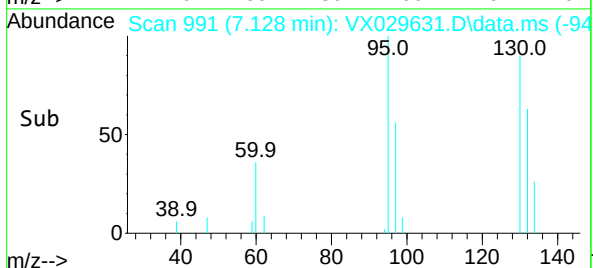

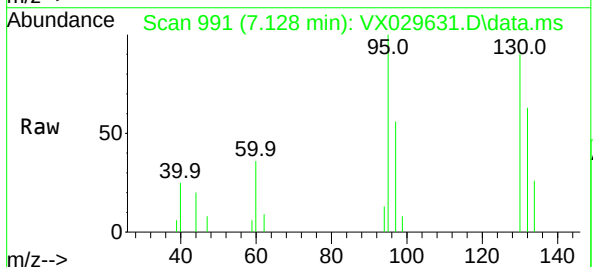




#50
Toluene-d8
Concen: 47.668 ug/l
RT: 8.652 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 98 Resp: 494097
Ion Ratio Lower Upper
98 100
100 67.5 52.6 78.8

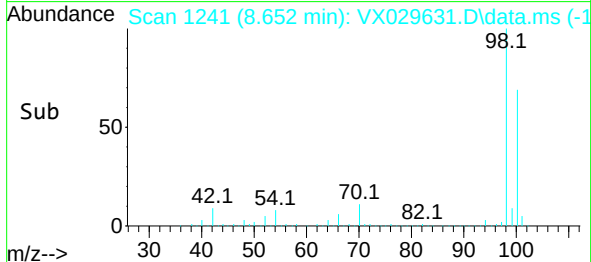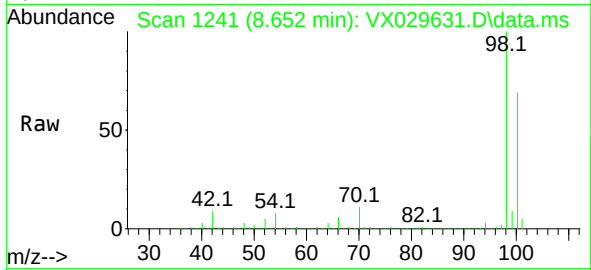

#51
4-Methyl-2-Pentanone
Concen: 0.780 ug/l
RT: 8.585 min Scan# 1230
Delta R.T. 0.011 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 43 Resp: 3078
Ion Ratio Lower Upper
43 100
58 45.2 36.1 54.1









#52
Toluene
Concen: 3.154 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 92 Resp: 22993
Ion Ratio Lower Upper
92 100
91 171.2 137.5 206.3

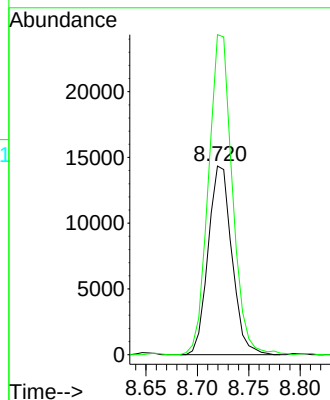

#59
2-Hexanone
Concen: 0.479 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 43 Resp: 1431
Ion Ratio Lower Upper
43 100
58 60.3 31.9 95.7



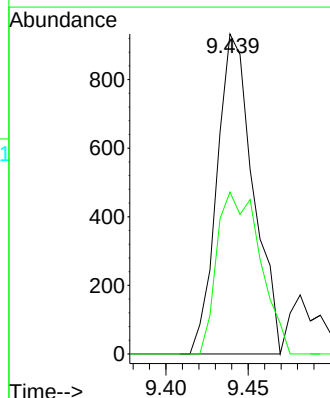





#62
4-Bromofluorobenzene
Concen: 44.752 ug/l
RT: 11.085 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 95 Resp: 174932
Ion Ratio Lower Upper
95 100
174 72.8 0.0 163.0
176 69.8 0.0 155.0

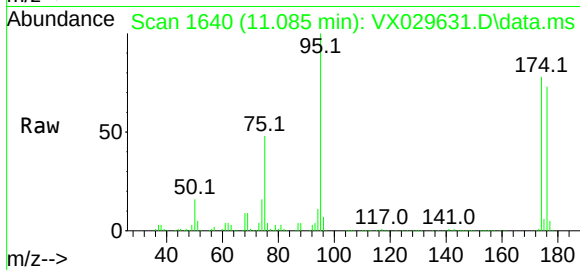

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 117 Resp: 378396
Ion Ratio Lower Upper
117 100
82 56.8 41.8 62.8
119 32.9 24.8 37.2

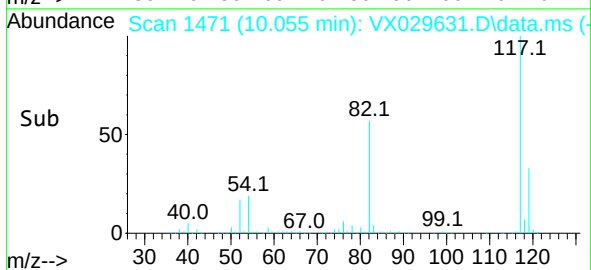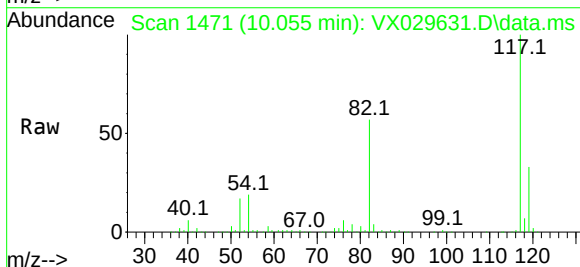

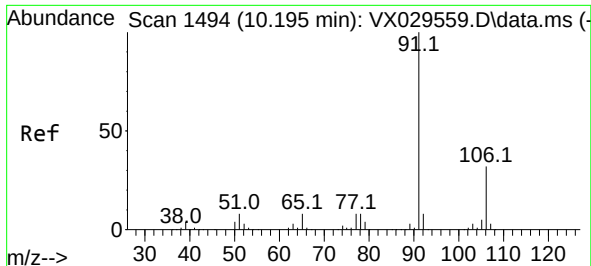

#67

Ethyl Benzene

Concen: 1.062 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX029631.D

Acq: 20 Jun 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :





WC-GW-20220613

Tgt Ion: 91 Resp: 14181

Ion Ratio Lower Upper

91 100

106 31.0 24.6 36.8

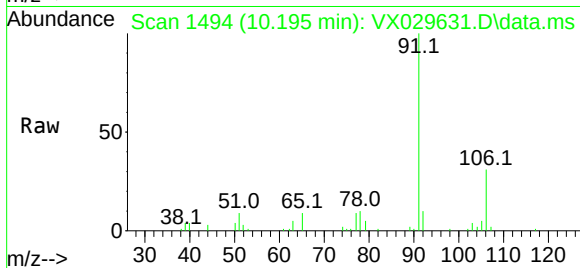

#68

m/p-Xylenes

Concen: 4.001 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX029631.D




Acq: 20 Jun 2022 18:23


Tgt Ion: 106 Resp: 20842

Ion Ratio Lower Upper

106 100

91 211.1 160.4 240.6









#69
o-Xylene
Concen: 2.690 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion:106 Resp: 13843
Ion Ratio Lower Upper
106 100
91 218.3 106.1 318.1

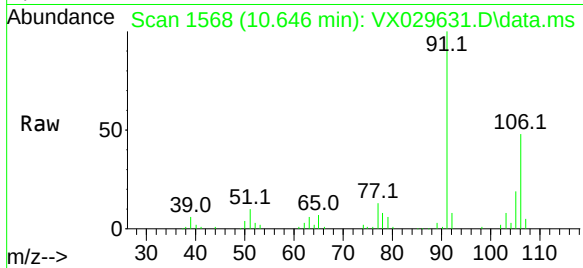

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion:152 Resp: 160985
Ion Ratio Lower Upper
152 100
115 63.2 37.5 112.7
150 157.8 0.0 338.2


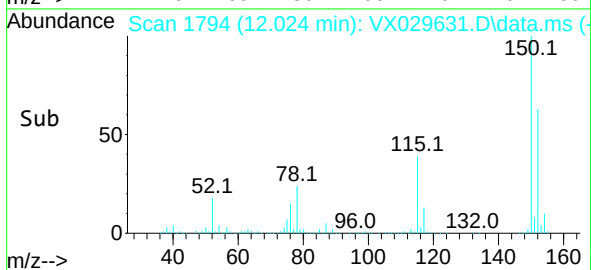

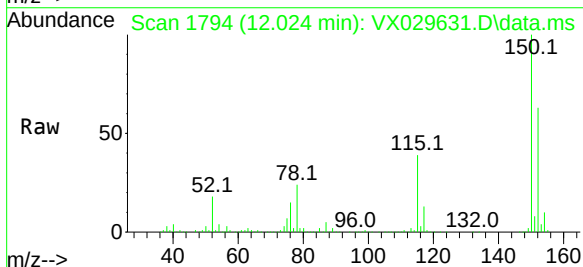




#76
 1,2,3-Trichloropropane
 Concen: 24.306 ug/l
 RT: 11.079 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: VX029631.D
 Acq: 20 Jun 2022 18:23




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-GW-20220613


Tgt Ion: 75 Resp: 85243
 Ion Ratio Lower Upper
 75 100
 77 1.3 19.4 58.2#

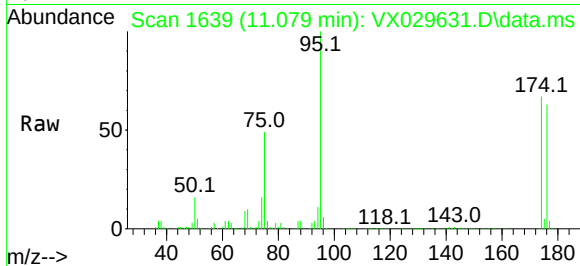

#80
 1,3,5-Trimethylbenzene
 Concen: 0.493 ug/l
 RT: 11.457 min Scan# 1701
 Delta R.T. 0.006 min
 Lab File: VX029631.D
 Acq: 20 Jun 2022 18:23

Tgt Ion: 105 Resp: 5011
 Ion Ratio Lower Upper
 105 100
 120 43.6 24.3 72.9




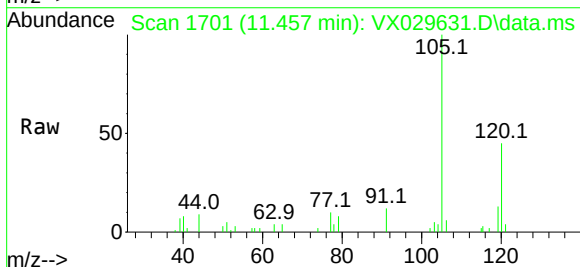


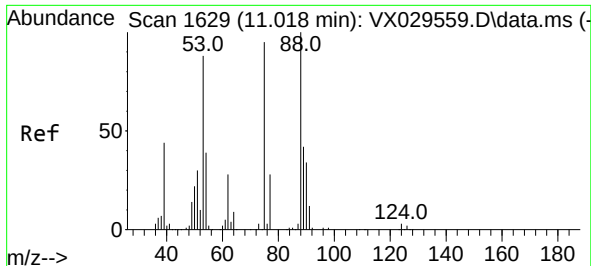

#81
trans-1,4-Dichloro-2-butene
Concen: 80.861 ug/l
RT: 11.079 min Scan# 1629
Delta R.T. 0.061 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613


Tgt Ion: 75 Resp: 85243
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

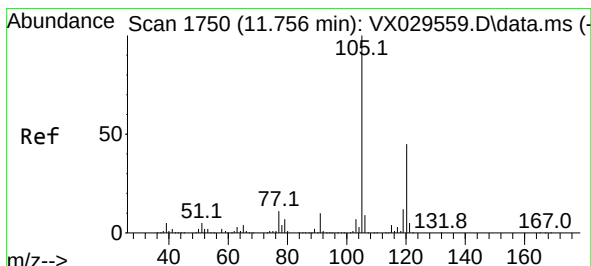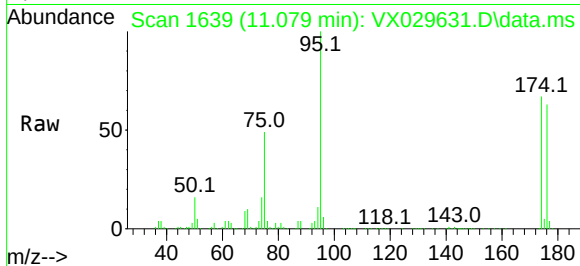

#84
1,2,4-Trimethylbenzene
Concen: 1.414 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion: 105 Resp: 14337
Ion Ratio Lower Upper
105 100
120 41.3 22.6 67.8


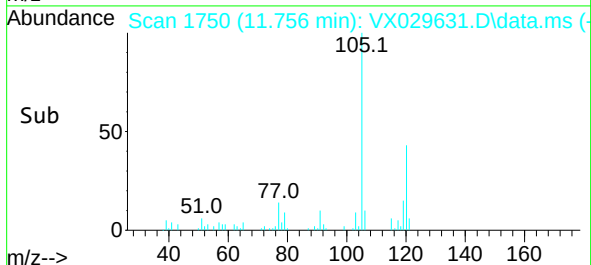

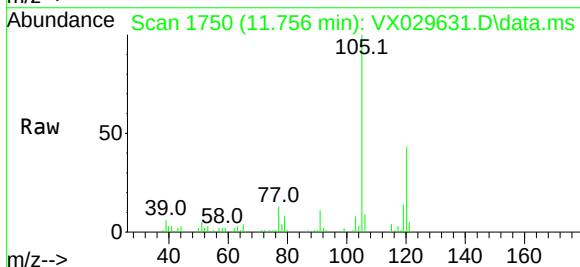


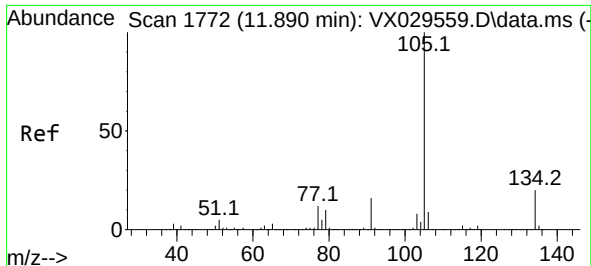

#85
sec-Butylbenzene
Concen: 1.167 ug/l
RT: 11.756 min Scan# 11
Delta R.T. -0.134 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Instrument :
MSVOA_X
ClientSampleId :
WC-GW-20220613

Tgt Ion:105 Resp: 14337
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#

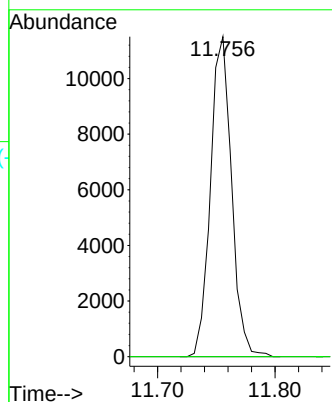

#95
Naphthalene
Concen: 2.155 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX029631.D
Acq: 20 Jun 2022 18:23

Tgt Ion:128 Resp: 24340
Ion Ratio Lower Upper
128 100
127 12.7 10.2 15.4
129 10.1 8.7 13.1

