
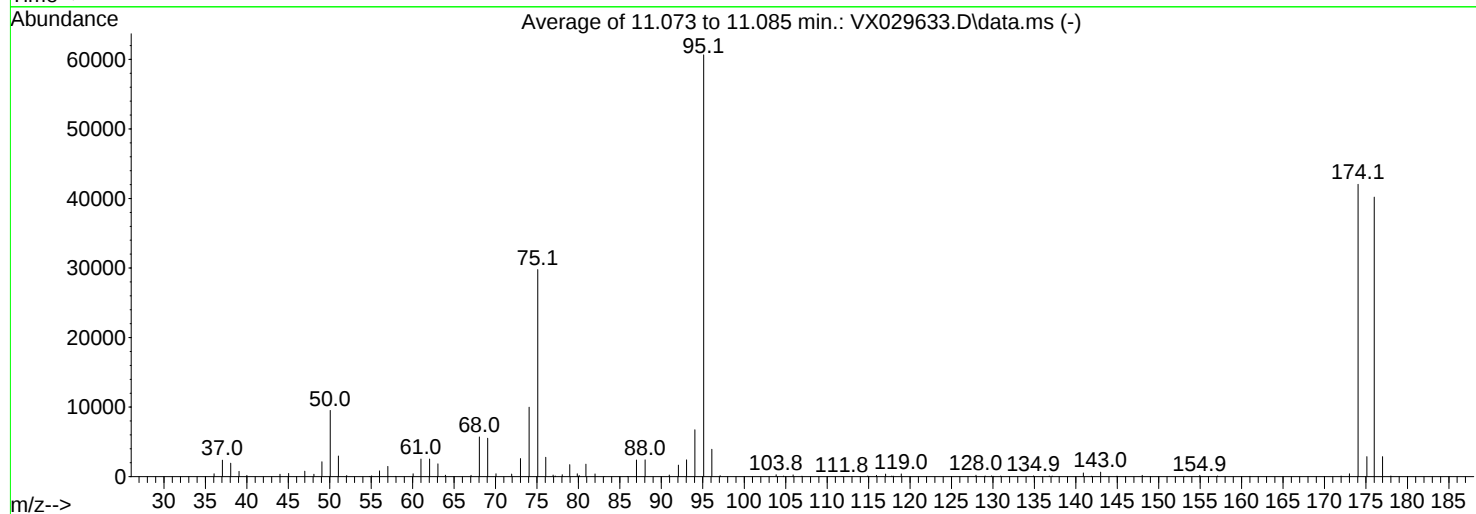


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062022\
 Data File : VX029633.D
 Acq On : 21 Jun 2022 01:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260
 Last Update : Mon Jun 20 01:31:01 2022

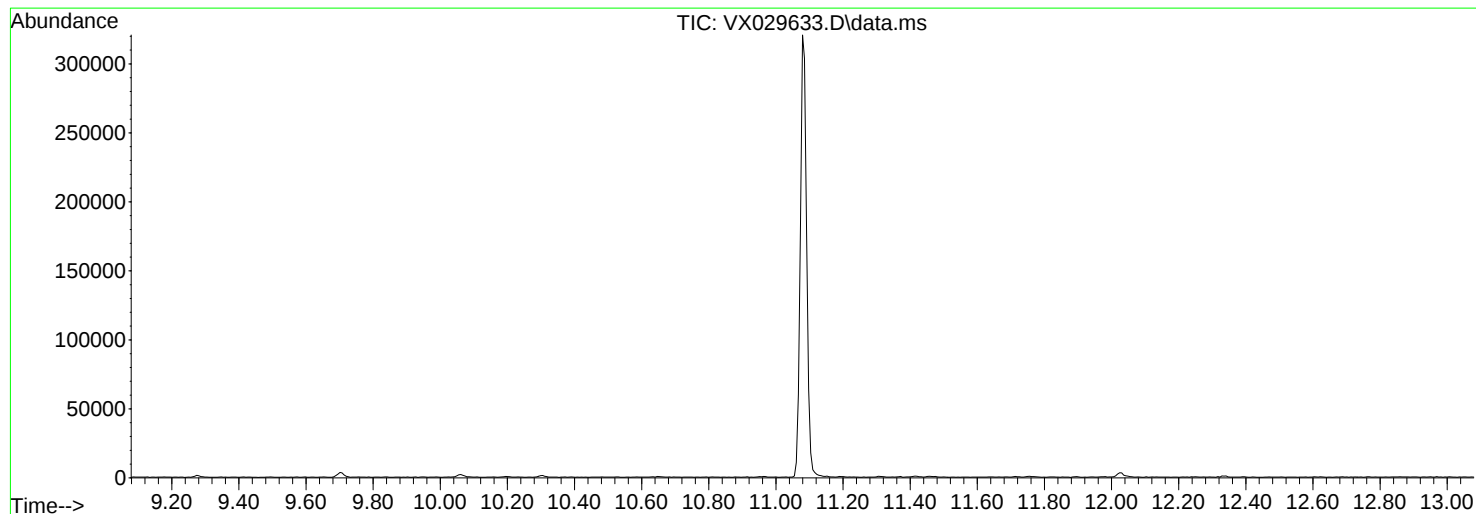

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	9517	PASS
75	95	30	60	49.1	29781	PASS
95	95	100	100	100.0	60659	PASS
96	95	5	9	6.5	3944	PASS
173	174	0.00	2	1.0	424	PASS
174	95	50	100	69.3	42040	PASS
175	174	5	9	6.9	2883	PASS
176	174	95	101	95.6	40192	PASS
177	176	5	9	7.2	2880	PASS