

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062023\  
Data File : VX036233.D  
Acq On : 20 Jun 2023 11:23  
Operator : JC/MD  
Sample : 03238-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X061623W.M

Title : SW846 8260

Signal : TIC: VX036233.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.099       | 647           | 658         | 669          | rVB2     | 5182           | 15362         | 1.54%           | 0.290%        |
| 2         | 5.385       | 693           | 705         | 721          | rBV      | 115137         | 339644        | 34.05%          | 6.404%        |
| 3         | 5.550       | 721           | 732         | 745          | rVV      | 184087         | 530203        | 53.16%          | 9.997%        |
| 4         | 5.958       | 788           | 799         | 812          | rBV      | 148439         | 400336        | 40.14%          | 7.548%        |
| 5         | 6.763       | 921           | 931         | 946          | rBV      | 303049         | 728444        | 73.03%          | 13.735%       |
| 6         | 8.647       | 1233          | 1240        | 1255         | rBV      | 645188         | 997453        | 100.00%         | 18.807%       |
| 7         | 10.055      | 1465          | 1471        | 1483         | rBV      | 622336         | 853775        | 85.60%          | 16.098%       |
| 8         | 11.079      | 1633          | 1639        | 1649         | rBV      | 521535         | 655192        | 65.69%          | 12.354%       |
| 9         | 12.018      | 1788          | 1793        | 1803         | rBV      | 626811         | 783269        | 78.53%          | 14.768%       |




Sum of corrected areas: 5303678

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062023\  
Data File : VX036233.D  
Acq On : 20 Jun 2023 11:23  
Operator : JC/MD  
Sample : 03238-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X061623W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

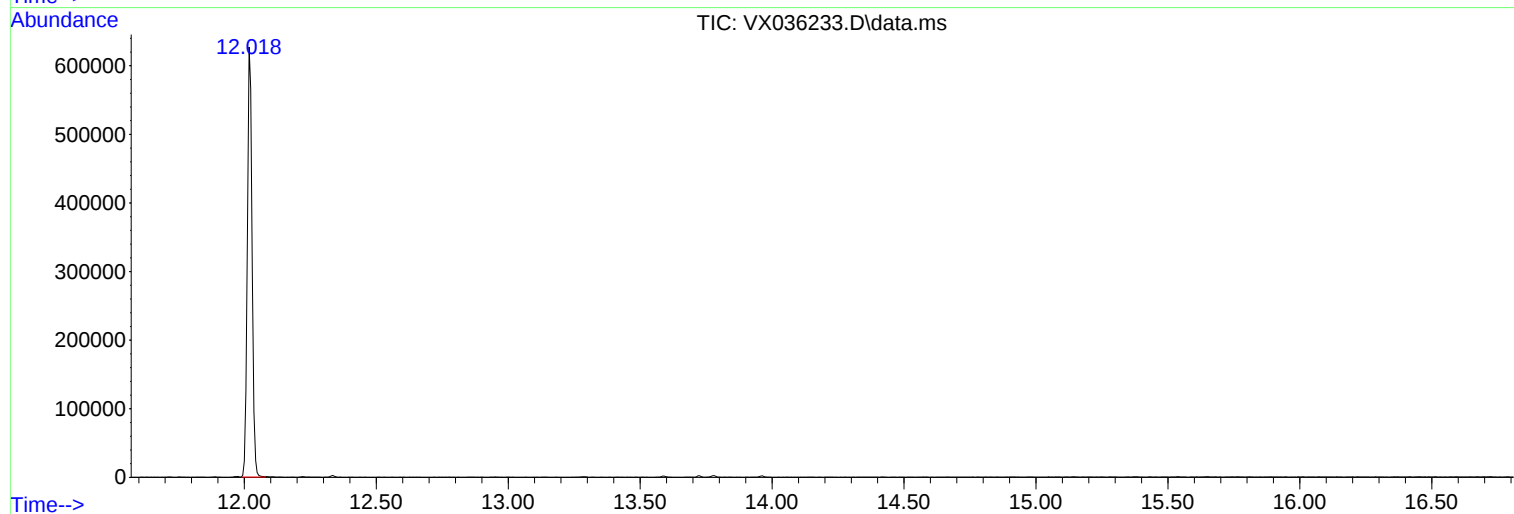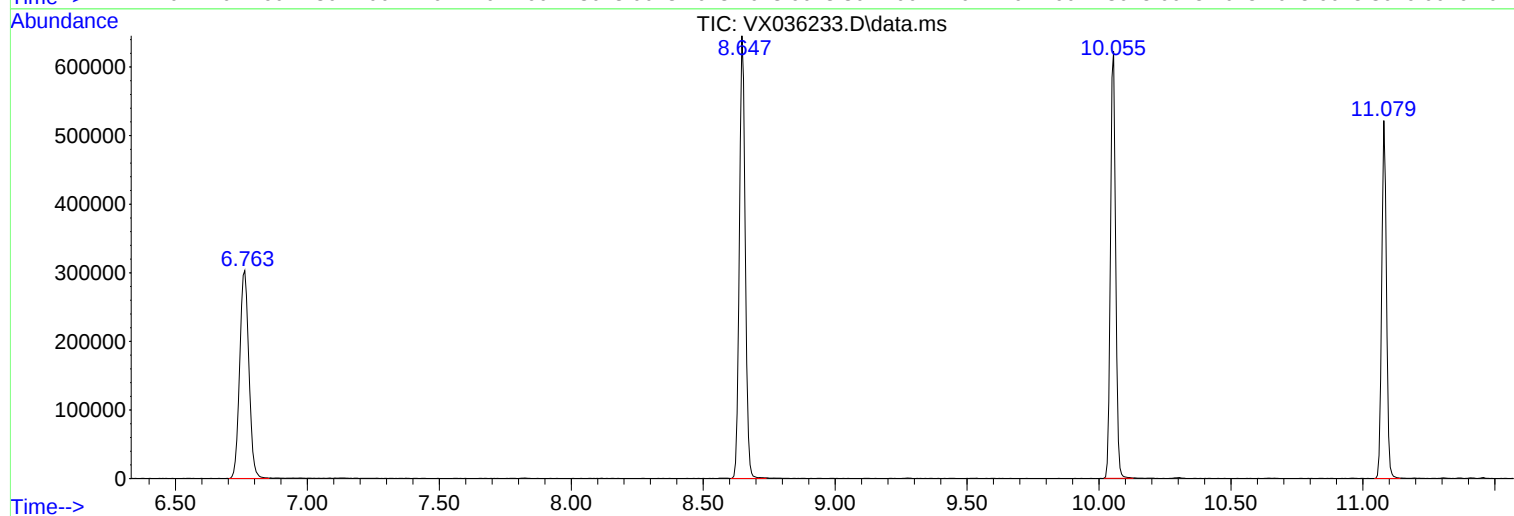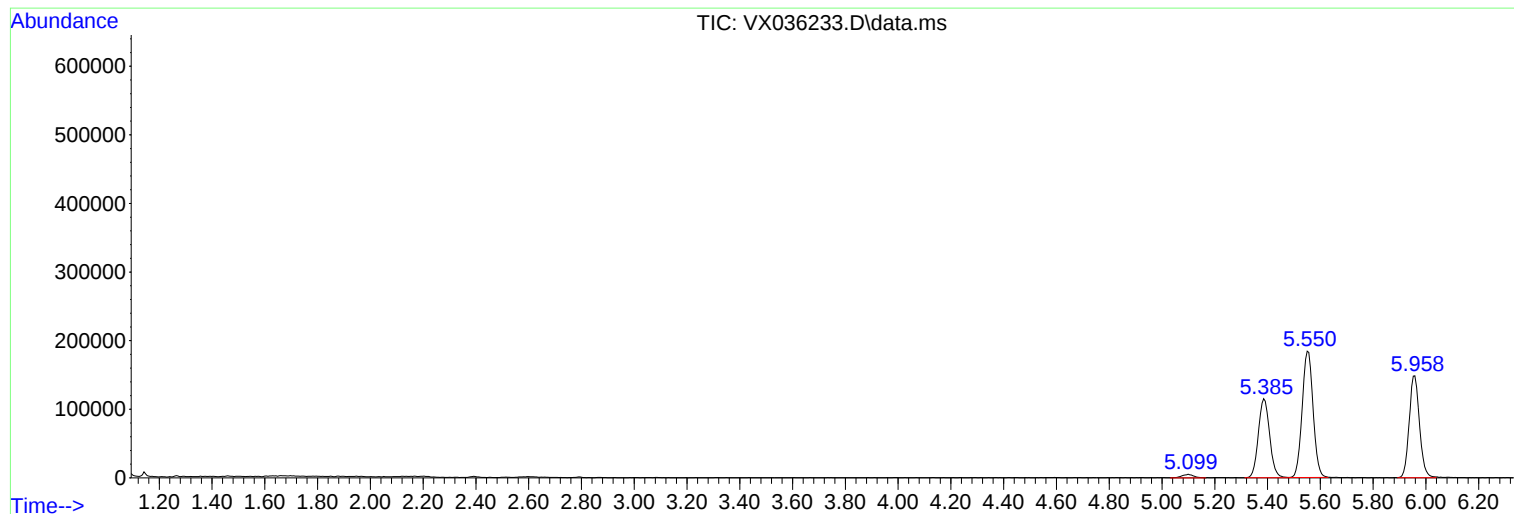

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062023\  
Data File : VX036233.D  
Acq On : 20 Jun 2023 11:23  
Operator : JC/MD  
Sample : 03238-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X061623W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062023\  
Data File : VX036233.D  
Acq On : 20 Jun 2023 11:23  
Operator : JC/MD  
Sample : 03238-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X061623W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|