

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
 Data File : VX036241.D
 Acq On : 20 Jun 2023 14:30
 Operator : JC/MD
 Sample : 03291-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
 Title : SW846 8260

Signal : TIC: VX036241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	41	46	52	rBV	77910	78827	5.18%	0.300%
2	1.752	102	109	122	rBV	345041	473087	31.11%	1.802%
3	1.953	138	142	155	rVB	197037	289857	19.06%	1.104%
4	2.069	156	161	167	rBV	36522	51103	3.36%	0.195%
5	2.166	172	177	180	rVV	20298	32044	2.11%	0.122%
6	2.215	180	185	194	rVB	58751	91873	6.04%	0.350%
7	2.343	199	206	210	rVV	26767	52437	3.45%	0.200%
8	2.715	257	267	271	rBV4	21450	56612	3.72%	0.216%
9	2.782	271	278	281	rVV	90784	205154	13.49%	0.782%
10	2.825	281	285	289	rVV	181592	372275	24.48%	1.418%
11	2.867	289	292	307	rVB2	98850	252648	16.62%	0.963%
12	3.099	317	330	343	rBV	198191	452241	29.74%	1.723%
13	3.325	357	367	378	rBV2	46416	118249	7.78%	0.451%
14	3.446	378	387	398	rVB	65030	143962	9.47%	0.548%
15	3.587	401	410	416	rBV3	16127	42276	2.78%	0.161%
16	3.666	416	423	429	rBV2	35028	83644	5.50%	0.319%
17	3.727	429	433	442	rVB	15272	34098	2.24%	0.130%
18	3.837	442	451	457	rBV2	39671	103493	6.81%	0.394%
19	3.904	457	462	466	rBV	15222	35049	2.31%	0.134%
20	4.105	486	495	504	rVB3	26997	69121	4.55%	0.263%
21	4.306	518	528	539	rVV	378045	1087316	71.51%	4.143%
22	5.135	649	664	665	rBV6	9904	37343	2.46%	0.142%
23	5.190	665	673	689	rVB3	30762	108946	7.17%	0.415%
24	5.385	689	705	711	rBV2	101861	308529	20.29%	1.176%
25	5.470	711	719	726	rVV	218352	625944	41.17%	2.385%
26	5.550	726	732	740	rVB	125253	320924	21.11%	1.223%
27	5.836	766	779	790	rBV5	51495	181201	11.92%	0.690%
28	5.952	790	798	807	rBV	118083	310694	20.43%	1.184%
29	6.159	819	832	842	rBV3	69371	247472	16.28%	0.943%
30	6.257	842	848	857	rVB2	61842	161634	10.63%	0.616%
31	6.361	857	865	875	rVB	76652	210878	13.87%	0.803%
32	6.604	893	905	912	rBV6	14977	39470	2.60%	0.150%
33	6.757	922	930	939	rBV	261930	677658	44.57%	2.582%
34	7.062	972	980	989	rVB2	17619	37368	2.46%	0.142%
35	7.171	990	998	1007	rBV3	39334	92601	6.09%	0.353%
36	7.379	1019	1032	1045	rBV2	367072	914352	60.14%	3.484%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
 Data File : VX036241.D
 Acq On : 20 Jun 2023 14:30
 Operator : JC/MD
 Sample : 03291-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
 Title : SW846 8260

37	7.659	1070	1078	1086	rBV2	38491	76849	5.05%	0.293%
38	7.854	1103	1110	1111	rBV	29462	44848	2.95%	0.171%
39	7.879	1112	1114	1121	rVB4	34143	57031	3.75%	0.217%
40	8.141	1153	1157	1162	rVB2	27421	48044	3.16%	0.183%
41	8.311	1176	1185	1194	rBV7	14177	38823	2.55%	0.148%
42	8.507	1210	1217	1224	rVB	79579	136896	9.00%	0.522%
43	8.598	1224	1232	1235	rBV4	33317	73370	4.83%	0.280%
44	8.647	1235	1240	1246	rVV	524332	835069	54.92%	3.182%
45	8.720	1246	1252	1257	rVV	364355	555495	36.53%	2.116%
46	8.976	1289	1294	1299	rVB	32713	52072	3.42%	0.198%
47	9.098	1306	1314	1319	rBV4	23833	47635	3.13%	0.181%
48	9.159	1319	1324	1334	rVB	53617	90638	5.96%	0.345%
49	9.433	1364	1369	1371	rBV3	24120	41514	2.73%	0.158%
50	9.531	1381	1385	1389	rVV	55637	71616	4.71%	0.273%
51	10.055	1461	1471	1476	rBV	549986	759618	49.96%	2.894%
52	10.128	1476	1483	1487	rVV	22622	45424	2.99%	0.173%
53	10.195	1487	1494	1499	rVB2	178356	263382	17.32%	1.003%
54	10.299	1504	1511	1518	rVB	1145103	1520471	100.00%	5.793%
55	10.640	1562	1567	1579	rVB	871382	1115426	73.36%	4.250%
56	10.963	1614	1620	1628	rVB	174176	230693	15.17%	0.879%
57	11.079	1634	1639	1645	rBV	452768	565830	37.21%	2.156%
58	11.305	1667	1676	1683	rBV	239280	301797	19.85%	1.150%
59	11.378	1683	1688	1696	rVV	809364	1354580	89.09%	5.161%
60	11.451	1696	1700	1706	rVB	188878	227829	14.98%	0.868%
61	11.610	1719	1726	1734	rBV	619378	767797	50.50%	2.925%
62	11.750	1744	1749	1755	rVB	1126515	1316947	86.61%	5.018%
63	11.866	1762	1768	1770	rBV	28135	43633	2.87%	0.166%
64	11.890	1770	1772	1780	rVB	43879	53228	3.50%	0.203%
65	11.969	1780	1785	1788	rBV	93987	110539	7.27%	0.421%
66	12.018	1788	1793	1799	rVV	593718	781602	51.41%	2.978%
67	12.085	1799	1804	1809	rVV	415840	494417	32.52%	1.884%
68	12.244	1824	1830	1832	rBV	238730	314715	20.70%	1.199%
69	12.268	1832	1834	1837	rVV	194538	199549	13.12%	0.760%
70	12.311	1837	1841	1849	rVB4	174485	290795	19.13%	1.108%
71	12.408	1851	1857	1861	rVB2	34017	48274	3.17%	0.184%
72	12.463	1861	1866	1871	rVB	76863	95870	6.31%	0.365%
73	12.530	1871	1877	1879	rBV	167996	209868	13.80%	0.800%
74	12.555	1879	1881	1885	rVB	128709	129369	8.51%	0.493%
75	12.609	1885	1890	1894	rBV	470052	576746	37.93%	2.197%
76	12.646	1894	1896	1900	rVB	52391	53593	3.52%	0.204%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
 Data File : VX036241.D
 Acq On : 20 Jun 2023 14:30
 Operator : JC/MD
 Sample : 03291-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
 Title : SW846 8260

77	12.701	1900	1905	1912	rBV2	363502	547746	36.02%	2.087%
78	12.847	1924	1929	1934	rVB2	114896	151323	9.95%	0.577%
79	12.920	1934	1941	1945	rBV	259629	312379	20.54%	1.190%
80	12.963	1945	1948	1954	rVB	109838	131383	8.64%	0.501%
81	13.036	1954	1960	1967	rBV3	37493	87683	5.77%	0.334%
82	13.134	1972	1976	1978	rVV	32510	43649	2.87%	0.166%
83	13.164	1978	1981	1992	rVV	190697	272941	17.95%	1.040%
84	13.256	1992	1996	1997	rVV2	27512	31934	2.10%	0.122%
85	13.292	1997	2002	2007	rVV2	413980	575071	37.82%	2.191%
86	13.341	2007	2010	2013	rVV4	30782	47851	3.15%	0.182%
87	13.420	2019	2023	2031	rVB	67151	89675	5.90%	0.342%
88	13.506	2031	2037	2039	rBV2	44095	59848	3.94%	0.228%
89	13.542	2039	2043	2046	rVV	101899	137261	9.03%	0.523%
90	13.585	2046	2050	2054	rVV3	93805	155094	10.20%	0.591%
91	13.658	2055	2062	2068	rVV2	112905	253222	16.65%	0.965%
92	13.774	2074	2081	2088	rVV	343015	436991	28.74%	1.665%
93	13.865	2088	2096	2100	rVV4	28401	56688	3.73%	0.216%
94	13.926	2100	2106	2110	rVV3	30379	44401	2.92%	0.169%
95	13.969	2110	2113	2117	rVB2	32809	37071	2.44%	0.141%
96	14.073	2125	2130	2137	rBV	45123	56514	3.72%	0.215%
97	14.213	2148	2153	2159	rBV2	36901	67918	4.47%	0.259%
98	14.371	2175	2179	2183	rVB	30895	36233	2.38%	0.138%
99	14.633	2218	2222	2232	rVB	73039	99485	6.54%	0.379%
100	14.780	2241	2246	2254	rBV	50809	71904	4.73%	0.274%




Sum of corrected areas: 26246537

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036241.D
Acq On : 20 Jun 2023 14:30
Operator : JC/MD
Sample : 03291-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

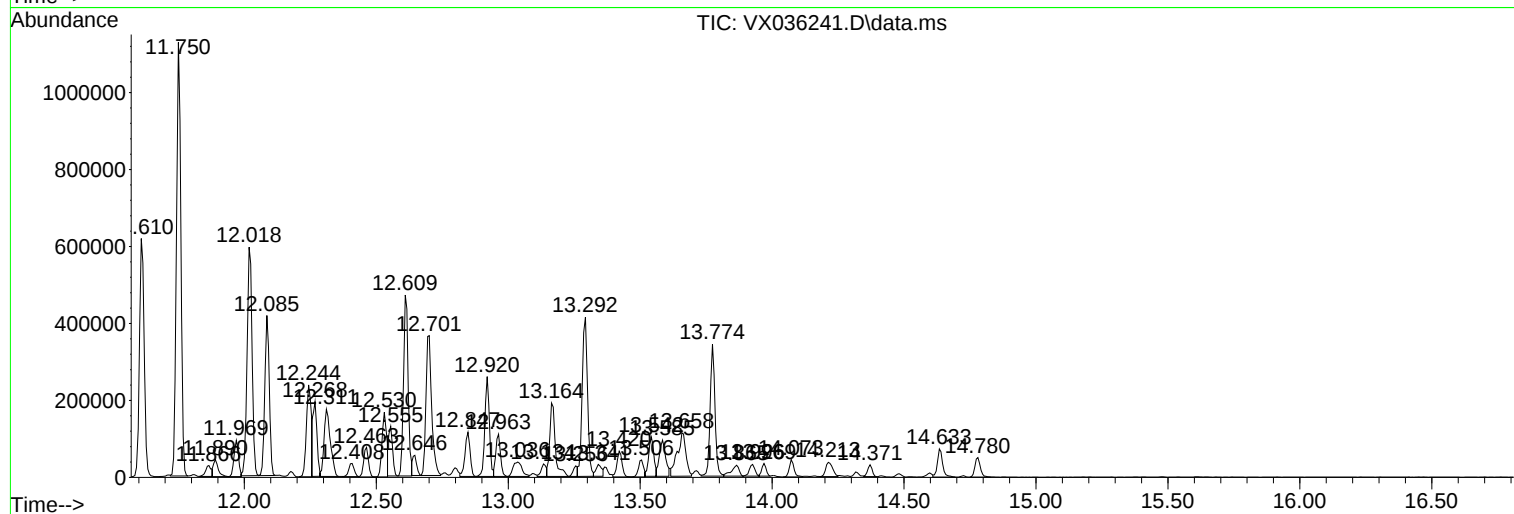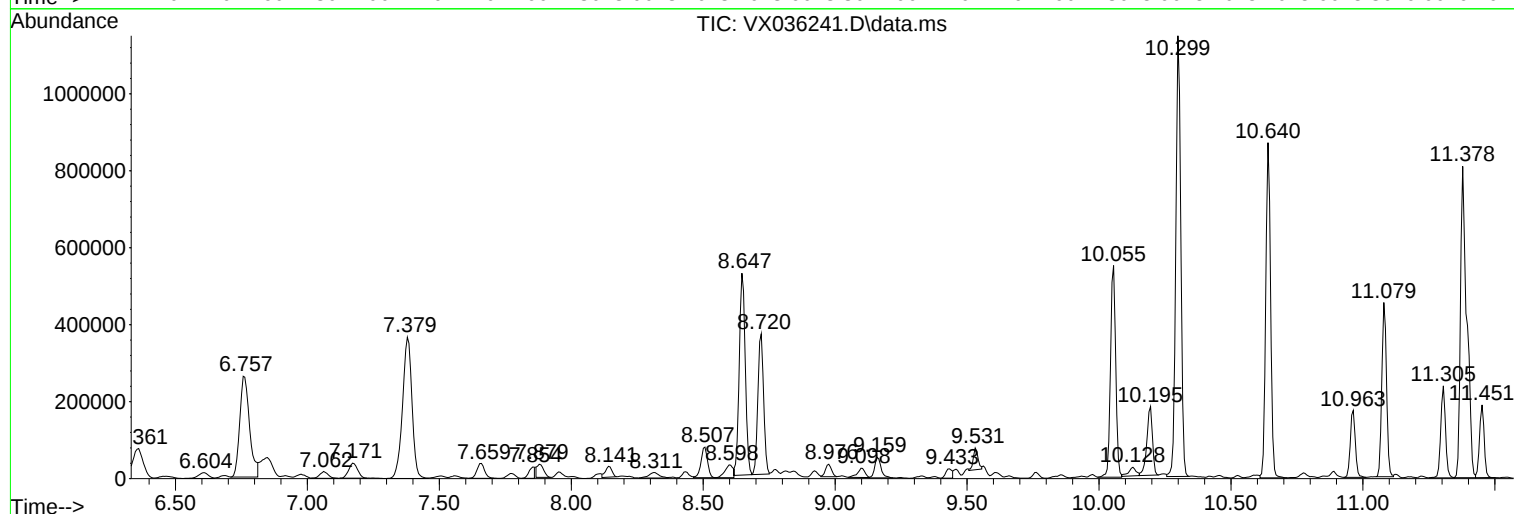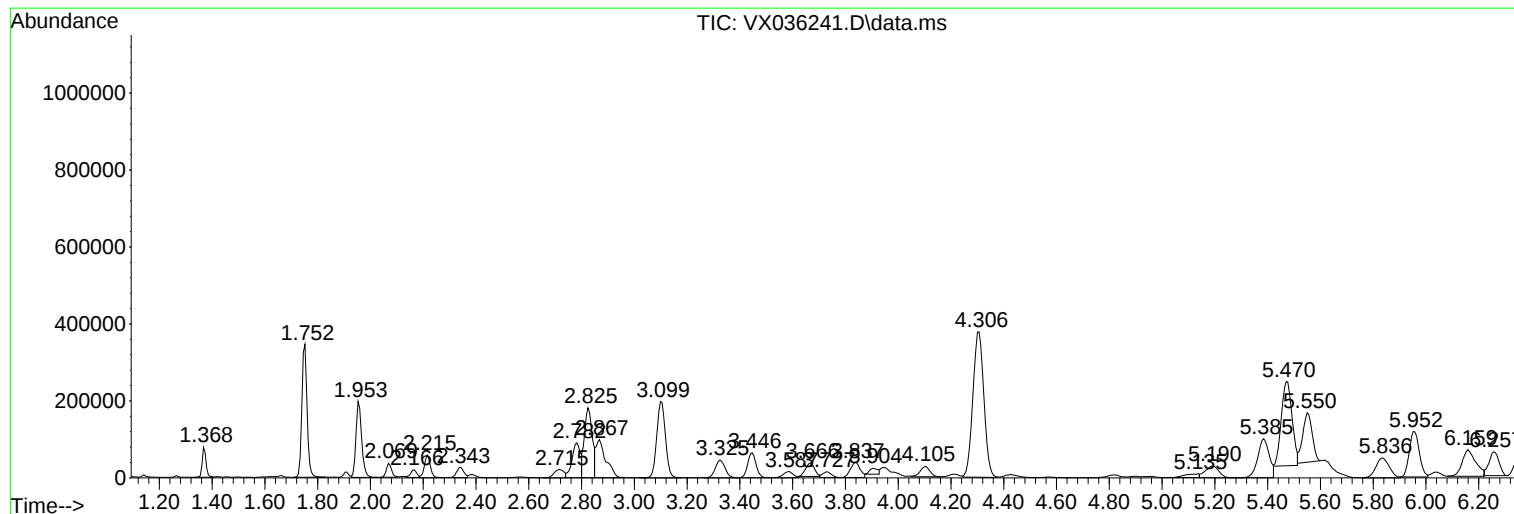

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036241.D
Acq On : 20 Jun 2023 14:30
Operator : JC/MD
Sample : 03291-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036241.D
Acq On : 20 Jun 2023 14:30
Operator : JC/MD
Sample : 03291-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc