

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
 Data File : VX036247.D
 Acq On : 20 Jun 2023 16:51
 Operator : JC/MD
 Sample : 03339-05 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-13

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M

Title : SW846 8260

Signal : TIC: VX036247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	7059	7404	1.05%	0.186%
2	5.385	694	705	722	rBV2	68135	201715	28.57%	5.064%
3	5.550	722	732	746	rVV	164617	460506	65.23%	11.561%
4	5.958	788	799	810	rBV	88968	239397	33.91%	6.010%
5	6.763	921	931	948	rBV	265149	631045	89.39%	15.843%
6	8.647	1233	1240	1248	rBV	366636	578630	81.96%	14.527%
7	8.720	1248	1252	1261	rVB	13185	22012	3.12%	0.553%
8	10.055	1465	1471	1481	rBV	529723	705958	100.00%	17.723%
9	10.195	1489	1494	1500	rVB	11514	13907	1.97%	0.349%
10	10.299	1505	1511	1518	rBV	36062	49722	7.04%	1.248%
11	10.646	1561	1568	1572	rBV	11339	15082	2.14%	0.379%
12	11.079	1634	1639	1650	rBV	292531	373679	52.93%	9.381%
13	11.378	1683	1688	1690	rBV	7768	9981	1.41%	0.251%
14	11.750	1745	1749	1755	rVB	13959	17522	2.48%	0.440%
15	12.024	1788	1794	1802	rBV	510683	649318	91.98%	16.301%
16	13.774	2077	2081	2086	rBV2	5632	7305	1.03%	0.183%




Sum of corrected areas: 3983183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036247.D
Acq On : 20 Jun 2023 16:51
Operator : JC/MD
Sample : 03339-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

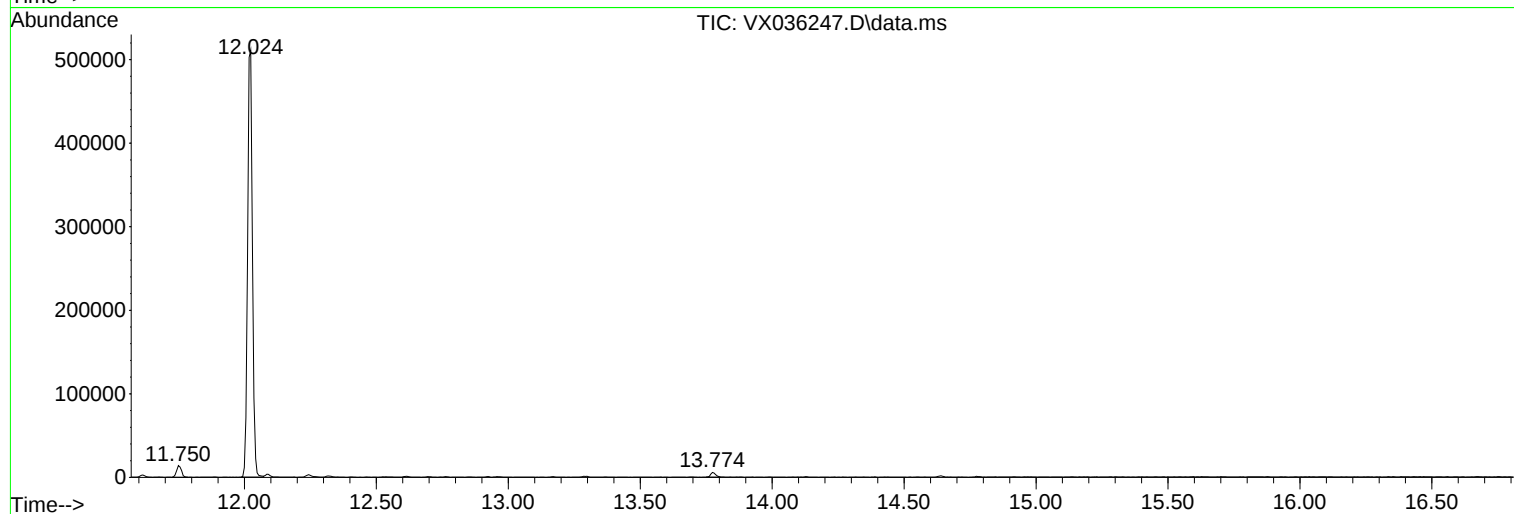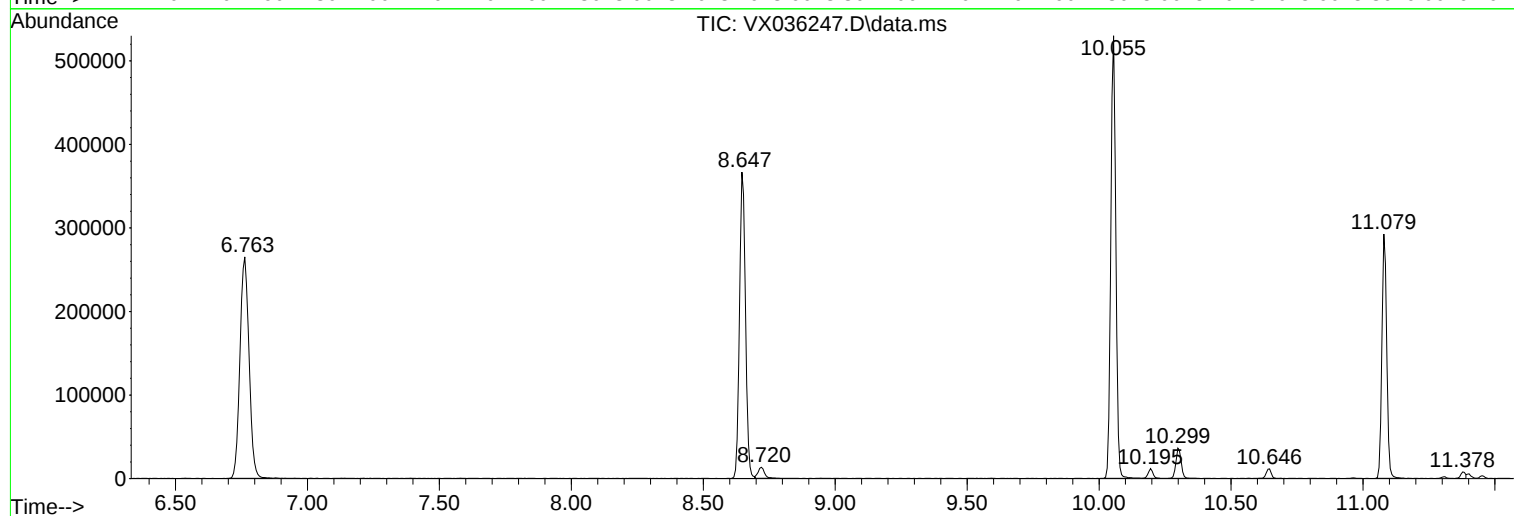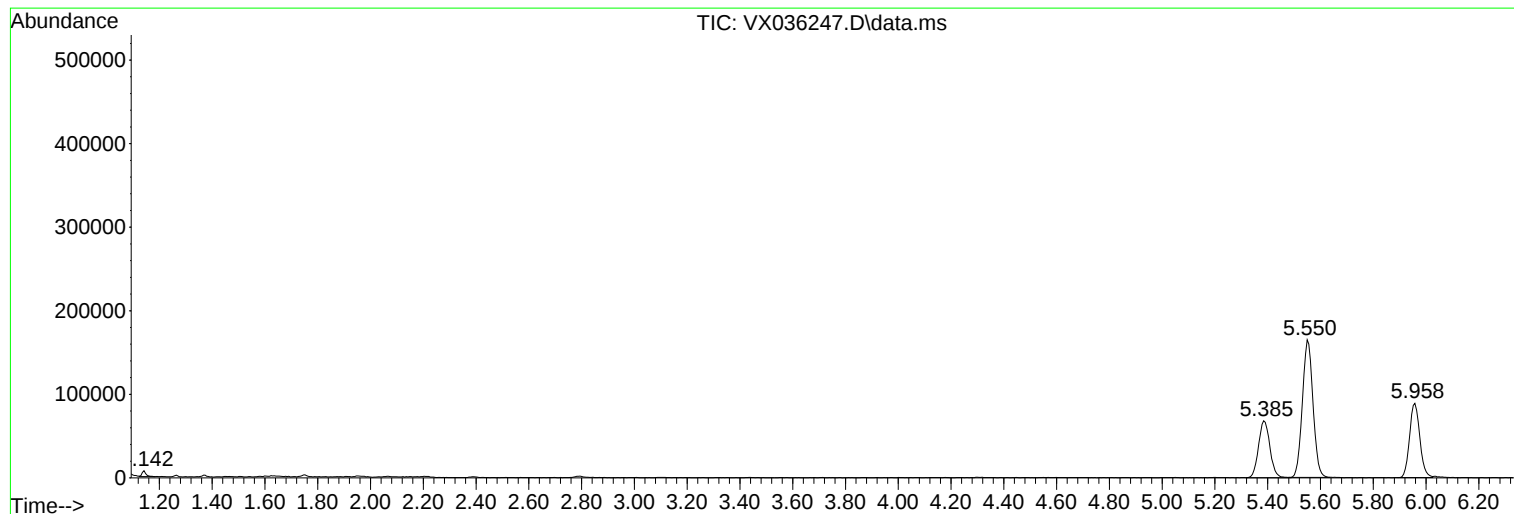

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036247.D
Acq On : 20 Jun 2023 16:51
Operator : JC/MD
Sample : 03339-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036247.D
Acq On : 20 Jun 2023 16:51
Operator : JC/MD
Sample : 03339-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------