

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
 Data File : VX036249.D
 Acq On : 20 Jun 2023 17:38
 Operator : JC/MD
 Sample : 03342-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50047

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
 Title : SW846 8260

Signal : TIC: VX036249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	720	rBV	101566	298087	34.10%	6.048%
2	5.550	722	732	749	rVB	155968	438565	50.16%	8.899%
3	5.952	785	798	820	rBV	136837	367167	42.00%	7.450%
4	6.763	920	931	945	rBV	278408	654108	74.82%	13.273%
5	8.647	1233	1240	1248	rBV	559926	874271	100.00%	17.740%
6	8.720	1248	1252	1259	rVB	20171	32187	3.68%	0.653%
7	10.055	1465	1471	1487	rBV	555632	762019	87.16%	15.462%
8	10.195	1490	1494	1501	rVB	9352	11524	1.32%	0.234%
9	10.299	1506	1511	1517	rBV	37191	49985	5.72%	1.014%
10	10.640	1562	1567	1573	rBV	31165	39181	4.48%	0.795%
11	11.079	1634	1639	1651	rBV	434732	560541	64.12%	11.374%
12	11.378	1683	1688	1691	rBV	10352	15332	1.75%	0.311%
13	11.616	1721	1727	1733	rVB	8136	10880	1.24%	0.221%
14	11.750	1744	1749	1756	rBV	20213	25763	2.95%	0.523%
15	12.024	1788	1794	1801	rBV	546666	705899	80.74%	14.323%
16	12.085	1801	1804	1810	rVB	14343	17570	2.01%	0.357%
17	12.244	1825	1830	1833	rBV2	6300	9015	1.03%	0.183%
18	13.292	1993	2002	2007	rBV2	15497	22561	2.58%	0.458%
19	13.420	2019	2023	2030	rVB2	9866	12073	1.38%	0.245%
20	14.225	2147	2155	2161	rBV4	6903	12167	1.39%	0.247%
21	14.481	2190	2197	2201	rVB	7328	9385	1.07%	0.190%




Sum of corrected areas: 4928280

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036249.D
Acq On : 20 Jun 2023 17:38
Operator : JC/MD
Sample : 03342-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50047

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

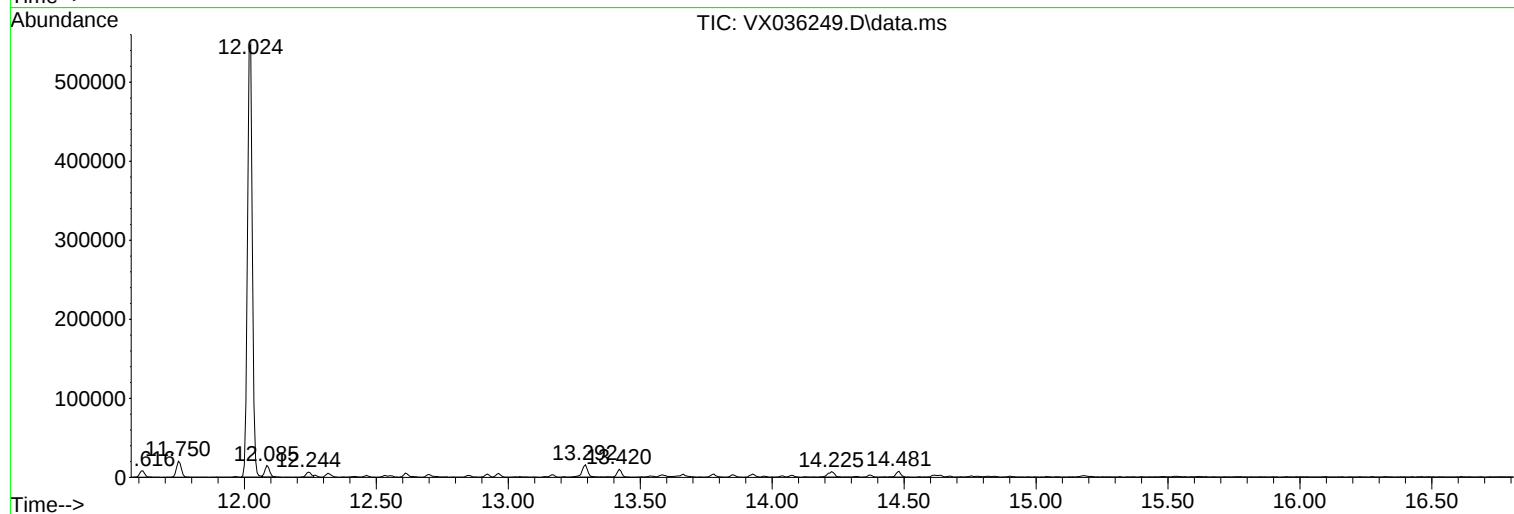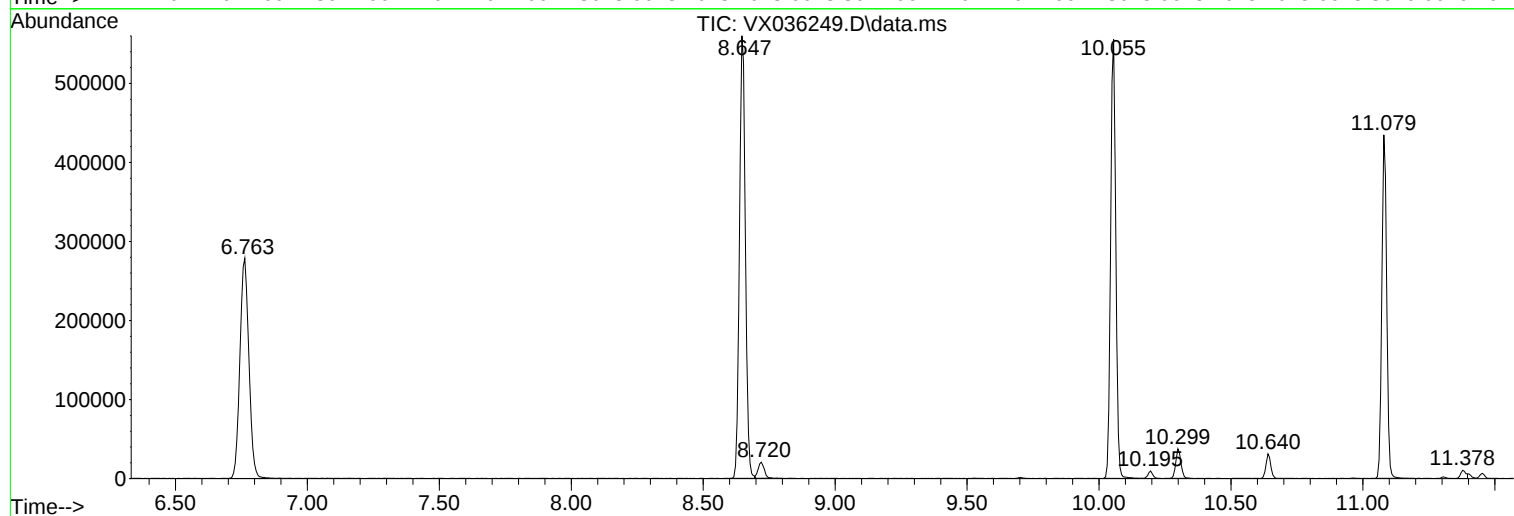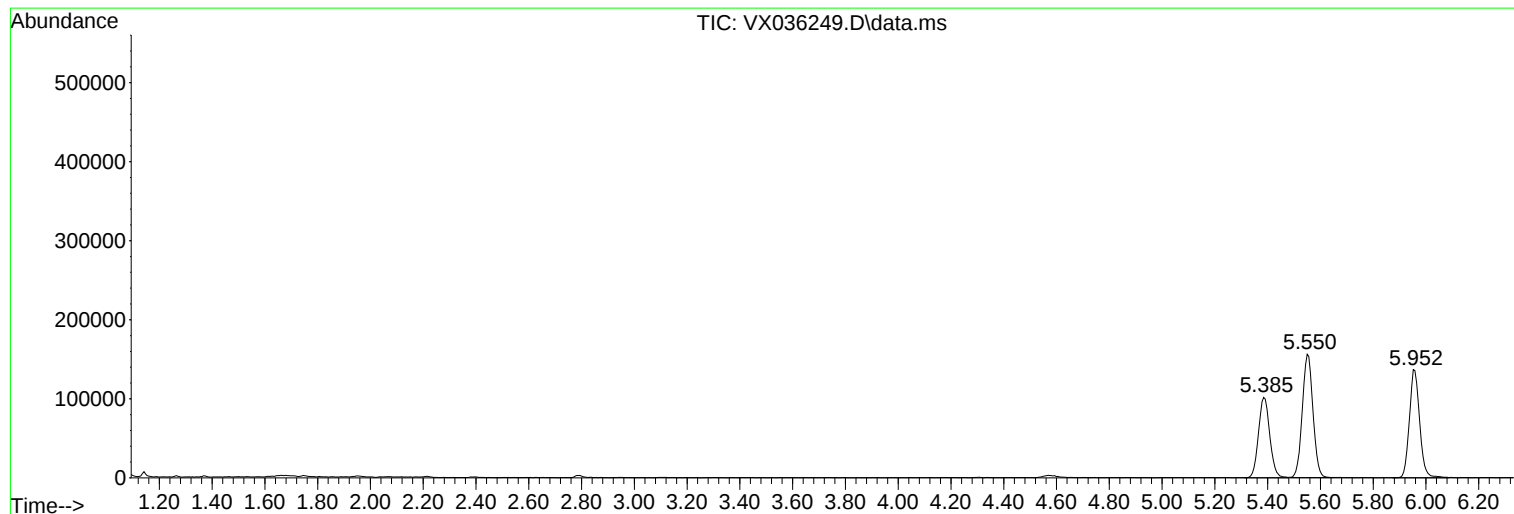

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036249.D
Acq On : 20 Jun 2023 17:38
Operator : JC/MD
Sample : 03342-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50047

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036249.D
Acq On : 20 Jun 2023 17:38
Operator : JC/MD
Sample : 03342-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50047

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------