

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
 Data File : VX036250.D
 Acq On : 20 Jun 2023 18:02
 Operator : JC/MD
 Sample : 03274-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
 Title : SW846 8260

Signal : TIC: VX036250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	55	60	65	rBV	7148	10016	1.25%	0.216%
2	2.386	206	213	223	rBV	14080	25109	3.13%	0.541%
3	4.221	505	514	521	rBV5	3266	10308	1.29%	0.222%
4	5.385	693	705	720	rBV2	94509	277410	34.62%	5.982%
5	5.550	720	732	747	rVB	140697	393913	49.17%	8.494%
6	5.958	788	799	813	rBV	127620	345599	43.14%	7.452%
7	6.763	921	931	946	rBV	253576	609411	76.06%	13.141%
8	8.647	1233	1240	1248	rBV	508654	801189	100.00%	17.276%
9	8.720	1248	1252	1260	rVB	15886	24595	3.07%	0.530%
10	9.525	1378	1384	1388	rBV2	7111	10690	1.33%	0.231%
11	9.580	1388	1393	1402	rVB2	6252	9898	1.24%	0.213%
12	10.055	1465	1471	1487	rBV	539898	740678	92.45%	15.971%
13	10.195	1489	1494	1499	rBV	9965	12375	1.54%	0.267%
14	10.299	1505	1511	1522	rBV	36934	51379	6.41%	1.108%
15	10.640	1562	1567	1575	rBV	12020	15402	1.92%	0.332%
16	11.079	1634	1639	1651	rVB	434180	546966	68.27%	11.794%
17	11.378	1683	1688	1691	rBV	8463	12868	1.61%	0.277%
18	11.750	1745	1749	1760	rVB	21490	25797	3.22%	0.556%
19	11.927	1774	1778	1783	rBV	9307	12122	1.51%	0.261%
20	12.018	1788	1793	1801	rVV	508070	671589	83.82%	14.481%
21	12.853	1926	1930	1937	rBV	23036	30269	3.78%	0.653%


Sum of corrected areas: 4637583

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036250.D
Acq On : 20 Jun 2023 18:02
Operator : JC/MD
Sample : 03274-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

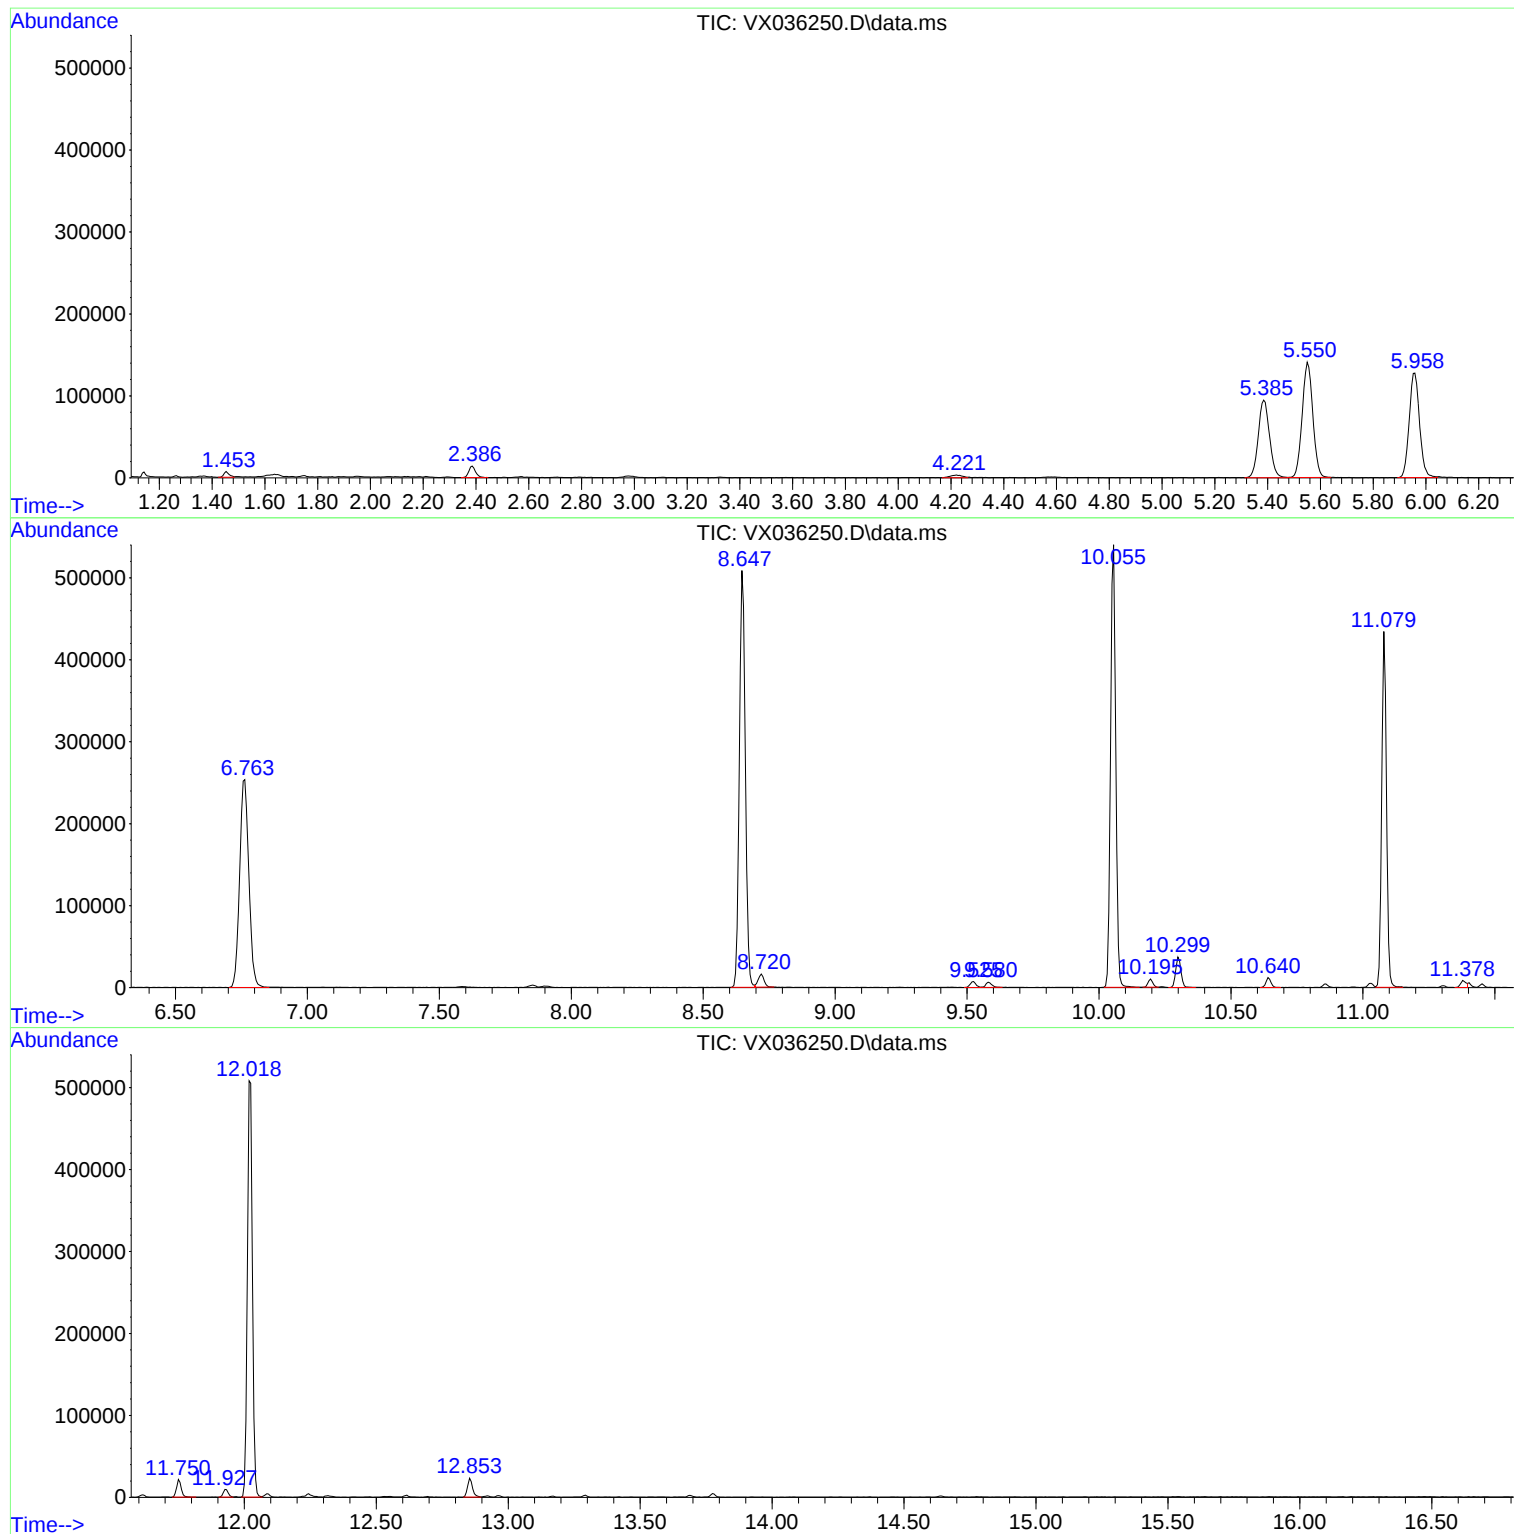

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036250.D
Acq On : 20 Jun 2023 18:02
Operator : JC/MD
Sample : 03274-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062023\
Data File : VX036250.D
Acq On : 20 Jun 2023 18:02
Operator : JC/MD
Sample : 03274-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------