

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062024\
 Data File : VX041957.D
 Acq On : 20 Jun 2024 11:51
 Operator : JC/MD
 Sample : P2981-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 240619057-03-TRIP-BLANK

Quant Time: Jun 21 03:15:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Jun 15 04:02:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.897	128	29753	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	166027	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	146663	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	64197	31.344	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	104.467%
60) 4-Bromofluorobenzene	11.079	95	59585	26.246	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	87.500%
63) Toluene-d8	8.647	98	189985	30.278	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.933%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062024\
Data File : VX041957.D
Acq On : 20 Jun 2024 11:51
Operator : JC/MD
Sample : P2981-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
240619057-03-TRIP-BLANK

Quant Time: Jun 21 03:15:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Jun 15 04:02:59 2024
Response via : Initial Calibration




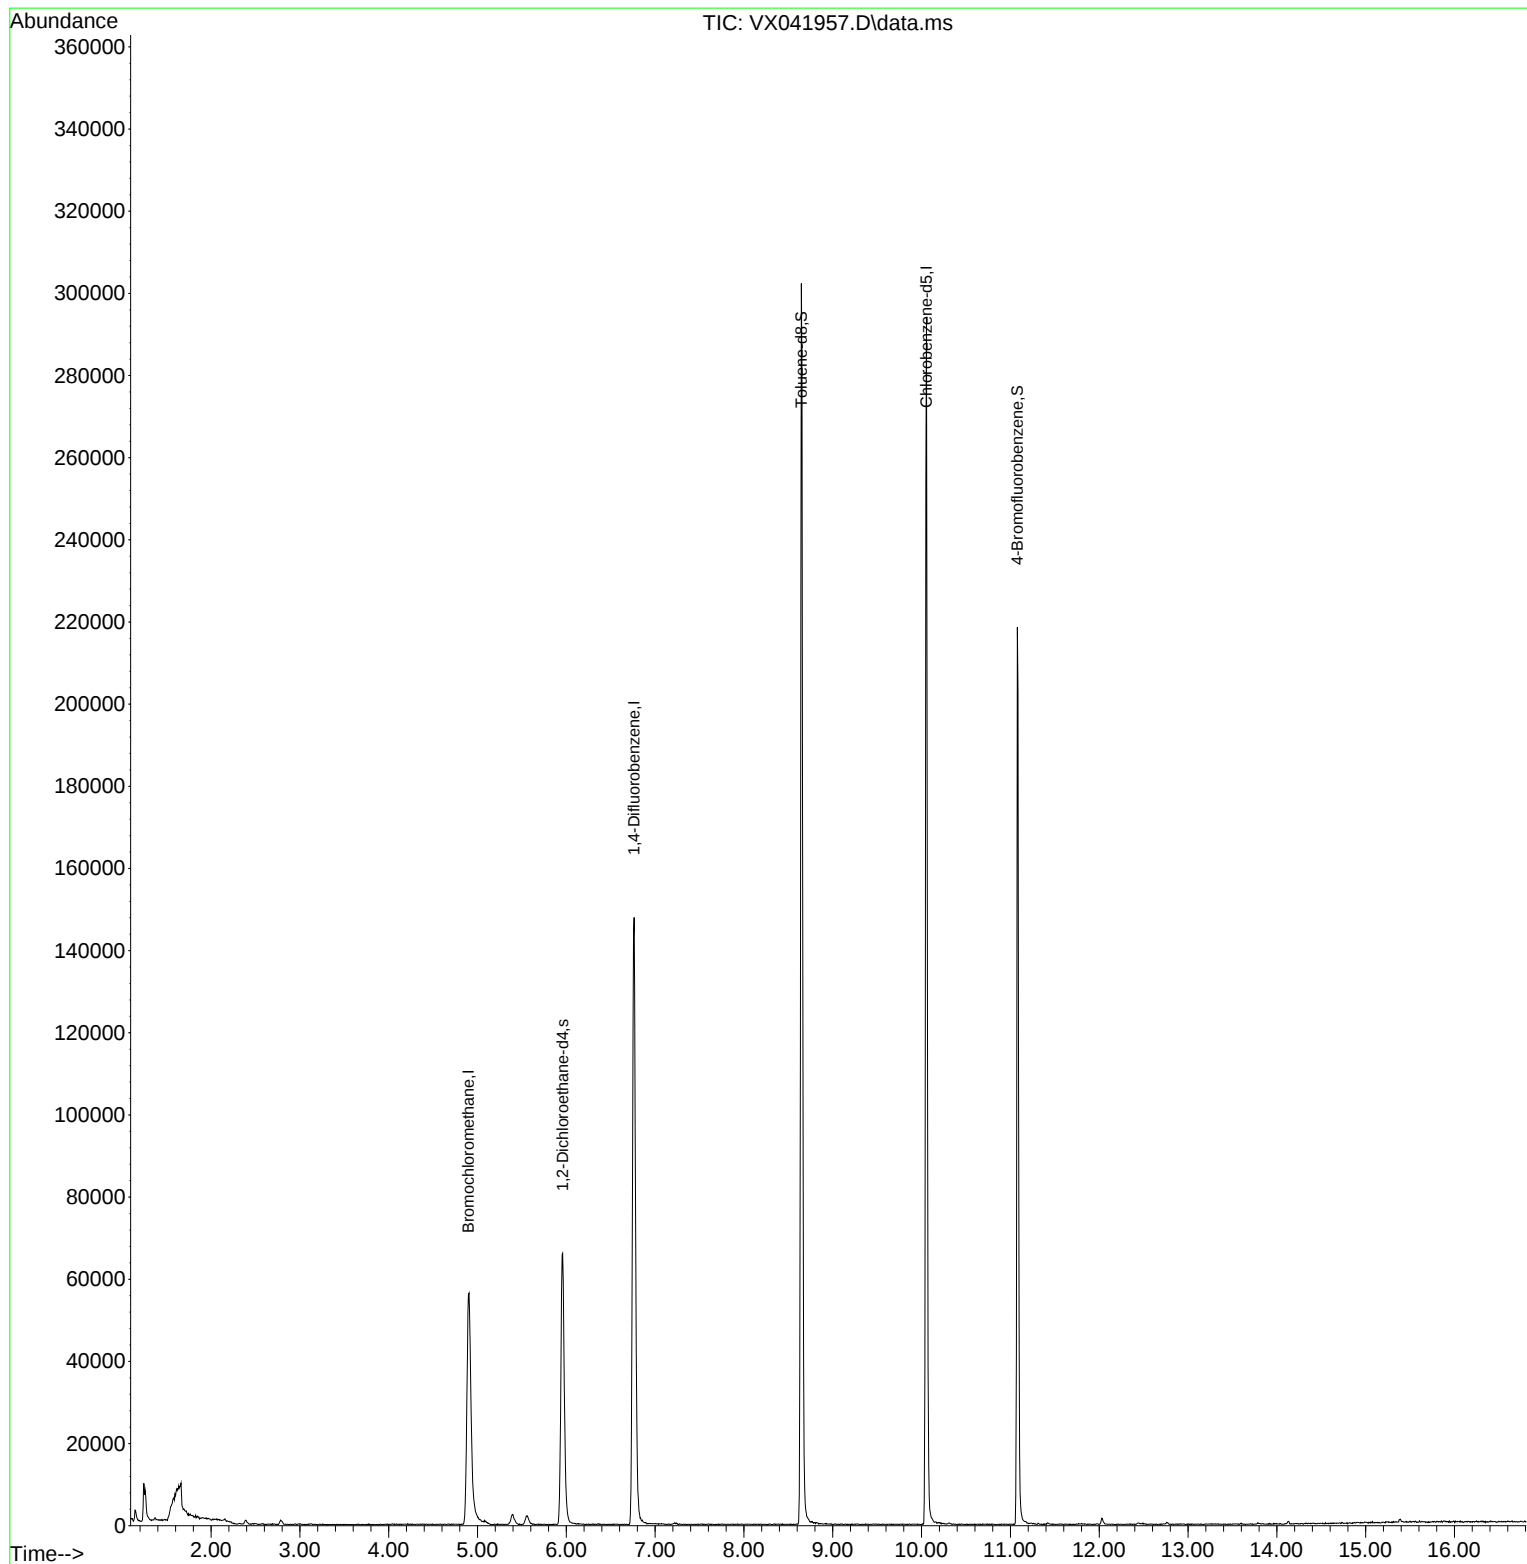


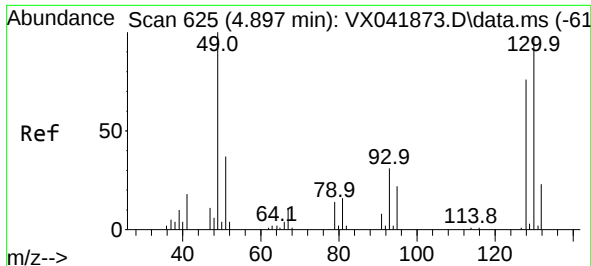

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.897 min Scan# 61
Delta R.T. 0.000 min
Lab File: VX041957.D
Acq: 20 Jun 2024 11:51




Instrument :
MSVOA_X
ClientSampleId :
240619057-03-TRIP-BLANK


Tgt Ion:128 Resp: 29753
Ion Ratio Lower Upper
128 100
49 140.9 0.0 338.5
130 131.6 0.0 324.5

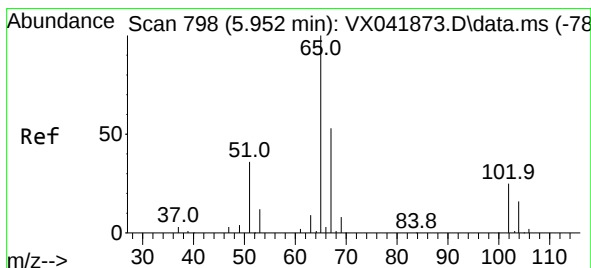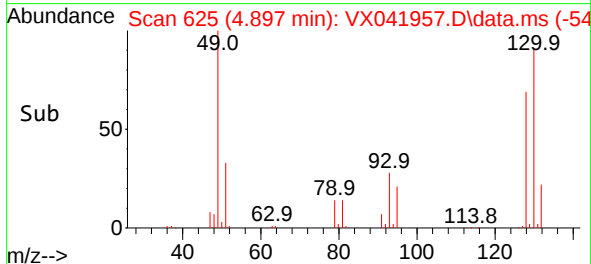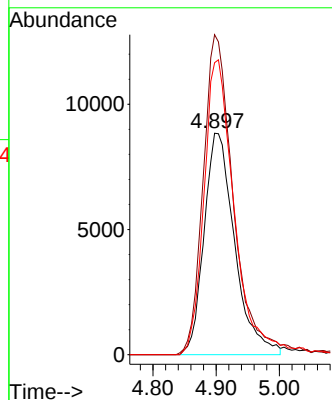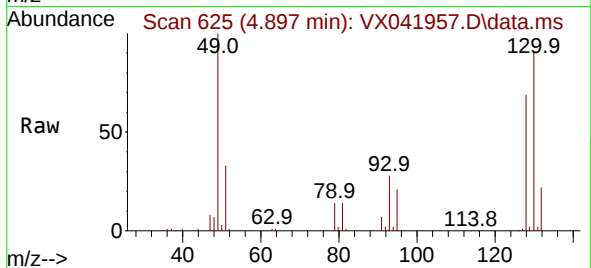

#27
1,2-Dichloroethane-d4
Concen: 31.344 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX041957.D
Acq: 20 Jun 2024 11:51

Tgt Ion: 65 Resp: 64197
Ion Ratio Lower Upper
65 100
67 52.7 43.4 65.0


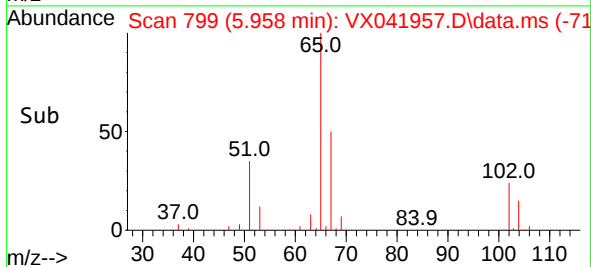
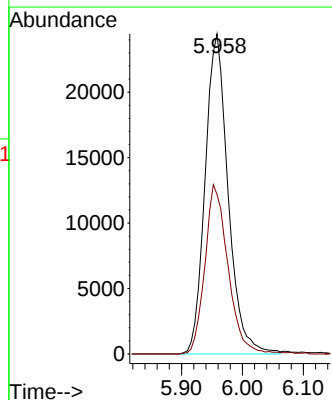
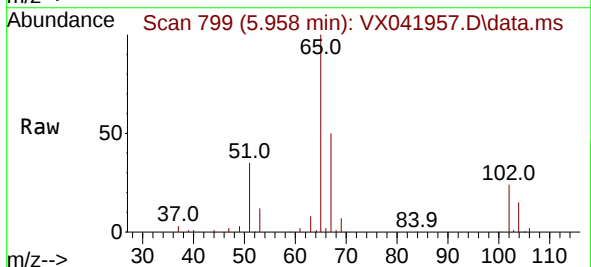


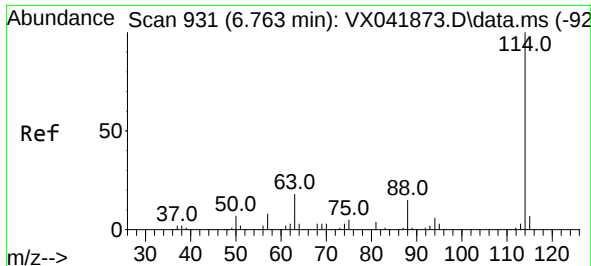

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX041957.D
Acq: 20 Jun 2024 11:51




Instrument :
MSVOA_X
ClientSampleId :
240619057-03-TRIP-BLANK


Tgt Ion:114 Resp: 166027
Ion Ratio Lower Upper
114 100
63 18.4 14.6 21.8
88 14.8 11.8 17.8

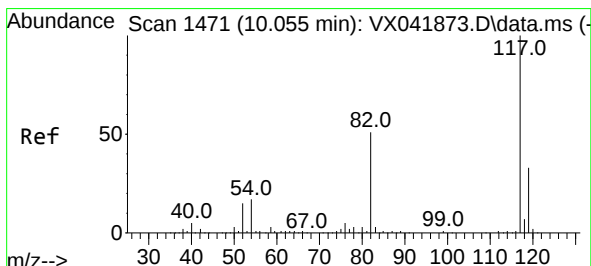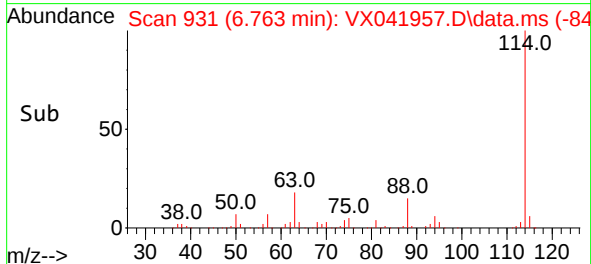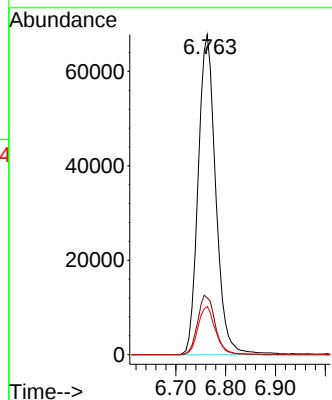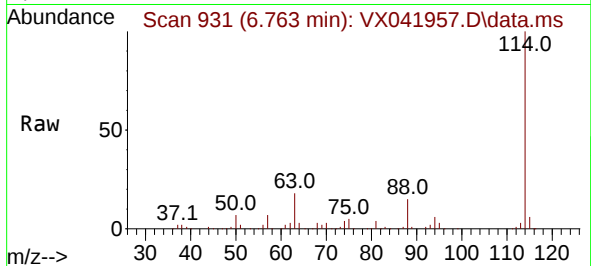

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041957.D
Acq: 20 Jun 2024 11:51

Tgt Ion:117 Resp: 146663
Ion Ratio Lower Upper
117 100
82 51.0 41.1 61.7
119 32.1 26.1 39.1


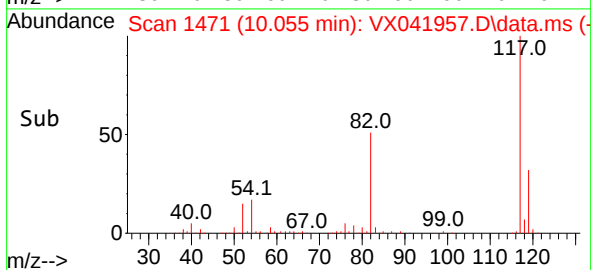
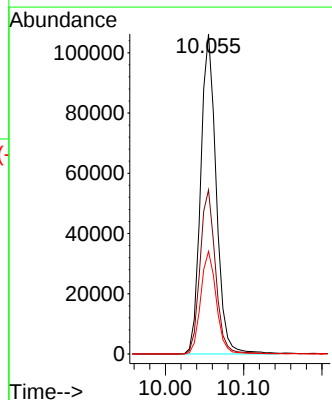
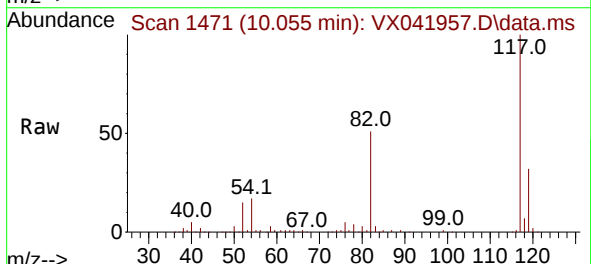


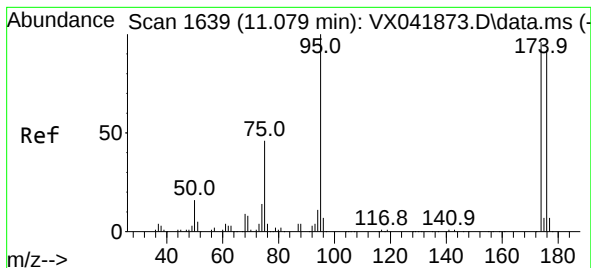

#60
4-Bromofluorobenzene
Concen: 26.246 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041957.D
Acq: 20 Jun 2024 11:51

Instrument :
MSVOA_X
ClientSampleId :
240619057-03-TRIP-BLANK

Tgt Ion: 95 Resp: 59585
Ion Ratio Lower Upper
95 100
174 98.1 78.9 118.3
176 94.2 77.1 115.7

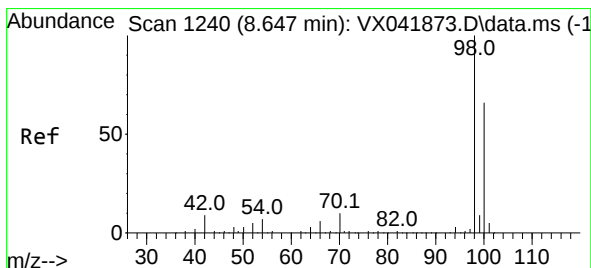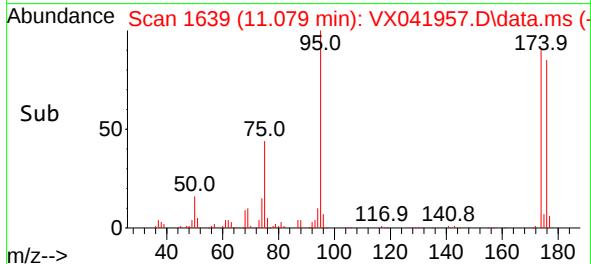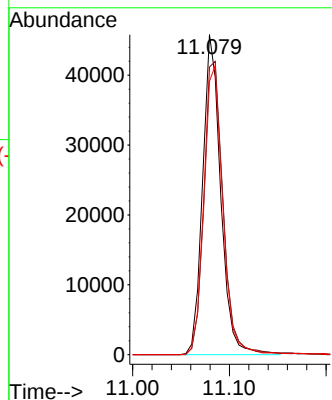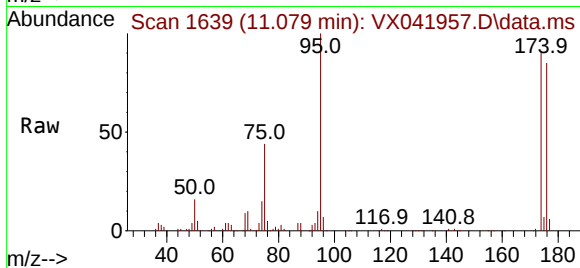

#63
Toluene-d8
Concen: 30.278 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX041957.D
Acq: 20 Jun 2024 11:51

Tgt Ion: 98 Resp: 189985
Ion Ratio Lower Upper
98 100
100 66.6 52.7 79.1

