
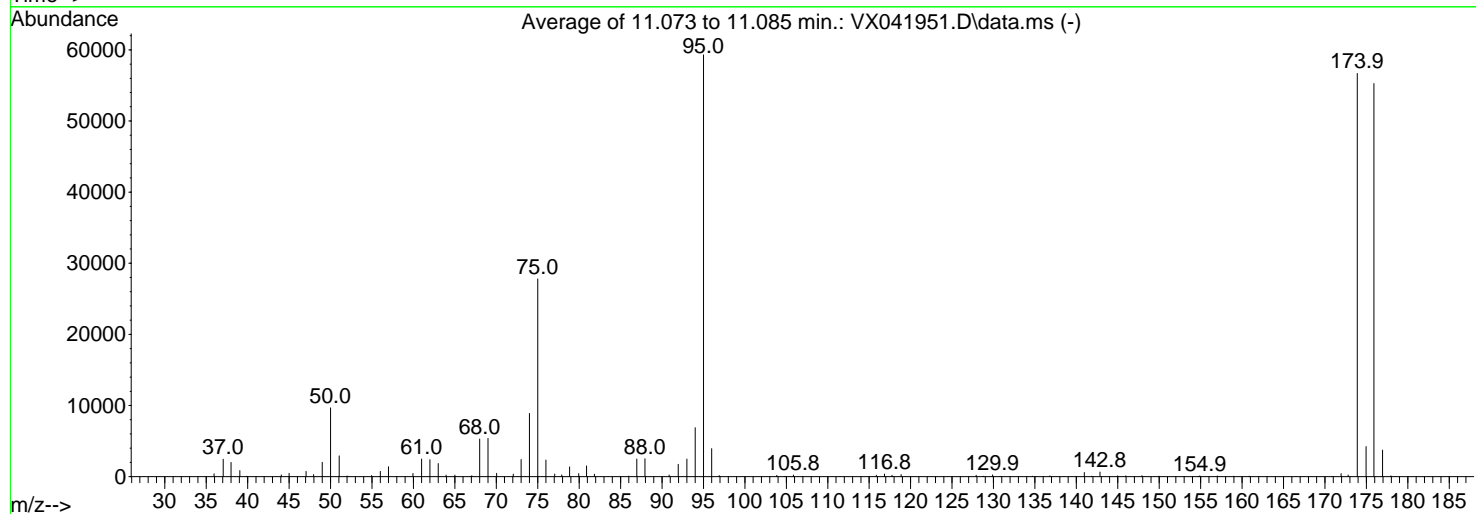


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062024\
 Data File : VX041951.D
 Acq On : 20 Jun 2024 09:03
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sat Jun 15 04:02:59 2024

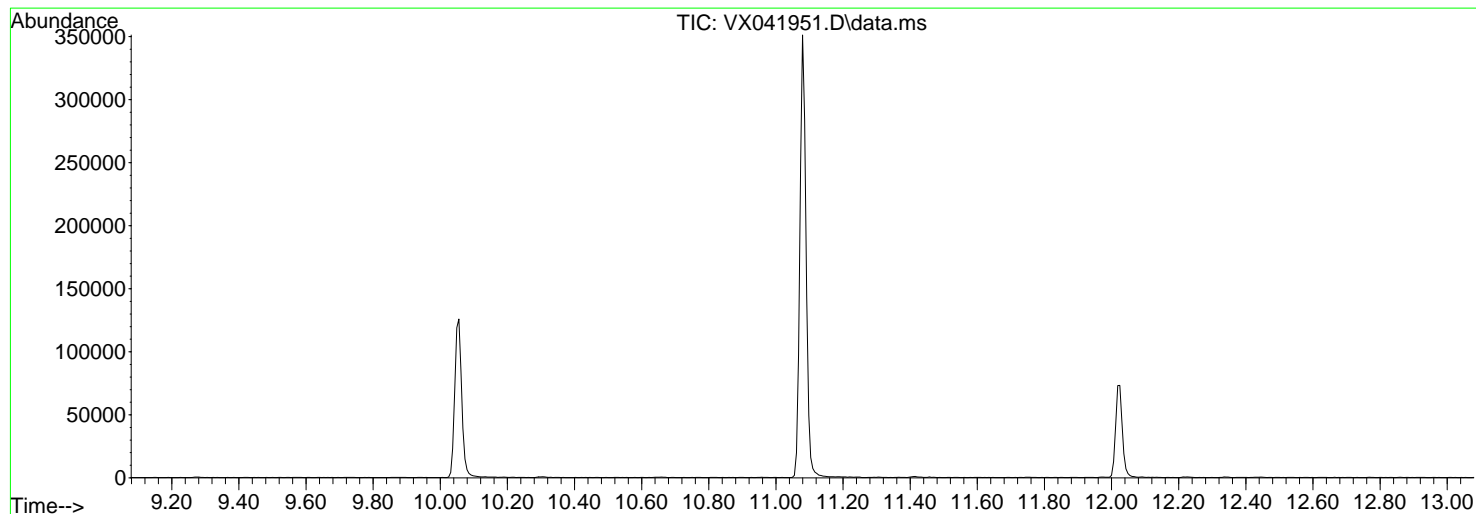

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9671	PASS
75	95	30	60	46.9	27795	PASS
95	95	100	100	100.0	59299	PASS
96	95	5	9	6.6	3933	PASS
173	174	0.00	2	0.4	217	PASS
174	95	50	100	95.6	56691	PASS
175	174	5	9	7.5	4229	PASS
176	174	95	101	97.5	55277	PASS
177	176	5	9	6.7	3725	PASS