

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062025\
 Data File : VX046799.D
 Acq On : 20 Jun 2025 21:07
 Operator : JC/MD
 Sample : Q2378-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Jun 21 00:15:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 18 03:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	179697	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	311845	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	274663	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	133303	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	120570	48.509	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.020%
35) Dibromofluoromethane	5.397	113	99867	48.402	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.800%
50) Toluene-d8	8.647	98	367935	49.635	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.260%
62) 4-Bromofluorobenzene	11.079	95	134631	48.722	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	97.440%
Target Compounds						
					Qvalue	
3) Chloromethane	1.258	50	2196	1.060	ug/l #	44
10) Methyl Iodide	2.483	142	220	4.412	ug/l #	38
16) Acetone	2.398	43	394	0.475	ug/l #	44
31) Cyclohexane	5.568	56	3794	1.019	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	14212	4.772	ug/l #	47
38) Carbon Tetrachloride	5.562	117	18351	5.677	ug/l #	17
76) 1,2,3-Trichloropropane	11.079	75	67523	27.657	ug/l #	41
81) trans-1,4-Dichloro-2-b...	11.079	75	67523	78.174	ug/l #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062025\
Data File : VX046799.D
Acq On : 20 Jun 2025 21:07
Operator : JC/MD
Sample : Q2378-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Jun 21 00:15:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 18 03:09:16 2025
Response via : Initial Calibration




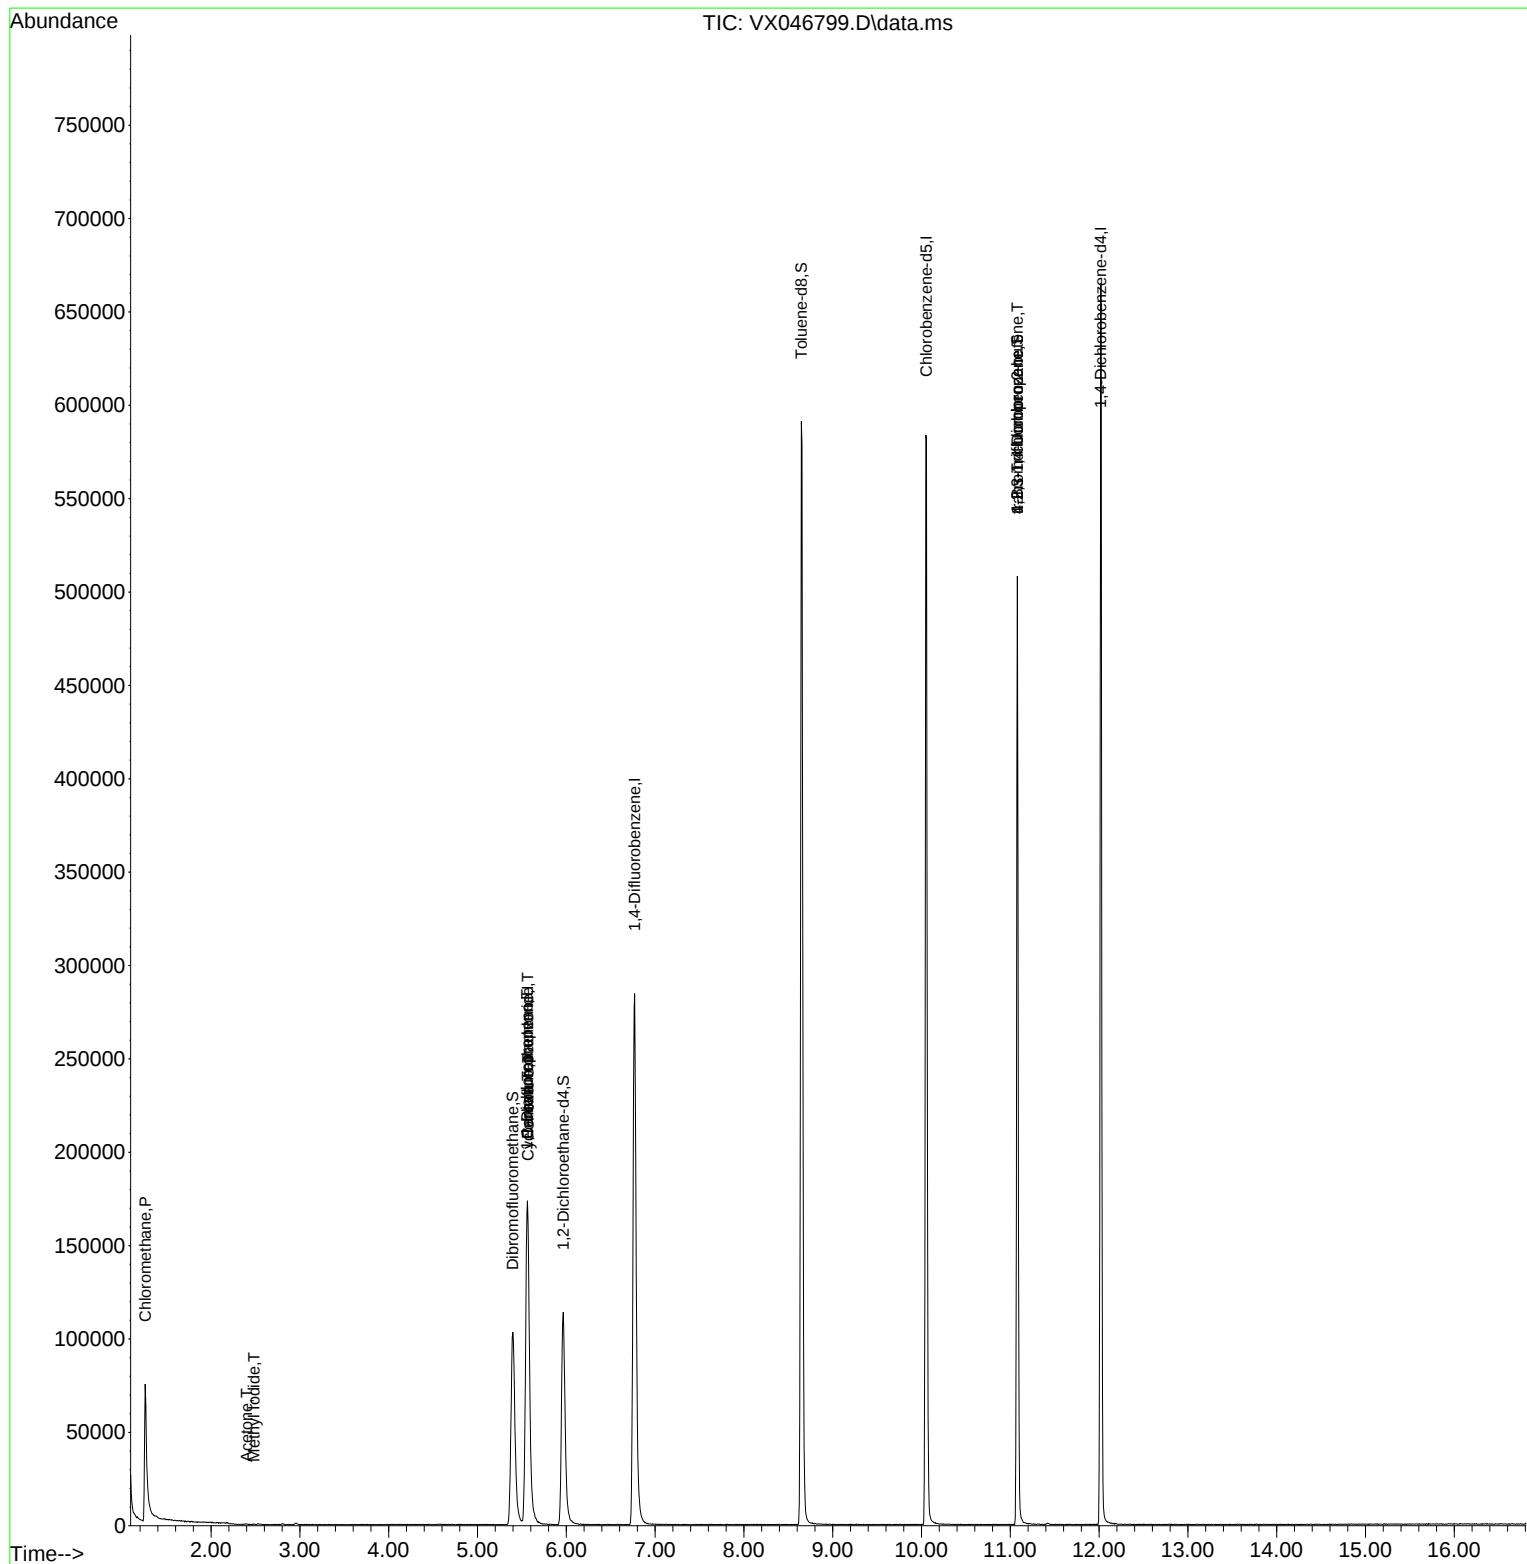


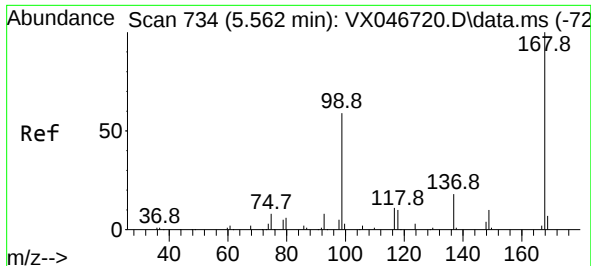

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 179697
Ion Ratio Lower Upper
168 100
99 61.9 48.5 72.7

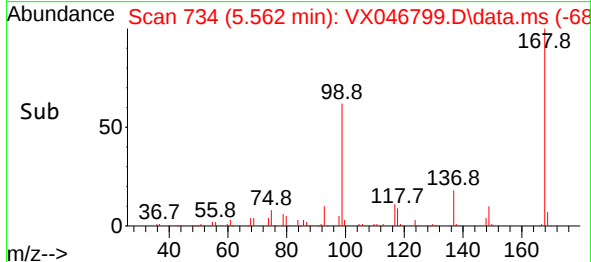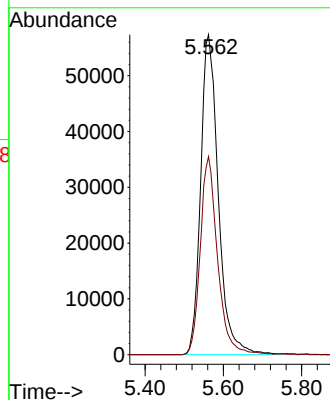

#3
Chloromethane
Concen: 1.060 ug/l
RT: 1.258 min Scan# 28
Delta R.T. -0.049 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion: 50 Resp: 2196
Ion Ratio Lower Upper
50 100
52 0.0 24.9 37.3#


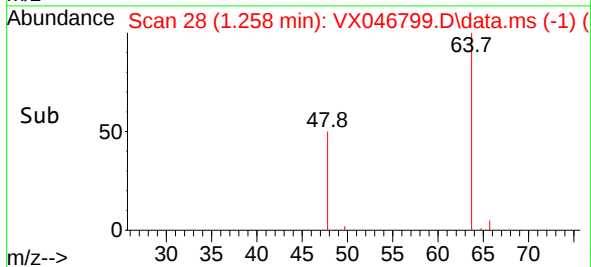
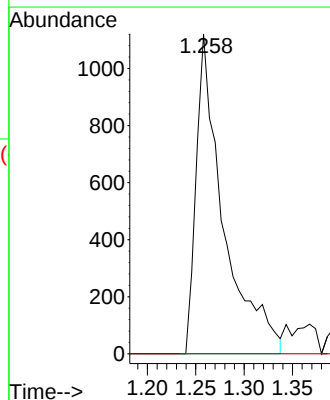
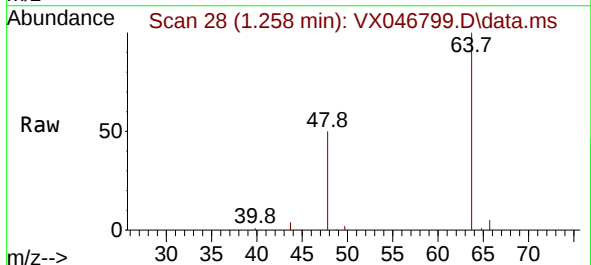


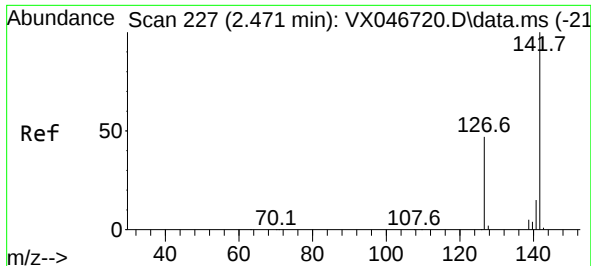

#10
Methyl Iodide
Concen: 4.412 ug/l
RT: 2.483 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:142 Resp: 220
Ion Ratio Lower Upper
142 100
127 0.0 37.0 55.6#
141 0.0 11.5 17.3#

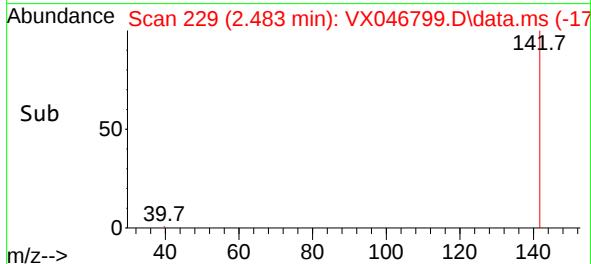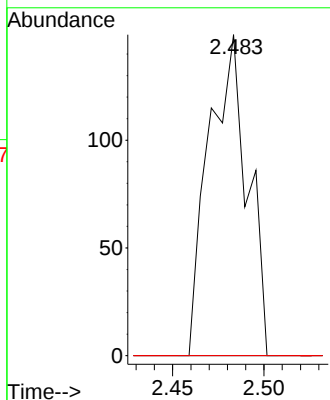

#16
Acetone
Concen: 0.475 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.012 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion: 43 Resp: 394
Ion Ratio Lower Upper
43 100
58 0.0 24.5 36.7#


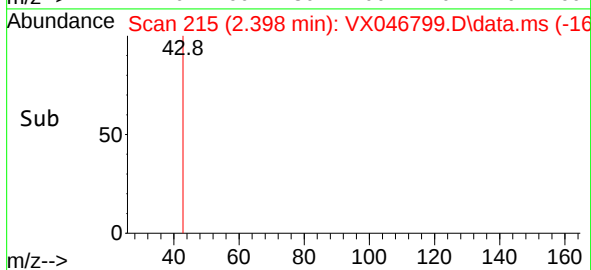
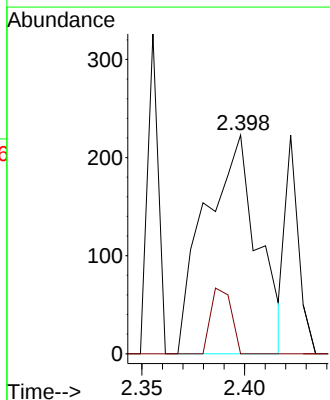
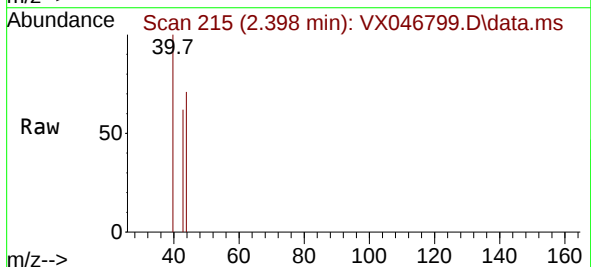




#31
Cyclohexane
Concen: 1.019 ug/l
RT: 5.568 min Scan# 71
Delta R.T. 0.085 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 56 Resp: 3794
Ion Ratio Lower Upper
56 100
69 177.2 24.8 37.2#
84 155.6 68.2 102.2#

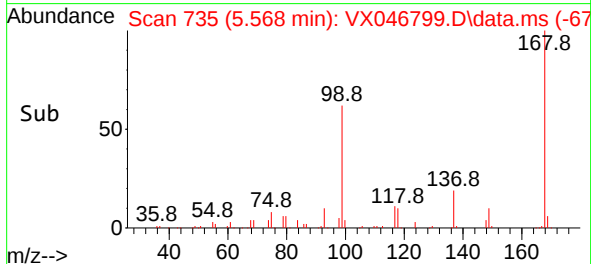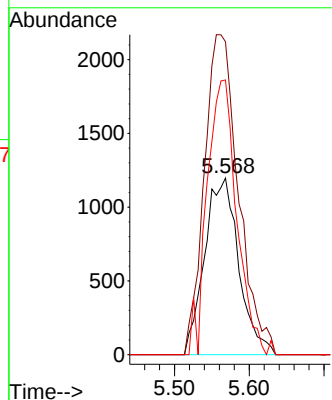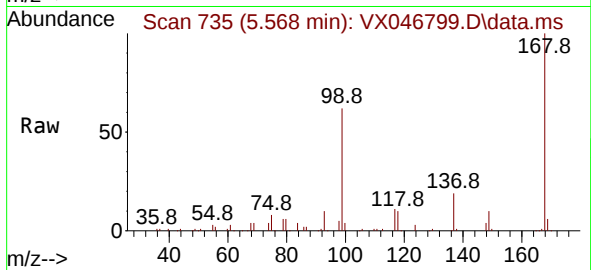

#33
1,2-Dichloroethane-d4
Concen: 48.509 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion: 65 Resp: 120570
Ion Ratio Lower Upper
65 100
67 51.6 0.0 105.4



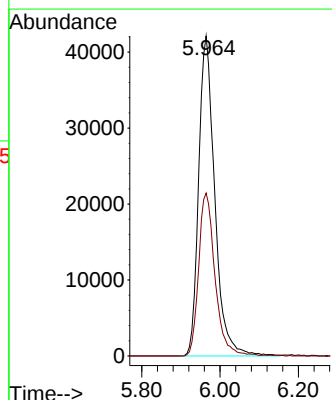
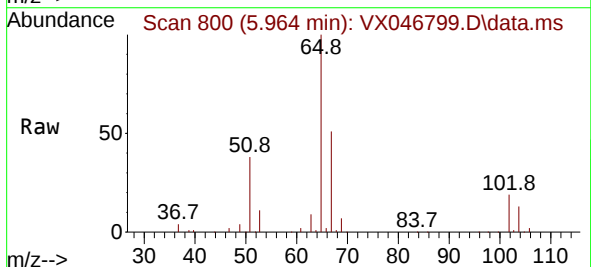


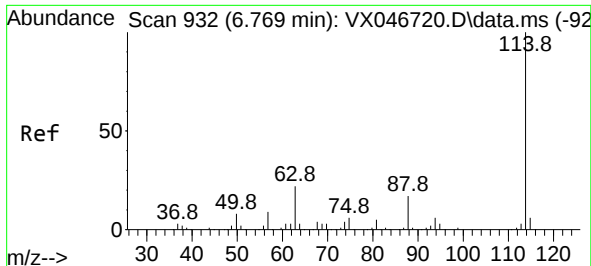

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 311845
Ion Ratio Lower Upper
114 100
63 20.8 0.0 44.2
88 16.4 0.0 33.2

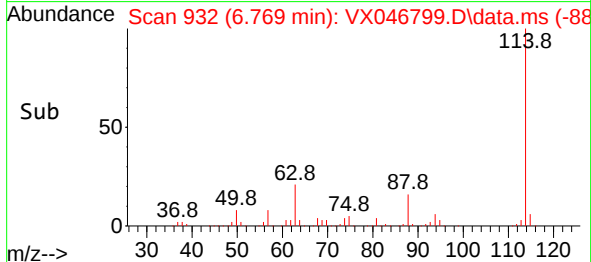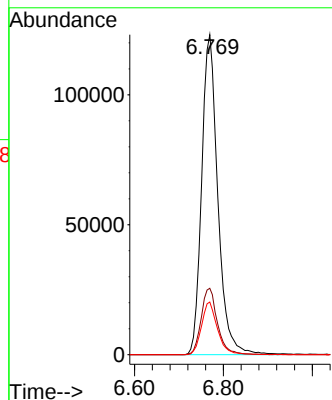

#35
Dibromofluoromethane
Concen: 48.402 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion:113 Resp: 99867
Ion Ratio Lower Upper
113 100
111 103.3 82.0 123.0
192 19.1 15.3 22.9


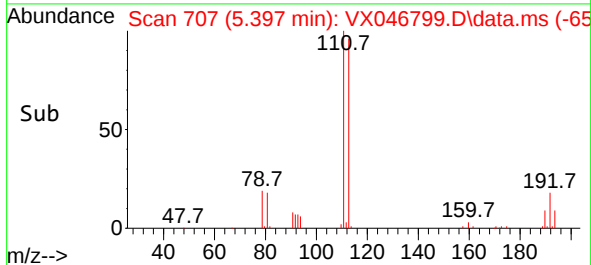
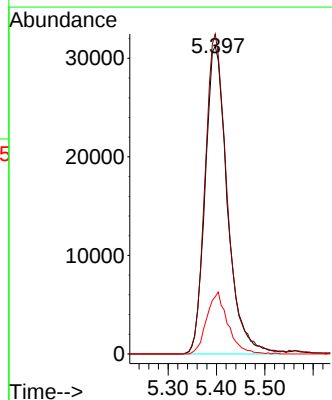
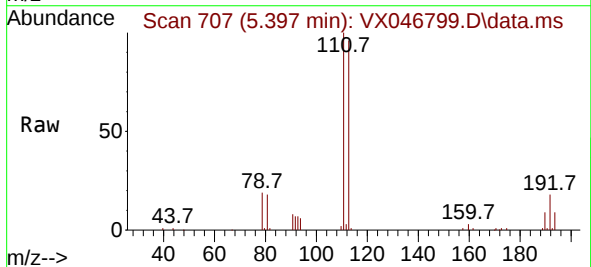


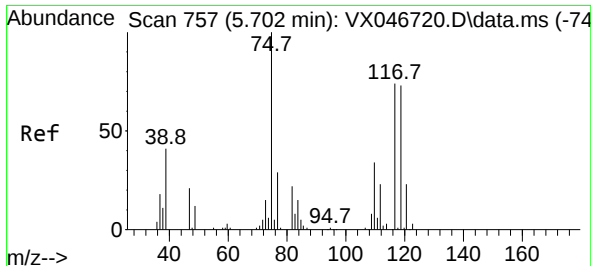

#36
1,1-Dichloropropene
Concen: 4.772 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.146 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 75 Resp: 14212
Ion Ratio Lower Upper
75 100
110 5.1 17.2 51.5#
77 0.0 24.2 36.4#

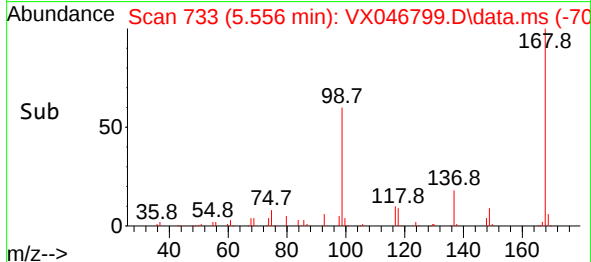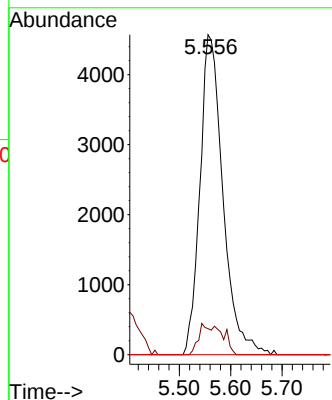

#38
Carbon Tetrachloride
Concen: 5.677 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion: 117 Resp: 18351
Ion Ratio Lower Upper
117 100
119 4.7 75.2 112.8#
121 0.0 24.1 36.1#


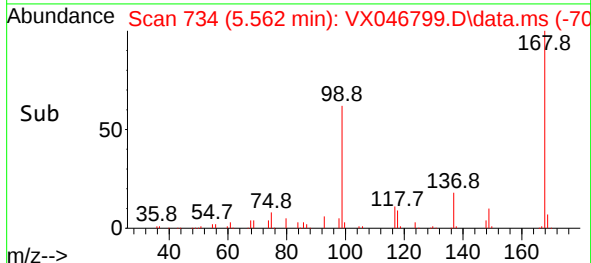
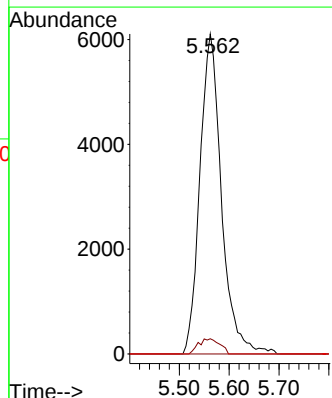
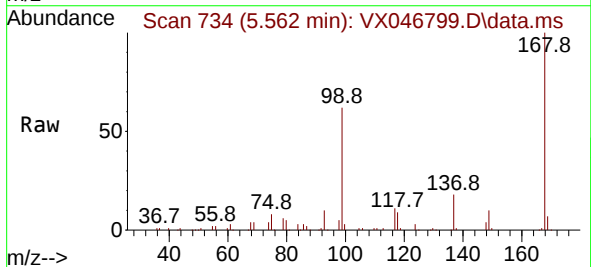


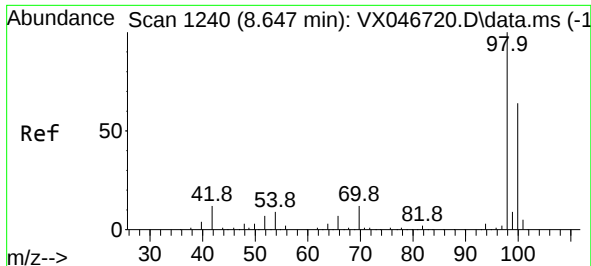

#50
Toluene-d8
Concen: 49.635 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 367935
Ion Ratio Lower Upper
98 100
100 66.6 53.0 79.4

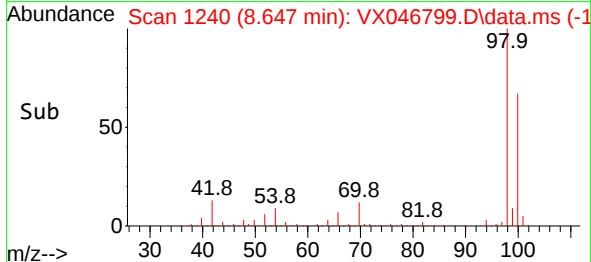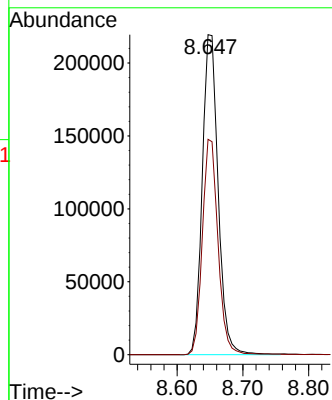

#62
4-Bromofluorobenzene
Concen: 48.722 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion: 95 Resp: 134631
Ion Ratio Lower Upper
95 100
174 75.3 0.0 150.4
176 71.8 0.0 145.0


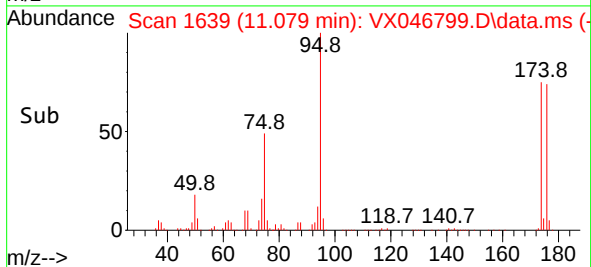
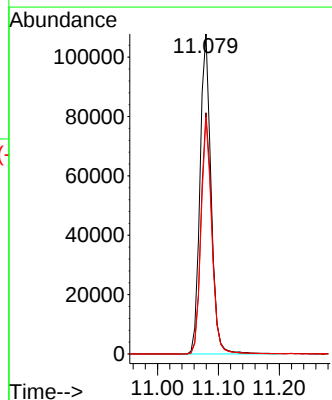
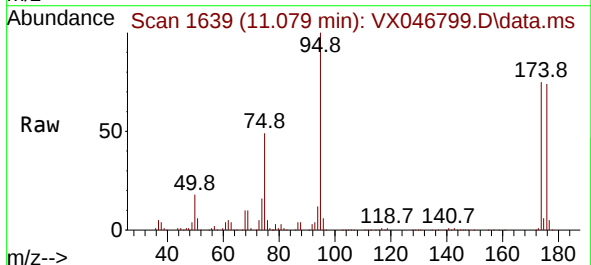




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:117 Resp: 274663
Ion Ratio Lower Upper
117 100
82 54.6 44.6 66.8
119 32.9 25.8 38.8

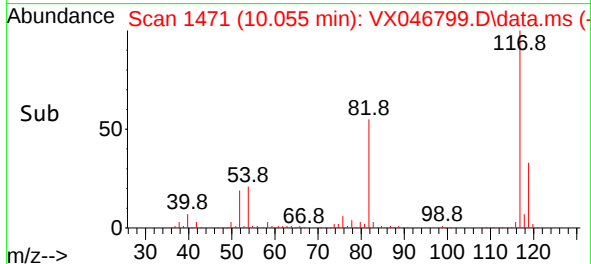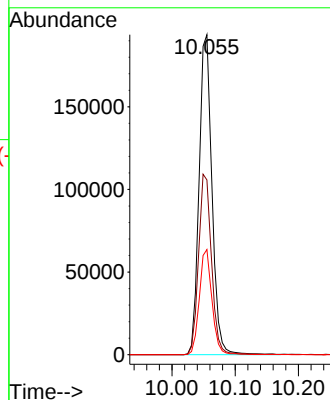

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion:152 Resp: 133303
Ion Ratio Lower Upper
152 100
115 60.6 43.2 129.6
150 157.6 0.0 346.8



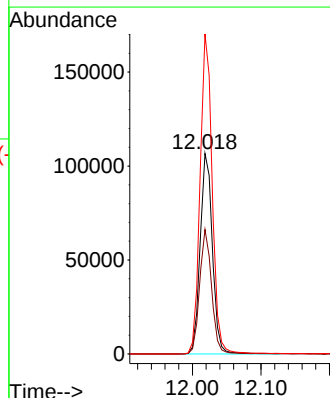
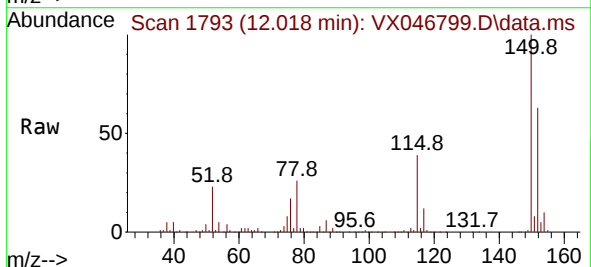


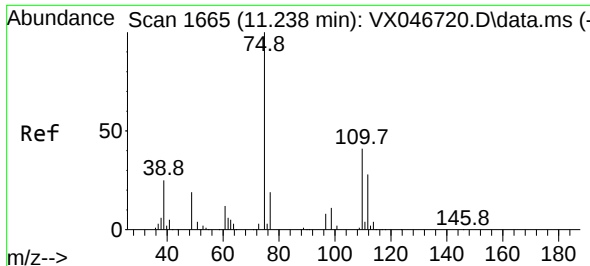

#76
1,2,3-Trichloropropane
Concen: 27.657 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion: 75 Resp: 67523
Ion Ratio Lower Upper
75 100
77 1.9 18.5 55.5#

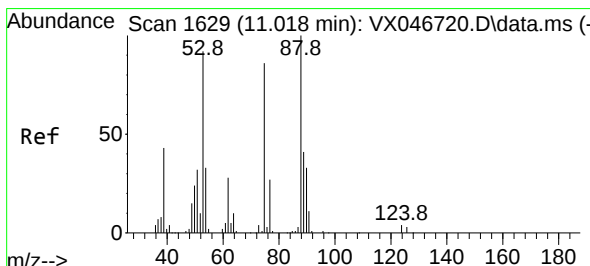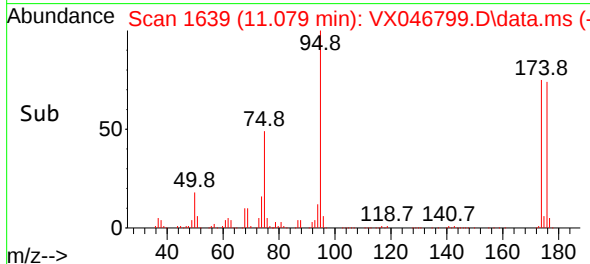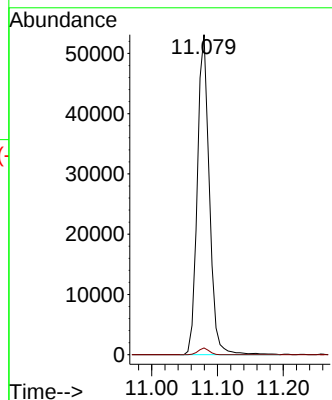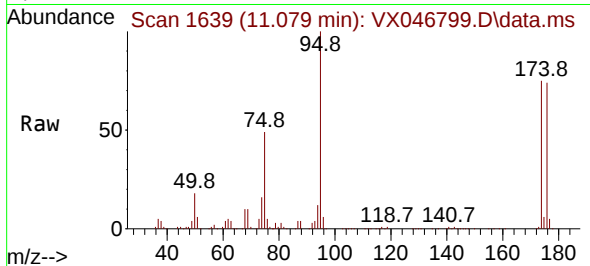

#81
trans-1,4-Dichloro-2-butene
Concen: 78.174 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046799.D
Acq: 20 Jun 2025 21:07

Tgt Ion: 75 Resp: 67523
Ion Ratio Lower Upper
75 100
53 0.0 86.8 130.2#
89 0.0 36.9 55.3#

