
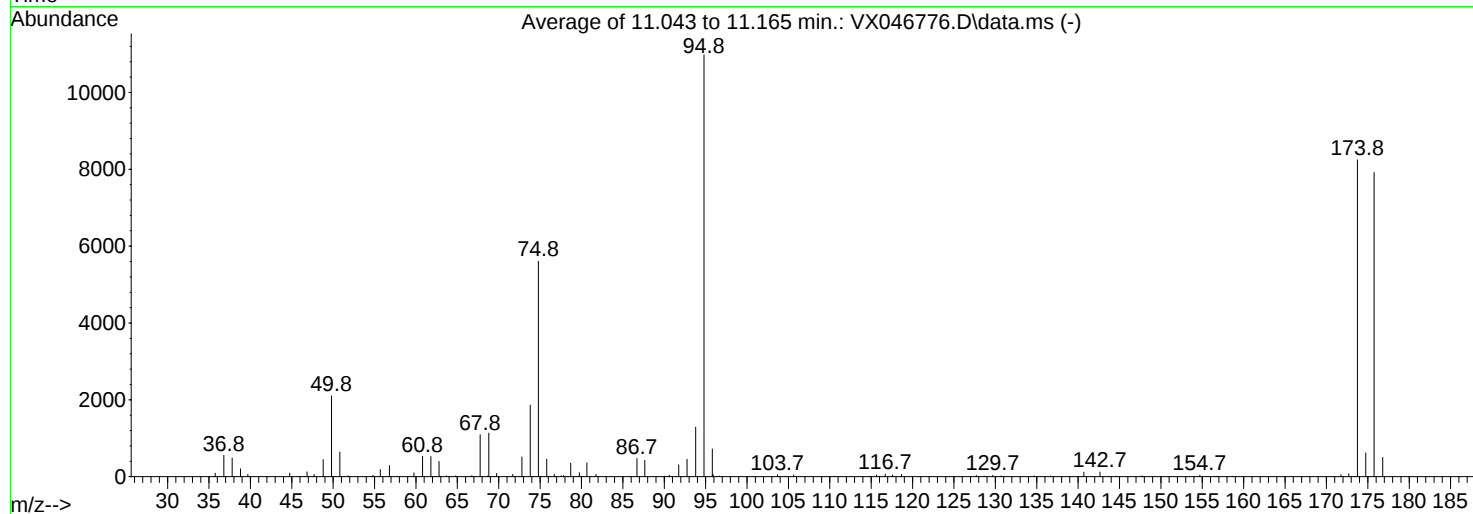


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062025\
Data File : VX046776.D
Acq On : 20 Jun 2025 08:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061025W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jun 11 06:20:28 2025

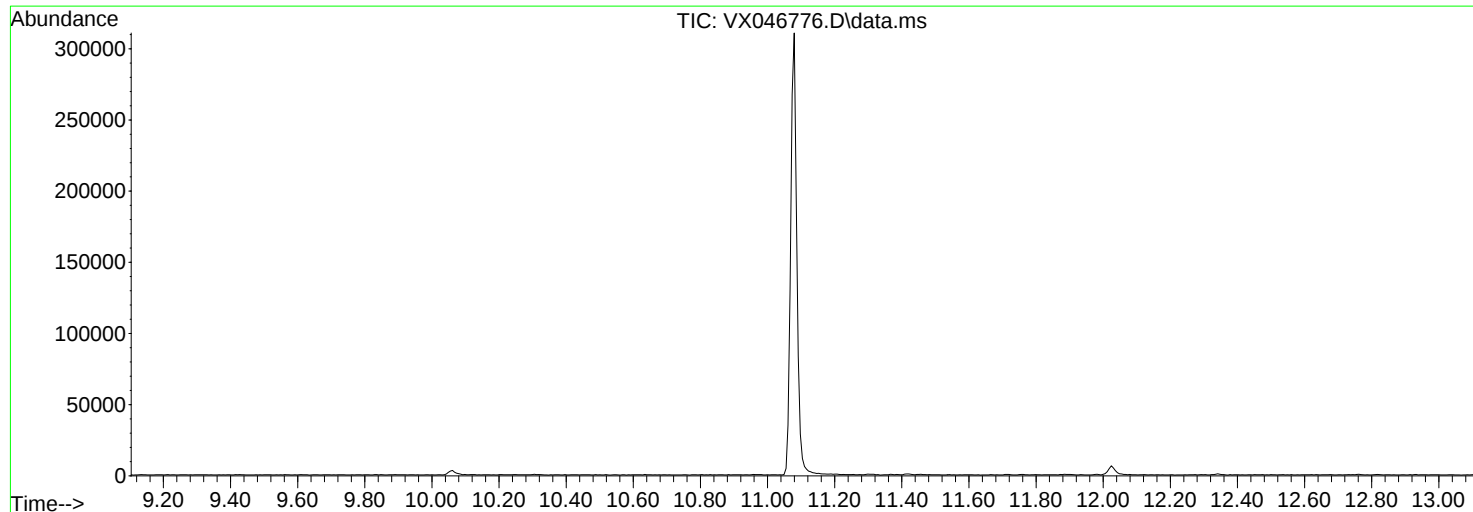

AutoFind: Averaged scan 1633 to 1653; Bkg corrected with scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	2105	PASS
75	95	30	60	51.1	5607	PASS
95	95	100	100	100.0	10980	PASS
96	95	5	9	6.6	720	PASS
173	174	0.00	2	0.9	76	PASS
174	95	50	100	75.1	8245	PASS
175	174	5	9	7.5	617	PASS
176	174	95	101	96.0	7918	PASS
177	176	5	9	6.3	502	PASS