

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062119\
 Data File : VX010393.D
 Acq On : 21 Jun 2019 18:32
 Operator : JC/SP
 Sample : K3477-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	16	21	30	rBV2	53592	77206	5.81%	1.086%
2	1.611	66	75	78	rBV5	6350	14277	1.08%	0.201%
3	2.611	233	239	246	rBV	22140	40665	3.06%	0.572%
4	3.019	297	306	315	rBV	8143	21244	1.60%	0.299%
5	5.501	702	713	727	rBV	158685	449191	33.82%	6.321%
6	5.659	727	739	754	rVB	272376	765140	57.62%	10.768%
7	6.061	795	805	818	rBV	153290	400454	30.15%	5.635%
8	6.860	926	936	950	rBV	406270	952407	71.72%	13.403%
9	8.713	1232	1240	1255	rBV	855627	1328011	100.00%	18.689%
10	10.110	1463	1469	1483	rBV	817180	1126434	84.82%	15.852%
11	11.134	1631	1637	1648	rBV	692846	884973	66.64%	12.454%
12	12.079	1786	1792	1803	rVB	807000	1045998	78.76%	14.720%


Sum of corrected areas: 7106000

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062119\
Data File : VX010393.D
Acq On : 21 Jun 2019 18:32
Operator : JC/SP
Sample : K3477-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

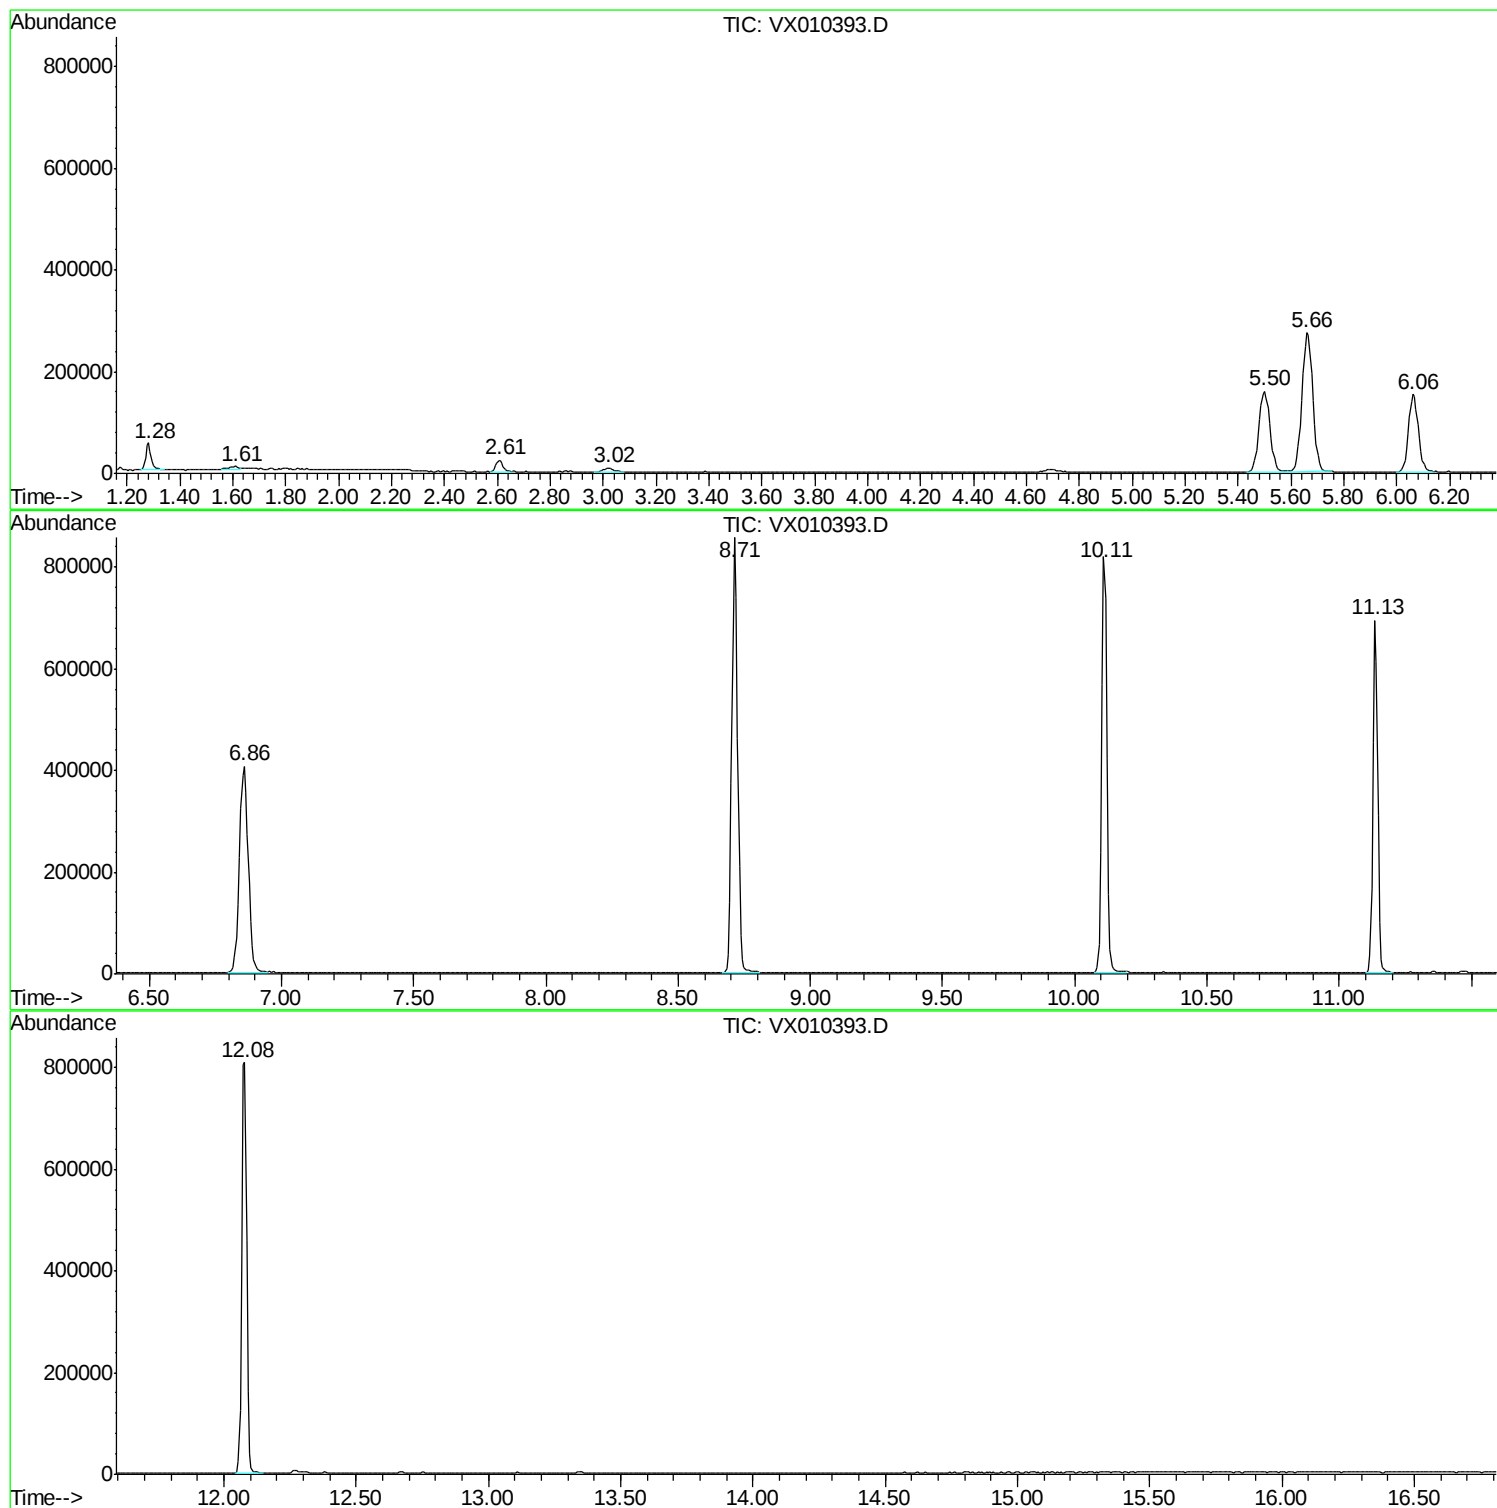

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062119\
Data File : VX010393.D
Acq On : 21 Jun 2019 18:32
Operator : JC/SP
Sample : K3477-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.28	5.05 ug/l	77206	Pentafluorobenzene	5.67
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		Sulfur dioxide	64 O2S	007446-09-5 72
2		Aminomethanesulfonic acid	111 CH5NO3S	013881-91-9 39
3		L-Alanine, 3-sulfo-	169 C3H7NO5S	000498-40-8 9
4		Ethanol, 2-fluoro-	64 C2H5FO	000371-62-0 3
5		Ethyl Chloride	64 C2H5Cl	000075-00-3 3

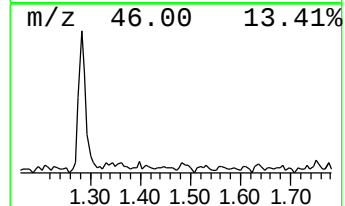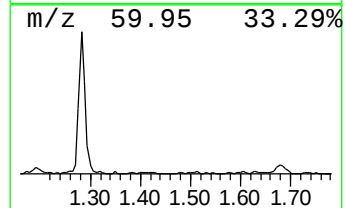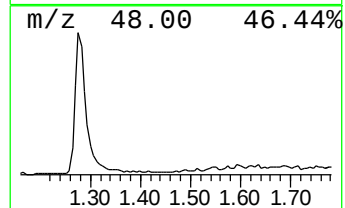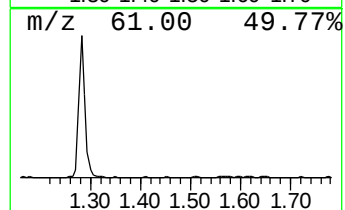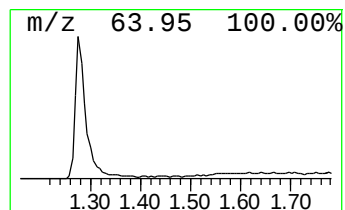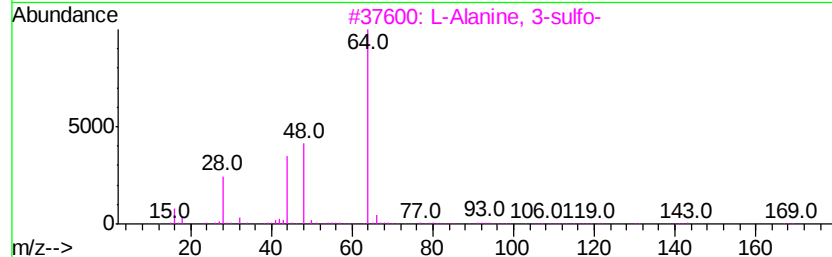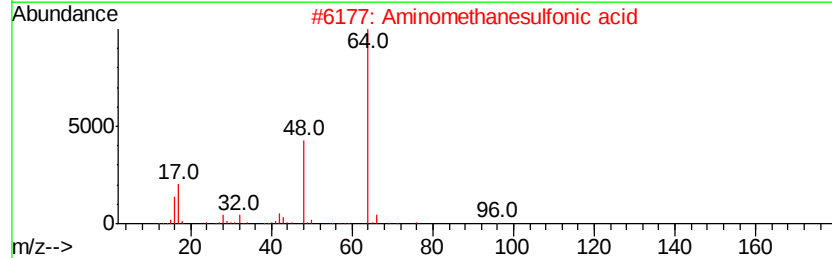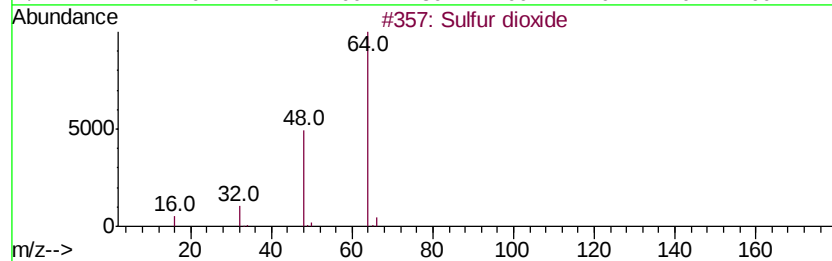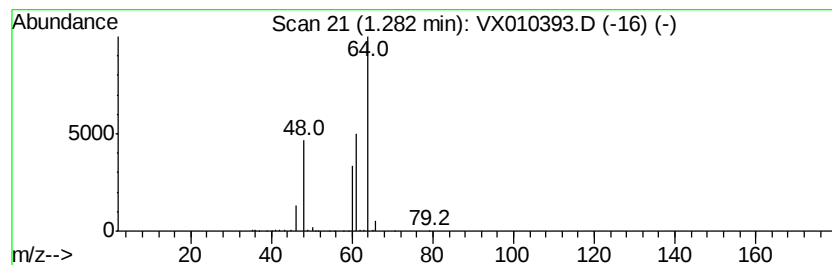

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX062119\
Data File : VX010393.D
Acq On : 21 Jun 2019 18:32
Operator : JC/SP
Sample : K3477-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.28	5.0	ug/l	77206	1	5.67	765140	50.0