

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062121\
 Data File : VX022786.D
 Acq On : 21 Jun 2021 11:52
 Operator : JC/MD
 Sample : M2753-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB01-20210616

Quant Time: Jun 22 01:11:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 12:20:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	56559	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	113260	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	98869	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	35789	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	53362	52.460	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	104.920%
35) Dibromofluoromethane	5.397	113	38271	52.961	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	105.920%
50) Toluene-d8	8.653	98	151605	53.220	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.440%
62) 4-Bromofluorobenzene	11.085	95	50265	46.656	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.320%
Target Compounds						
16) Acetone	2.392	43	1770	3.886	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062121\
Data File : VX022786.D
Acq On : 21 Jun 2021 11:52
Operator : JC/MD
Sample : M2753-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB01-20210616

Quant Time: Jun 22 01:11:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration




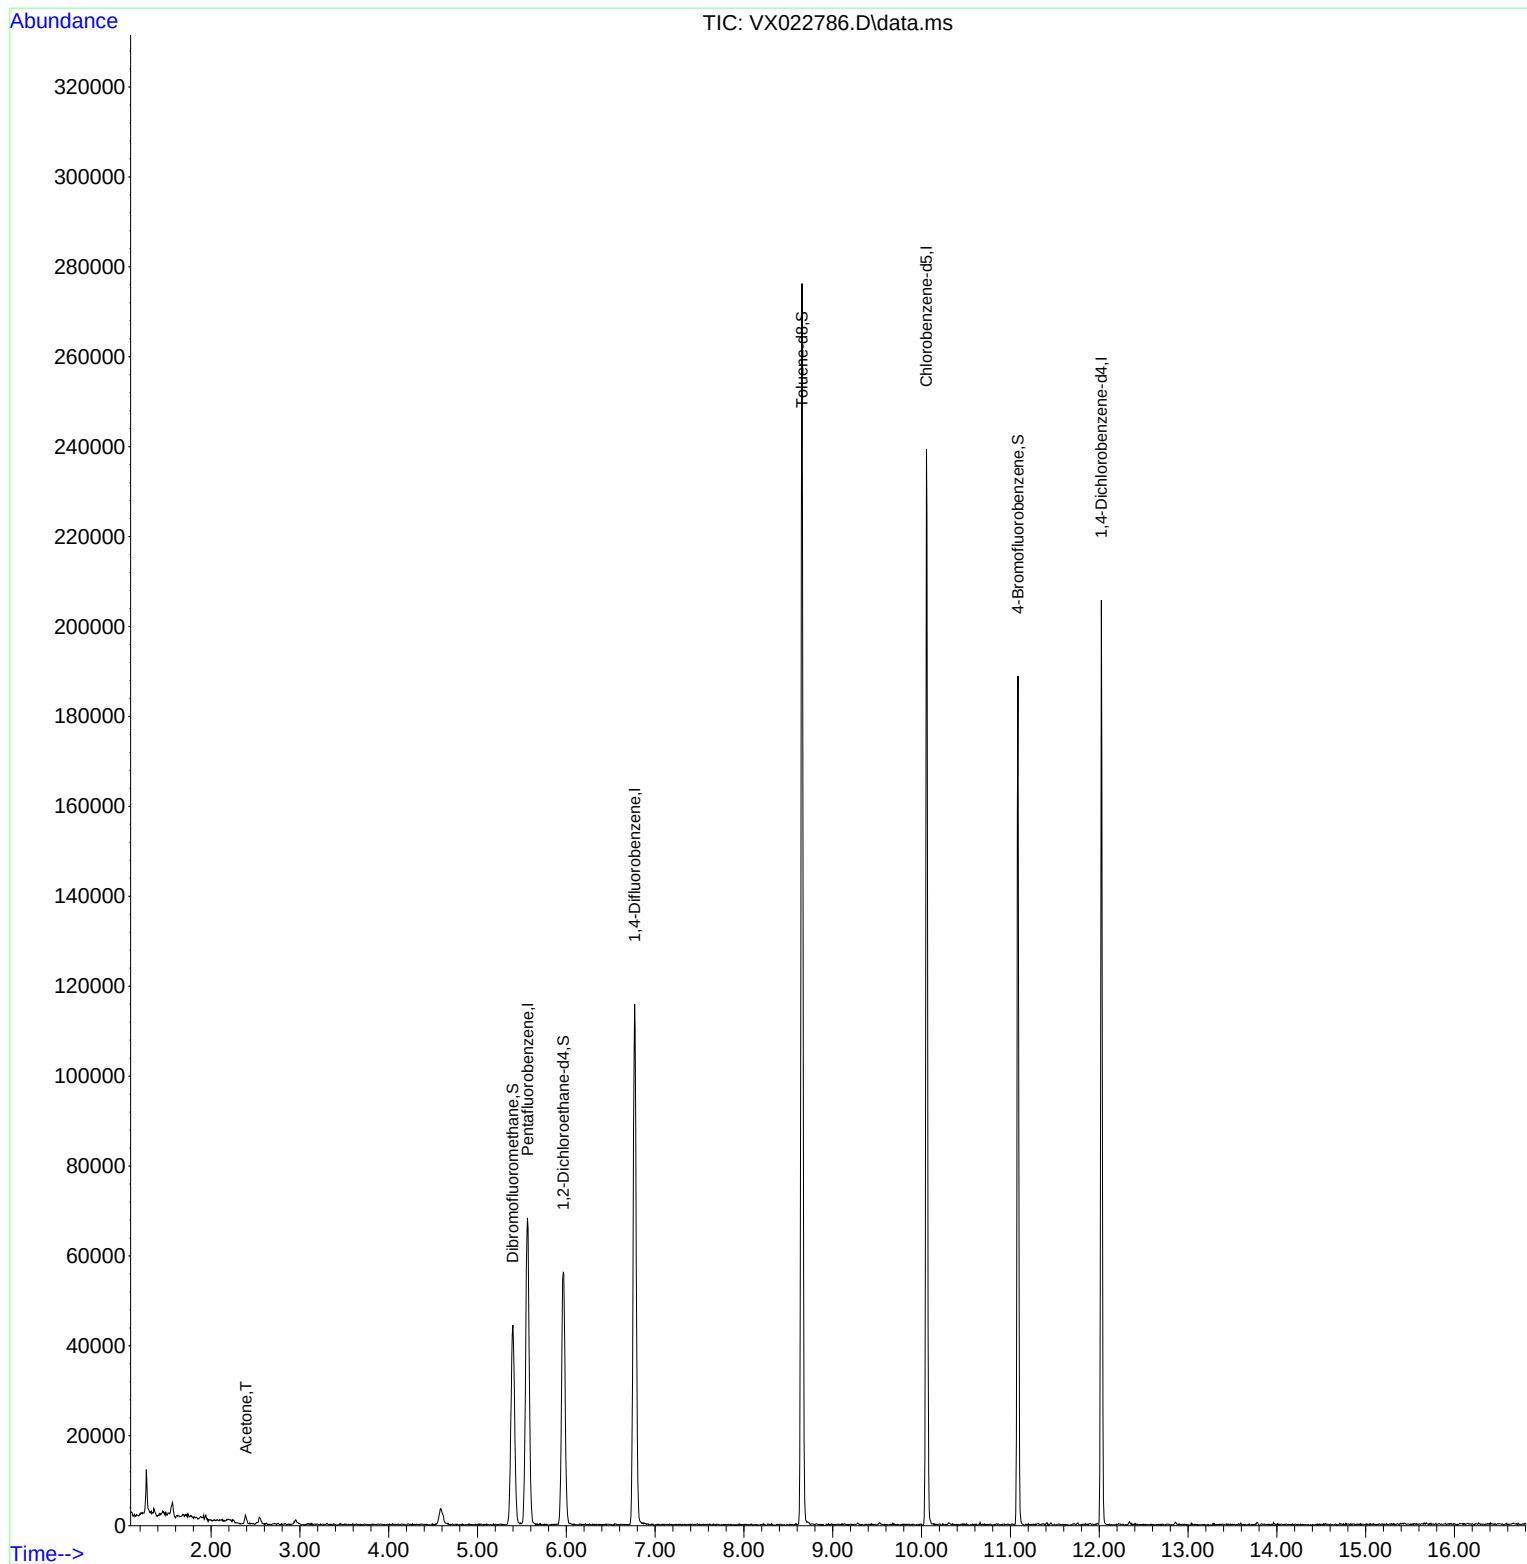


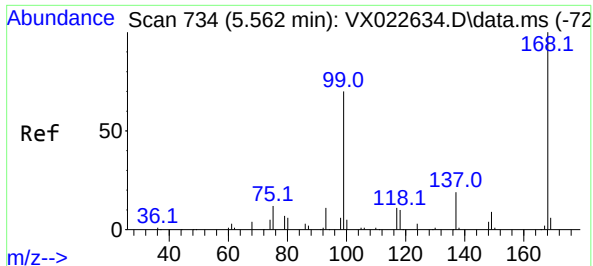

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52




Instrument :
MSVOA_X
ClientSampleId :
EB01-20210616


Tgt Ion:168 Resp: 56559
Ion Ratio Lower Upper
168 100
99 73.6 45.8 68.6#

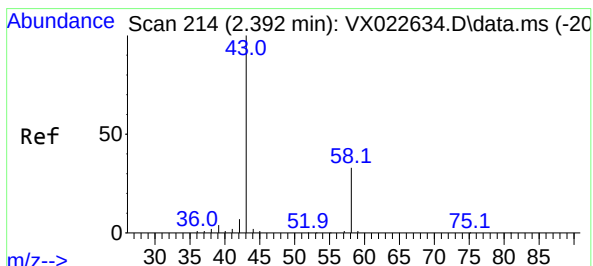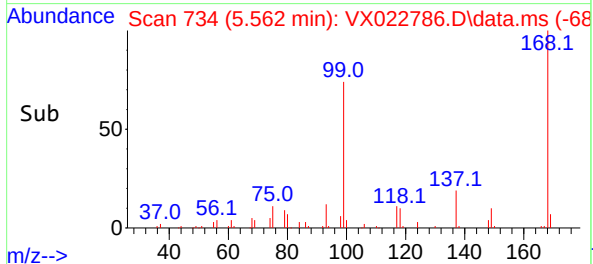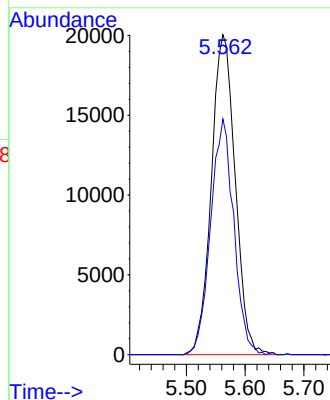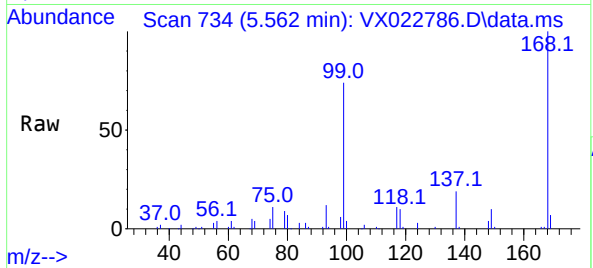

#16
Acetone
Concen: 3.886 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52

Tgt Ion: 43 Resp: 1770
Ion Ratio Lower Upper
43 100
58 29.5 27.8 41.8

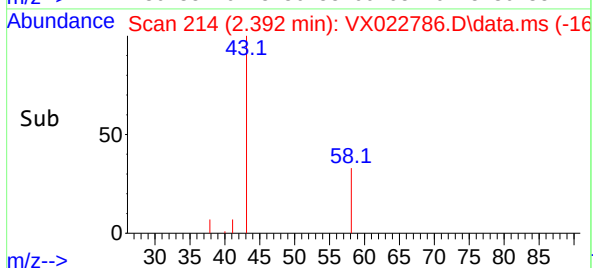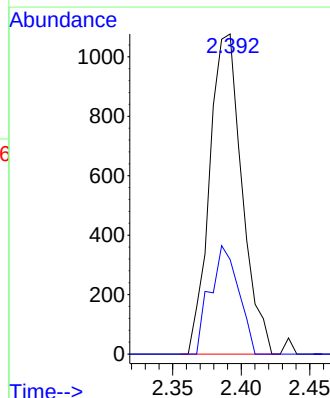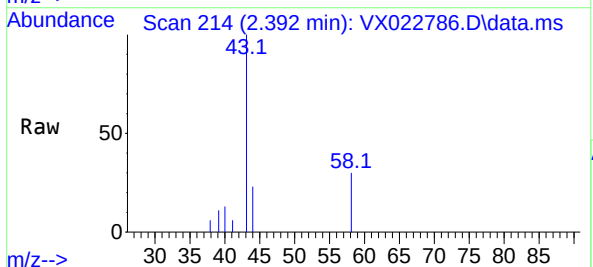




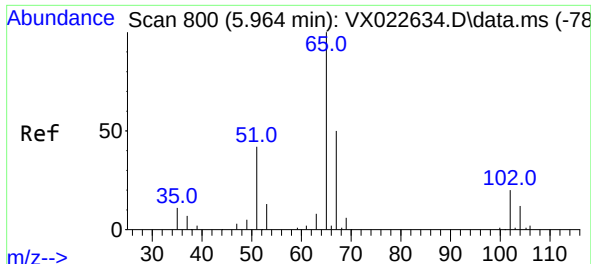


#33

1,2-Dichloroethane-d4
Concen: 52.460 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52

Instrument :
MSVOA_X
ClientSampleId :
EB01-20210616




Tgt Ion: 65 Resp: 53362
Ion Ratio Lower Upper
65 100
67 51.4 0.0 105.4

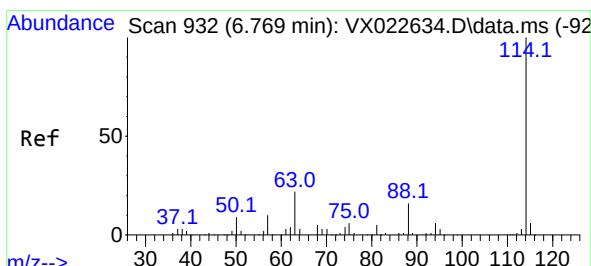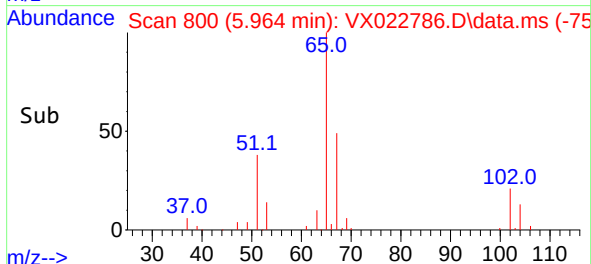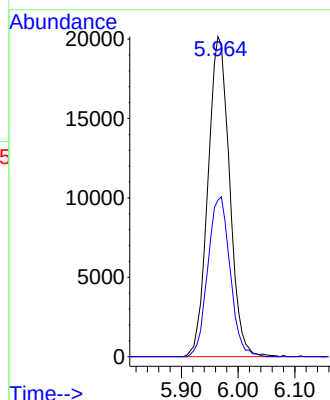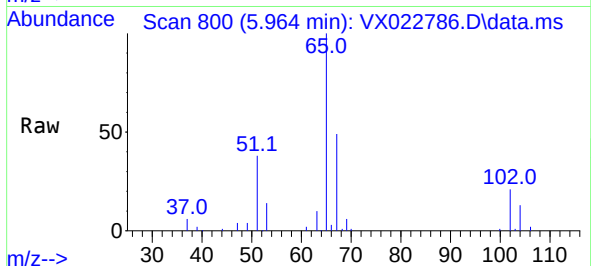


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52

Tgt Ion: 114 Resp: 113260
Ion Ratio Lower Upper
114 100
63 21.6 0.0 40.8
88 15.9 0.0 32.8


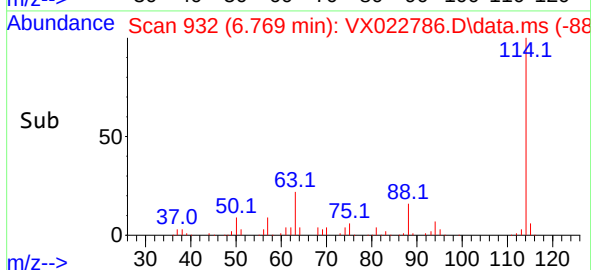
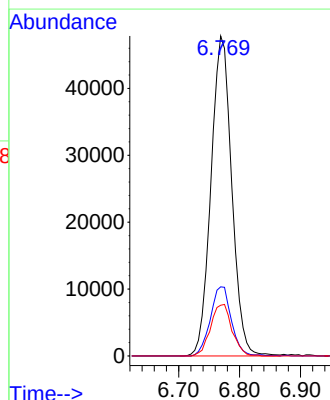
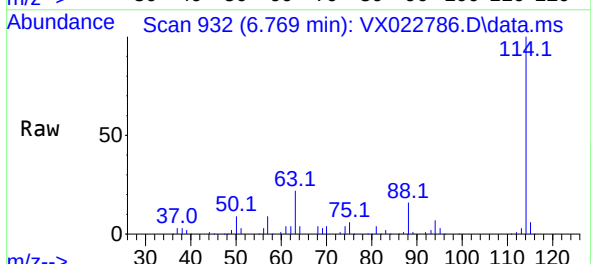


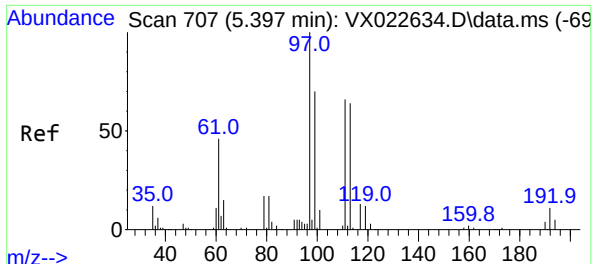

#35
Dibromofluoromethane
Concen: 52.961 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52




Instrument :
MSVOA_X
ClientSampleId :
EB01-20210616


Tgt Ion:113 Resp: 38271
Ion Ratio Lower Upper
113 100
111 105.6 81.9 122.9
192 14.7 16.7 25.1#

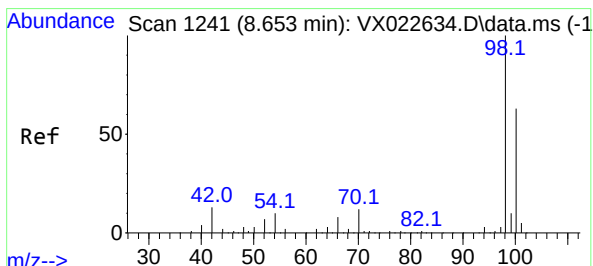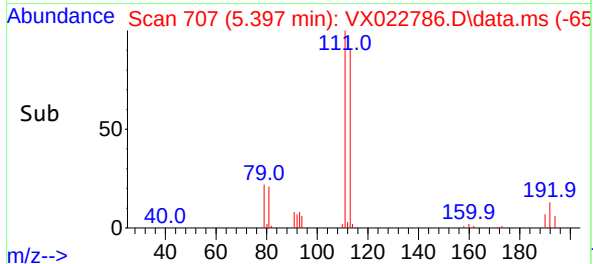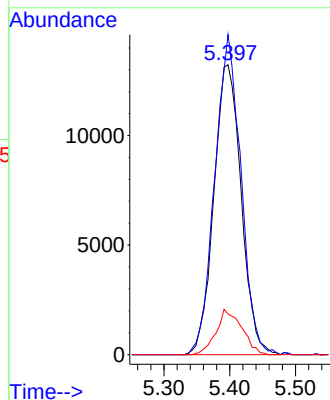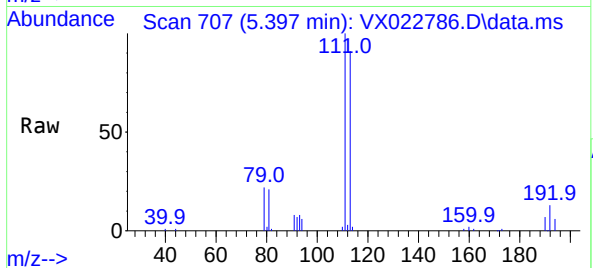

#50
Toluene-d8
Concen: 53.220 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52

Tgt Ion: 98 Resp: 151605
Ion Ratio Lower Upper
98 100
100 64.8 51.9 77.9

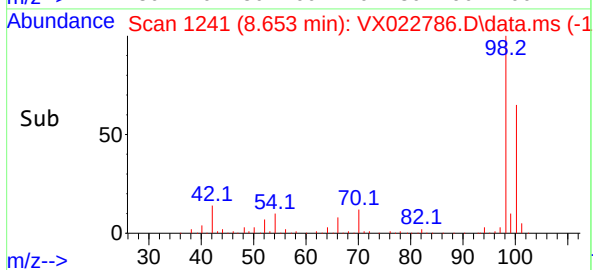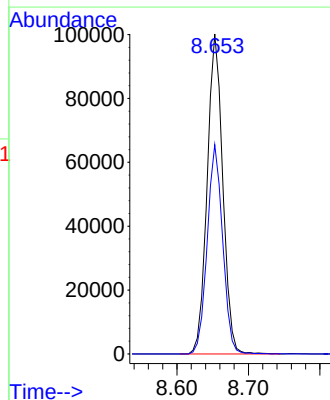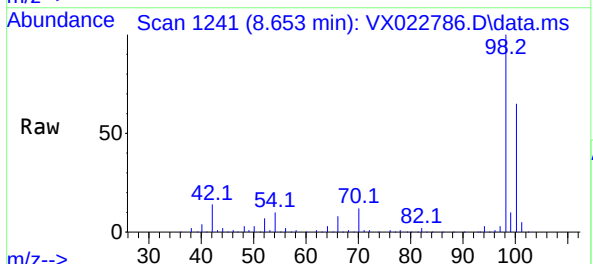




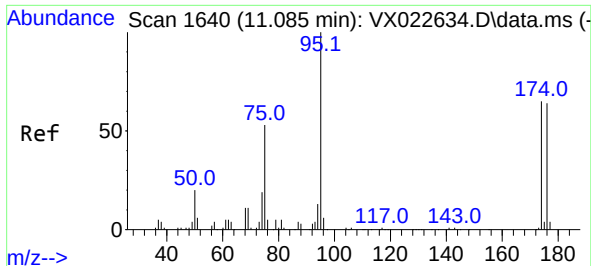


#62
4-Bromofluorobenzene
Concen: 46.656 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52

Instrument :
MSVOA_X
ClientSampleId :
EB01-20210616

Tgt Ion: 95 Resp: 50265




Ion	Ratio	Lower	Upper
95	100		
174	60.9	0.0	154.6
176	60.3	0.0	155.8

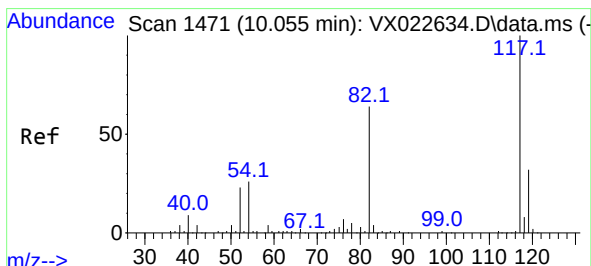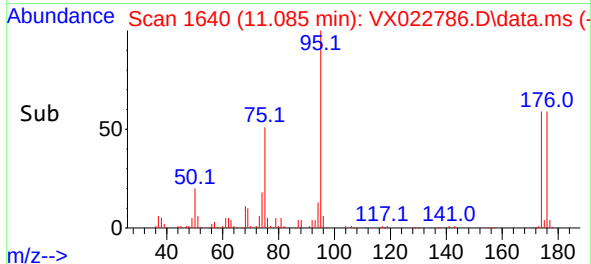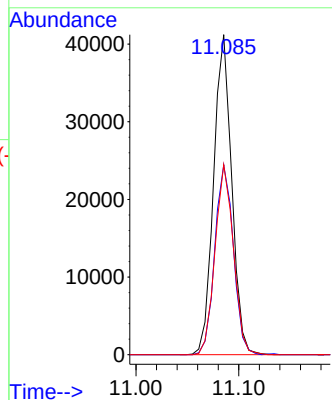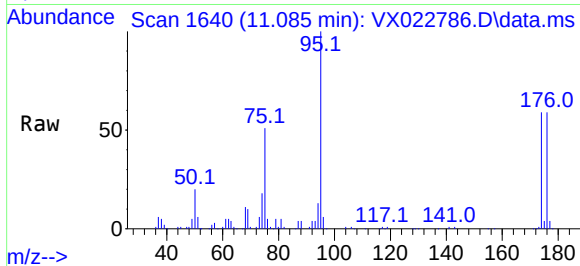


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX022786.D
Acq: 21 Jun 2021 11:52

Tgt Ion: 117 Resp: 98869

Ion	Ratio	Lower	Upper
117	100		
82	62.9	47.4	71.2
119	31.6	26.6	39.8

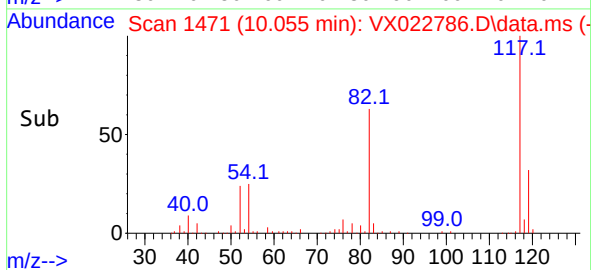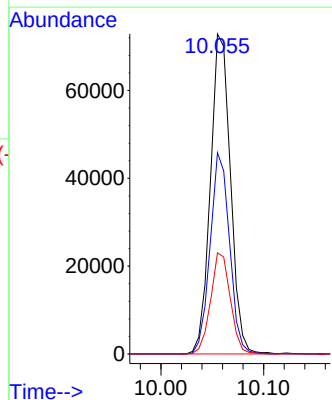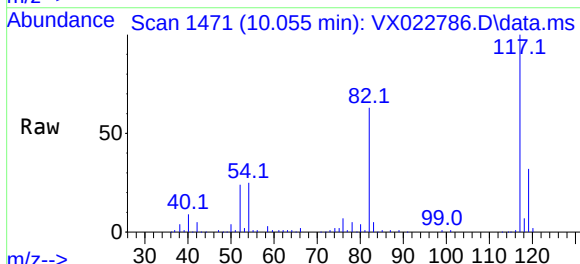

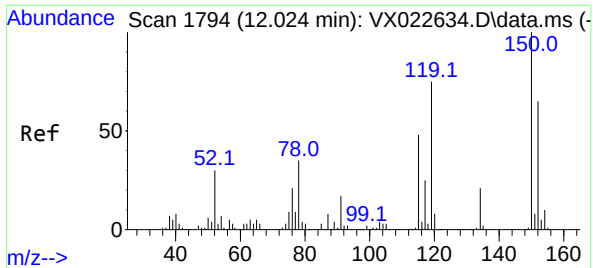

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX022786.D
 Acq: 21 Jun 2021 11:52

Instrument :
 MSVOA_X
 ClientSampleId :
 EB01-20210616

Tgt Ion:152 Resp: 35789
 Ion Ratio Lower Upper
 152 100
 115 67.4 41.1 123.3
 150 157.7 0.0 349.0

