

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
 Data File : VX029663.D
 Acq On : 21 Jun 2022 15:23
 Operator : JC/MD
 Sample : N3286-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1RDL

Quant Time: Jun 22 01:11:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	243207	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	411619	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	359485	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	162294	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	139136	43.218	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.440%
35) Dibromofluoromethane	5.391	113	122285	45.587	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.180%
50) Toluene-d8	8.653	98	466478	47.602	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.200%
62) 4-Bromofluorobenzene	11.085	95	169029	45.739	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.480%


Target Compounds				Qvalue		
3) Chloromethane	1.294	50	1233	0.389	ug/l	98
5) Bromomethane	1.617	94	806	0.541	ug/l #	60
6) Chloroethane	1.697	64	582	1.540	ug/l #	43
10) Methyl Iodide	2.465	142	1007	3.343	ug/l #	75
11) Tert butyl alcohol	2.940	59	6804	0.462	ug/l #	72
13) Acrolein	2.343	56	130	0.733	ug/l #	15
16) Acetone	2.380	43	2522	1.965	ug/l #	87
20) Methylene Chloride	2.794	84	1295	0.453	ug/l #	78
25) 2-Butanone	4.580	43	1411	0.696	ug/l	90
29) Tetrahydrofuran	5.032	42	597	0.442	ug/l #	47
31) Cyclohexane	5.470	56	4800	1.111	ug/l	94
36) 1,1-Dichloropropene	5.556	75	18109	4.988	ug/l #	49
38) Carbon Tetrachloride	5.556	117	24859	6.963	ug/l #	15
39) Methylcyclohexane	7.379	83	3364	0.743	ug/l	97
44) Trichloroethene	7.135	130	1941	Below Cal		97
52) Toluene	8.720	92	1628	0.236	ug/l	84
67) Ethyl Benzene	10.195	91	237000	18.677	ug/l	98
68) m/p-Xylenes	10.305	106	401536	81.144	ug/l	100
69) o-Xylene	10.646	106	16899	3.457	ug/l	92
73) Isopropylbenzene	10.963	105	14381	1.182	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	80072	22.648	ug/l #	36
78) n-propylbenzene	11.305	91	36945	2.696	ug/l	97
79) 2-Chlorotoluene	11.378	91	30696	3.617	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	80303	7.836	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	80072	75.343	ug/l #	15
82) 4-Chlorotoluene	11.451	91	8755	0.905	ug/l #	48
83) tert-Butylbenzene	11.756	119	44796	4.483	ug/l #	55
84) 1,2,4-Trimethylbenzene	11.756	105	365805	35.790	ug/l	100
85) sec-Butylbenzene	11.756	105	365805	29.540	ug/l #	56
89) n-Butylbenzene	12.323	91	4950	0.566	ug/l #	14
90) Hexachloroethane	12.646	117	3594	2.421	ug/l #	10
95) Naphthalene	13.780	128	203742	17.897	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029663.D
Acq On : 21 Jun 2022 15:23
Operator : JC/MD
Sample : N3286-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL

Quant Time: Jun 22 01:11:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




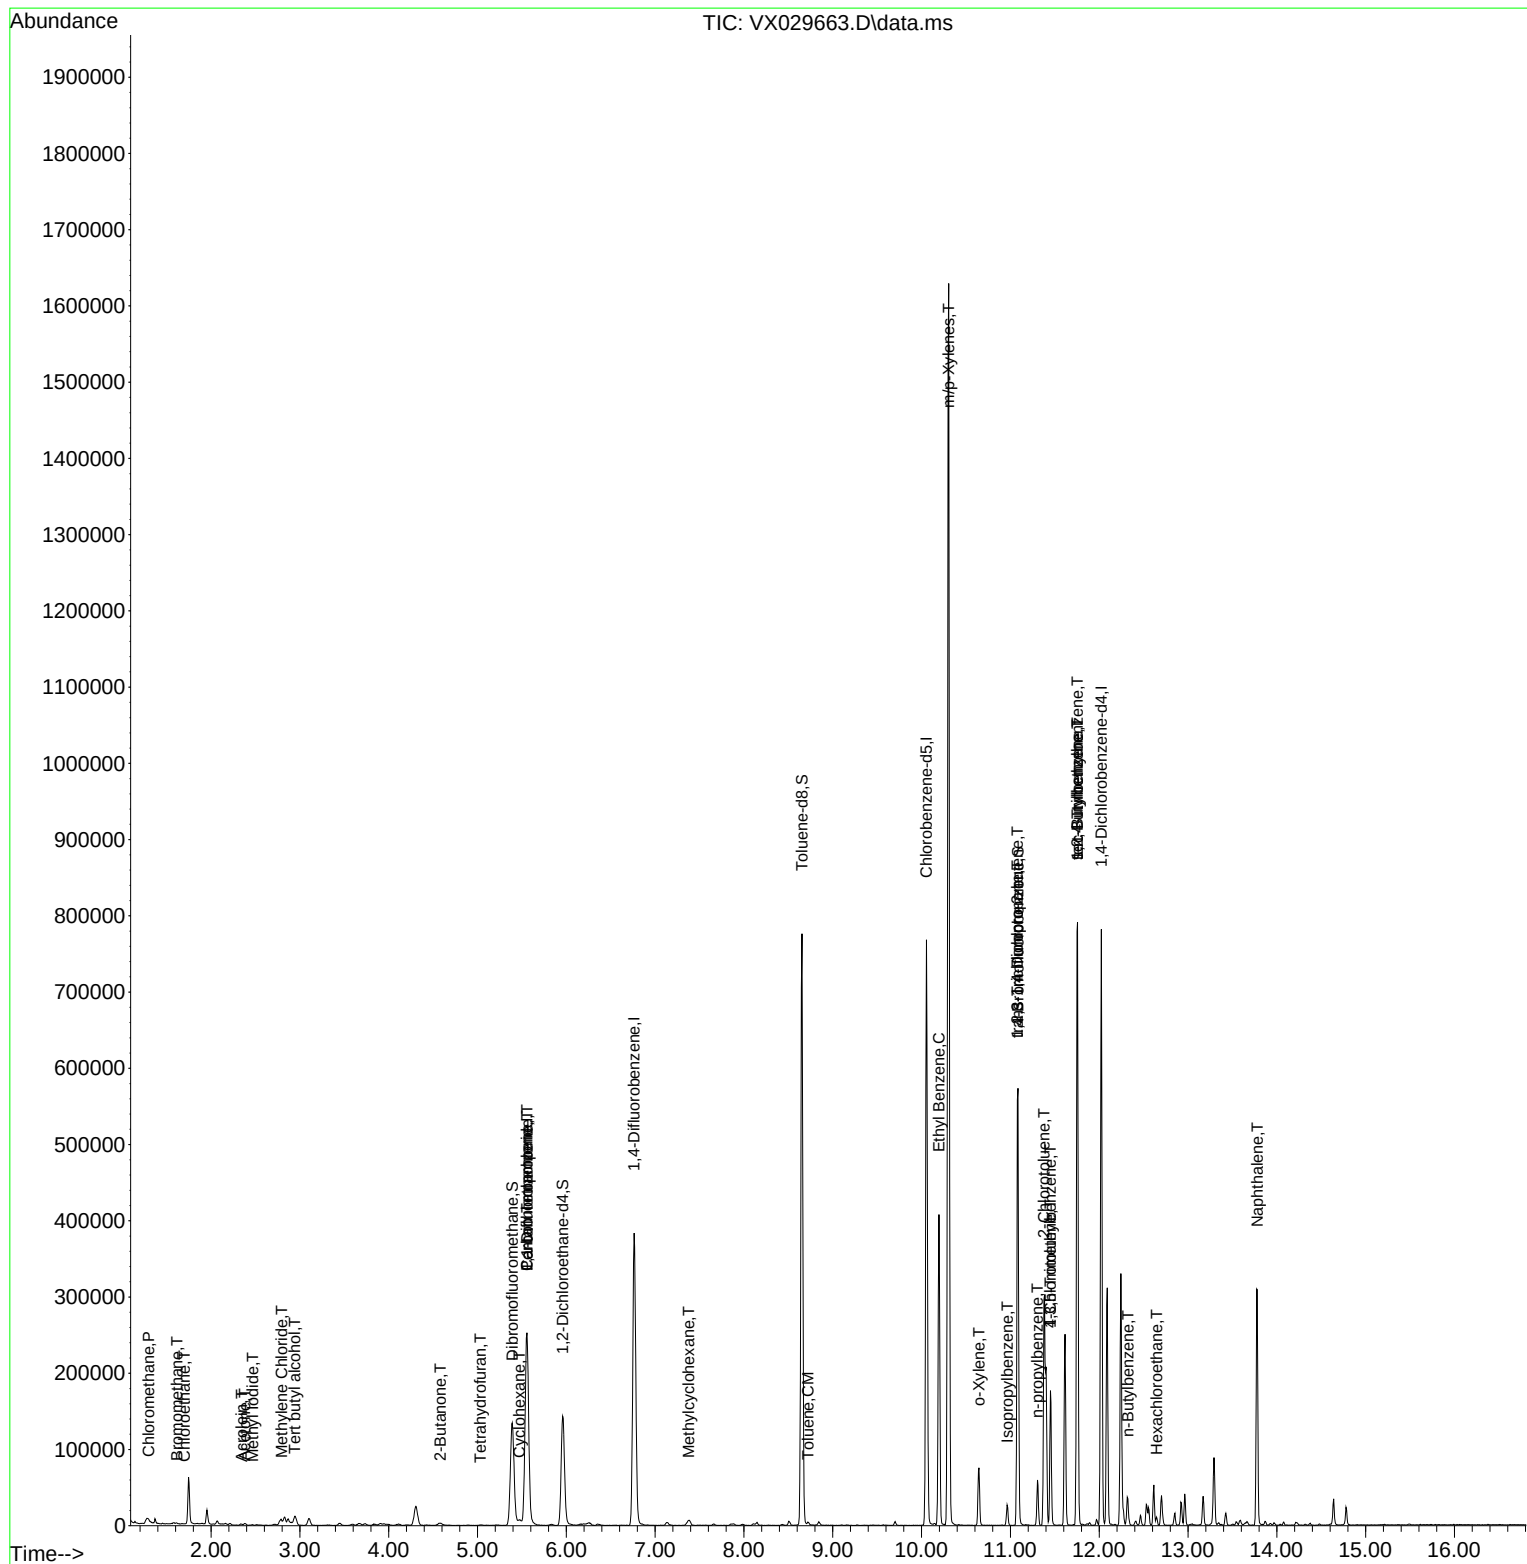


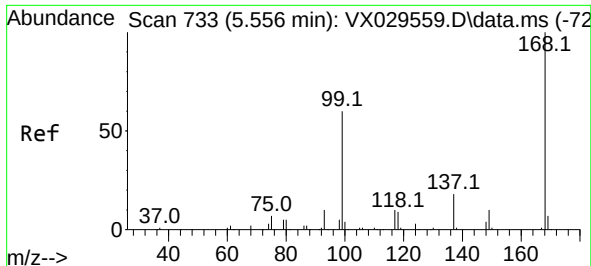

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:168 Resp: 243207
Ion Ratio Lower Upper
168 100
99 57.9 41.7 62.5

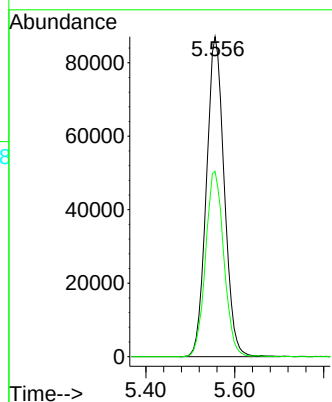

#3
Chloromethane
Concen: 0.389 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 50 Resp: 1233
Ion Ratio Lower Upper
50 100
52 31.7 26.4 39.6


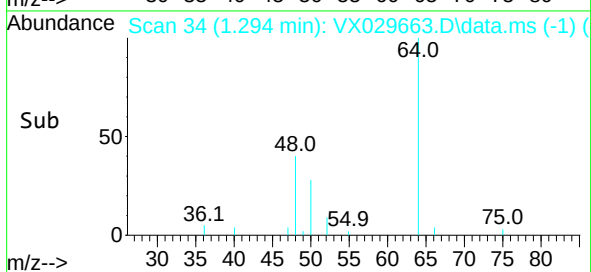
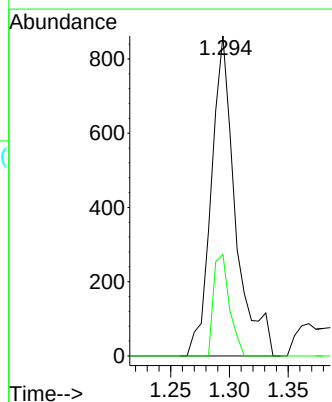
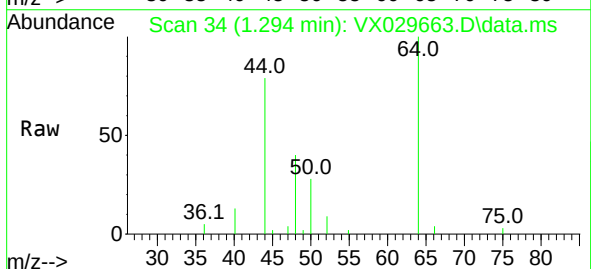


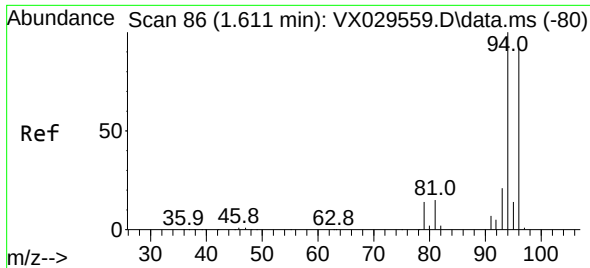

#5
Bromomethane
Concen: 0.541 ug/l
RT: 1.617 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion: 94 Resp: 806
Ion Ratio Lower Upper
94 100
96 55.5 75.3 112.9#

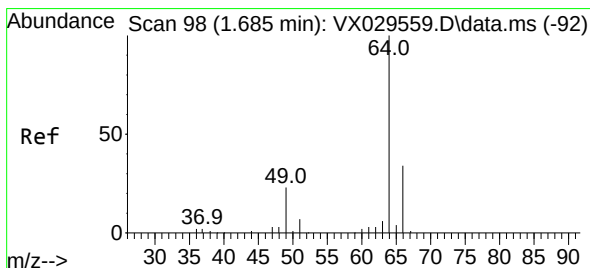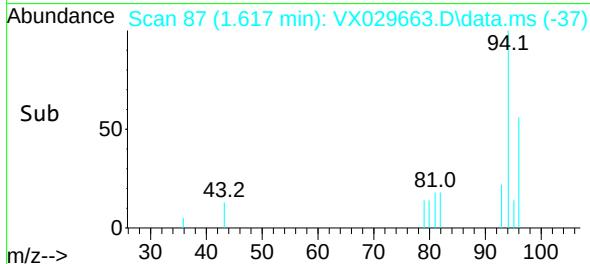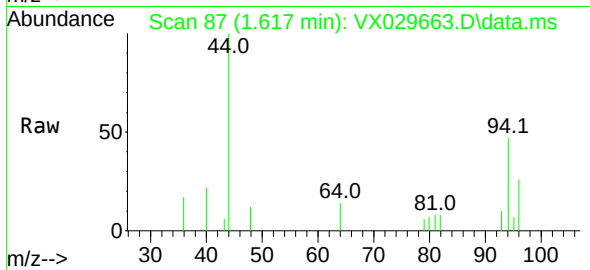

#6
Chloroethane
Concen: 1.540 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.012 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 64 Resp: 582
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#


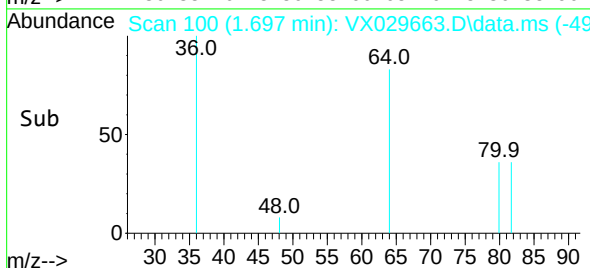

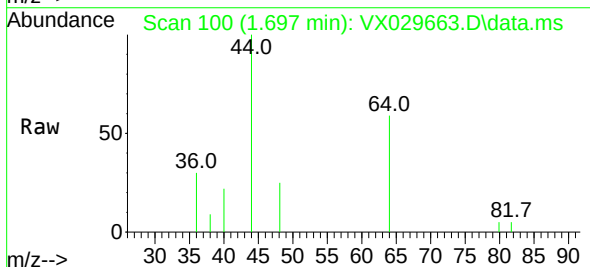


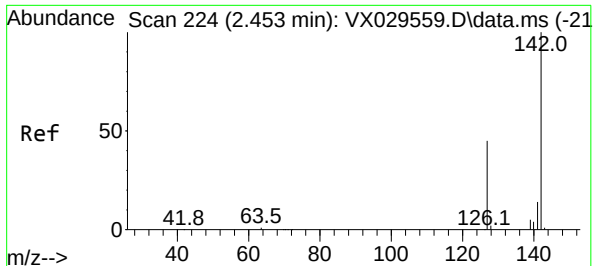

#10
Methyl Iodide
Concen: 3.343 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:142 Resp: 1007
Ion Ratio Lower Upper
142 100
127 27.5 33.9 50.9#
141 2.2 11.4 17.2#

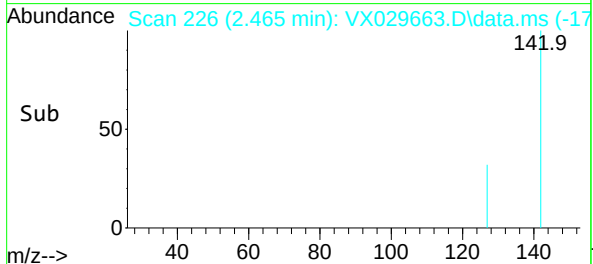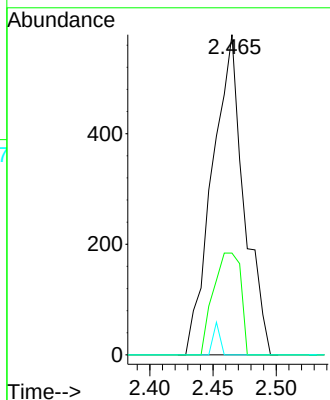

#11
Tert butyl alcohol
Concen: 0.462 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.043 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 59 Resp: 6804
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

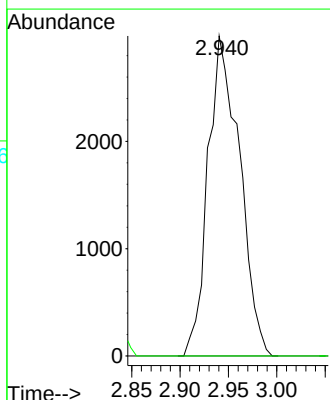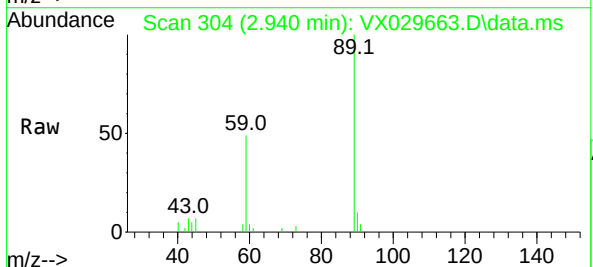

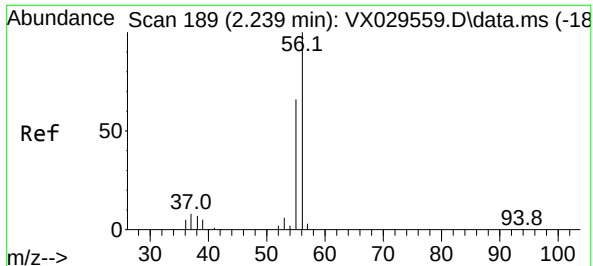

#13

Acrolein

Concen: 0.733 ug/l

RT: 2.343 min Scan# 206

Delta R.T. 0.104 min

Lab File: VX029663.D

Acq: 21 Jun 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :





MW-1RDL

Tgt Ion: 56 Resp: 130

Ion Ratio Lower Upper

56 100

55 0.0 55.0 82.6#

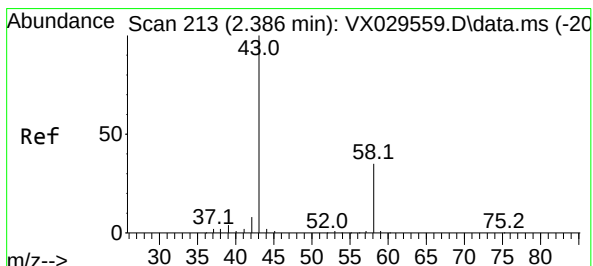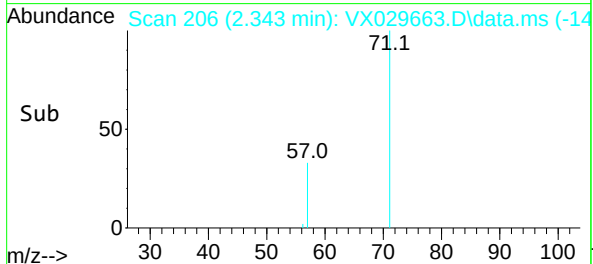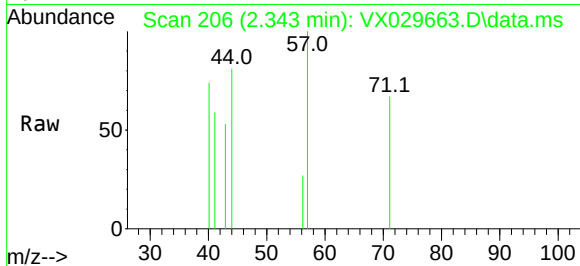

#16

Acetone

Concen: 1.965 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX029663.D




Acq: 21 Jun 2022 15:23


Tgt Ion: 43 Resp: 2522

Ion Ratio Lower Upper

43 100

58 28.2 28.8 43.2#


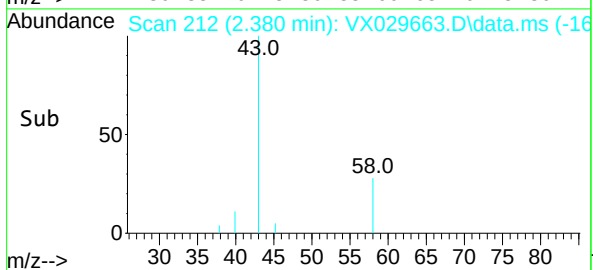

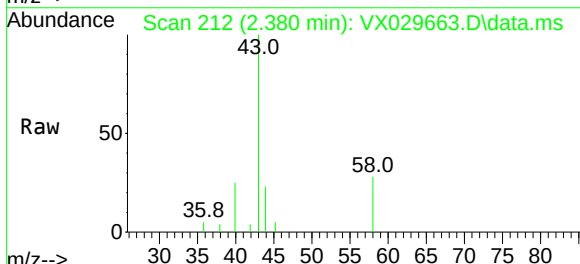


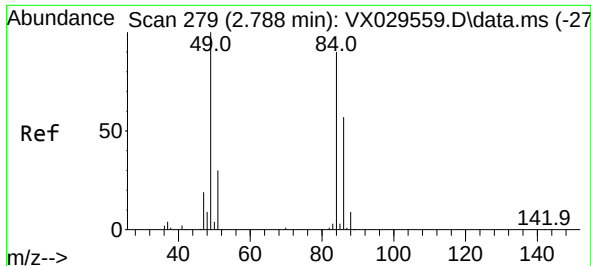

#20
Methylene Chloride
Concen: 0.453 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:	84	Resp:	1295
Ion	Ratio	Lower	Upper
84	100		
49	88.7	85.5	128.3
51	29.3	26.6	39.8
86	94.8	51.5	77.3

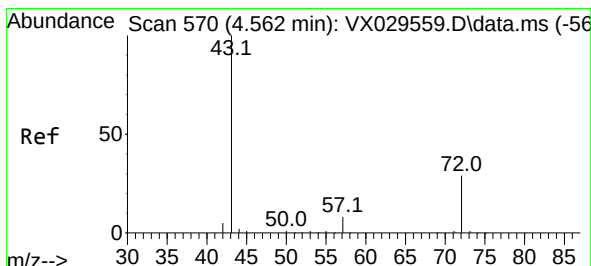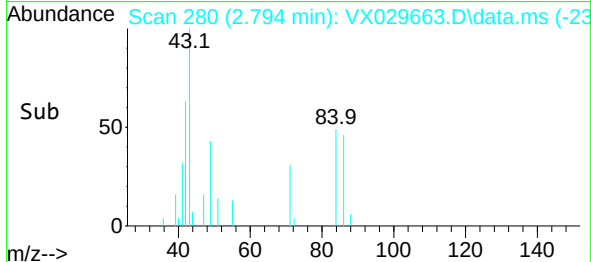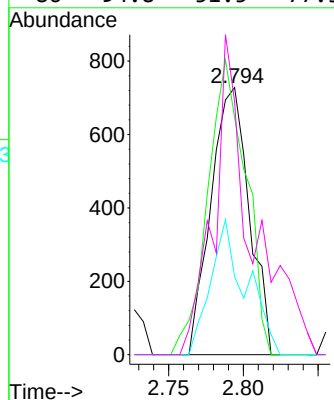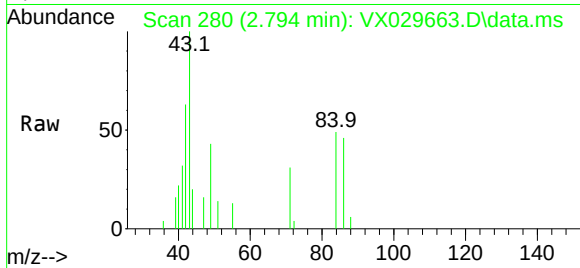

#25
2-Butanone
Concen: 0.696 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.018 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion:	43	Resp:	1411
Ion	Ratio	Lower	Upper
43	100		
72	24.9	24.4	36.6

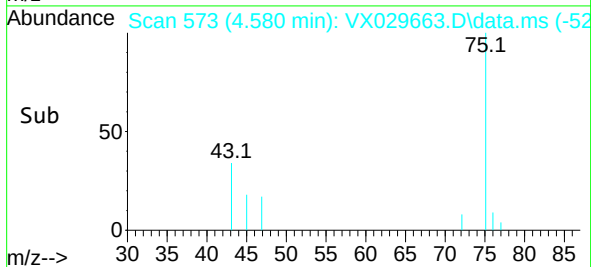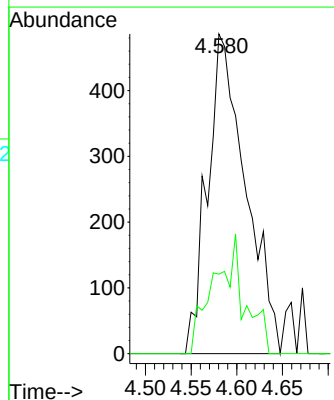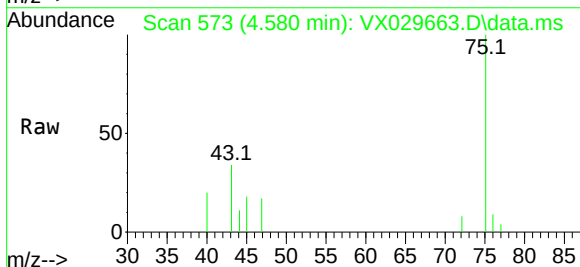

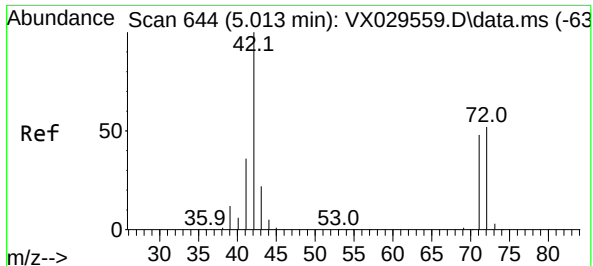

#29

Tetrahydrofuran

Concen: 0.442 ug/l

RT: 5.032 min Scan# 644

Delta R.T. 0.019 min

Lab File: VX029663.D

Acq: 21 Jun 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :

MW-1RDL





Tgt Ion: 42 Resp: 597

Ion Ratio Lower Upper

42 100

72 30.7 44.1 66.1#

71 0.0 40.5 60.7#

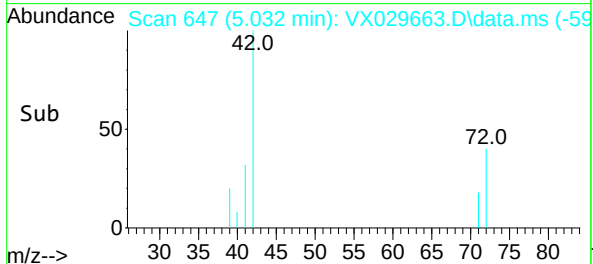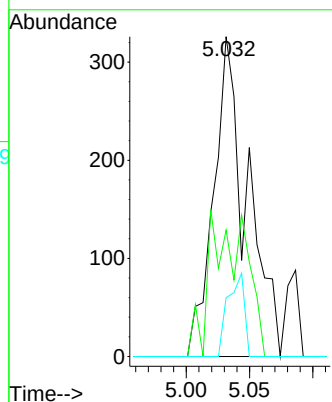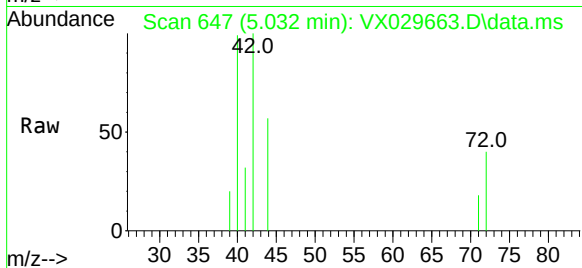

#31

Cyclohexane

Concen: 1.111 ug/l

RT: 5.470 min Scan# 719

Delta R.T. -0.007 min

Lab File: VX029663.D

Acq: 21 Jun 2022 15:23




Tgt Ion: 56 Resp: 4800


Ion Ratio Lower Upper

56 100

69 31.5 26.7 40.1

84 103.4 77.2 115.8

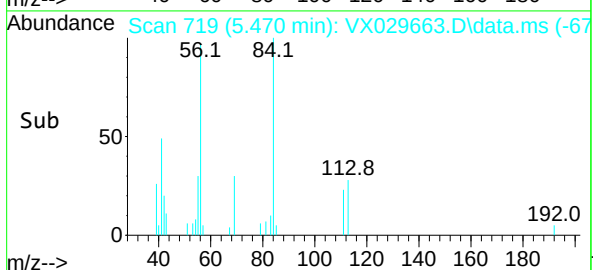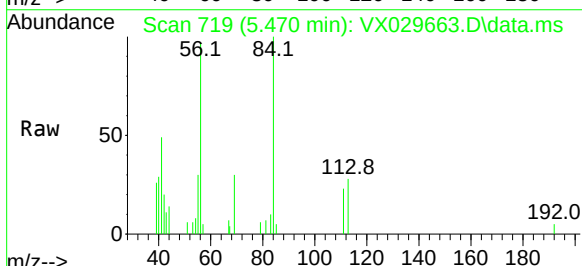

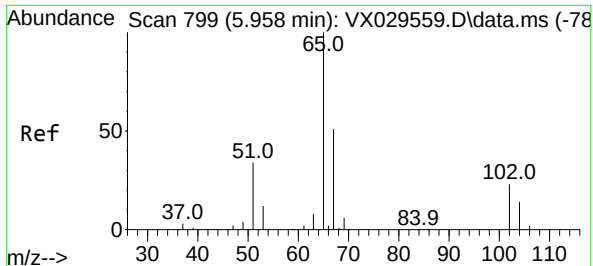

#33

1,2-Dichloroethane-d4

Concen: 43.218 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029663.D

Acq: 21 Jun 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :





MW-1RDL

Tgt Ion: 65 Resp: 139136

Ion Ratio Lower Upper

65 100

67 53.1 0.0 107.4

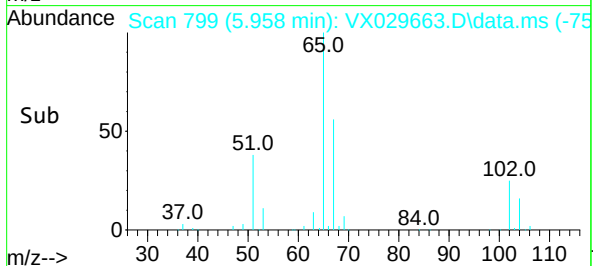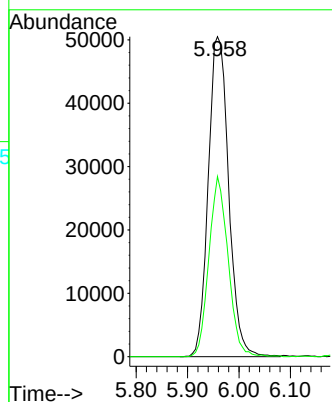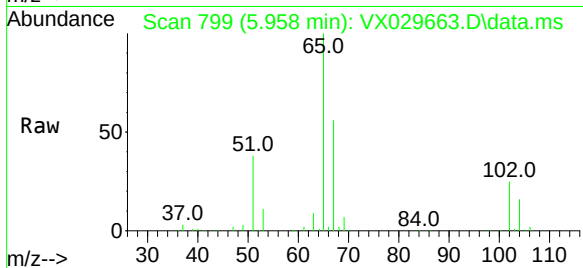

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX029663.D

Acq: 21 Jun 2022 15:23




Tgt Ion: 114 Resp: 411619


Ion Ratio Lower Upper

114 100

63 19.4 0.0 36.8

88 15.7 0.0 32.4


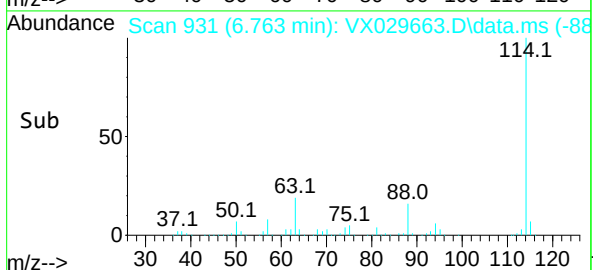

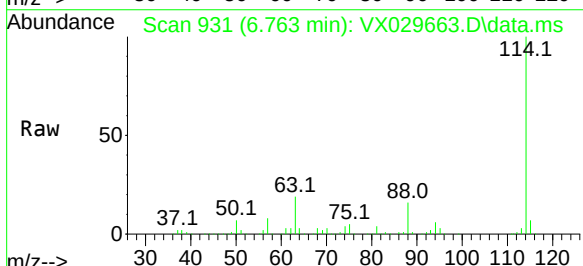


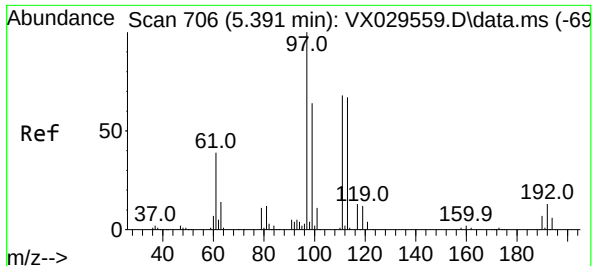

#35
Dibromofluoromethane
Concen: 45.587 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:113 Resp: 122285
Ion Ratio Lower Upper
113 100
111 102.7 82.8 124.2
192 18.5 16.9 25.3

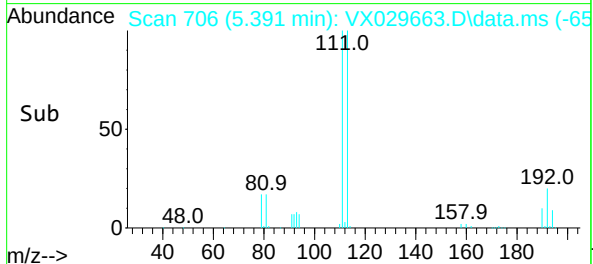

#36
1,1-Dichloropropene
Concen: 4.988 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 75 Resp: 18109
Ion Ratio Lower Upper
75 100
110 8.9 18.3 54.8#
77 0.0 24.8 37.2#



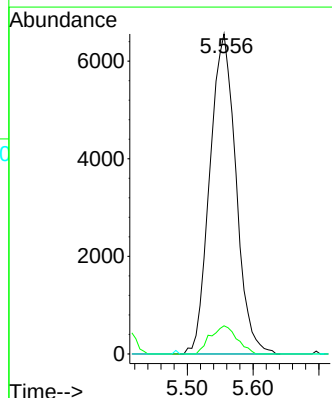
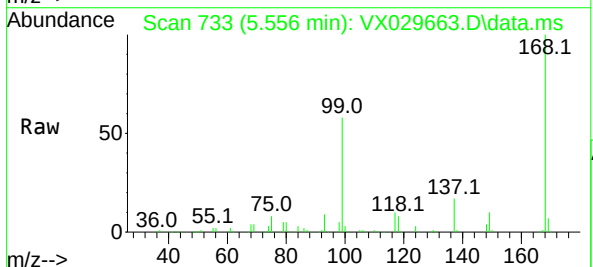


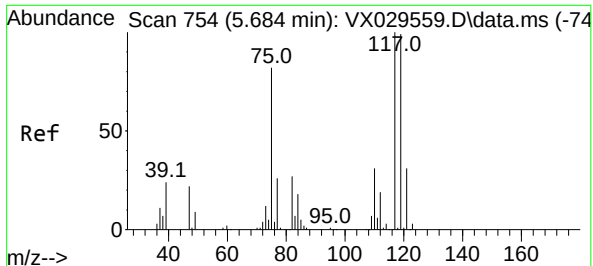

#38
Carbon Tetrachloride
Concen: 6.963 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:117 Resp: 24859
Ion Ratio Lower Upper
117 100
119 3.9 77.3 115.9#
121 0.0 24.2 36.2#

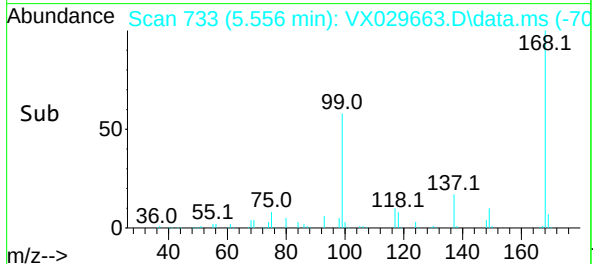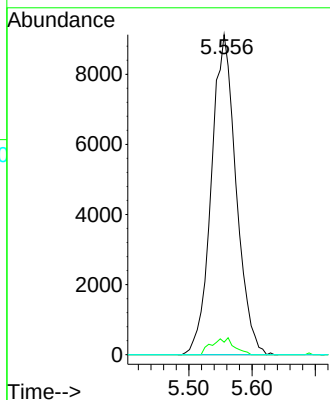

#39
Methylcyclohexane
Concen: 0.743 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 83 Resp: 3364
Ion Ratio Lower Upper
83 100
55 71.3 54.6 81.8
98 45.8 37.4 56.2


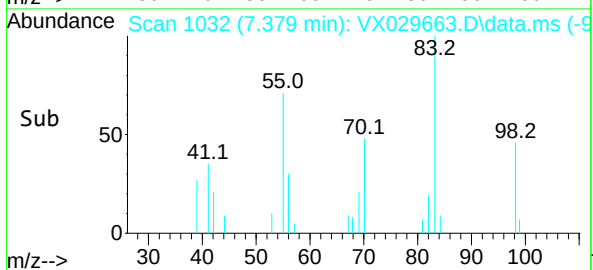
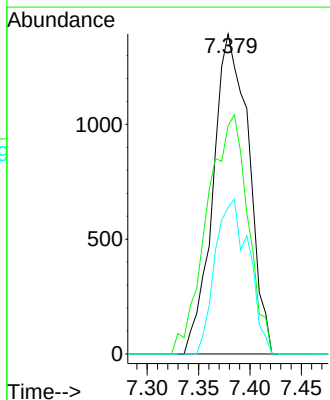
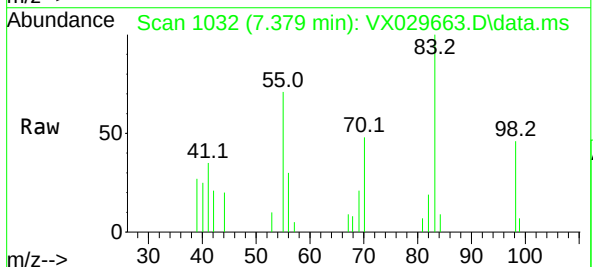


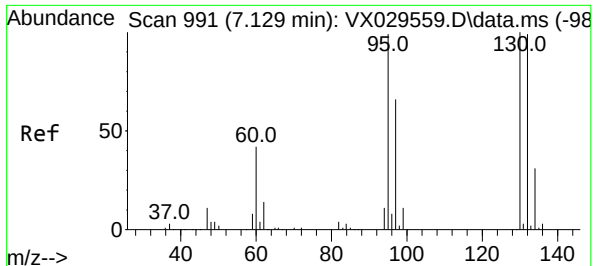

#44
 Trichloroethene
 Concen: Below Cal
 RT: 7.135 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX029663.D
 Acq: 21 Jun 2022 15:23




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1RDL


Tgt Ion:130 Resp: 1941
 Ion Ratio Lower Upper
 130 100
 95 96.8 0.0 188.8

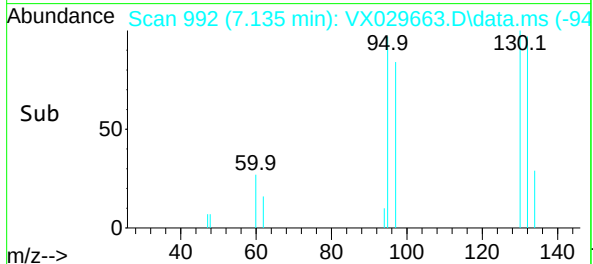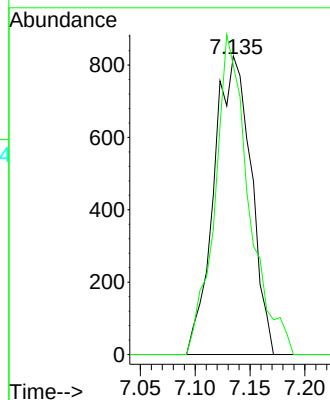

#50
 Toluene-d8
 Concen: 47.602 ug/l
 RT: 8.653 min Scan# 1241
 Delta R.T. -0.000 min
 Lab File: VX029663.D
 Acq: 21 Jun 2022 15:23

Tgt Ion: 98 Resp: 466478
 Ion Ratio Lower Upper
 98 100
 100 66.8 52.6 78.8


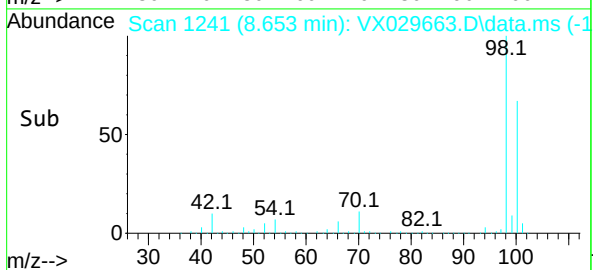
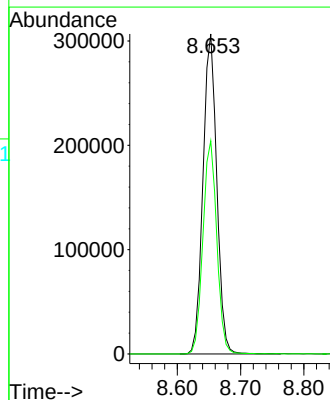
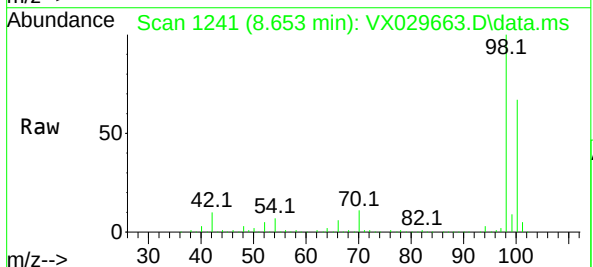


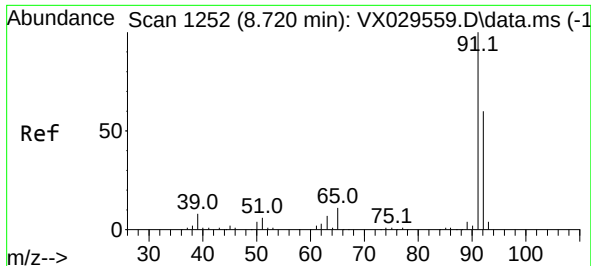

#52
Toluene
Concen: 0.236 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion: 92 Resp: 1628
Ion Ratio Lower Upper
92 100
91 149.7 137.5 206.3



#62
4-Bromofluorobenzene
Concen: 45.739 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 95 Resp: 169029
Ion Ratio Lower Upper
95 100
174 73.4 0.0 163.0
176 71.0 0.0 155.0



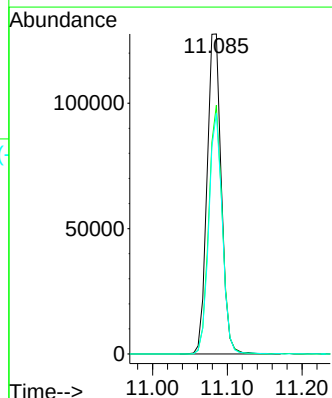
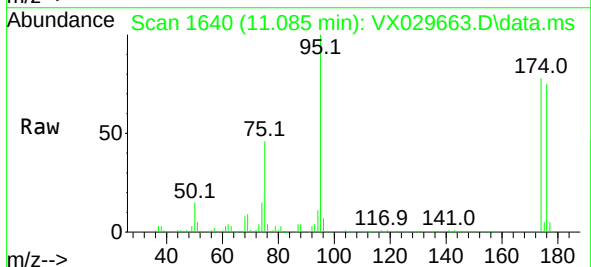


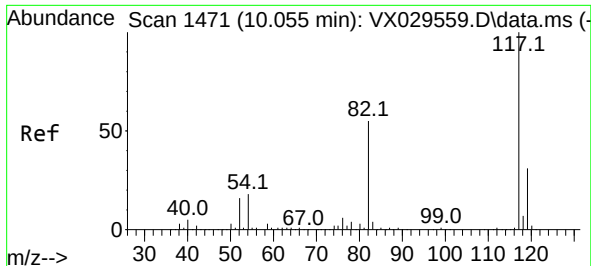

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:117 Resp: 359485
Ion Ratio Lower Upper
117 100
82 54.8 41.8 62.8
119 30.9 24.8 37.2

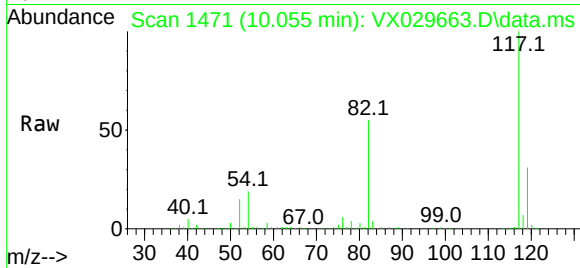

#67
Ethyl Benzene
Concen: 18.677 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 91 Resp: 237000
Ion Ratio Lower Upper
91 100
106 31.7 24.6 36.8



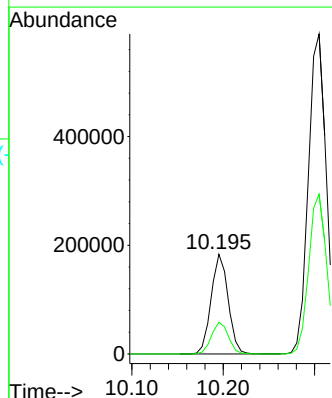
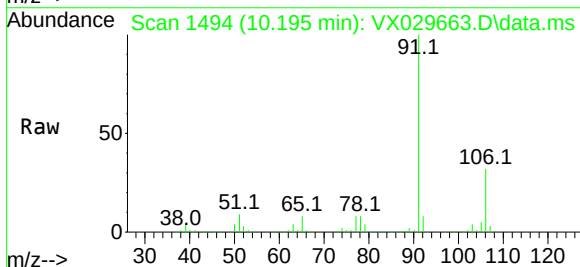


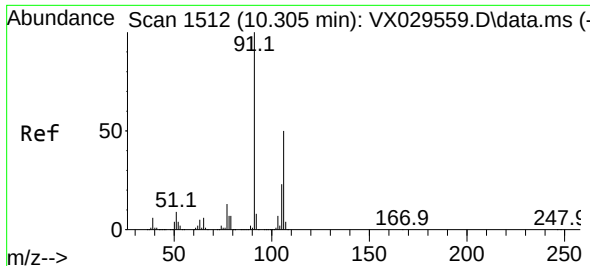

#68
m/p-Xylenes
Concen: 81.144 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:106 Resp: 401536
Ion Ratio Lower Upper
106 100
91 200.4 160.4 240.6

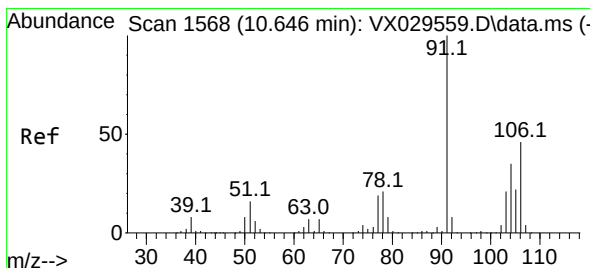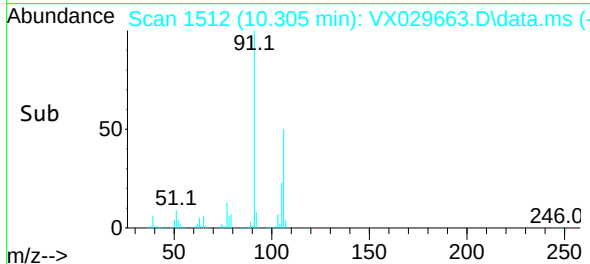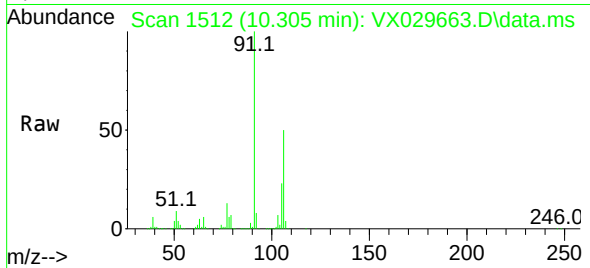

#69
o-Xylene
Concen: 3.457 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion:106 Resp: 16899
Ion Ratio Lower Upper
106 100
91 224.0 106.1 318.1


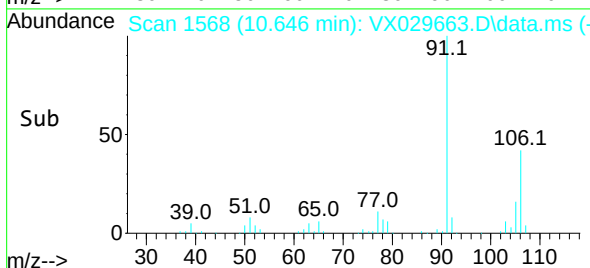

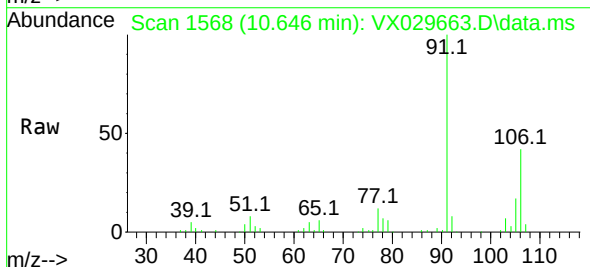




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:152 Resp: 162294
Ion Ratio Lower Upper
152 100
115 62.1 37.5 112.7
150 156.1 0.0 338.2

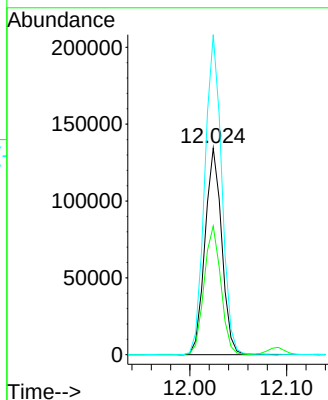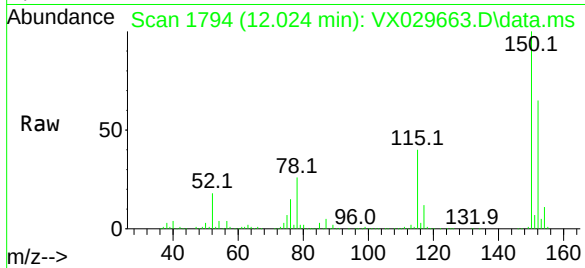

#73
Isopropylbenzene
Concen: 1.182 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion:105 Resp: 14381
Ion Ratio Lower Upper
105 100
120 27.8 13.5 40.5

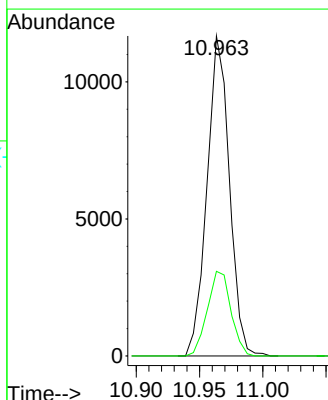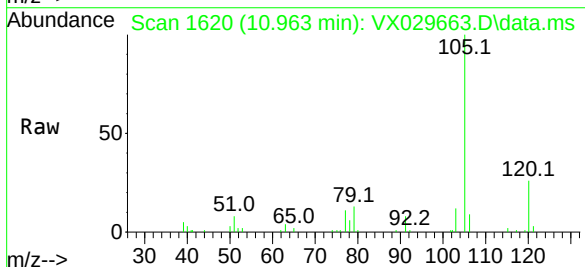



#76

1,2,3-Trichloropropane

Concen: 22.648 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.165 min

Lab File: VX029663.D

Acq: 21 Jun 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :





MW-1RDL

Tgt Ion: 75 Resp: 80072

Ion Ratio Lower Upper

75 100

77 0.0 19.4 58.2#

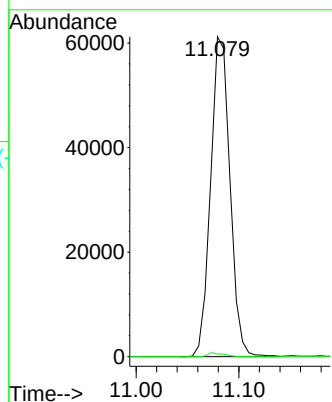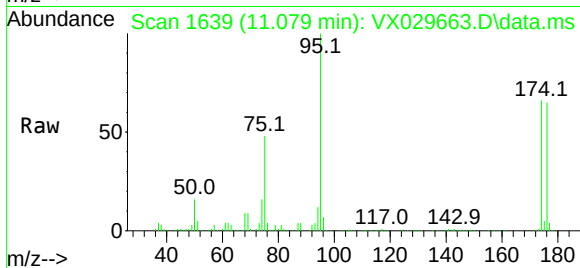

#78

n-propylbenzene

Concen: 2.696 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX029663.D




Acq: 21 Jun 2022 15:23


Tgt Ion: 91 Resp: 36945

Ion Ratio Lower Upper

91 100

120 22.0 11.6 34.8




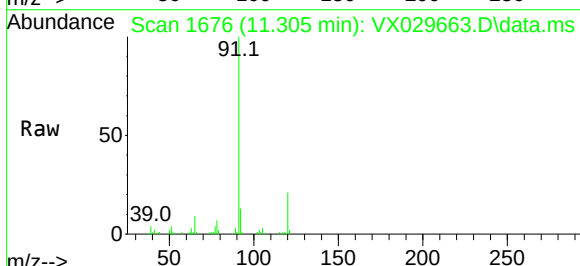




#79
2-Chlorotoluene
Concen: 3.617 ug/l
RT: 11.378 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion: 91 Resp: 30696
Ion Ratio Lower Upper
91 100
126 0.1 17.3 51.9#

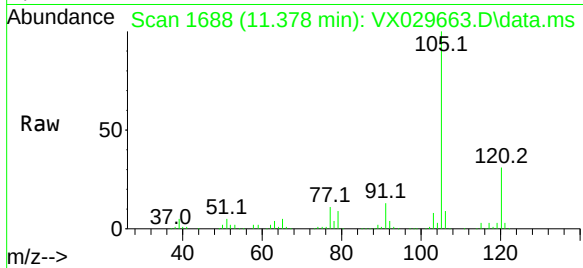

#80
1,3,5-Trimethylbenzene
Concen: 7.836 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 105 Resp: 80303
Ion Ratio Lower Upper
105 100
120 47.3 24.3 72.9




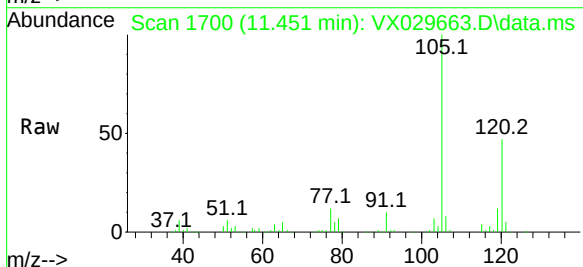




#81
trans-1,4-Dichloro-2-butene
Concen: 75.343 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion: 75 Resp: 80072
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

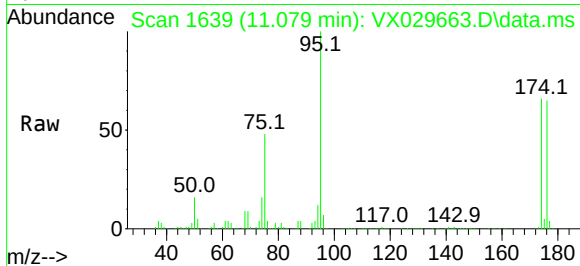

#82
4-Chlorotoluene
Concen: 0.905 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion: 91 Resp: 8755
Ion Ratio Lower Upper
91 100
126 1.8 14.9 44.5#




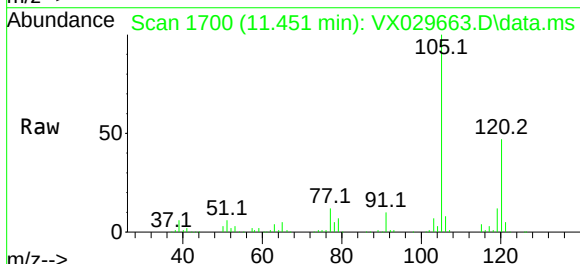


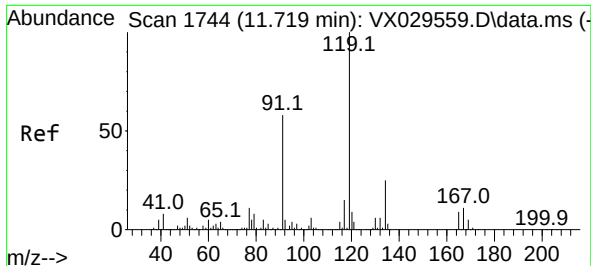

#83
tert-Butylbenzene
Concen: 4.483 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL


Tgt Ion:119 Resp: 44796
Ion Ratio Lower Upper
119 100
91 85.0 26.9 80.6#
134 0.0 11.4 34.2#

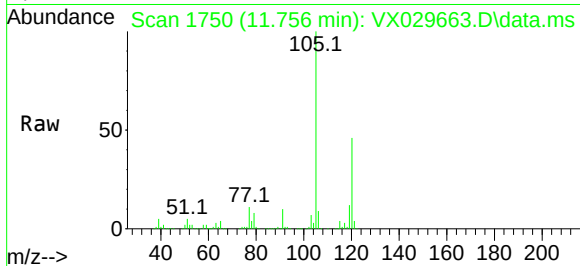

#84
1,2,4-Trimethylbenzene
Concen: 35.790 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion:105 Resp: 365805
Ion Ratio Lower Upper
105 100
120 45.1 22.6 67.8


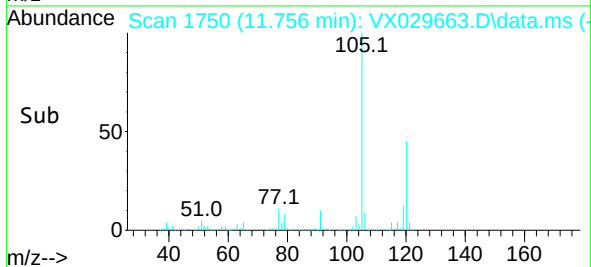

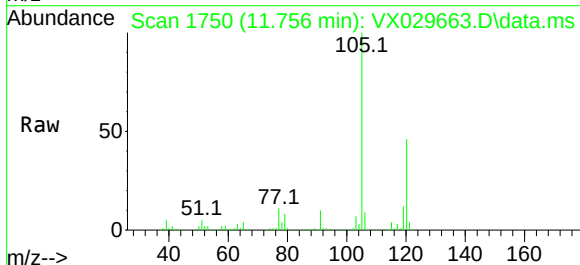




#85
 sec-Butylbenzene
 Concen: 29.540 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. -0.134 min
 Lab File: VX029663.D
 Acq: 21 Jun 2022 15:23




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1RDL


Tgt Ion:105 Resp: 365805
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4#

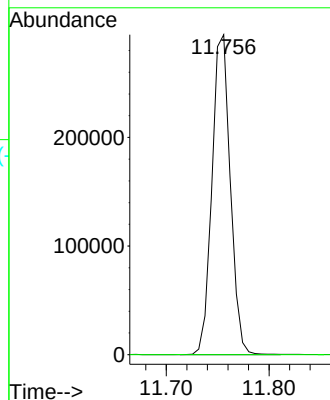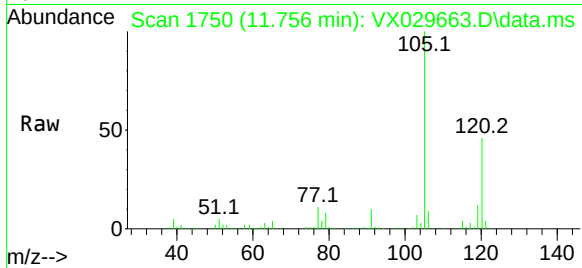

#89
 n-Butylbenzene
 Concen: 0.566 ug/l
 RT: 12.323 min Scan# 1843
 Delta R.T. -0.012 min
 Lab File: VX029663.D
 Acq: 21 Jun 2022 15:23

Tgt Ion: 91 Resp: 4950
 Ion Ratio Lower Upper
 91 100
 92 25.3 27.8 83.3#
 134 118.8 13.3 39.8#



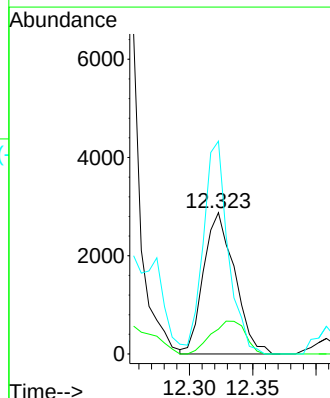
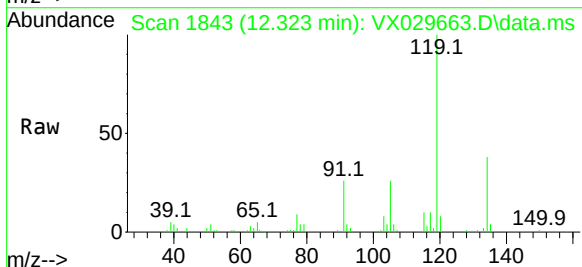


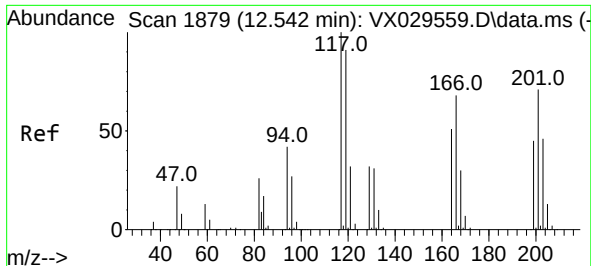

#90
Hexachloroethane
Concen: 2.421 ug/l
RT: 12.646 min Scan# 1879
Delta R.T. 0.104 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Instrument :
MSVOA_X
ClientSampleId :
MW-1RDL

Tgt Ion:117 Resp: 3594
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

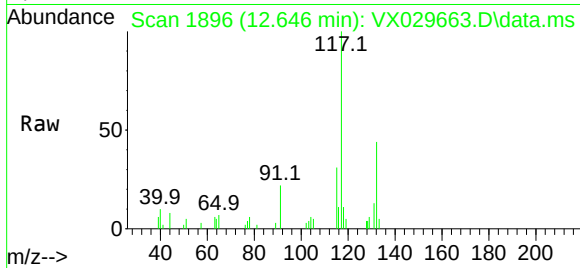

#95
Naphthalene
Concen: 17.897 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX029663.D
Acq: 21 Jun 2022 15:23

Tgt Ion:128 Resp: 203742
Ion Ratio Lower Upper
128 100
127 12.6 10.2 15.4
129 10.8 8.7 13.1

