

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
 Data File : VX029664.D
 Acq On : 21 Jun 2022 15:46
 Operator : JC/MD
 Sample : N3286-08 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-101RDL

Quant Time: Jun 22 01:11:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	249497	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	421645	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	368965	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	169172	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	139850	42.345	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	84.680%
35) Dibromofluoromethane	5.391	113	124616	45.351	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.700%
50) Toluene-d8	8.653	98	476071	47.426	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.860%
62) 4-Bromofluorobenzene	11.079	95	176293	46.570	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.140%

Target Compounds						Qvalue
3) Chloromethane	1.294	50	1111	0.341	ug/l #	79
5) Bromomethane	1.617	94	702	0.459	ug/l	92
6) Chloroethane	1.691	64	192	1.372	ug/l #	43
10) Methyl Iodide	2.459	142	717	3.243	ug/l #	91
11) Tert butyl alcohol	2.946	59	5965	Below Cal	#	72
13) Acrolein	2.215	56	1155	6.349	ug/l #	1
16) Acetone	2.380	43	2072	1.574	ug/l	98
20) Methylene Chloride	2.788	84	1973	0.673	ug/l	92
25) 2-Butanone	4.593	43	1123	0.540	ug/l	90
31) Cyclohexane	5.477	56	3606	0.813	ug/l	91
36) 1,1-Dichloropropene	5.556	75	18951	5.096	ug/l #	49
38) Carbon Tetrachloride	5.556	117	25505	6.974	ug/l #	15
39) Methylcyclohexane	7.385	83	2360	0.509	ug/l #	86
44) Trichloroethene	7.135	130	1753	Below Cal		98
51) 4-Methyl-2-Pentanone	8.586	43	1207	0.316	ug/l	91
52) Toluene	8.720	92	132812	18.814	ug/l	98
53) t-1,3-Dichloropropene	8.720	75	1430	0.378	ug/l #	1
59) 2-Hexanone	9.439	43	1937	0.669	ug/l	81
67) Ethyl Benzene	10.195	91	525995	40.387	ug/l	98
68) m/p-Xylenes	10.305	106	653975	128.762	ug/l	100
69) o-Xylene	10.646	106	254394	50.697	ug/l	99
70) Styrene	10.646	104	12832	1.562	ug/l #	1
73) Isopropylbenzene	10.963	105	17076	1.346	ug/l	99
76) 1,2,3-Trichloropropane	11.384	75	2665	0.723	ug/l #	1
78) n-propylbenzene	11.305	91	58507	4.095	ug/l	99
79) 2-Chlorotoluene	11.378	91	36514	4.128	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	114089	10.680	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	83928	75.760	ug/l #	15
82) 4-Chlorotoluene	11.451	91	12270	1.216	ug/l #	45
83) tert-Butylbenzene	11.756	119	51489	4.943	ug/l #	55
84) 1,2,4-Trimethylbenzene	11.756	105	421783	39.589	ug/l	100
85) sec-Butylbenzene	11.756	105	421783	32.675	ug/l #	56
89) n-Butylbenzene	12.323	91	10149	1.113	ug/l #	17
90) Hexachloroethane	12.530	117	3273	2.115	ug/l #	10
95) Naphthalene	13.780	128	155154	13.075	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029664.D
Acq On : 21 Jun 2022 15:46
Operator : JC/MD
Sample : N3286-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL

Quant Time: Jun 22 01:11:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029664.D
Acq On : 21 Jun 2022 15:46
Operator : JC/MD
Sample : N3286-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL

Quant Time: Jun 22 01:11:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




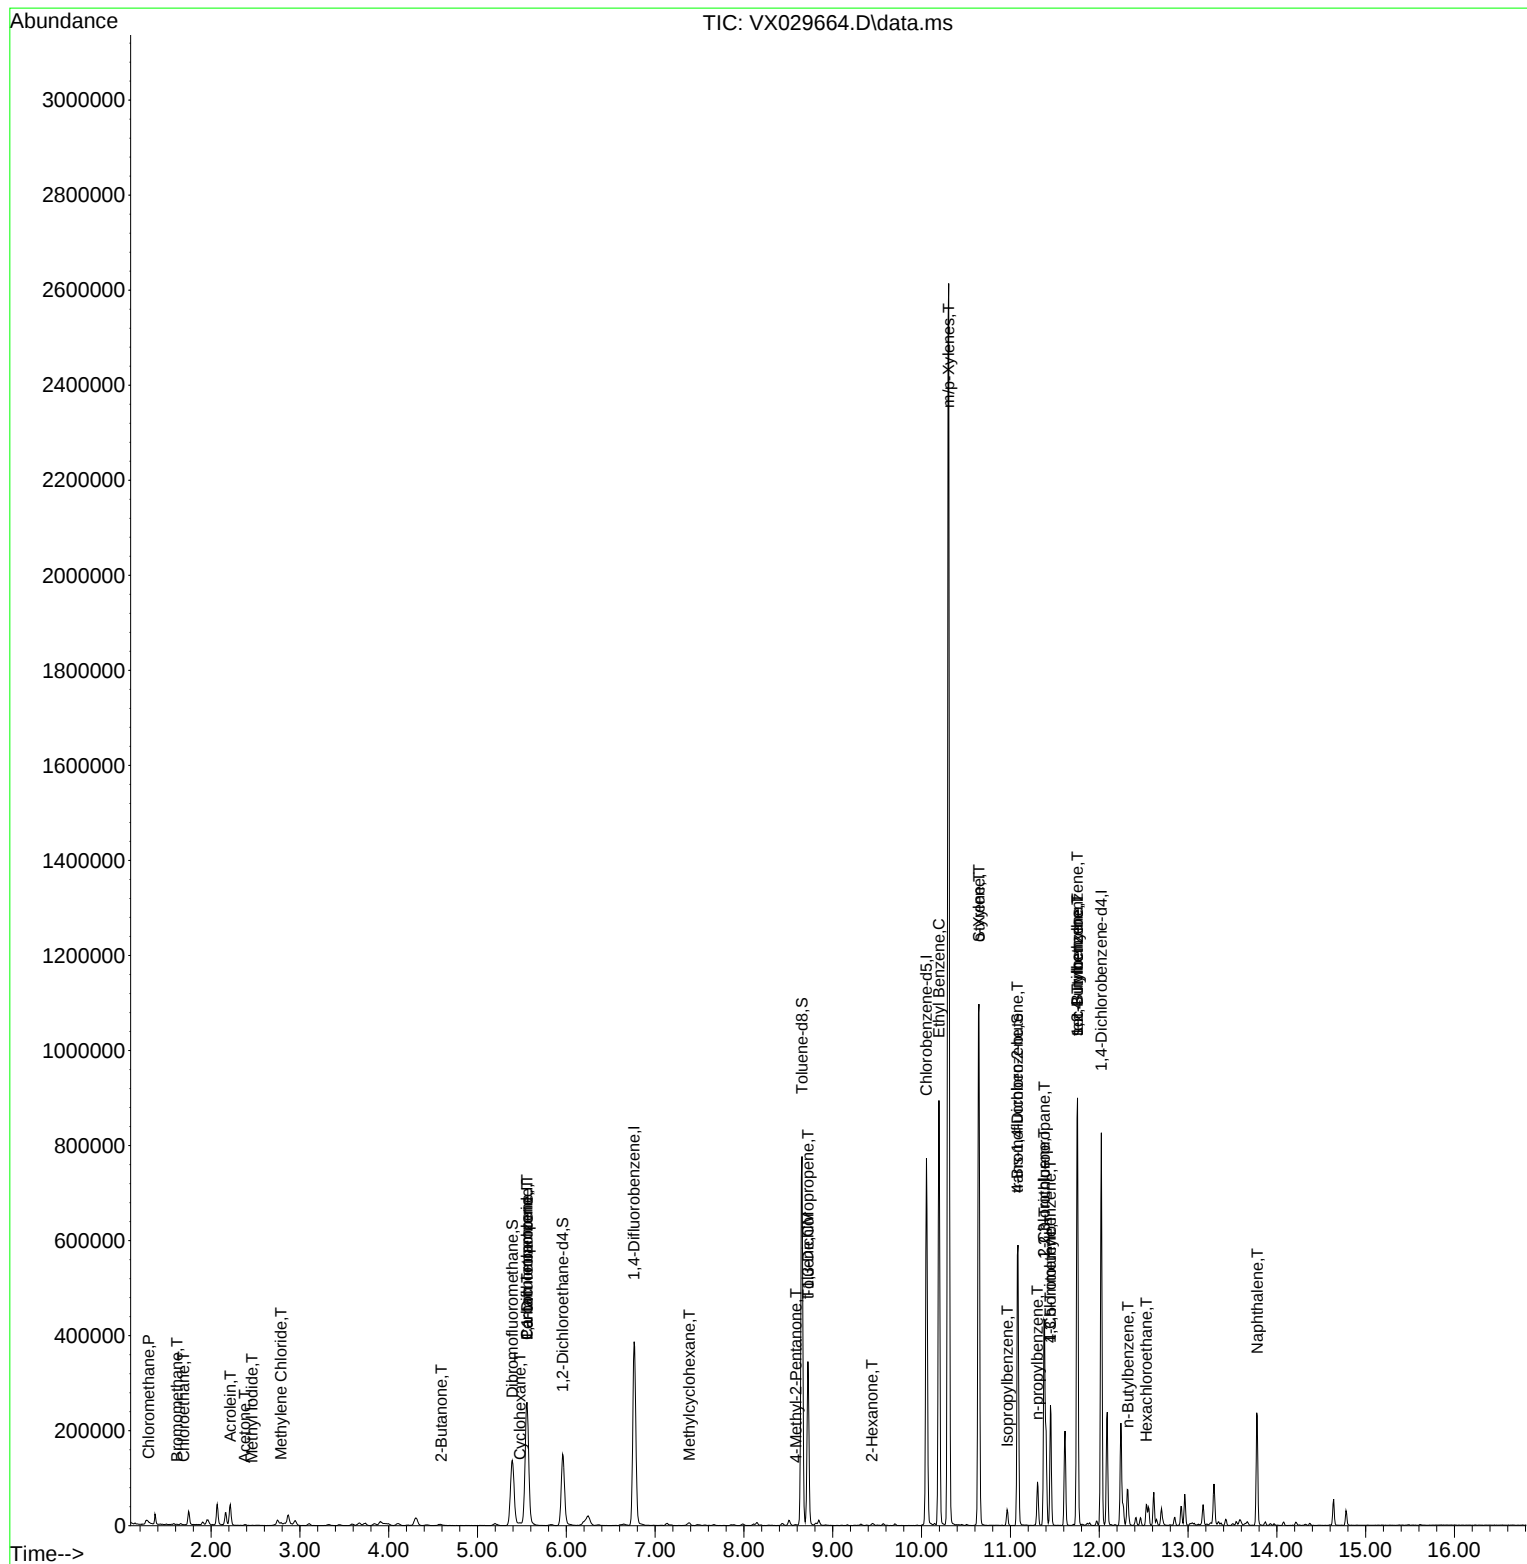




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:168 Resp: 249497
Ion Ratio Lower Upper
168 100
99 60.4 41.7 62.5



#3
Chloromethane
Concen: 0.341 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 50 Resp: 1111
Ion Ratio Lower Upper
50 100
52 21.4 26.4 39.6#







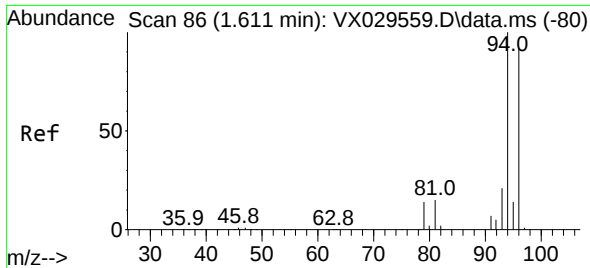

#5
Bromomethane
Concen: 0.459 ug/l
RT: 1.617 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion: 94 Resp: 702
Ion Ratio Lower Upper
94 100
96 85.9 75.3 112.9

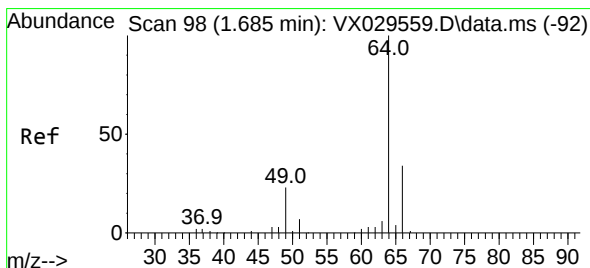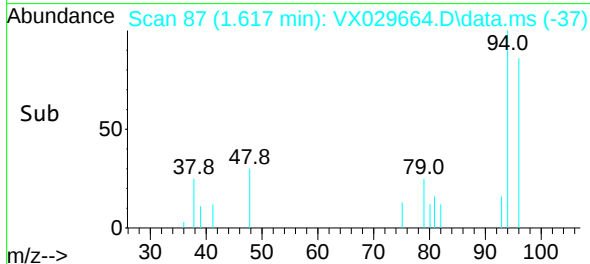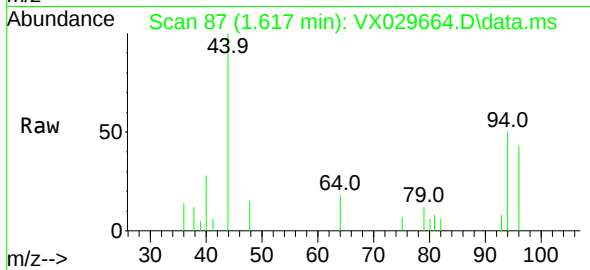

#6
Chloroethane
Concen: 1.372 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 64 Resp: 192
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9


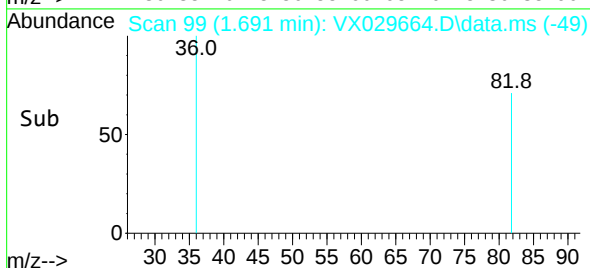

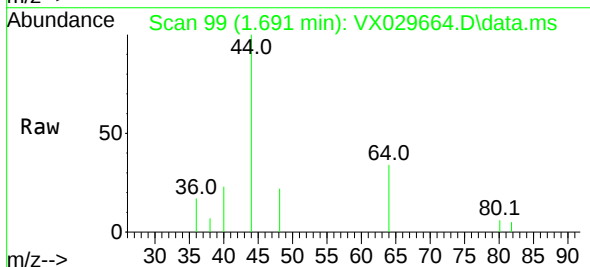


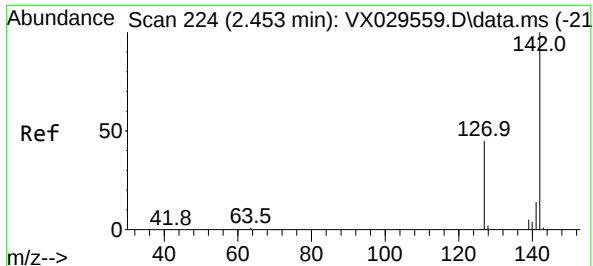

#10
Methyl Iodide
Concen: 3.243 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:142 Resp: 717
Ion Ratio Lower Upper
142 100
127 42.7 33.9 50.9
141 0.0 11.4 17.2#

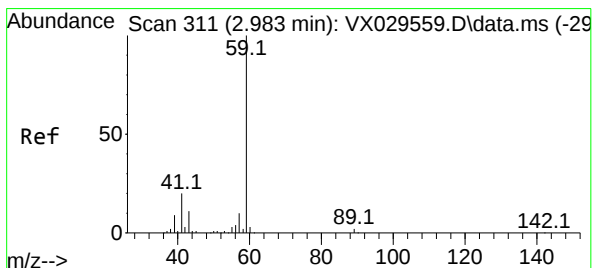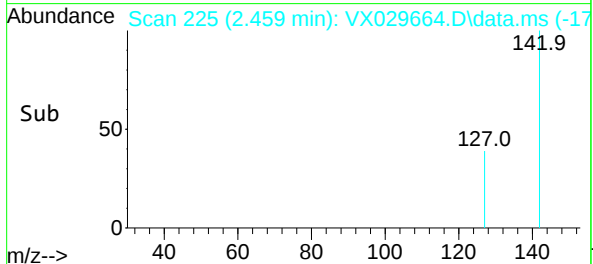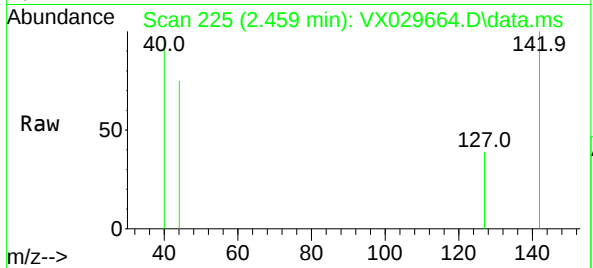

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.946 min Scan# 305
Delta R.T. -0.037 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 59 Resp: 5965
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


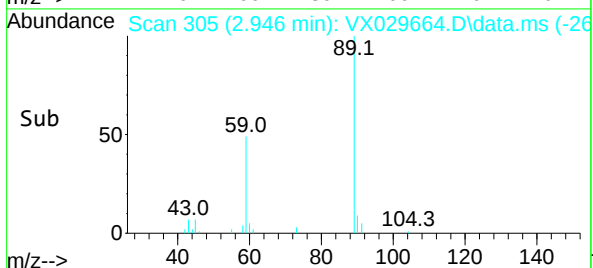

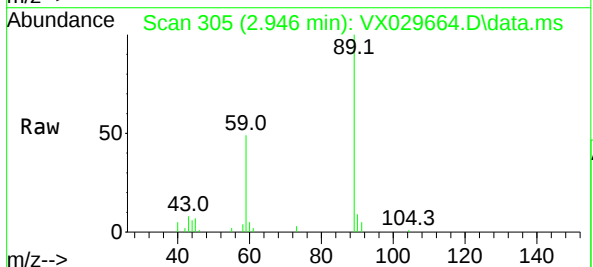




#13
Acrolein
Concen: 6.349 ug/l
RT: 2.215 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion: 56 Resp: 1155
Ion Ratio Lower Upper
56 100
55 2027.0 55.0 82.6#

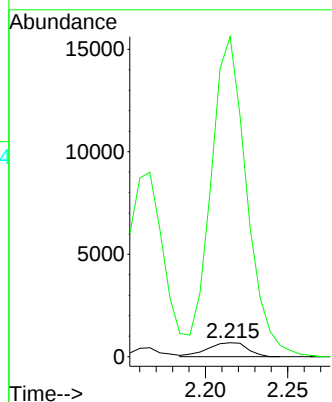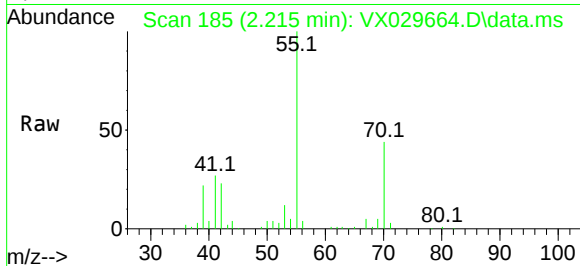

#16
Acetone
Concen: 1.574 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 43 Resp: 2072
Ion Ratio Lower Upper
43 100
58 37.0 28.8 43.2


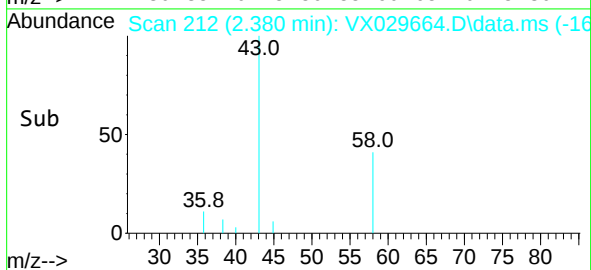

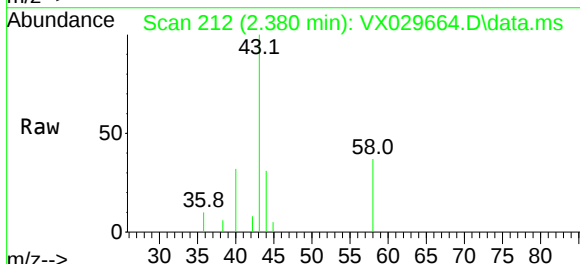




#20
Methylene Chloride
Concen: 0.673 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:	84	Resp:	1973
Ion	Ratio	Lower	Upper
84	100		
49	115.5	85.5	128.3
51	35.4	26.6	39.8
86	72.6	51.5	77.3

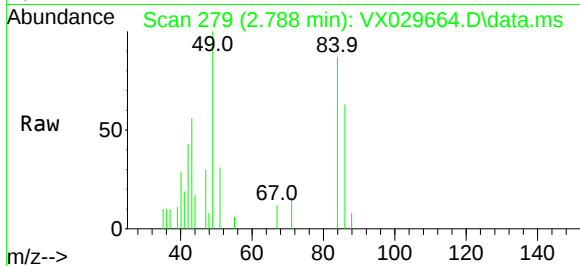

#25
2-Butanone
Concen: 0.540 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.031 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion:	43	Resp:	1123
Ion	Ratio	Lower	Upper
43	100		
72	25.2	24.4	36.6


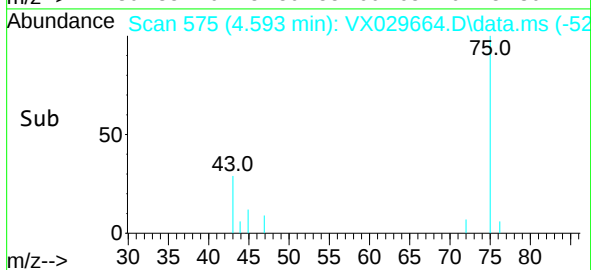
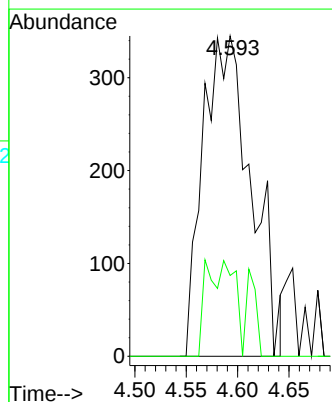
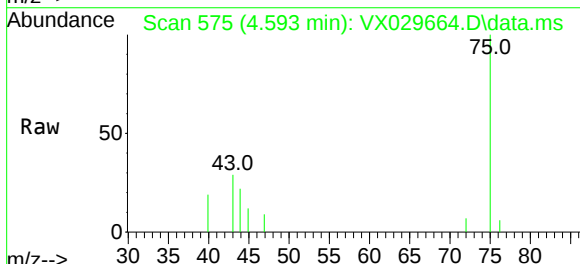




#31
Cyclohexane
Concen: 0.813 ug/l
RT: 5.477 min Scan# 720
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion: 56 Resp: 3606
Ion Ratio Lower Upper
56 100
69 27.6 26.7 40.1
84 88.2 77.2 115.8



#33
1,2-Dichloroethane-d4
Concen: 42.345 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 65 Resp: 139850
Ion Ratio Lower Upper
65 100
67 54.0 0.0 107.4



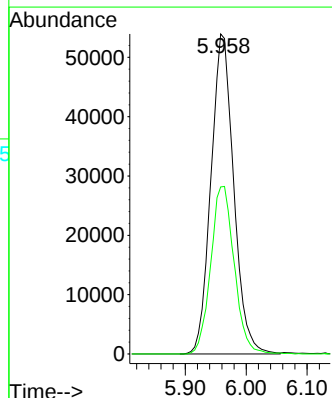





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:114 Resp: 421645
Ion Ratio Lower Upper
114 100
63 19.0 0.0 36.8
88 16.5 0.0 32.4



#35
Dibromofluoromethane
Concen: 45.351 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion:113 Resp: 124616
Ion Ratio Lower Upper
113 100
111 102.6 82.8 124.2
192 18.4 16.9 25.3


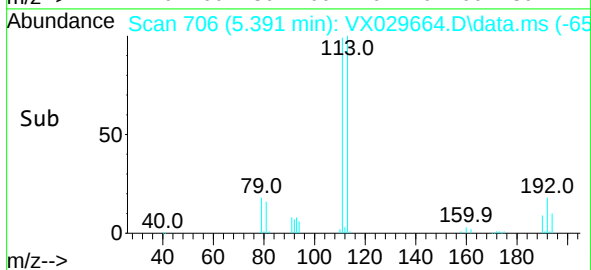

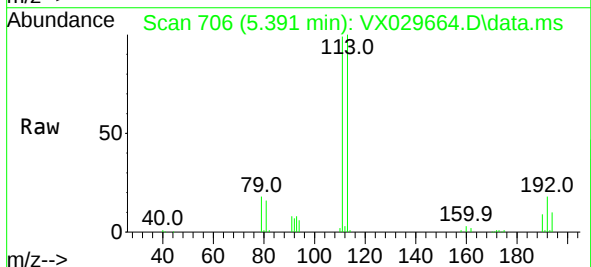




#36
1,1-Dichloropropene
Concen: 5.096 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion: 75 Resp: 18951
Ion Ratio Lower Upper
75 100
110 9.0 18.3 54.8#
77 0.0 24.8 37.2#

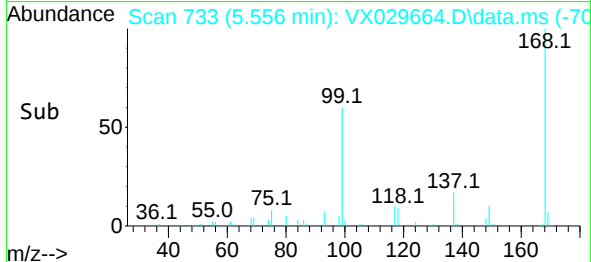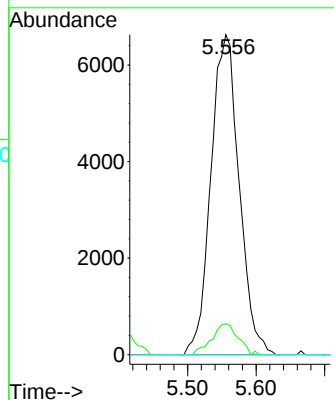

#38
Carbon Tetrachloride
Concen: 6.974 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 117 Resp: 25505
Ion Ratio Lower Upper
117 100
119 4.7 77.3 115.9#
121 0.0 24.2 36.2#

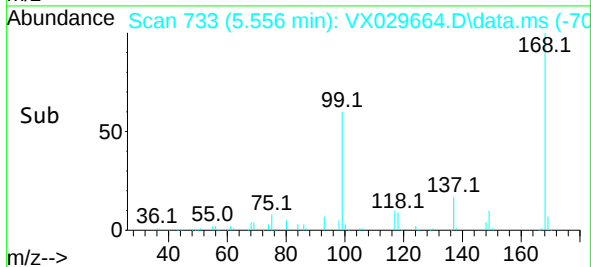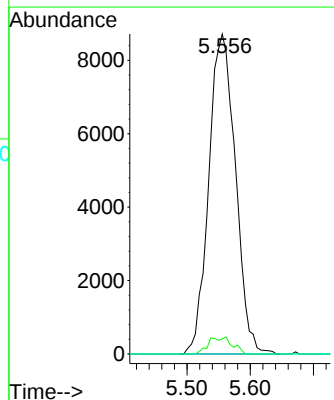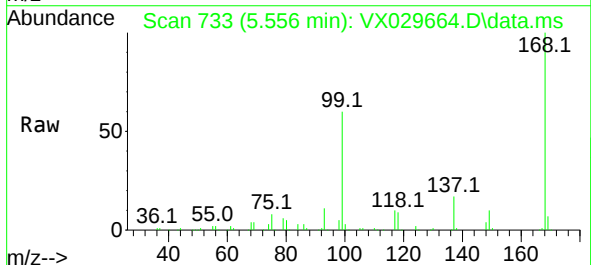

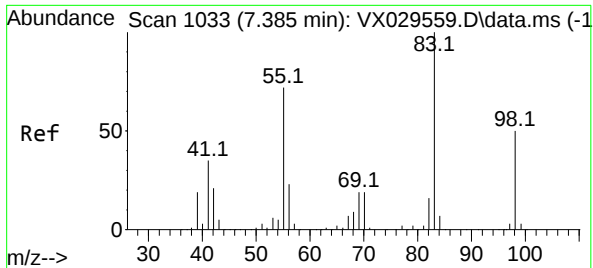

#39

Methylcyclohexane

Concen: 0.509 ug/l

RT: 7.385 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46

Instrument :

MSVOA_X

ClientSampleId :

MW-101RDL





Tgt Ion: 83 Resp: 2360

Ion Ratio Lower Upper

83 100

55 75.6 54.6 81.8

98 61.7 37.4 56.2#

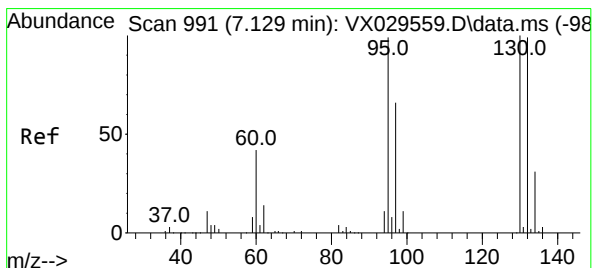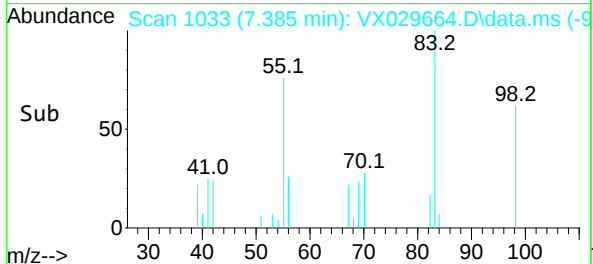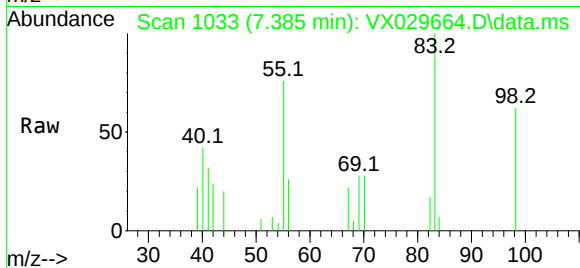

#44

Trichloroethene

Concen: Below Cal

RT: 7.135 min Scan# 992

Delta R.T. 0.006 min

Lab File: VX029664.D




Acq: 21 Jun 2022 15:46


Tgt Ion:130 Resp: 1753

Ion Ratio Lower Upper

130 100

95 96.0 0.0 188.8


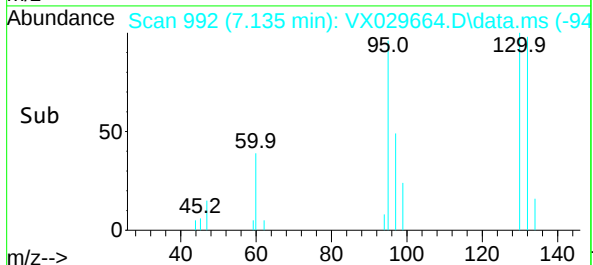
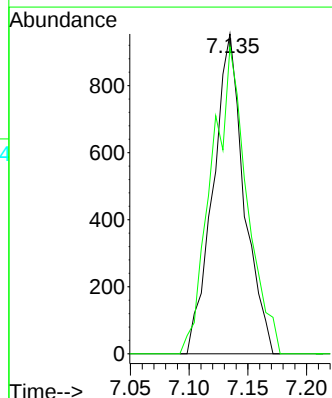
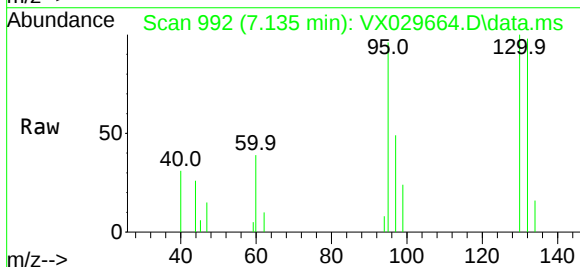




#50
Toluene-d8
Concen: 47.426 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion: 98 Resp: 476071
Ion Ratio Lower Upper
98 100
100 67.3 52.6 78.8

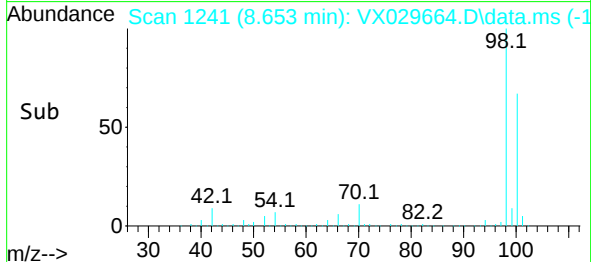

#51
4-Methyl-2-Pentanone
Concen: 0.316 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.012 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 43 Resp: 1207
Ion Ratio Lower Upper
43 100
58 39.5 36.1 54.1

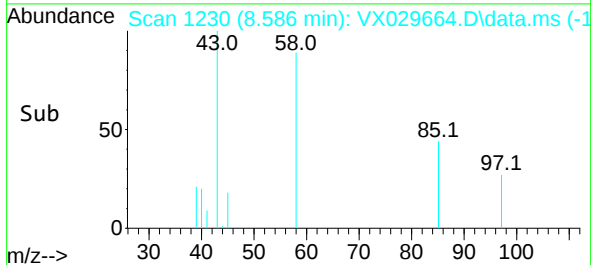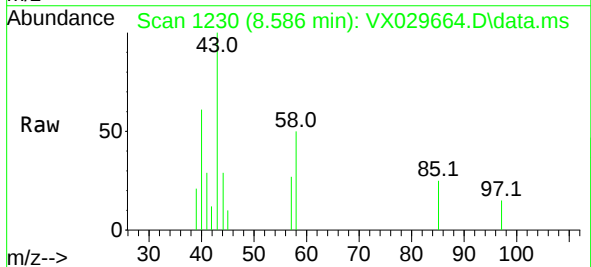

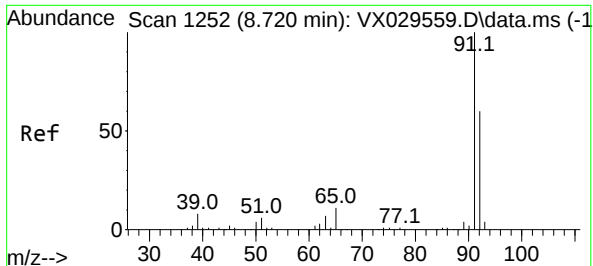

#52

Toluene

Concen: 18.814 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46

Instrument :

MSVOA_X

ClientSampleId :





MW-101RDL

Tgt Ion: 92 Resp: 132812

Ion Ratio Lower Upper

92 100

91 169.3 137.5 206.3

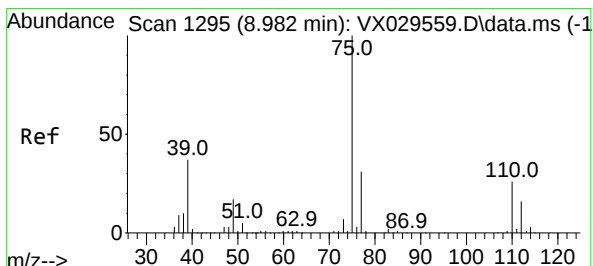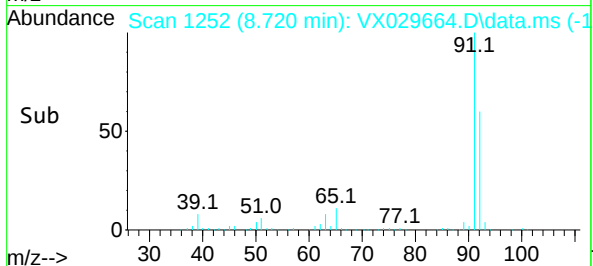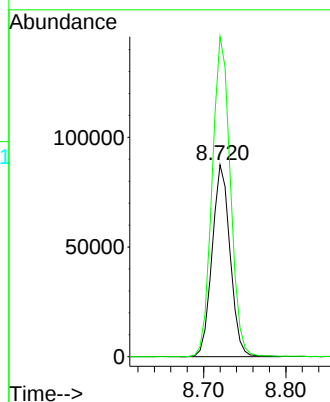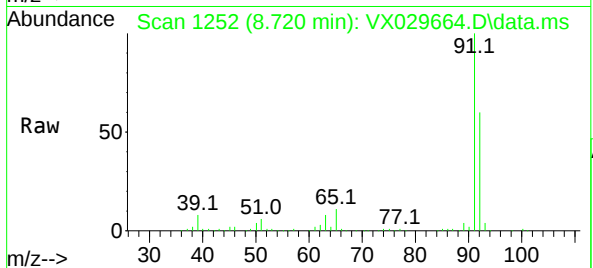

#53

t-1,3-Dichloropropene

Concen: 0.378 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.262 min

Lab File: VX029664.D




Acq: 21 Jun 2022 15:46


Tgt Ion: 75 Resp: 1430

Ion Ratio Lower Upper

75 100

77 118.5 25.4 38.0#

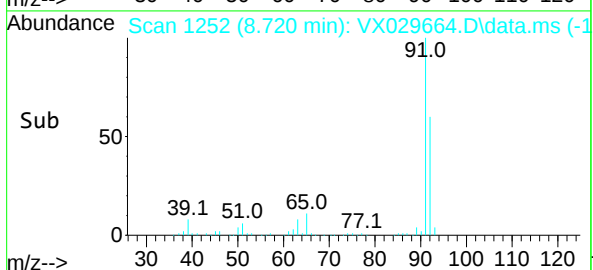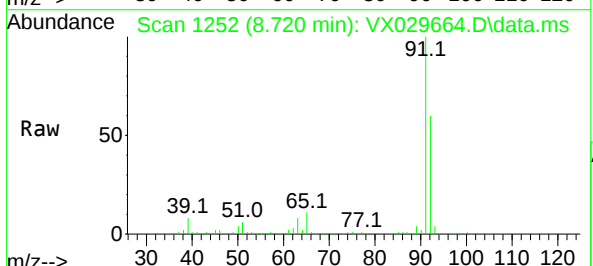

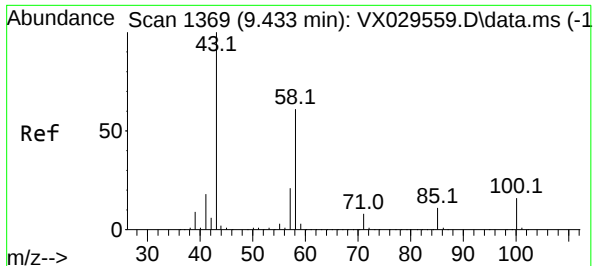

#59

2-Hexanone

Concen: 0.669 ug/l

RT: 9.439 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46

Instrument :

MSVOA_X

ClientSampleId :





MW-101RDL

Tgt Ion: 43 Resp: 1937

Ion Ratio Lower Upper

43 100

58 49.0 31.9 95.7

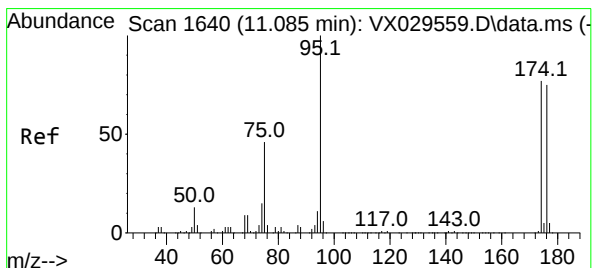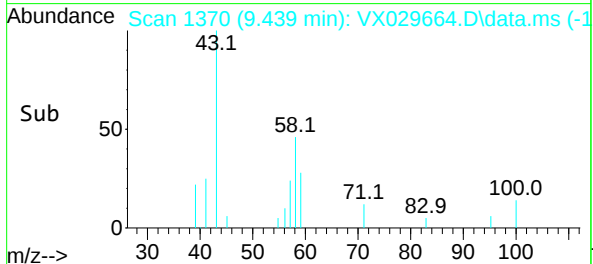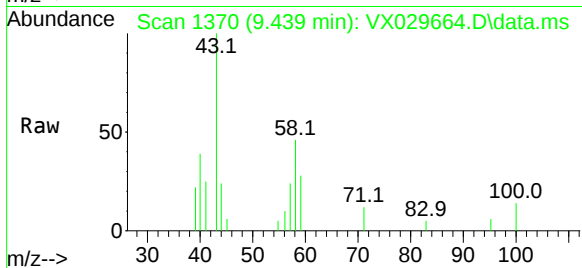

#62

4-Bromofluorobenzene

Concen: 46.570 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46




Tgt Ion: 95 Resp: 176293


Ion Ratio Lower Upper

95 100

174 73.0 0.0 163.0

176 69.7 0.0 155.0


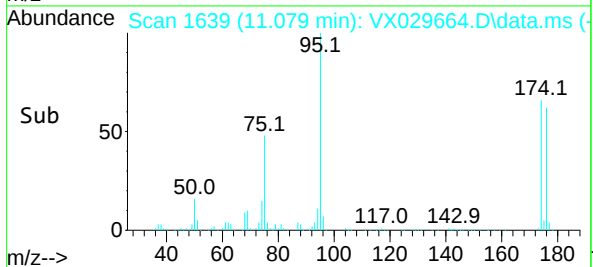

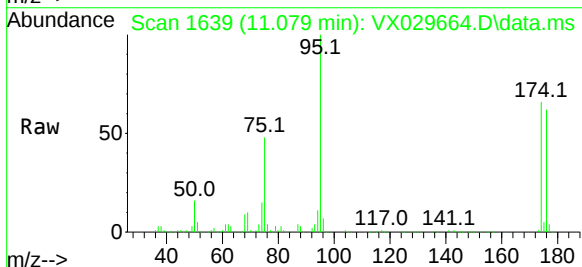




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:117 Resp: 368965
Ion Ratio Lower Upper
117 100
82 55.1 41.8 62.8
119 32.2 24.8 37.2

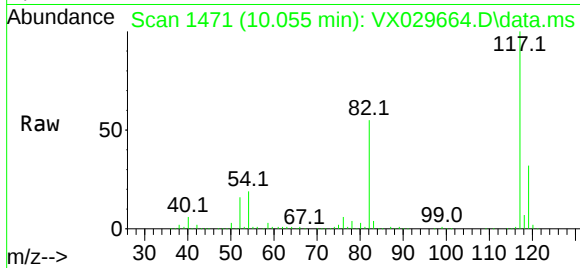

#67
Ethyl Benzene
Concen: 40.387 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 91 Resp: 525995
Ion Ratio Lower Upper
91 100
106 31.6 24.6 36.8




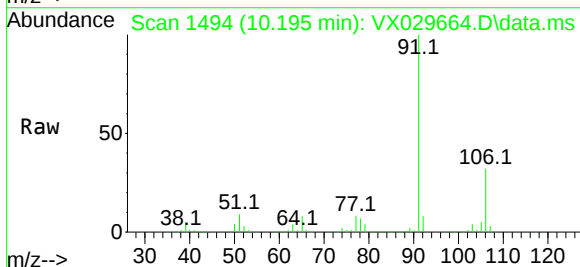


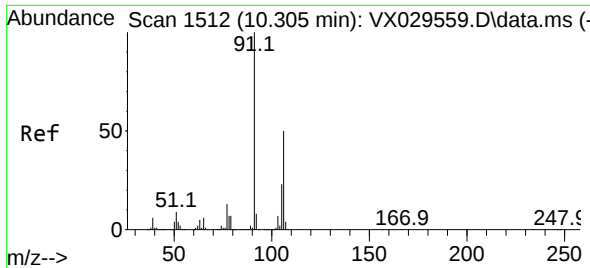

#68
m/p-Xylenes
Concen: 128.762 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:106 Resp: 653975
Ion Ratio Lower Upper
106 100
91 200.7 160.4 240.6

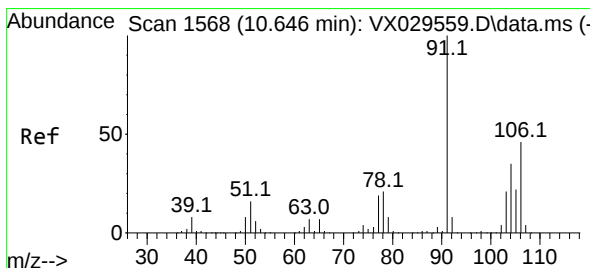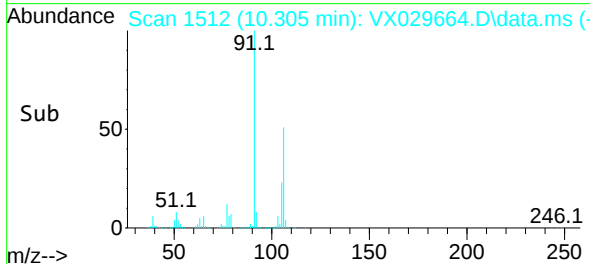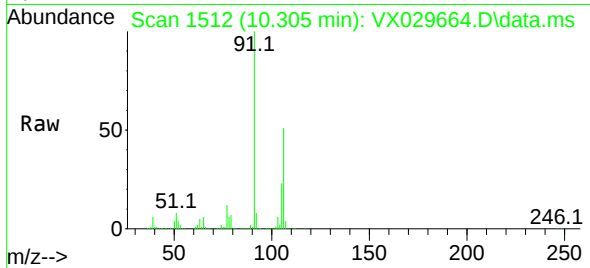

#69
o-Xylene
Concen: 50.697 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion:106 Resp: 254394
Ion Ratio Lower Upper
106 100
91 214.4 106.1 318.1


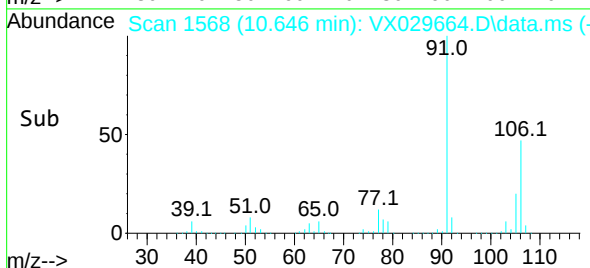

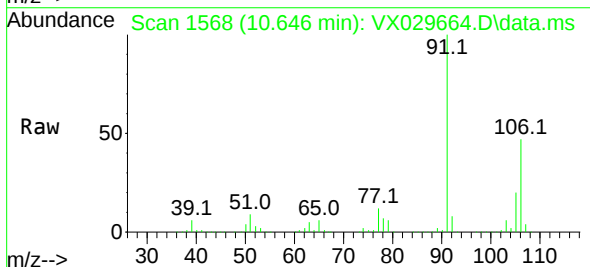




#70
Styrene
Concen: 1.562 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:104 Resp: 12832
Ion Ratio Lower Upper
104 100
78 286.7 38.6 57.8#
103 262.5 43.8 65.8#

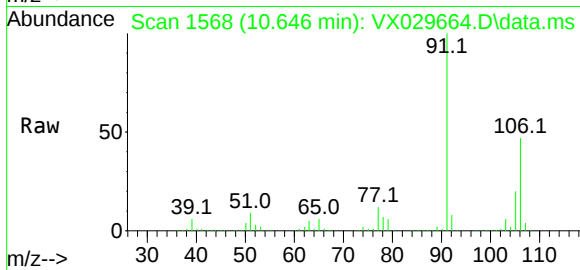

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion:152 Resp: 169172
Ion Ratio Lower Upper
152 100
115 63.0 37.5 112.7
150 156.8 0.0 338.2

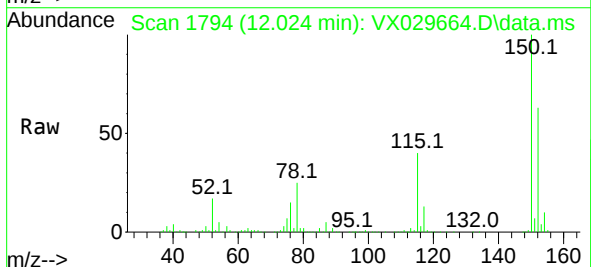



#73

Isopropylbenzene

Concen: 1.346 ug/l

RT: 10.963 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46

Instrument :

MSVOA_X

ClientSampleId :





MW-101RDL

Tgt Ion:105 Resp: 17076

Ion Ratio Lower Upper

105 100

120 27.6 13.5 40.5

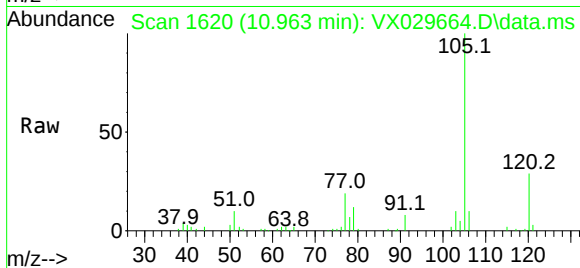

#76

1,2,3-Trichloropropane

Concen: 0.723 ug/l

RT: 11.384 min Scan# 1689

Delta R.T. 0.140 min

Lab File: VX029664.D




Acq: 21 Jun 2022 15:46


Tgt Ion: 75 Resp: 2665

Ion Ratio Lower Upper

75 100

77 1277.7 19.4 58.2#


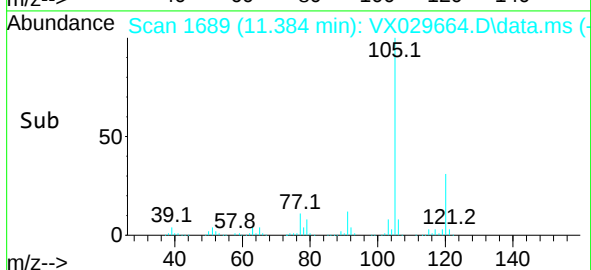

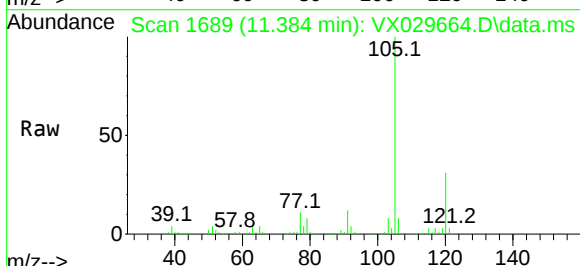


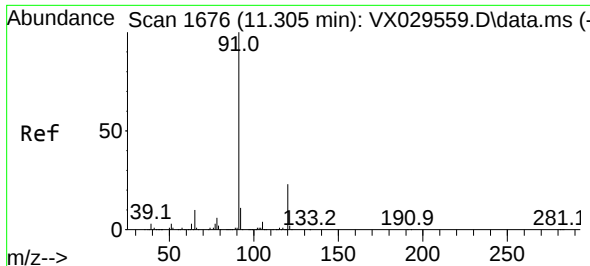

#78
n-propylbenzene
Concen: 4.095 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion: 91 Resp: 58507
Ion Ratio Lower Upper
91 100
120 22.6 11.6 34.8

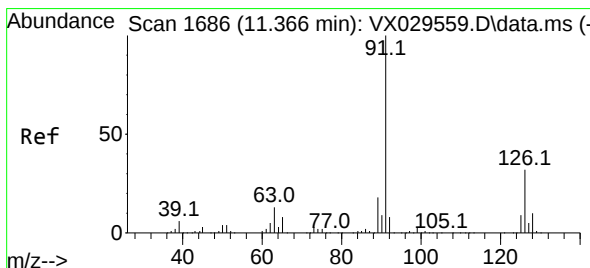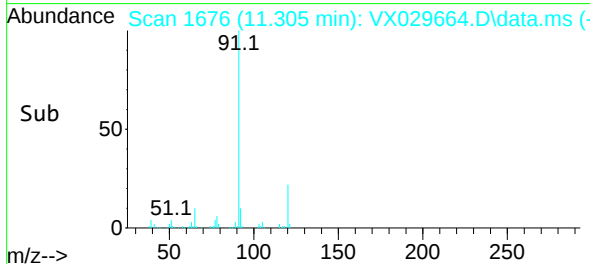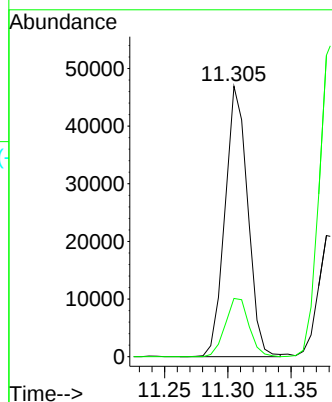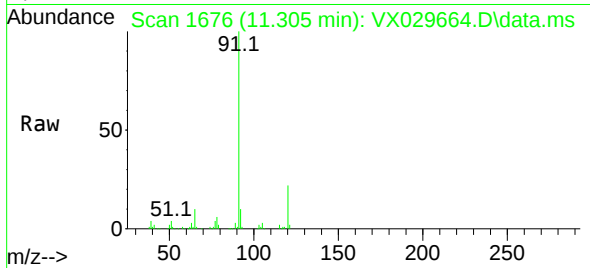

#79
2-Chlorotoluene
Concen: 4.128 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 91 Resp: 36514
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#


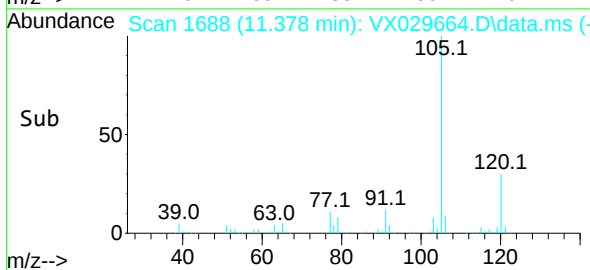
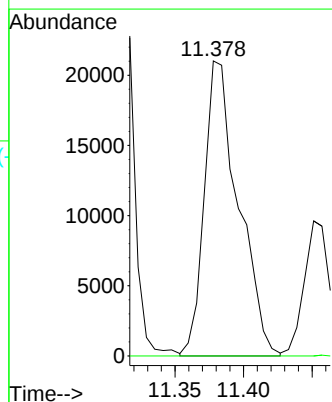
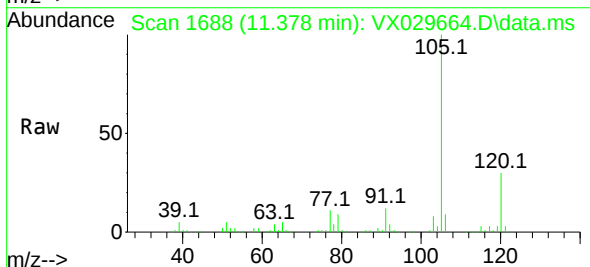




#80
1,3,5-Trimethylbenzene
Concen: 10.680 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46




Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL


Tgt Ion:105 Resp: 114089
Ion Ratio Lower Upper
105 100
120 47.1 24.3 72.9

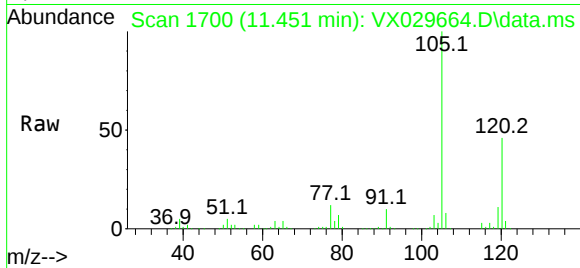

#81
trans-1,4-Dichloro-2-butene
Concen: 75.760 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Tgt Ion: 75 Resp: 83928
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

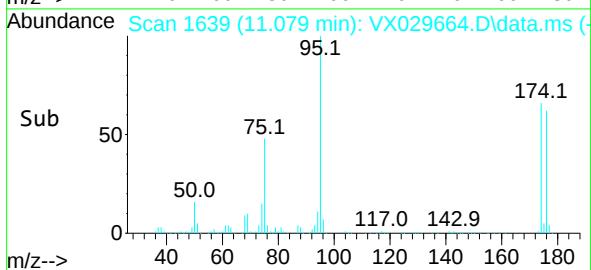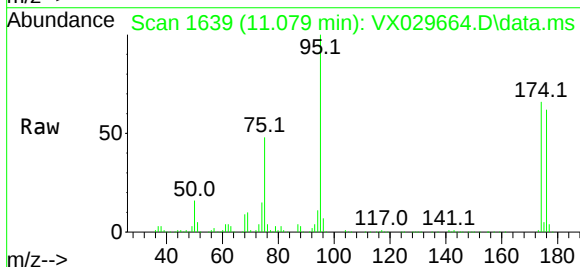



#82

4-Chlorotoluene

Concen: 1.216 ug/l

RT: 11.451 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46

Instrument :

MSVOA_X

ClientSampleId :





MW-101RDL

Tgt Ion: 91 Resp: 12270

Ion Ratio Lower Upper

91 100

126 0.2 14.9 44.5#

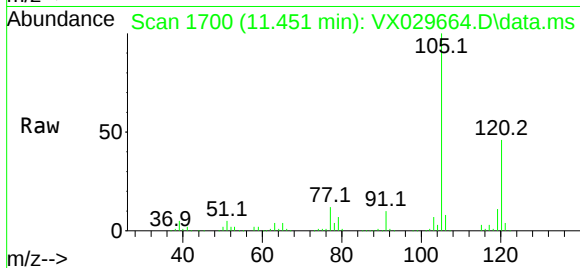

#83

tert-Butylbenzene

Concen: 4.943 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.037 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46




Tgt Ion: 119 Resp: 51489


Ion Ratio Lower Upper

119 100

91 84.7 26.9 80.6#

134 0.0 11.4 34.2#




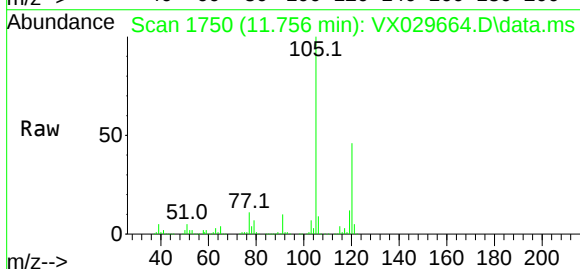




#84
 1,2,4-Trimethylbenzene
 Concen: 39.589 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.000 min
 Lab File: VX029664.D
 Acq: 21 Jun 2022 15:46




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-101RDL


Tgt Ion:105 Resp: 421783
 Ion Ratio Lower Upper
 105 100
 120 45.4 22.6 67.8

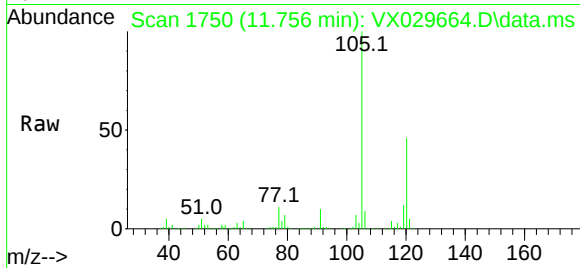

#85
 sec-Butylbenzene
 Concen: 32.675 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.134 min
 Lab File: VX029664.D
 Acq: 21 Jun 2022 15:46

Tgt Ion:105 Resp: 421783
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4#

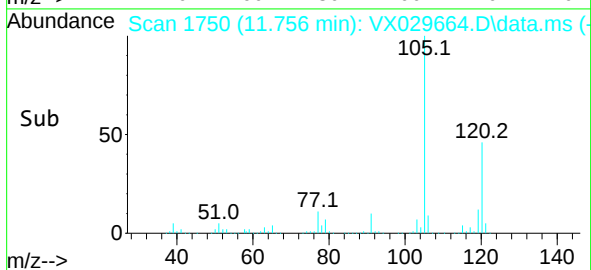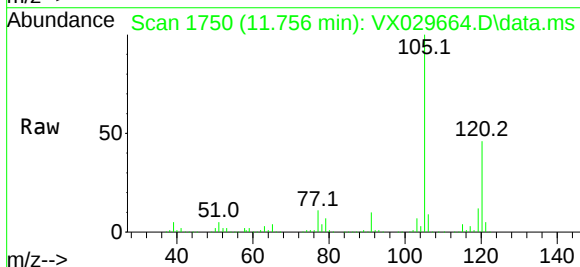



#89

n-Butylbenzene

Concen: 1.113 ug/l

RT: 12.323 min Scan# 1843

Delta R.T. -0.012 min

Lab File: VX029664.D

Acq: 21 Jun 2022 15:46

Instrument :

MSVOA_X

ClientSampleId :

MW-101RDL





Tgt Ion: 91 Resp: 10149

Ion Ratio Lower Upper

91 100

92 30.2 27.8 83.3

134 120.5 13.3 39.8#

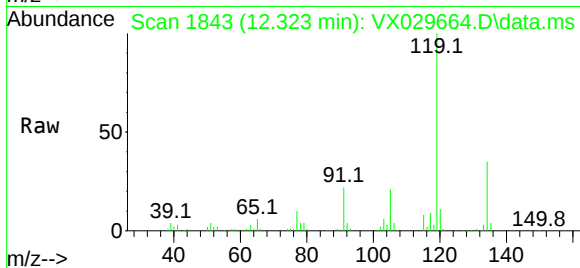

#90

Hexachloroethane

Concen: 2.115 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.012 min

Lab File: VX029664.D




Acq: 21 Jun 2022 15:46


Tgt Ion:117 Resp: 3273

Ion Ratio Lower Upper

117 100


201 0.0 39.5 118.5#

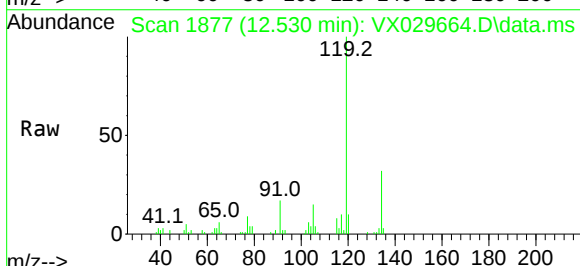



#95
Naphthalene
Concen: 13.075 ug/l
RT: 13.780 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX029664.D
Acq: 21 Jun 2022 15:46

Instrument :
MSVOA_X
ClientSampleId :
MW-101RDL

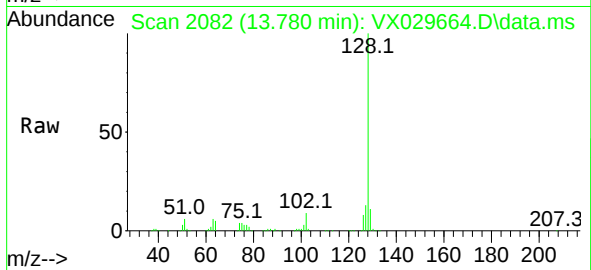

Tgt Ion:128 Resp: 155154
Ion Ratio Lower Upper
128 100
127 12.7 10.2 15.4
129 11.3 8.7 13.1

