

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
 Data File : VX029671.D
 Acq On : 21 Jun 2022 18:53
 Operator : JC/MD
 Sample : N3342-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW149S1-230-232

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rVB	54303	48232	3.89%	0.687%
2	1.264	24	29	40	rVB4	17440	26509	2.14%	0.378%
3	1.368	41	46	55	rVB2	17798	25177	2.03%	0.359%
4	1.453	56	60	66	rBV	25297	29794	2.41%	0.425%
5	2.380	207	212	222	rVB	21698	35314	2.85%	0.503%
6	2.947	295	305	317	rVB	27364	63643	5.14%	0.907%
7	3.111	323	332	343	rBV	10943	26170	2.11%	0.373%
8	4.233	507	516	525	rBV3	19576	52144	4.21%	0.743%
9	4.568	561	571	586	rBV	14976	49079	3.96%	0.699%
10	5.391	694	706	721	rBV	144359	412991	33.34%	5.885%
11	5.556	721	733	747	rVV	261216	741199	59.84%	10.562%
12	5.958	788	799	811	rBV	149981	402554	32.50%	5.736%
13	6.763	921	931	944	rBV	395756	948793	76.60%	13.520%
14	7.135	985	992	1000	rBV2	11907	26334	2.13%	0.375%
15	7.220	1000	1006	1018	rBV2	7485	19328	1.56%	0.275%
16	8.653	1234	1241	1249	rBV	804640	1238590	100.00%	17.649%
17	10.055	1465	1471	1481	rBV	794703	1064693	85.96%	15.171%
18	11.085	1634	1640	1655	rBV	604402	792432	63.98%	11.292%
19	12.024	1789	1794	1802	rBV	790828	976880	78.87%	13.920%
20	12.219	1821	1826	1835	rBV2	25743	37982	3.07%	0.541%




Sum of corrected areas: 7017838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029671.D
Acq On : 21 Jun 2022 18:53
Operator : JC/MD
Sample : N3342-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW149S1-230-232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

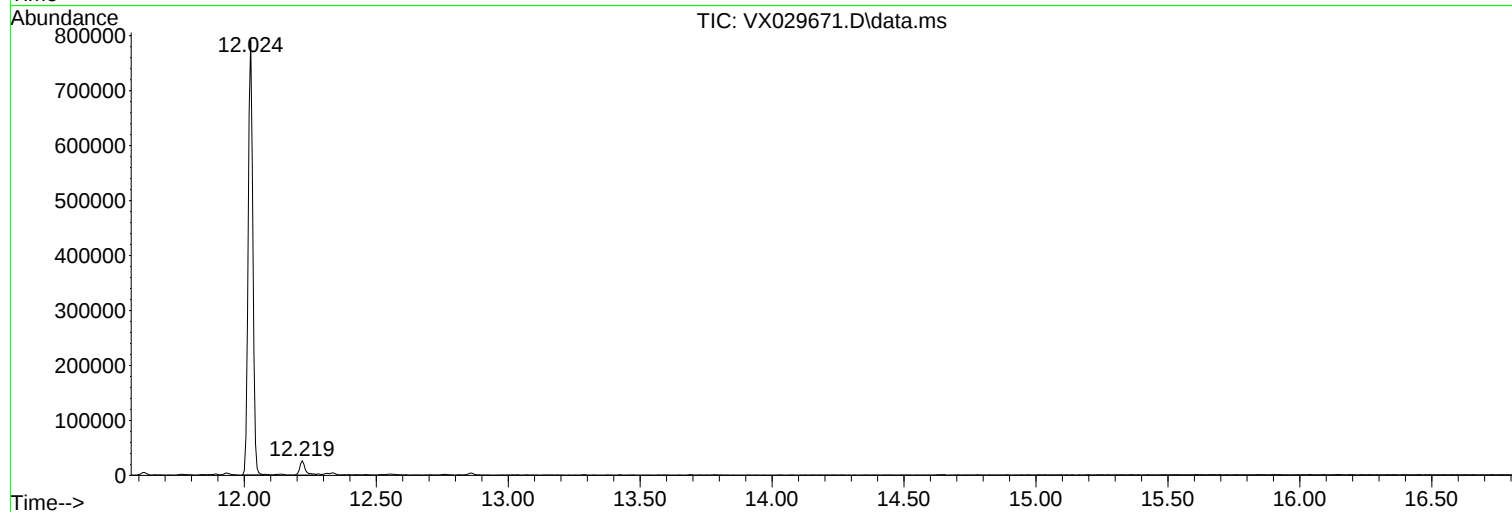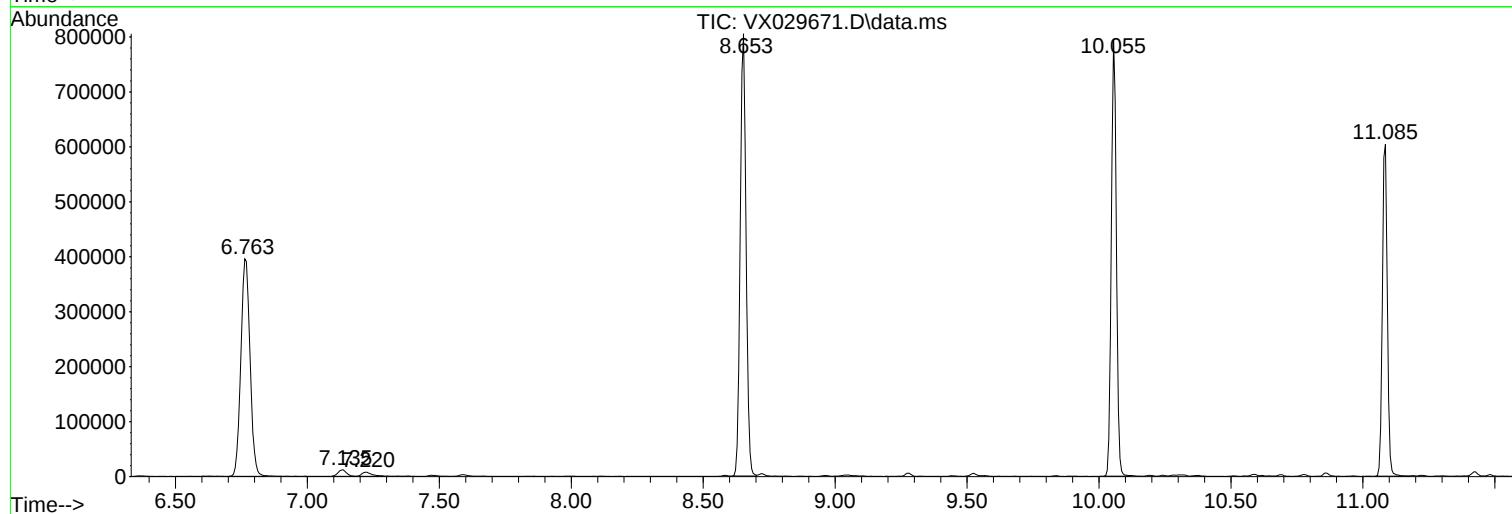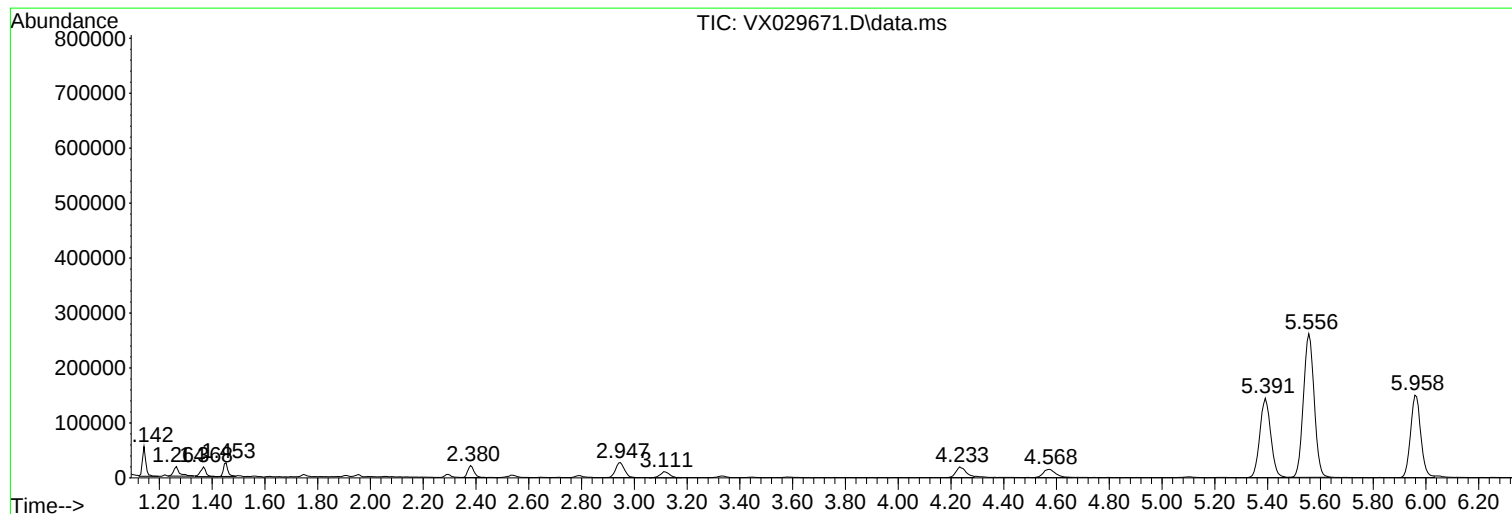

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029671.D
Acq On : 21 Jun 2022 18:53
Operator : JC/MD
Sample : N3342-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW149S1-230-232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029671.D
Acq On : 21 Jun 2022 18:53
Operator : JC/MD
Sample : N3342-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW149S1-230-232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------