

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
 Data File : VX029676.D
 Acq On : 21 Jun 2022 20:49
 Operator : JC/MD
 Sample : N3325-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	45	rBV	297309	597579	47.95%	8.234%
2	2.532	229	237	245	rBV2	6616	17713	1.42%	0.244%
3	2.782	271	278	282	rBV3	5769	12936	1.04%	0.178%
4	5.391	694	706	720	rBV	138039	405800	32.56%	5.591%
5	5.556	722	733	753	rVB	262509	749895	60.18%	10.332%
6	5.958	789	799	812	rBV	148938	394226	31.64%	5.432%
7	6.245	839	846	857	rVB3	9059	28190	2.26%	0.388%
8	6.763	921	931	944	rBV	395000	943175	75.69%	12.996%
9	7.988	1124	1132	1141	rVB3	9502	20649	1.66%	0.285%
10	8.110	1143	1152	1160	rBV2	15147	30580	2.45%	0.421%
11	8.653	1230	1241	1249	rBV	799316	1246166	100.00%	17.170%
12	9.244	1333	1338	1344	rVB2	11707	17426	1.40%	0.240%
13	10.055	1465	1471	1485	rVB	790891	1052832	84.49%	14.507%
14	11.086	1634	1640	1651	rBV	585408	771527	61.91%	10.631%
15	12.024	1789	1794	1802	rBV	775280	935503	75.07%	12.890%
16	12.250	1826	1831	1837	rVB2	13412	19995	1.60%	0.276%
17	13.024	1953	1958	1967	rBV7	5817	13455	1.08%	0.185%


Sum of corrected areas: 7257647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029676.D
Acq On : 21 Jun 2022 20:49
Operator : JC/MD
Sample : N3325-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

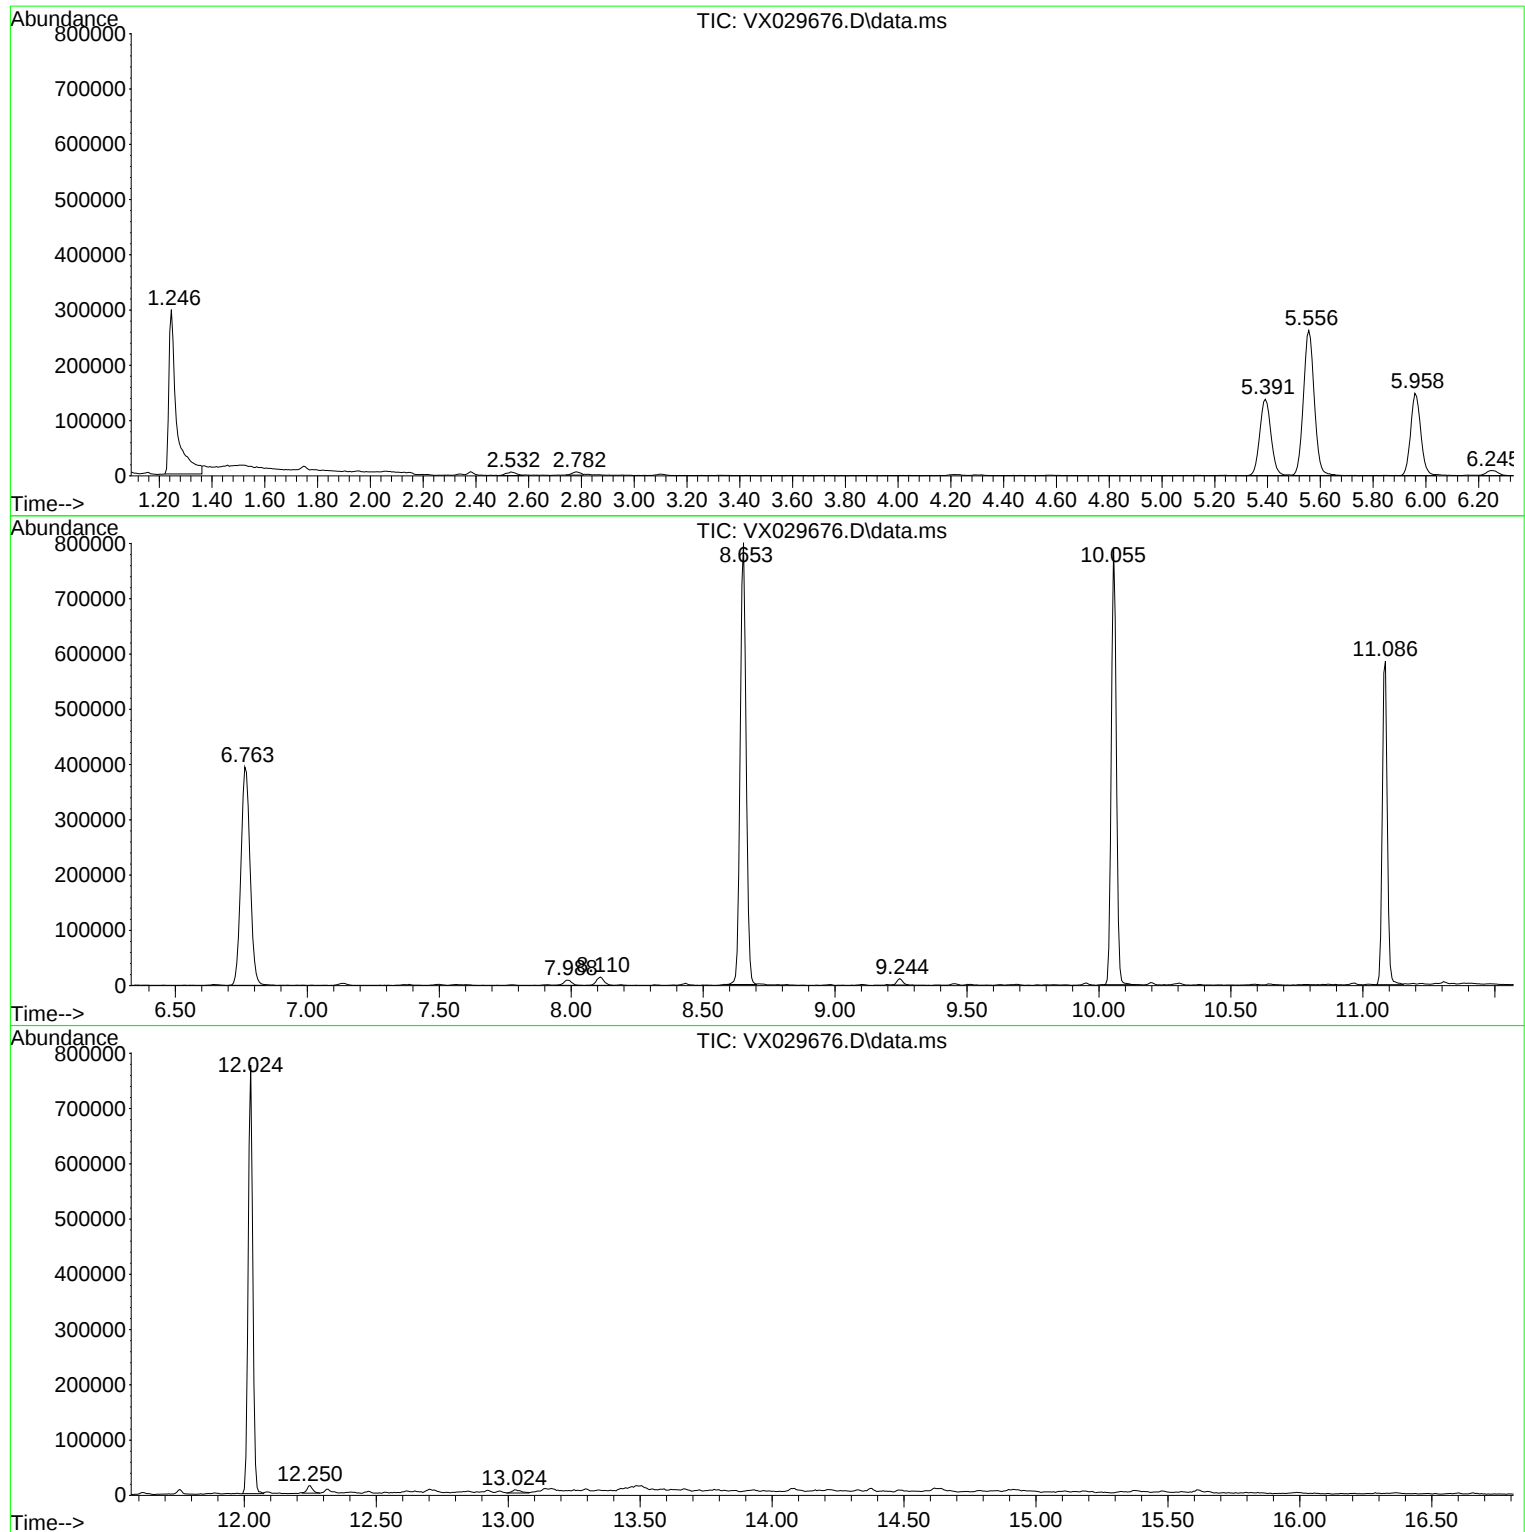

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029676.D
Acq On : 21 Jun 2022 20:49
Operator : JC/MD
Sample : N3325-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11








Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	39.84 ug/l	597579	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

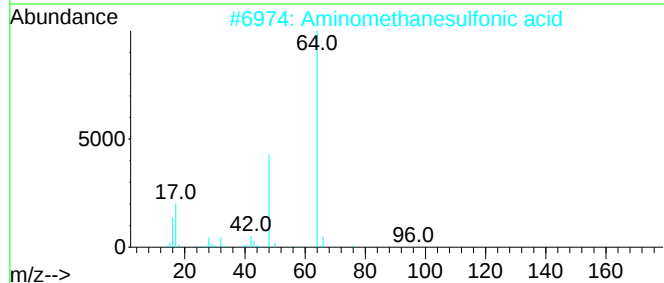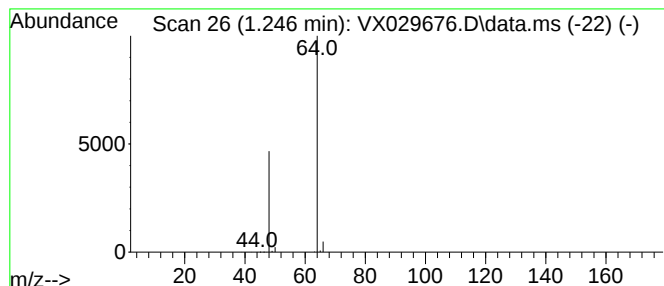

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029676.D
Acq On : 21 Jun 2022 20:49
Operator : JC/MD
Sample : N3325-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	39.8	ug/l	597579	1	5.556	749895	50.0