

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
 Data File : VX029677.D
 Acq On : 21 Jun 2022 21:12
 Operator : JC/MD
 Sample : N3354-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB061422

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	41	rBV	289608	381873	29.98%	5.272%
2	2.532	228	237	248	rBV	24748	47539	3.73%	0.656%
3	2.947	296	305	319	rVB	39262	88314	6.93%	1.219%
4	4.574	561	572	585	rBV	5318	18426	1.45%	0.254%
5	5.391	694	706	720	rBV2	143343	416729	32.72%	5.753%
6	5.556	720	733	750	rVB	265381	754260	59.22%	10.413%
7	5.958	789	799	816	rBV	151084	406358	31.90%	5.610%
8	6.763	922	931	947	rBV	398981	960951	75.45%	13.267%
9	8.653	1234	1241	1261	rBV	802645	1273706	100.00%	17.585%
10	10.055	1465	1471	1487	rBV	812351	1094639	85.94%	15.113%
11	11.086	1634	1640	1654	rBV	618000	803228	63.06%	11.090%
12	12.024	1788	1794	1803	rBV	826854	997112	78.28%	13.766%




Sum of corrected areas: 7243135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029677.D
Acq On : 21 Jun 2022 21:12
Operator : JC/MD
Sample : N3354-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB061422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

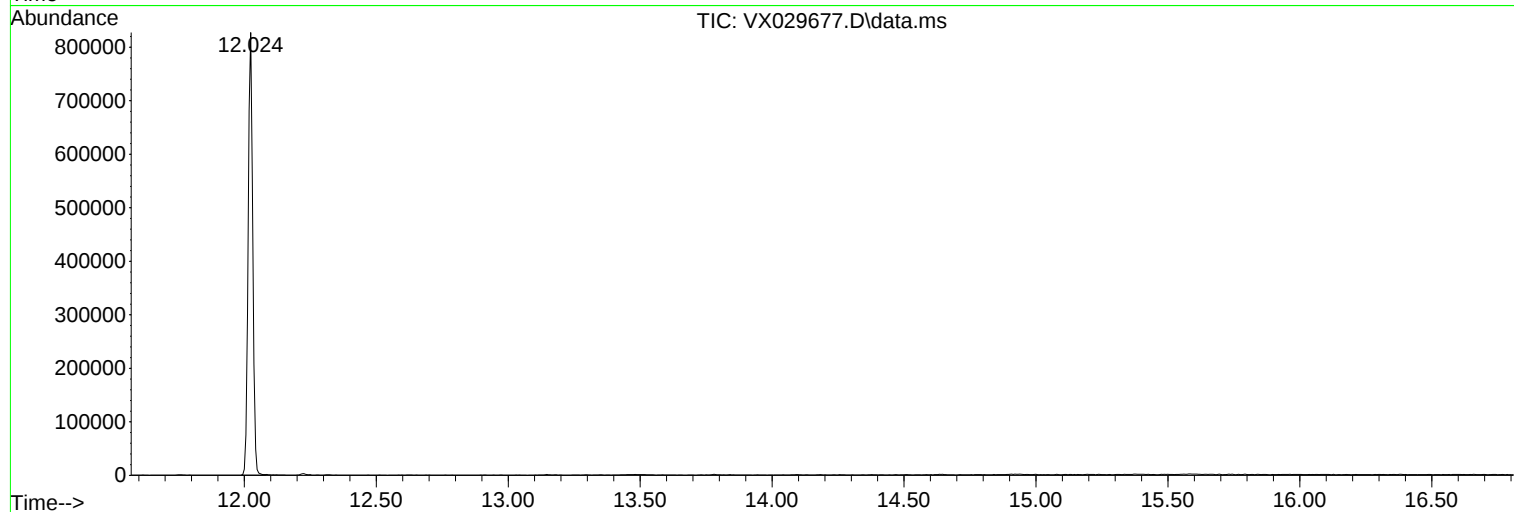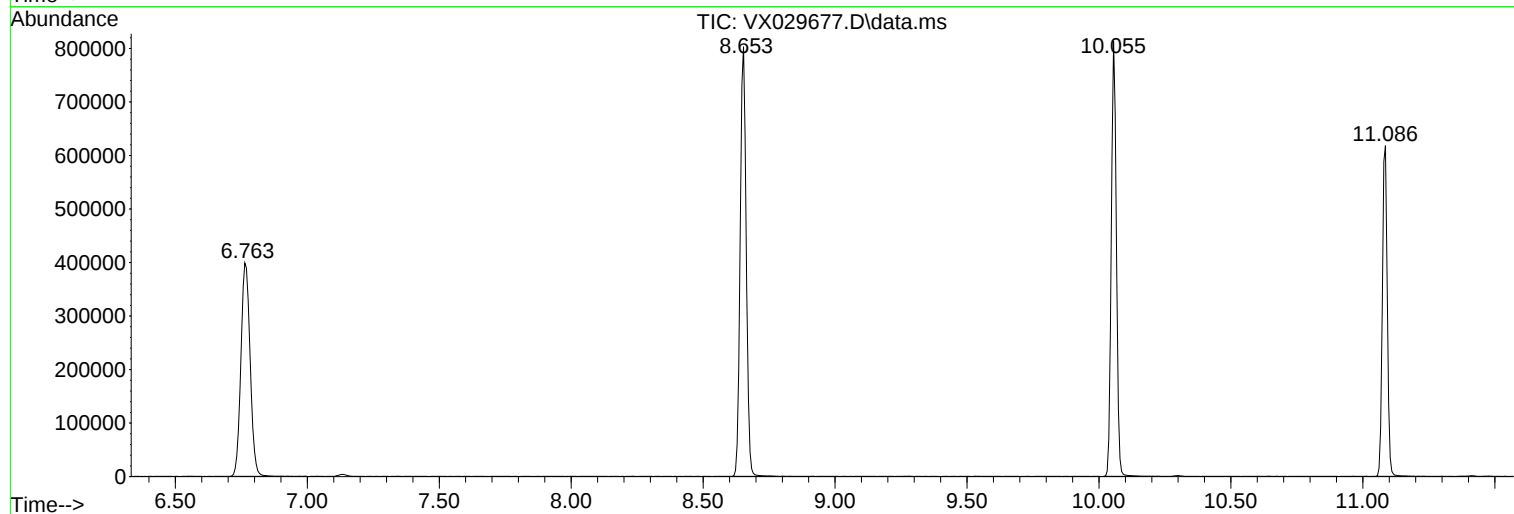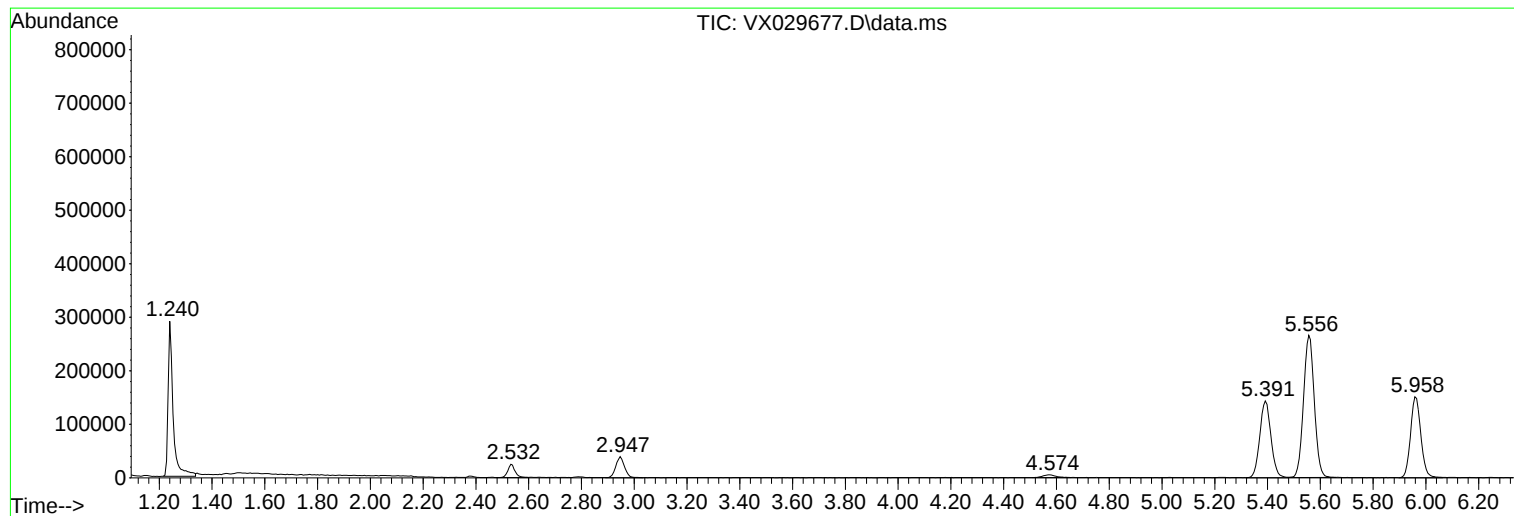

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029677.D
Acq On : 21 Jun 2022 21:12
Operator : JC/MD
Sample : N3354-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB061422










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.240	25.31 ug/l	381873	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

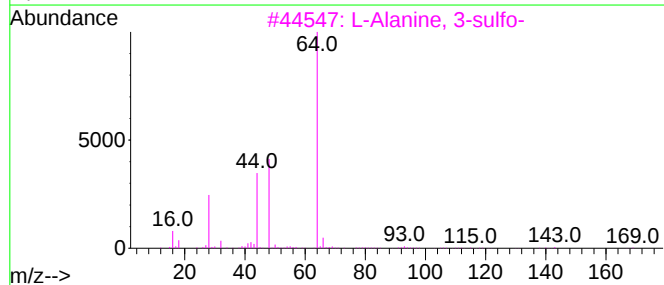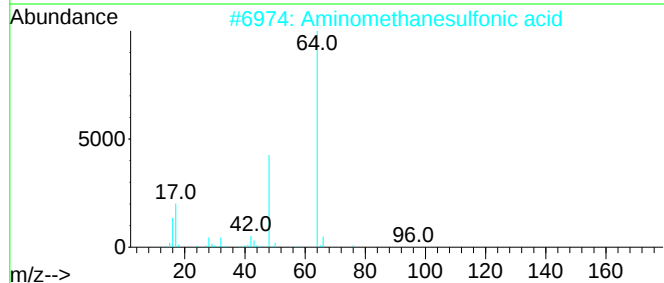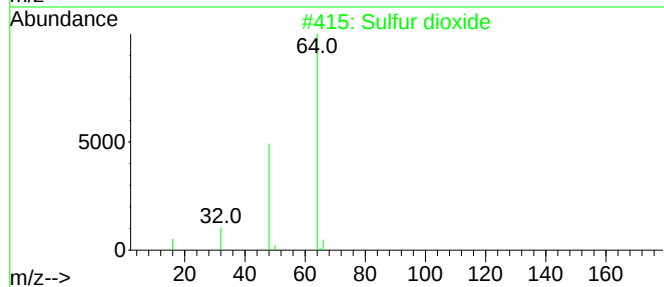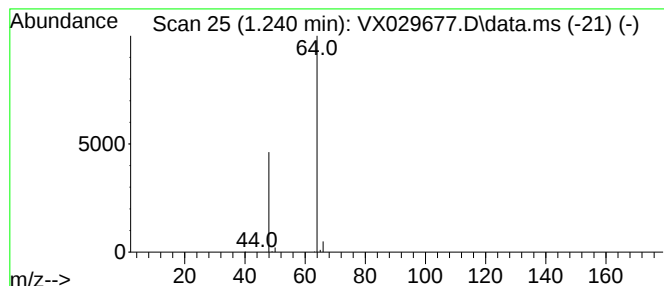

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029677.D
Acq On : 21 Jun 2022 21:12
Operator : JC/MD
Sample : N3354-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB061422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.240	25.3	ug/l	381873	1	5.556	754260	50.0