

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029679.D
Acq On : 21 Jun 2022 21:59
Operator : JC/MD
Sample : N3286-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	40	rBV	137808	252414	12.08%	2.260%
2	5.391	691	706	720	rBV	243167	715822	34.26%	6.409%
3	5.556	720	733	747	rVV	389374	1102842	52.78%	9.875%
4	5.964	788	800	816	rBV	258525	692830	33.15%	6.204%
5	6.763	920	931	951	rBV	604585	1441798	69.00%	12.910%
6	8.653	1233	1241	1256	rBV	1341761	2089684	100.00%	18.711%
7	10.055	1465	1471	1486	rBV	1300142	1705817	81.63%	15.274%
8	10.305	1506	1512	1519	rVB	23763	34438	1.65%	0.308%
9	11.085	1634	1640	1654	rBV	1035614	1343107	64.27%	12.026%
10	11.616	1723	1727	1734	rVB	16656	21025	1.01%	0.188%
11	12.024	1788	1794	1801	rBV	1484723	1768407	84.63%	15.834%




Sum of corrected areas: 11168184

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029679.D
Acq On : 21 Jun 2022 21:59
Operator : JC/MD
Sample : N3286-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

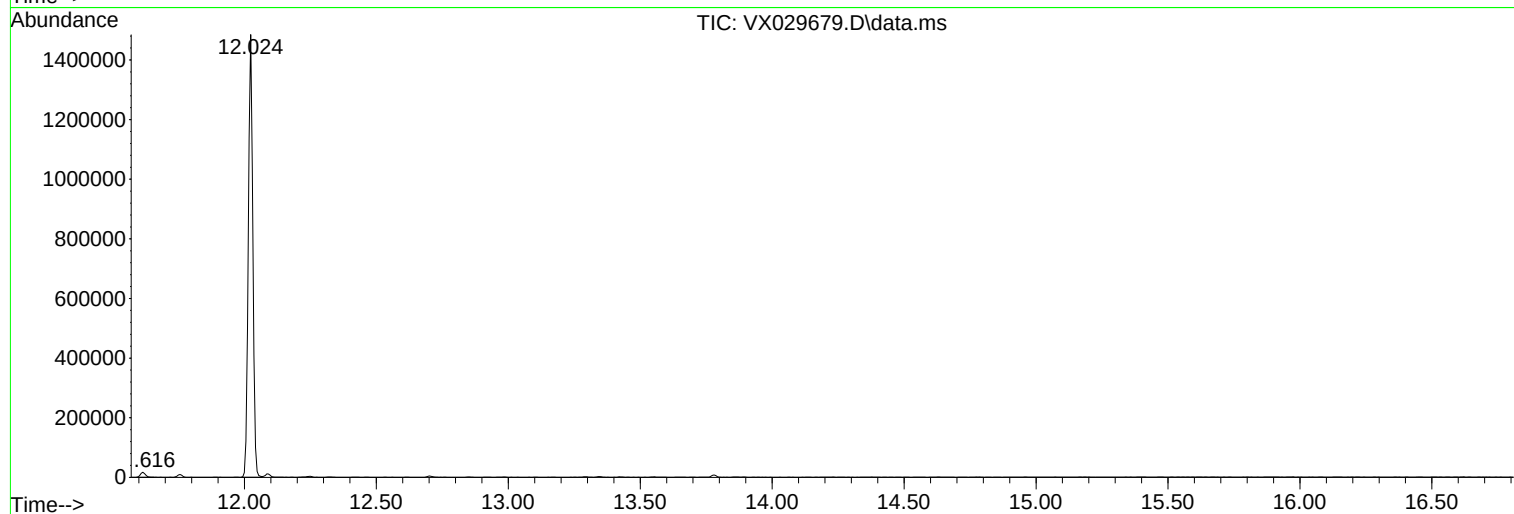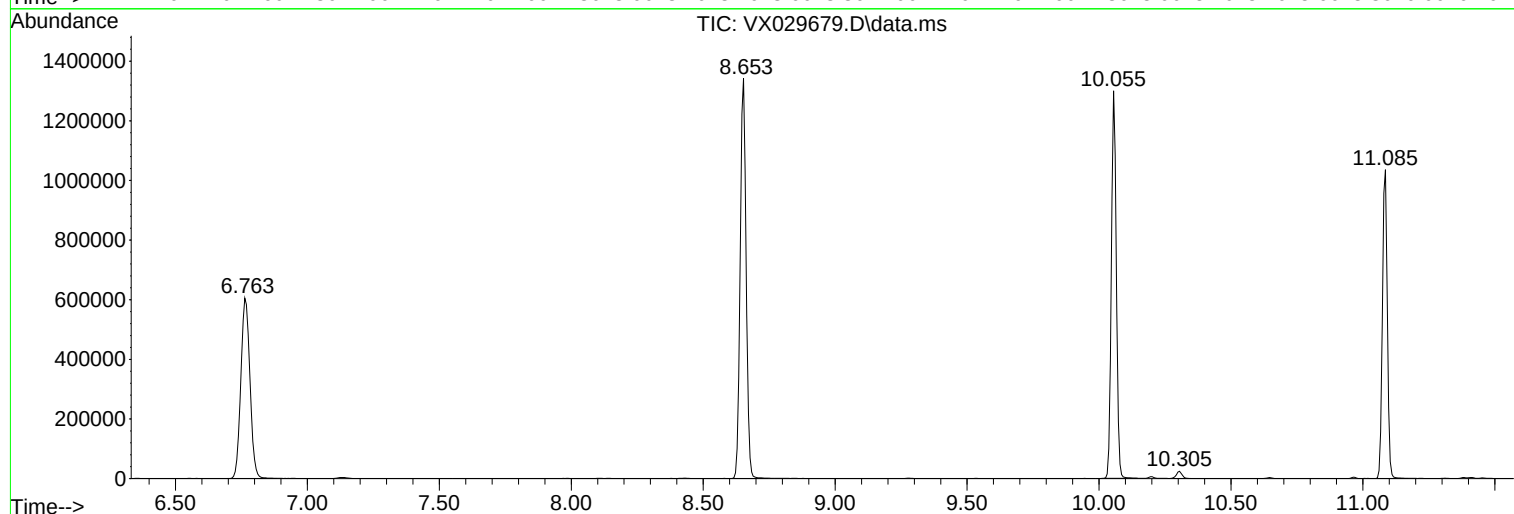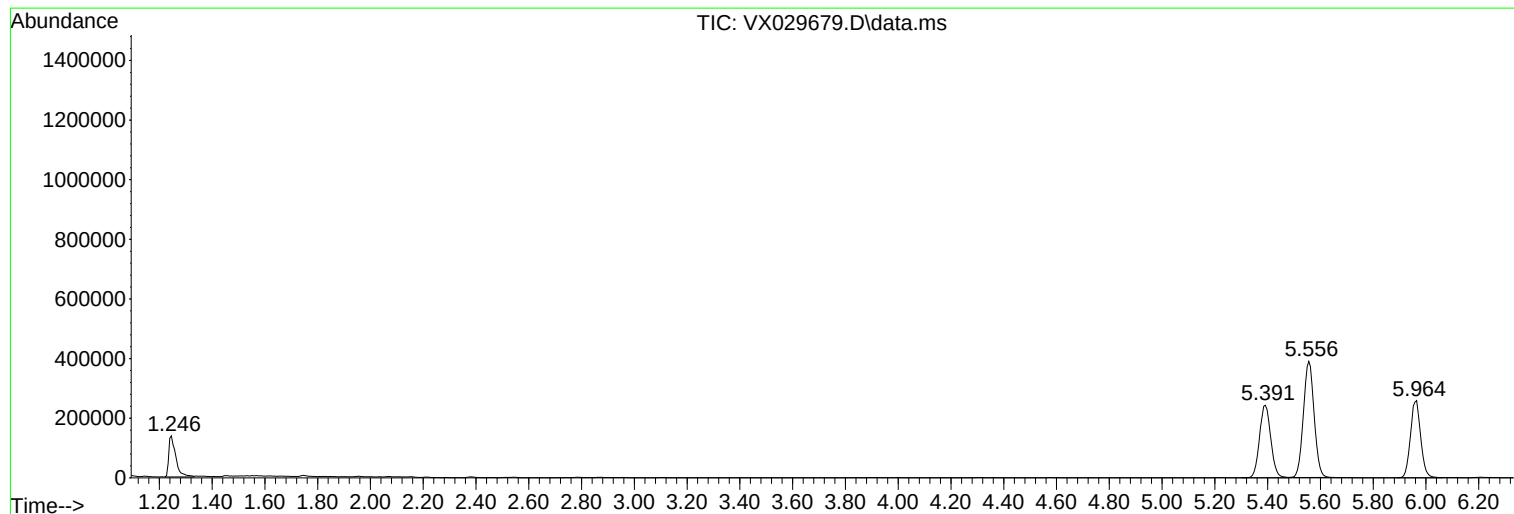

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029679.D
Acq On : 21 Jun 2022 21:59
Operator : JC/MD
Sample : N3286-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	11.44 ug/l	252414	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

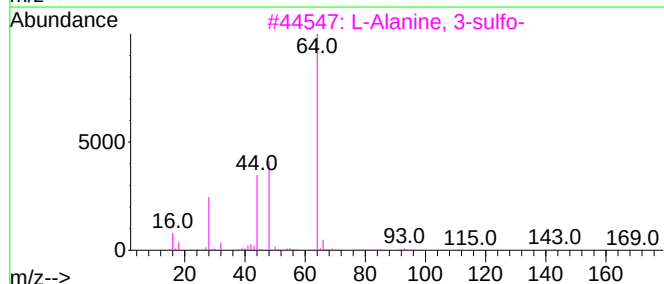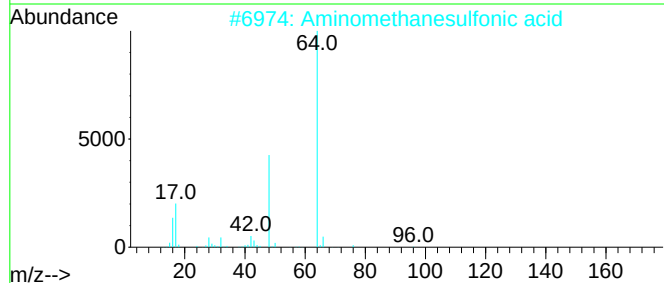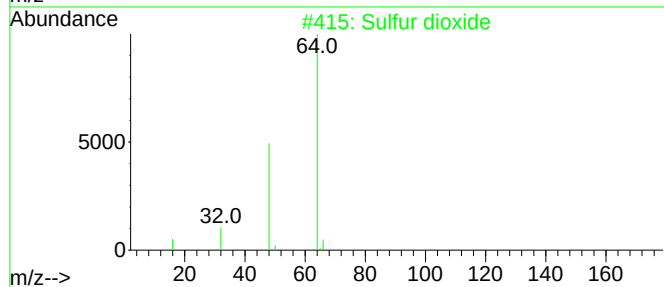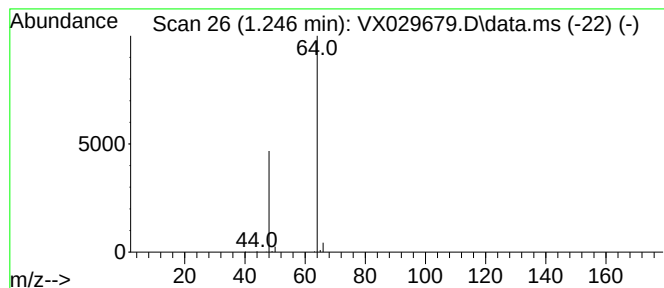

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062122\
Data File : VX029679.D
Acq On : 21 Jun 2022 21:59
Operator : JC/MD
Sample : N3286-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	11.4	ug/l	252414	1	5.556	1102840	50.0