
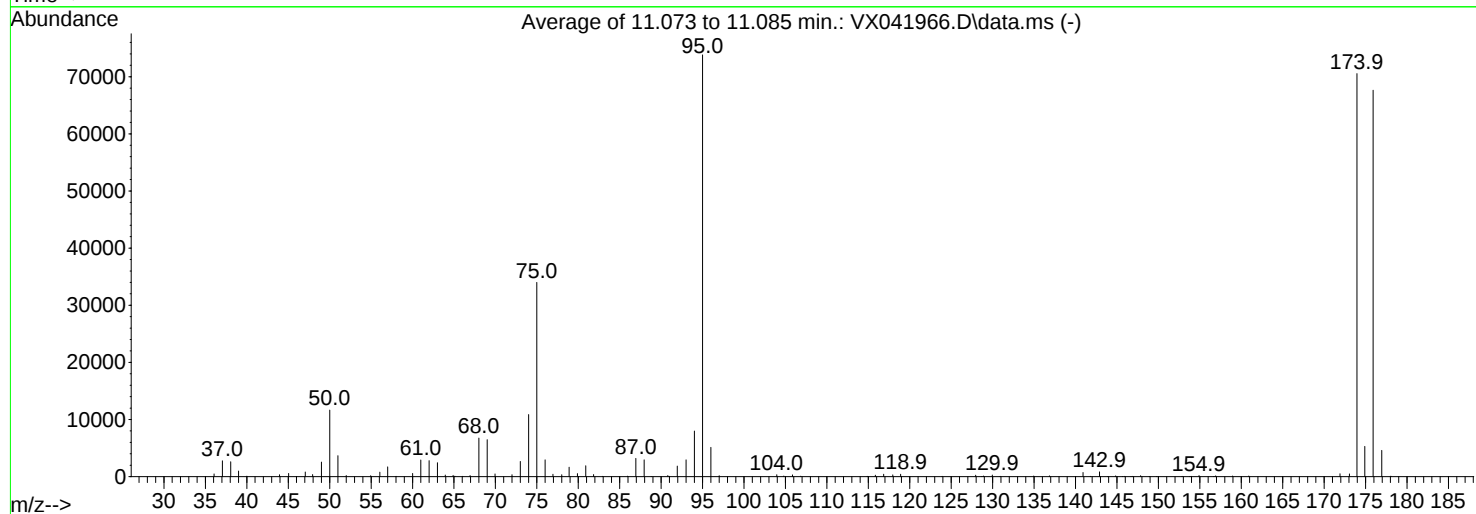


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062124\
Data File : VX041966.D
Acq On : 21 Jun 2024 08:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Title : SW846 8260
Last Update : Fri Jun 21 23:51:58 2024

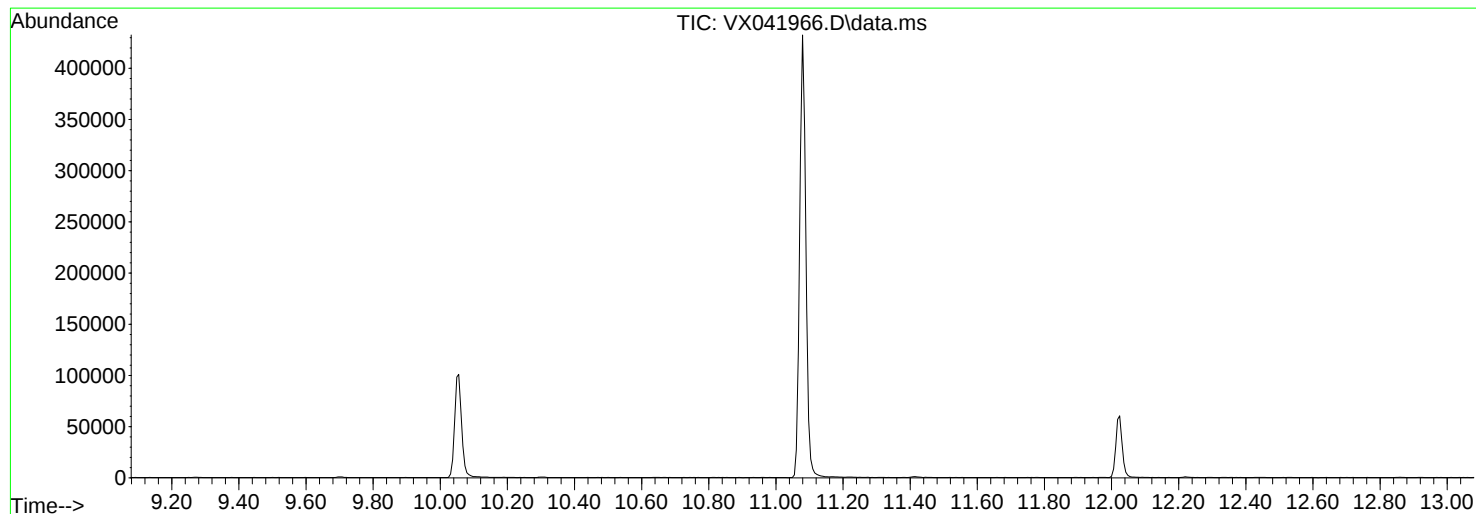

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	11654	PASS
75	95	30	60	46.0	33992	PASS
95	95	100	100	100.0	73829	PASS
96	95	5	9	6.9	5127	PASS
173	174	0.00	2	0.7	468	PASS
174	95	50	100	95.5	70541	PASS
175	174	5	9	7.5	5294	PASS
176	174	95	101	95.9	67651	PASS
177	176	5	9	6.8	4603	PASS