

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062218\
 Data File : VX002848.D
 Acq On : 22 Jun 2018 23:05
 Operator : JC/MD
 Sample : J3631-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S83-0018

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	845400	1038656	81.21%	13.076%
2	1.270	107	112	120	rBV2	20091	35038	2.74%	0.441%
3	2.617	328	333	344	rVB	12826	26808	2.10%	0.337%
4	4.611	650	660	670	rBV2	5210	19219	1.50%	0.242%
5	5.507	793	807	822	rBV	158595	450884	35.25%	5.676%
6	5.665	822	833	850	rVB	242585	681731	53.30%	8.583%
7	6.074	890	900	923	rBV	173446	455090	35.58%	5.729%
8	6.866	1019	1030	1043	rBV	339819	802615	62.75%	10.104%
9	7.220	1081	1088	1096	rVB	10844	23224	1.82%	0.292%
10	8.720	1327	1334	1344	rBV	823565	1279021	100.00%	16.102%
11	10.116	1557	1563	1573	rBV	738569	969366	75.79%	12.204%
12	10.256	1580	1586	1592	rVB	12654	18030	1.41%	0.227%
13	10.360	1595	1603	1609	rBV	18543	29971	2.34%	0.377%
14	11.140	1725	1731	1737	rBV	755833	923870	72.23%	11.631%
15	11.670	1813	1818	1826	rVB2	13539	19304	1.51%	0.243%
16	11.811	1837	1841	1845	rVB	13893	16073	1.26%	0.202%
17	12.079	1880	1885	1893	rBV	844753	1093252	85.48%	13.763%
18	12.146	1893	1896	1903	rVB	9682	13524	1.06%	0.170%
19	12.902	2013	2020	2024	rVB3	9371	15263	1.19%	0.192%
20	13.024	2036	2040	2045	rVB3	9626	13153	1.03%	0.166%
21	13.725	2145	2155	2160	rVB4	6504	19156	1.50%	0.241%


Sum of corrected areas: 7943248

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062218\
Data File : VX002848.D
Acq On : 22 Jun 2018 23:05
Operator : JC/MD
Sample : J3631-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0018

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

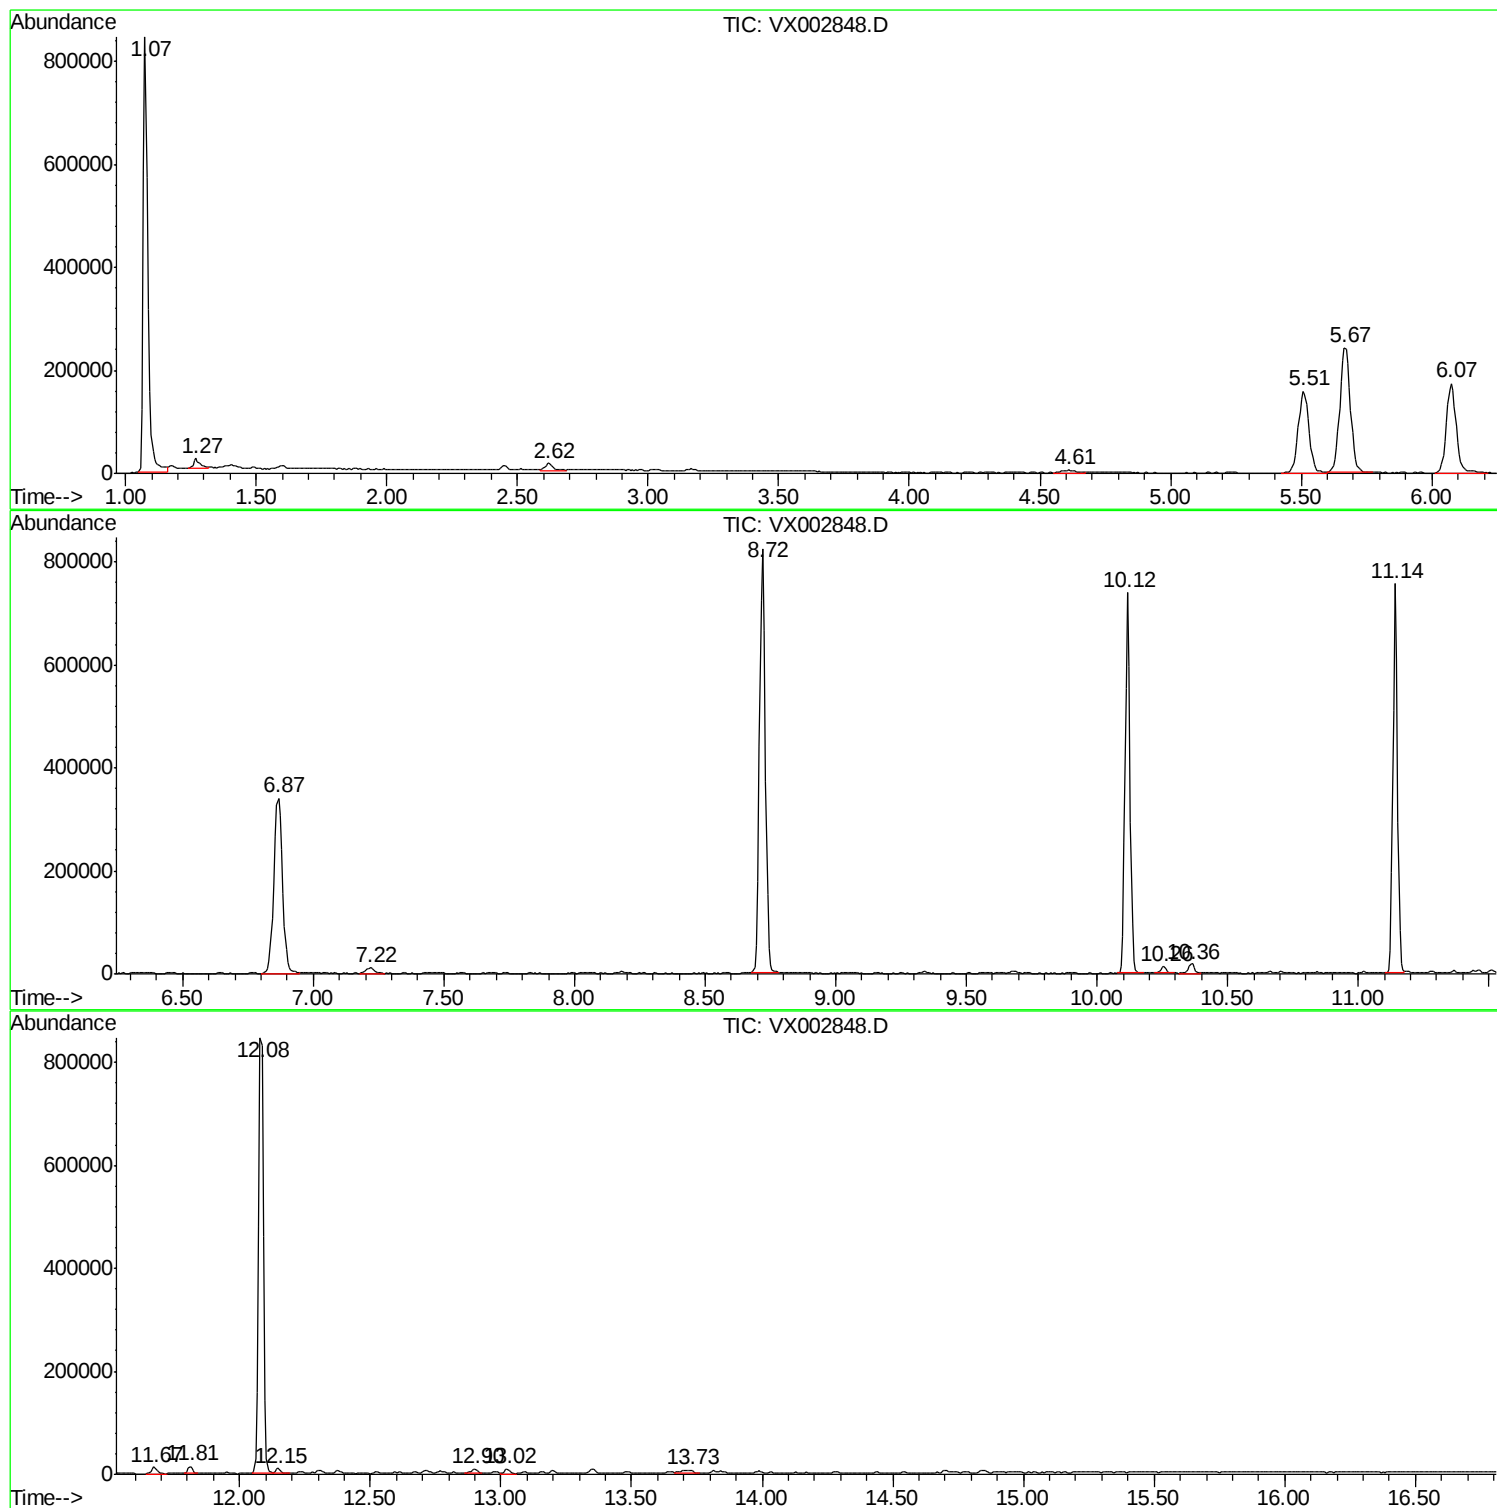

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062218\
Data File : VX002848.D
Acq On : 22 Jun 2018 23:05
Operator : JC/MD
Sample : J3631-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0018

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062218\
Data File : VX002848.D
Acq On : 22 Jun 2018 23:05
Operator : JC/MD
Sample : J3631-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0018

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc