


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX062218\
 Data File : VX002828.D
 Acq On : 22 Jun 2018 09:47
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X061818W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Jun 18 15:18:02 2018

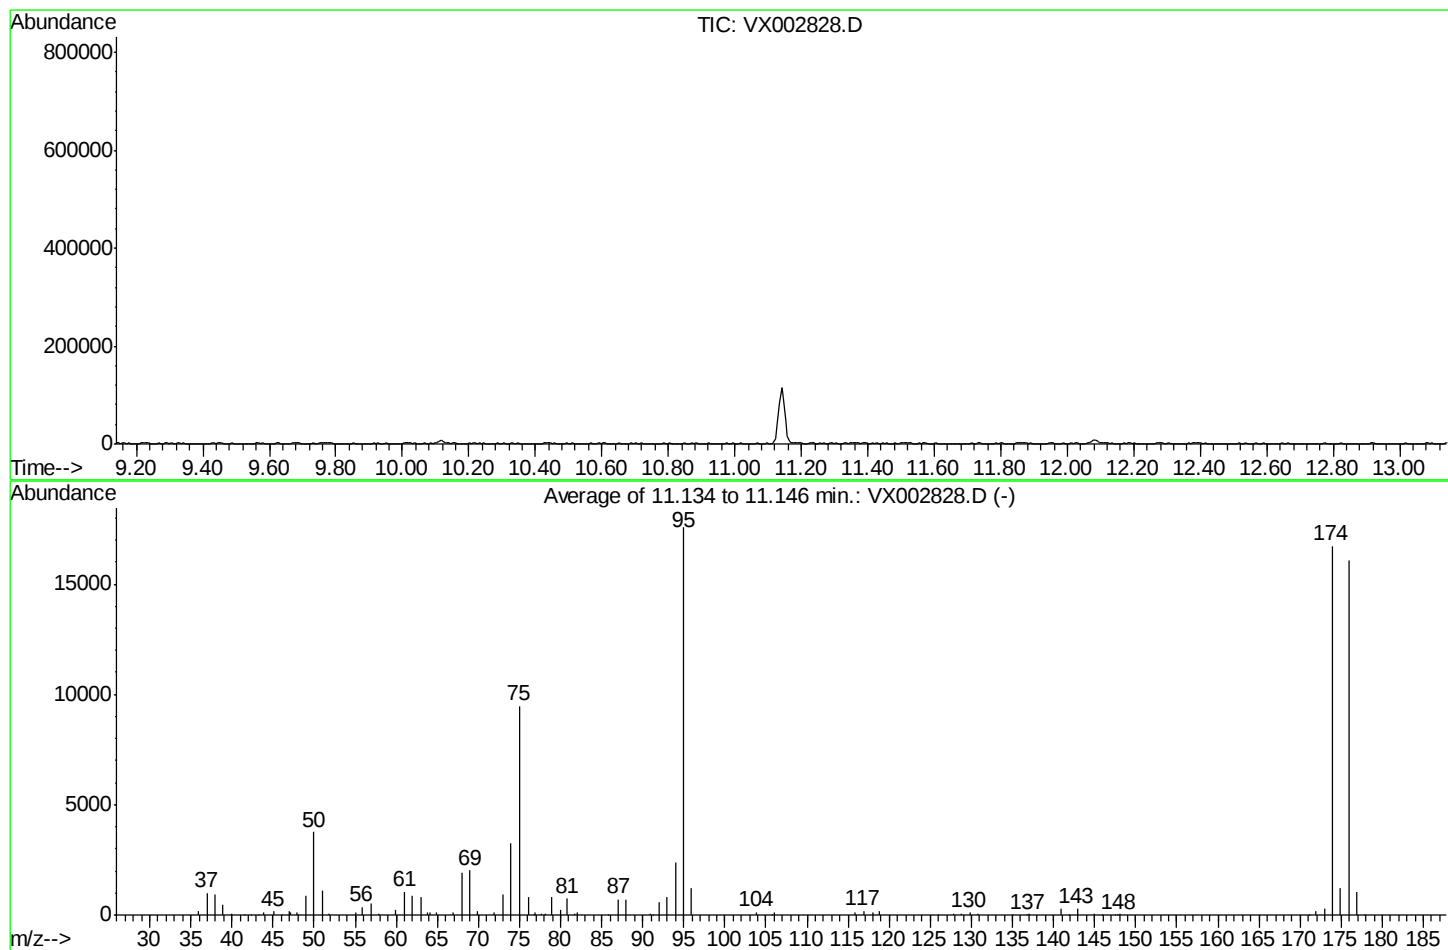

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	3757	PASS
75	95	30	60	53.8	9458	PASS
95	95	100	100	100.0	17572	PASS
96	95	5	9	7.1	1243	PASS
173	174	0.00	2	1.6	265	PASS
174	95	50	100	95.2	16734	PASS
175	174	5	9	7.4	1241	PASS
176	174	95	101	96.1	16077	PASS
177	176	5	9	6.5	1040	PASS