


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062218\
Data File : VX002834.D
Acq On : 22 Jun 2018 15:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:37:33 2018

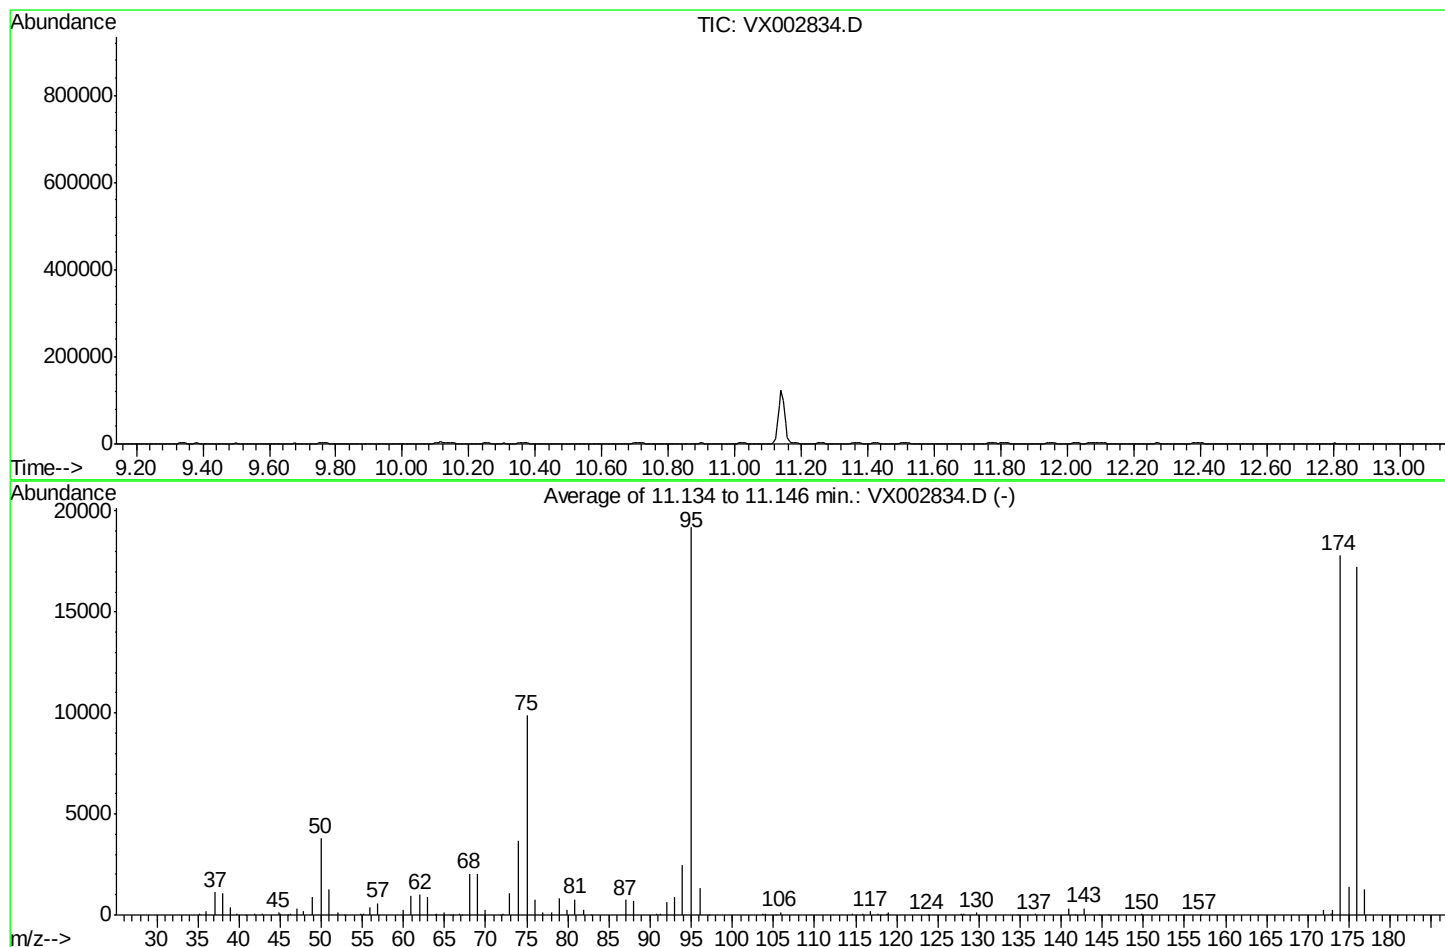

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	3782	PASS
75	95	30	60	51.4	9874	PASS
95	95	100	100	100.0	19192	PASS
96	95	5	9	7.0	1339	PASS
173	174	0.00	2	1.3	225	PASS
174	95	50	100	92.7	17786	PASS
175	174	5	9	7.8	1387	PASS
176	174	95	101	96.8	17222	PASS
177	176	5	9	7.4	1273	PASS