

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
 Data File : VX029726.D
 Acq On : 23 Jun 2022 06:54
 Operator : JC/MD
 Sample : N3334-23 10X
 Misc : 5.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14A-1A-5-GR

Quant Time: Jun 23 07:21:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	289342	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	482046	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	423397	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	191866	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	153755	40.144	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	80.280%		
35) Dibromofluoromethane	5.391	113	137241	43.688	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	87.380%		
50) Toluene-d8	8.653	98	544774	47.470	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	94.940%		
62) 4-Bromofluorobenzene	11.079	95	198197	45.796	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	91.600%		
Target Compounds						Qvalue
5) Bromomethane	1.612	94	574	0.324	ug/l #	58
6) Chloroethane	1.709	64	646	1.524	ug/l #	43
10) Methyl Iodide	2.459	142	462	3.143	ug/l #	79
11) Tert butyl alcohol	2.947	59	14293	8.173	ug/l #	73
16) Acetone	2.386	43	1125	0.737	ug/l #	82
18) Methyl Acetate	2.709	43	2426	0.601	ug/l	90
20) Methylene Chloride	2.794	84	905	0.266	ug/l #	71
25) 2-Butanone	4.587	43	860	0.356	ug/l #	44
36) 1,1-Dichloropropene	5.550	75	20573	4.839	ug/l #	50
38) Carbon Tetrachloride	5.550	117	29621	7.084	ug/l #	15
39) Methylcyclohexane	7.385	83	5394	1.018	ug/l	91
44) Trichloroethene	7.129	130	1156	Below Cal		69
55) 1,1,2-Trichloroethane	9.104	97	3029	0.928	ug/l #	21
59) 2-Hexanone	9.385	43	2968	0.897	ug/l #	20
67) Ethyl Benzene	10.201	91	3622	0.242	ug/l #	88
68) m/p-Xylenes	10.305	106	3769	0.647	ug/l	99
69) o-Xylene	10.647	106	2841	0.493	ug/l	91
73) Isopropylbenzene	10.964	105	9866	0.686	ug/l	95
74) N-amyl acetate	10.860	43	5449	1.091	ug/l #	1
76) 1,2,3-Trichloropropane	11.079	75	93067	22.266	ug/l #	39
78) n-propylbenzene	11.305	91	18573	1.146	ug/l	98
79) 2-Chlorotoluene	11.378	91	3850	0.384	ug/l #	63
80) 1,3,5-Trimethylbenzene	11.451	105	25532	2.107	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	93067	74.073	ug/l #	15
82) 4-Chlorotoluene	11.616	91	3077	0.269	ug/l	75
84) 1,2,4-Trimethylbenzene	11.756	105	66487	5.502	ug/l	100
85) sec-Butylbenzene	11.890	105	16979	1.160	ug/l #	73
86) p-Isopropyltoluene	12.012	119	9907	0.808	ug/l	89
89) n-Butylbenzene	12.335	91	18973	1.834	ug/l #	52
90) Hexachloroethane	12.555	117	1732	0.987	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.963	75	460	0.446	ug/l #	21
95) Naphthalene	13.780	128	42261	3.140	ug/l #	86
96) 1,2,3-Trichlorobenzene	13.975	180	754	0.201	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-1A-5-GR

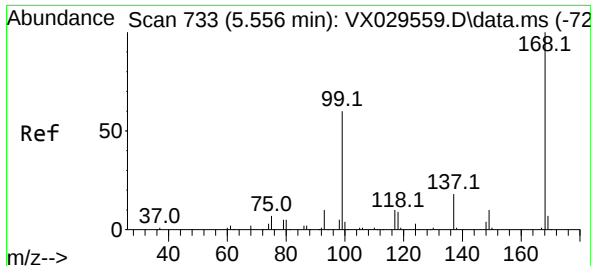

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion:168 Resp: 289342
Ion Ratio Lower Upper
168 100
99 60.2 41.7 62.5

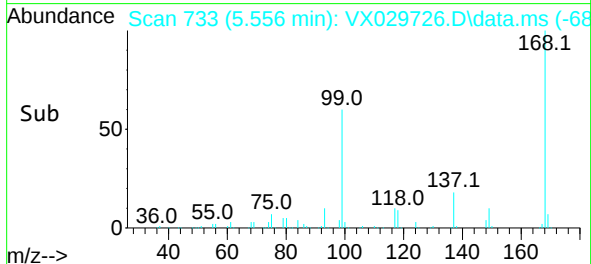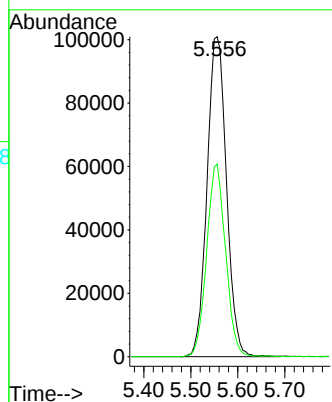

#5
Bromomethane
Concen: 0.324 ug/l
RT: 1.612 min Scan# 86
Delta R.T. 0.001 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 94 Resp: 574
Ion Ratio Lower Upper
94 100
96 53.5 75.3 112.9#




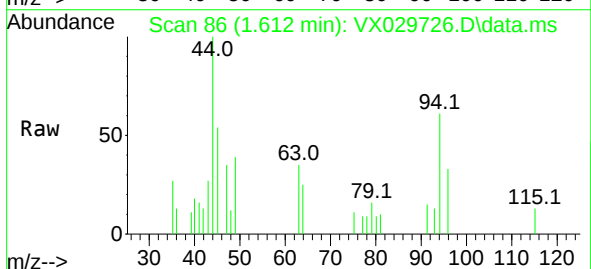


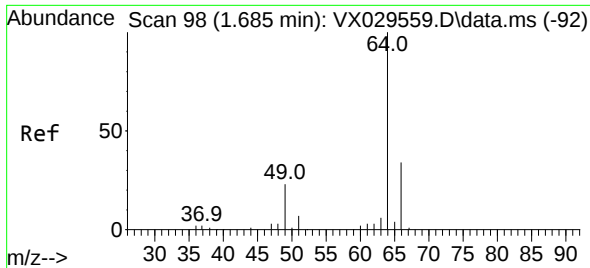

#6
Chloroethane
Concen: 1.524 ug/l
RT: 1.709 min Scan# 102
Delta R.T. 0.024 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 64 Resp: 646
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#

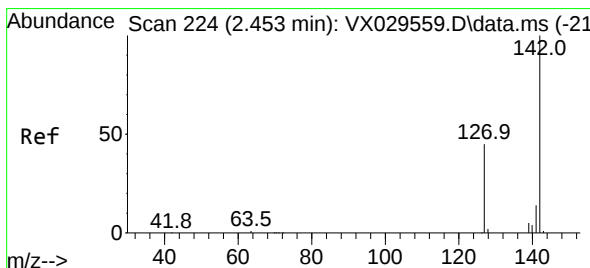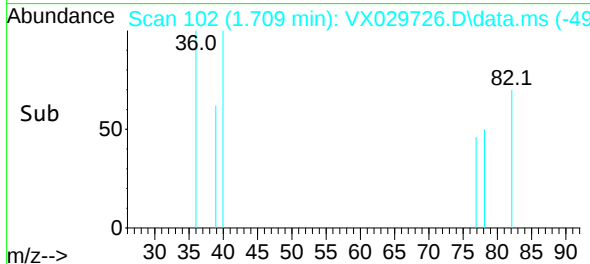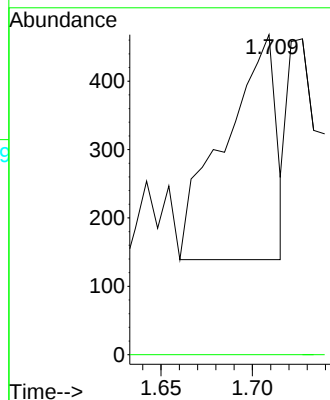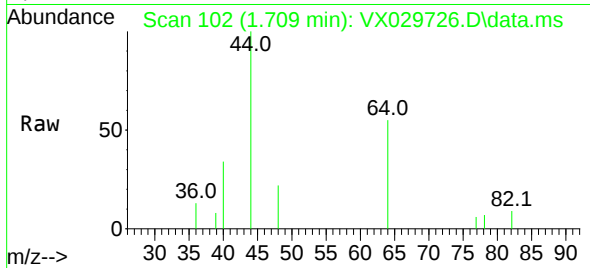

#10
Methyl Iodide
Concen: 3.143 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 142 Resp: 462
Ion Ratio Lower Upper
142 100
127 31.8 33.9 50.9#
141 0.0 11.4 17.2#

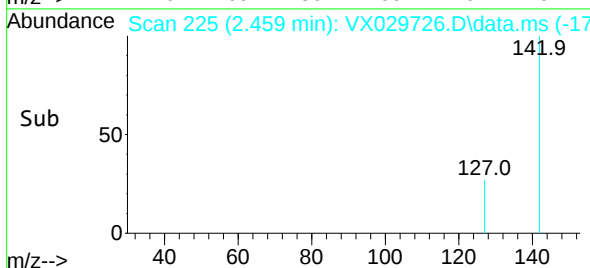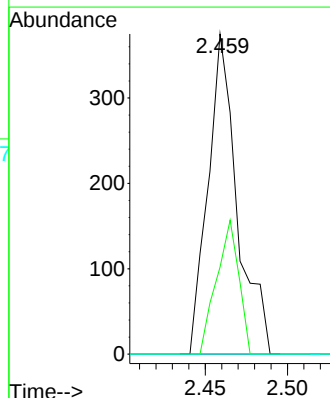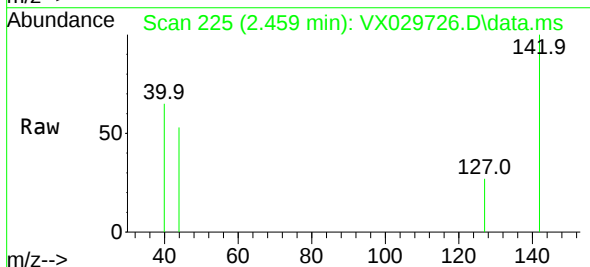

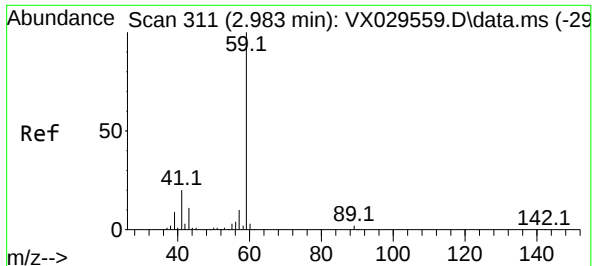

#11

Tert butyl alcohol

Concen: 8.173 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.036 min

Lab File: VX029726.D

Acq: 23 Jun 2022 06:54

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-1A-5-GR

Tgt Ion: 59 Resp: 14293

Ion Ratio Lower Upper

59 100

57 0.5 8.3 12.5#

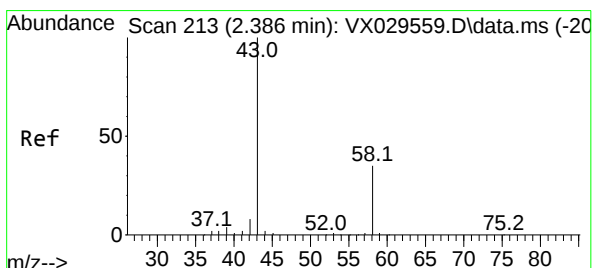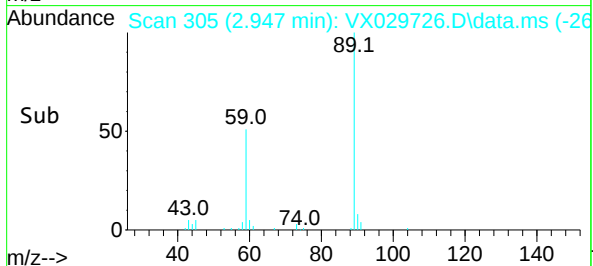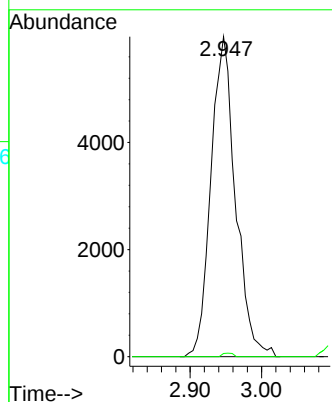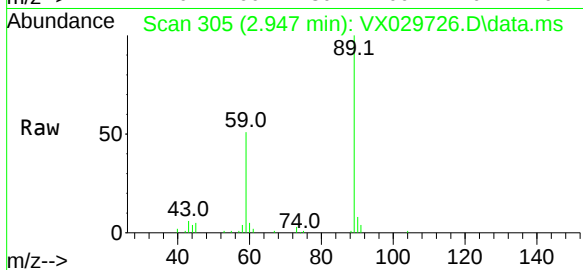

#16

Acetone

Concen: 0.737 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX029726.D




Acq: 23 Jun 2022 06:54


Tgt Ion: 43 Resp: 1125

Ion Ratio Lower Upper

43 100

58 25.3 28.8 43.2#


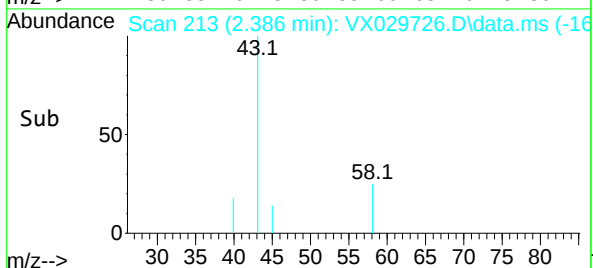

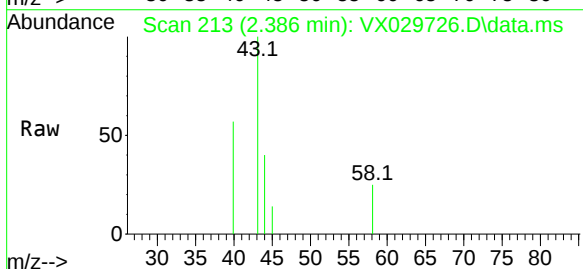


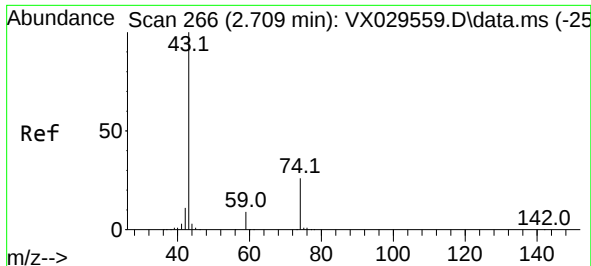

#18
Methyl Acetate
Concen: 0.601 ug/l
RT: 2.709 min Scan# 218
Delta R.T. -0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 43 Resp: 2426
Ion Ratio Lower Upper
43 100
74 23.0 22.8 34.2

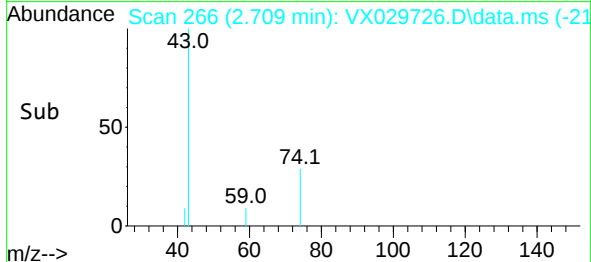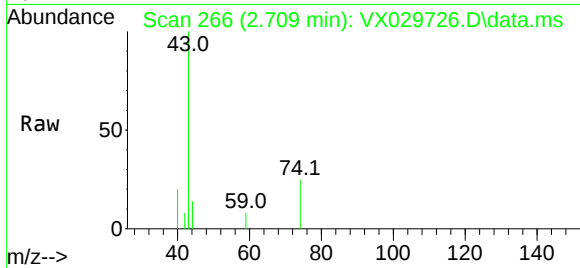

#20
Methylene Chloride
Concen: 0.266 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 84 Resp: 905
Ion Ratio Lower Upper
84 100
49 80.2 85.5 128.3#
51 22.1 26.6 39.8#
86 33.7 51.5 77.3#

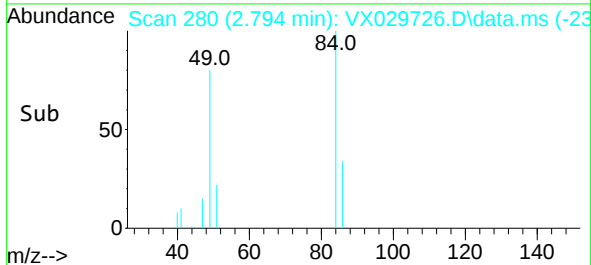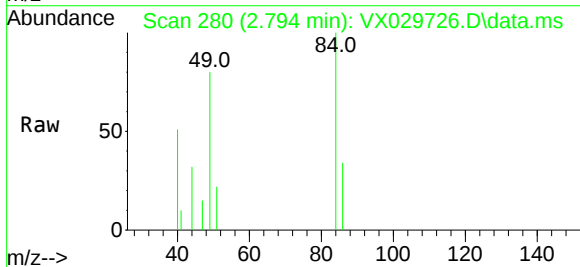

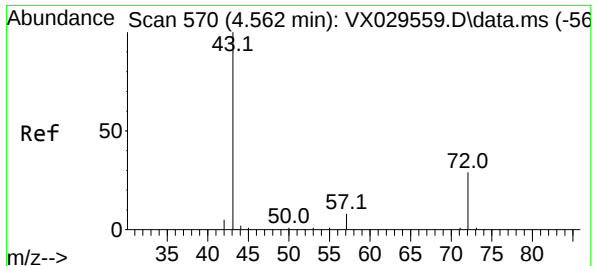

#25

2-Butanone

Concen: 0.356 ug/l

RT: 4.587 min Scan# 51

Delta R.T. 0.025 min

Lab File: VX029726.D

Acq: 23 Jun 2022 06:54

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-1A-5-GR

Tgt Ion: 43 Resp: 860

Ion Ratio Lower Upper

43 100

72 0.0 24.4 36.6#

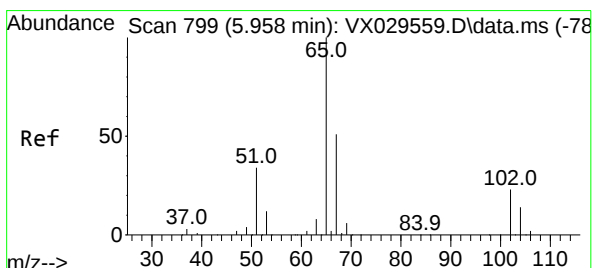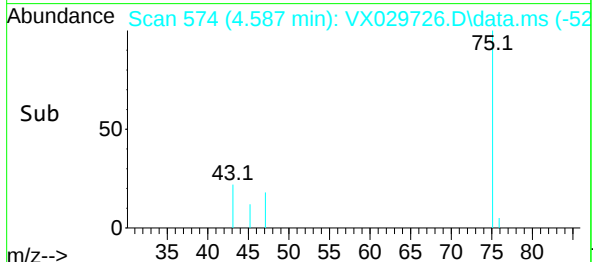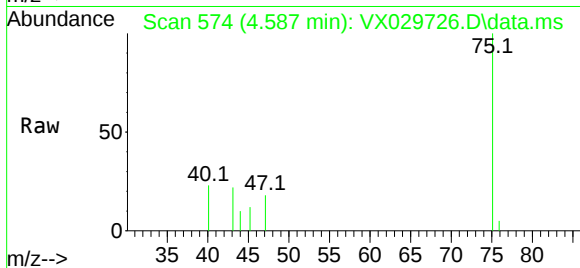

#33

1,2-Dichloroethane-d4

Concen: 40.144 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029726.D




Acq: 23 Jun 2022 06:54


Tgt Ion: 65 Resp: 153755

Ion Ratio Lower Upper

65 100

67 53.8 0.0 107.4


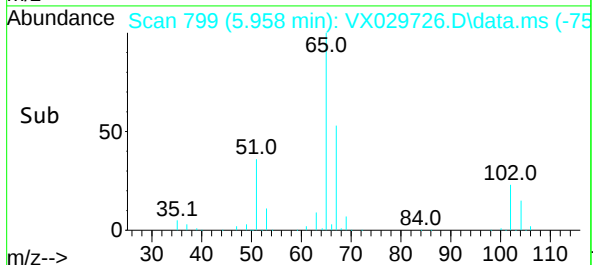

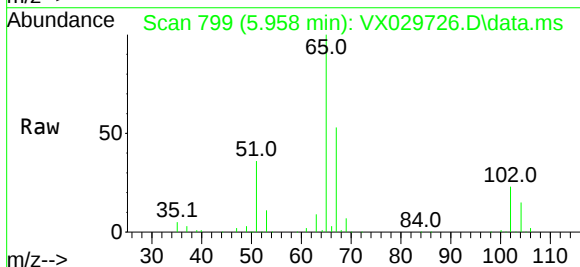


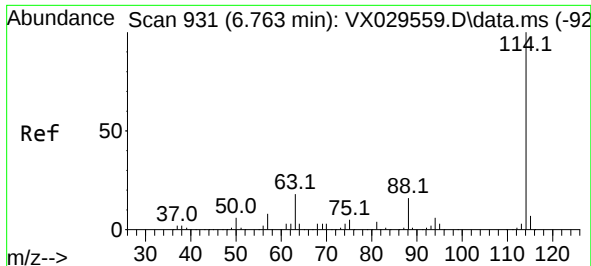

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion:114 Resp: 482046
Ion Ratio Lower Upper
114 100
63 18.4 0.0 36.8
88 15.7 0.0 32.4

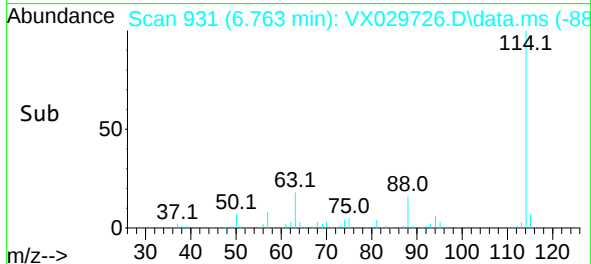

#35
Dibromofluoromethane
Concen: 43.688 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion:113 Resp: 137241
Ion Ratio Lower Upper
113 100
111 102.4 82.8 124.2
192 19.6 16.9 25.3


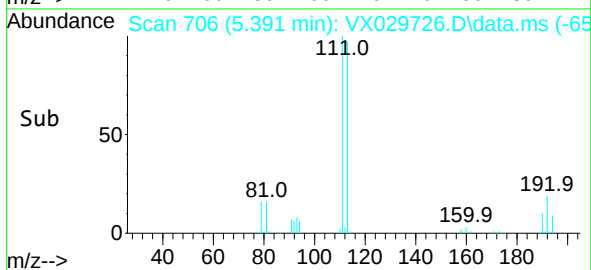

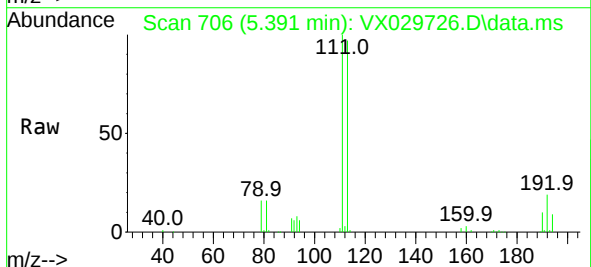


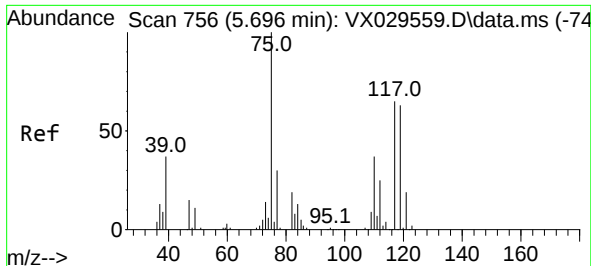

#36
1,1-Dichloropropene
Concen: 4.839 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.146 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 75 Resp: 20573
Ion Ratio Lower Upper
75 100
110 9.7 18.3 54.8#
77 0.0 24.8 37.2#

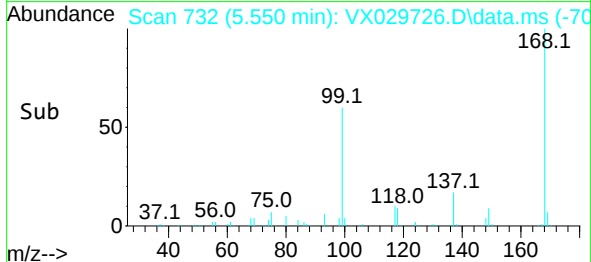

#38
Carbon Tetrachloride
Concen: 7.084 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 117 Resp: 29621
Ion Ratio Lower Upper
117 100
119 4.5 77.3 115.9#
121 0.0 24.2 36.2#


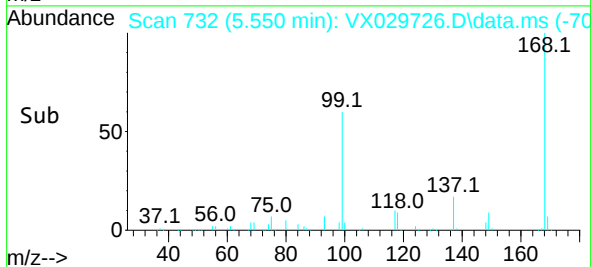

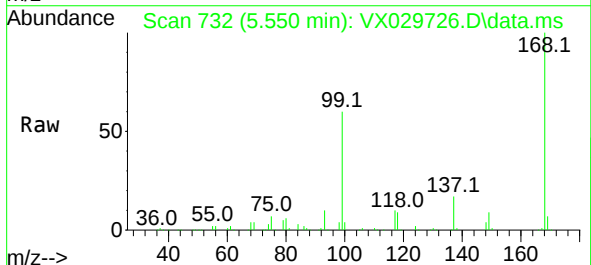


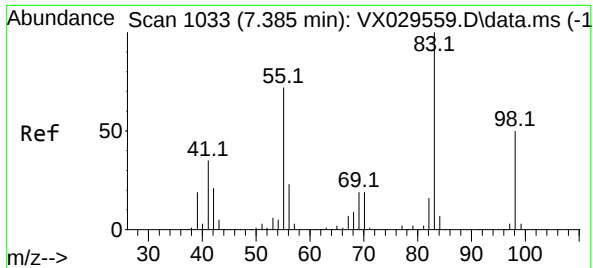

#39
Methylcyclohexane
Concen: 1.018 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 83 Resp: 5394
Ion Ratio Lower Upper
83 100
55 56.0 54.6 81.8
98 47.5 37.4 56.2

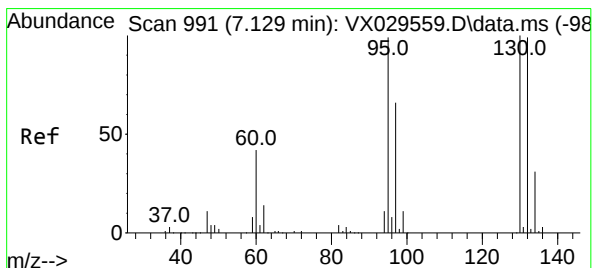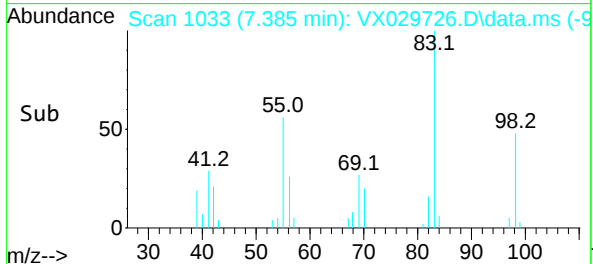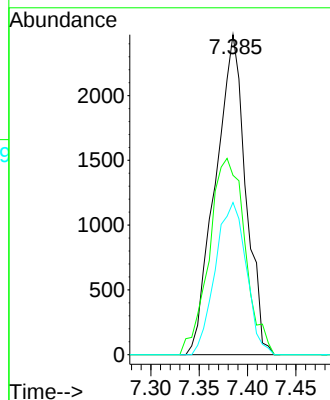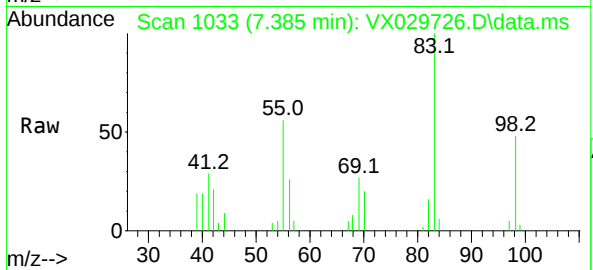

#44
Trichloroethene
Concen: Below Cal
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion:130 Resp: 1156
Ion Ratio Lower Upper
130 100
95 64.3 0.0 188.8


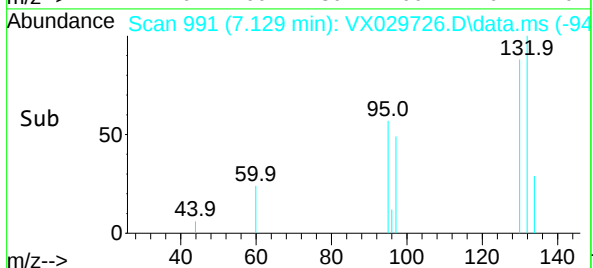
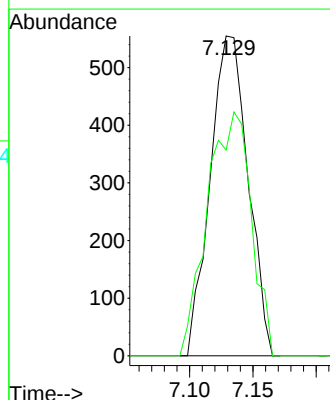
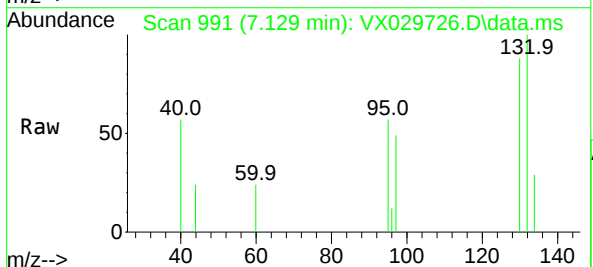


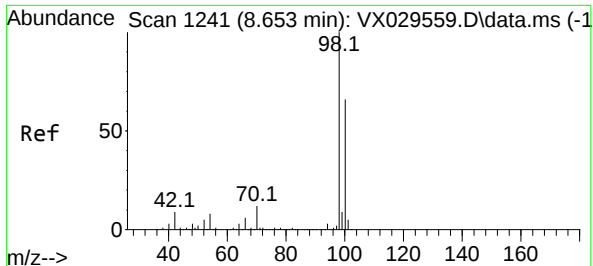

#50
Toluene-d8
Concen: 47.470 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 98 Resp: 544774
Ion Ratio Lower Upper
98 100
100 67.3 52.6 78.8

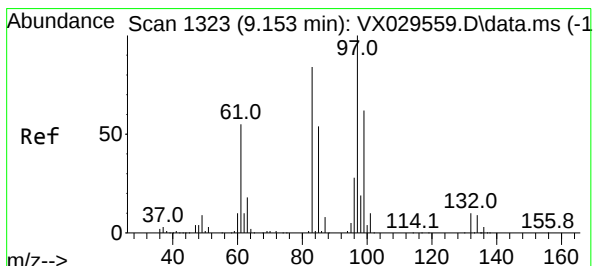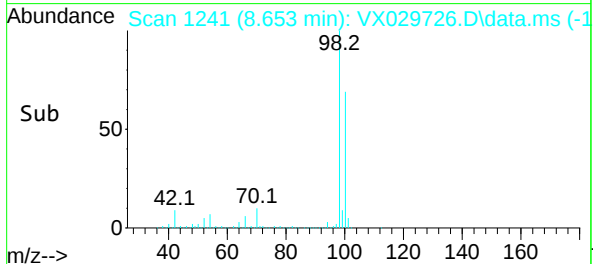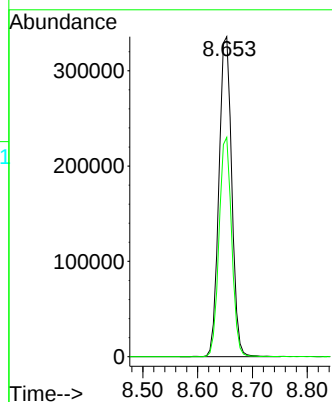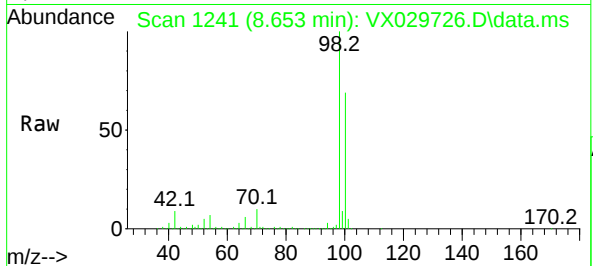

#55
1,1,2-Trichloroethane
Concen: 0.928 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 97 Resp: 3029
Ion Ratio Lower Upper
97 100
83 9.8 66.2 99.4#
85 0.0 42.9 64.3#
99 0.0 49.0 73.6#

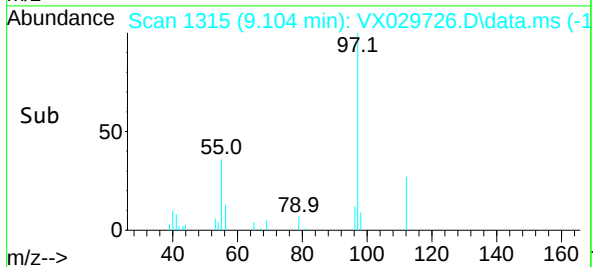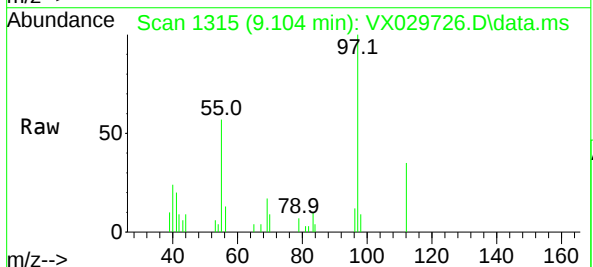

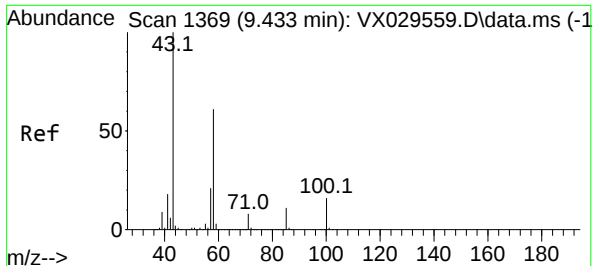

#59

2-Hexanone

Concen: 0.897 ug/l

RT: 9.385 min Scan# 1

Delta R.T. -0.048 min

Lab File: VX029726.D

Acq: 23 Jun 2022 06:54

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-1A-5-GR

Tgt Ion: 43 Resp: 2968

Ion Ratio Lower Upper

43 100

58 1.7 31.9 95.7#

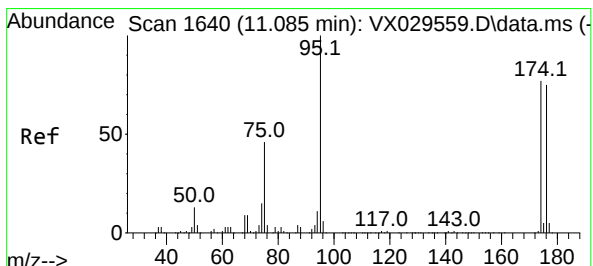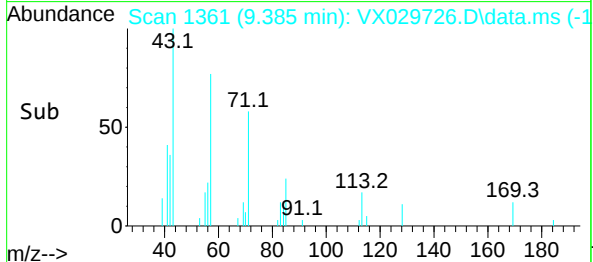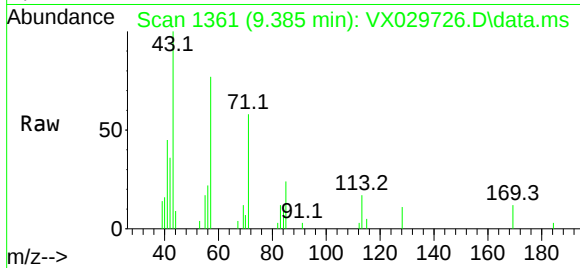

#62

4-Bromofluorobenzene

Concen: 45.796 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX029726.D

Acq: 23 Jun 2022 06:54




Tgt Ion: 95 Resp: 198197


Ion Ratio Lower Upper

95 100

174 73.7 0.0 163.0

176 71.0 0.0 155.0


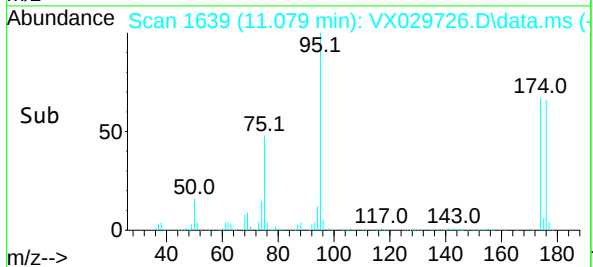

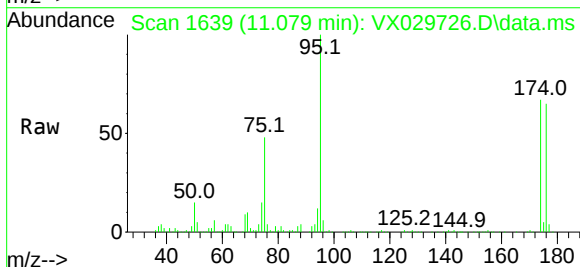




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion:117 Resp: 423397
Ion Ratio Lower Upper
117 100
82 54.7 41.8 62.8
119 32.7 24.8 37.2

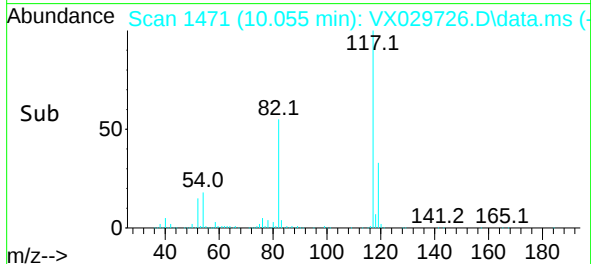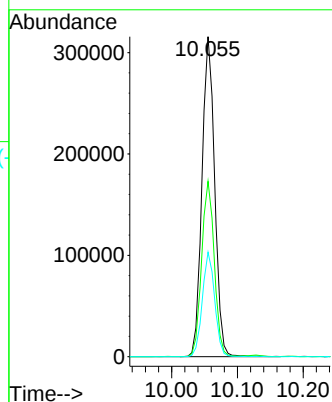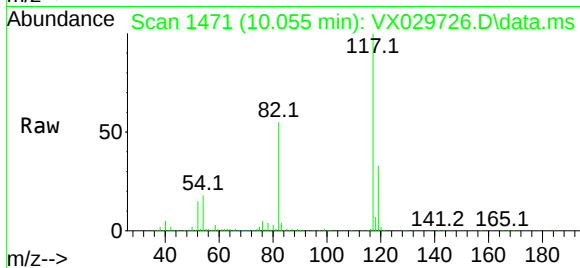

#67
Ethyl Benzene
Concen: 0.242 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 91 Resp: 3622
Ion Ratio Lower Upper
91 100
106 24.3 24.6 36.8#




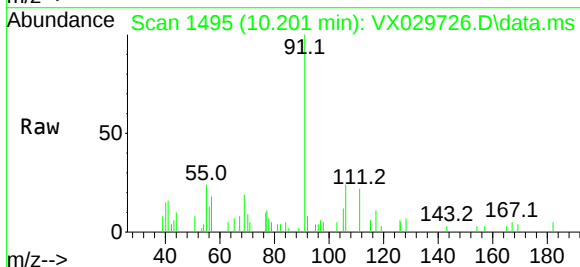


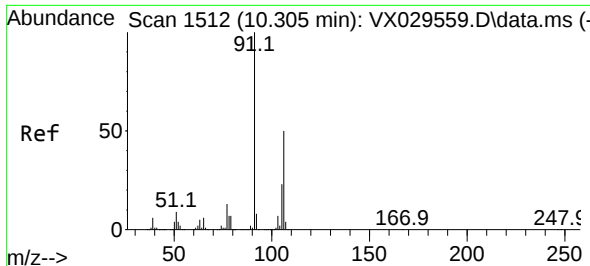

#68
m/p-Xylenes
Concen: 0.647 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion:106 Resp: 3769
Ion Ratio Lower Upper
106 100
91 201.9 160.4 240.6

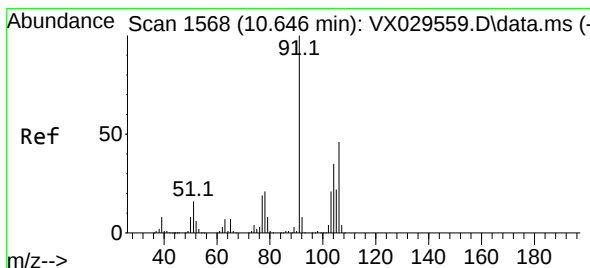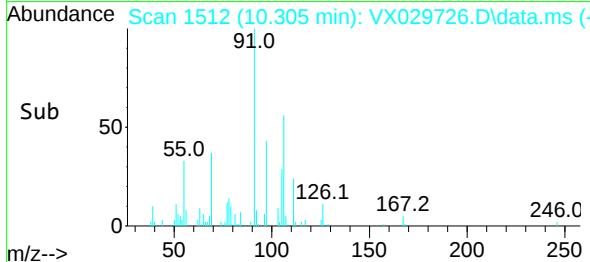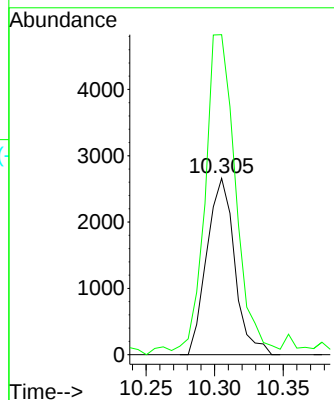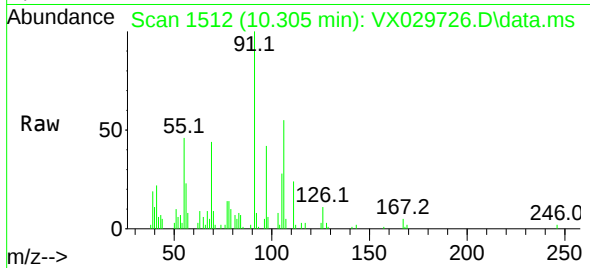

#69
o-Xylene
Concen: 0.493 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.001 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion:106 Resp: 2841
Ion Ratio Lower Upper
106 100
91 198.7 106.1 318.1


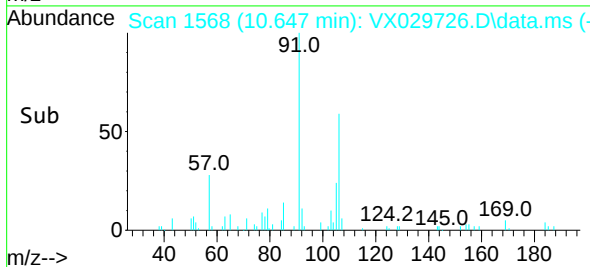
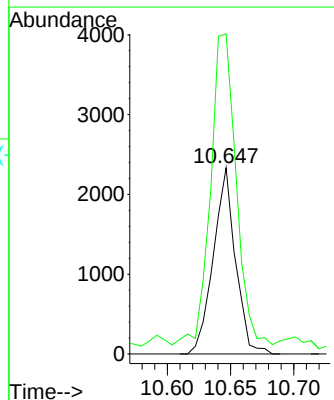
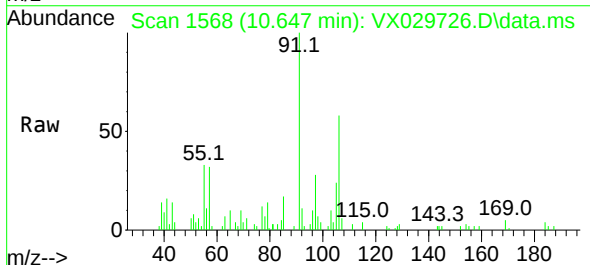




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion:152 Resp: 191866
Ion Ratio Lower Upper
152 100
115 61.1 37.5 112.7
150 157.0 0.0 338.2

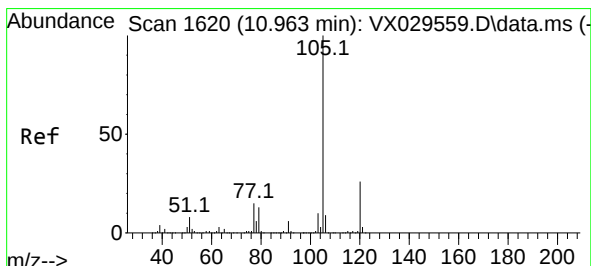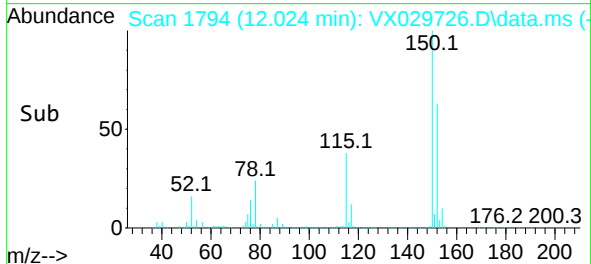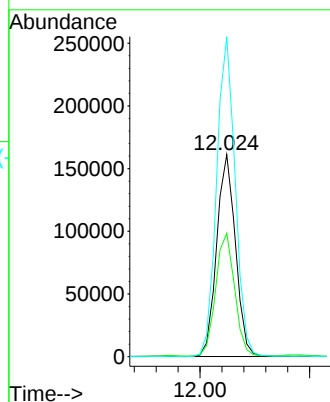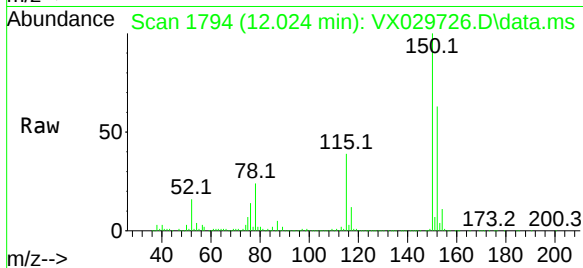

#73
Isopropylbenzene
Concen: 0.686 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion:105 Resp: 9866
Ion Ratio Lower Upper
105 100
120 29.4 13.5 40.5


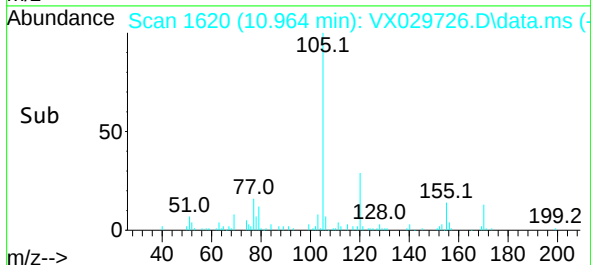
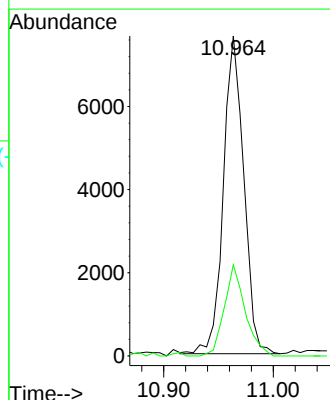
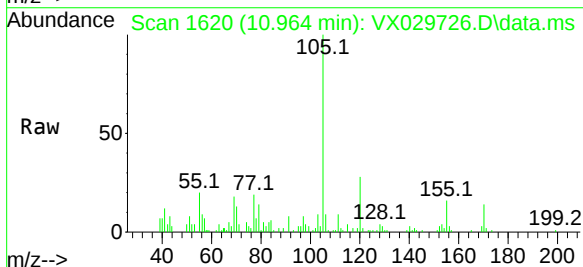


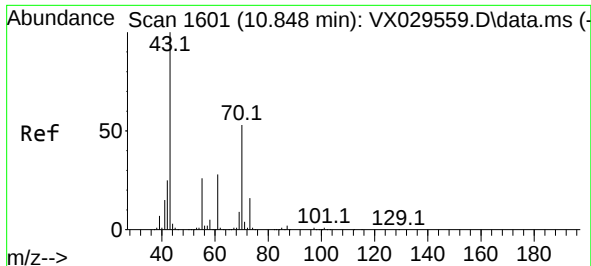

#74
N-amy1 acetate
Concen: 1.091 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.012 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 43 Resp: 5449
Ion Ratio Lower Upper
43 100
70 87.9 42.5 63.7#
55 338.7 23.1 34.7#
61 0.0 22.8 34.2#

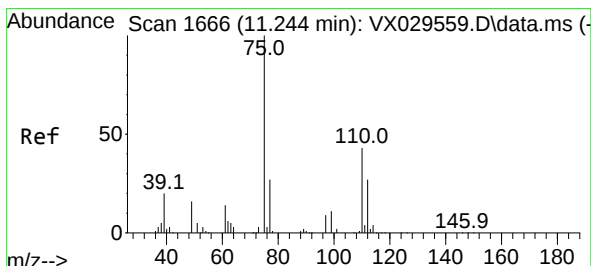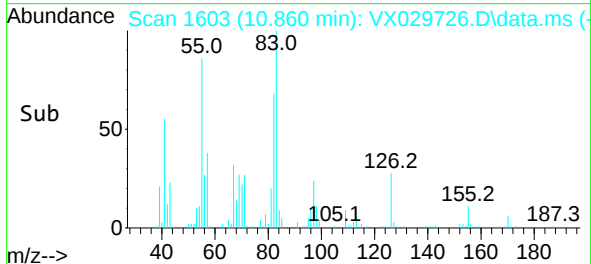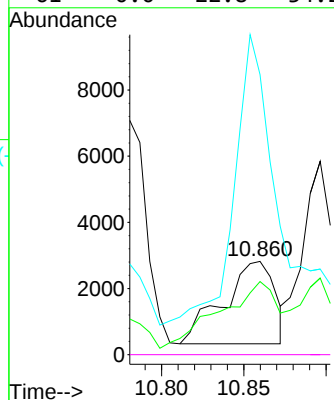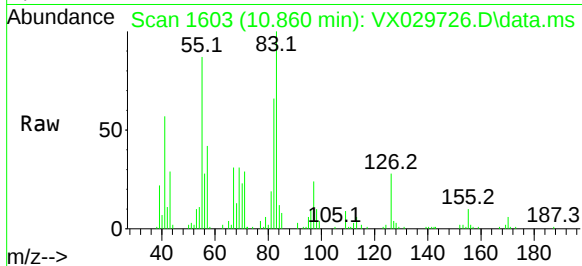

#76
1,2,3-Trichloropropane
Concen: 22.266 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 75 Resp: 93067
Ion Ratio Lower Upper
75 100
77 1.6 19.4 58.2#


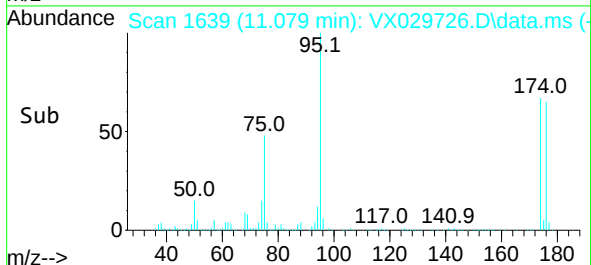
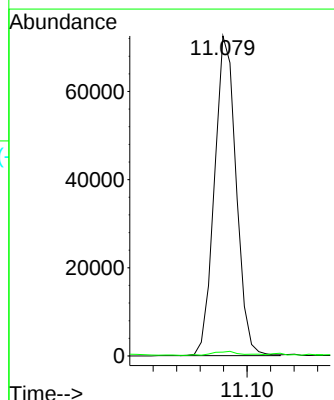
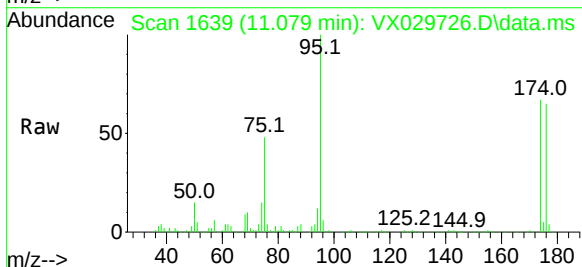


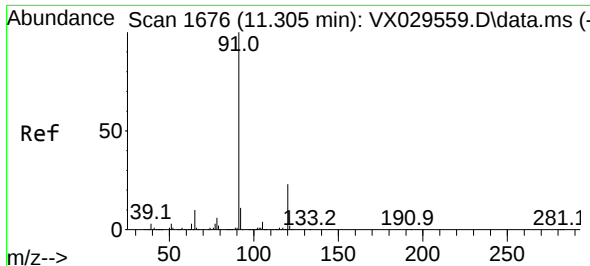

#78
n-propylbenzene
Concen: 1.146 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 91 Resp: 18573
Ion Ratio Lower Upper
91 100
120 22.2 11.6 34.8

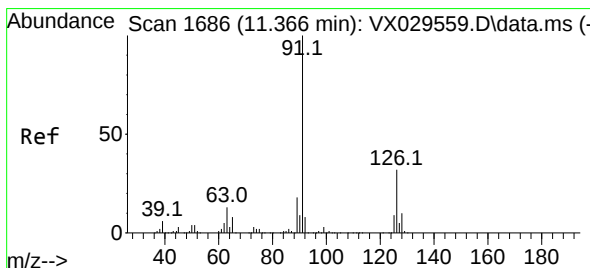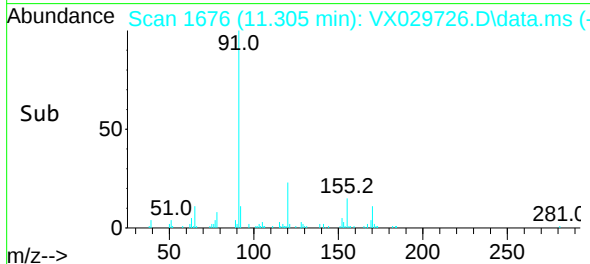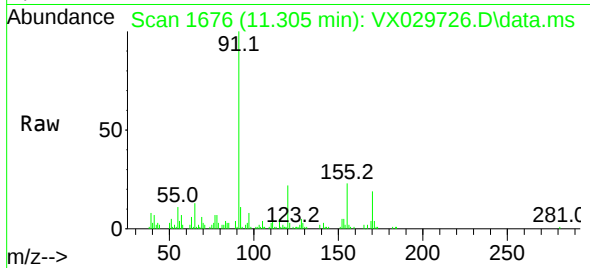

#79
2-Chlorotoluene
Concen: 0.384 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 91 Resp: 3850
Ion Ratio Lower Upper
91 100
126 13.0 17.3 51.9#

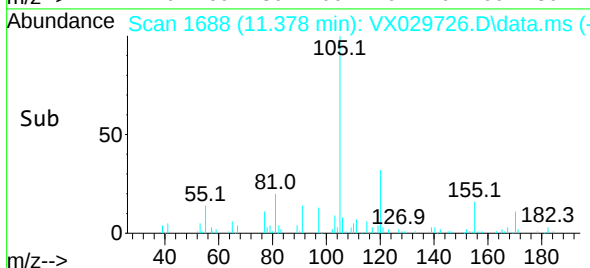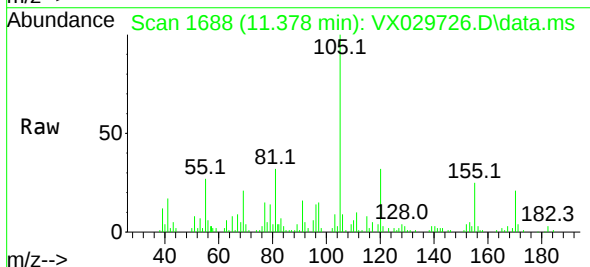



#80

1,3,5-Trimethylbenzene

Concen: 2.107 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX029726.D

Acq: 23 Jun 2022 06:54

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-1A-5-GR

Tgt Ion:105 Resp: 25532

Ion Ratio Lower Upper

105 100

120 48.8 24.3 72.9

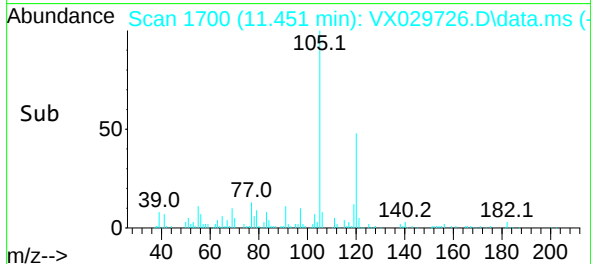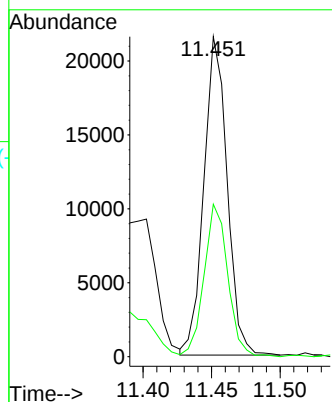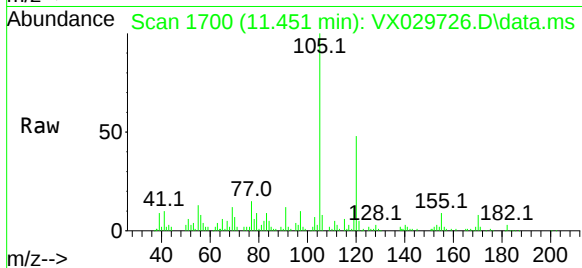

#81

trans-1,4-Dichloro-2-butene

Concen: 74.073 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX029726.D

Acq: 23 Jun 2022 06:54




Tgt Ion: 75 Resp: 93067


Ion Ratio Lower Upper

75 100

53 0.5 69.0 103.4#

89 0.1 37.0 55.6#


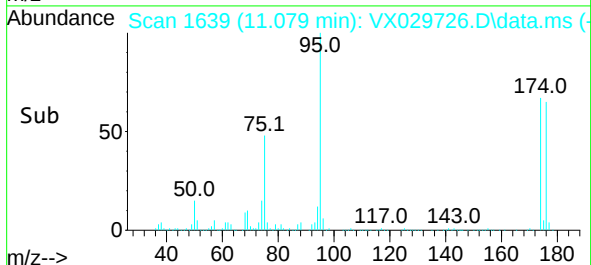

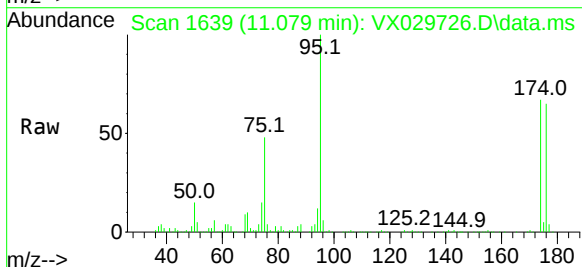


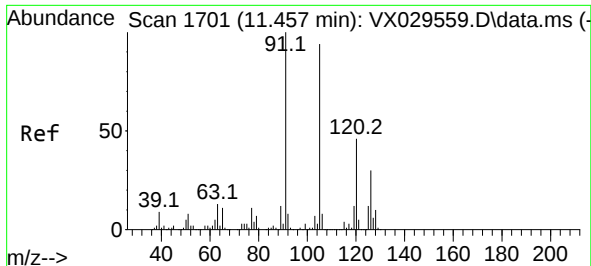

#82
4-Chlorotoluene
Concen: 0.269 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.159 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 91 Resp: 3077
Ion Ratio Lower Upper
91 100
126 16.3 14.9 44.5

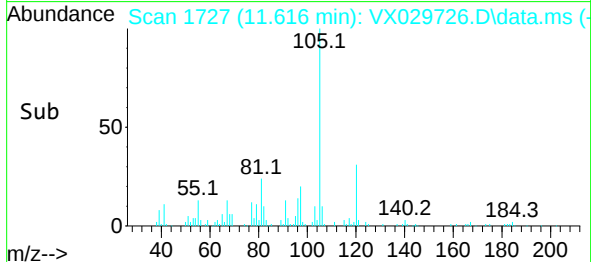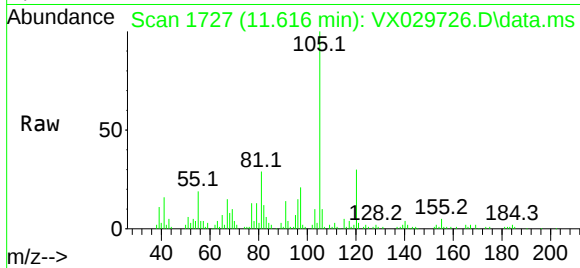

#84
1,2,4-Trimethylbenzene
Concen: 5.502 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 105 Resp: 66487
Ion Ratio Lower Upper
105 100
120 45.3 22.6 67.8


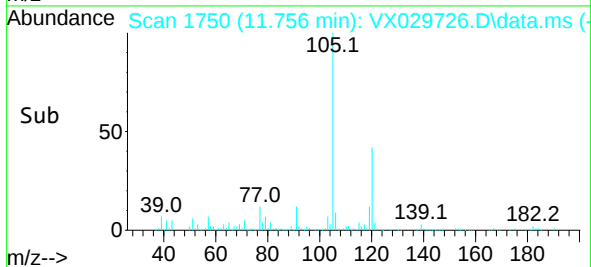

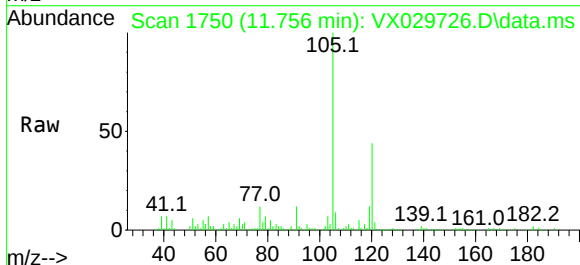




#85
 sec-Butylbenzene
 Concen: 1.160 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX029726.D
 Acq: 23 Jun 2022 06:54




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14A-1A-5-GR


Tgt Ion:105 Resp: 16979
 Ion Ratio Lower Upper
 105 100
 134 33.0 10.2 30.4#

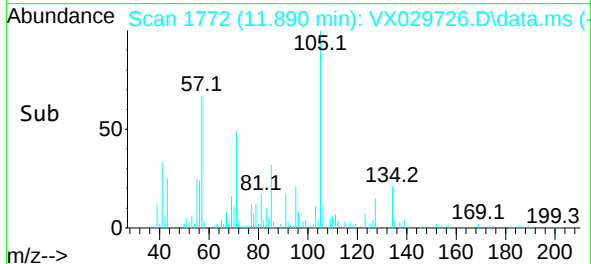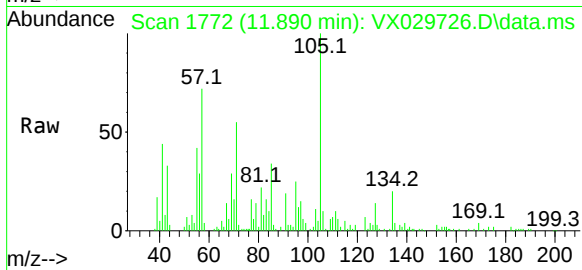

#86
 p-Isopropyltoluene
 Concen: 0.808 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX029726.D
 Acq: 23 Jun 2022 06:54

Tgt Ion:119 Resp: 9907
 Ion Ratio Lower Upper
 119 100
 134 28.9 13.0 39.0
 91 30.8 11.3 33.9


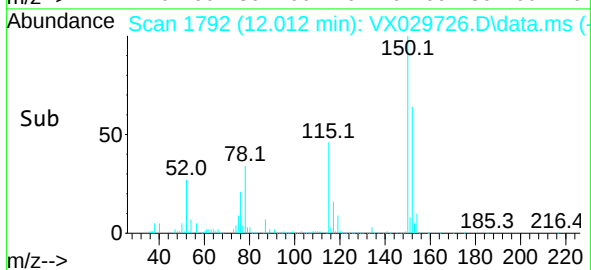

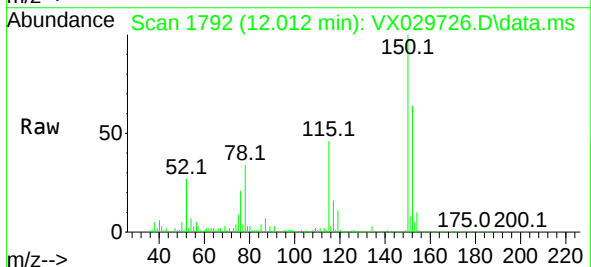




#89
n-Butylbenzene
Concen: 1.834 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 91 Resp: 18973
Ion Ratio Lower Upper
91 100
92 41.9 27.8 83.3
134 82.5 13.3 39.8#

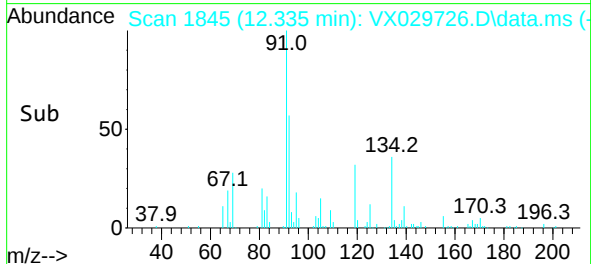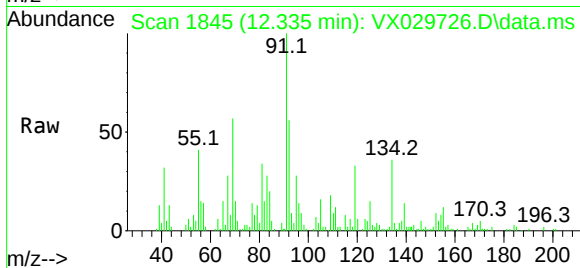

#90
Hexachloroethane
Concen: 0.987 ug/l
RT: 12.555 min Scan# 1881
Delta R.T. 0.013 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 117 Resp: 1732
Ion Ratio Lower Upper
117 100
201 5.9 39.5 118.5#


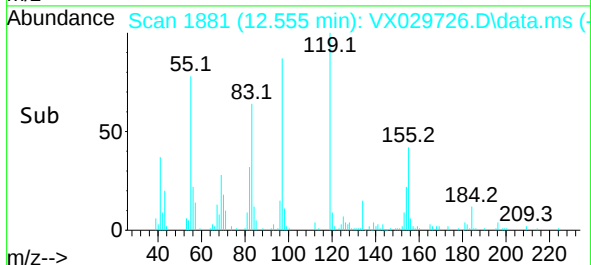

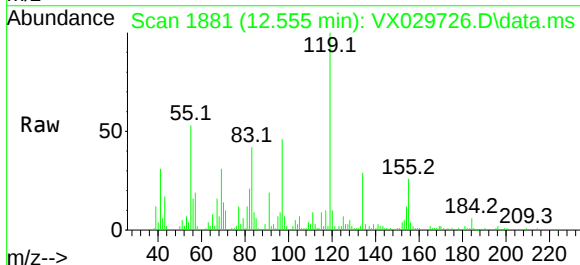


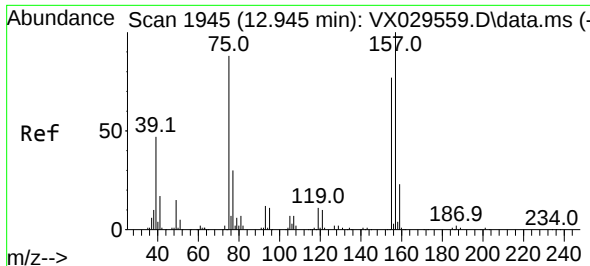

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.446 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5-GR


Tgt Ion: 75 Resp: 460
Ion Ratio Lower Upper
75 100
155 0.0 47.0 141.2#
157 46.3 57.9 173.6#

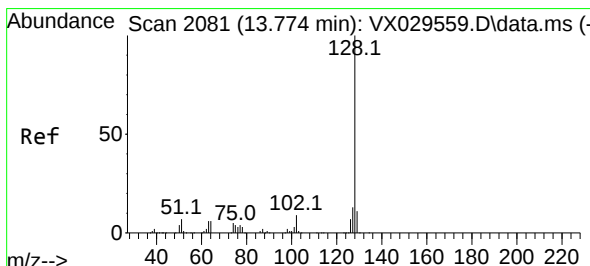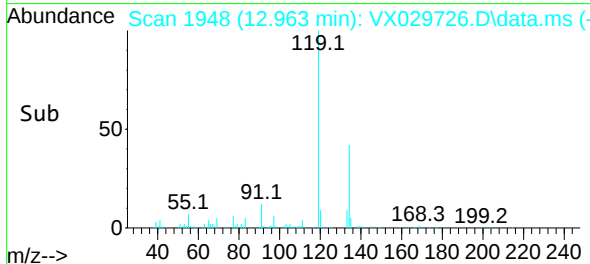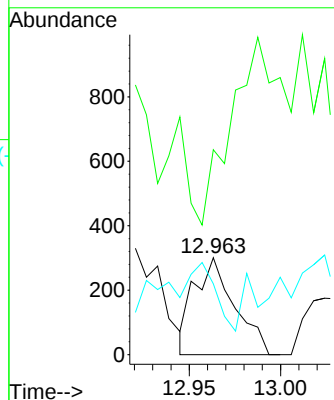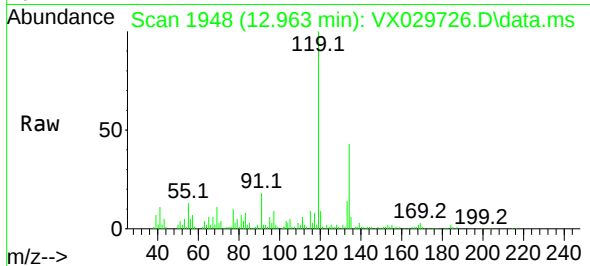

#95
Naphthalene
Concen: 3.140 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX029726.D
Acq: 23 Jun 2022 06:54

Tgt Ion: 128 Resp: 42261
Ion Ratio Lower Upper
128 100
127 14.5 10.2 15.4
129 20.9 8.7 13.1#

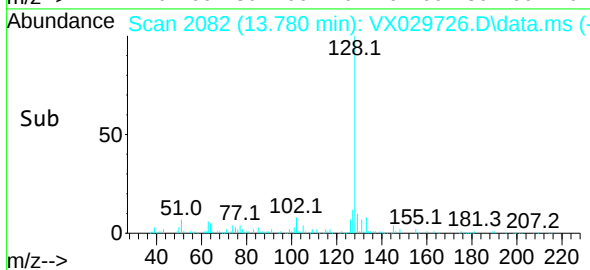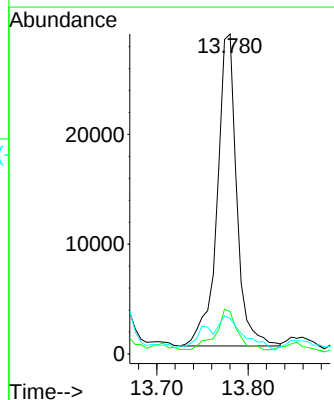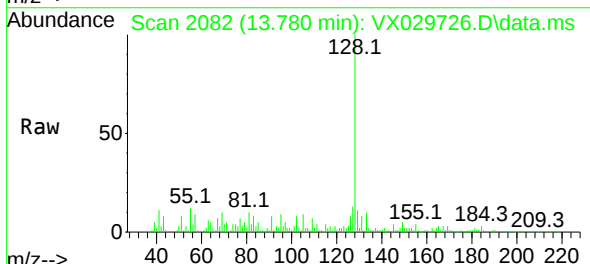



#96

1,2,3-Trichlorobenzene

Concen: 0.201 ug/l

RT: 13.975 min Scan# 21

Delta R.T. 0.012 min

Lab File: VX029726.D


Acq: 23 Jun 2022 06:54

Instrument :

MSVOA_X

ClientSampleId :

WC-14A-1A-5-GR

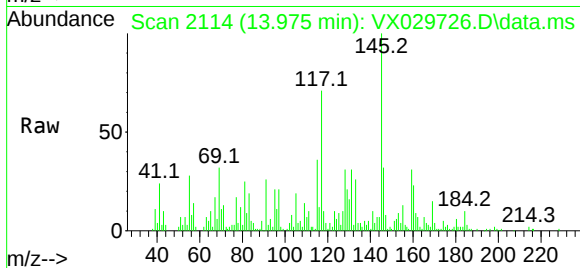

Tgt Ion:180 Resp: 754

Ion Ratio Lower Upper

180 100

182 0.0 50.0 149.8#

145 2380.2 16.2 48.5#

