

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
 Data File : VX029687.D
 Acq On : 22 Jun 2022 10:19
 Operator : JC/MD
 Sample : VX0622WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0622WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	26	35	43	rBV4	7206	20405	1.54%	0.289%
2	2.953	297	306	315	rVB	12340	29390	2.21%	0.416%
3	4.574	562	572	582	rBV2	4074	13509	1.02%	0.191%
4	5.391	693	706	720	rBV	152166	438833	33.04%	6.214%
5	5.556	722	733	749	rVB	283767	790646	59.52%	11.196%
6	5.958	788	799	819	rBV	155593	421457	31.73%	5.968%
7	6.763	921	931	947	rBV	426435	1010534	76.08%	14.310%
8	8.653	1233	1241	1251	rBV	846855	1328270	100.00%	18.809%
9	10.055	1465	1471	1485	rBV	853063	1137711	85.65%	16.111%
10	11.085	1634	1640	1653	rBV	627699	830979	62.56%	11.767%
11	12.024	1788	1794	1802	rBV	851102	1040006	78.30%	14.727%




Sum of corrected areas: 7061740

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029687.D
Acq On : 22 Jun 2022 10:19
Operator : JC/MD
Sample : VX0622WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0622WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

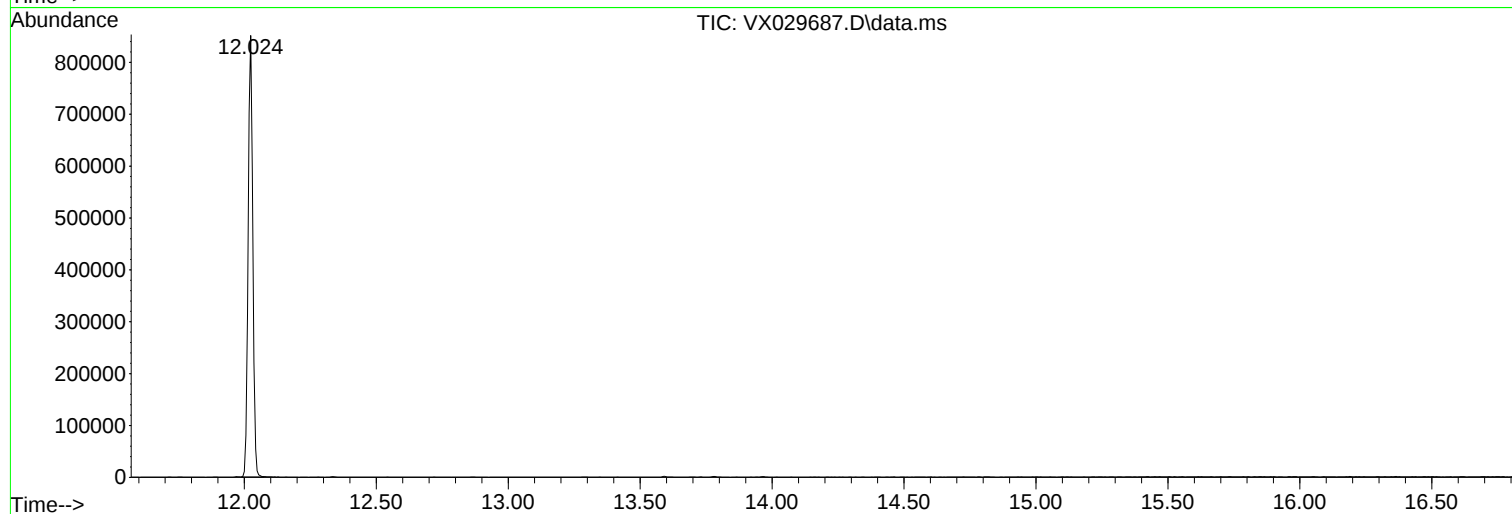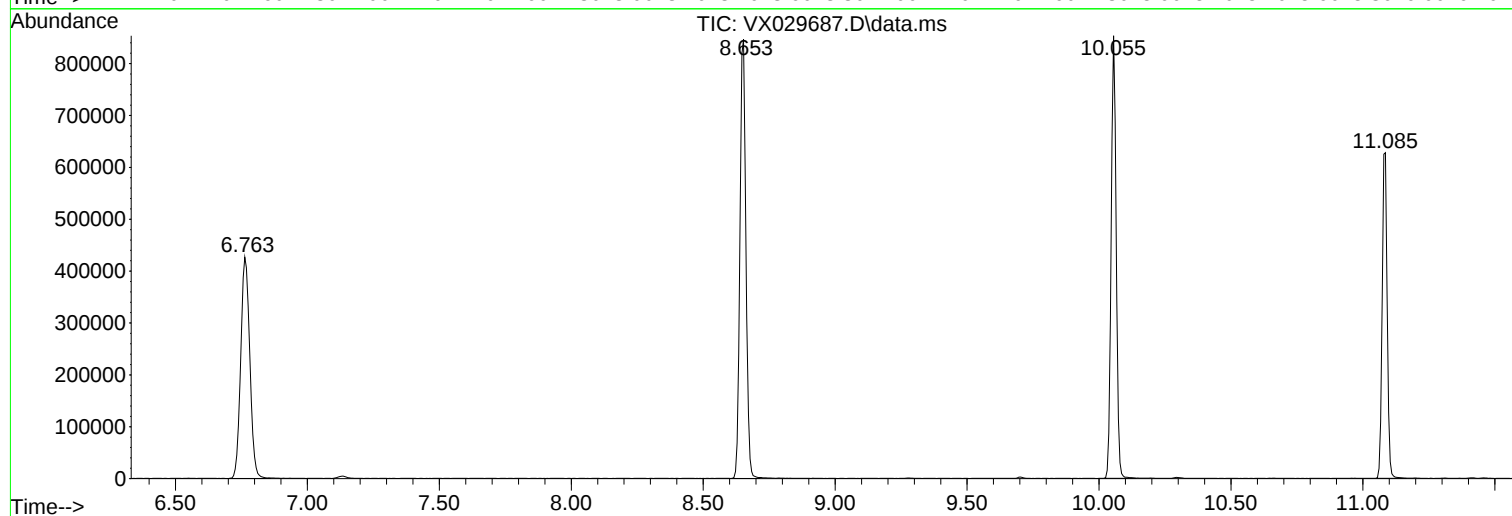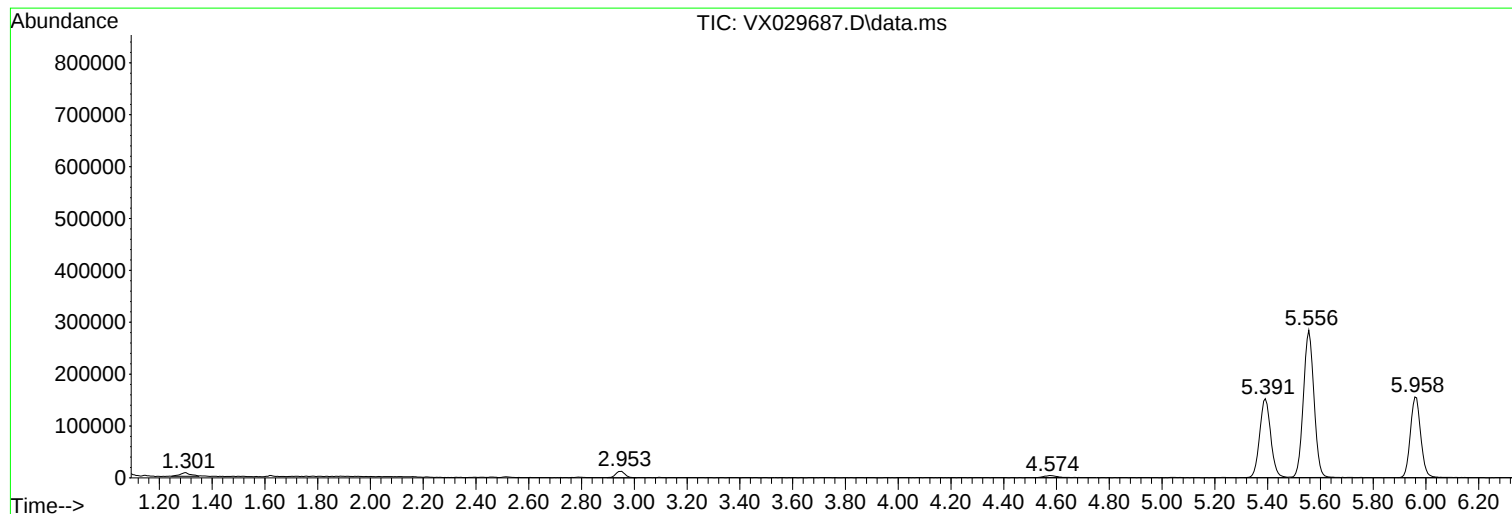

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029687.D
Acq On : 22 Jun 2022 10:19
Operator : JC/MD
Sample : VX0622WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0622WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029687.D
Acq On : 22 Jun 2022 10:19
Operator : JC/MD
Sample : VX0622WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0622WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc