

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
 Data File : VX029706.D
 Acq On : 22 Jun 2022 17:57
 Operator : JC/MD
 Sample : N3202-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	24	29	43	rBV	76697	211453	1.82%	0.259%
2	2.782	270	278	281	rBV	68560	145180	1.25%	0.178%
3	2.825	281	285	296	rVB	173418	352976	3.05%	0.432%
4	3.105	321	331	347	rVB	172552	396309	3.42%	0.485%
5	3.446	379	387	398	rVB2	69927	155692	1.34%	0.190%
6	4.306	519	528	541	rVB	247771	699926	6.04%	0.856%
7	5.391	689	706	713	rBV2	146840	458380	3.95%	0.561%
8	5.483	713	721	726	rBV3	83716	275940	2.38%	0.338%
9	5.556	726	733	740	rBV2	184326	454867	3.92%	0.556%
10	5.830	766	778	790	rBV3	114716	346791	2.99%	0.424%
11	5.958	790	799	808	rBV	144783	372486	3.21%	0.456%
12	6.159	819	832	839	rBV2	100072	327923	2.83%	0.401%
13	6.257	840	848	857	rVV3	211695	650610	5.61%	0.796%
14	6.361	857	865	877	rVB3	98876	279428	2.41%	0.342%
15	6.763	921	931	939	rBV	394385	965225	8.33%	1.181%
16	6.848	939	945	957	rVB2	87544	239855	2.07%	0.293%
17	7.177	992	999	1006	rVB2	56576	124535	1.07%	0.152%
18	7.379	1019	1032	1043	rBV3	490792	1337936	11.54%	1.637%
19	7.659	1072	1078	1091	rVB	116154	238864	2.06%	0.292%
20	7.885	1112	1115	1123	rVB3	75214	146895	1.27%	0.180%
21	7.988	1123	1132	1143	rVB	141268	317103	2.74%	0.388%
22	8.110	1143	1152	1155	rBV	312186	630187	5.44%	0.771%
23	8.141	1155	1157	1163	rVB	186941	288274	2.49%	0.353%
24	8.507	1210	1217	1226	rVB3	122669	251306	2.17%	0.307%
25	8.604	1226	1233	1236	rBV3	89950	179324	1.55%	0.219%
26	8.653	1236	1241	1249	rVB	807901	1271676	10.97%	1.556%
27	8.927	1281	1286	1290	rBV	79546	116569	1.01%	0.143%
28	9.104	1307	1315	1320	rBV	90187	167812	1.45%	0.205%
29	9.165	1320	1325	1335	rVB	172667	286971	2.48%	0.351%
30	9.458	1365	1373	1377	rBV4	54394	139990	1.21%	0.171%
31	10.055	1467	1471	1476	rVB	751458	994793	8.58%	1.217%
32	10.146	1481	1486	1490	rVV2	130949	210182	1.81%	0.257%
33	10.195	1490	1494	1499	rVV	699683	883110	7.62%	1.080%
34	10.305	1505	1512	1517	rVB	388574	529186	4.57%	0.647%
35	10.646	1563	1568	1572	rBV	110594	142279	1.23%	0.174%
36	10.963	1613	1620	1626	rBV	1801146	2202034	19.00%	2.694%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
 Data File : VX029706.D
 Acq On : 22 Jun 2022 17:57
 Operator : JC/MD
 Sample : N3202-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

37	11.085	1635	1640	1644	rBV	562896	714037	6.16%	0.874%
38	11.305	1672	1676	1683	rVB	1993211	2454562	21.17%	3.003%
39	11.384	1683	1689	1690	rVV	1492643	1938159	16.72%	2.371%
40	11.402	1690	1692	1696	rVV	1416237	1493895	12.89%	1.828%
41	11.451	1696	1700	1710	rVB	3877960	4821354	41.59%	5.899%
42	11.616	1721	1727	1735	rBV	2086922	2549419	21.99%	3.119%
43	11.756	1744	1750	1755	rBV	9377279	11591955	100.00%	14.182%
44	11.866	1763	1768	1770	rBV	105194	137988	1.19%	0.169%
45	11.890	1770	1772	1779	rVB	162642	194169	1.68%	0.238%
46	11.975	1781	1786	1789	rVV	239315	304045	2.62%	0.372%
47	12.024	1789	1794	1799	rVB2	791907	1023050	8.83%	1.252%
48	12.091	1799	1805	1816	rBV	4341790	5502085	47.46%	6.731%
49	12.244	1824	1830	1838	rBV3	2932018	4391657	37.89%	5.373%
50	12.317	1838	1842	1852	rVB2	1519111	2208557	19.05%	2.702%
51	12.408	1852	1857	1861	rBV3	218602	273852	2.36%	0.335%
52	12.463	1861	1866	1872	rVB	533424	649426	5.60%	0.795%
53	12.530	1872	1877	1880	rBV	1057267	1495446	12.90%	1.830%
54	12.555	1880	1881	1886	rVB	761750	666463	5.75%	0.815%
55	12.616	1886	1891	1894	rBV	2689979	3140847	27.10%	3.843%
56	12.646	1894	1896	1900	rVB	359805	384274	3.32%	0.470%
57	12.701	1900	1905	1913	rBV2	1330970	1964865	16.95%	2.404%
58	12.847	1924	1929	1934	rVB	564025	710493	6.13%	0.869%
59	12.920	1934	1941	1945	rBV	1547920	1987657	17.15%	2.432%
60	12.963	1945	1948	1954	rVB	1566705	1798798	15.52%	2.201%
61	13.024	1954	1958	1960	rBV	112299	148908	1.28%	0.182%
62	13.170	1978	1982	1987	rVB	1313461	1473031	12.71%	1.802%
63	13.256	1992	1996	1998	rBV2	121395	180158	1.55%	0.220%
64	13.292	1998	2002	2008	rVB2	2638005	3412182	29.44%	4.175%
65	13.426	2020	2024	2031	rVB	283643	369607	3.19%	0.452%
66	13.506	2031	2037	2040	rBV2	114142	161016	1.39%	0.197%
67	13.542	2040	2043	2046	rVV	243147	325101	2.80%	0.398%
68	13.585	2046	2050	2056	rVV3	309066	578216	4.99%	0.707%
69	13.664	2060	2063	2069	rVB2	251186	417242	3.60%	0.510%
70	13.774	2075	2081	2088	rBV	702597	941994	8.13%	1.152%
71	13.926	2100	2106	2110	rBV2	123351	181911	1.57%	0.223%
72	13.969	2110	2113	2117	rVB	97203	122315	1.06%	0.150%
73	14.079	2126	2131	2136	rBV	233055	286992	2.48%	0.351%
74	14.219	2148	2154	2164	rBV	213609	383249	3.31%	0.469%
75	14.323	2167	2171	2176	rVV	118955	163564	1.41%	0.200%
76	14.371	2176	2179	2184	rVB	157392	187580	1.62%	0.229%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029706.D
Acq On : 22 Jun 2022 17:57
Operator : JC/MD
Sample : N3202-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Title : SW846 8260

77	14.640	2218	2223	2234	rVB	1370925	1698696	14.65%	2.078%
78	14.780	2241	2246	2251	rBV	1000690	1202522	10.37%	1.471%
79	15.481	2354	2361	2370	rBV	85203	140512	1.21%	0.172%
80	15.615	2376	2383	2386	rBV	113729	174656	1.51%	0.214%




Sum of corrected areas: 81738572

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029706.D
Acq On : 22 Jun 2022 17:57
Operator : JC/MD
Sample : N3202-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

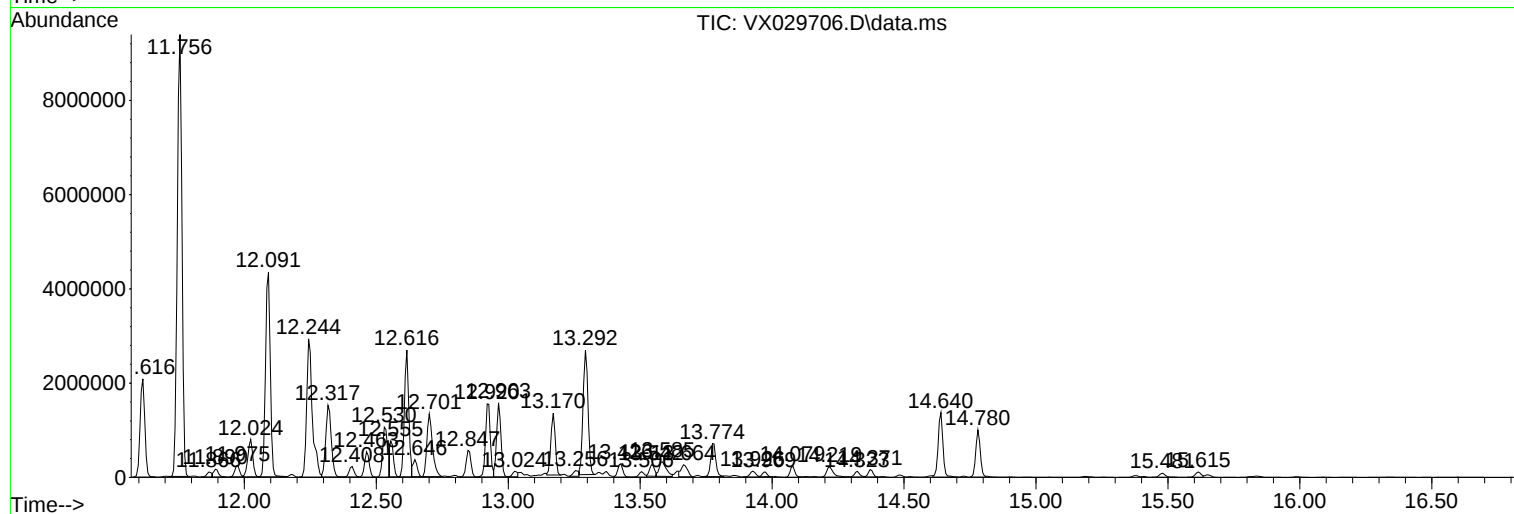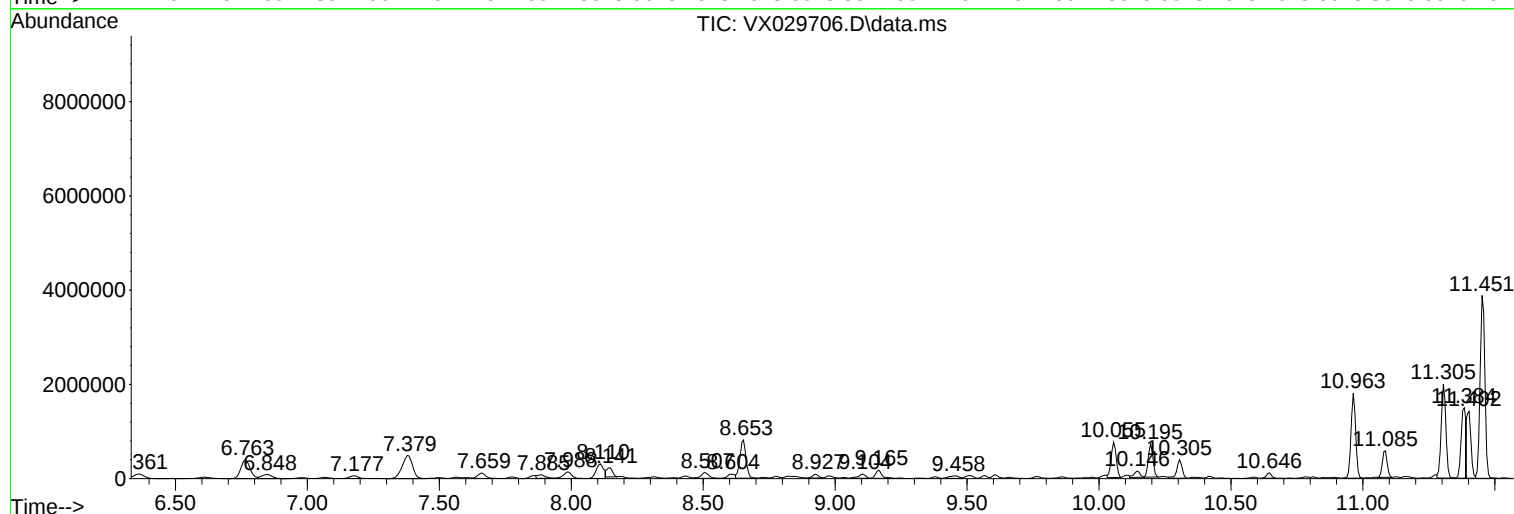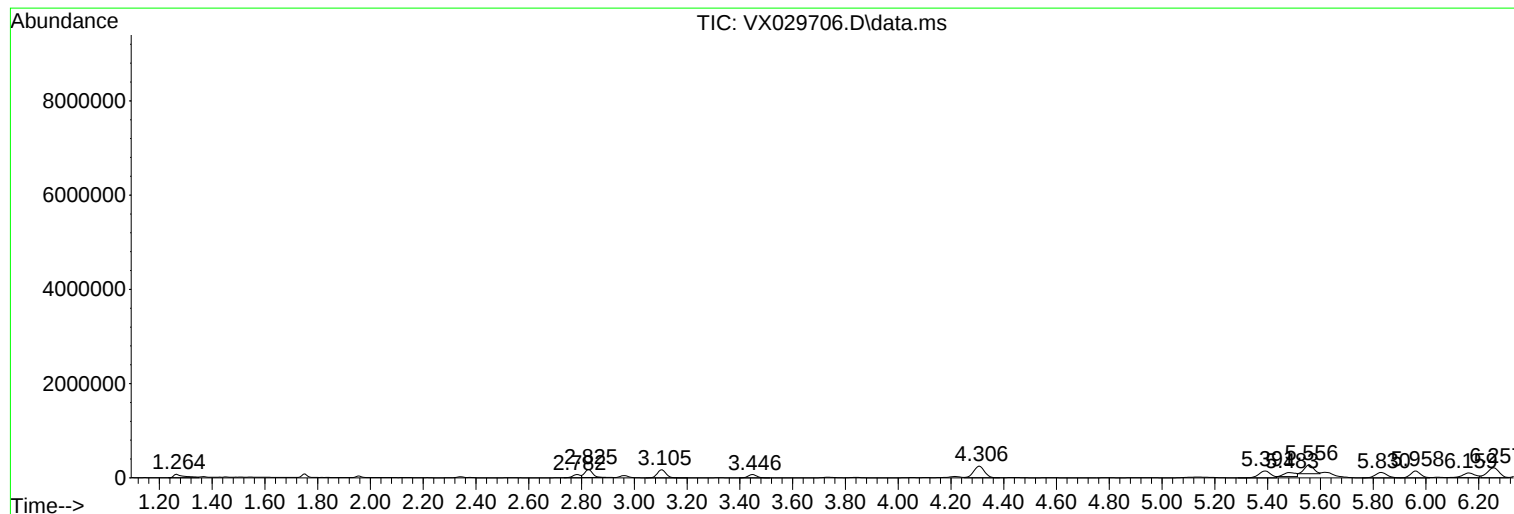

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029706.D
Acq On : 22 Jun 2022 17:57
Operator : JC/MD
Sample : N3202-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062222\
Data File : VX029706.D
Acq On : 22 Jun 2022 17:57
Operator : JC/MD
Sample : N3202-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc