


## Ethyl methacrylate

Response Ratio

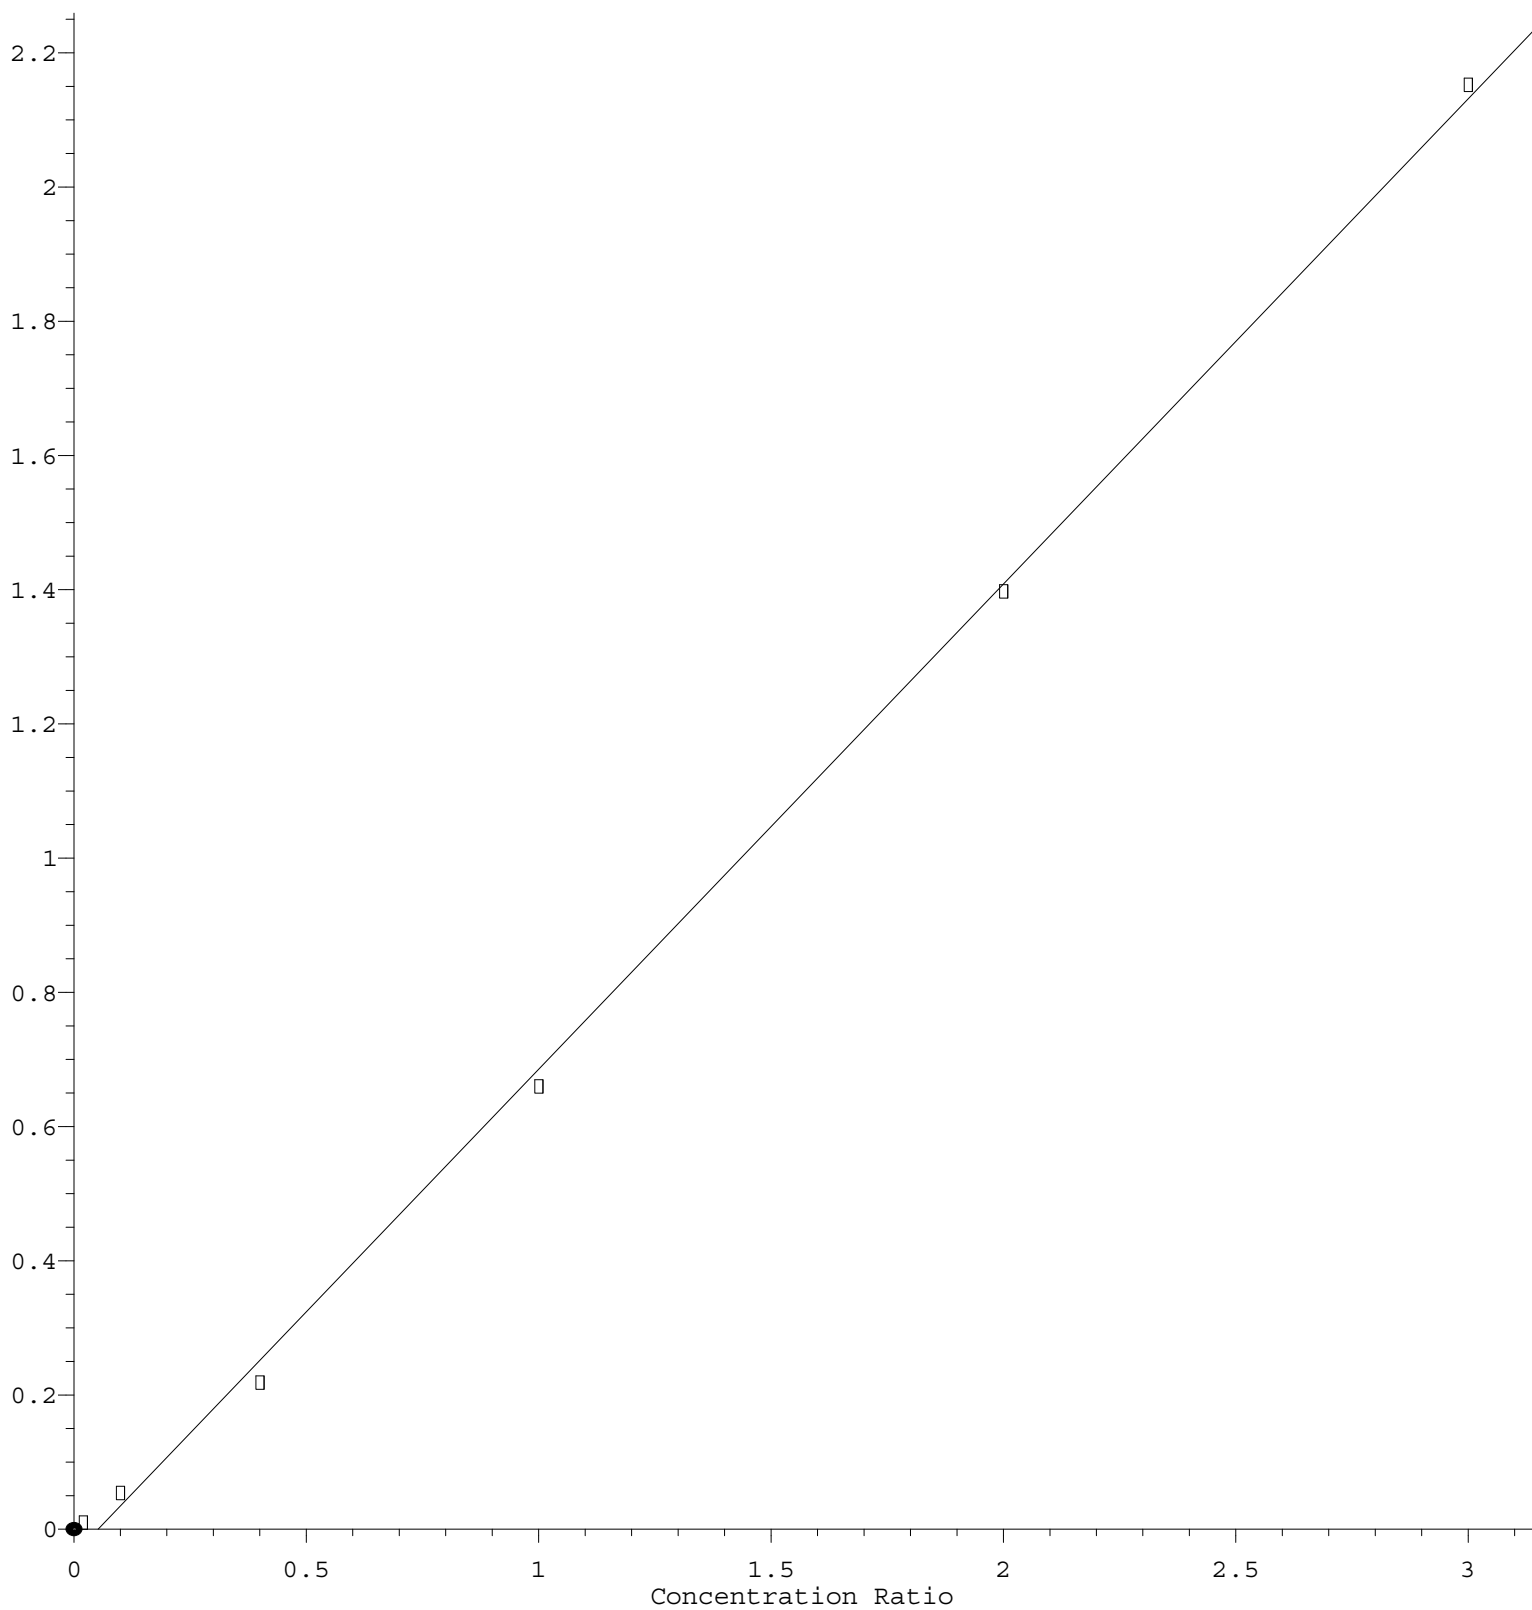

$$\text{Response} = 7.231\text{e-}001 * \text{Amt} - 3.730\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.998982 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# cis-1,3-Dichloropropene

Response Ratio

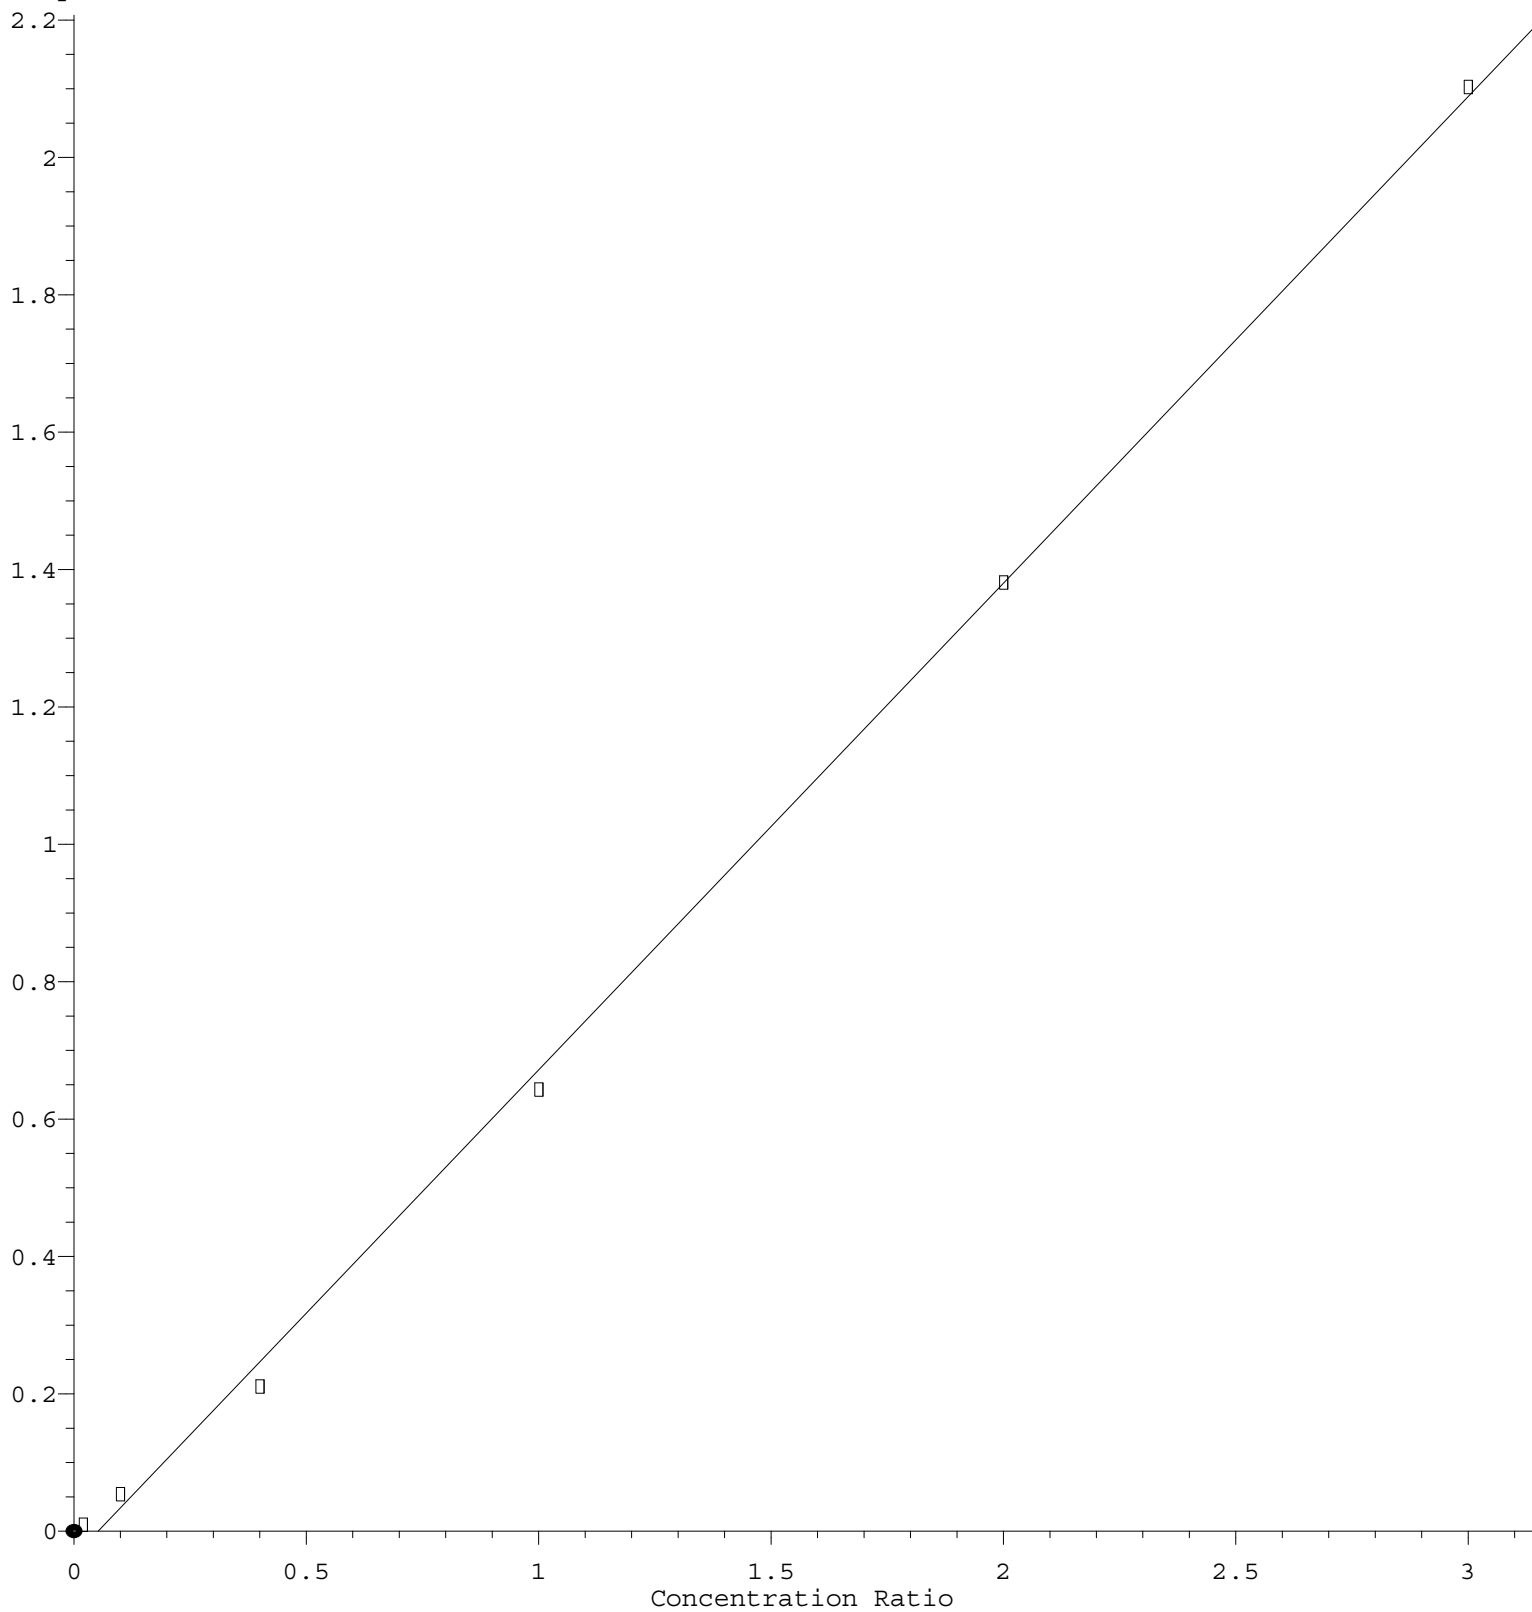

$$\text{Response} = 7.086\text{e-}001 * \text{Amt} - 3.670\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.998957 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

t-1,3-Dichloropropene

Response Ratio

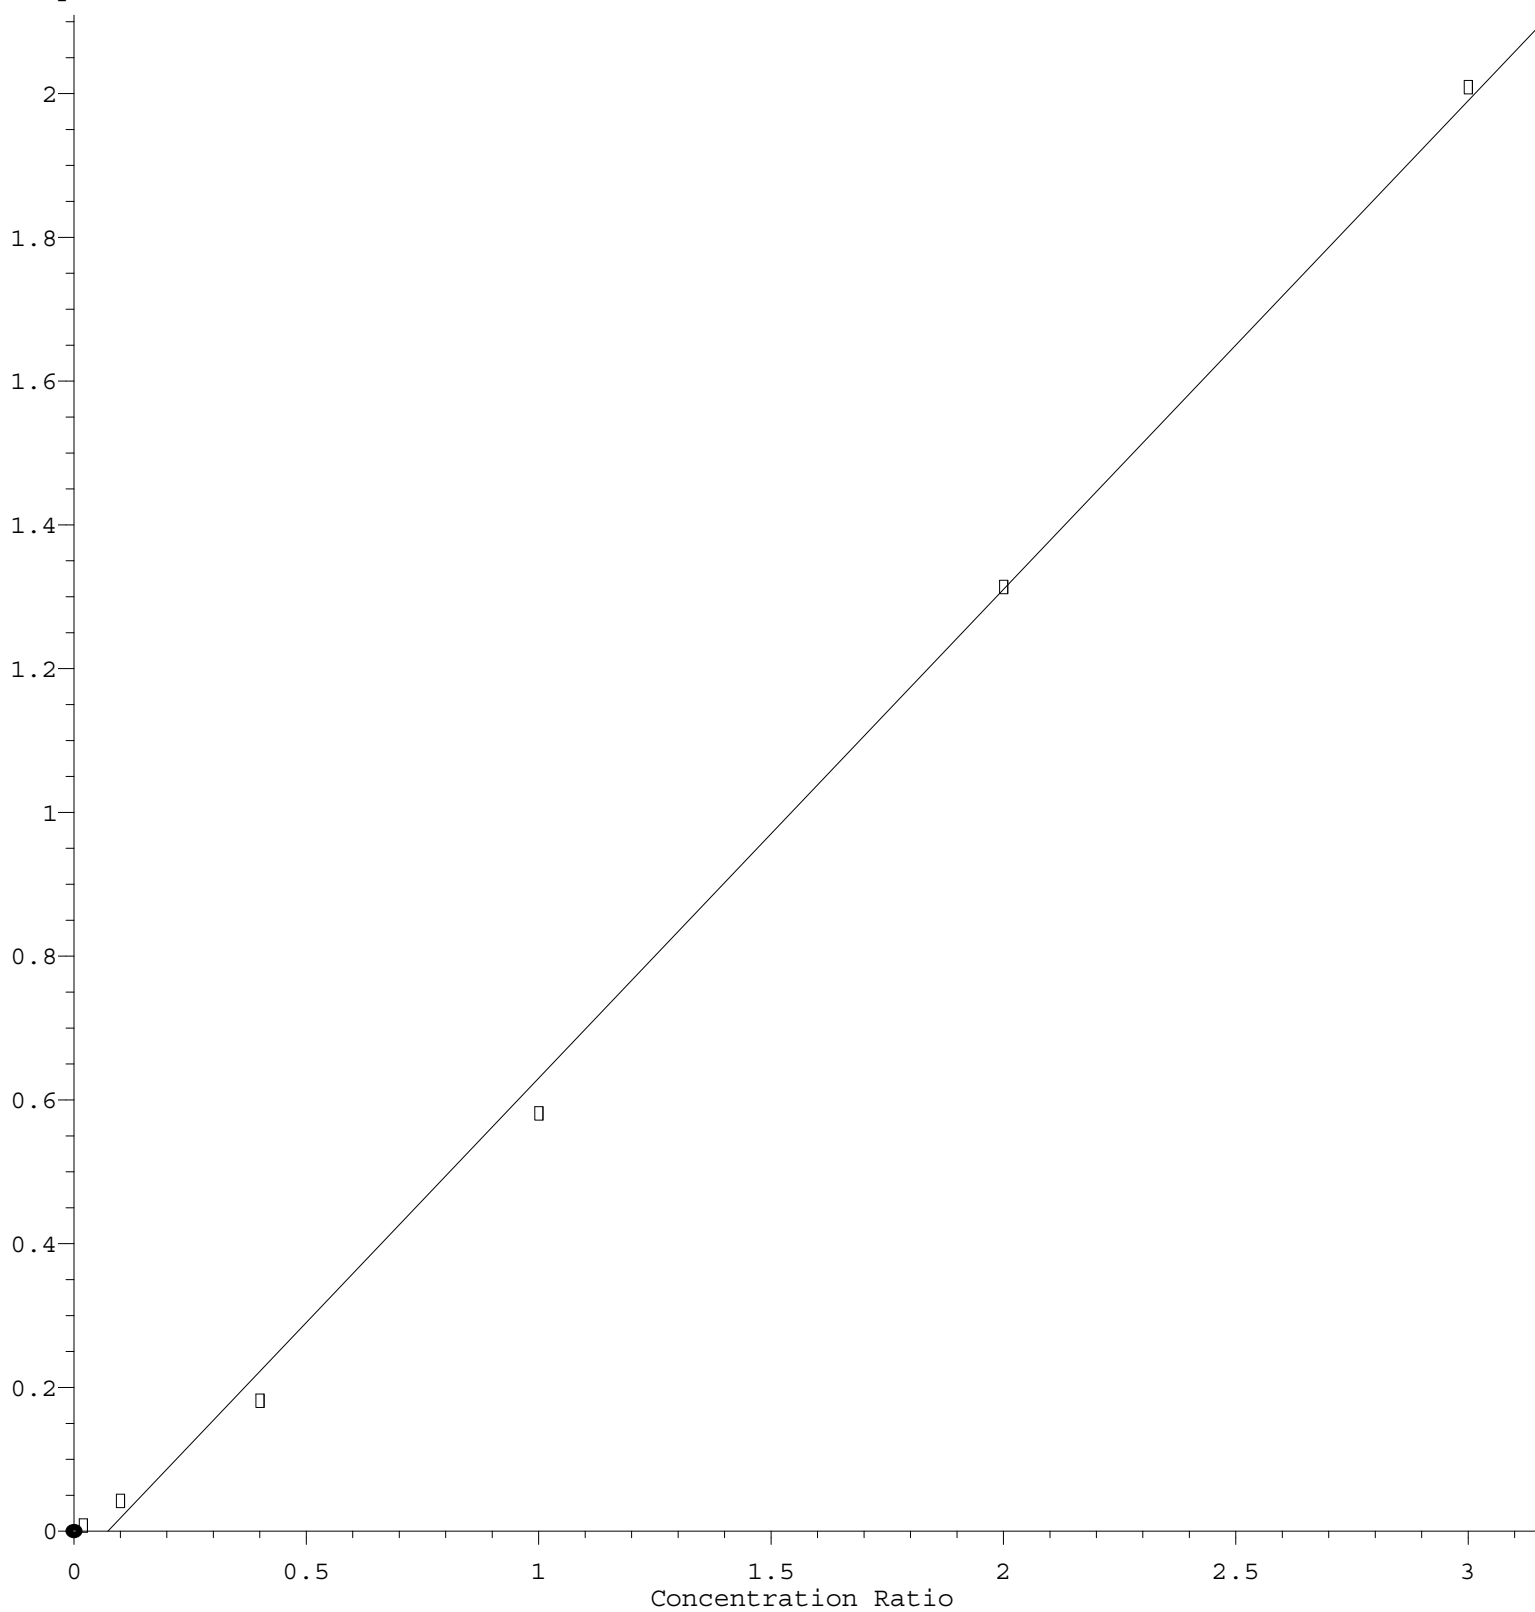

$$\text{Response} = 6.800\text{e-}001 * \text{Amt} - 4.987\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.997889 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# Bromodichloromethane

Response Ratio

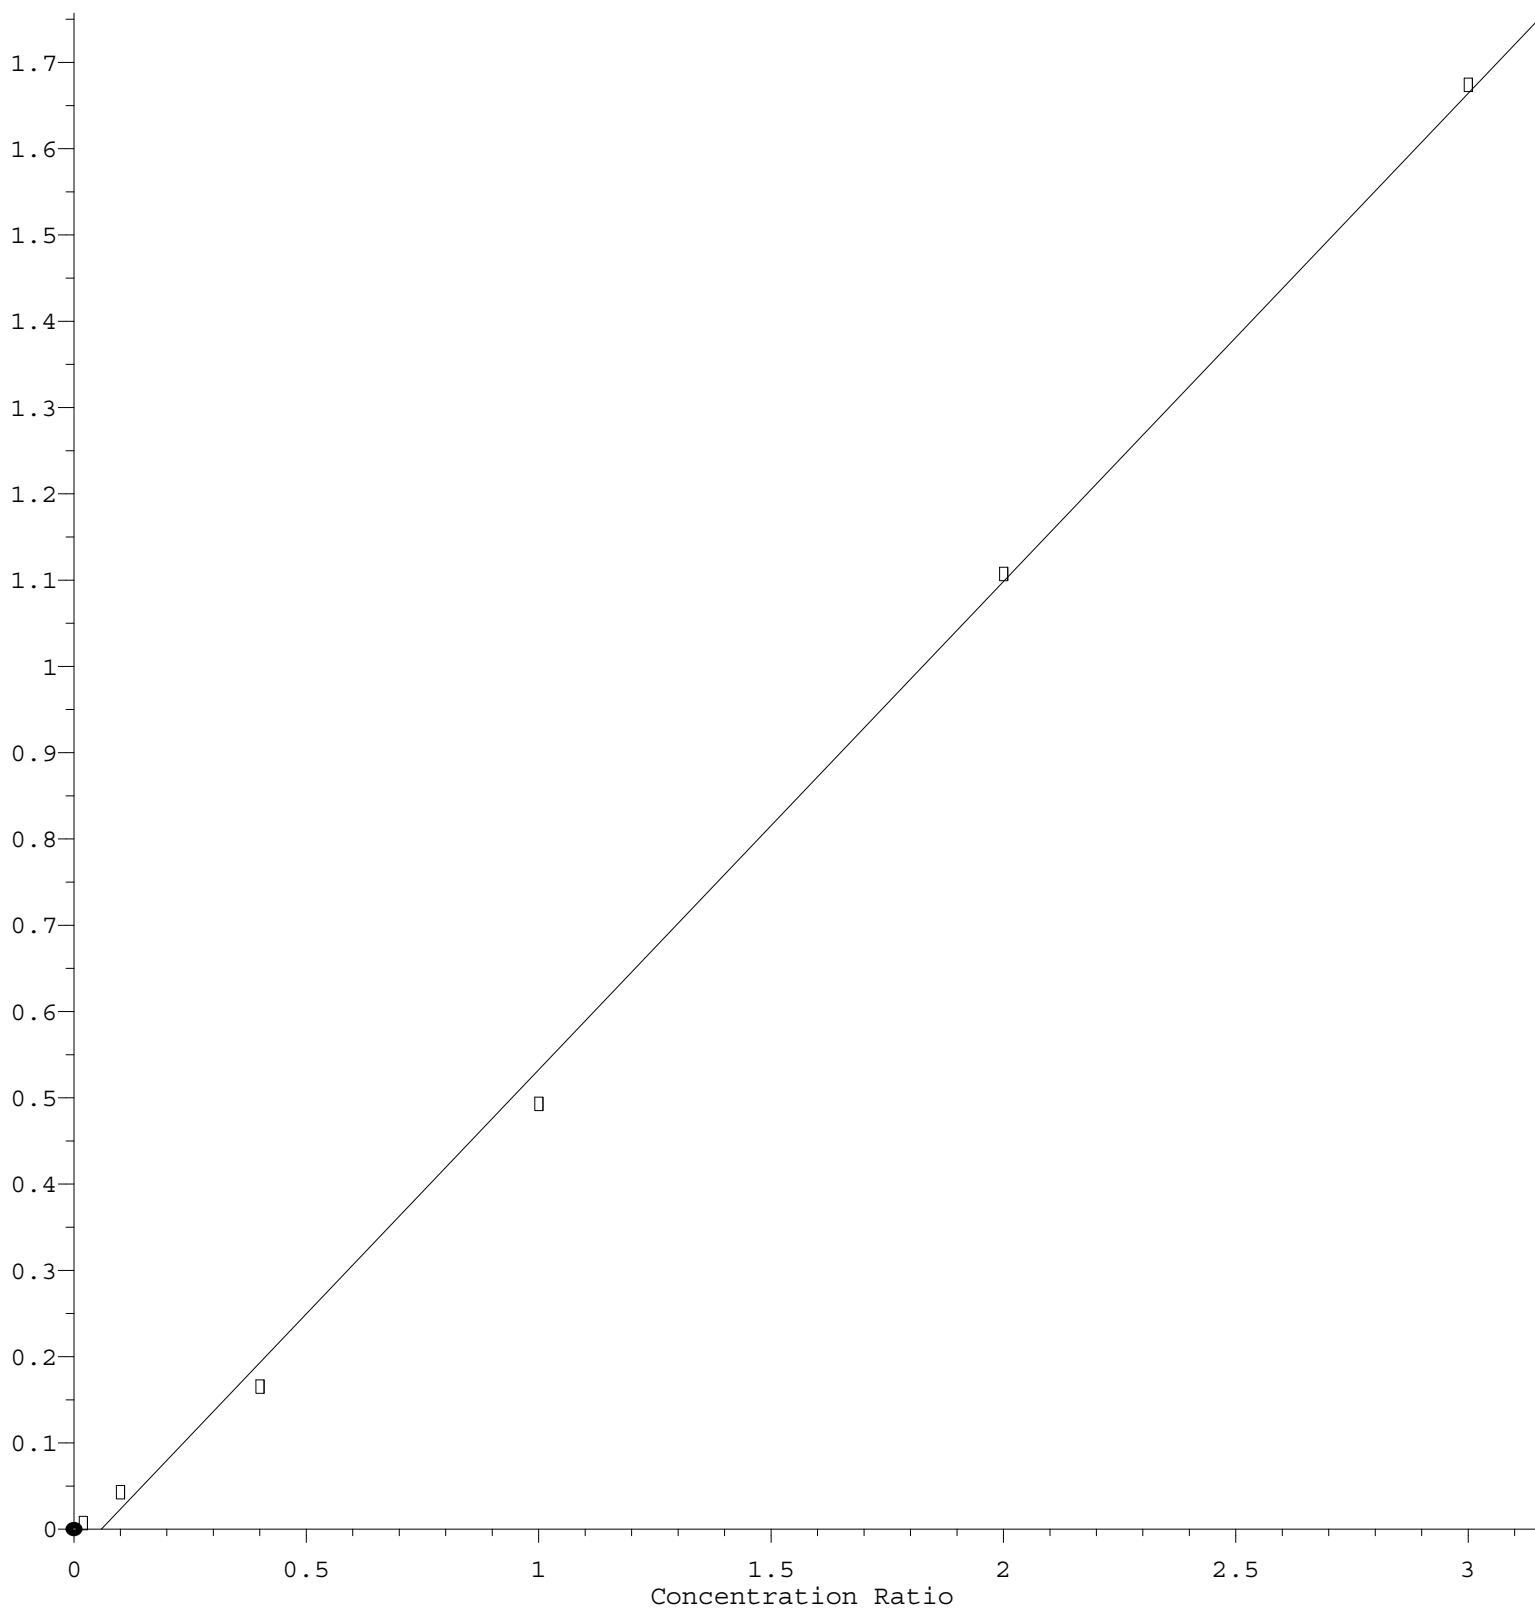

$$\text{Response} = 5.657\text{e-}001 * \text{Amt} - 3.319\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.998353 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# Methylene Chloride

Response Ratio

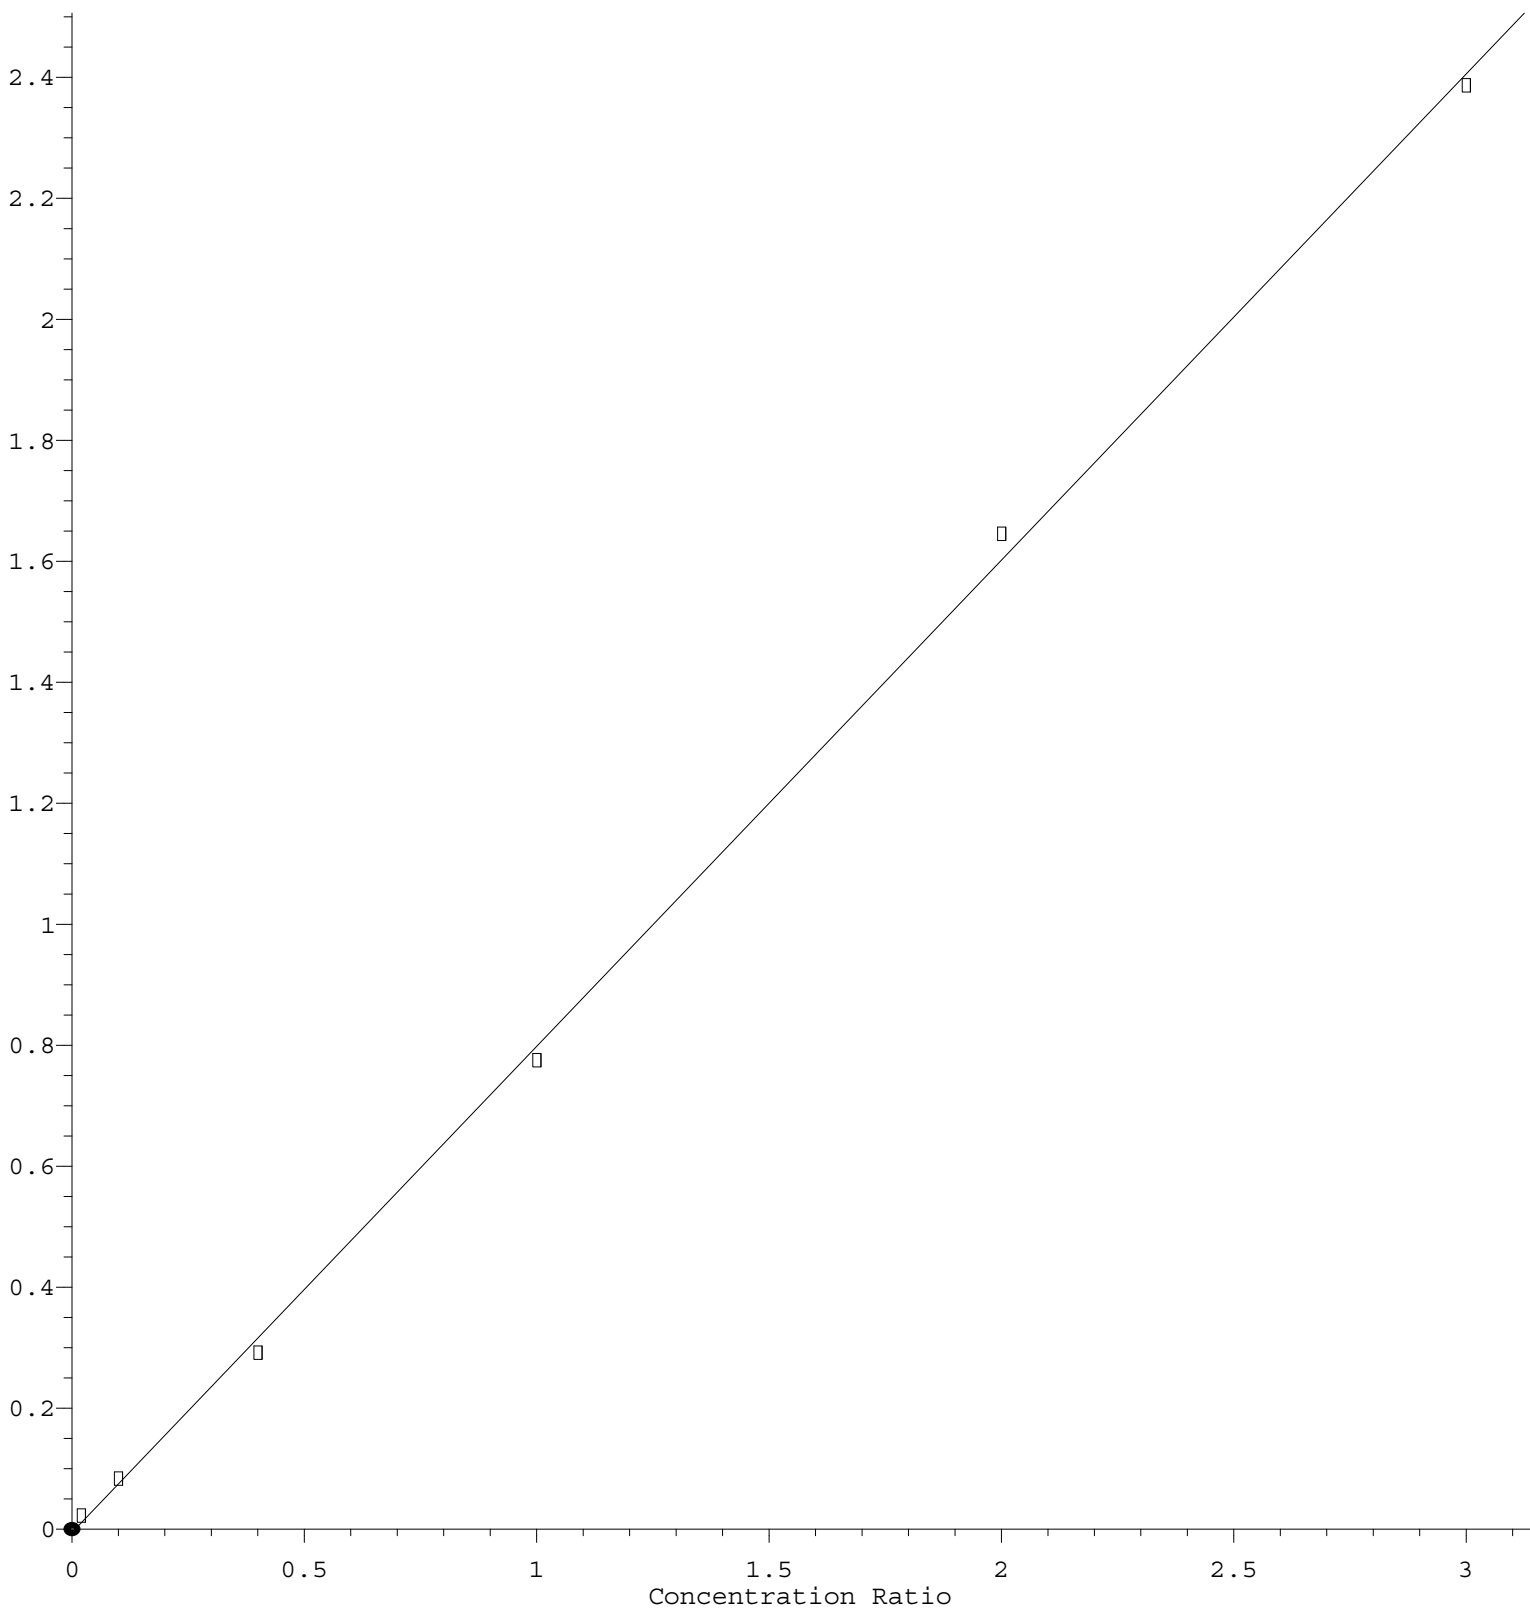

$$\text{Response} = 8.038\text{e-}001 * \text{Amt} - 5.985\text{e-}003$$


Coef of Det ( $r^2$ ) = 0.999215 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

## Carbon Disulfide

Response Ratio

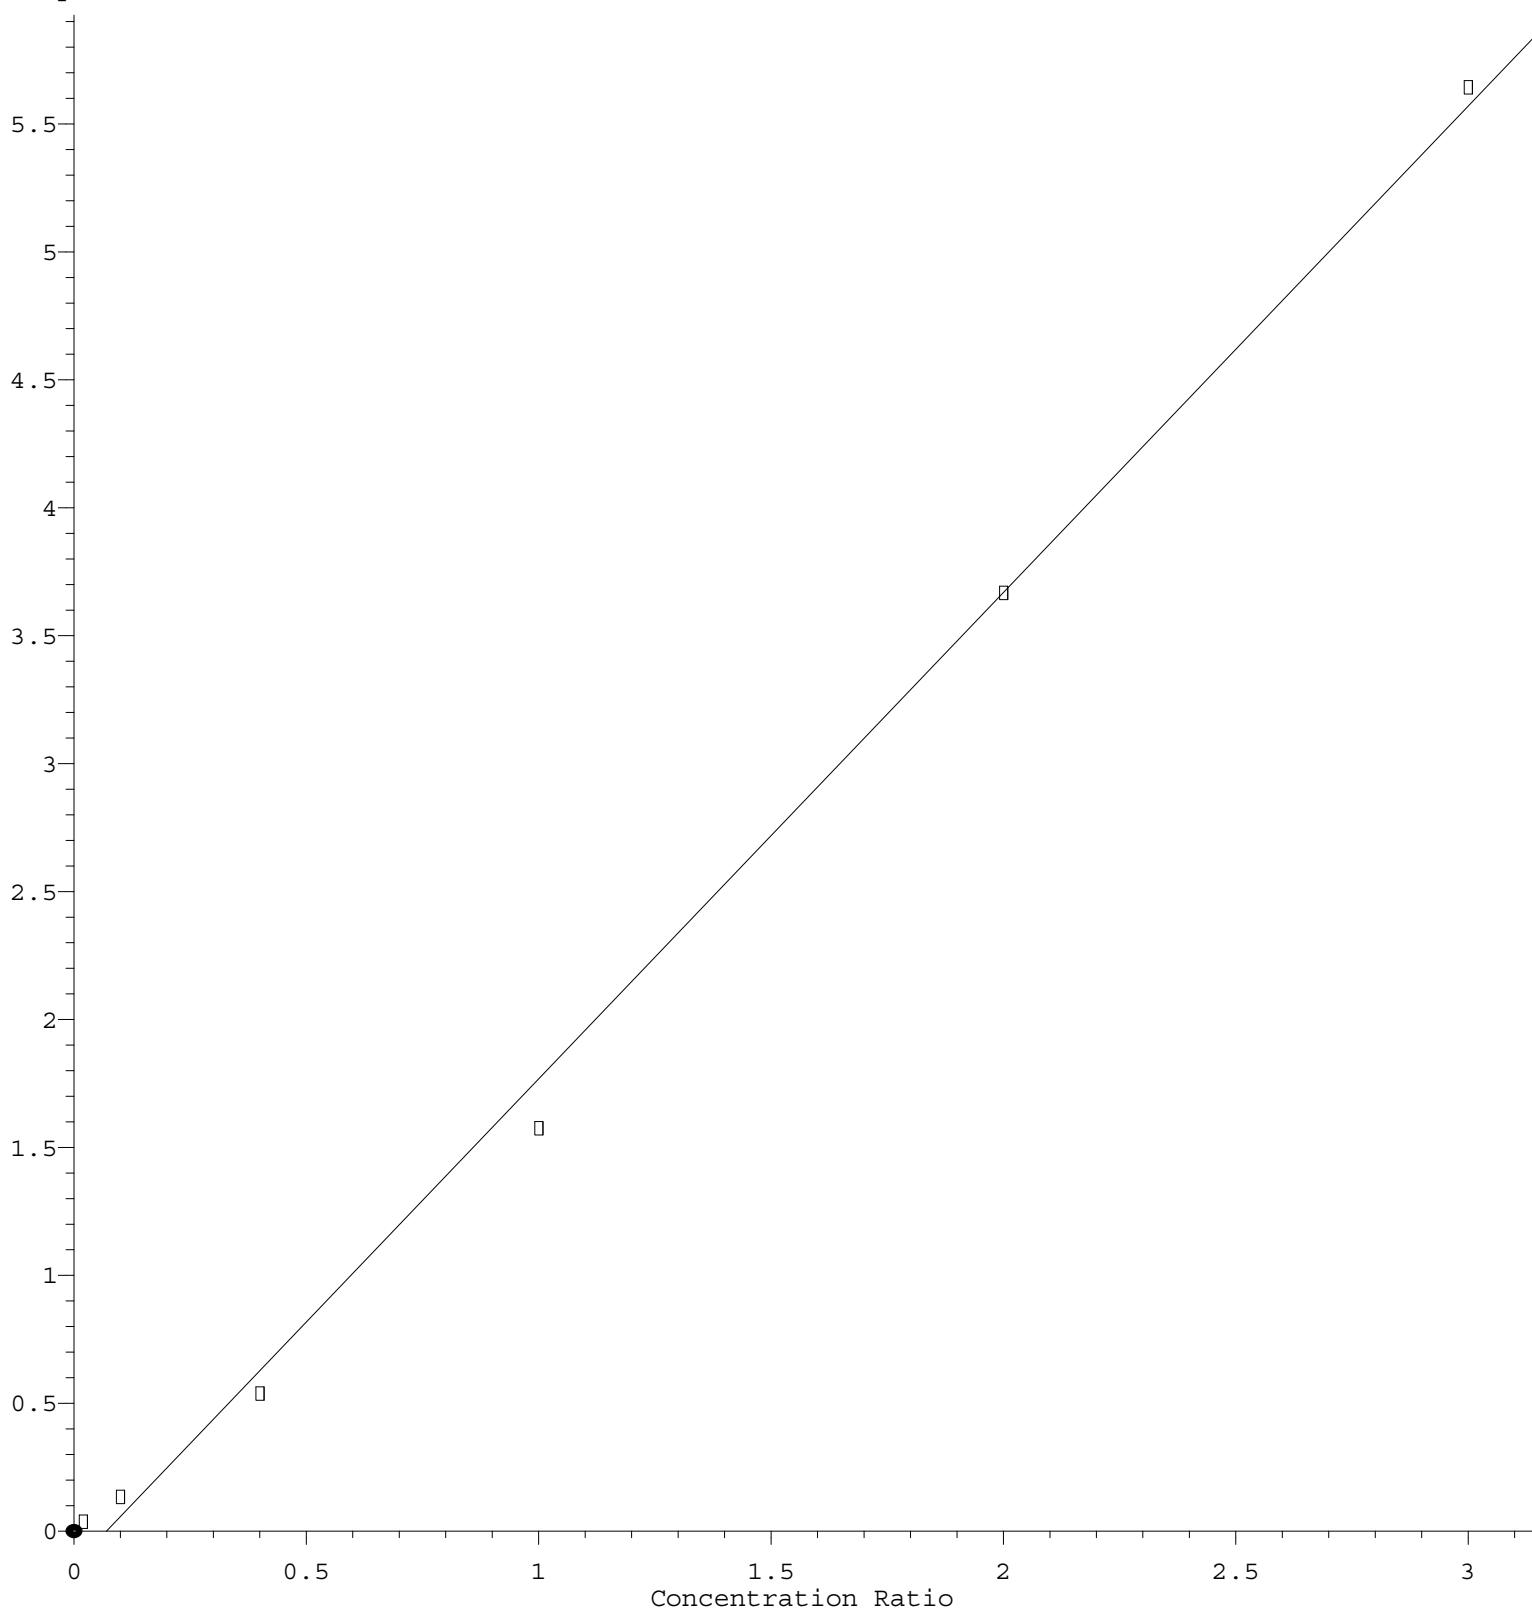

$$\text{Response} = 1.901\text{e}+000 * \text{Amt} - 1.337\text{e}-001$$


Coef of Det ( $r^2$ ) = 0.997118 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# Naphthalene

Response Ratio

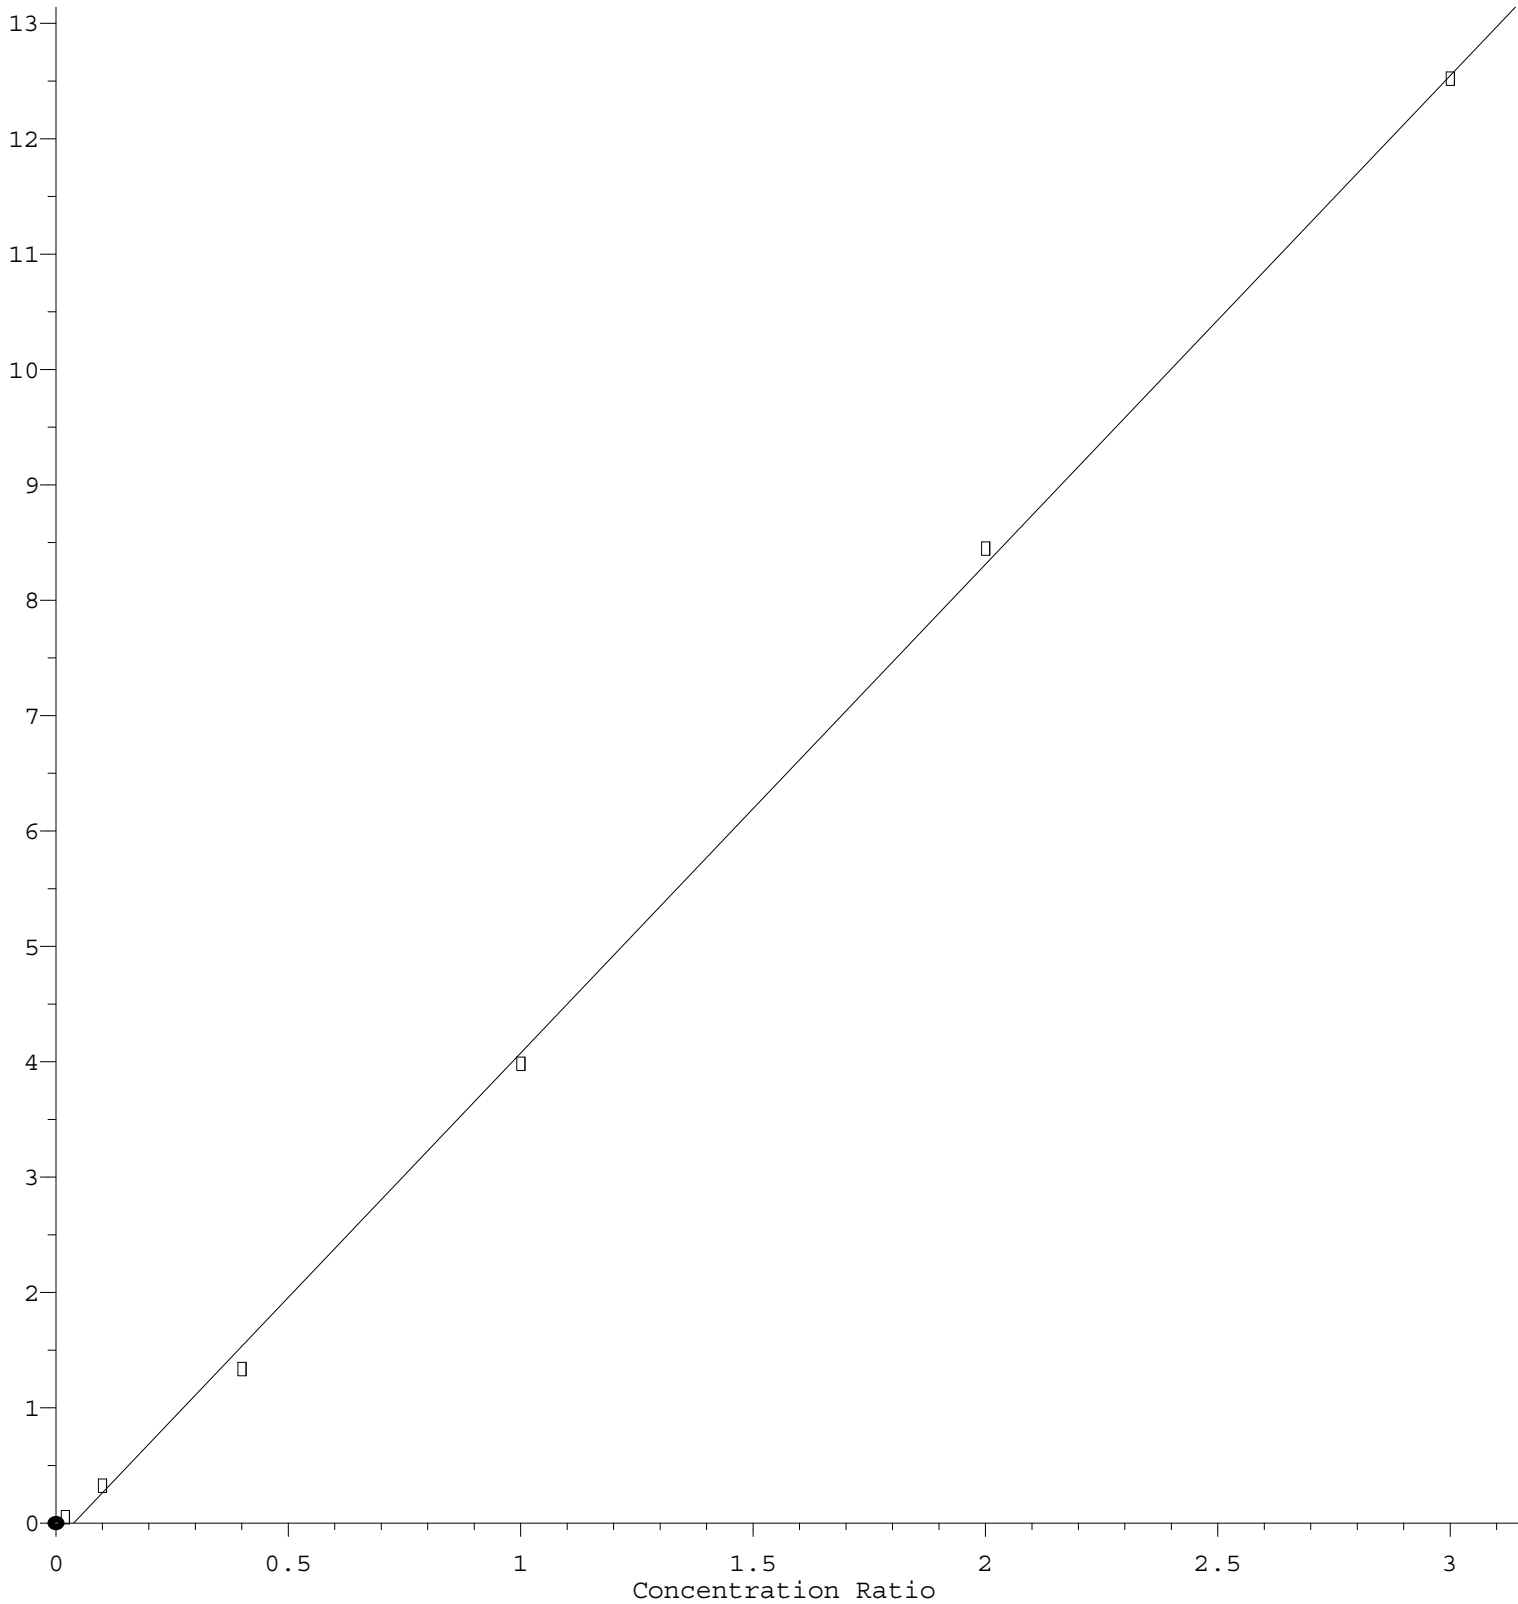

$$\text{Response} = 4.239\text{e}+000 * \text{Amt} - 1.630\text{e}-001$$


Coef of Det ( $r^2$ ) = 0.999314 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# 1,2-Dibromo-3-Chloropropane

Response Ratio

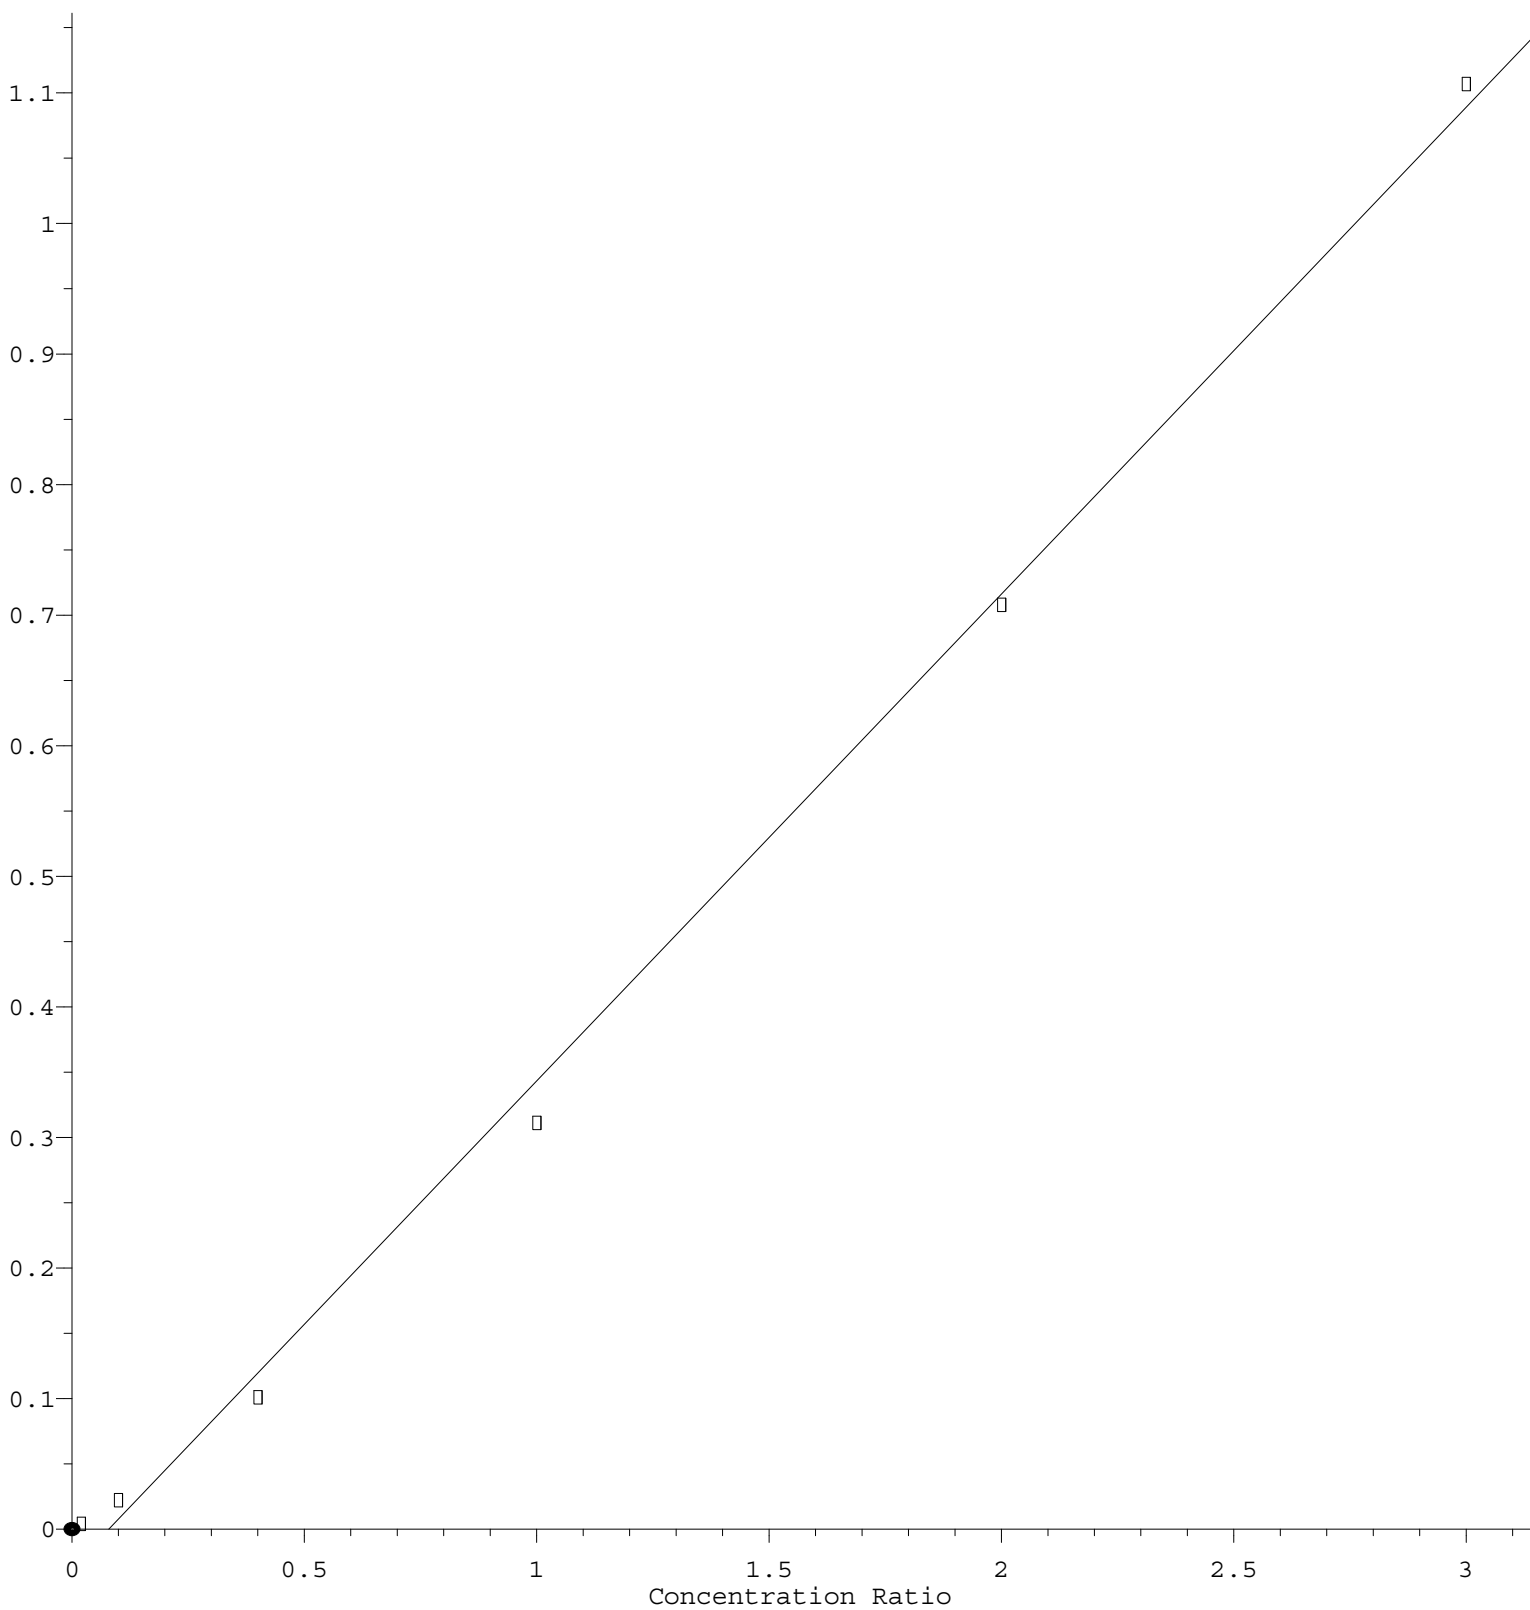

$$\text{Response} = 3.728\text{e-}001 * \text{Amt} - 2.962\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.997317 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

## Hexachloroethane

Response Ratio

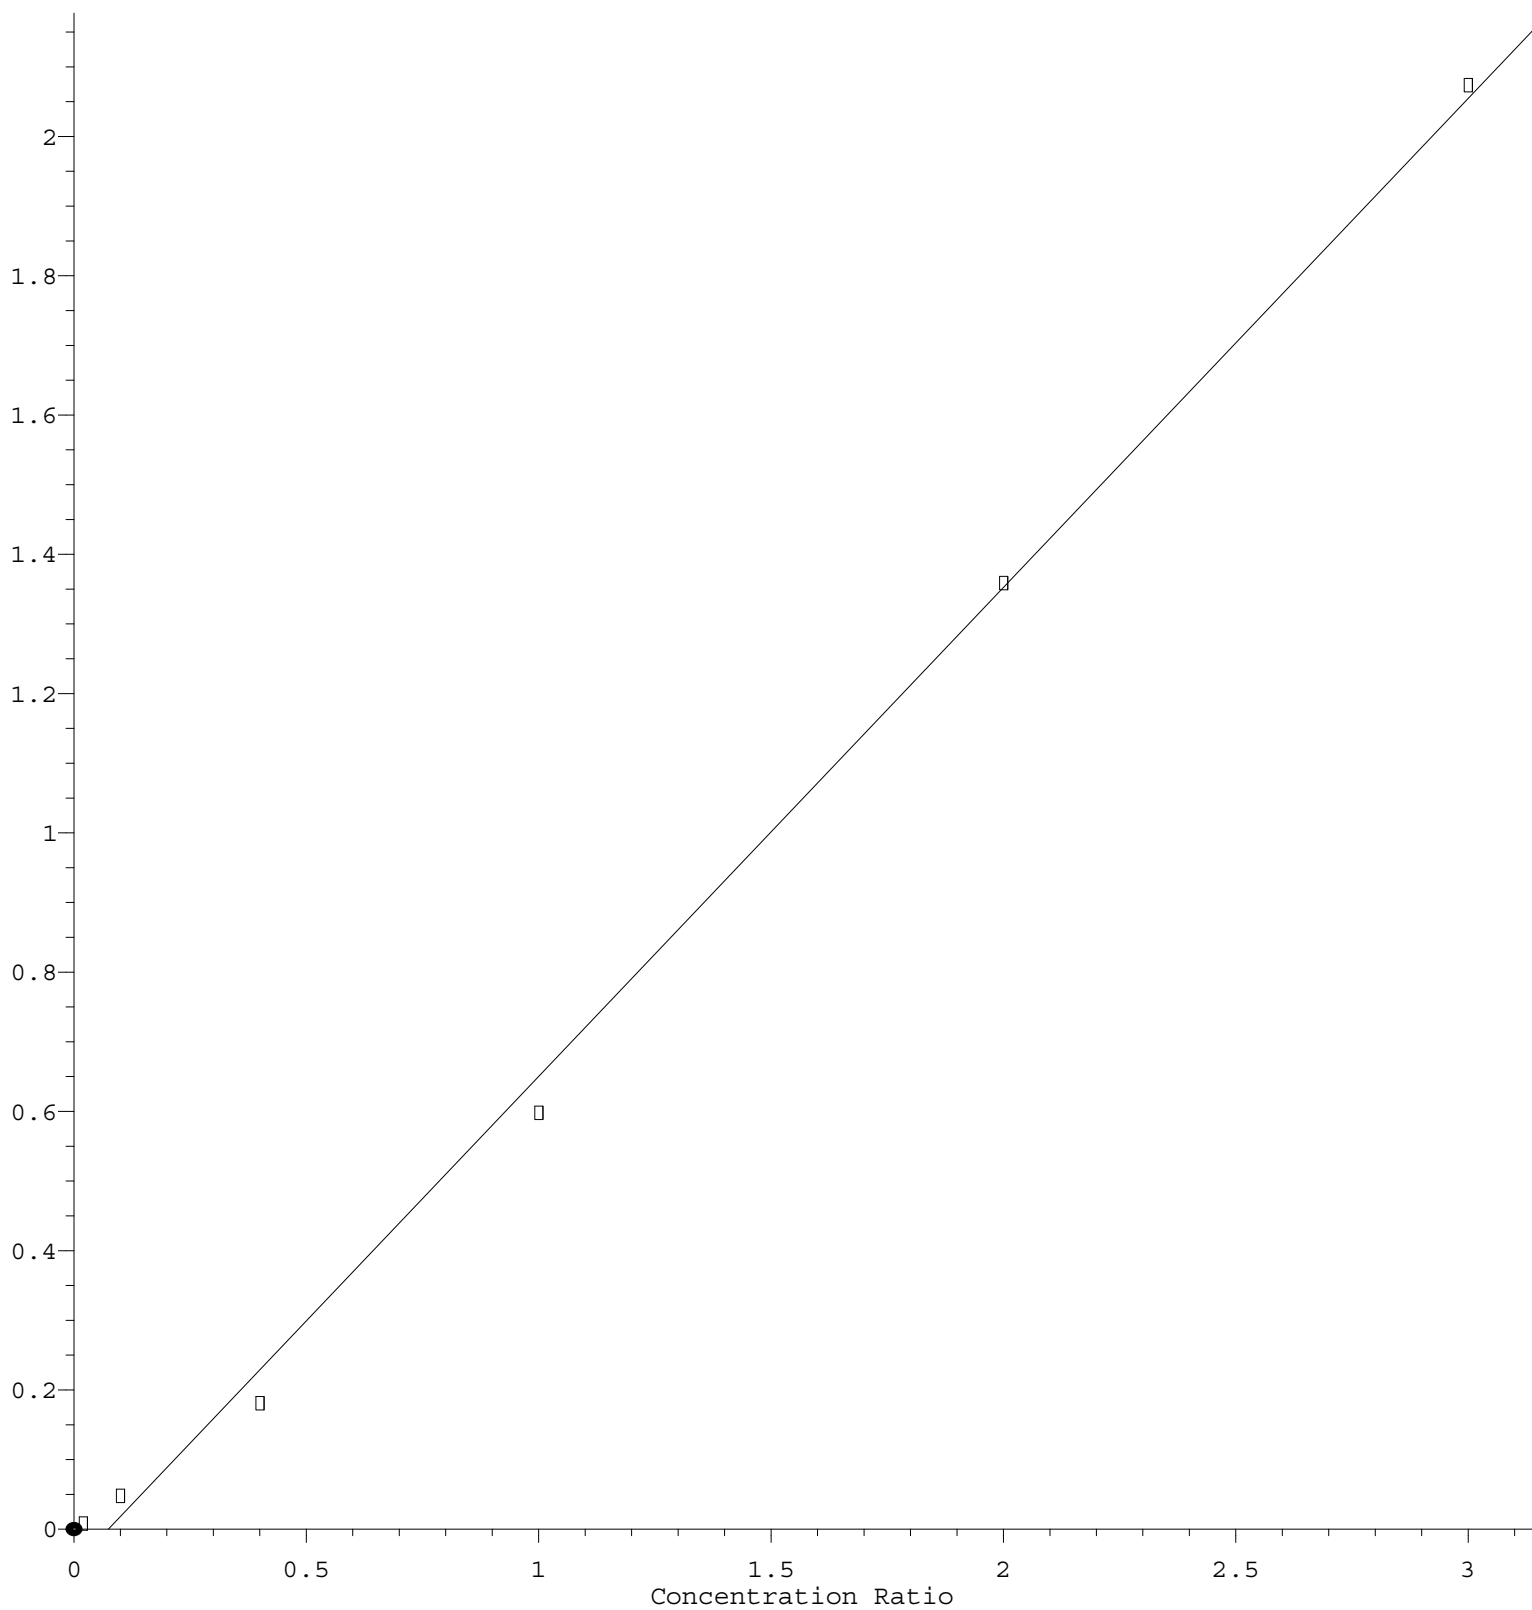

$$\text{Response} = 7.024\text{e-}001 * \text{Amt} - 5.212\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.997598 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

## trans-1,4-Dichloro-2-butene

Response Ratio

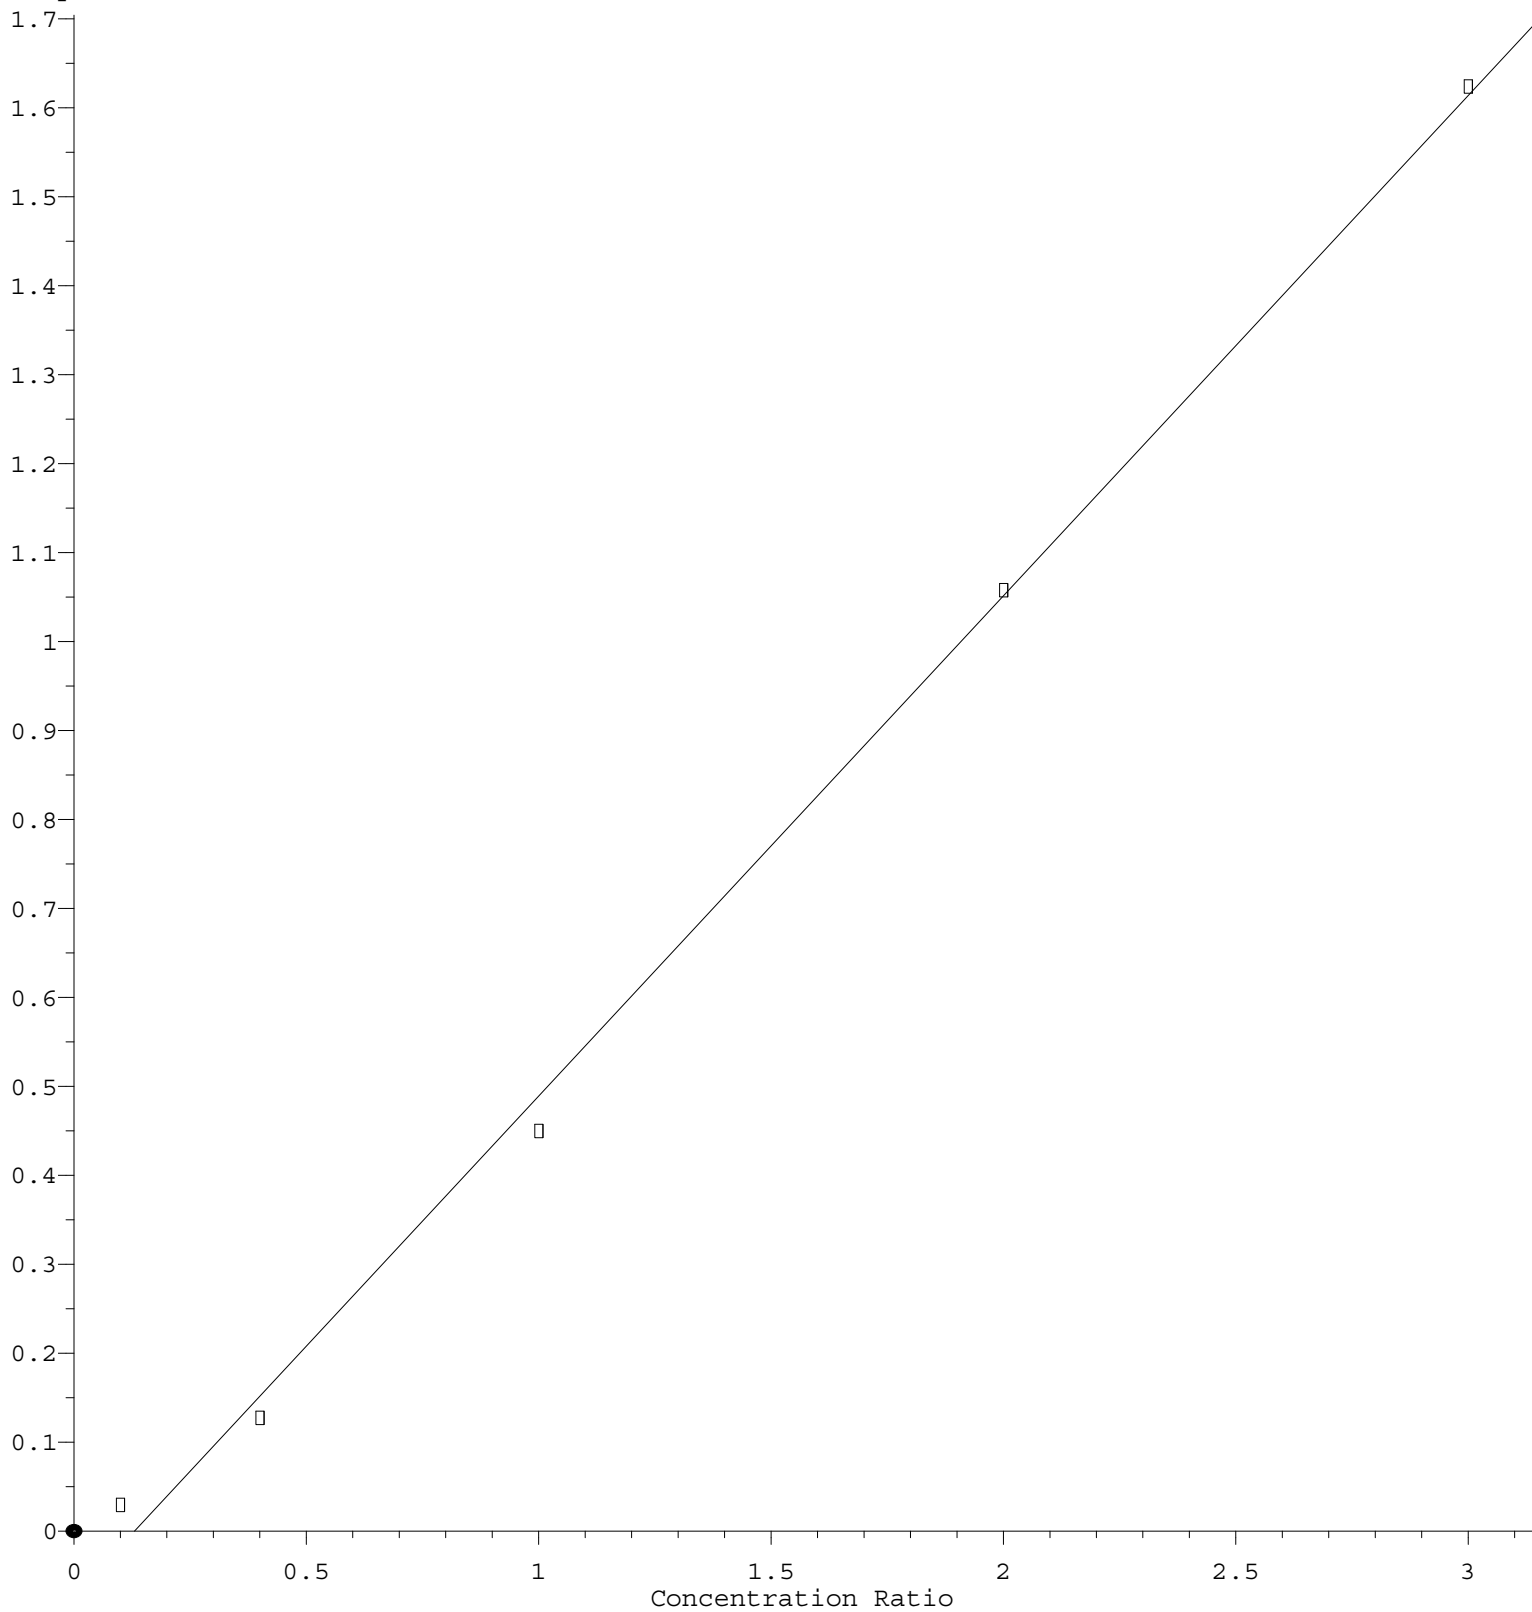

$$\text{Response} = 5.622\text{e-}001 * \text{Amt} - 7.322\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.997549 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# N-amyl acetate

Response Ratio

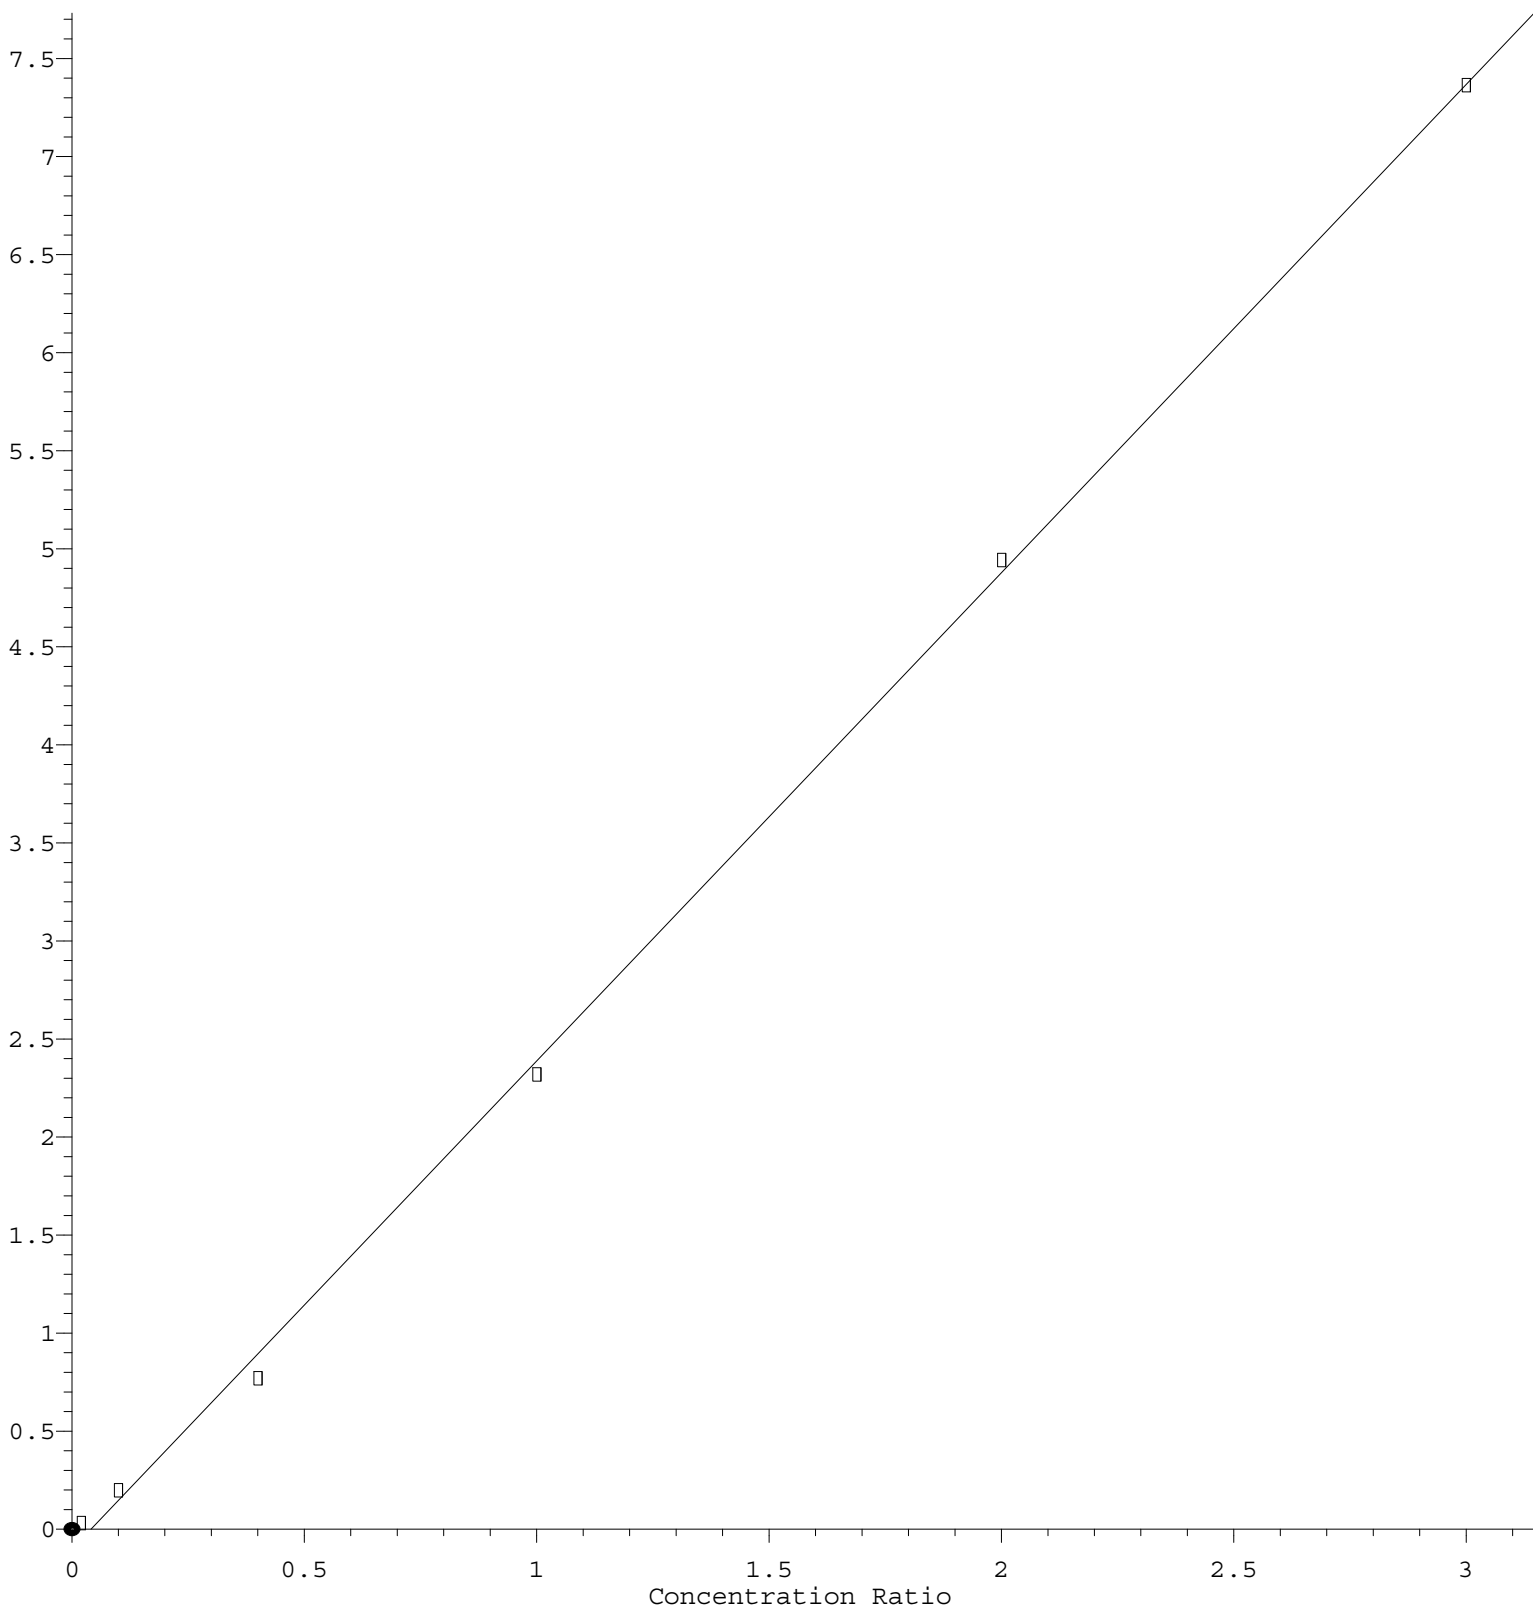


$$\text{Response} = 2.490\text{e}+000 * \text{Amt} - 1.023\text{e}-001$$

Coef of Det ( $r^2$ ) = 0.999226 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021


# Bromoform

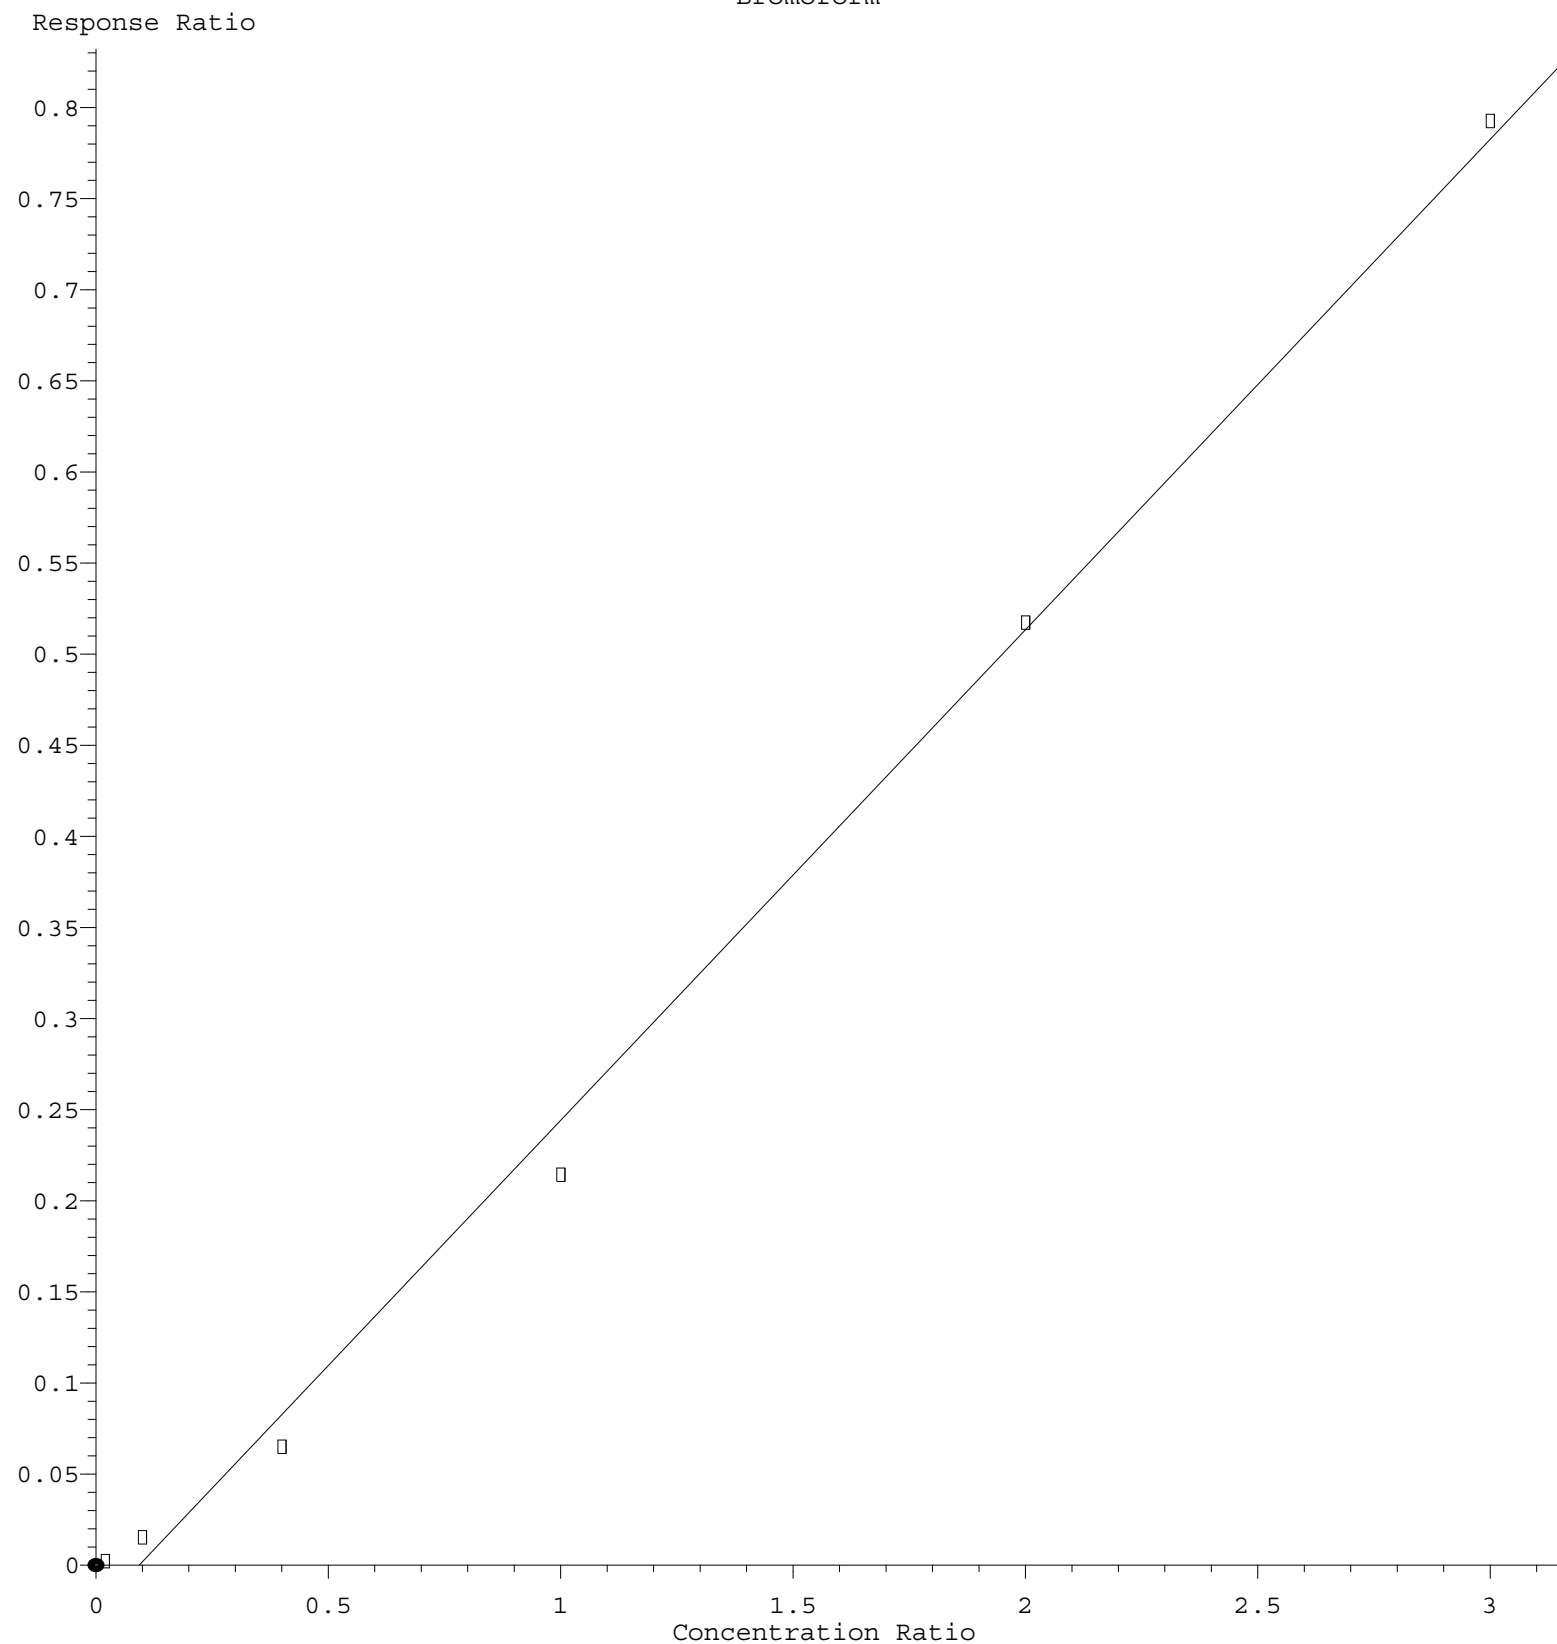

$\text{Response} = 2.693\text{e-}001 * \text{Amt} - 2.493\text{e-}002$   
 Coef of Det ( $r^2$ ) = 0.996168    Curve Fit: Linear  
 Method Name:    Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M  
 Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

# Dibromochloromethane

Response Ratio

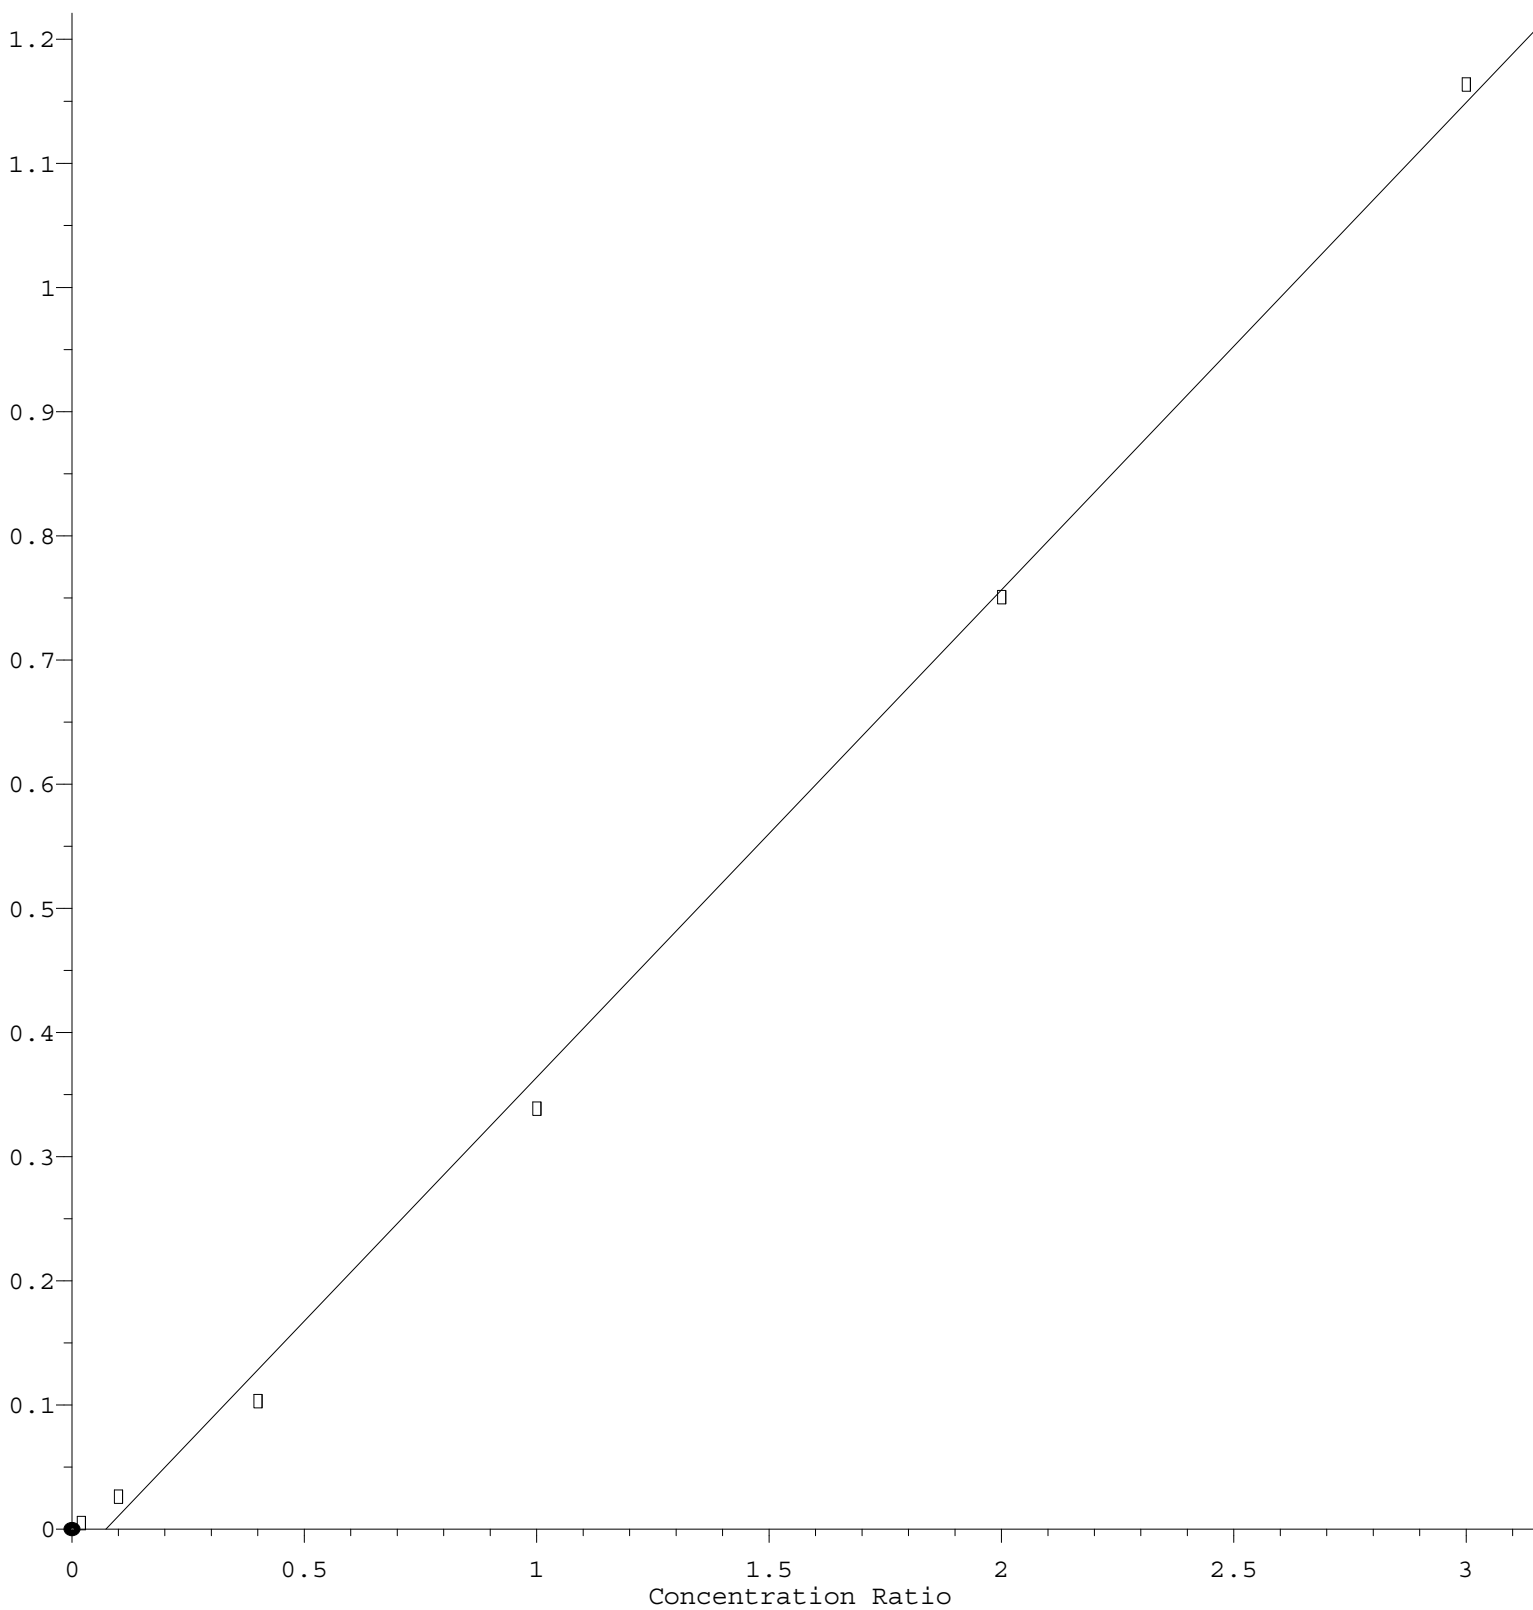

$$\text{Response} = 3.925\text{e-}001 * \text{Amt} - 2.865\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.997783 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

## 2-Chloroethyl Vinyl ether

Response Ratio

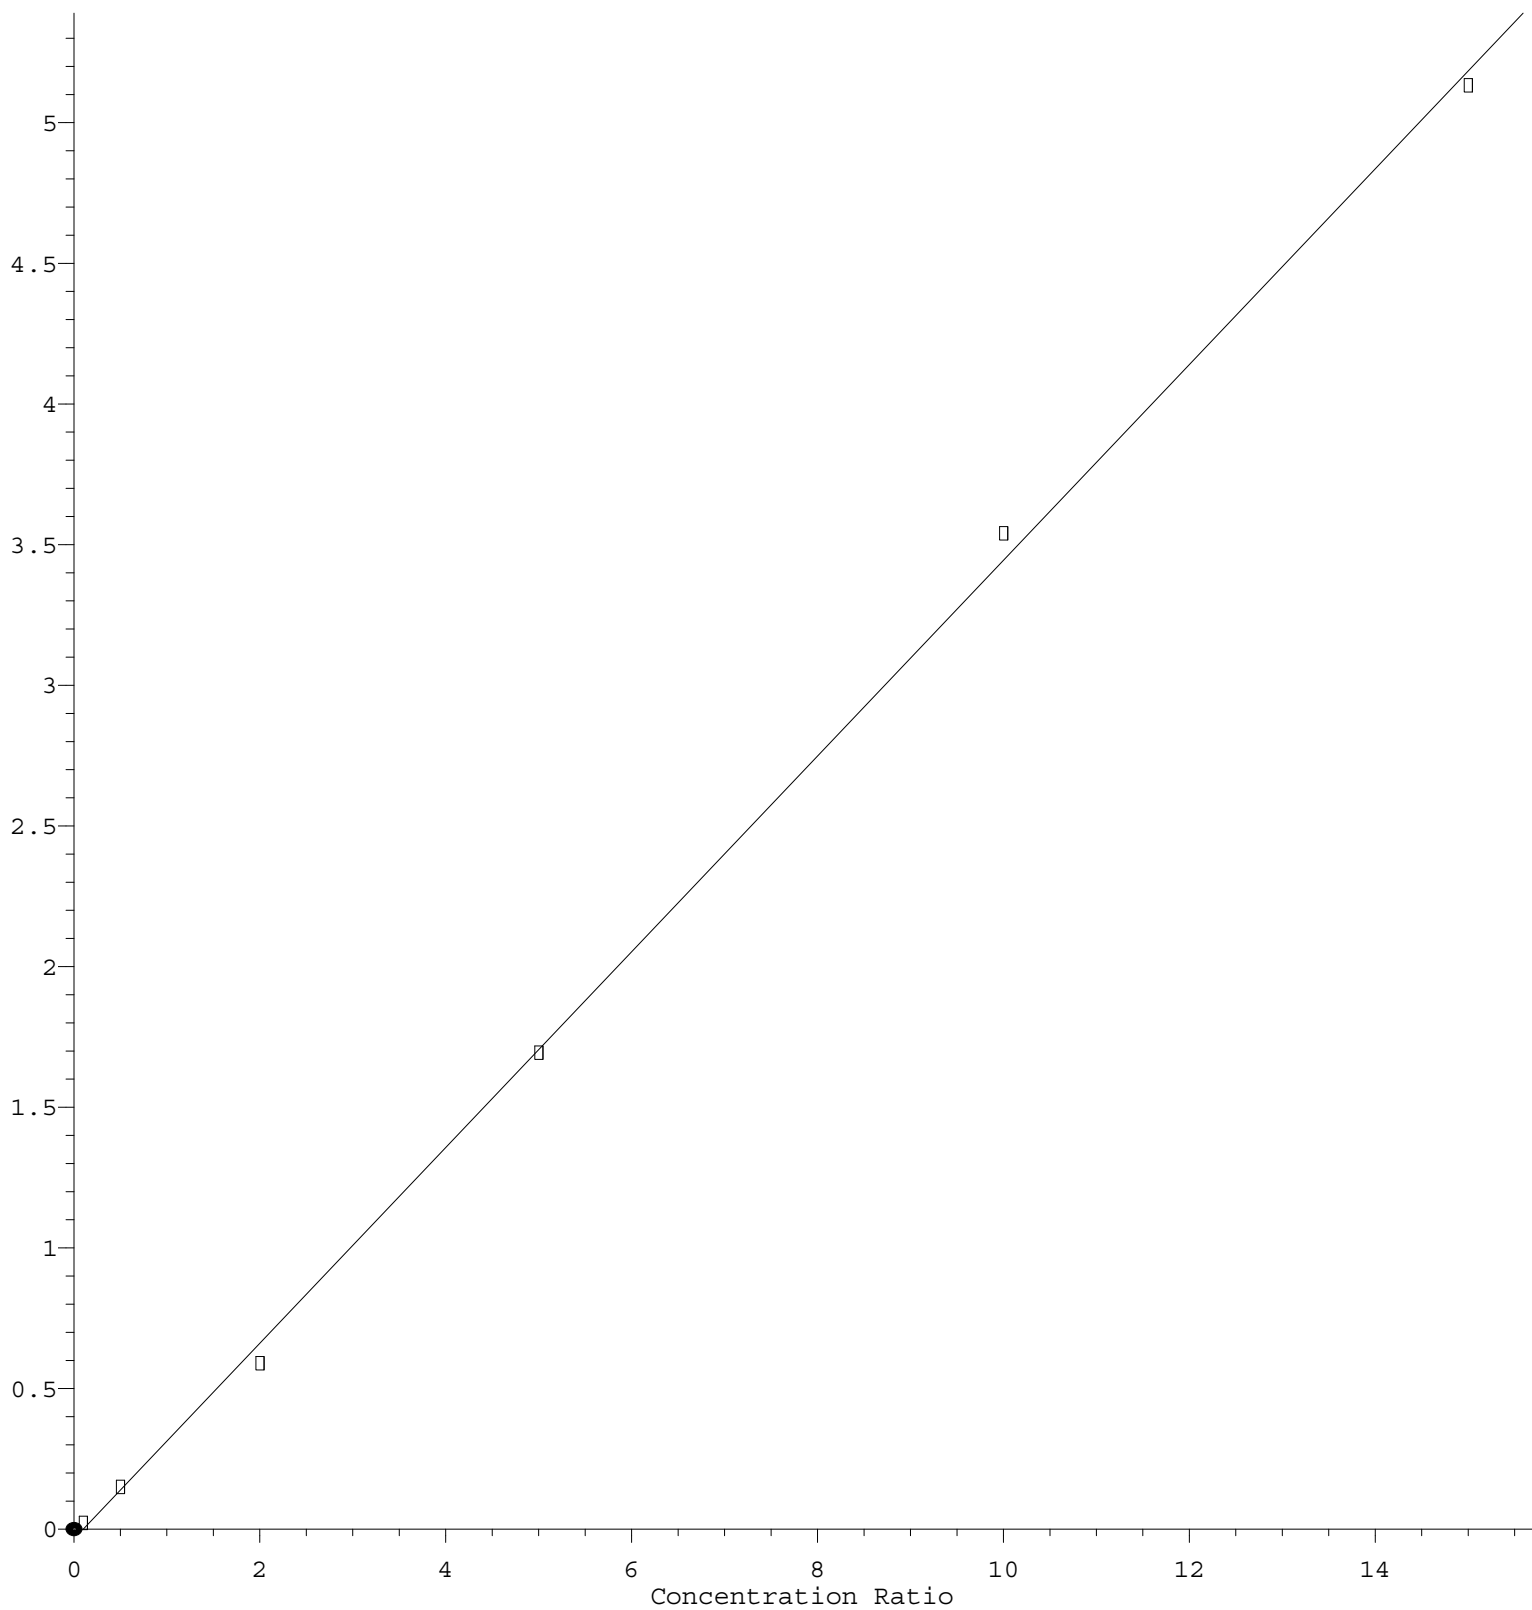

$$\text{Response} = 3.480\text{e-}001 * \text{Amt} - 3.626\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999181 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021

## Methyl Iodide

Response Ratio

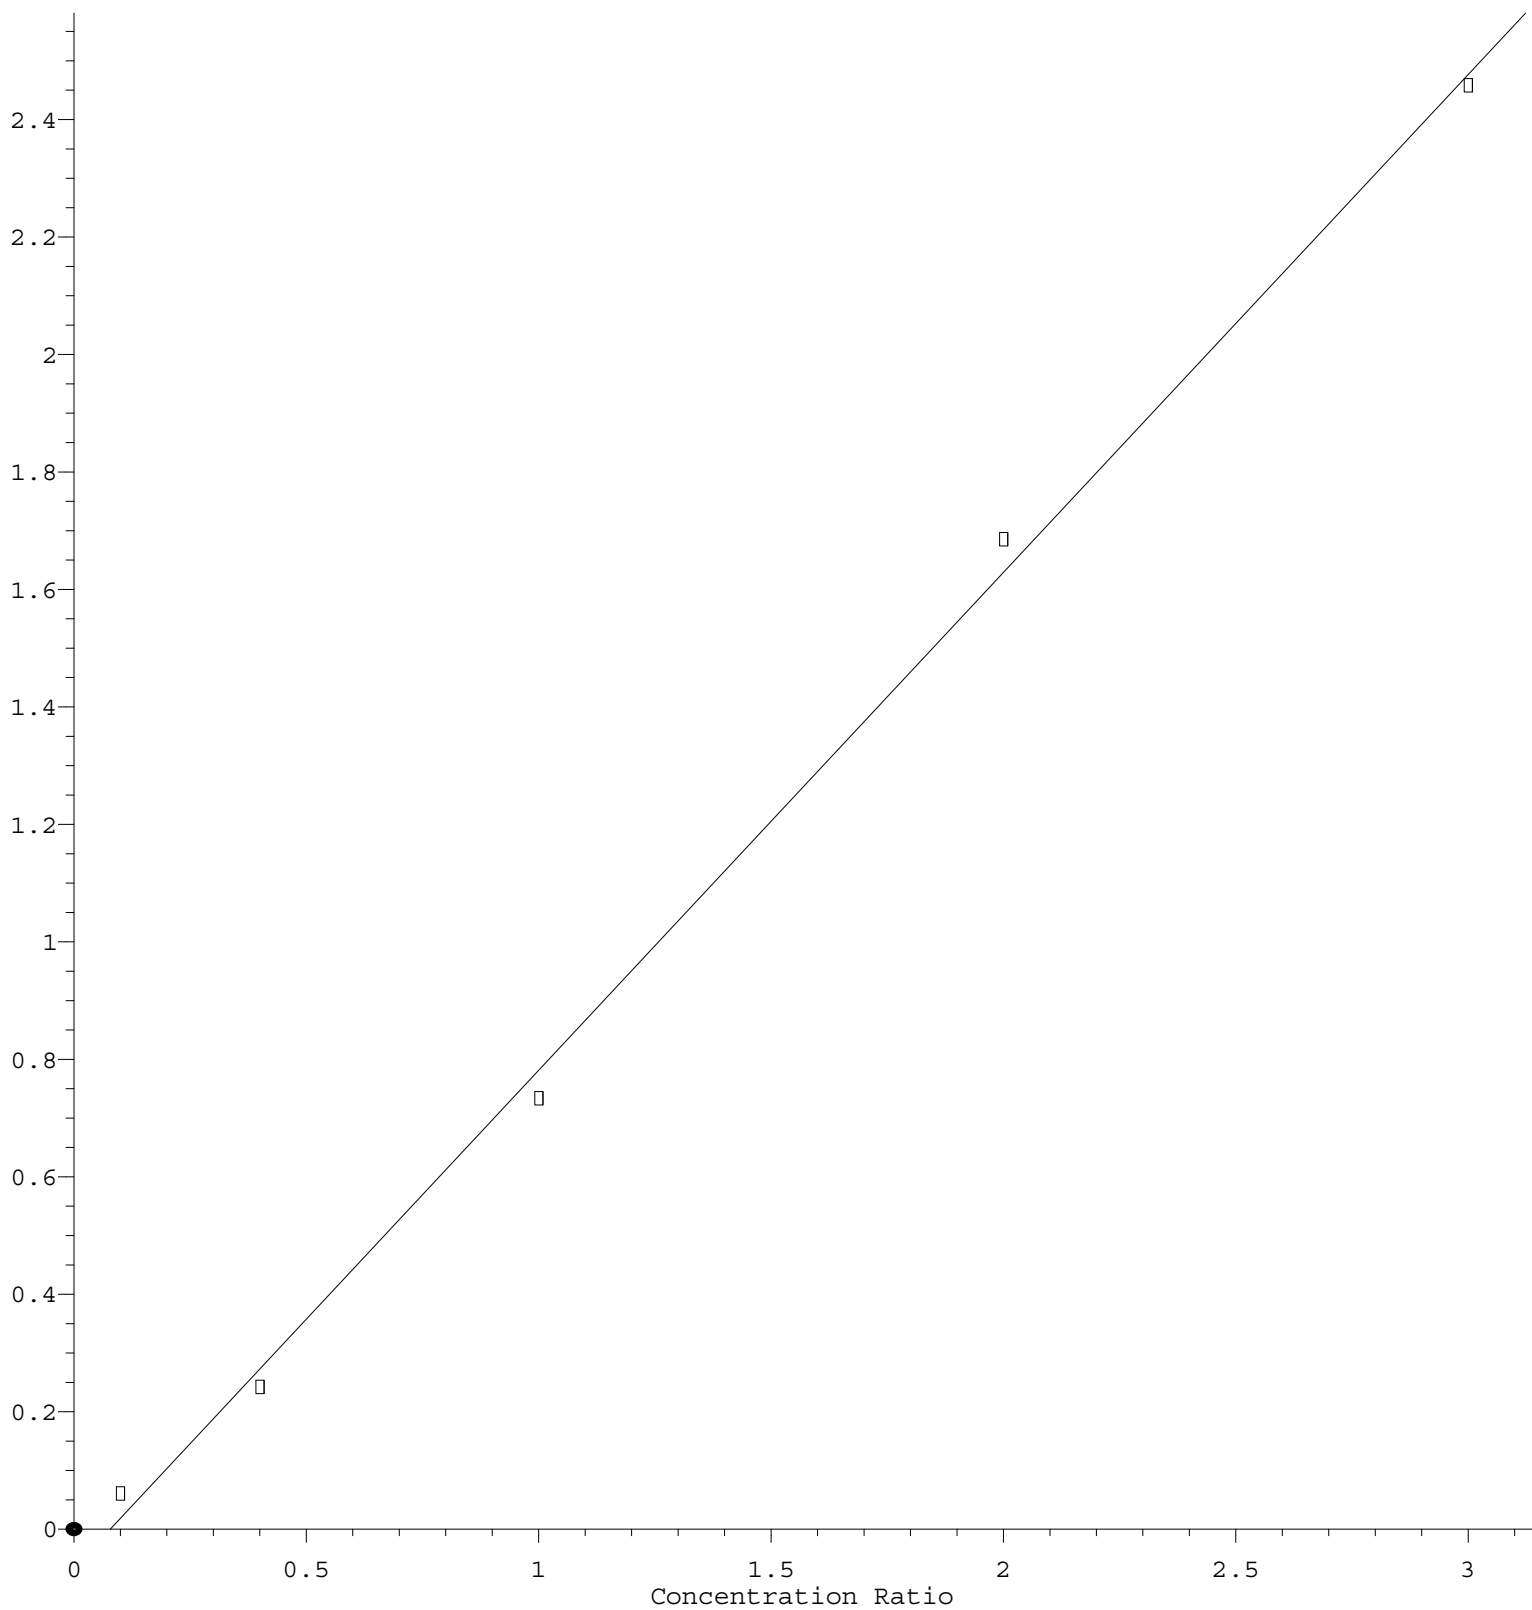

$$\text{Response} = 8.475\text{e-}001 * \text{Amt} - 6.575\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.997930 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X062321W.M

Calibration Table Last Updated: Wed Jun 23 19:12:26 2021