

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
 Data File : VX022850.D
 Acq On : 23 Jun 2021 19:18
 Operator : JC/MD
 Sample : M2783-11 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE139D2-20210617

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX022850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rVB2	8189	7986	1.91%	0.359%
2	1.569	73	79	83	rVB5	2949	5130	1.23%	0.231%
3	5.397	691	707	719	rBV2	44392	129991	31.04%	5.844%
4	5.562	721	734	745	rBV	67640	189362	45.22%	8.513%
5	5.964	788	800	812	rBV2	55969	154994	37.01%	6.968%
6	6.769	922	932	943	rBV	119734	283329	67.66%	12.738%
7	7.135	983	992	1007	rVB	87816	188201	44.94%	8.461%
8	8.653	1233	1241	1250	rBV	272125	418775	100.00%	18.827%
9	10.055	1465	1471	1485	rBV	248252	338482	80.83%	15.217%
10	11.085	1634	1640	1648	rBV	193143	242182	57.83%	10.888%
11	12.024	1789	1794	1802	rVB	217139	265892	63.49%	11.954%




Sum of corrected areas: 2224324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
Data File : VX022850.D
Acq On : 23 Jun 2021 19:18
Operator : JC/MD
Sample : M2783-11 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE139D2-20210617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

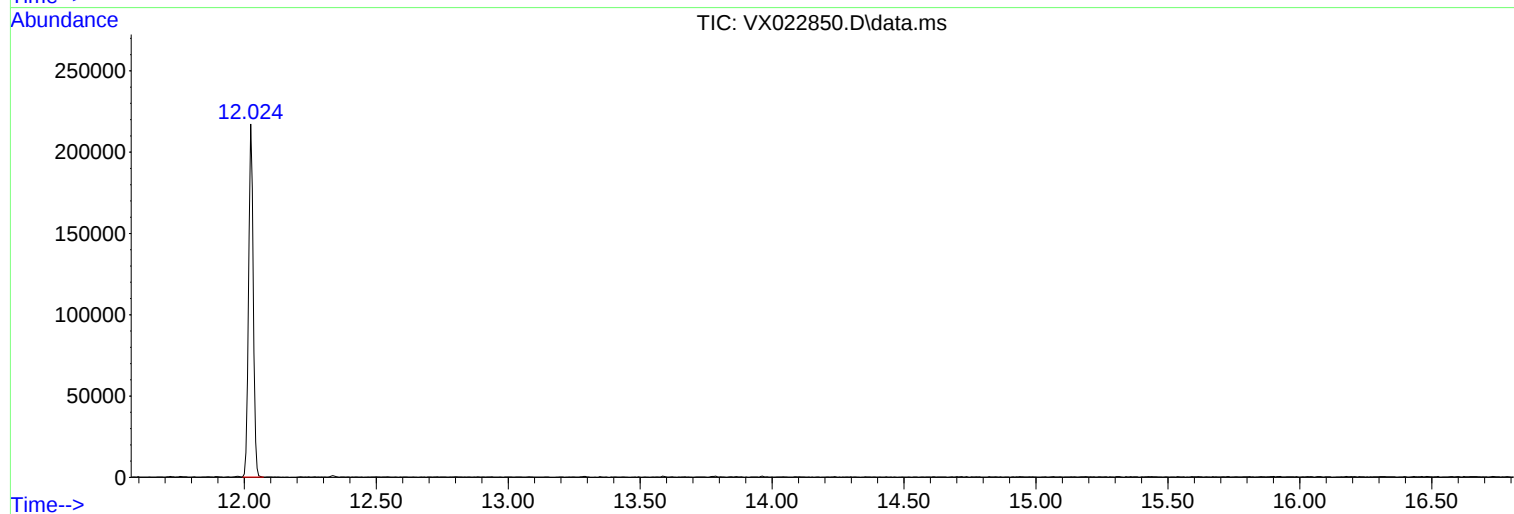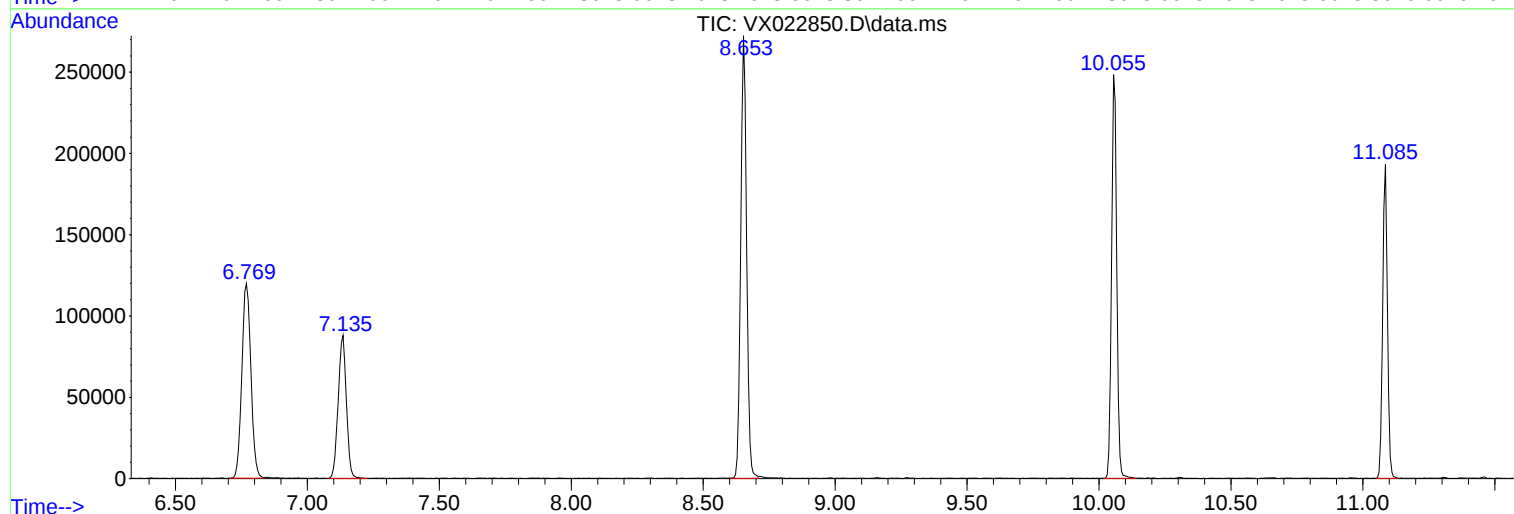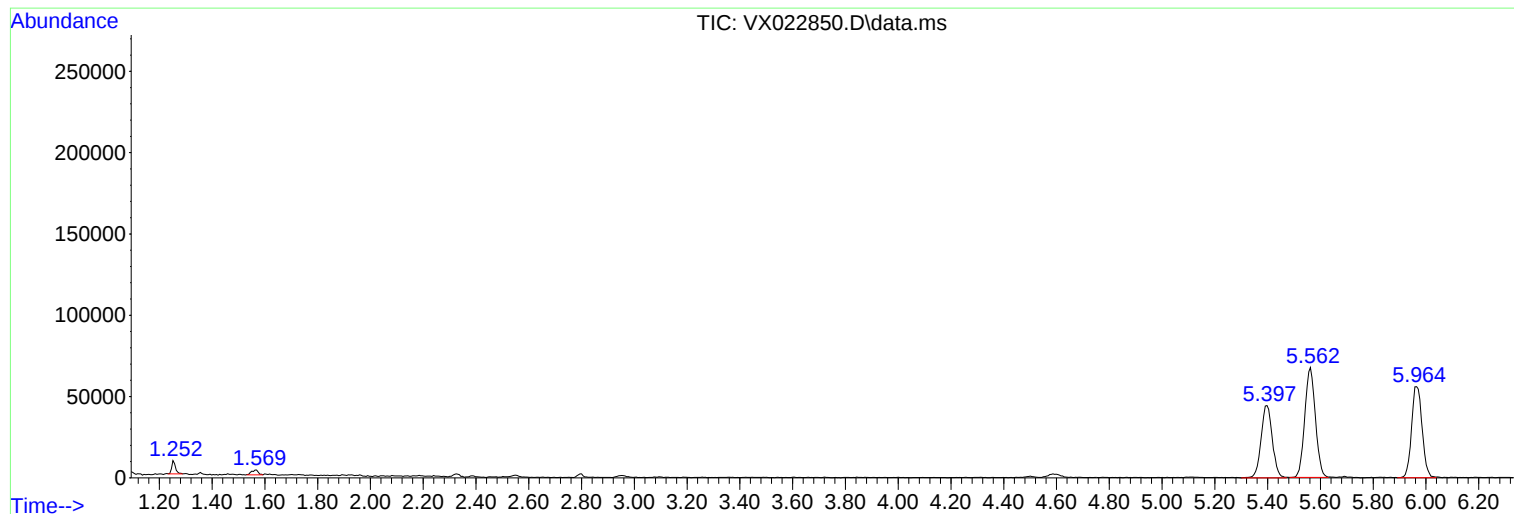

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
Data File : VX022850.D
Acq On : 23 Jun 2021 19:18
Operator : JC/MD
Sample : M2783-11 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE139D2-20210617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
Data File : VX022850.D
Acq On : 23 Jun 2021 19:18
Operator : JC/MD
Sample : M2783-11 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE139D2-20210617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------