

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
 Data File : VX022858.D
 Acq On : 23 Jun 2021 22:27
 Operator : JC/MD
 Sample : M2803-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW201D1-20210619

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Title : SW846 8260

Signal : TIC: VX022858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.568	72	79	83	rBV2	2370	3920	1.02%	0.207%
2	2.556	234	241	247	rVB2	2709	5180	1.35%	0.273%
3	2.800	275	281	286	rBV3	2548	4496	1.17%	0.237%
4	5.397	697	707	718	rBV2	42667	118472	30.82%	6.250%
5	5.556	724	733	744	rBV2	61359	176766	45.98%	9.326%
6	5.964	790	800	816	rBV2	57296	150584	39.17%	7.945%
7	6.769	920	932	946	rBV	114581	265578	69.08%	14.011%
8	8.652	1229	1241	1254	rBV	247156	384461	100.00%	20.284%
9	10.055	1466	1471	1481	rBV	219588	312622	81.31%	16.493%
10	11.085	1634	1640	1649	rBV	177411	221968	57.73%	11.711%
11	12.024	1789	1794	1803	rBV	204441	251382	65.39%	13.263%




Sum of corrected areas: 1895429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
Data File : VX022858.D
Acq On : 23 Jun 2021 22:27
Operator : JC/MD
Sample : M2803-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW201D1-20210619

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

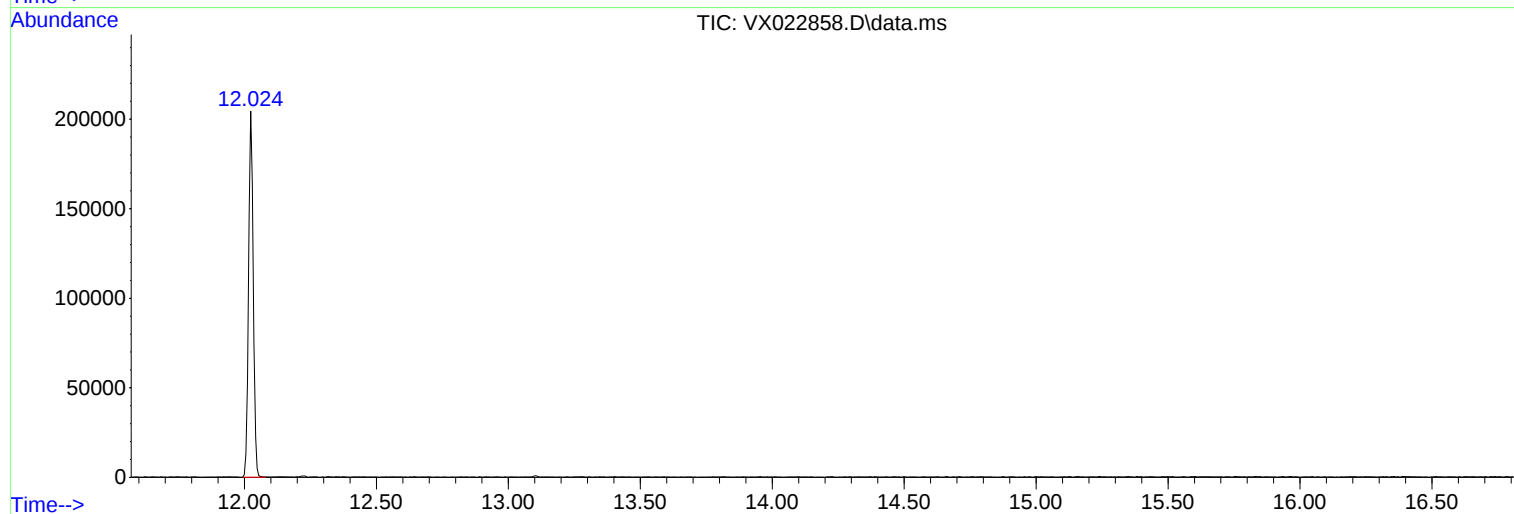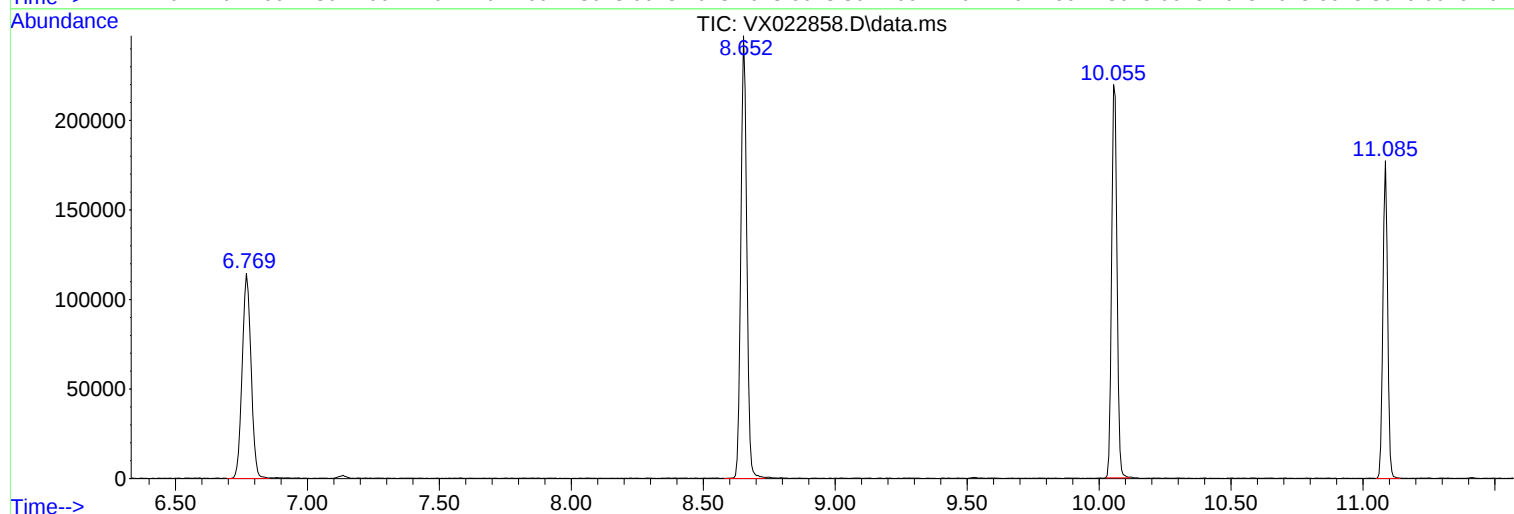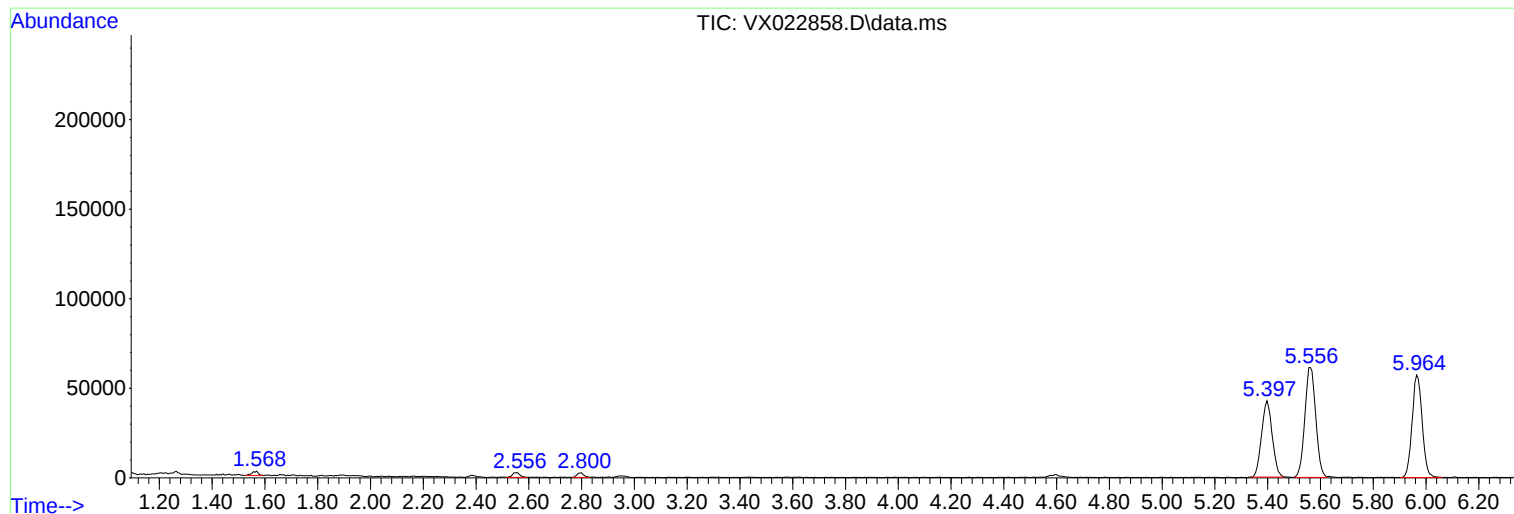

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
Data File : VX022858.D
Acq On : 23 Jun 2021 22:27
Operator : JC/MD
Sample : M2803-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW201D1-20210619

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062321\
Data File : VX022858.D
Acq On : 23 Jun 2021 22:27
Operator : JC/MD
Sample : M2803-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW201D1-20210619

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
