

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029732.D
Acq On : 23 Jun 2022 10:28
Operator : JC/MD
Sample : VX0623MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0623MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	32	34	47	rVB4	8123	21594	1.82%	0.352%
2	2.947	297	305	314	rVB	7093	15863	1.33%	0.259%
3	5.385	693	705	717	rBV2	132840	390390	32.82%	6.370%
4	5.550	720	732	746	rVV2	220171	628651	52.86%	10.257%
5	5.958	789	799	818	rBV	136302	362233	30.46%	5.910%
6	6.763	920	931	946	rBV	366990	877260	73.76%	14.314%
7	8.647	1234	1240	1250	rBV	753431	1189316	100.00%	19.405%
8	10.055	1465	1471	1481	rBV	764978	1002671	84.31%	16.360%
9	11.079	1634	1639	1650	rBV	575659	742234	62.41%	12.111%
10	12.024	1788	1794	1807	rBV	700620	898605	75.56%	14.662%




Sum of corrected areas: 6128817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029732.D
Acq On : 23 Jun 2022 10:28
Operator : JC/MD
Sample : VX0623MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0623MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

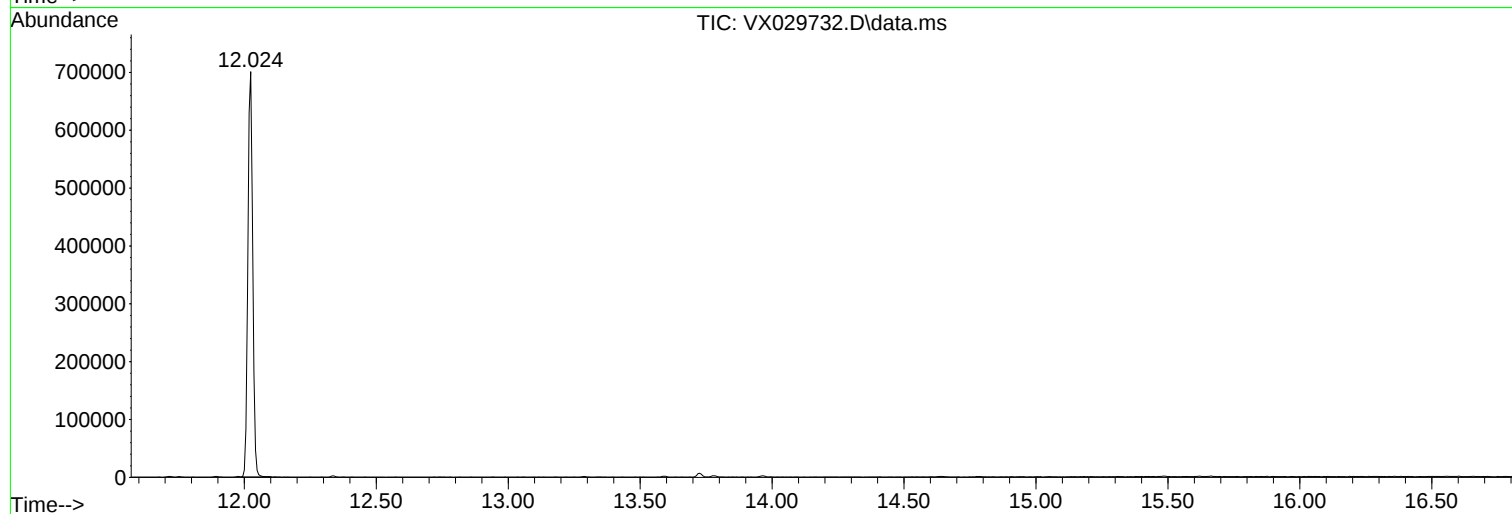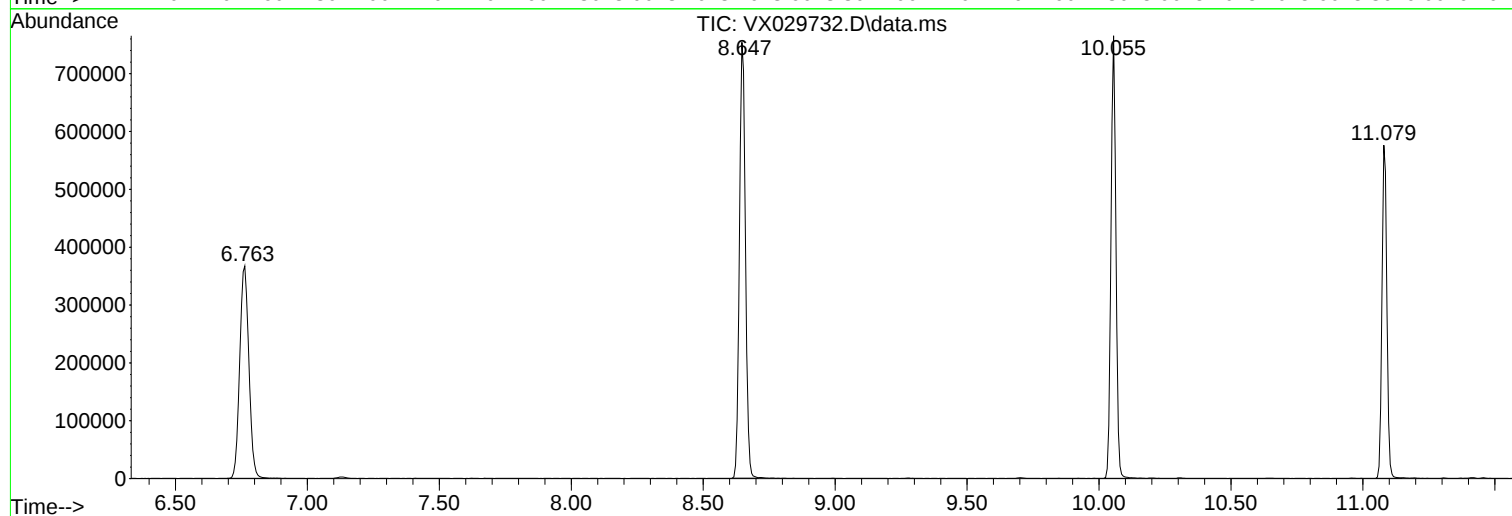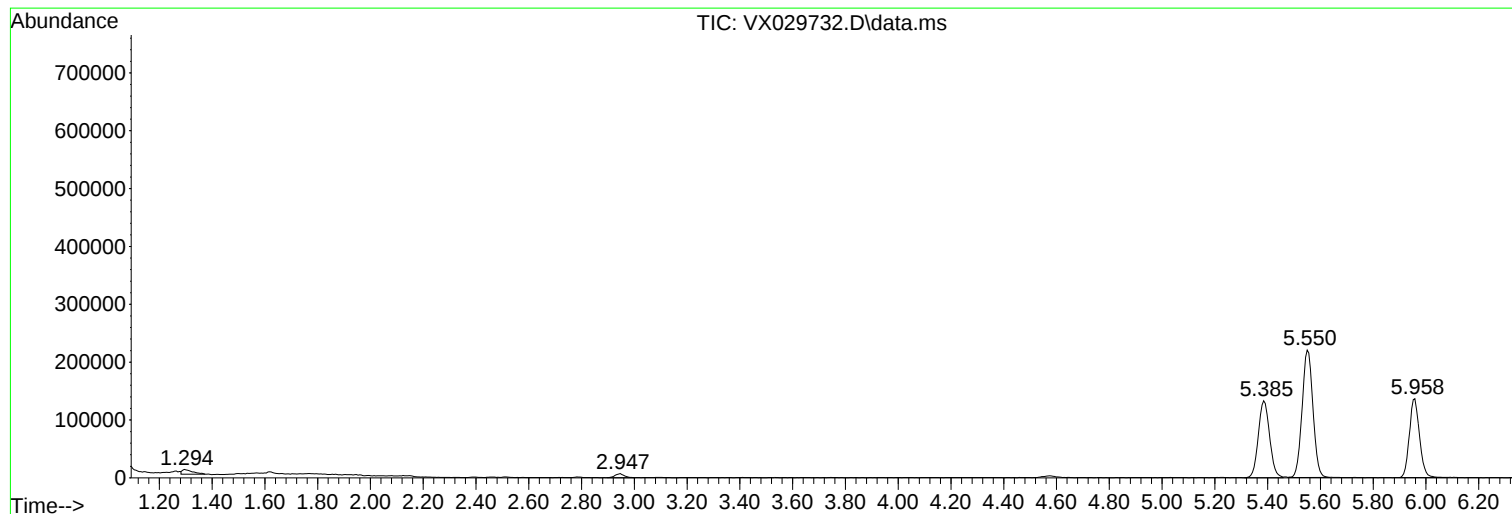

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029732.D
Acq On : 23 Jun 2022 10:28
Operator : JC/MD
Sample : VX0623MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0623MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029732.D
Acq On : 23 Jun 2022 10:28
Operator : JC/MD
Sample : VX0623MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0623MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
