

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
 Data File : VX029736.D
 Acq On : 23 Jun 2022 12:11
 Operator : JC/MD
 Sample : N3202-04 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-16

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	26	31	44	rBV2	12849	36150	2.90%	0.424%
2	1.752	104	109	114	rBV	16559	22774	1.83%	0.267%
3	2.788	268	279	282	rBV5	4728	12836	1.03%	0.151%
4	2.867	287	292	298	rVV2	10015	21140	1.70%	0.248%
5	2.941	298	304	318	rVB	23005	60343	4.84%	0.708%
6	3.111	322	332	348	rBV2	26304	63439	5.09%	0.744%
7	4.312	517	529	538	rVB3	12246	36371	2.92%	0.427%
8	4.568	563	571	582	rBV2	5883	18848	1.51%	0.221%
9	5.391	694	706	717	rBV	141377	413120	33.16%	4.845%
10	5.556	723	733	754	rVB	266526	769594	61.77%	9.025%
11	5.958	790	799	807	rBV	147671	391472	31.42%	4.591%
12	6.044	807	813	824	rVV	53933	143022	11.48%	1.677%
13	6.202	826	839	845	rVV7	5129	19218	1.54%	0.225%
14	6.763	921	931	952	rBV	404299	958315	76.91%	11.239%
15	8.653	1234	1241	1248	rBV	782606	1245943	100.00%	14.612%
16	8.720	1248	1252	1259	rVB	19755	31621	2.54%	0.371%
17	10.055	1460	1471	1482	rBV	802756	1075870	86.35%	12.617%
18	10.195	1489	1494	1501	rBV	586871	746554	59.92%	8.755%
19	10.305	1506	1512	1520	rVB	68876	90899	7.30%	1.066%
20	10.646	1562	1568	1577	rVB	41862	56882	4.57%	0.667%
21	10.964	1613	1620	1627	rBV	32717	41740	3.35%	0.490%
22	11.085	1634	1640	1649	rBV	602725	786657	63.14%	9.226%
23	11.305	1667	1676	1684	rBV	52194	69841	5.61%	0.819%
24	11.402	1684	1692	1697	rVV2	9978	19654	1.58%	0.230%
25	11.616	1721	1727	1734	rVB	33738	43814	3.52%	0.514%
26	11.756	1746	1750	1755	rVB2	14577	18817	1.51%	0.221%
27	12.024	1788	1794	1801	rBV	789069	967080	77.62%	11.341%
28	12.091	1801	1805	1810	rVB	28273	35872	2.88%	0.421%
29	12.244	1824	1830	1837	rBV2	101253	125507	10.07%	1.472%
30	12.414	1852	1858	1863	rBV2	10703	15070	1.21%	0.177%
31	12.616	1886	1891	1894	rBV	21852	26986	2.17%	0.316%
32	12.701	1900	1905	1912	rBV2	12501	17949	1.44%	0.210%
33	13.292	1993	2002	2008	rBV2	14472	20258	1.63%	0.238%
34	13.774	2076	2081	2090	rBV	96231	123272	9.89%	1.446%

Sum of corrected areas: 8526928




Instrument :
MSVOA_X
ClientSampleId :
MW-16

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029736.D
Acq On : 23 Jun 2022 12:11
Operator : JC/MD
Sample : N3202-04 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

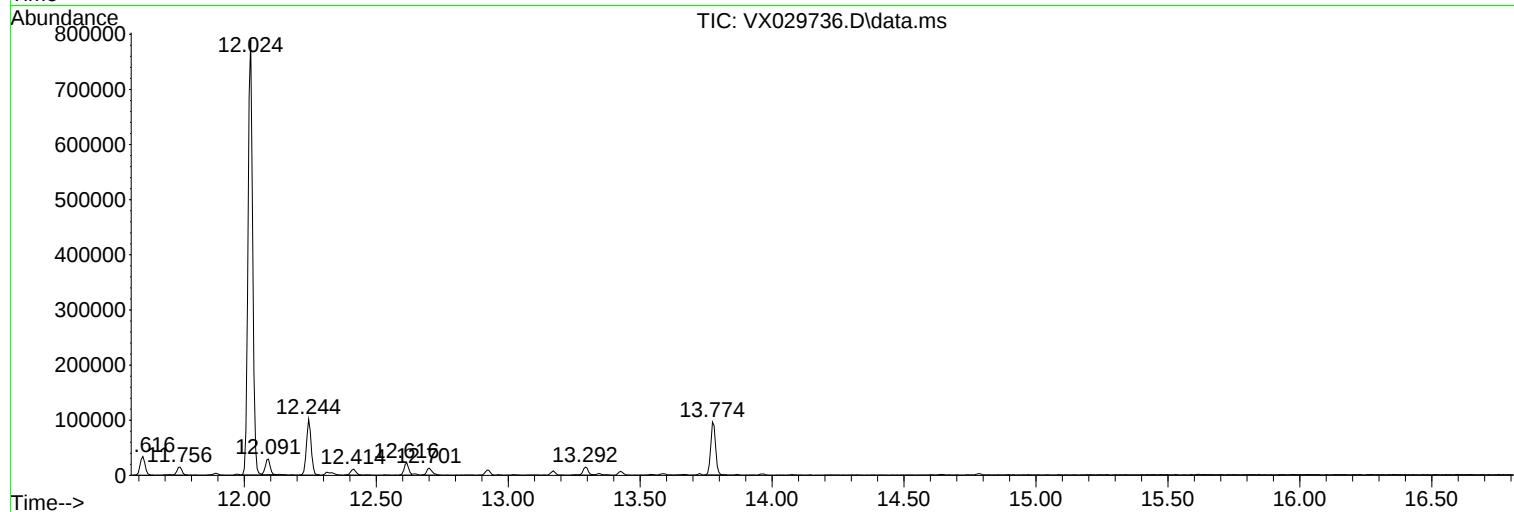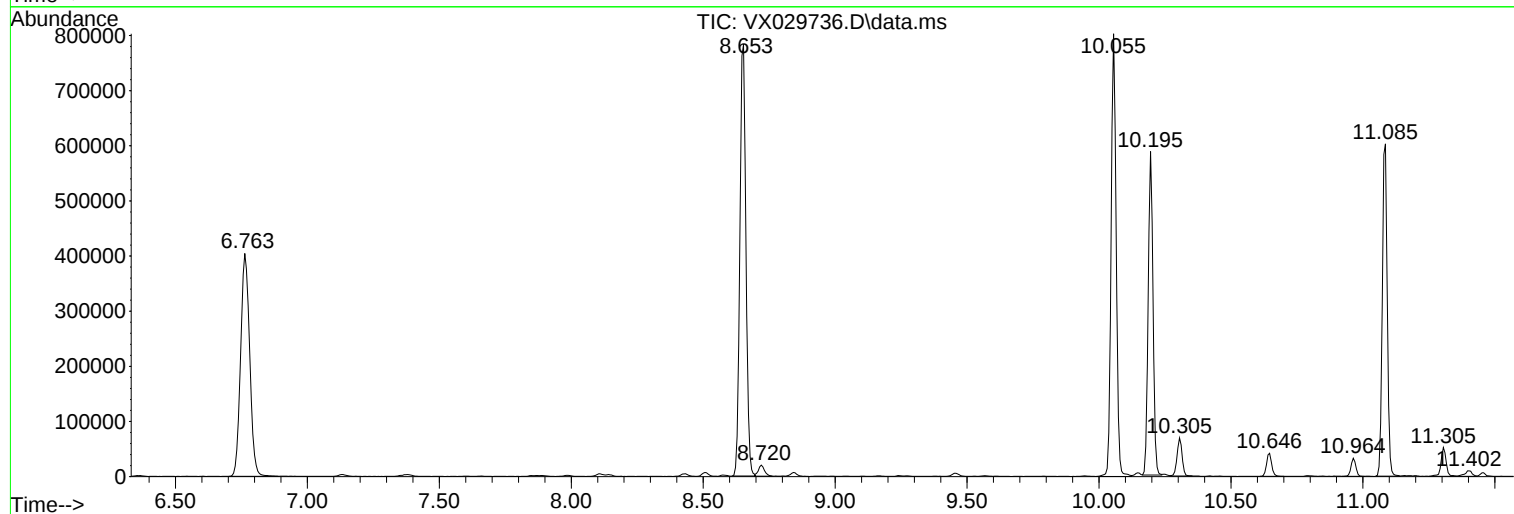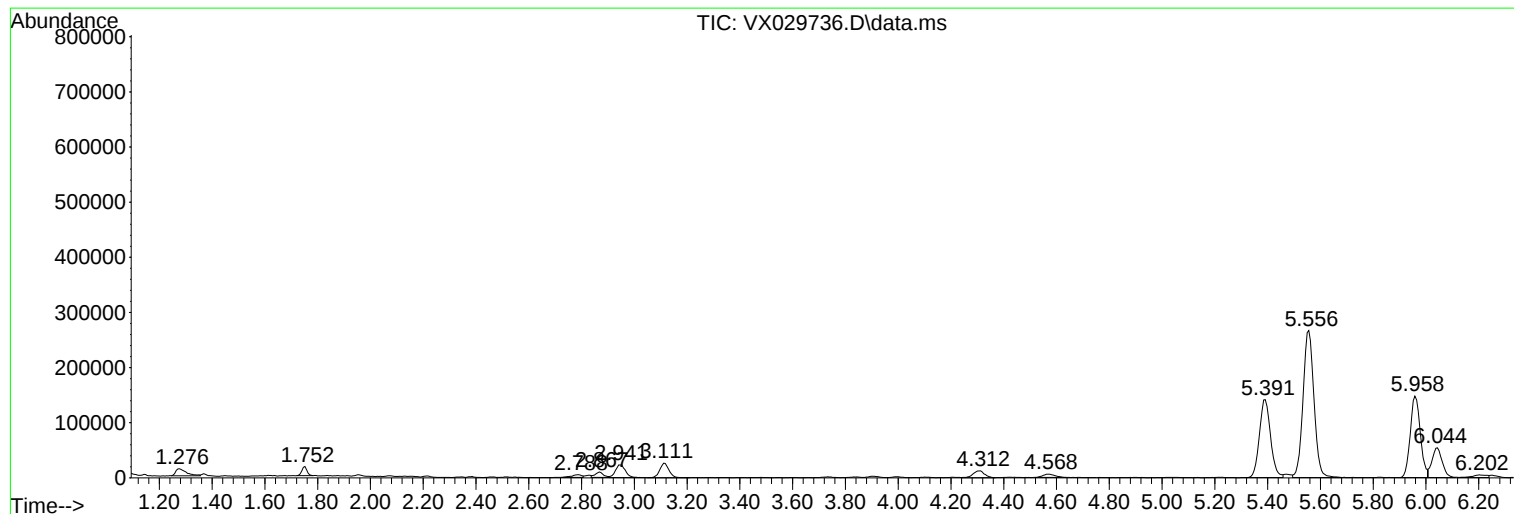

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029736.D
Acq On : 23 Jun 2022 12:11
Operator : JC/MD
Sample : N3202-04 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.244	6.49 ug/l	125507	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	81
2			Benzene, 2-propenyl-	118	C9H10	000300-57-2	72
3			Benzene, 1-ethenyl-2-methyl-	118	C9H10	000611-15-4	72
4			Benzene, cyclopropyl-	118	C9H10	000873-49-4	72
5			Benzeneethanol, .beta.-ethenyl-....	162	C11H14O	040596-14-3	50

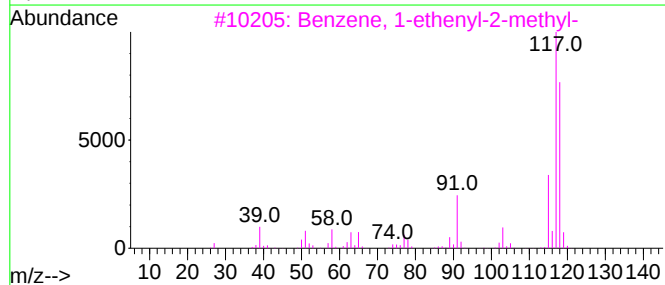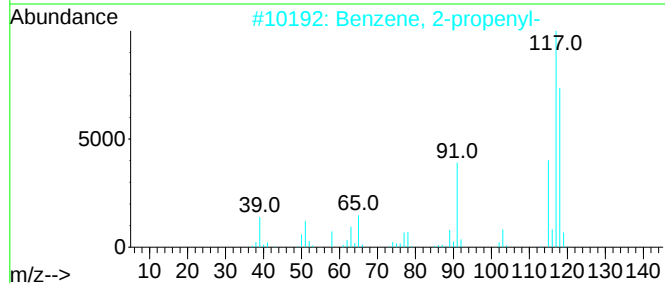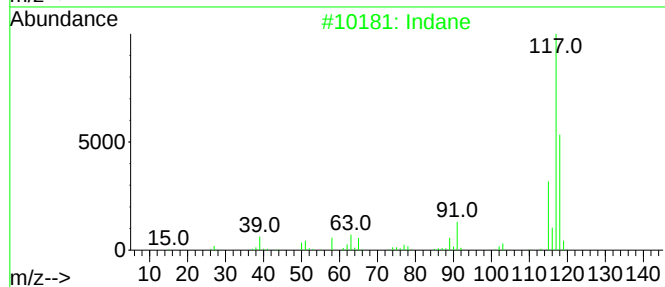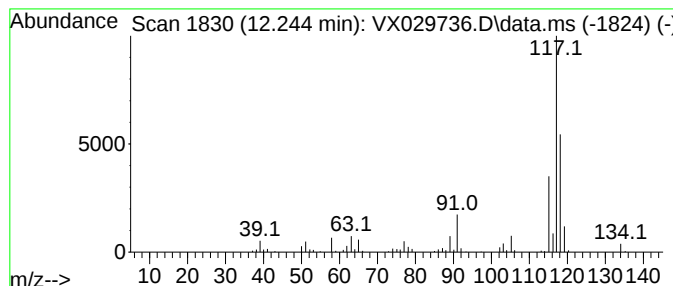

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062322\
Data File : VX029736.D
Acq On : 23 Jun 2022 12:11
Operator : JC/MD
Sample : N3202-04 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.244	6.5	ug/l	125507	4	12.024	967080	50.0