

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062323\
 Data File : VX036295.D
 Acq On : 23 Jun 2023 17:23
 Operator : JC/MD
 Sample : 03366-05RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB02RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

Signal : TIC: VX036295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.398	210	215	222	rVB2	2194	4991	1.19%	0.195%
2	4.568	561	571	587	rBV2	8411	32481	7.78%	1.266%
3	5.385	695	705	720	rBV	68567	200539	48.00%	7.818%
4	5.550	720	732	745	rVV2	92310	265569	63.57%	10.353%
5	5.958	787	799	817	rBV	87099	236442	56.60%	9.217%
6	6.763	920	931	945	rBV	157055	377224	90.30%	14.705%
7	8.647	1233	1240	1249	rBV	264752	417756	100.00%	16.285%
8	10.055	1465	1471	1482	rBV	244435	334470	80.06%	13.039%
9	11.079	1634	1639	1652	rVB	172248	229204	54.87%	8.935%
10	12.018	1788	1793	1800	rBV	181195	239612	57.36%	9.341%
11	13.262	1992	1997	2000	rBV5	3273	4849	1.16%	0.189%
12	13.847	2088	2093	2099	rVB7	2145	4558	1.09%	0.178%
13	14.036	2120	2124	2127	rVB4	4561	5387	1.29%	0.210%
14	14.225	2146	2155	2159	rVB7	5568	10852	2.60%	0.423%
15	14.481	2191	2197	2206	rBV7	5864	10533	2.52%	0.411%
16	14.615	2215	2219	2222	rBV4	9133	12714	3.04%	0.496%
17	14.670	2225	2228	2233	rVB3	3775	5209	1.25%	0.203%
18	14.755	2238	2242	2245	rVV2	10744	10883	2.61%	0.424%
19	15.036	2284	2288	2293	rBV7	2778	5184	1.24%	0.202%
20	15.103	2294	2299	2302	rBV6	2910	5437	1.30%	0.212%
21	15.182	2307	2312	2314	rVV3	9476	15347	3.67%	0.598%
22	15.206	2314	2316	2320	rVV3	11600	15631	3.74%	0.609%
23	15.274	2324	2327	2331	rVV5	5159	7211	1.73%	0.281%
24	15.371	2338	2343	2348	rBV7	4384	8047	1.93%	0.314%
25	15.487	2357	2362	2368	rBV2	30367	47365	11.34%	1.846%
26	15.609	2379	2382	2386	rVB6	5580	7759	1.86%	0.302%
27	16.030	2449	2451	2455	rVB5	4855	6171	1.48%	0.241%
28	16.084	2455	2460	2469	rBV9	5679	16876	4.04%	0.658%
29	16.371	2501	2507	2514	rVB7	7665	15832	3.79%	0.617%
30	16.590	2540	2543	2549	rVB8	3373	5321	1.27%	0.207%
31	16.645	2549	2552	2559	rVV9	3020	5753	1.38%	0.224%




Sum of corrected areas: 2565207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062323\
Data File : VX036295.D
Acq On : 23 Jun 2023 17:23
Operator : JC/MD
Sample : 03366-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB02RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

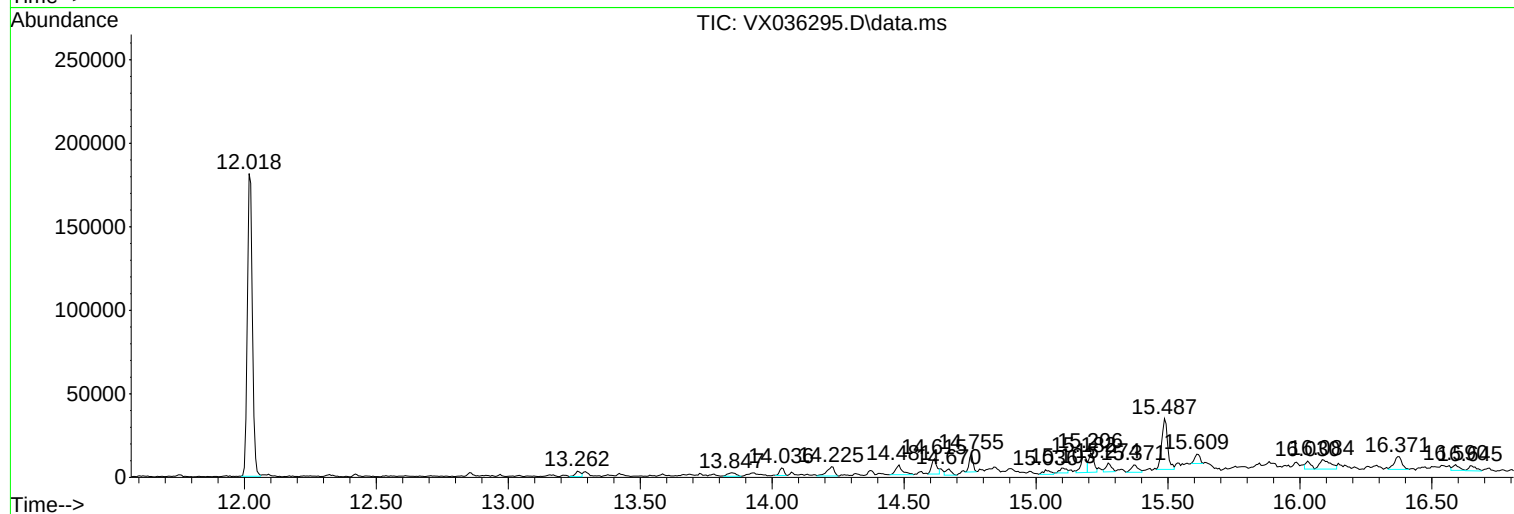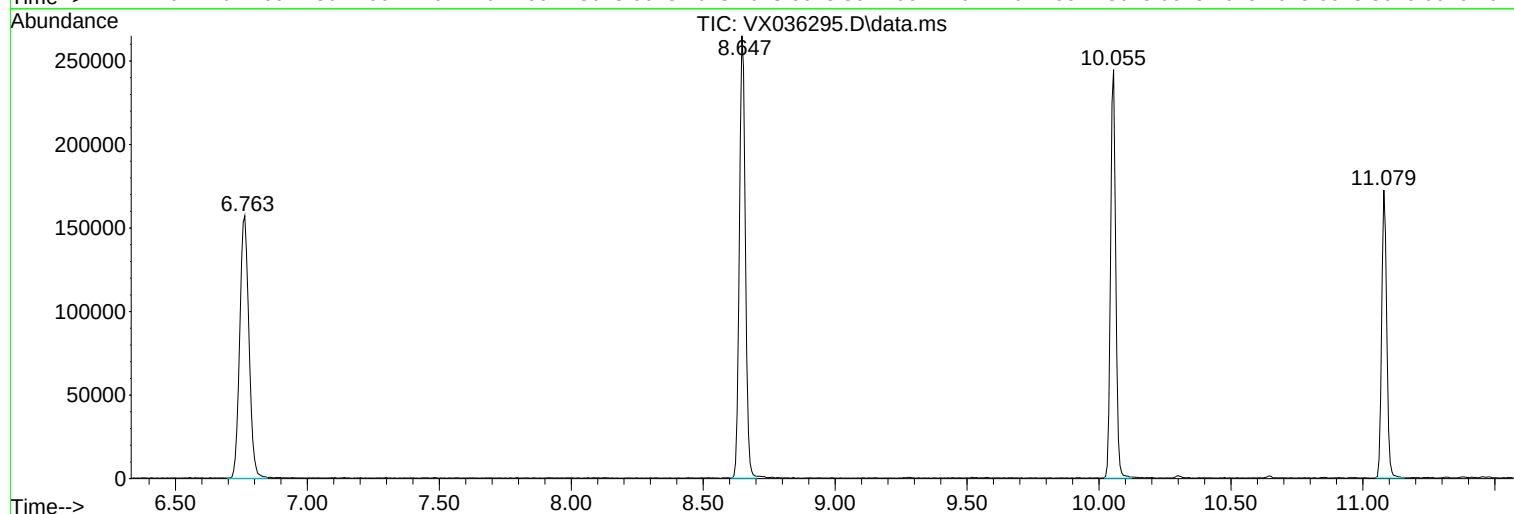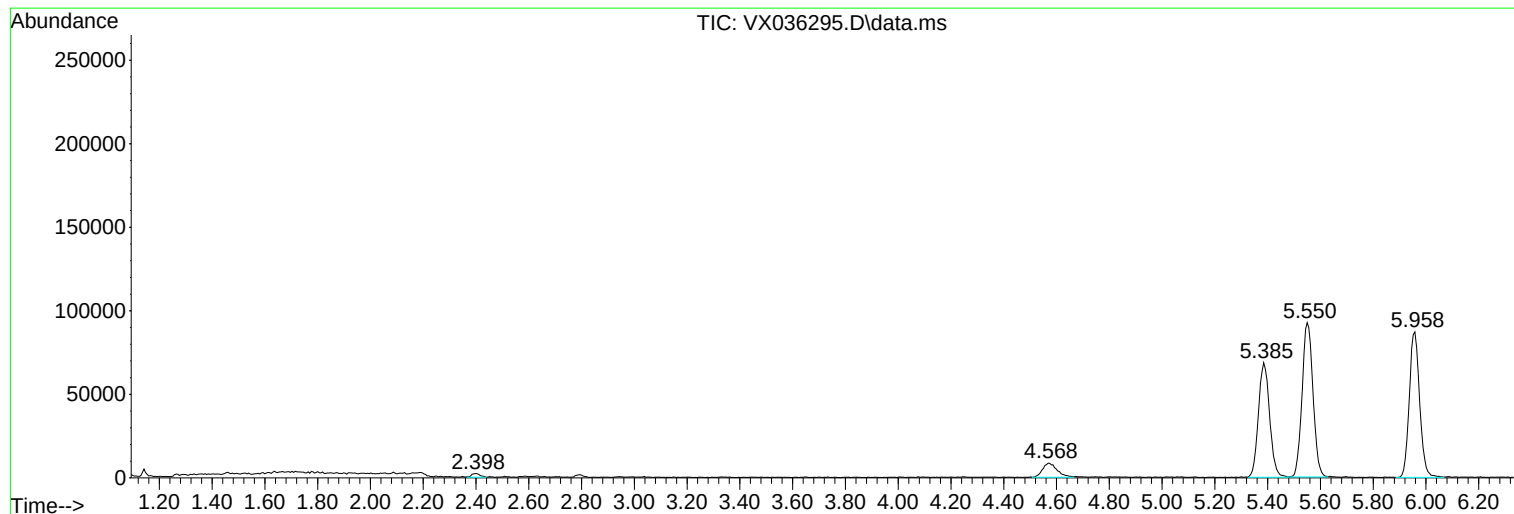

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062323\
Data File : VX036295.D
Acq On : 23 Jun 2023 17:23
Operator : JC/MD
Sample : 03366-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB02RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062323\
Data File : VX036295.D
Acq On : 23 Jun 2023 17:23
Operator : JC/MD
Sample : 03366-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB02RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------