

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
 Data File : VX046820.D
 Acq On : 23 Jun 2025 15:11
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
 Title : SW846 8260

Signal : TIC: VX046820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.397	698	707	725	rBV2	67498	216256	32.14%	5.577%
2	5.568	725	735	759	rVB2	114182	352384	52.38%	9.088%
3	5.970	791	801	825	rBV	79880	224669	33.39%	5.794%
4	6.769	924	932	950	rBV	191715	486467	72.31%	12.546%
5	8.653	1234	1241	1259	rBV	421767	672767	100.00%	17.350%
6	10.055	1465	1471	1482	rBV	432217	583546	86.74%	15.049%
7	10.201	1489	1495	1502	rVB	5818	9255	1.38%	0.239%
8	10.305	1507	1512	1518	rVV	25726	37774	5.61%	0.974%
9	10.646	1563	1568	1577	rBV2	4398	7166	1.07%	0.185%
10	11.079	1634	1639	1651	rBV	357385	462346	68.72%	11.923%
11	11.475	1700	1704	1710	rVB	13833	17456	2.59%	0.450%
12	12.018	1788	1793	1800	rBV	460523	586740	87.21%	15.131%
13	12.097	1804	1806	1811	rVV3	5886	8167	1.21%	0.211%
14	12.170	1815	1818	1825	rVB4	5520	7623	1.13%	0.197%
15	12.420	1855	1859	1864	rBV	28234	33577	4.99%	0.866%
16	12.817	1919	1924	1929	rVB8	4603	7465	1.11%	0.193%
17	12.884	1929	1935	1936	rBV3	6313	7965	1.18%	0.205%
18	12.975	1947	1950	1955	rVB4	6630	7833	1.16%	0.202%
19	13.268	1993	1998	2001	rBV	27313	35645	5.30%	0.919%
20	13.384	2014	2017	2019	rBV	6933	6780	1.01%	0.175%
21	13.731	2071	2074	2077	rVB4	5704	6994	1.04%	0.180%
22	13.835	2088	2091	2095	rVB3	6272	9511	1.41%	0.245%
23	14.036	2120	2124	2128	rBV	27516	29087	4.32%	0.750%
24	14.499	2197	2200	2206	rVB4	5503	8346	1.24%	0.215%
25	14.609	2215	2218	2224	rBV5	5537	7770	1.15%	0.200%
26	14.755	2238	2242	2246	rBV	23159	27113	4.03%	0.699%
27	15.487	2358	2362	2366	rBV2	11716	16906	2.51%	0.436%




Sum of corrected areas: 3877608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046820.D
Acq On : 23 Jun 2025 15:11
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

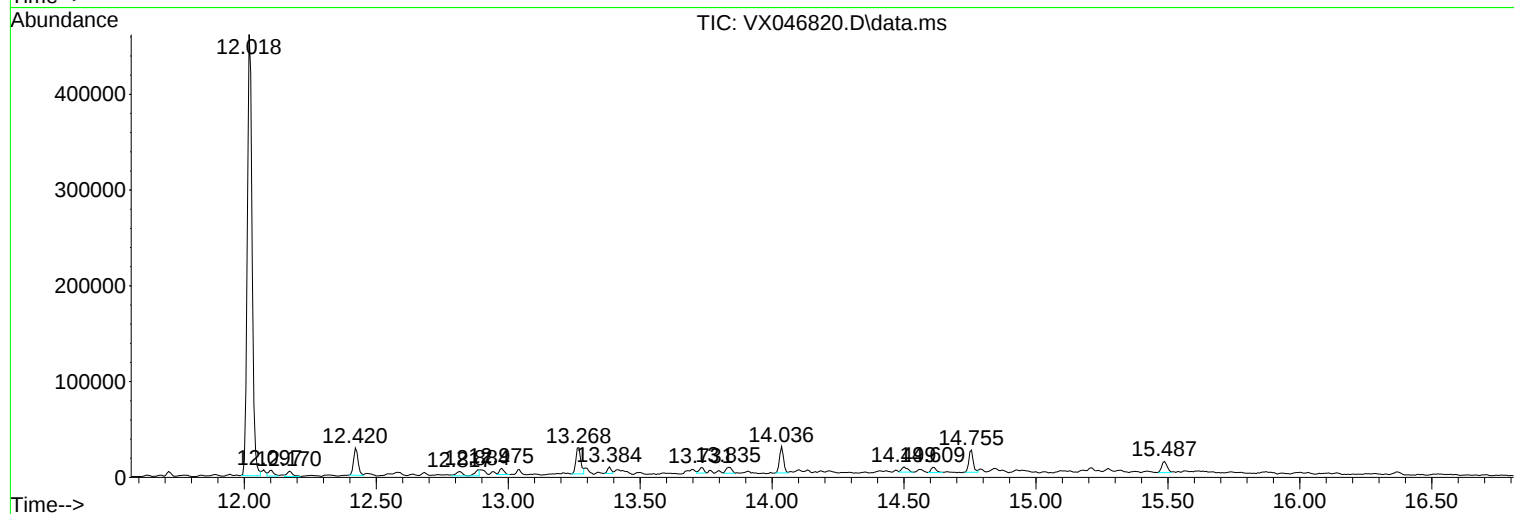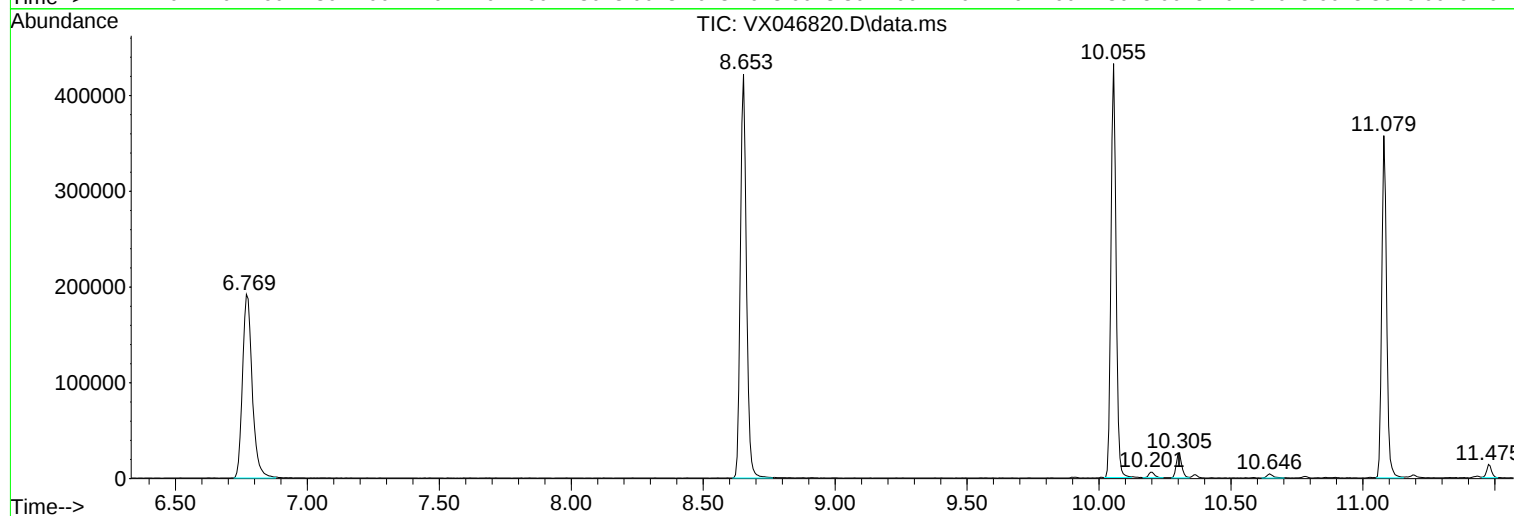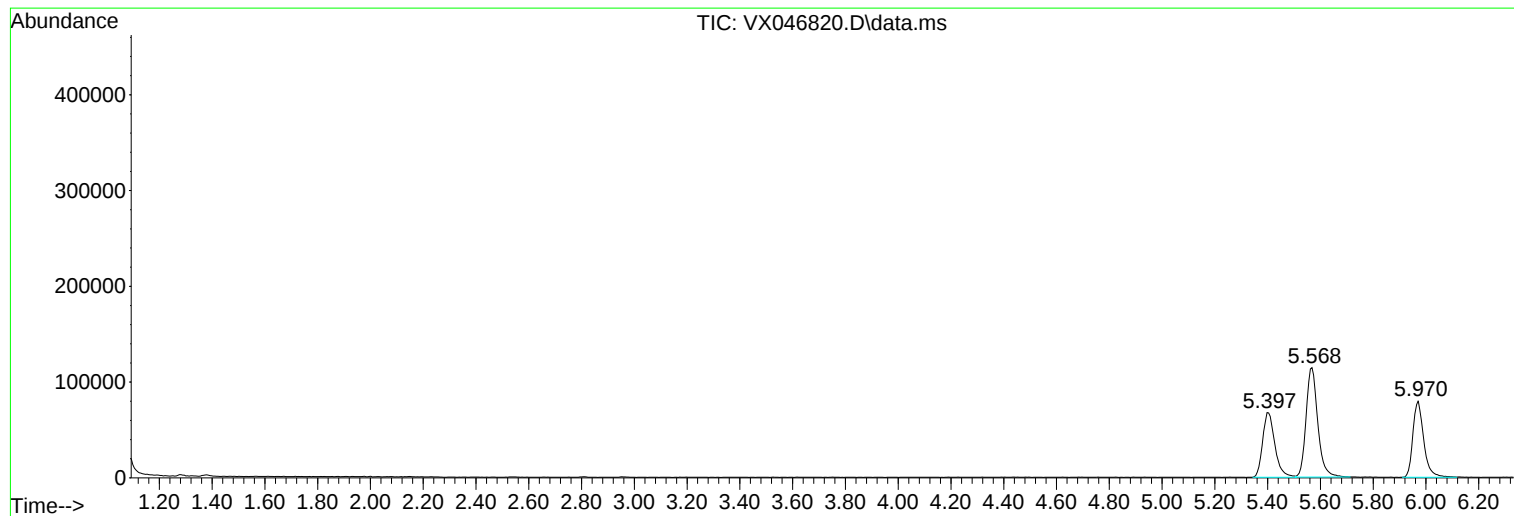

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046820.D
Acq On : 23 Jun 2025 15:11
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046820.D
Acq On : 23 Jun 2025 15:11
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc