

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
 Data File : VX046822.D
 Acq On : 23 Jun 2025 15:55
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M

Title : SW846 8260

Signal : TIC: VX046822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.403	694	708	724	rBV2	111521	351323	32.51%	5.971%
2	5.568	724	735	759	rVB	190982	582577	53.90%	9.901%
3	5.970	791	801	824	rBV2	124201	358526	33.17%	6.093%
4	6.769	923	932	956	rBV	308758	791158	73.20%	13.446%
5	8.653	1234	1241	1260	rBV	669371	1080815	100.00%	18.369%
6	10.055	1465	1471	1484	rBV	685362	927687	85.83%	15.767%
7	11.079	1634	1639	1651	rBV	560081	728010	67.36%	12.373%
8	11.475	1700	1704	1711	rVB	10021	14085	1.30%	0.239%
9	12.018	1788	1793	1800	rBV	737958	930204	86.07%	15.809%
10	12.420	1854	1859	1864	rBV	22190	27211	2.52%	0.462%
11	13.268	1993	1998	2001	rBV	22634	29157	2.70%	0.496%
12	14.036	2120	2124	2128	rBV	20747	23308	2.16%	0.396%
13	14.755	2237	2242	2245	rBV	18914	22406	2.07%	0.381%
14	15.487	2357	2362	2369	rBV2	12232	17409	1.61%	0.296%




Sum of corrected areas: 5883876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046822.D
Acq On : 23 Jun 2025 15:55
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

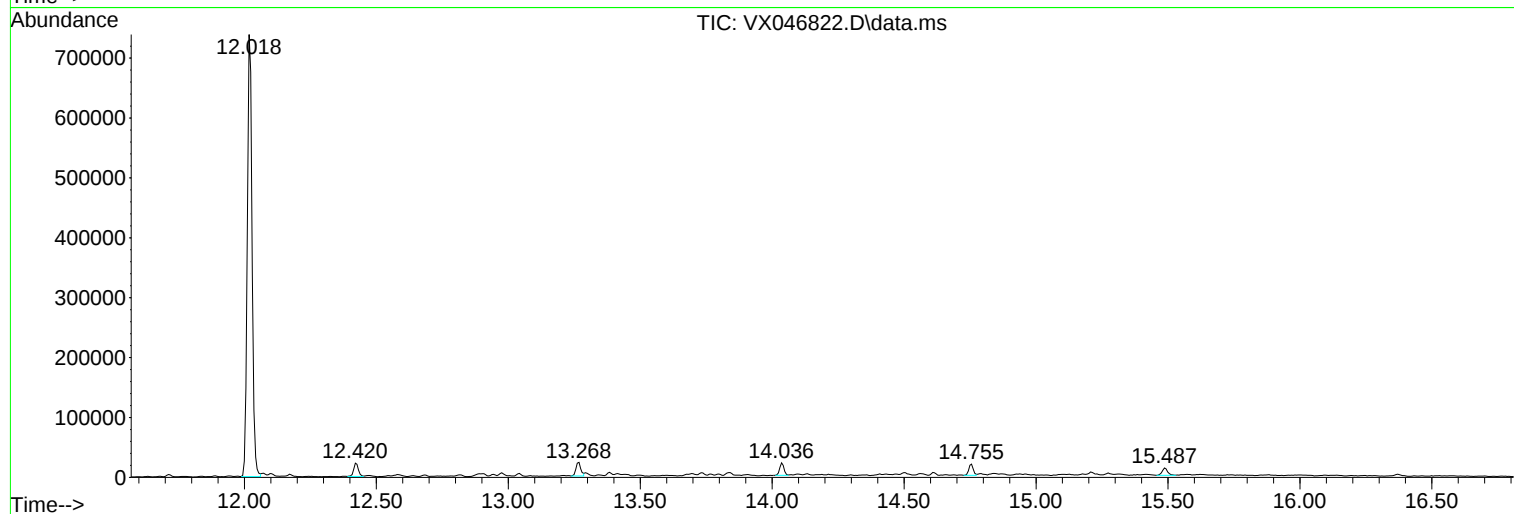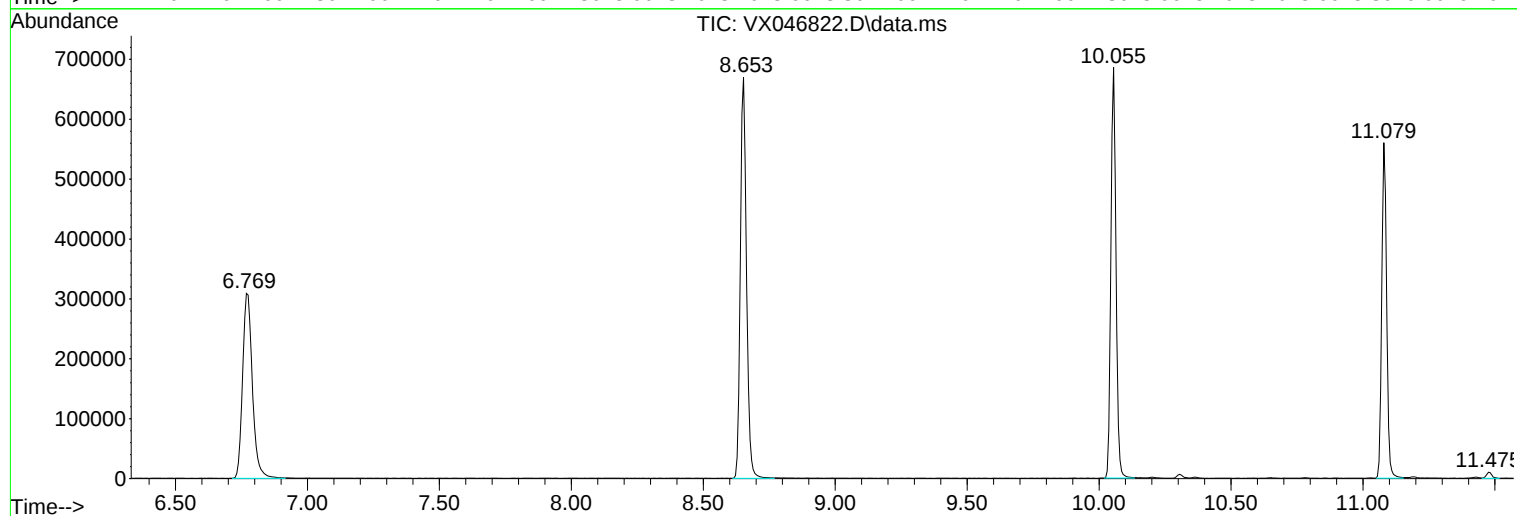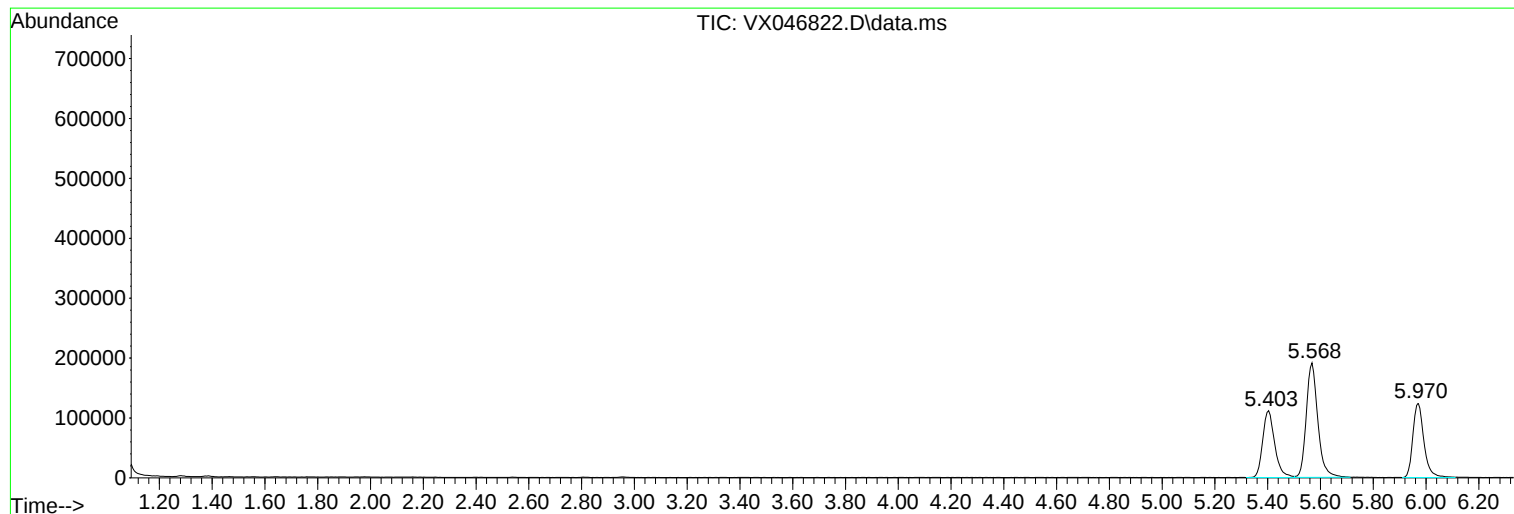

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046822.D
Acq On : 23 Jun 2025 15:55
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046822.D
Acq On : 23 Jun 2025 15:55
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc