


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062325\
Data File : VX046803.D
Acq On : 23 Jun 2025 08:05
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Title : SW846 8260
Last Update : Wed Jun 18 03:09:16 2025

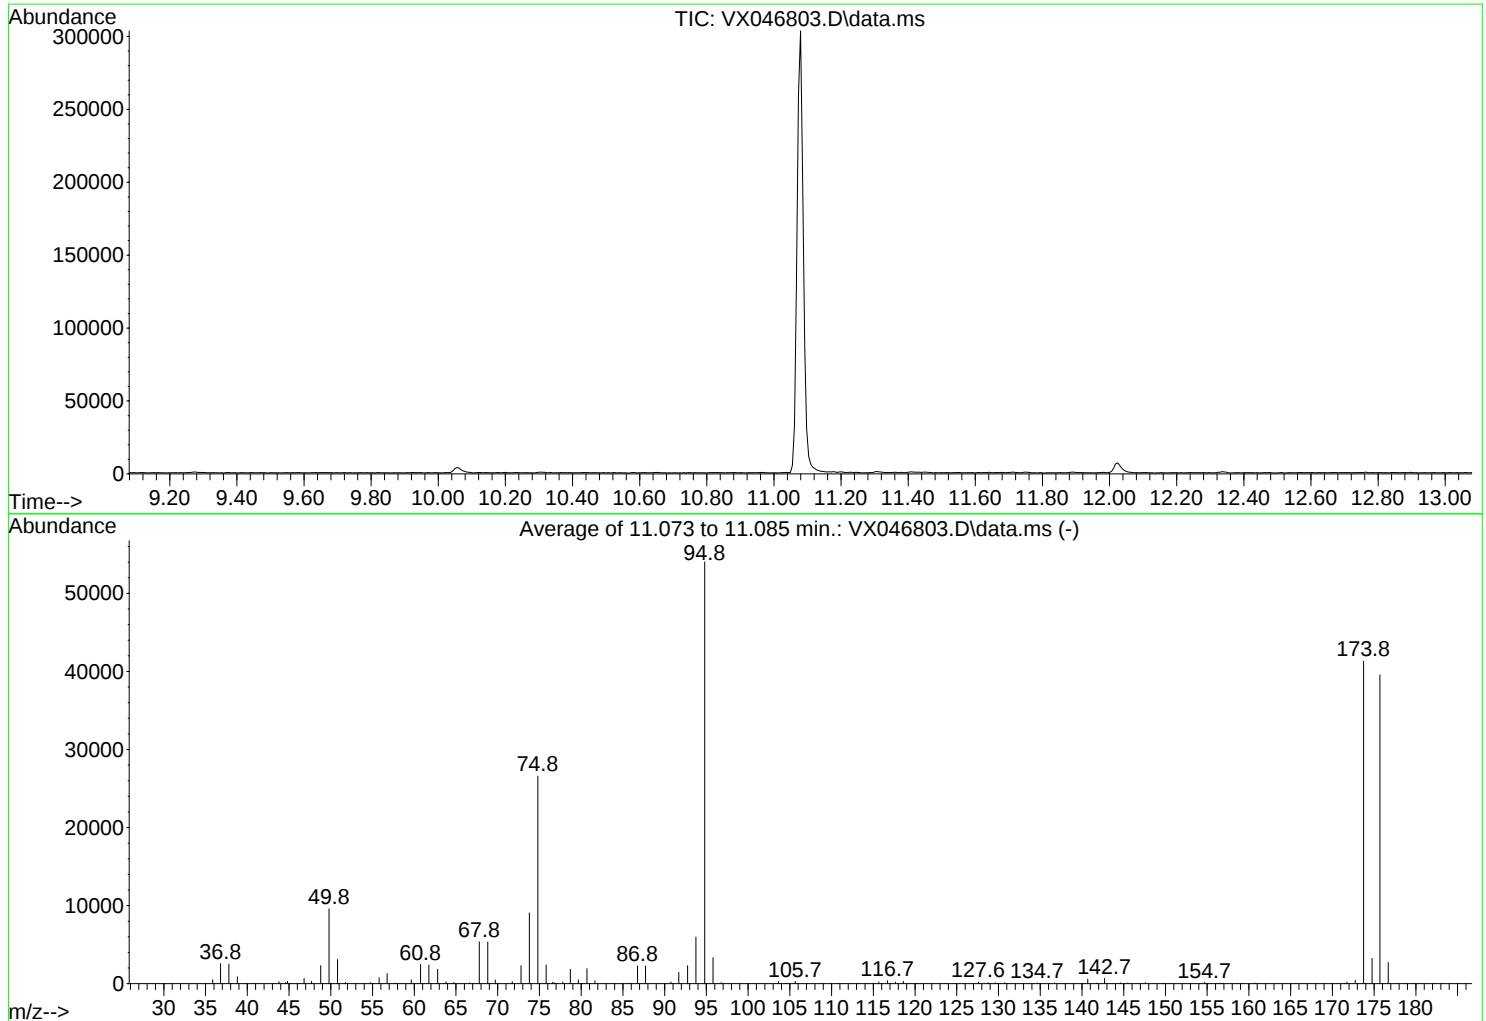

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	9595	PASS
75	95	30	60	49.2	26589	PASS
95	95	100	100	100.0	54040	PASS
96	95	5	9	6.1	3323	PASS
173	174	0.00	2	1.1	435	PASS
174	95	50	100	76.4	41304	PASS
175	174	5	9	7.8	3230	PASS
176	174	95	101	95.8	39555	PASS
177	176	5	9	6.8	2700	PASS