

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062419\
 Data File : VX010416.D
 Acq On : 24 Jun 2019 17:01
 Operator : JC/SP
 Sample : K3164-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BAT-B03

Quant Time: Jun 25 04:23:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 20 03:31:56 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	285075	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	434457	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	392074	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	180985	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	132607	49.61	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.22%	
35) Dibromofluoromethane	5.50	113	131927	49.63	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.26%	
50) Toluene-d8	8.71	98	509270	50.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.16%	
62) 4-Bromofluorobenzene	11.13	95	171721	46.77	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.54%	
Target Compounds						
3) Chloromethane	1.33	50	5654	2.450	ug/l	100
16) Acetone	2.44	43	16643	12.424	ug/l	98
17) Carbon Disulfide	2.57	76	3039	0.458	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062419\
Data File : VX010416.D
Acq On : 24 Jun 2019 17:01
Operator : JC/SP
Sample : K3164-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BAT-B03

Quant Time: Jun 25 04:23:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 20 03:31:56 2019
Response via : Initial Calibration

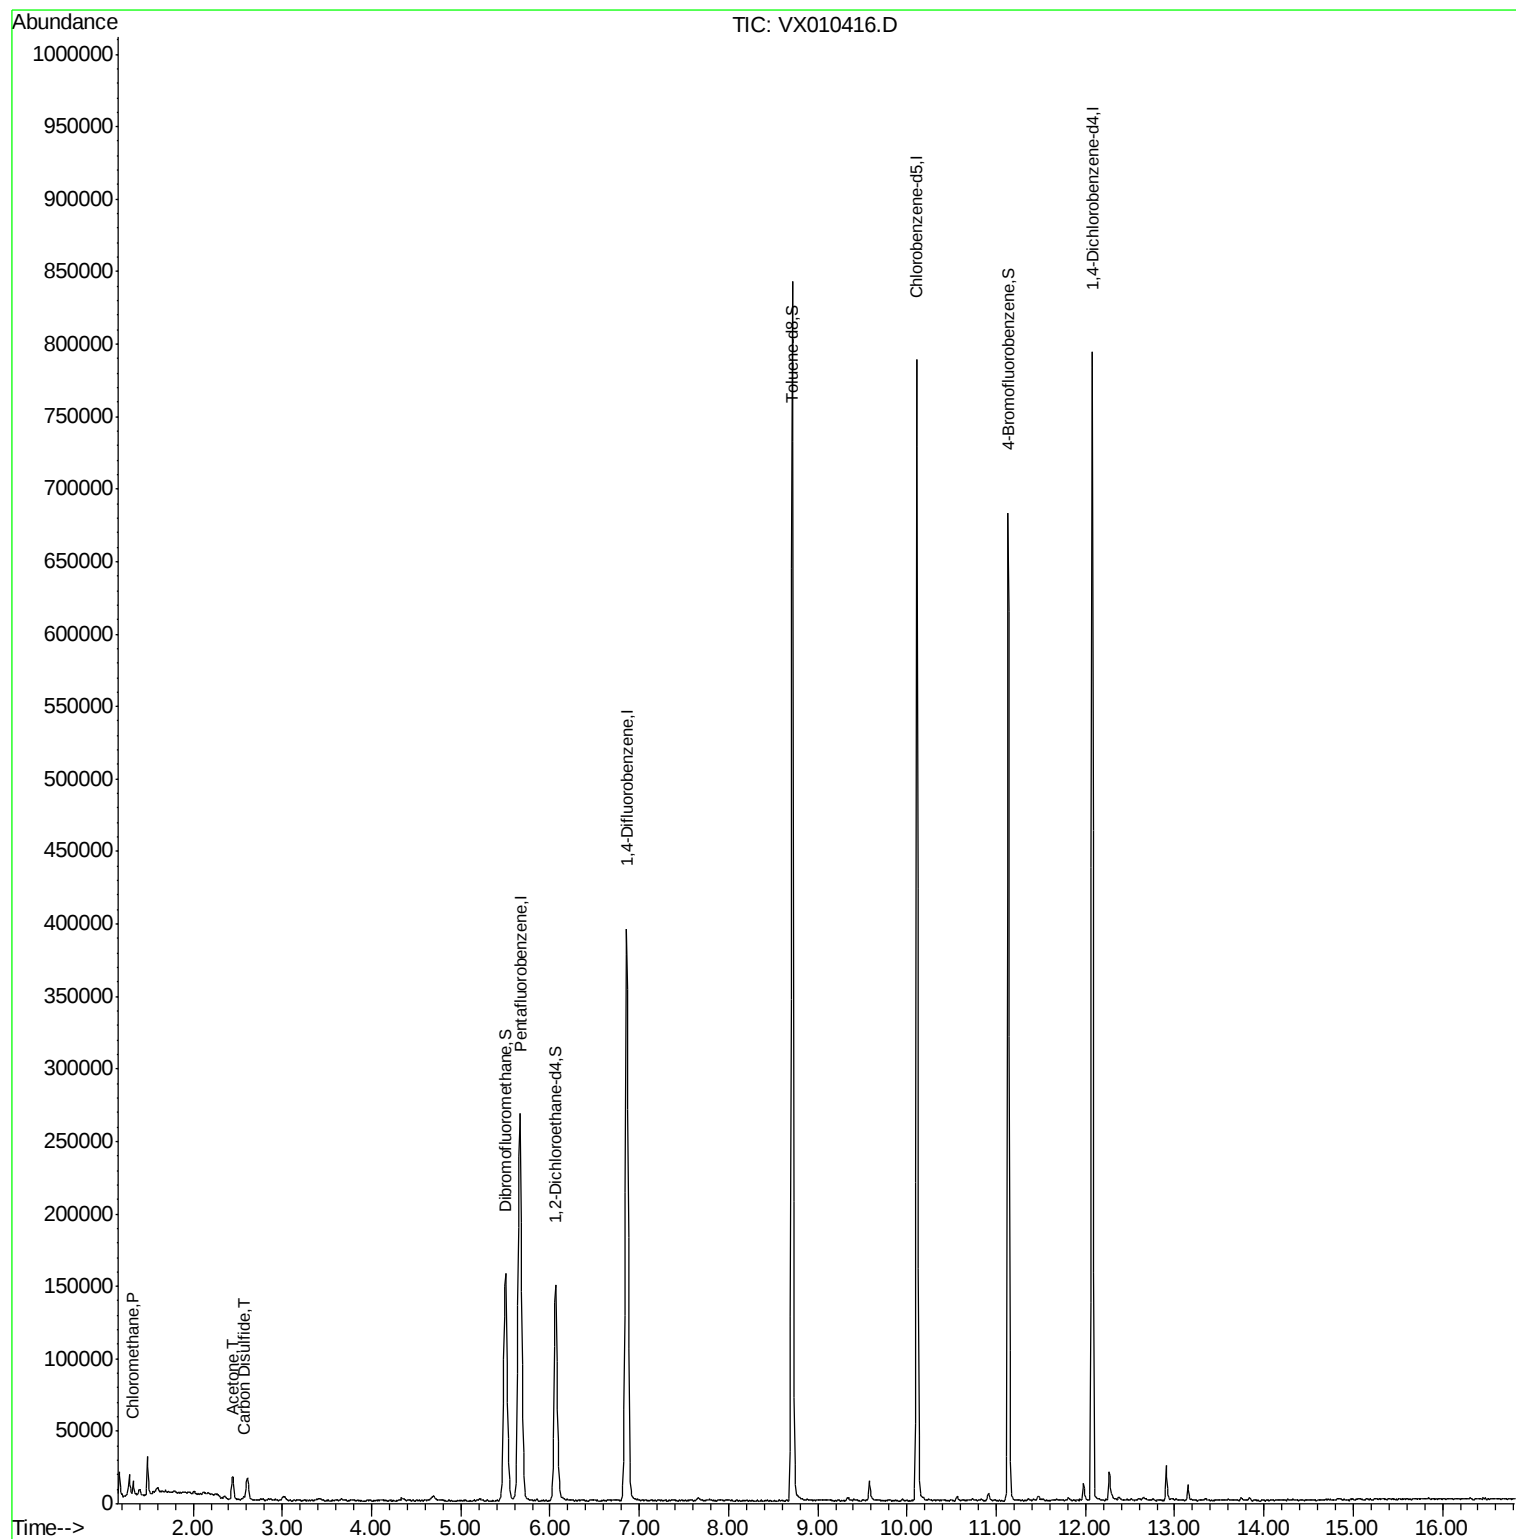

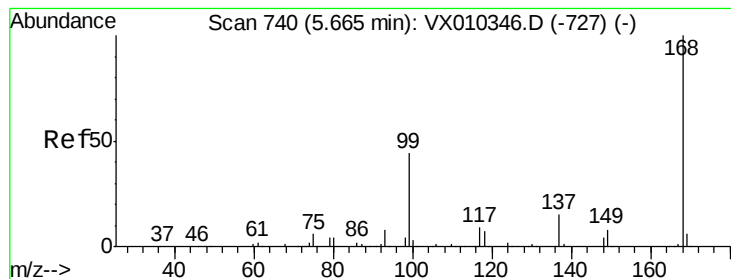

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX010416.D

Acq: 24 Jun 2019 17:01

Instrument :

MSVOA_X

ClientSampleId :


BAT-B03

Tot Ion:168 Resp: 285075

Ion Ratio Lower Upper




168 100

99 45.8 35.5 53.3

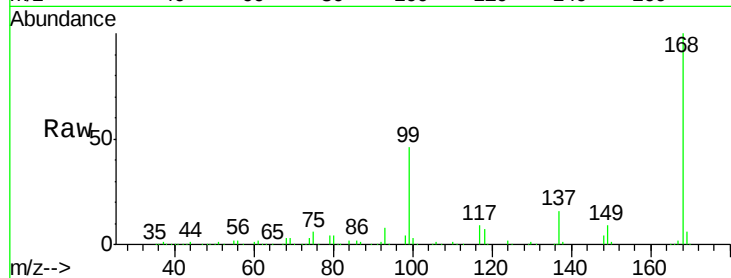

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

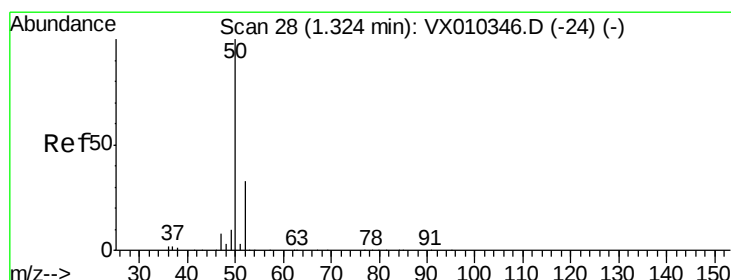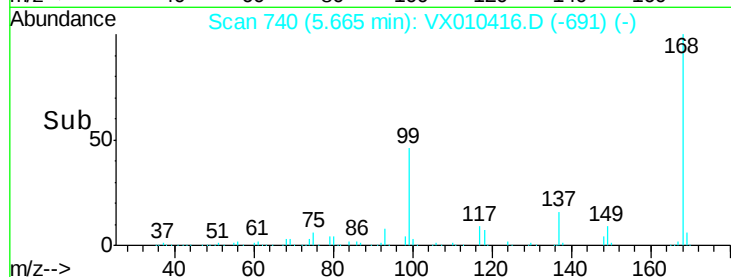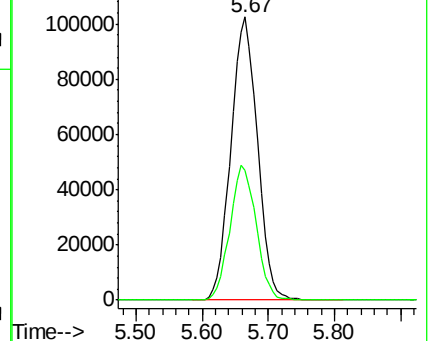

#3

Chloromethane

Concen: 2.450 ug/l

RT: 1.33 min Scan# 29

Delta R.T. 0.01 min

Lab File: VX010416.D


Acq: 24 Jun 2019 17:01

Tgt Ion: 50 Resp: 5654

Ion Ratio Lower Upper



50 100


52 33.1 26.5 39.7

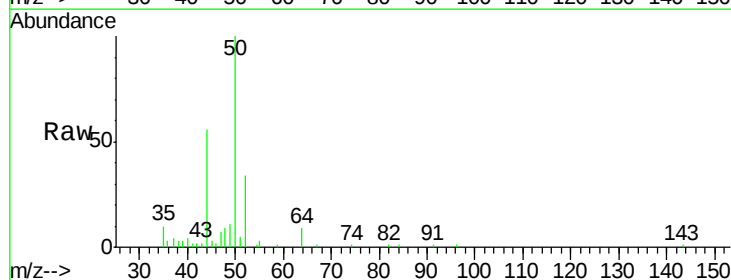

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

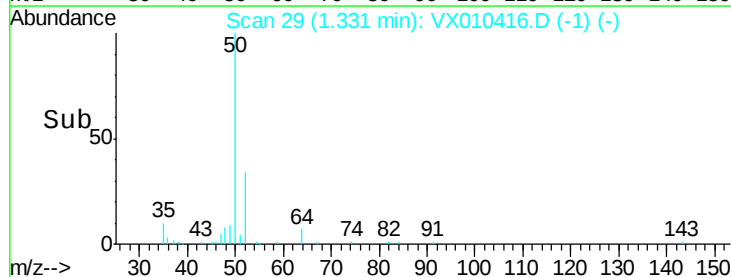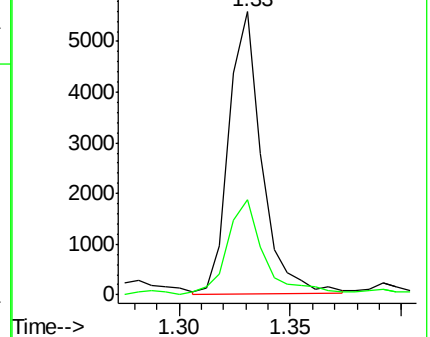

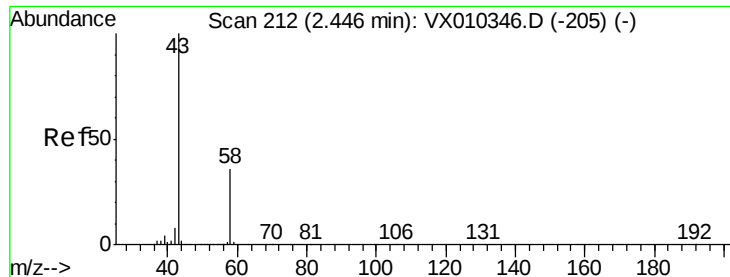

#16

Acetone

Concen: 12.424 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX010416.D

Acq: 24 Jun 2019 17:01

Instrument :

MSVOA_X

ClientSampled :


BAT-B03

Tot Ion: 43 Resp: 16643

Ion Ratio Lower Upper




43 100

58 37.1 28.9 43.3

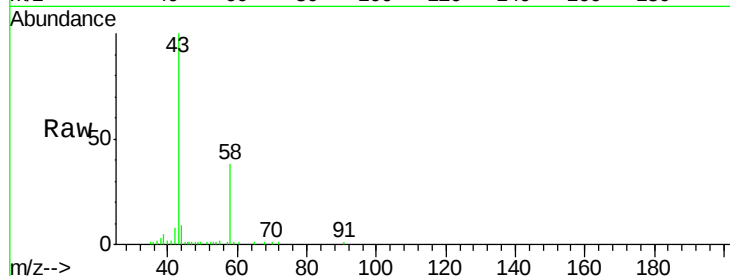

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

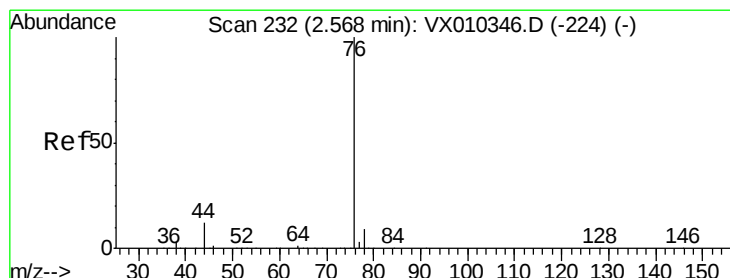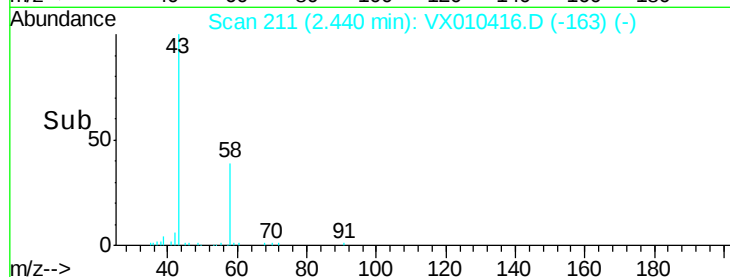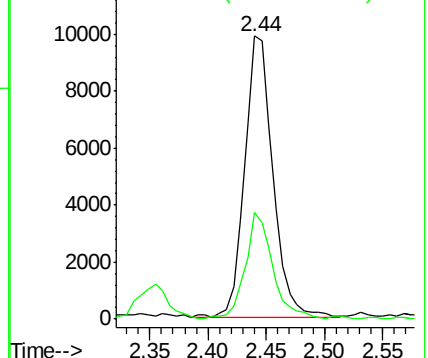

#17

Carbon Disulfide

Concen: 0.458 ug/l

RT: 2.57 min Scan# 233

Delta R.T. 0.01 min

Lab File: VX010416.D


Acq: 24 Jun 2019 17:01

Tgt Ion: 76 Resp: 3039

Ion Ratio Lower Upper



76 100


78 12.0 7.3 10.9#

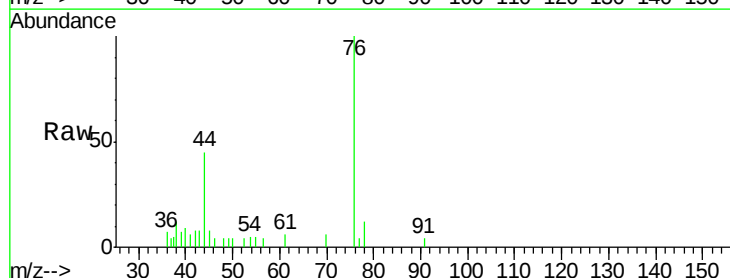

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

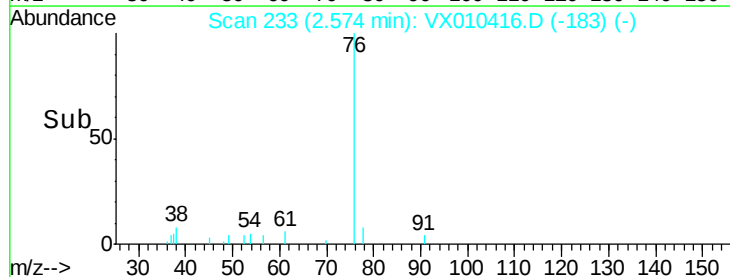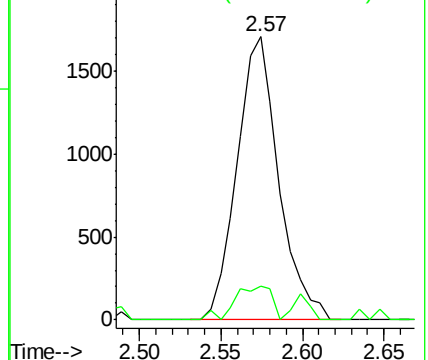

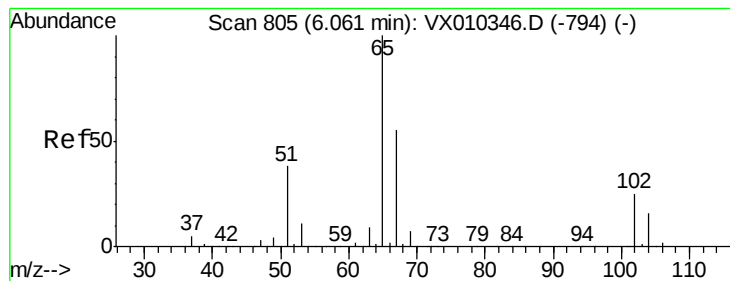

#33

1,2-Dichloroethane-d4

Concen: 49.612 ug/l

RT: 6.06 min Scan# 805

Delta R.T. 0.00 min

Lab File: VX010416.D

Acq: 24 Jun 2019 17:01

Instrument :

MSVOA_X

ClientSampleId :





BAT-B03

Tot Ion: 65 Resp: 132607

Ion Ratio Lower Upper

65 100

67 55.5 0.0 110.2

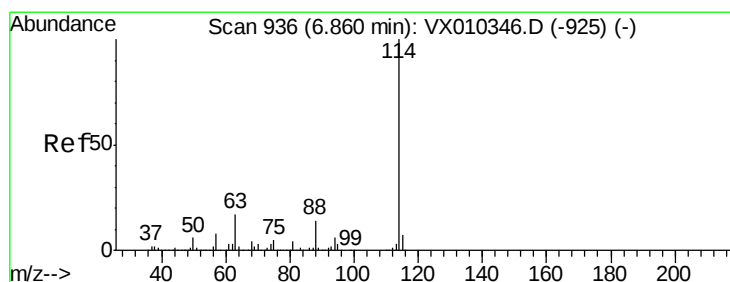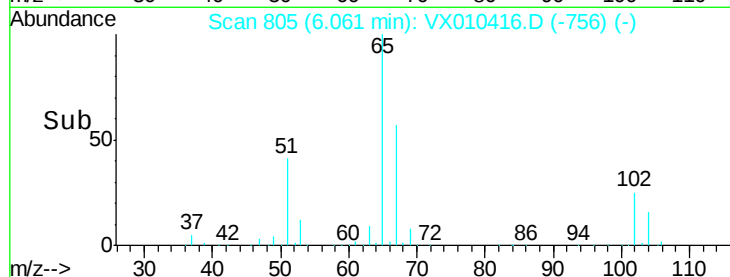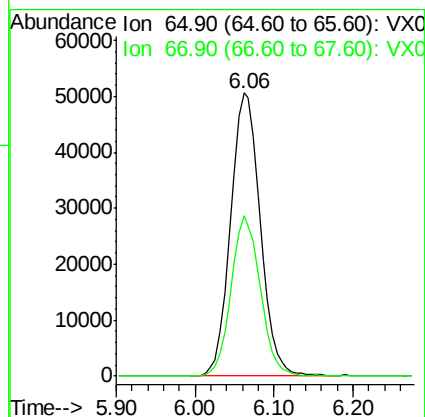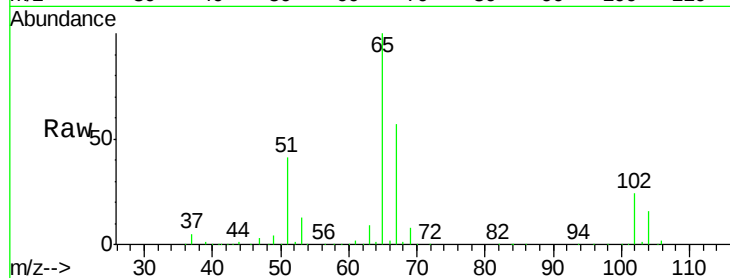

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX010416.D

Acq: 24 Jun 2019 17:01




Tgt Ion: 114 Resp: 434457


Ion Ratio Lower Upper

114 100

63 16.5 0.0 33.8

88 14.3 0.0 27.6


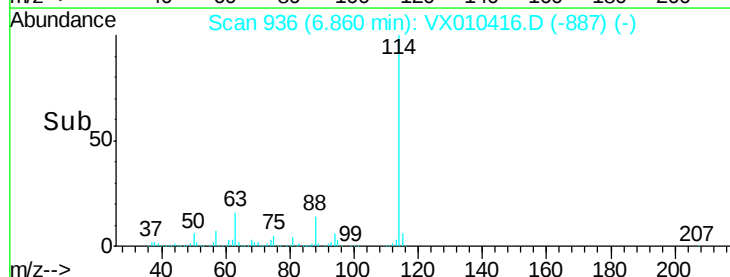
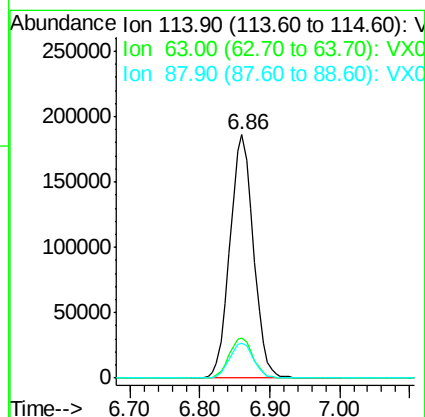
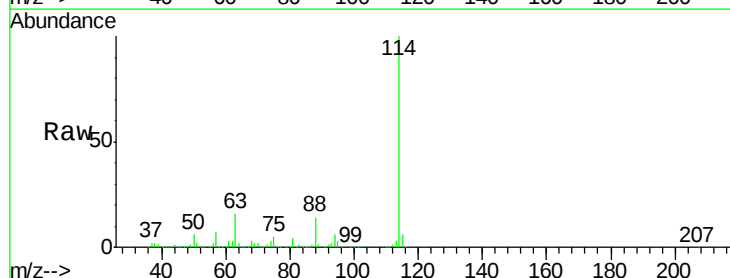


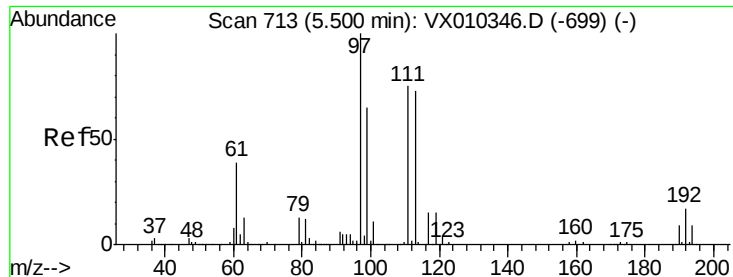

#35
 Dibromofluoromethane
 Concen: 49.631 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.00 min
 Lab File: VX010416.D
 Acq: 24 Jun 2019 17:01




Instrument :
 MSVOA_X
 ClientSampleId :
 BAT-B03


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.5	81.2	121.8
192	23.2	18.6	27.8

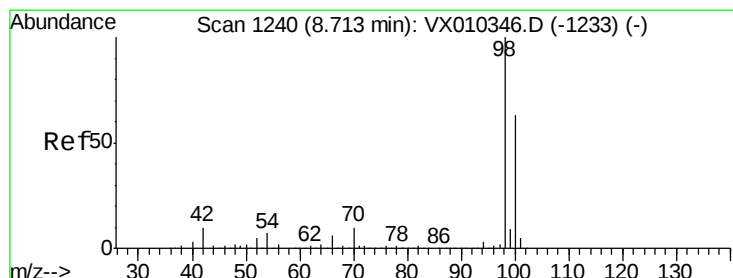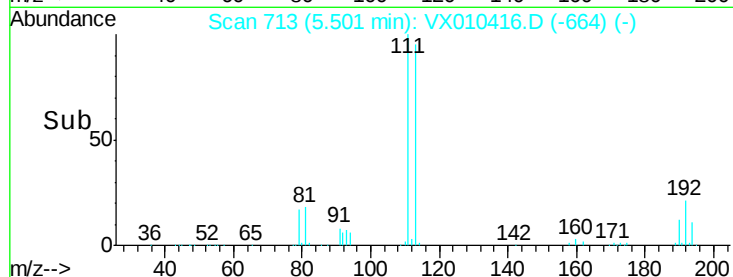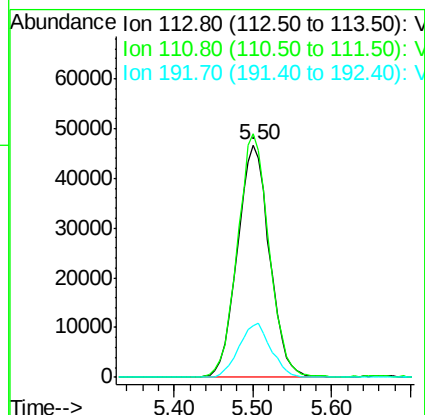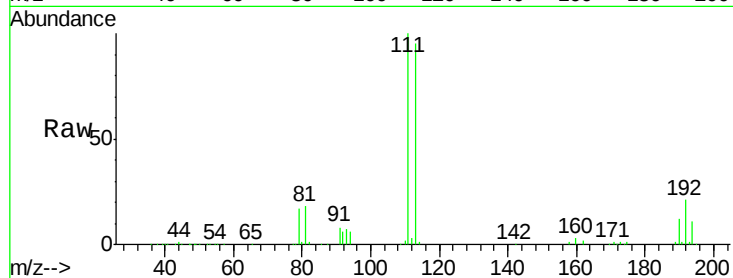

#50
 Toluene-d8
 Concen: 50.078 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. 0.00 min
 Lab File: VX010416.D
 Acq: 24 Jun 2019 17:01

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.7	51.6	77.4

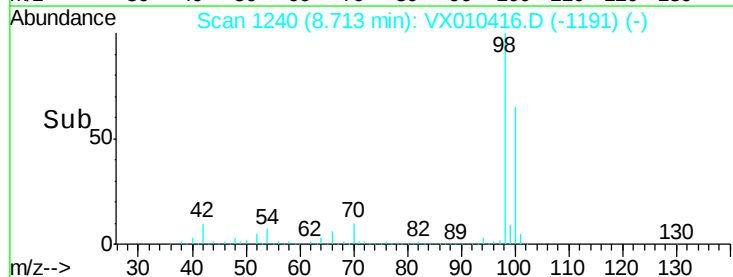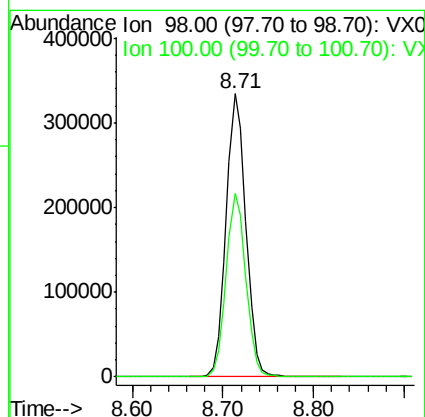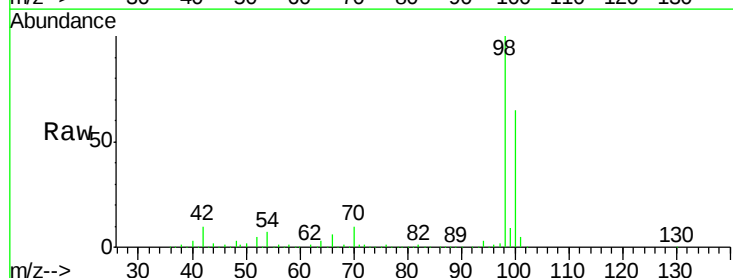

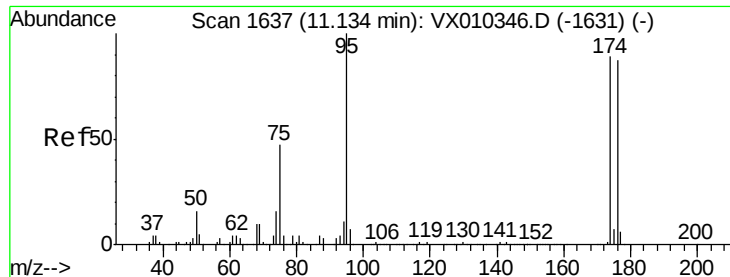

#62

4-Bromofluorobenzene

Concen: 46.771 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX010416.D

Acq: 24 Jun 2019 17:01

Instrument :

MSVOA_X

ClientSampleId :

BAT-B03


Tot Ion: 95 Resp: 171721

Ion Ratio Lower Upper

95 100

174 94.4 0.0 187.6




176 91.3 0.0 184.0

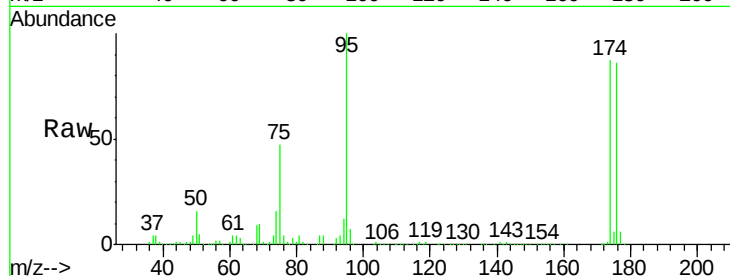

Abundance Ion 94.90 (94.60 to 95.60): VX010346.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX010346.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX010346.D (-1631) (-)

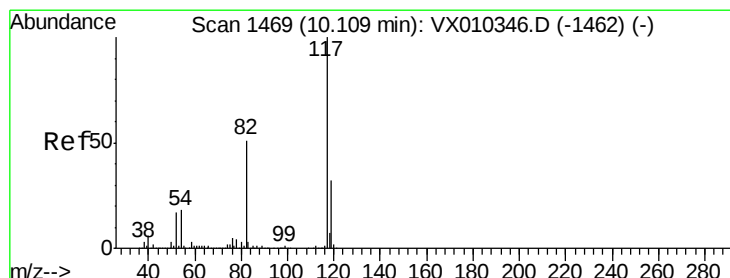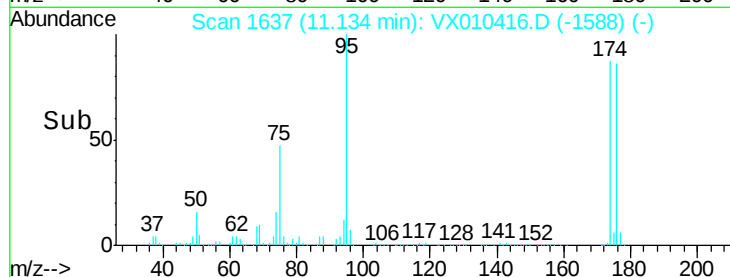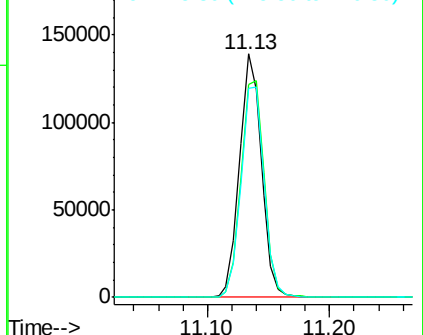

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX010416.D

Acq: 24 Jun 2019 17:01


Tgt Ion: 117 Resp: 392074

Ion Ratio Lower Upper

117 100

82 49.8 41.2 61.8



119 31.6 25.5 38.3

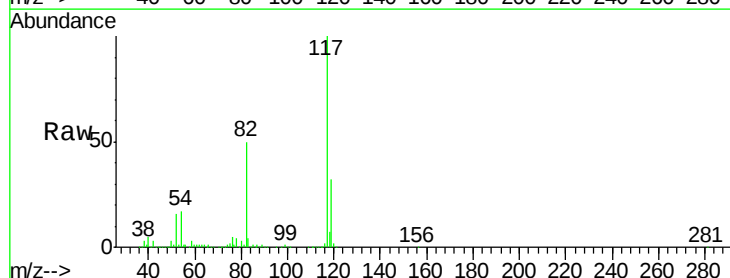


Abundance Ion 116.90 (116.60 to 117.60): VX010346.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX010346.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX010346.D (-1462) (-)

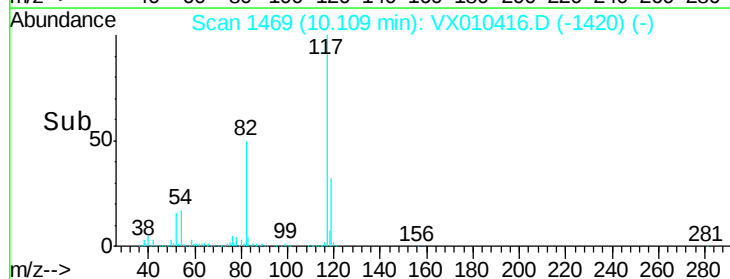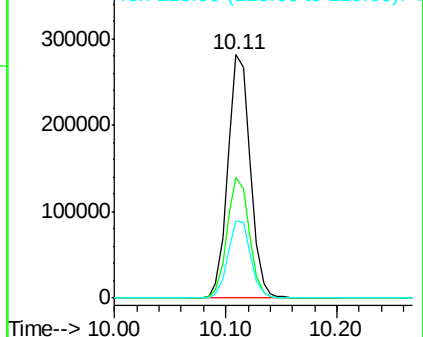


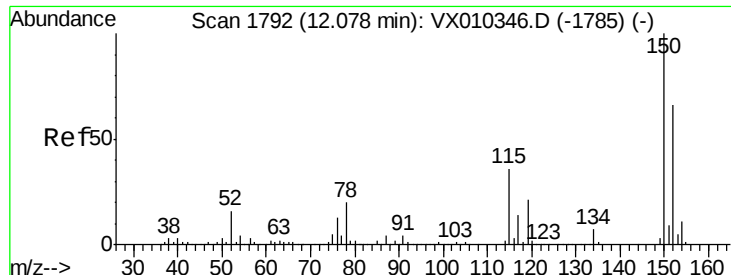

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: VX010416.D
 Acq: 24 Jun 2019 17:01

Instrument :
 MSVOA_X
 ClientSampleId :
 BAT-B03

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.0	38.6	115.7
150	157.7	0.0	347.4

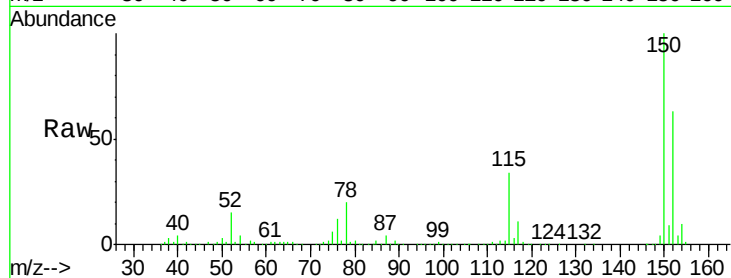

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

