

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062419\  
 Data File : VX010416.D  
 Acq On : 24 Jun 2019 17:01  
 Operator : JC/SP  
 Sample : K3164-15  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BAT-B03

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.282       | 17            | 21          | 26           | rBV      | 14127          | 20671         | 1.61%           | 0.294%        |
| 2         | 1.489       | 51            | 55          | 61           | rBV      | 26336          | 30089         | 2.34%           | 0.428%        |
| 3         | 2.446       | 207           | 212         | 219          | rVB      | 15456          | 26446         | 2.06%           | 0.376%        |
| 4         | 2.611       | 233           | 239         | 247          | rVB      | 14821          | 28979         | 2.26%           | 0.412%        |
| 5         | 5.501       | 699           | 713         | 725          | rBV2     | 156866         | 448065        | 34.88%          | 6.372%        |
| 6         | 5.665       | 728           | 740         | 752          | rVV      | 266162         | 749458        | 58.34%          | 10.658%       |
| 7         | 6.061       | 794           | 805         | 823          | rBV      | 148932         | 396353        | 30.86%          | 5.636%        |
| 8         | 6.860       | 925           | 936         | 951          | rBV      | 394813         | 931866        | 72.54%          | 13.252%       |
| 9         | 8.713       | 1232          | 1240        | 1248         | rBV      | 841154         | 1284563       | 100.00%         | 18.268%       |
| 10        | 9.579       | 1377          | 1382        | 1393         | rBV      | 13298          | 20824         | 1.62%           | 0.296%        |
| 11        | 10.109      | 1463          | 1469        | 1481         | rBV      | 786641         | 1094424       | 85.20%          | 15.564%       |
| 12        | 11.134      | 1630          | 1637        | 1651         | rBV      | 681798         | 871670        | 67.86%          | 12.396%       |
| 13        | 11.981      | 1771          | 1776        | 1785         | rBV2     | 12127          | 15851         | 1.23%           | 0.225%        |
| 14        | 12.079      | 1785          | 1792        | 1801         | rBV      | 792068         | 1040790       | 81.02%          | 14.801%       |
| 15        | 12.268      | 1819          | 1823        | 1827         | rBV      | 19653          | 25822         | 2.01%           | 0.367%        |
| 16        | 12.908      | 1924          | 1928        | 1934         | rBV2     | 24235          | 31293         | 2.44%           | 0.445%        |
| 17        | 13.152      | 1961          | 1968        | 1974         | rBV2     | 10875          | 14788         | 1.15%           | 0.210%        |


Sum of corrected areas: 7031952

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062419\  
Data File : VX010416.D  
Acq On : 24 Jun 2019 17:01  
Operator : JC/SP  
Sample : K3164-15  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BAT-B03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

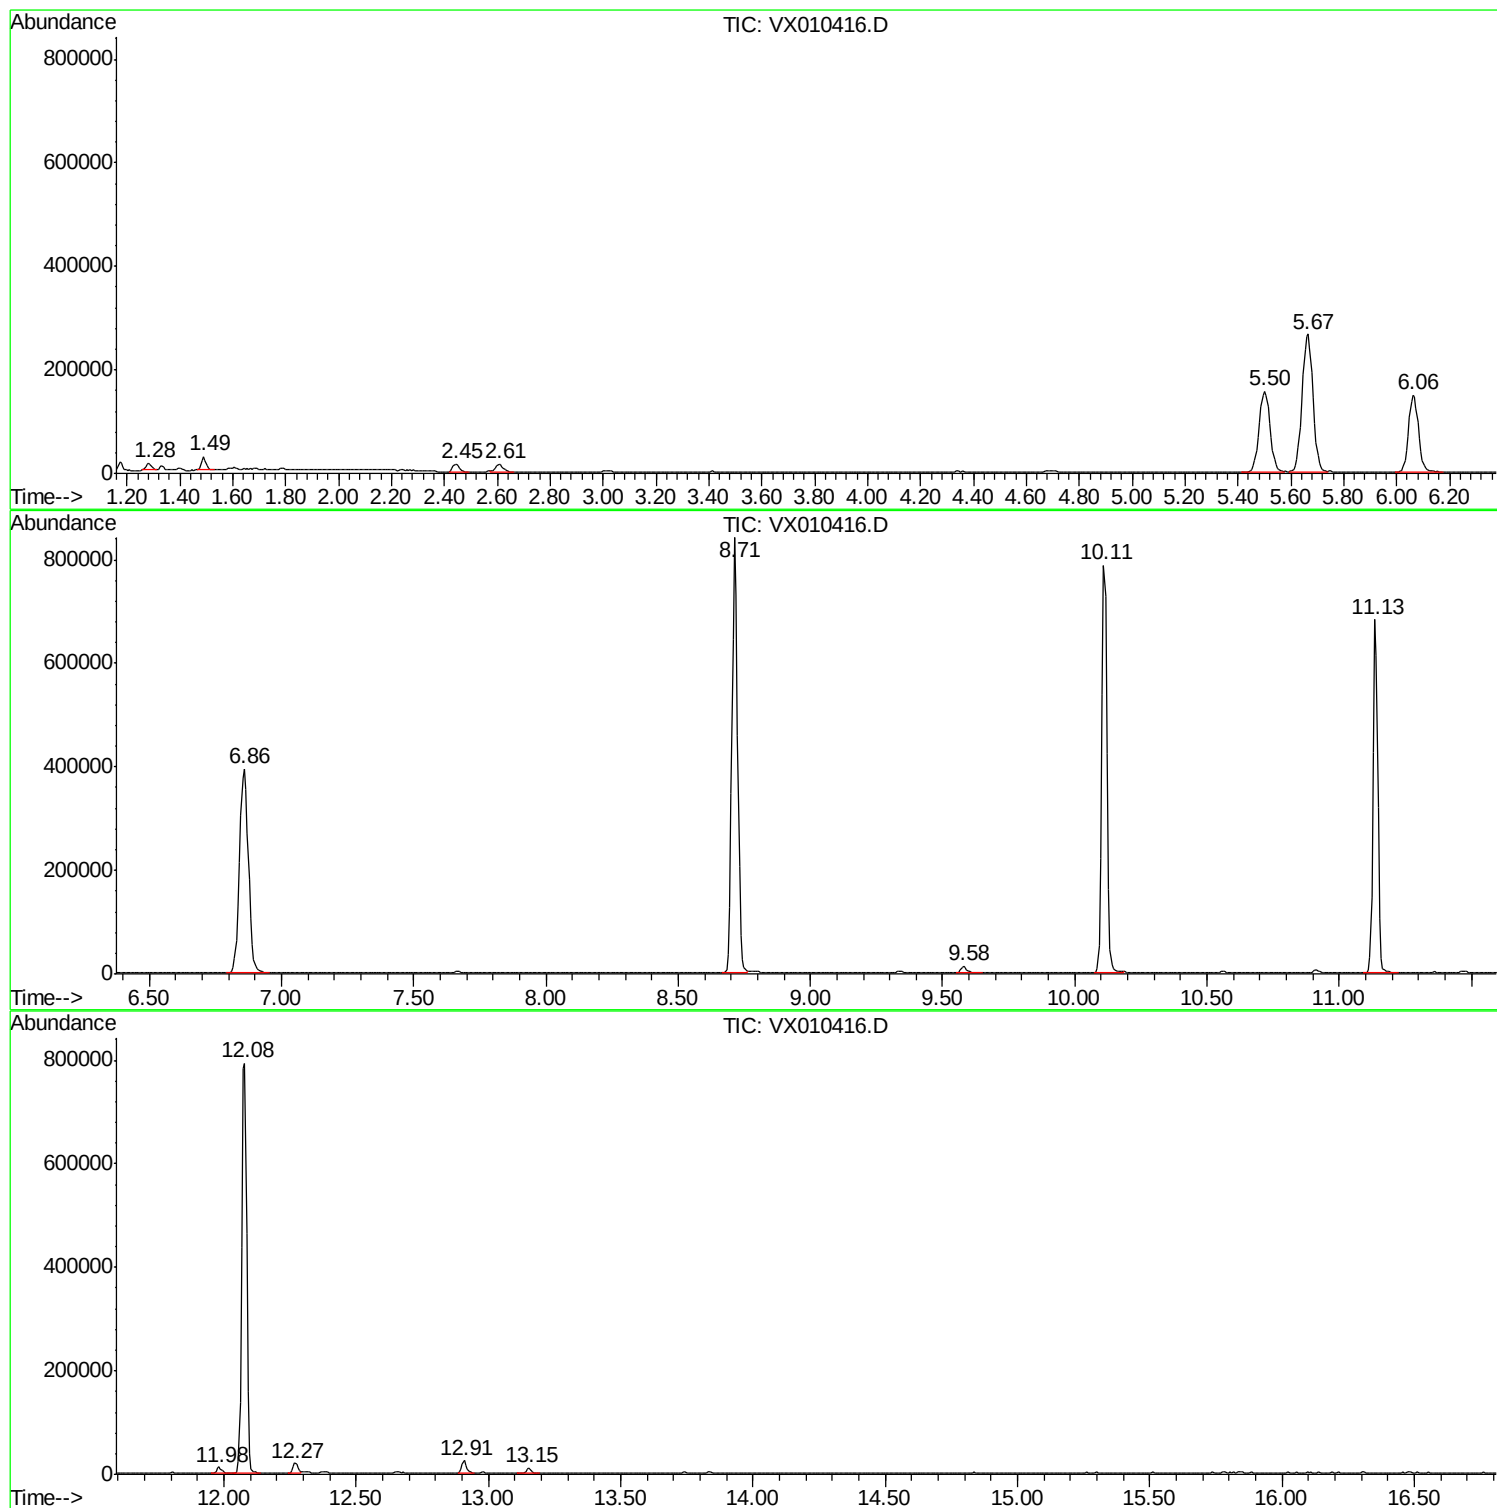

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX062419\  
Data File : VX010416.D  
Acq On : 24 Jun 2019 17:01  
Operator : JC/SP  
Sample : K3164-15  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BAT-B03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX062419\  
Data File : VX010416.D  
Acq On : 24 Jun 2019 17:01  
Operator : JC/SP  
Sample : K3164-15  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BAT-B03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |