


Methylene Chloride

Response Ratio

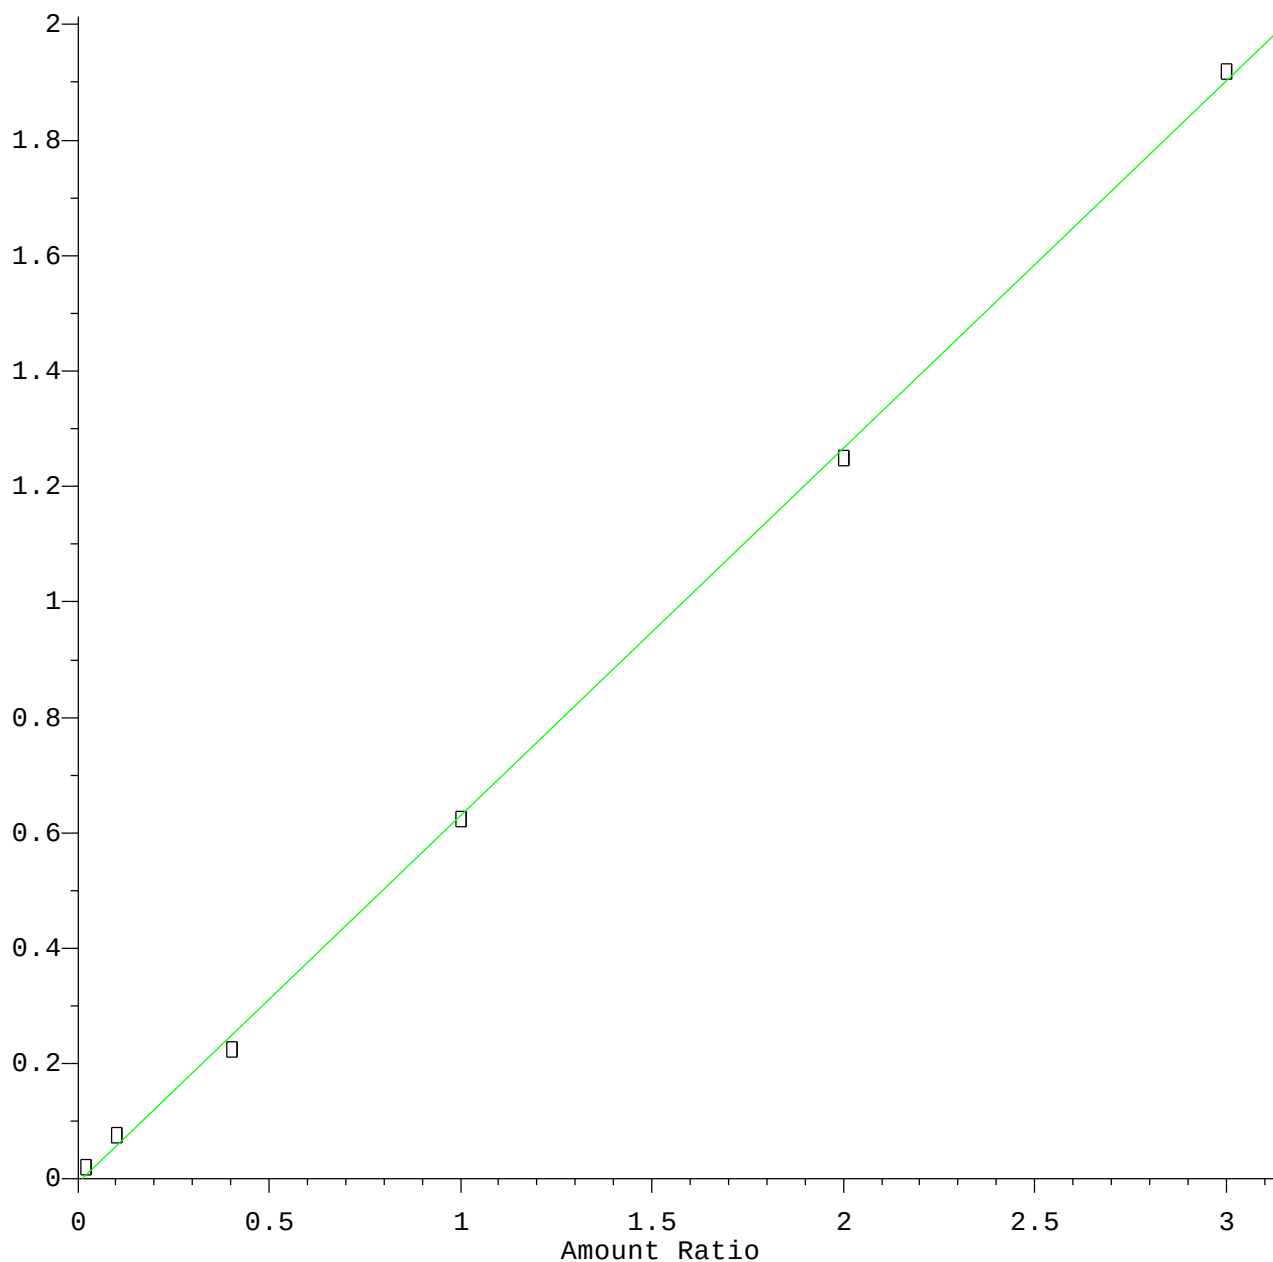


Resp Ratio = $6.36 \times 10^{-1} \times \text{Amt} - 6.32 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020


Bromochloromethane

Response Ratio

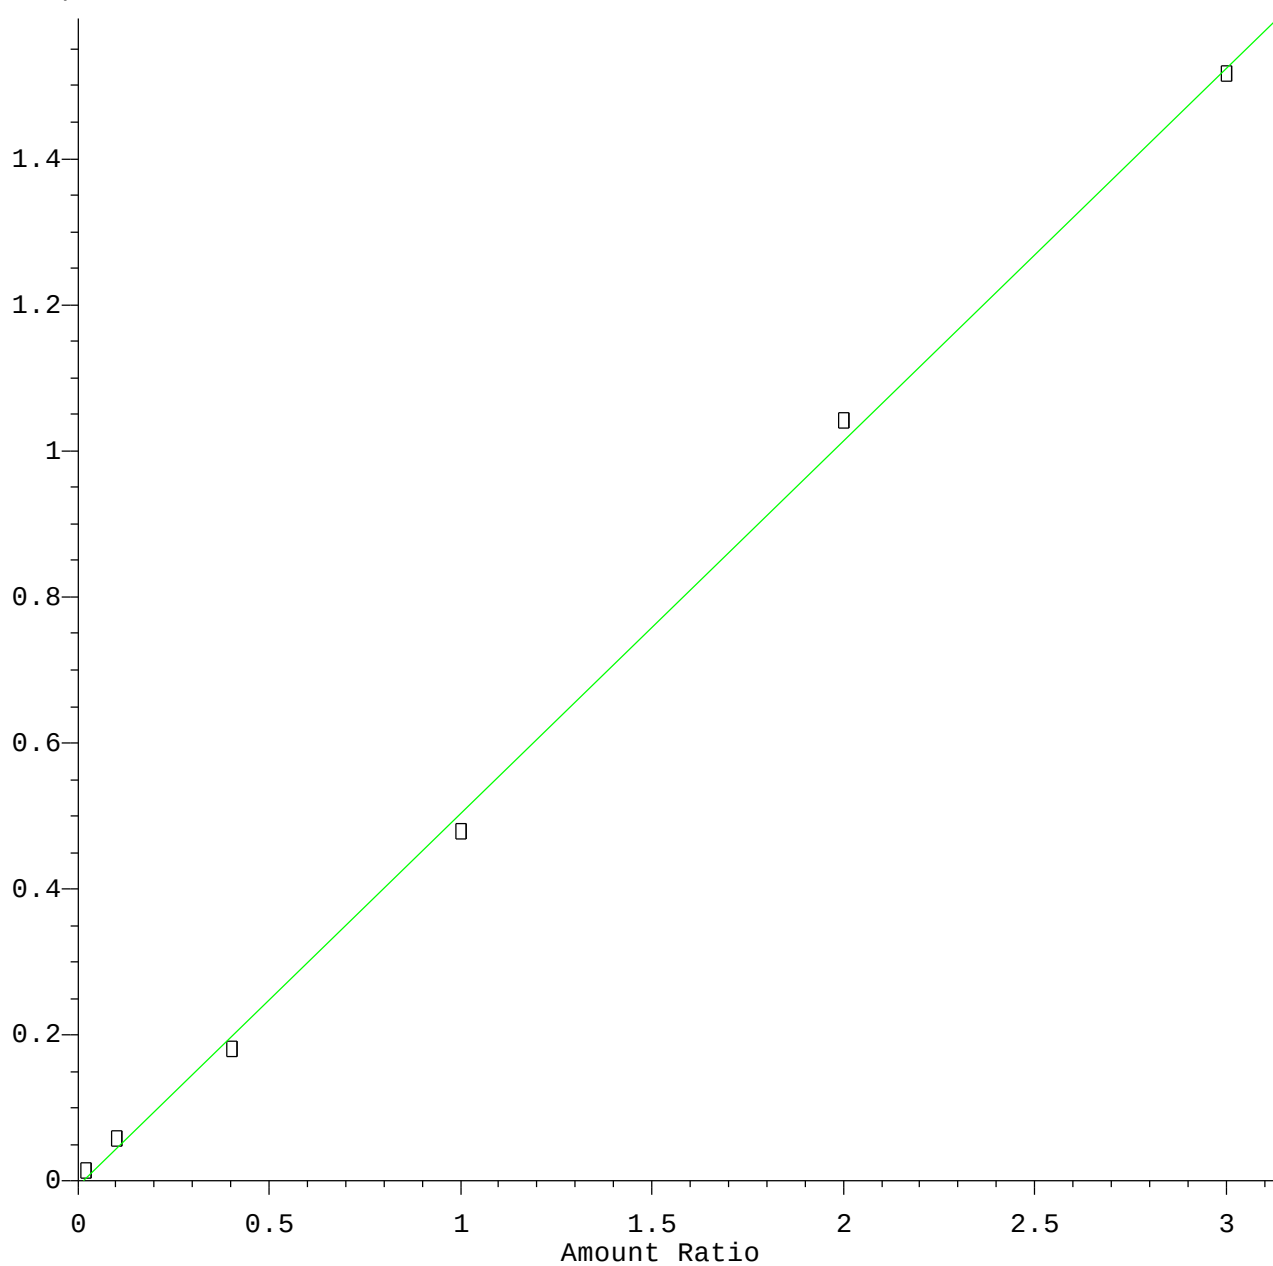


Resp Ratio = $5.10 \times 10^{-1} \times \text{Amt} - 6.74 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020

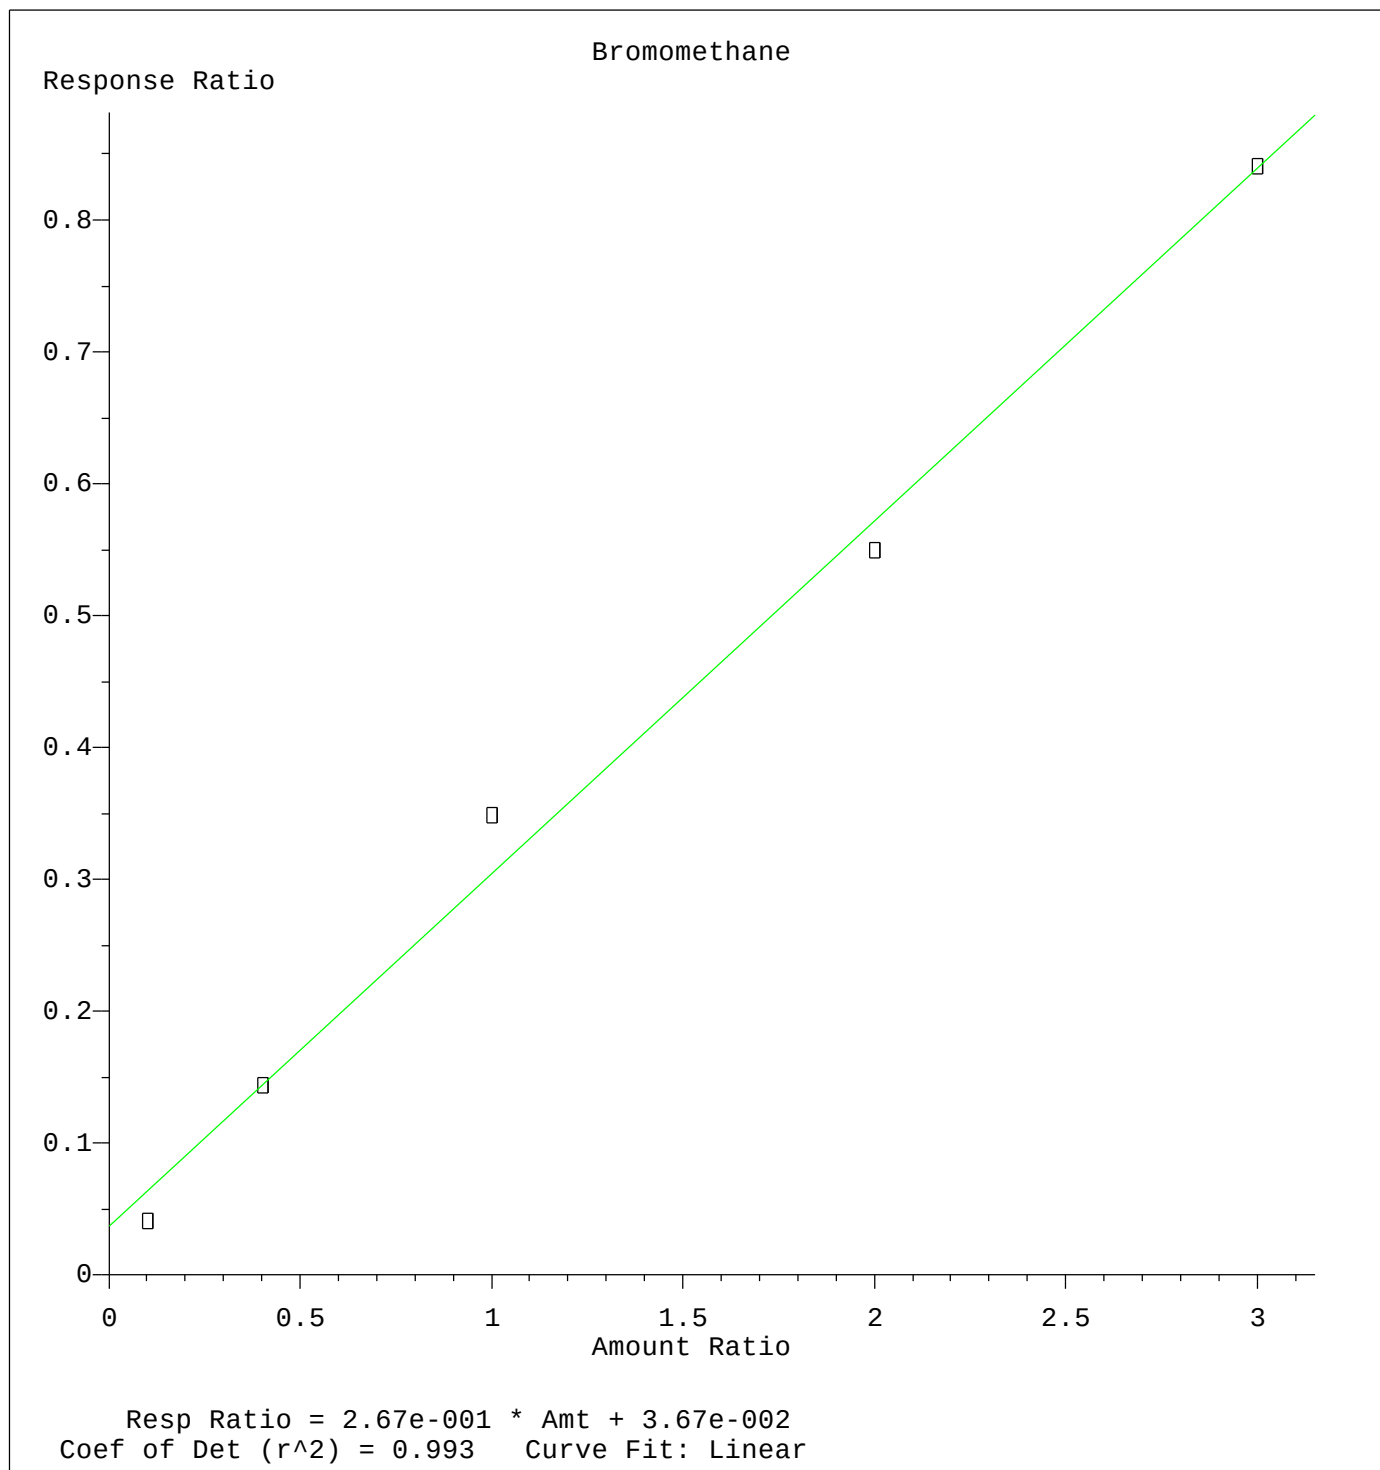


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020

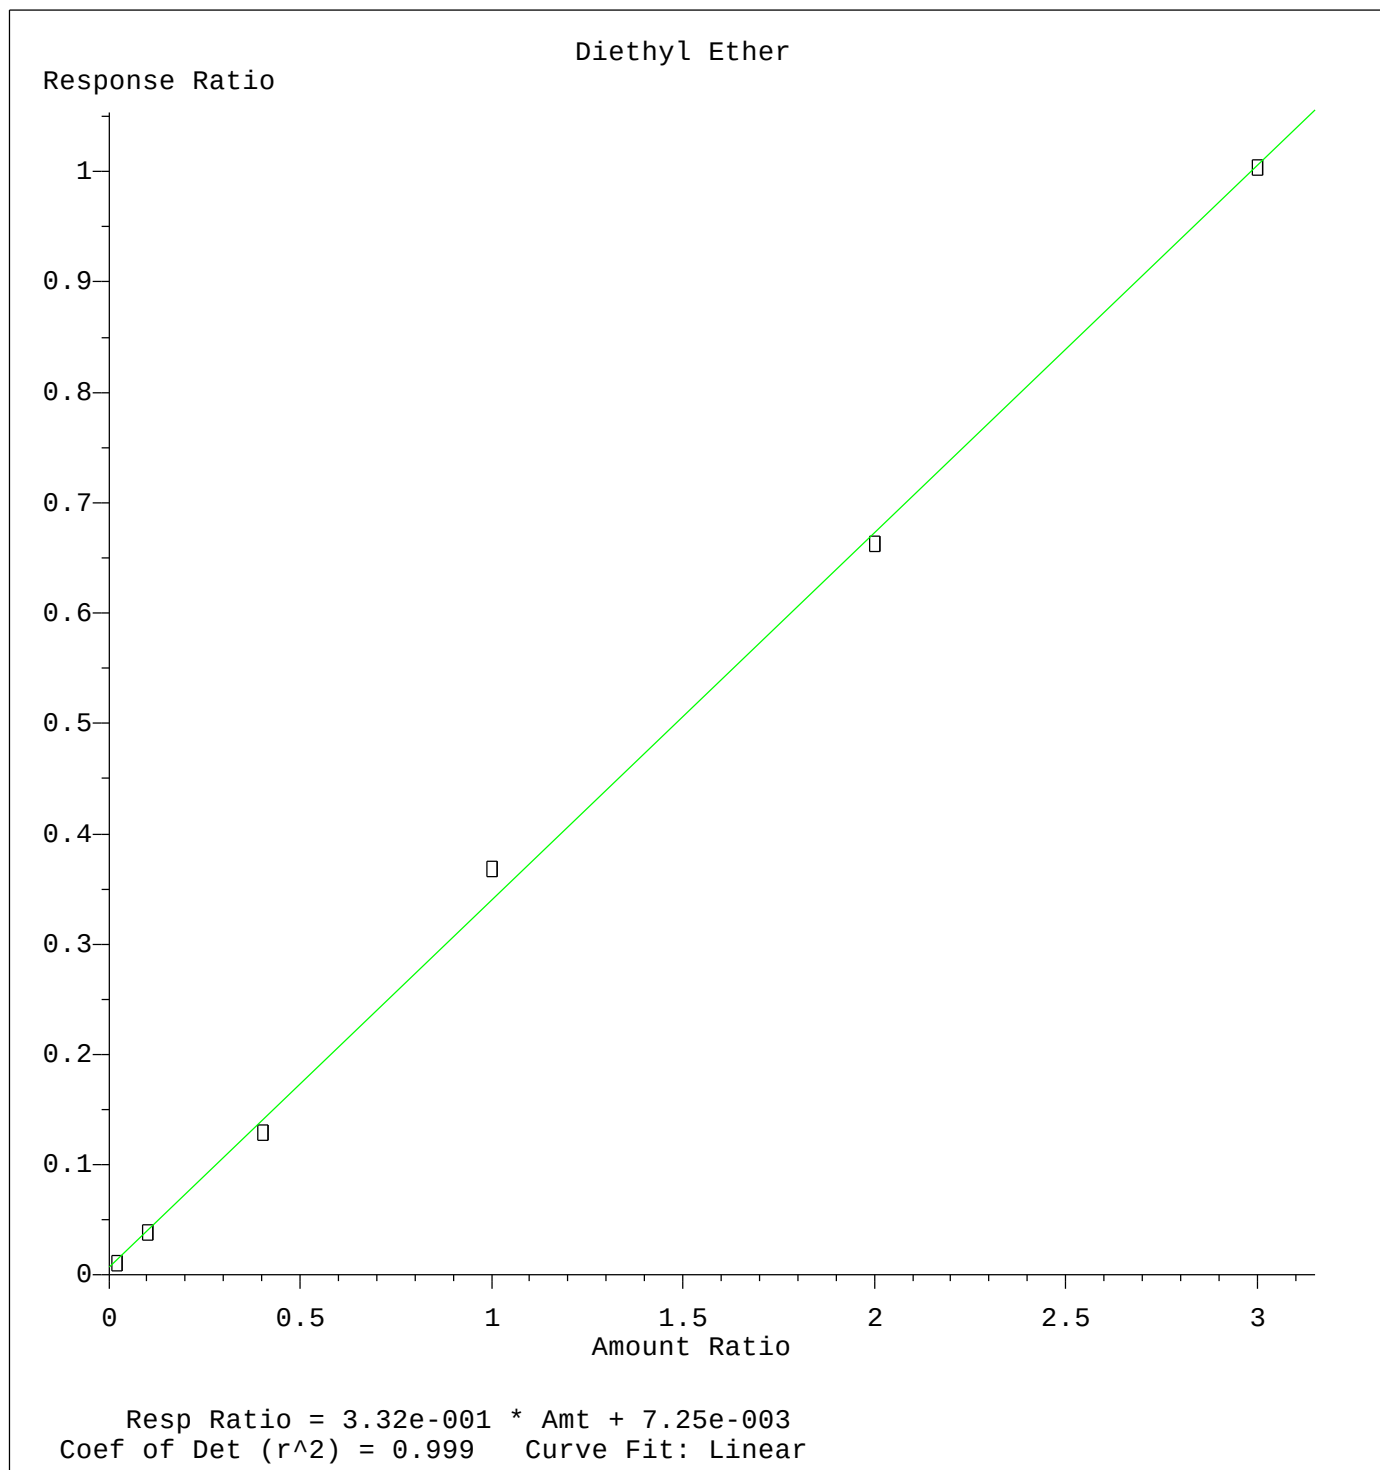

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020

Methylene Chloride

Response Ratio

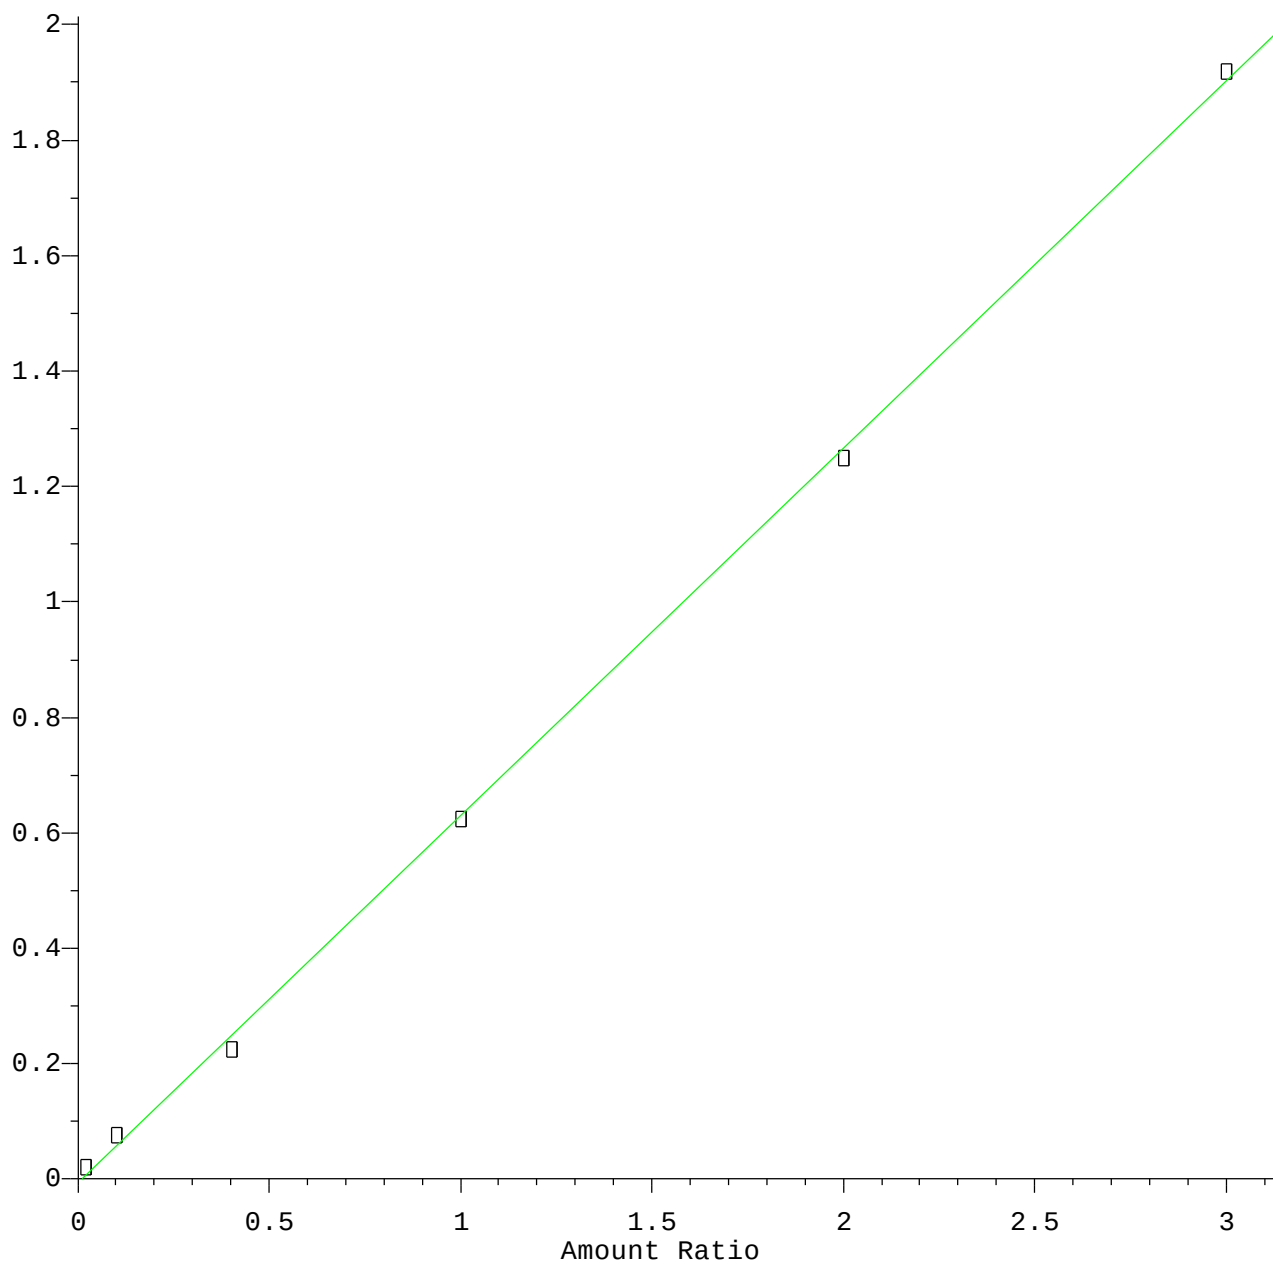


Resp Ratio = 6.36e-001 * Amt - 6.32e-003
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020


Bromochloromethane

Response Ratio

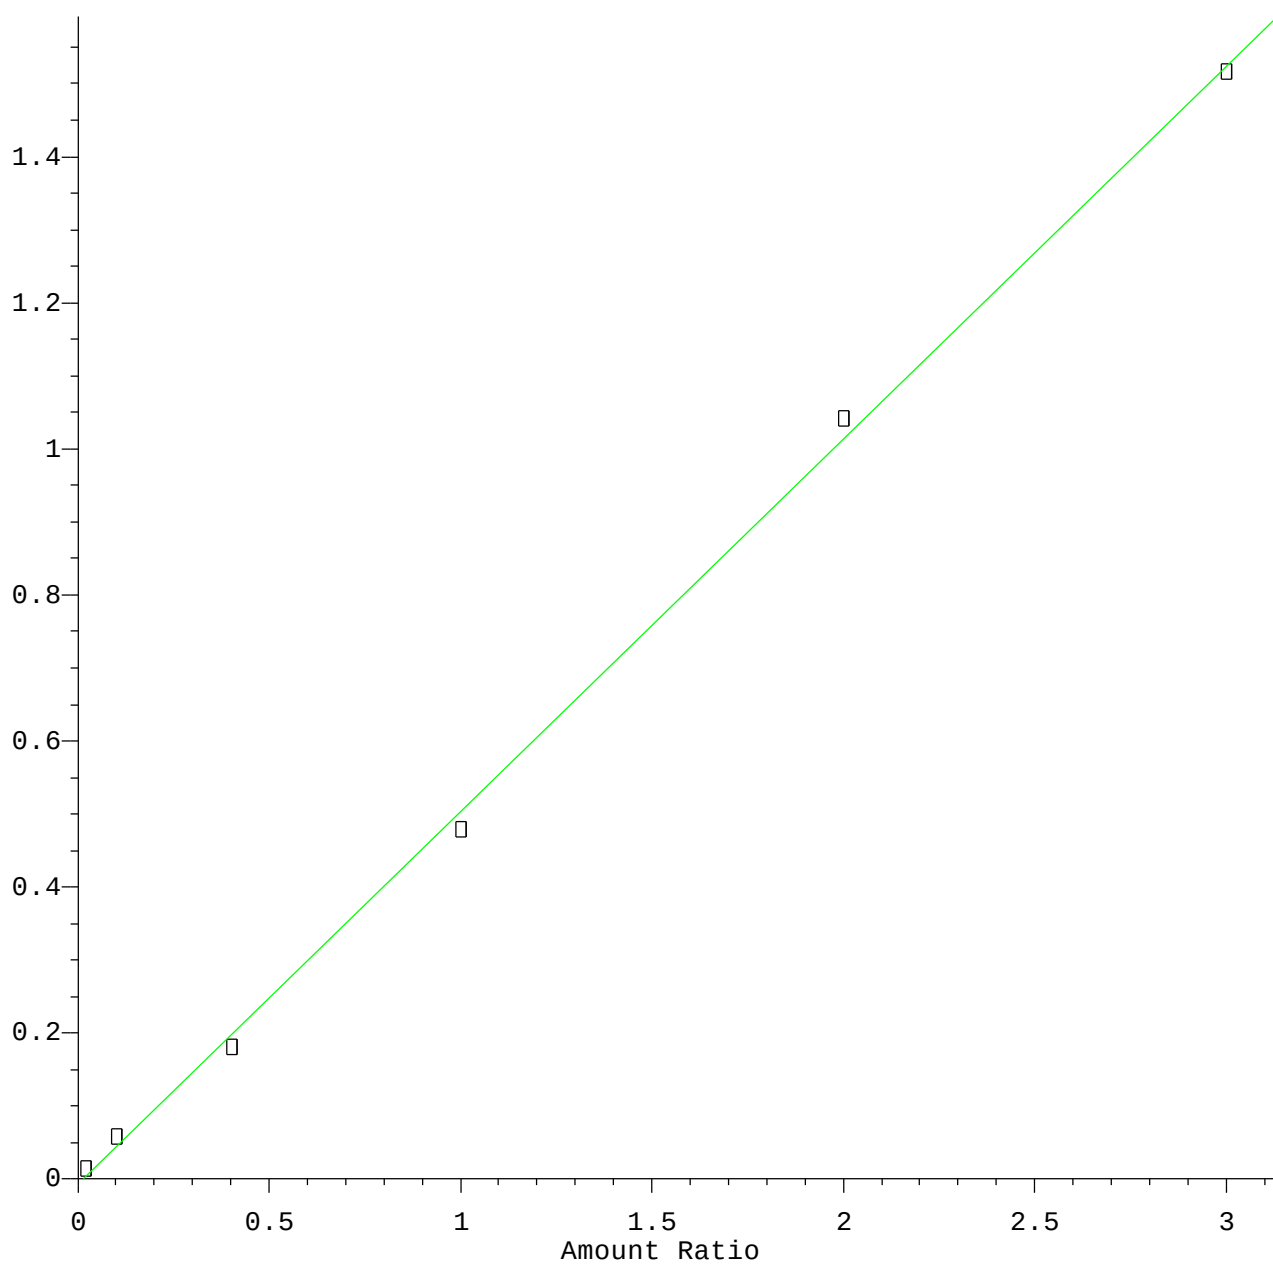


Resp Ratio = $5.10 \times 10^{-1} \times \text{Amt} - 6.74 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020

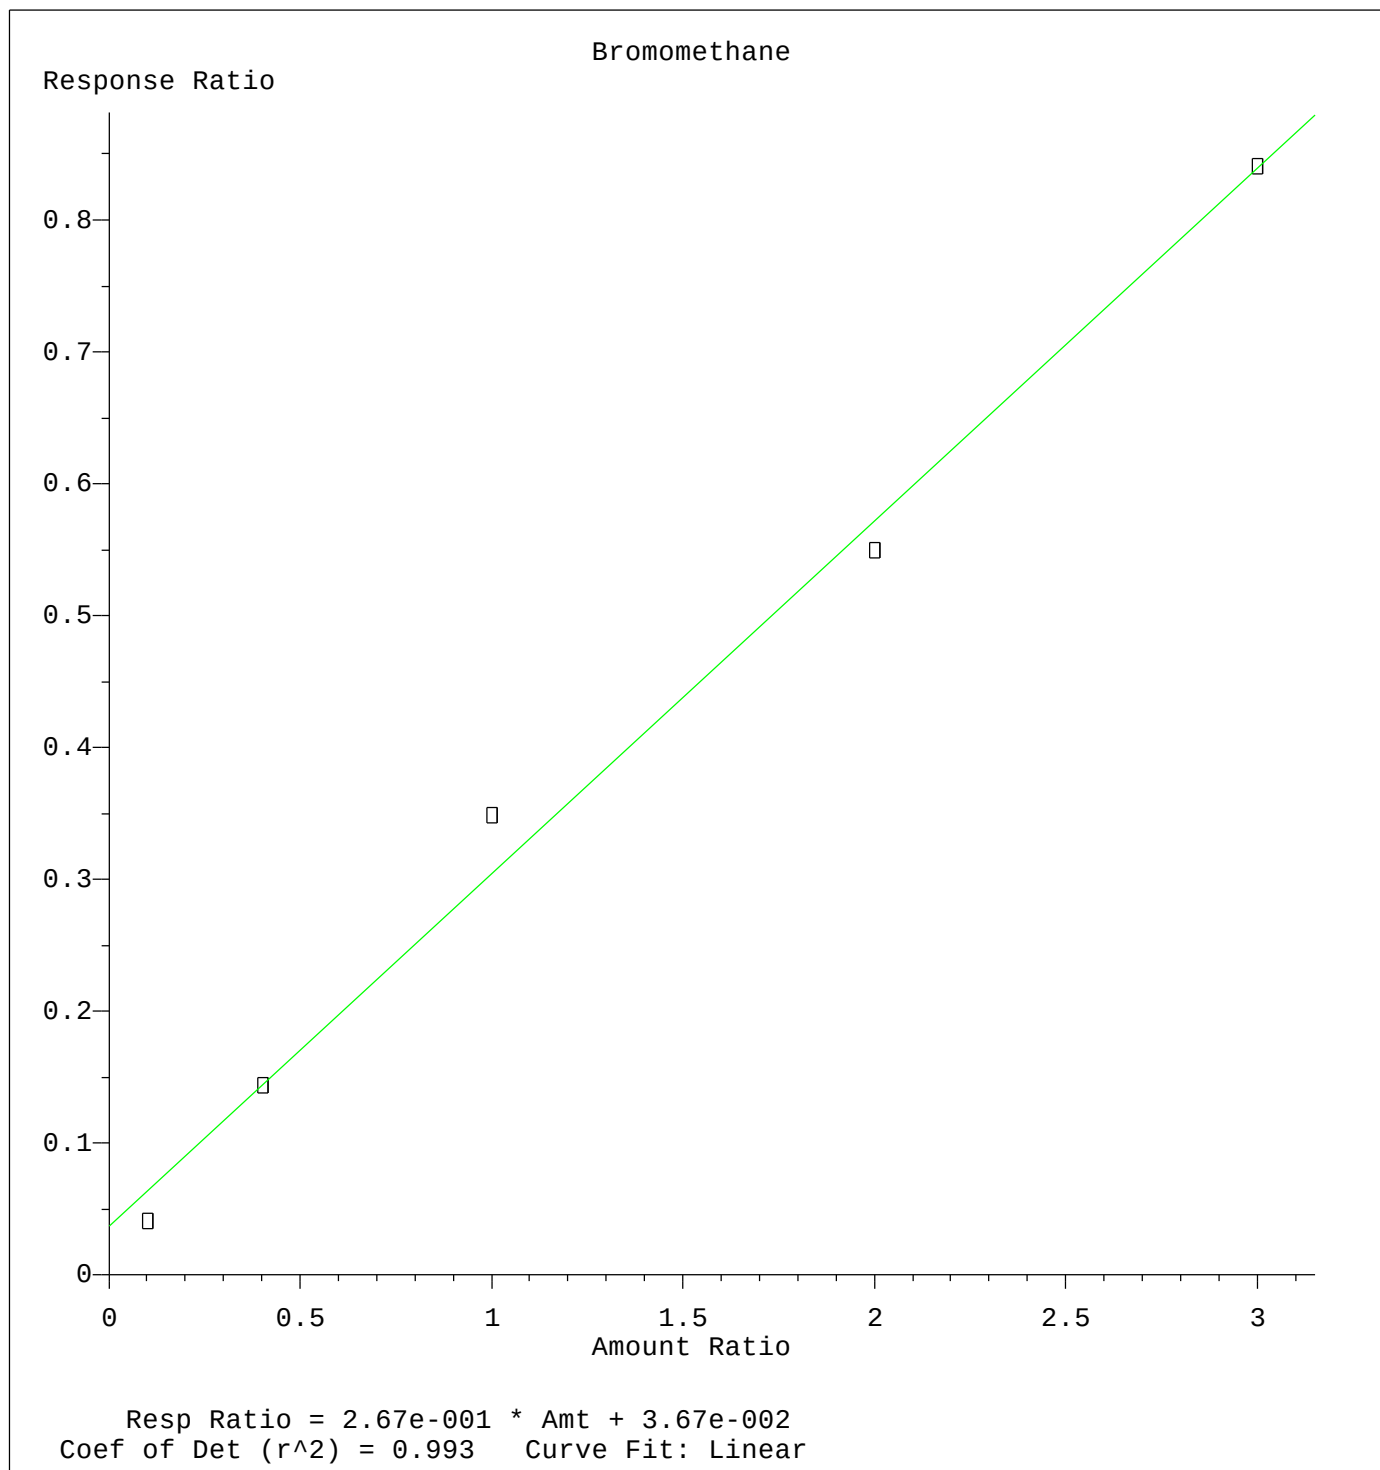


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020

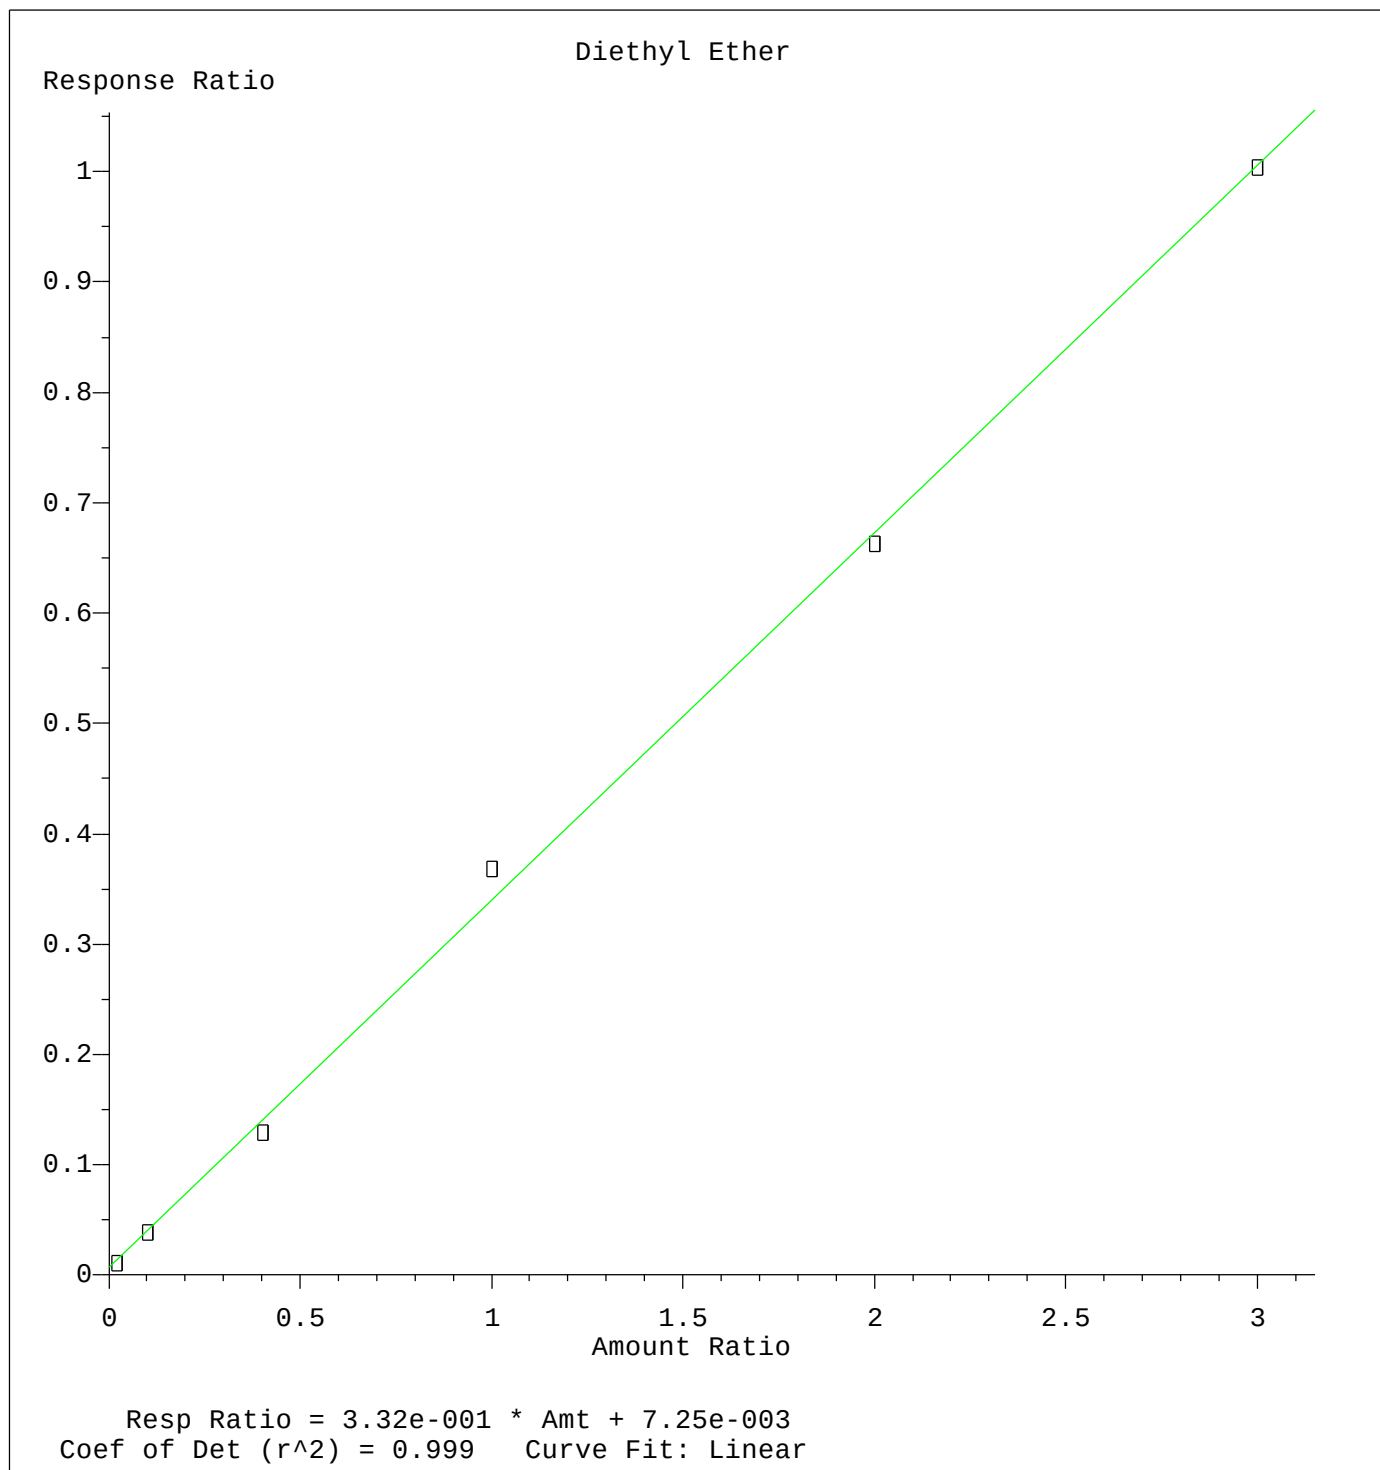

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020

Methylene Chloride

Response Ratio

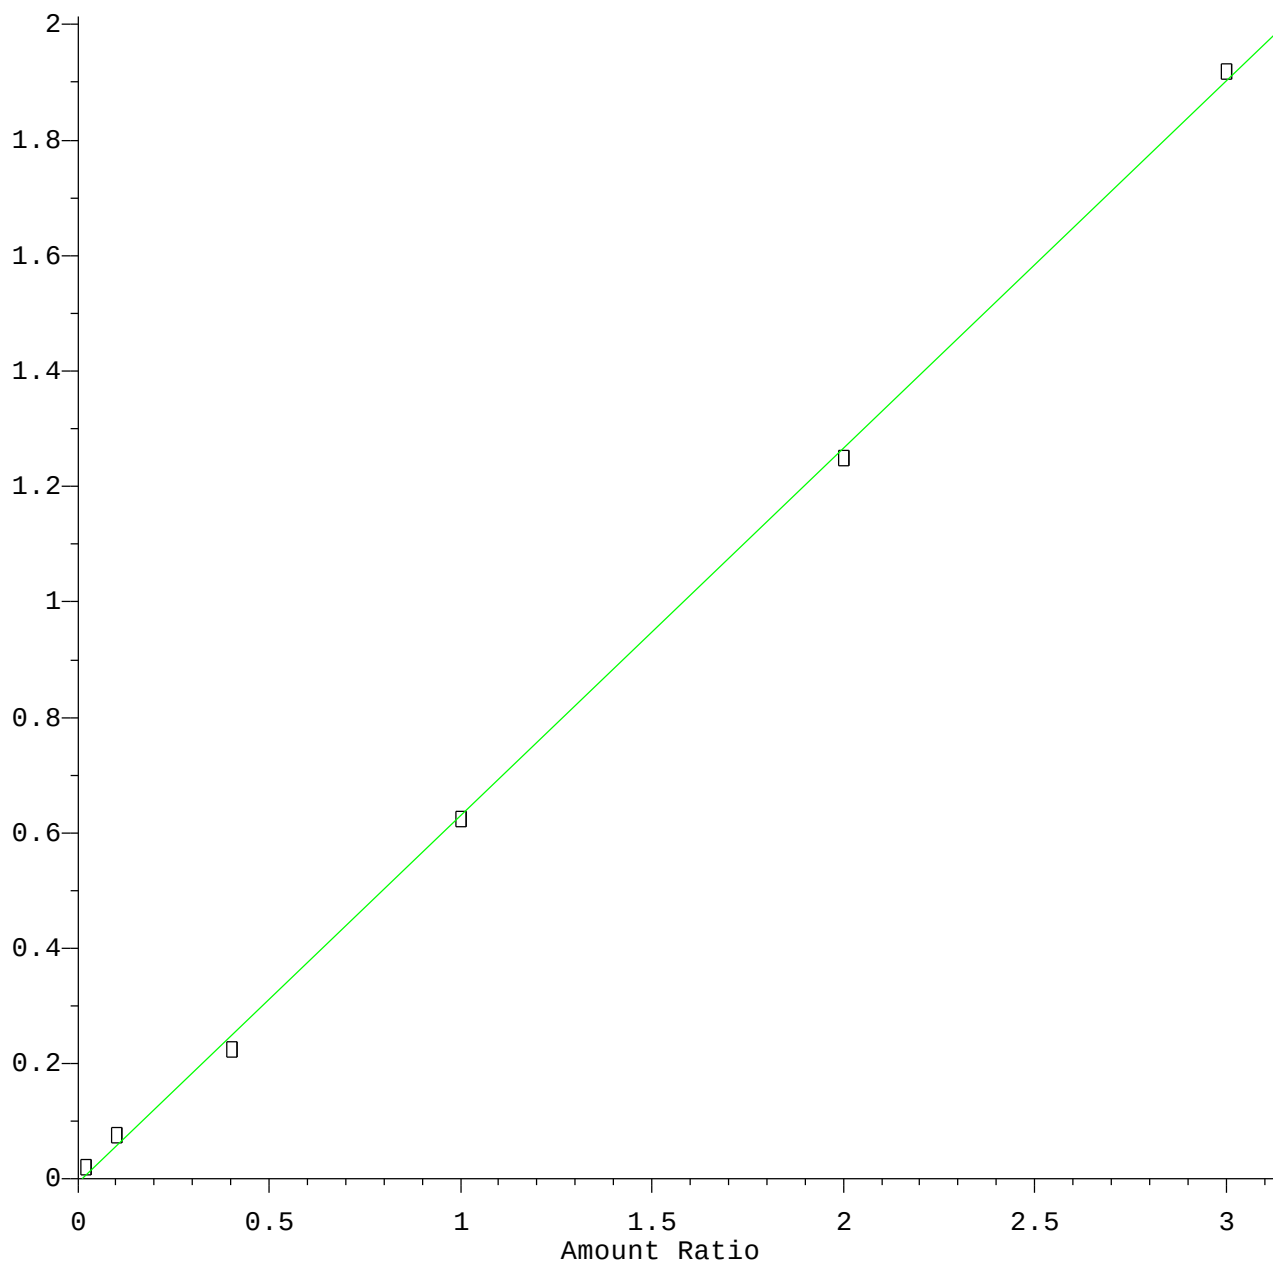

Resp Ratio = 6.36e-001 * Amt - 6.32e-003
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062420W.M
Calibration Table Last Updated: Wed Jun 24 13:10:00 2020