

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
 Data File : VX022875.D
 Acq On : 24 Jun 2021 17:45
 Operator : JC/MD
 Sample : M2803-08 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP04-20210618

Quant Time: Jun 25 05:39:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 19:12:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.568	168	52909	50.00	ug/l	0.01
34) 1,4-Difluorobenzene	6.775	114	108832	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	93483	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	34731	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.971	65	48977	51.01	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.02%			
35) Dibromofluoromethane	5.404	113	37496	54.25	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 108.50%			
50) Toluene-d8	8.653	98	143647	53.03	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 106.06%			
62) 4-Bromofluorobenzene	11.085	95	48602	48.08	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 96.16%			
Target Compounds						Qvalue
5) Bromomethane	1.618	94	292	0.70	ug/l #	68
7) Trichlorofluoromethane	1.898	101	224	0.20	ug/l #	17
9) 1,1,2-Trichlorotrifluo...	2.337	101	2671	3.88	ug/l #	84
10) Methyl Iodide	2.459	142	385	4.31	ug/l #	85
11) Tert butyl alcohol	2.959	59	339	1.69	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	1649	2.40	ug/l	98
15) Acrylonitrile	3.081	53	200	0.44	ug/l #	35
16) Acetone	2.398	43	426	1.00	ug/l #	40
17) Carbon Disulfide	2.514	76	784	3.91	ug/l #	90
20) Methylene Chloride	2.800	84	627	1.11	ug/l	89
21) trans-1,2-Dichloroethene	3.105	96	316	0.41	ug/l #	49
24) 1,1-Dichloroethane	3.623	63	377	0.26	ug/l #	81
27) cis-1,2-Dichloroethene	4.513	96	194	0.23	ug/l	13
31) Cyclohexane	5.568	56	1768	1.30	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	5359	4.64	ug/l #	48
38) Carbon Tetrachloride	5.562	117	6389	6.59	ug/l #	15
44) Trichloroethene	7.135	130	31690	40.09	ug/l	92
60) Dibromochloromethane	9.275	129	133	3.81	ug/l #	11
68) m/p-Xylenes	10.311	106	281	0.21	ug/l	99
76) 1,2,3-Trichloropropane	11.085	75	26589	28.98	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.085	75	26589	74.60	ug/l #	12
82) 4-Chlorotoluene	11.463	91	546	0.22	ug/l #	45
85) sec-Butylbenzene	11.890	105	655	0.21	ug/l	94
87) 1,3-Dichlorobenzene	11.976	146	264	0.22	ug/l	93
88) 1,4-Dichlorobenzene	11.976	146	264	0.21	ug/l	92
89) n-Butylbenzene	12.335	91	508	0.22	ug/l	95
93) 1,2,4-Trichlorobenzene	13.591	180	221	0.35	ug/l	89
94) Hexachlorobutadiene	13.731	225	53	0.21	ug/l #	19
95) Naphthalene	13.780	128	666	2.15	ug/l #	69
96) 1,2,3-Trichlorobenzene	13.957	180	250	0.39	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022875.D
Acq On : 24 Jun 2021 17:45
Operator : JC/MD
Sample : M2803-08 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Quant Time: Jun 25 05:39:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration

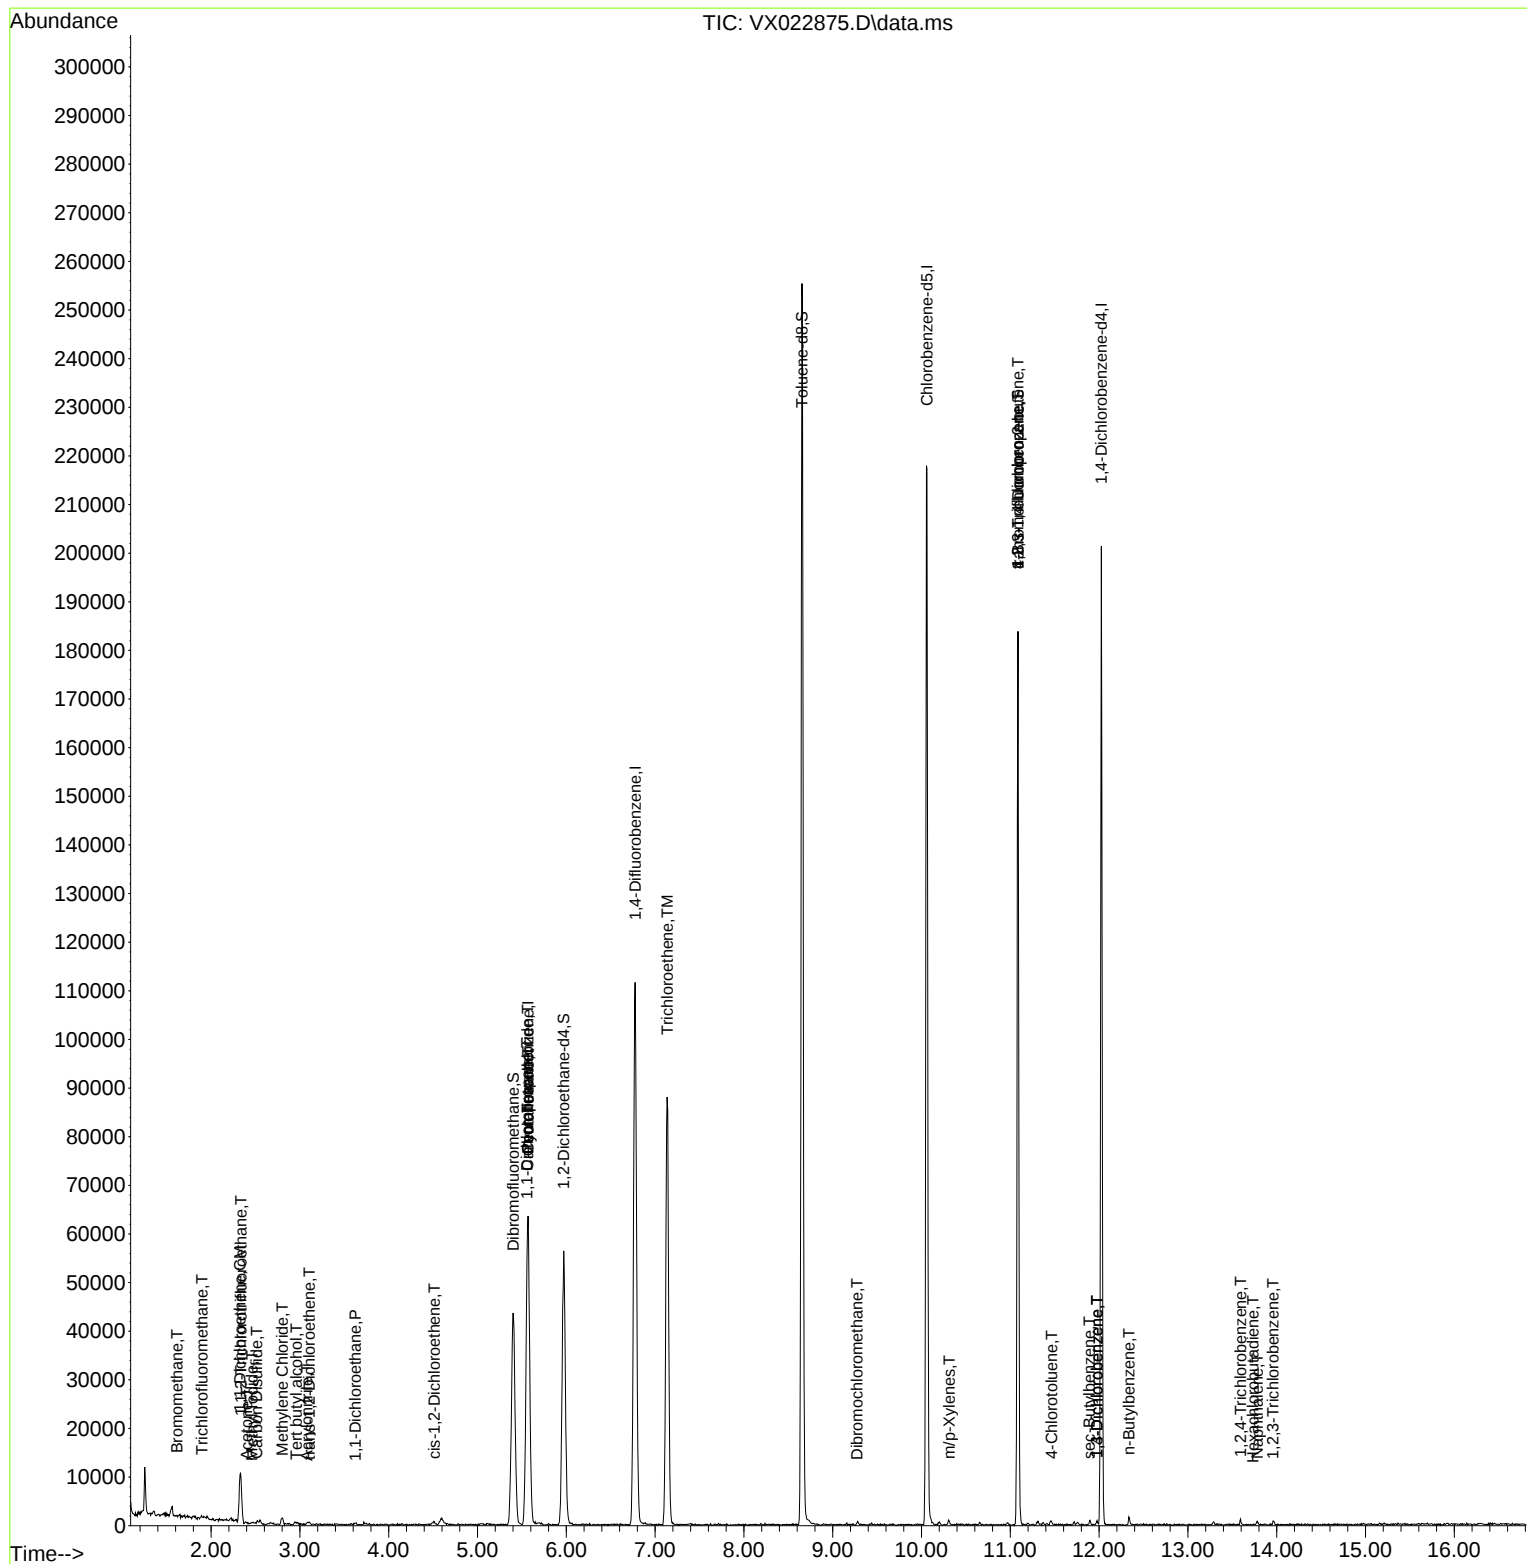






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.012 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618



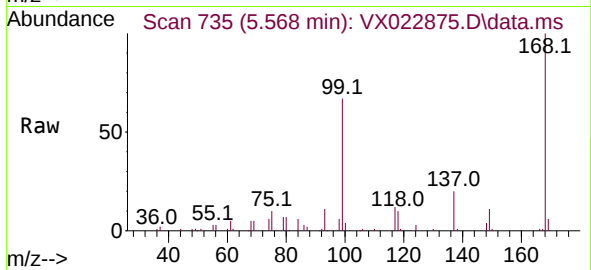



Tgt Ion:168 Resp: 52909
Ion Ratio Lower Upper
168 100
99 67.0 45.8 68.6

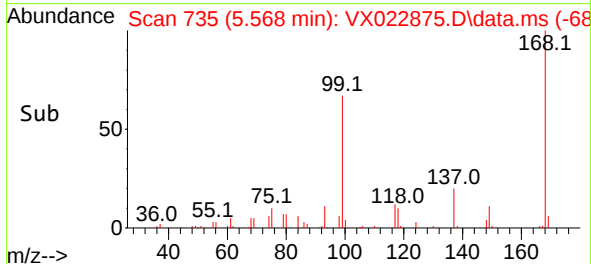

#5
Bromomethane
Concen: 0.70 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 94 Resp: 292
Ion Ratio Lower Upper
94 100
96 126.6 76.4 114.6


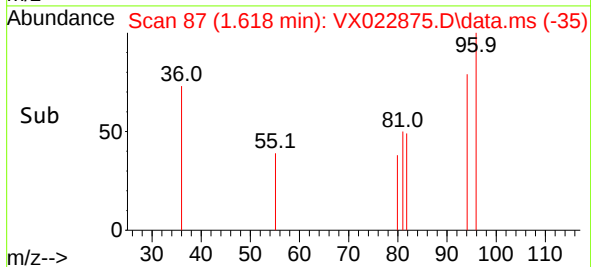

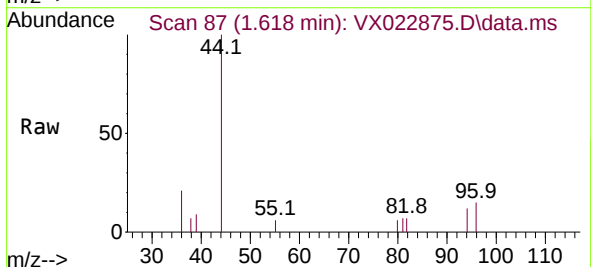




#7
Trichlorofluoromethane
Concen: 0.20 ug/l
RT: 1.898 min Scan# 133
Delta R.T. 0.012 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:101 Resp: 224
Ion Ratio Lower Upper
101 100
103 0.0 53.2 79.8#

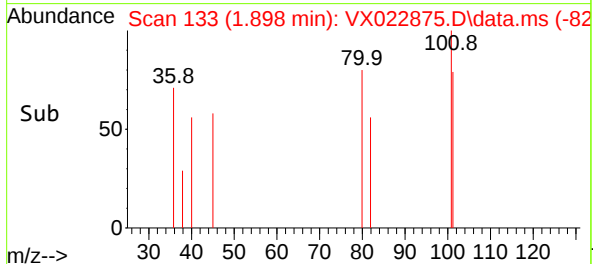

#9
1,1,2-Trichlorotrifluoroethane
Concen: 3.88 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion:101 Resp: 2671
Ion Ratio Lower Upper
101 100
85 45.8 34.9 52.3
151 56.5 61.4 92.2#


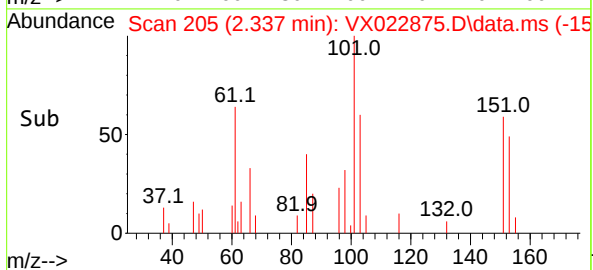

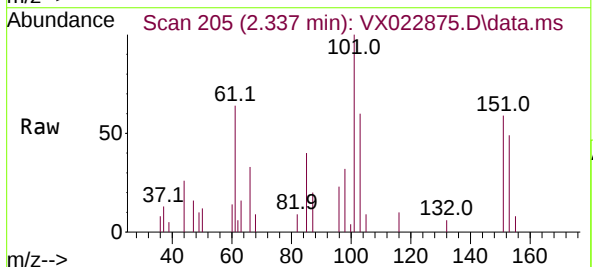




#10
Methyl Iodide
Concen: 4.31 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:142 Resp: 385
Ion Ratio Lower Upper
142 100
127 36.6 33.3 49.9
141 0.0 11.4 17.0#

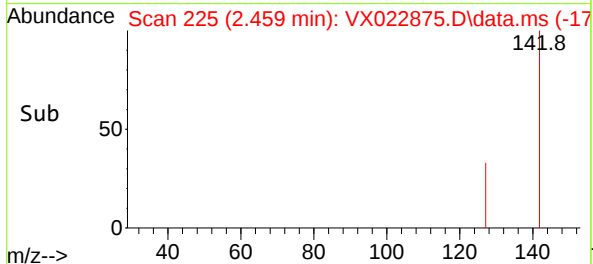

#11
Tert butyl alcohol
Concen: 1.69 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.018 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 59 Resp: 339
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

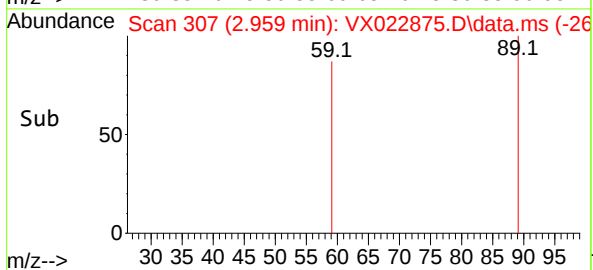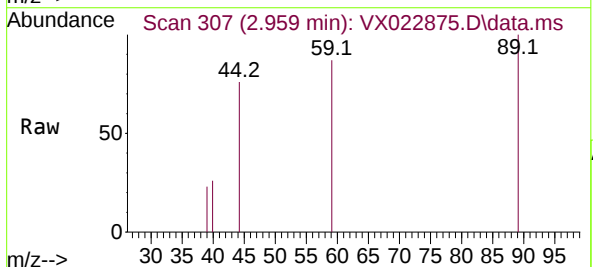



#12

1,1-Dichloroethene

Concen: 2.40 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.007 min

Lab File: VX022875.D

Acq: 24 Jun 2021 17:45





Tgt Ion: 96 Resp: 1649

Ion Ratio Lower Upper

96 100

61 152.4 124.6 187.0

98 62.2 50.6 76.0

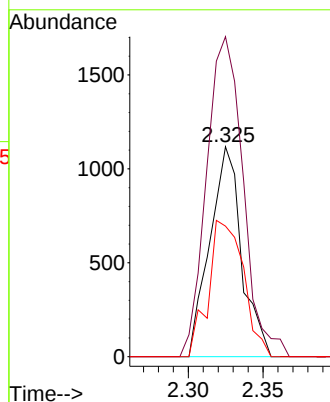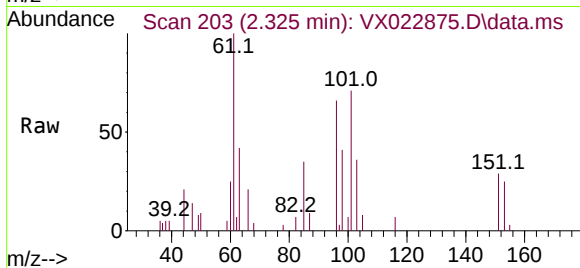

#15

Acrylonitrile

Concen: 0.44 ug/l

RT: 3.081 min Scan# 327

Delta R.T. 0.007 min

Lab File: VX022875.D

Acq: 24 Jun 2021 17:45




Tgt Ion: 53 Resp: 200


Ion Ratio Lower Upper

53 100

52 21.5 65.3 97.9#

51 0.0 28.2 42.2#


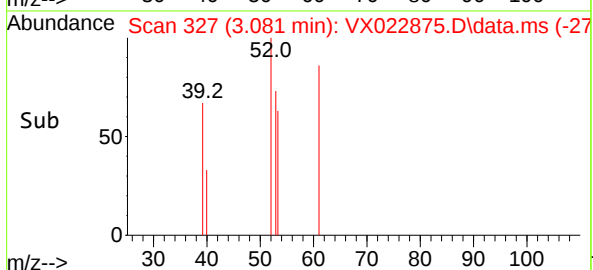

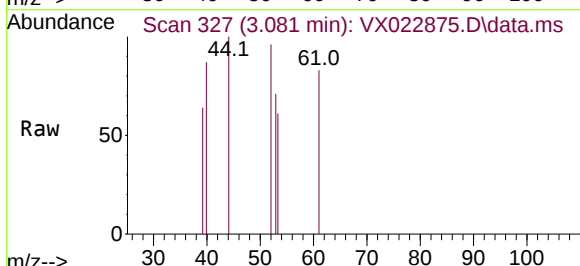




#16
Acetone
Concen: 1.00 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion: 43 Resp: 426
Ion Ratio Lower Upper
43 100
58 0.0 27.8 41.8#

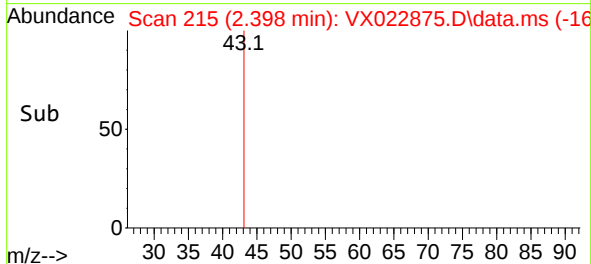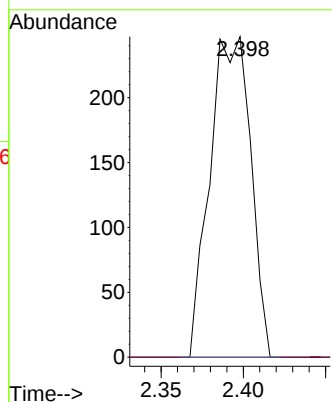

#17
Carbon Disulfide
Concen: 3.91 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 76 Resp: 784
Ion Ratio Lower Upper
76 100
78 12.5 7.2 10.8#

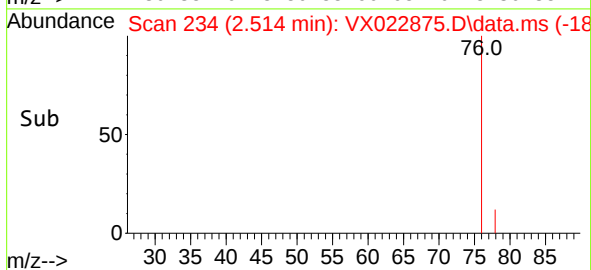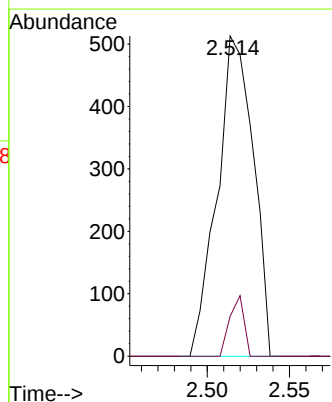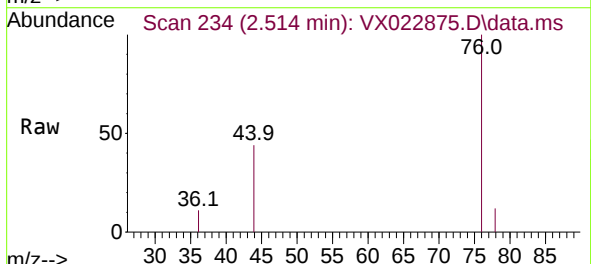







#20
Methylene Chloride
Concen: 1.11 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618

Tgt Ion: 84 Resp: 627




Ion	Ratio	Lower	Upper
84	100		
49	126.3	88.6	132.8
51	38.7	27.0	40.6
86	58.1	50.3	75.5

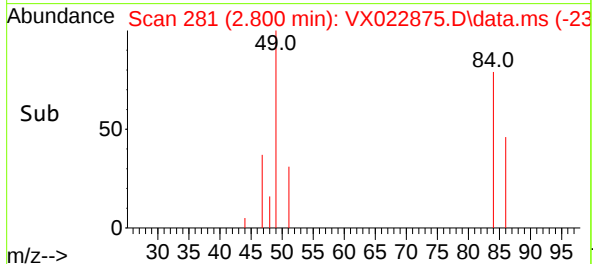


#21
trans-1,2-Dichloroethene
Concen: 0.41 ug/l
RT: 3.105 min Scan# 331
Delta R.T. 0.012 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 96 Resp: 316

Ion	Ratio	Lower	Upper
96	100		
61	69.4	107.7	161.5#
98	28.6	50.4	75.6#


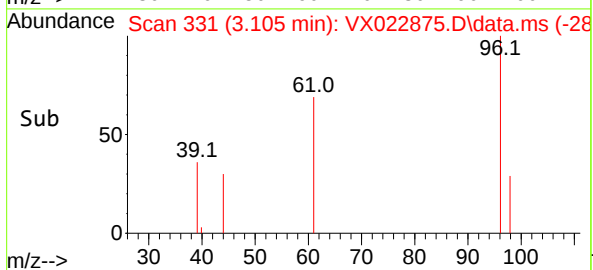

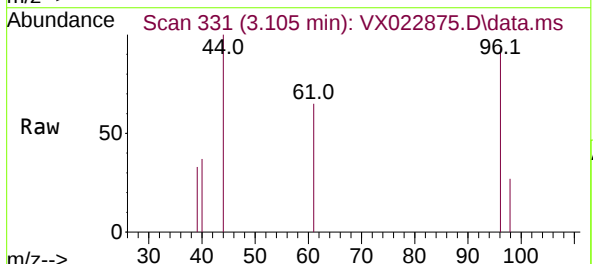




#24
1,1-Dichloroethane
Concen: 0.26 ug/l
RT: 3.623 min Scan# 416
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion: 63 Resp: 377
Ion Ratio Lower Upper
63 100
98 0.0 3.8 11.2#
100 0.0 2.5 7.5#

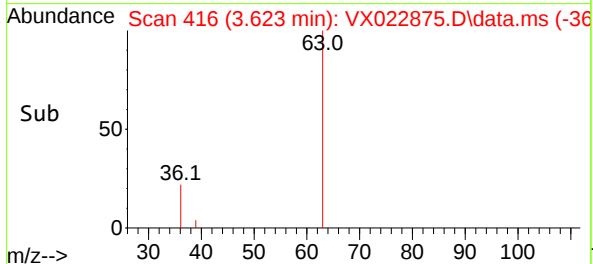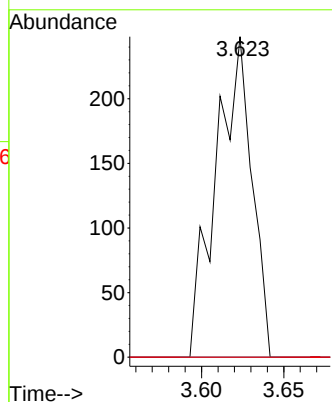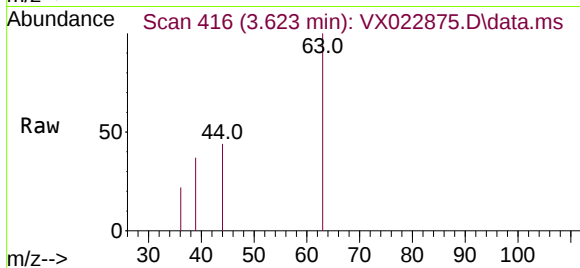

#27
cis-1,2-Dichloroethene
Concen: 0.23 ug/l
RT: 4.513 min Scan# 562
Delta R.T. 0.018 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45


Tgt Ion: 96 Resp: 194
Ion Ratio Lower Upper
96 100
61 285.6 0.0 285.6
98 46.4 0.0 129.6

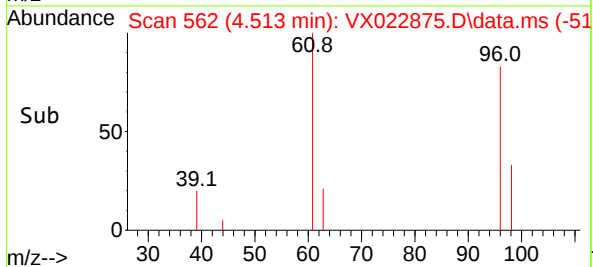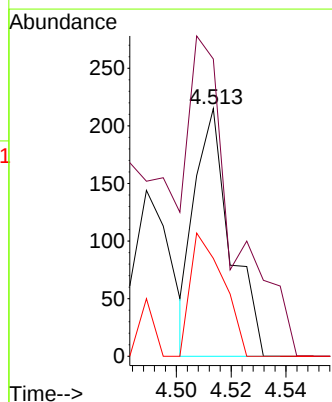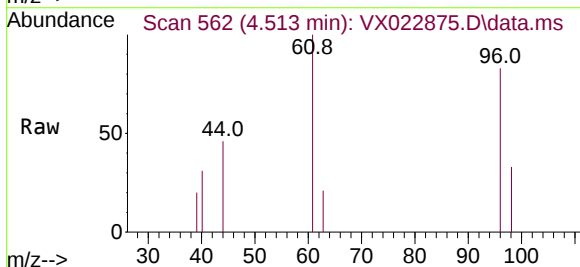






#31
Cyclohexane
Concen: 1.30 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.092 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45


Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618

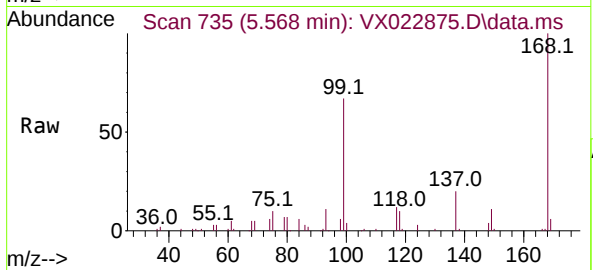



Tgt Ion: 56 Resp: 1768
Ion Ratio Lower Upper
56 100
69 161.5 25.3 37.9#
84 195.6 71.4 107.0#

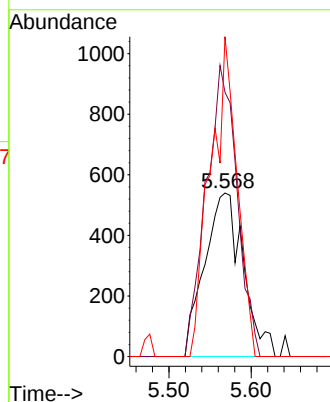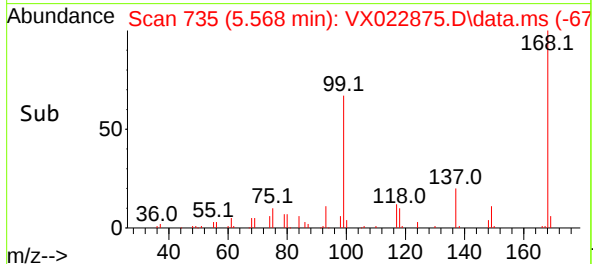


#33
1,2-Dichloroethane-d4
Concen: 51.01 ug/l
RT: 5.971 min Scan# 801
Delta R.T. 0.007 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

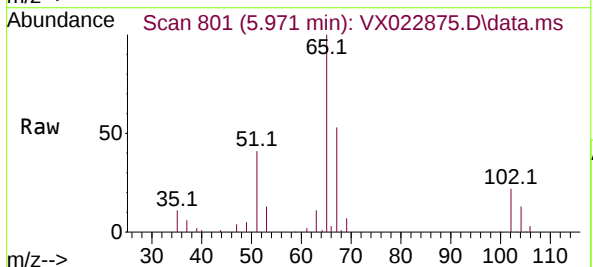

Tgt Ion: 65 Resp: 48977
Ion Ratio Lower Upper
65 100
67 51.9 0.0 105.4









#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.775 min Scan# 933
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:114 Resp: 108832
Ion Ratio Lower Upper
114 100
63 22.9 0.0 40.8
88 16.3 0.0 32.8

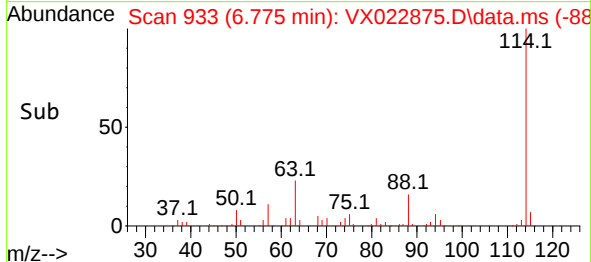

#35
Dibromofluoromethane
Concen: 54.25 ug/l
RT: 5.404 min Scan# 708
Delta R.T. 0.007 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion:113 Resp: 37496
Ion Ratio Lower Upper
113 100
111 102.1 81.9 122.9
192 14.1 16.7 25.1#

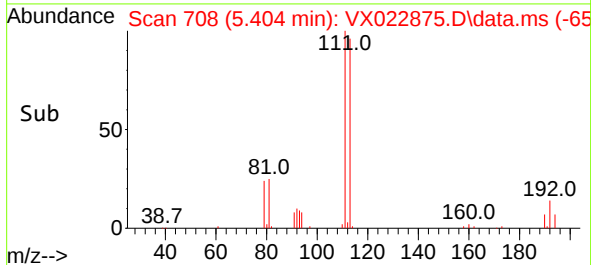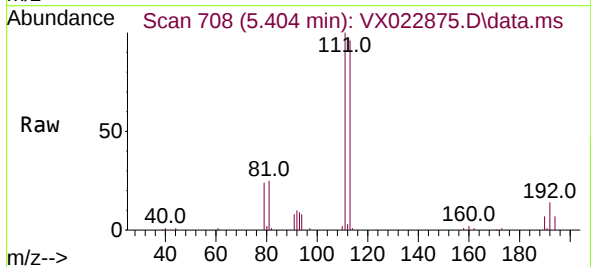



#36

1,1-Dichloropropene

Concen: 4.64 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.146 min

Lab File: VX022875.D

Acq: 24 Jun 2021 17:45

Tgt Ion: 75 Resp: 5359

Ion Ratio Lower Upper

75 100

110 7.8 18.1 54.4#





77 0.0 25.3 37.9#

Instrument :

MSVOA_X

ClientSampleId :

DUP04-20210618



#38

Carbon Tetrachloride

Concen: 6.59 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.128 min

Lab File: VX022875.D

Acq: 24 Jun 2021 17:45




Tgt Ion: 117 Resp: 6389


Ion Ratio Lower Upper

117 100

119 2.9 76.2 114.2#

121 0.0 24.8 37.2#



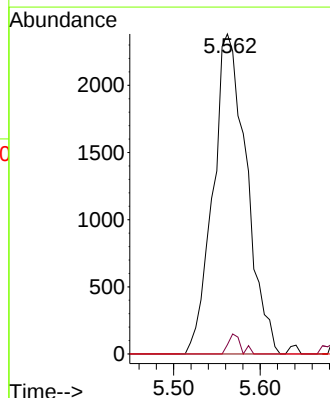
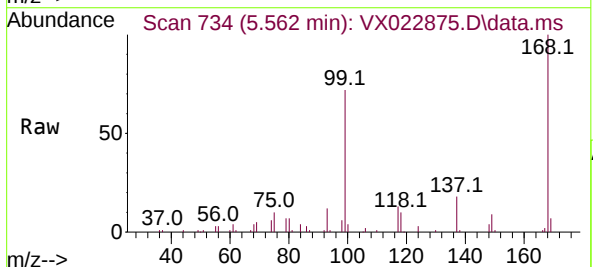




#44
Trichloroethene
Concen: 40.09 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:130 Resp: 31690
Ion Ratio Lower Upper
130 100
95 107.1 0.0 198.0

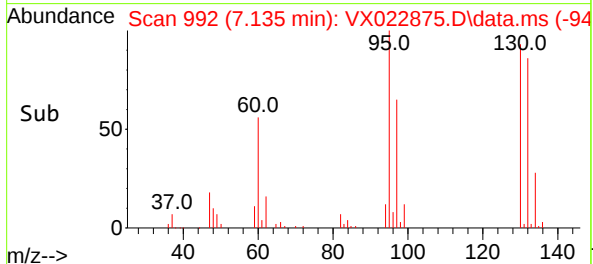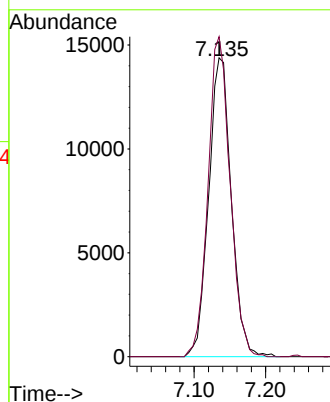

#50
Toluene-d8
Concen: 53.03 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 98 Resp: 143647
Ion Ratio Lower Upper
98 100
100 66.6 51.9 77.9




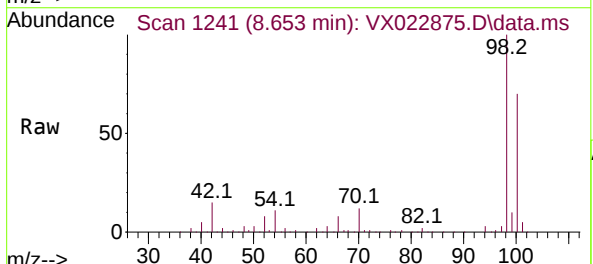




#60
Dibromochloromethane
Concen: 3.81 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.249 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:129 Resp: 133
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

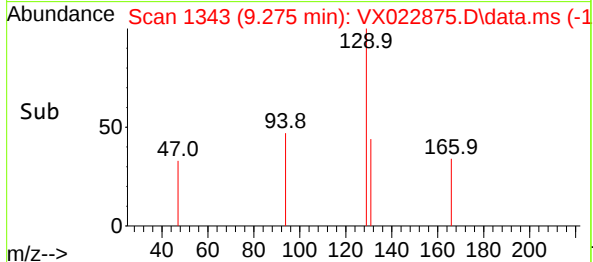

#62
4-Bromofluorobenzene
Concen: 48.08 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 95 Resp: 48602
Ion Ratio Lower Upper
95 100
174 61.8 0.0 154.6
176 57.3 0.0 155.8


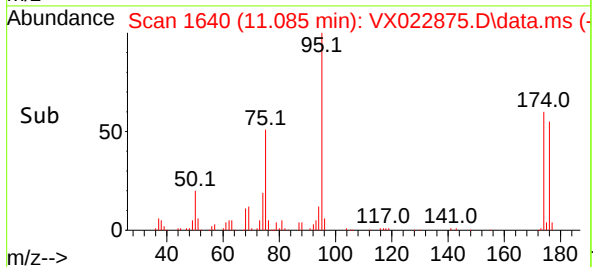

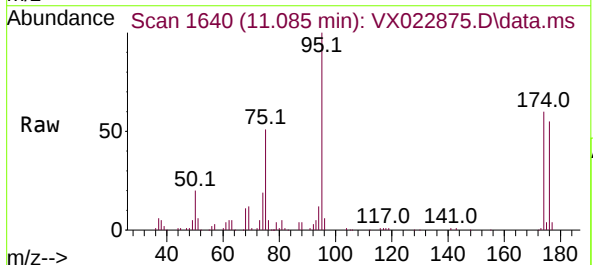




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:117 Resp: 93483
Ion Ratio Lower Upper
117 100
82 60.1 47.4 71.2
119 33.1 26.6 39.8

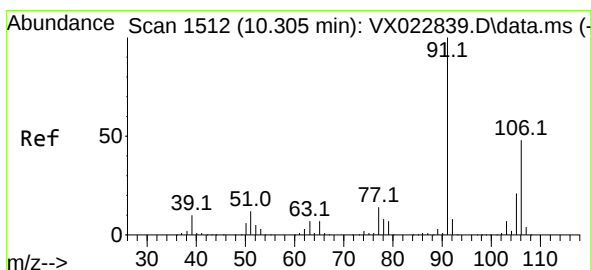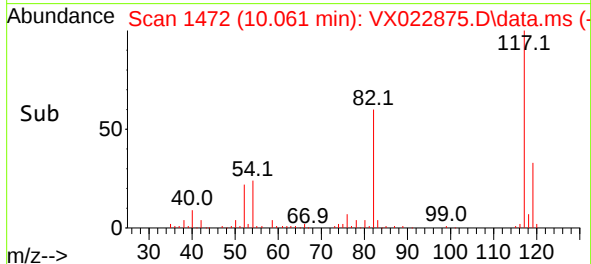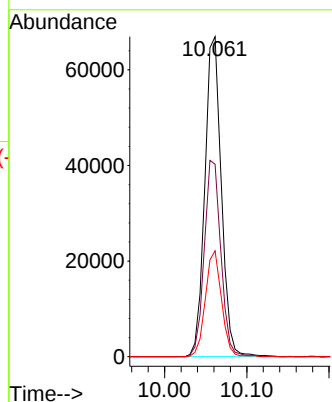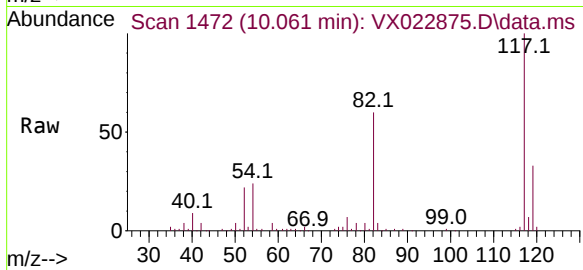

#68
m/p-Xylenes
Concen: 0.21 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion:106 Resp: 281
Ion Ratio Lower Upper
106 100
91 204.6 162.8 244.2


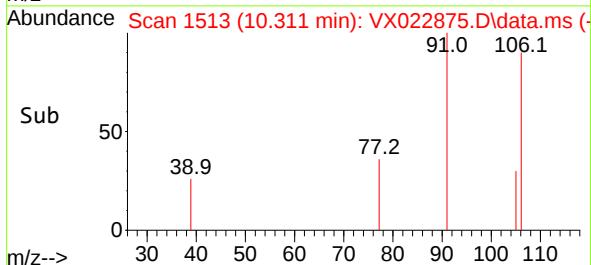

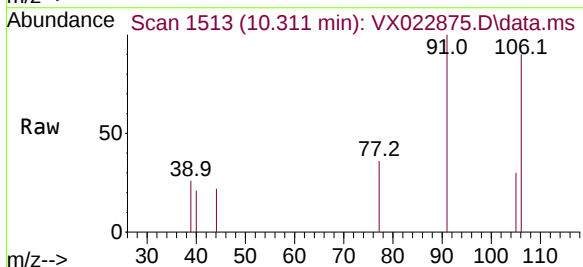




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX022875.D
 Acq: 24 Jun 2021 17:45




Instrument :
 MSVOA_X
 ClientSampleId :
 DUP04-20210618


Tgt Ion:152 Resp: 34731
 Ion Ratio Lower Upper
 152 100
 115 67.7 41.1 123.3
 150 157.7 0.0 349.0

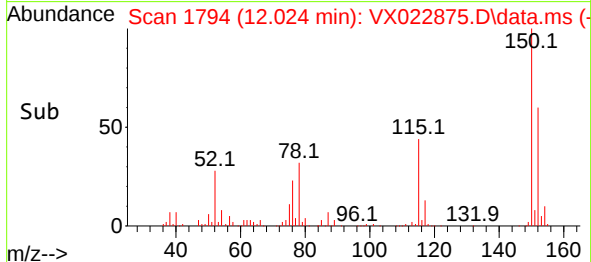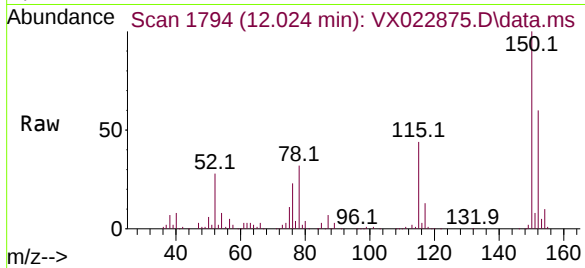

#76
 1,2,3-Trichloropropane
 Concen: 28.98 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX022875.D
 Acq: 24 Jun 2021 17:45

Tgt Ion: 75 Resp: 26589
 Ion Ratio Lower Upper
 75 100
 77 1.2 19.1 57.5#


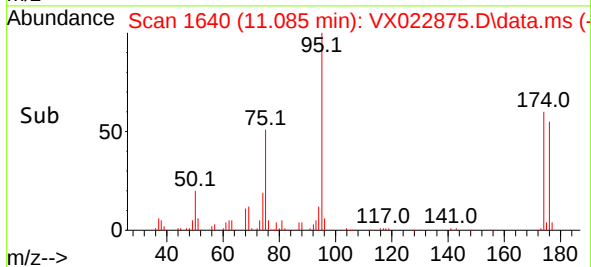

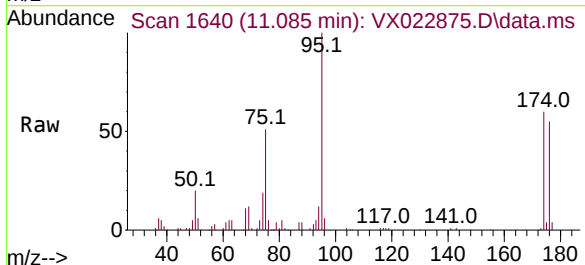




#81
trans-1,4-Dichloro-2-butene
Concen: 74.60 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion: 75 Resp: 26589
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

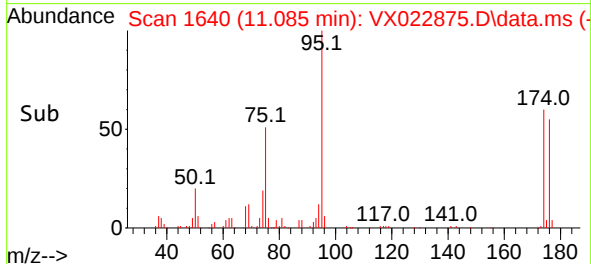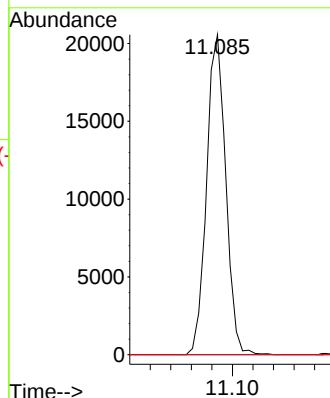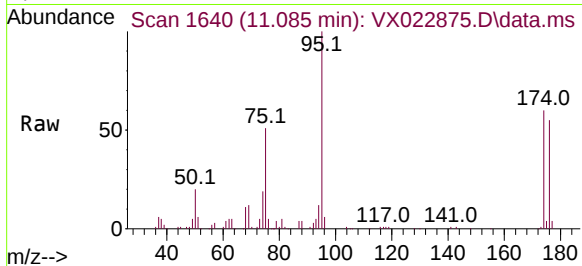

#82
4-Chlorotoluene
Concen: 0.22 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 91 Resp: 546
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


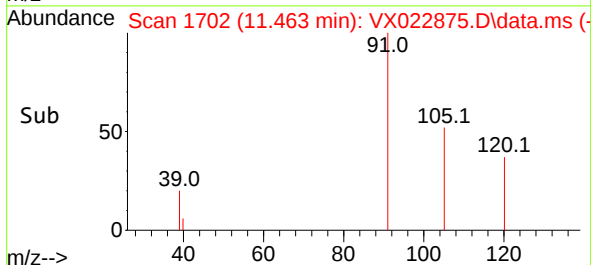
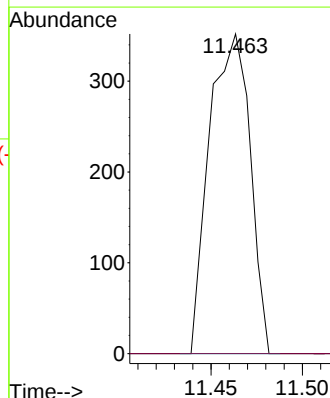
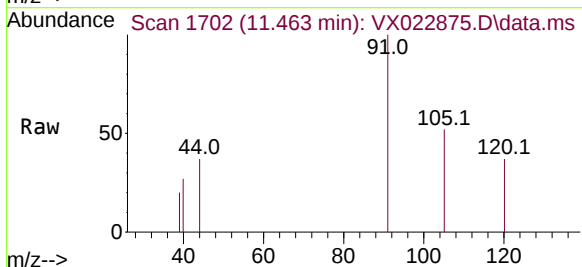




#85
 sec-Butylbenzene
 Concen: 0.21 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. -0.006 min
 Lab File: VX022875.D
 Acq: 24 Jun 2021 17:45




Instrument :
 MSVOA_X
 ClientSampleId :
 DUP04-20210618


Tgt Ion:105 Resp: 655
 Ion Ratio Lower Upper
 105 100
 134 22.6 10.0 29.8

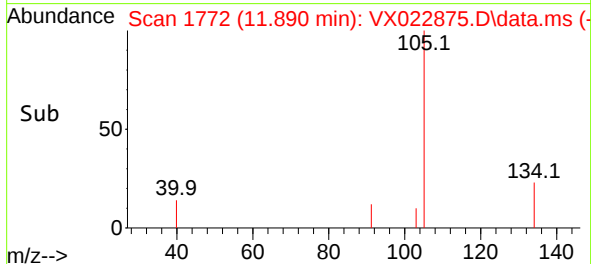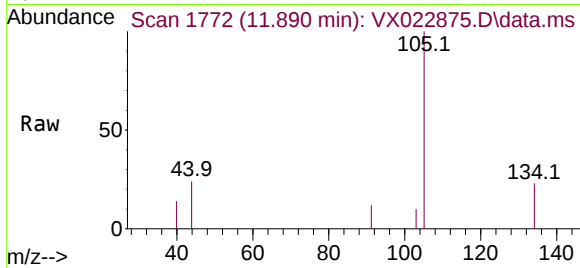

#87
 1,3-Dichlorobenzene
 Concen: 0.22 ug/l
 RT: 11.976 min Scan# 1786
 Delta R.T. 0.001 min
 Lab File: VX022875.D
 Acq: 24 Jun 2021 17:45

Tgt Ion:146 Resp: 264
 Ion Ratio Lower Upper
 146 100
 111 48.1 20.2 60.5
 148 60.6 31.9 95.7


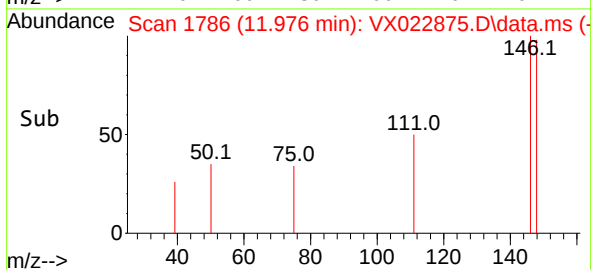

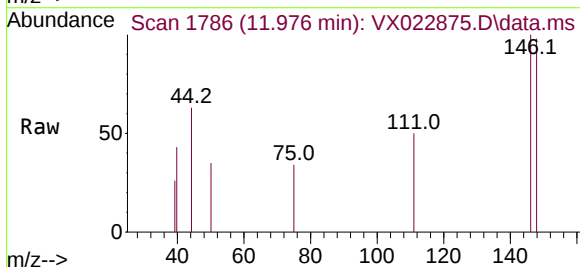




#88
1,4-Dichlorobenzene
Concen: 0.21 ug/l
RT: 11.976 min Scan# 1786
Delta R.T. -0.066 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:146	Resp:	264
Ion	Ratio	Lower Upper
146	100	
111	48.1	19.6 58.8
148	60.6	31.6 95.0

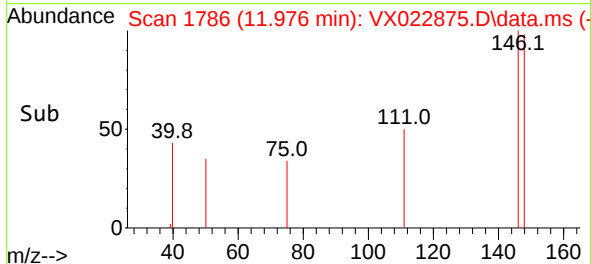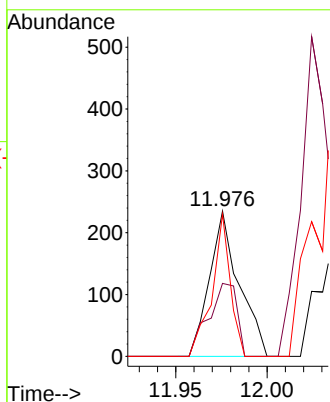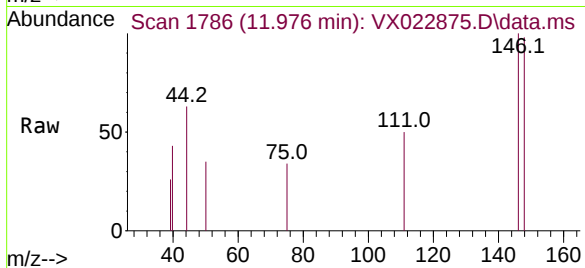

#89
n-Butylbenzene
Concen: 0.22 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion: 91	Resp:	508
Ion	Ratio	Lower Upper
91	100	
92	56.9	27.4 82.0
134	31.5	13.2 39.5


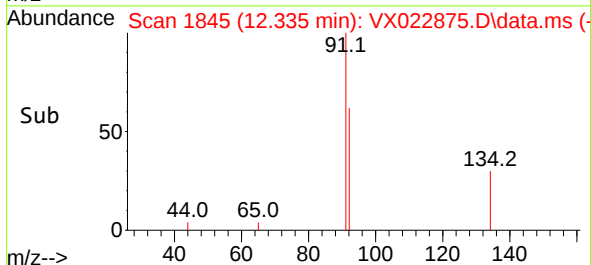

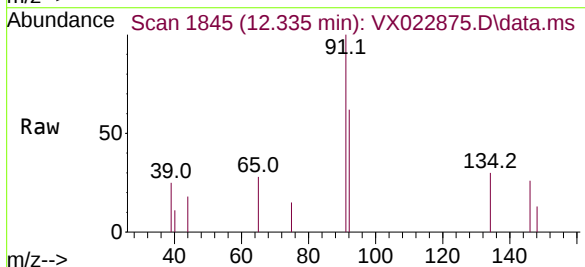




#93
1,2,4-Trichlorobenzene
Concen: 0.35 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.000 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618


Tgt Ion:180	Resp:	221
Ion	Ratio	Lower Upper
180	100	
182	102.3	47.7 143.1
145	16.3	15.0 45.0

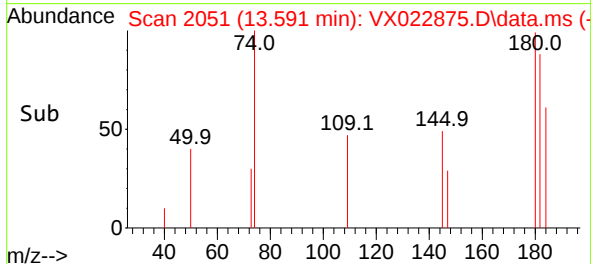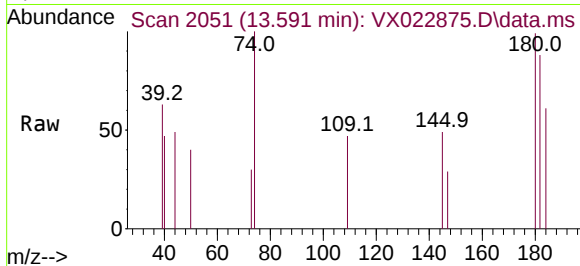

#94
Hexachlorobutadiene
Concen: 0.21 ug/l
RT: 13.731 min Scan# 2074
Delta R.T. 0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion:225	Resp:	53
Ion	Ratio	Lower Upper
225	100	
223	0.0	31.1 93.2#
227	0.0	31.6 95.0#


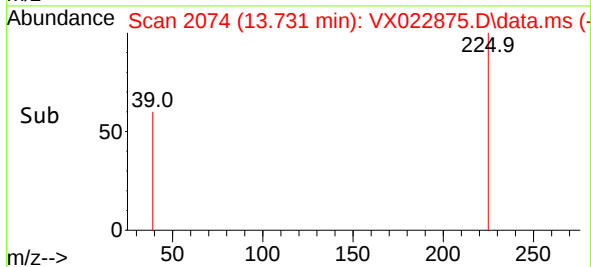

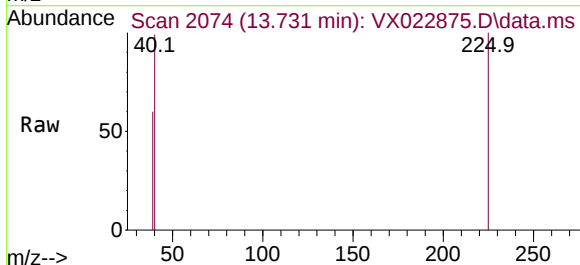




#95
Naphthalene
Concen: 2.15 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20210618

Tgt Ion:128 Resp: 666
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.8 13.2#

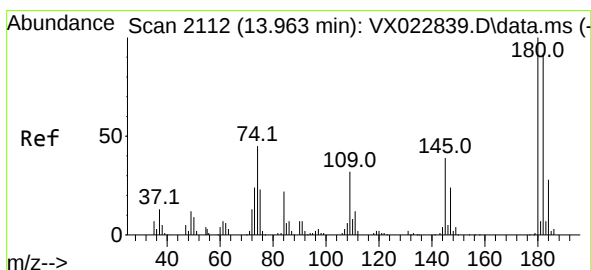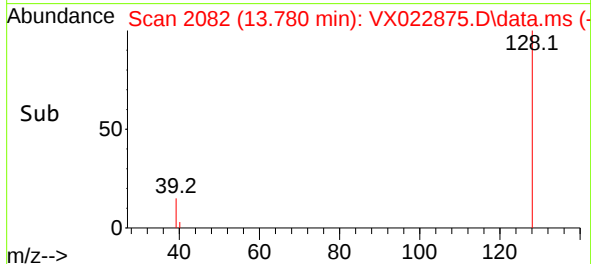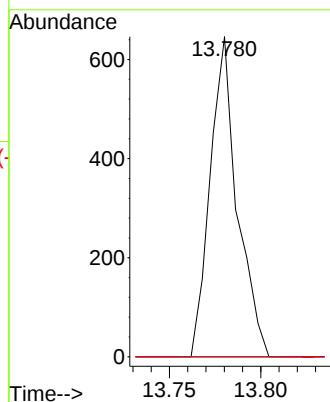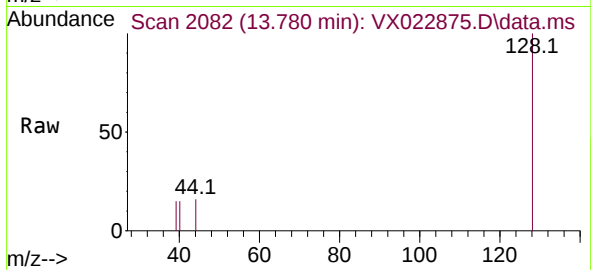

#96
1,2,3-Trichlorobenzene
Concen: 0.39 ug/l
RT: 13.957 min Scan# 2111
Delta R.T. -0.006 min
Lab File: VX022875.D
Acq: 24 Jun 2021 17:45

Tgt Ion:180 Resp: 250
Ion Ratio Lower Upper
180 100
182 90.8 47.6 142.9
145 22.0 16.1 48.3

