

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
 Data File : VX022869.D
 Acq On : 24 Jun 2021 13:37
 Operator : JC/MD
 Sample : M2783-14 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP03-20210617

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Title : SW846 8260

Signal : TIC: VX022869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rVB2	8983	9533	2.39%	0.451%
2	1.569	73	79	82	rBV3	3060	4397	1.10%	0.208%
3	5.397	696	707	719	rBV3	42445	120700	30.28%	5.707%
4	5.562	722	734	746	rBV	64010	178722	44.83%	8.450%
5	5.964	790	800	813	rBV	56000	148902	37.35%	7.040%
6	6.769	922	932	944	rBV	112435	266520	66.86%	12.601%
7	7.129	982	991	1002	rBV	97965	206324	51.76%	9.755%
8	8.653	1234	1241	1249	rBV	257294	398623	100.00%	18.847%
9	10.055	1465	1471	1483	rBV	222467	311699	78.19%	14.737%
10	11.085	1634	1640	1648	rVB	175973	224684	56.37%	10.623%
11	12.024	1789	1794	1802	rVB	201013	244986	61.46%	11.583%




Sum of corrected areas: 2115090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022869.D
Acq On : 24 Jun 2021 13:37
Operator : JC/MD
Sample : M2783-14 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20210617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

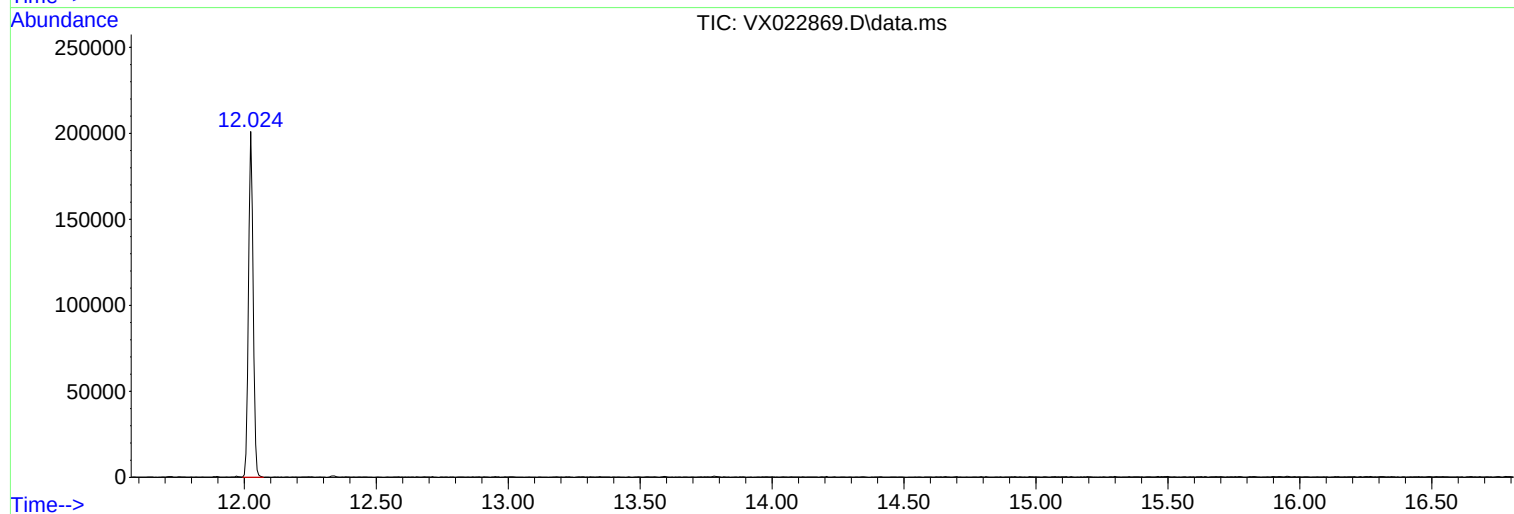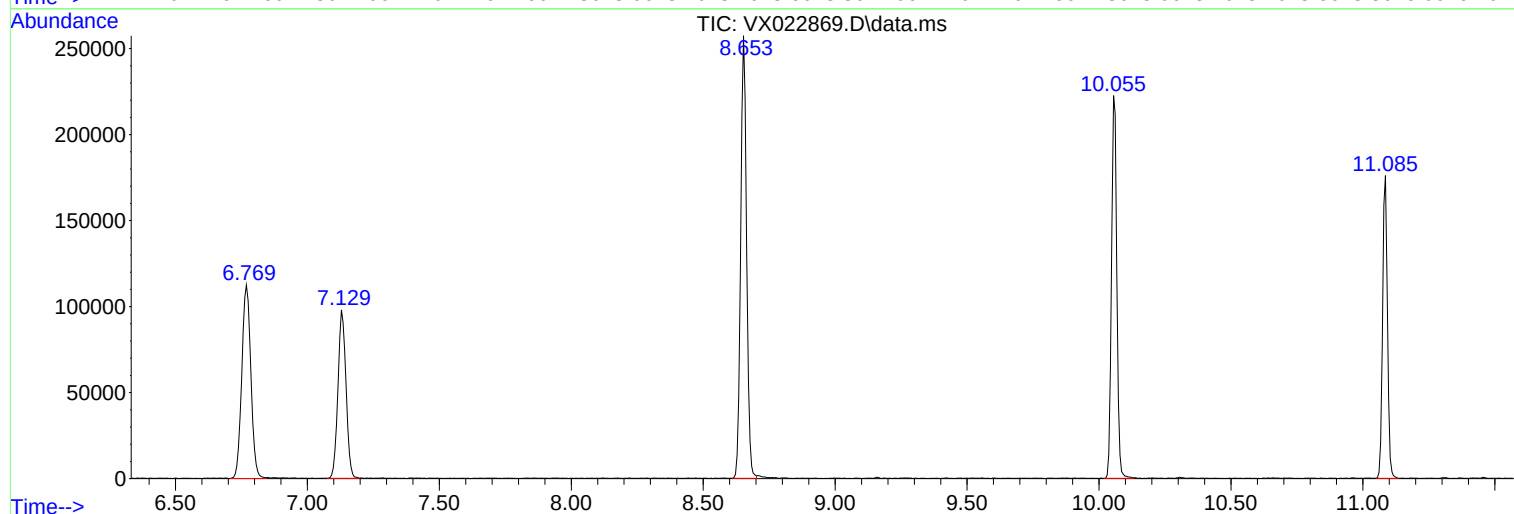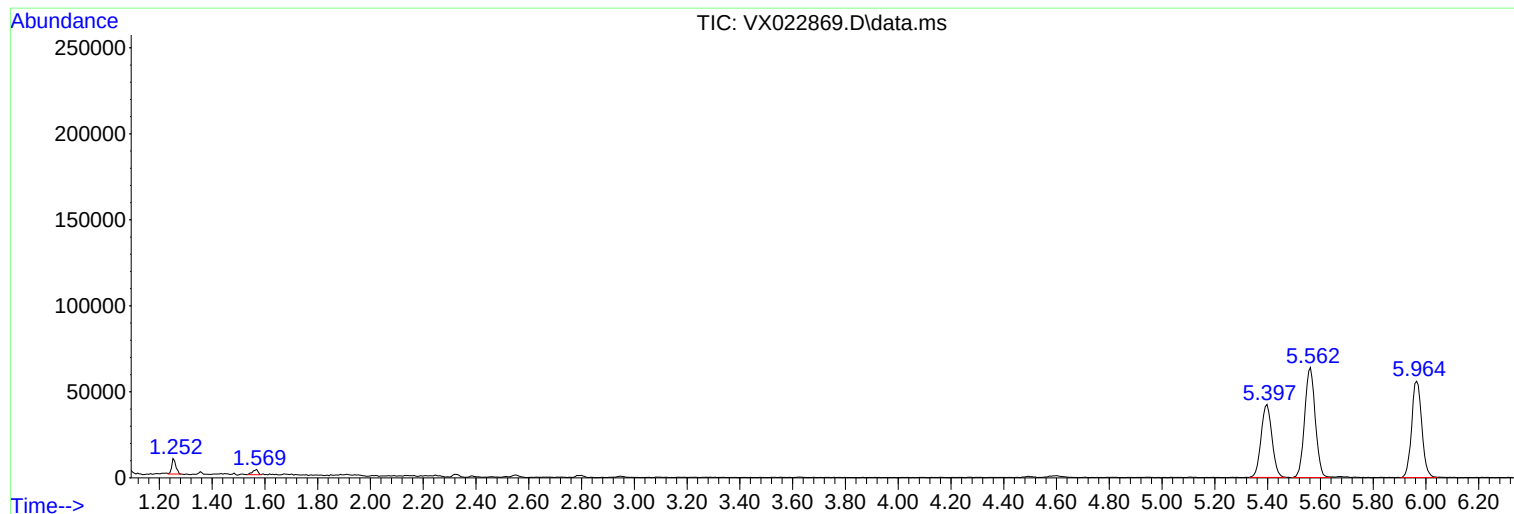

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022869.D
Acq On : 24 Jun 2021 13:37
Operator : JC/MD
Sample : M2783-14 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20210617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022869.D
Acq On : 24 Jun 2021 13:37
Operator : JC/MD
Sample : M2783-14 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20210617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
