

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
 Data File : VX022907.D
 Acq On : 25 Jun 2021 07:29
 Operator : JC/MD
 Sample : M2838-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE103D1-20210621

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX022907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	198	204	211	rBV2	13976	25658	1.08%	0.609%
2	5.397	696	707	718	rBV	38432	107246	4.50%	2.545%
3	5.562	723	734	747	rBV2	60843	168763	7.08%	4.005%
4	5.964	789	800	817	rBV2	50799	133761	5.61%	3.175%
5	6.769	922	932	943	rBV	106448	252733	10.60%	5.998%
6	7.135	982	992	1018	rBV	1083510	2384607	100.00%	56.595%
7	8.653	1234	1241	1251	rBV	226196	353299	14.82%	8.385%
8	9.275	1338	1343	1349	rBV2	20517	30965	1.30%	0.735%
9	10.055	1466	1471	1478	rBV	222473	301213	12.63%	7.149%
10	11.085	1634	1640	1649	rVB	162113	205407	8.61%	4.875%
11	12.024	1789	1794	1802	rVB	205844	249791	10.48%	5.928%




Sum of corrected areas: 4213443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022907.D
Acq On : 25 Jun 2021 07:29
Operator : JC/MD
Sample : M2838-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D1-20210621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

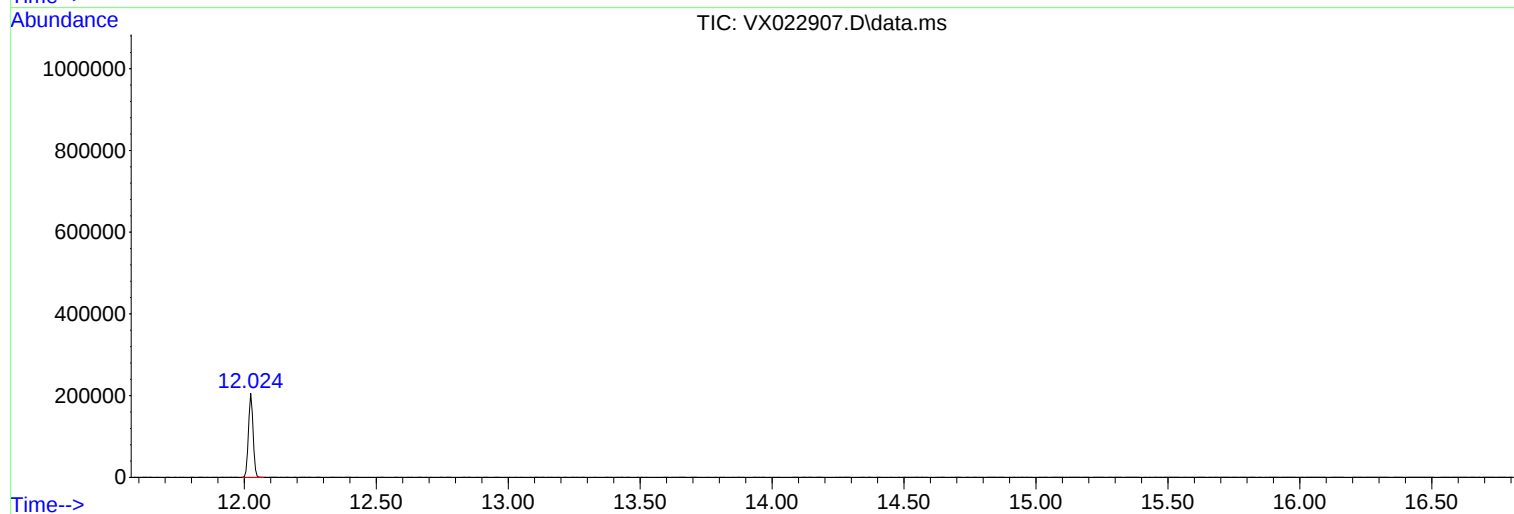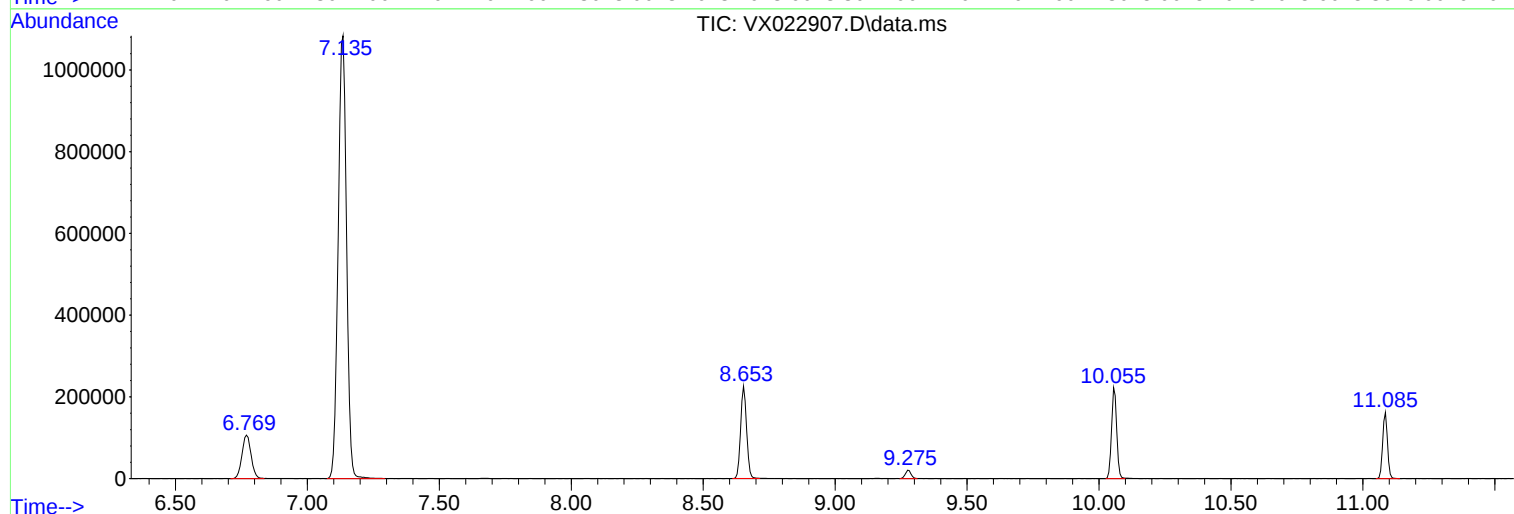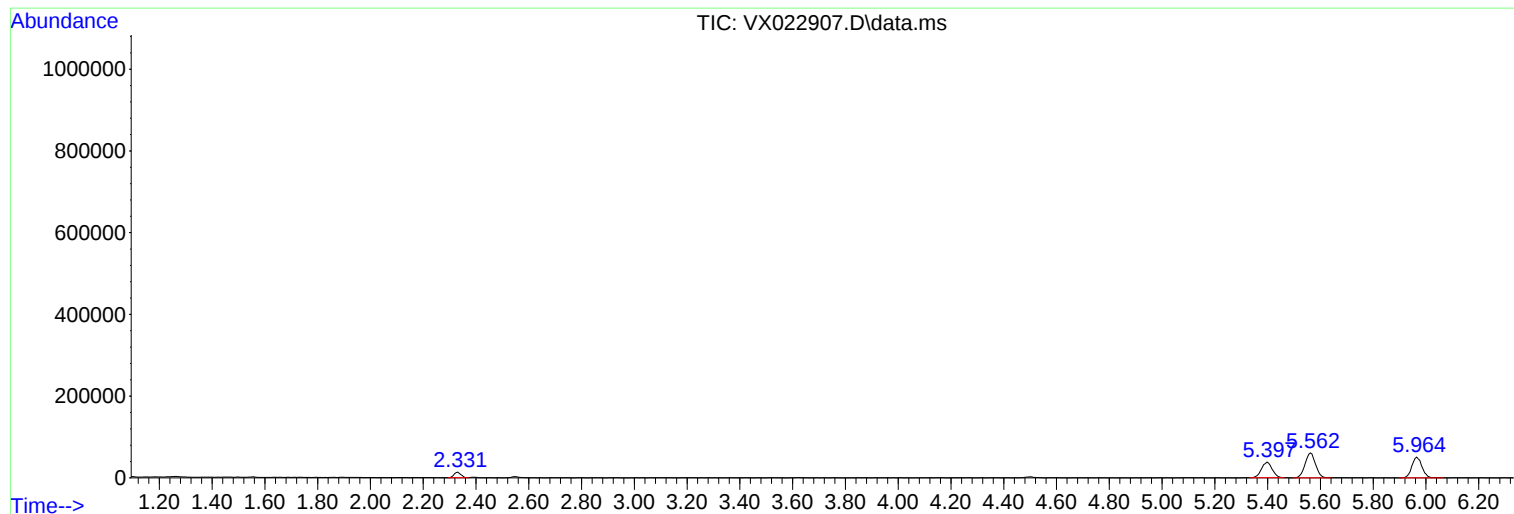

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022907.D
Acq On : 25 Jun 2021 07:29
Operator : JC/MD
Sample : M2838-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D1-20210621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062421\
Data File : VX022907.D
Acq On : 25 Jun 2021 07:29
Operator : JC/MD
Sample : M2838-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D1-20210621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc