

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029794.D
 Acq On : 25 Jun 2022 03:07
 Operator : JC/MD
 Sample : N3386-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB01-20220613

Quant Time: Jun 25 05:32:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	261662	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	433802	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	374603	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	162812	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	137369	39.660	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	79.320%
35) Dibromofluoromethane	5.391	113	125627	44.438	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.880%
50) Toluene-d8	8.653	98	485680	47.027	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.060%
62) 4-Bromofluorobenzene	11.079	95	173478	44.542	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029794.D
Acq On : 25 Jun 2022 03:07
Operator : JC/MD
Sample : N3386-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20220613

Quant Time: Jun 25 05:32:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




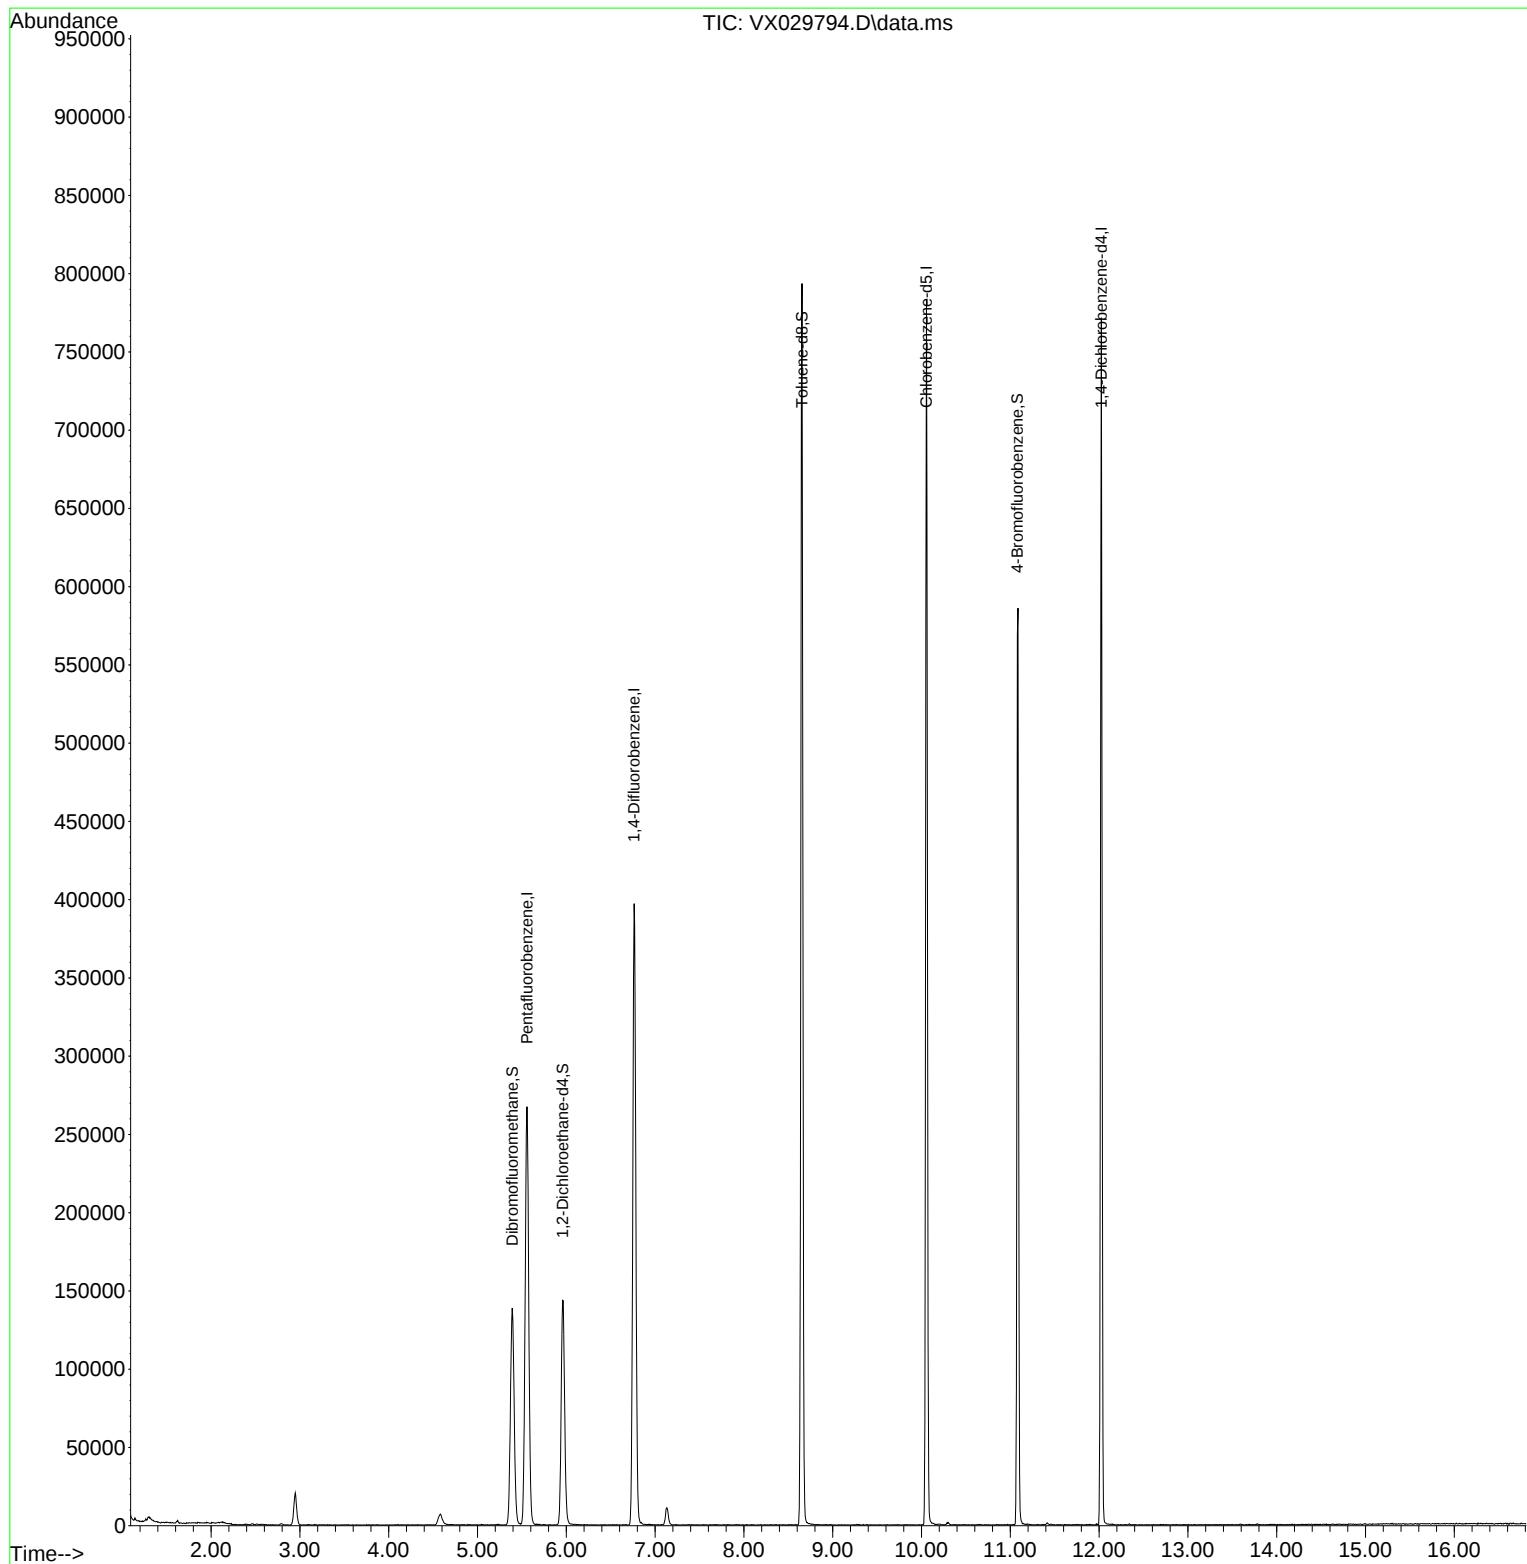


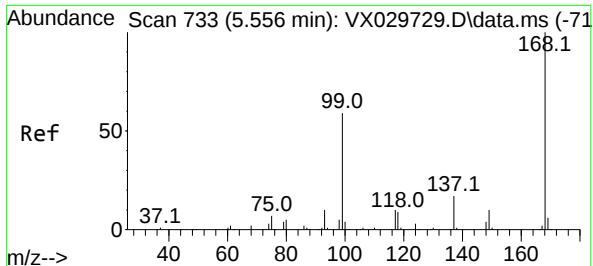

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07




Instrument :
MSVOA_X
ClientSampleId :
TB01-20220613


Tgt Ion:168 Resp: 261662
Ion Ratio Lower Upper
168 100
99 57.6 41.7 62.5

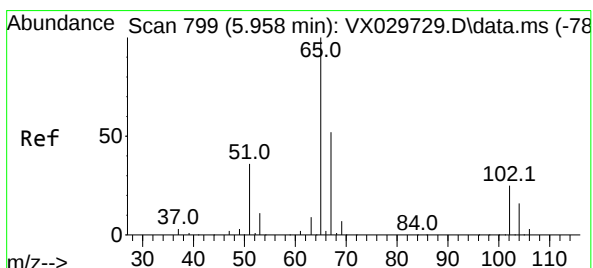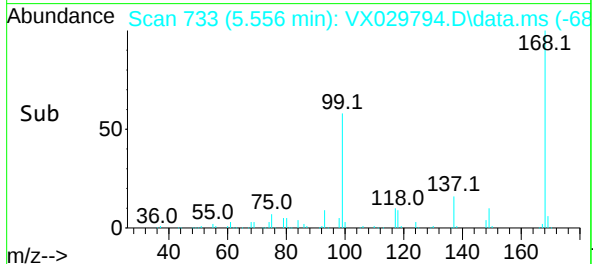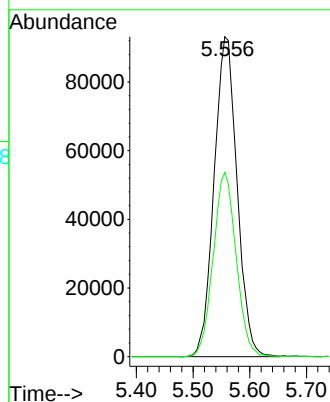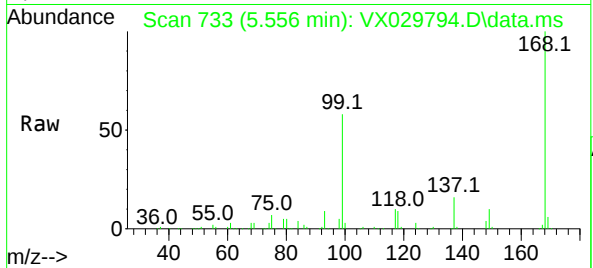

#33
1,2-Dichloroethane-d4
Concen: 39.660 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07

Tgt Ion: 65 Resp: 137369
Ion Ratio Lower Upper
65 100
67 54.4 0.0 107.4


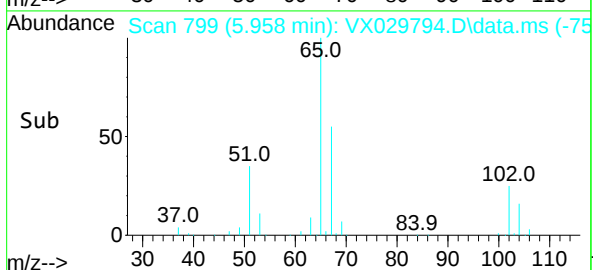
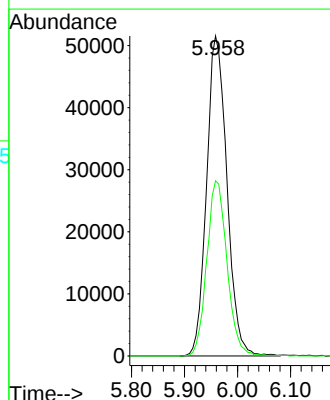
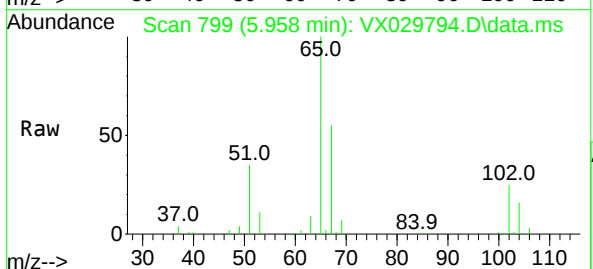


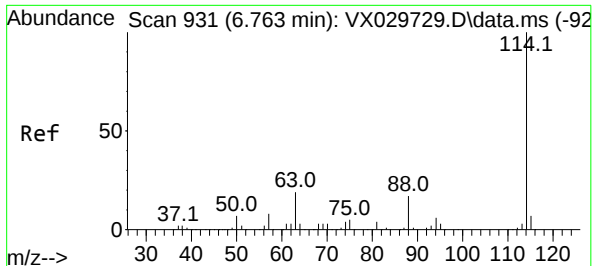

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07




Instrument :
MSVOA_X
ClientSampleId :
TB01-20220613


Tgt Ion:114 Resp: 433802
Ion Ratio Lower Upper
114 100
63 19.0 0.0 36.8
88 16.6 0.0 32.4

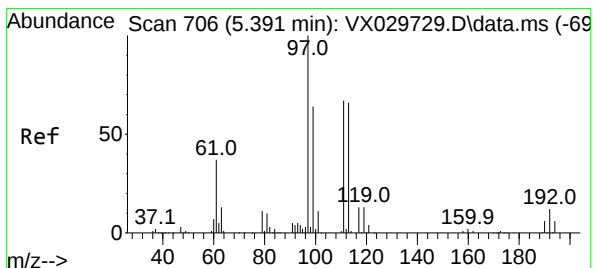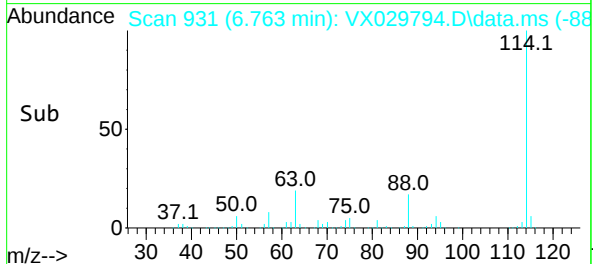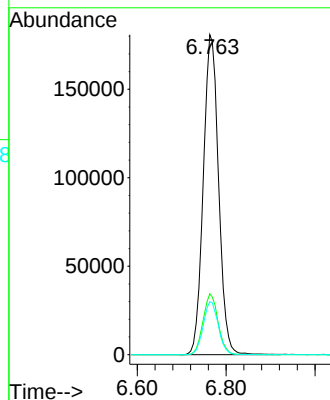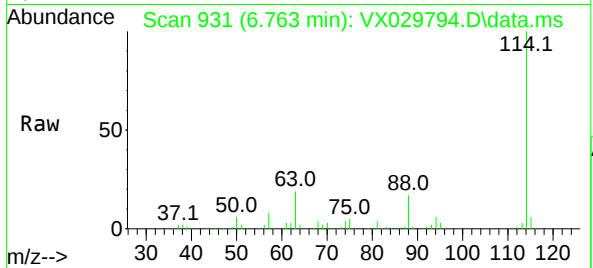

#35
Dibromofluoromethane
Concen: 44.438 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07

Tgt Ion:113 Resp: 125627
Ion Ratio Lower Upper
113 100
111 103.3 82.8 124.2
192 19.3 16.9 25.3


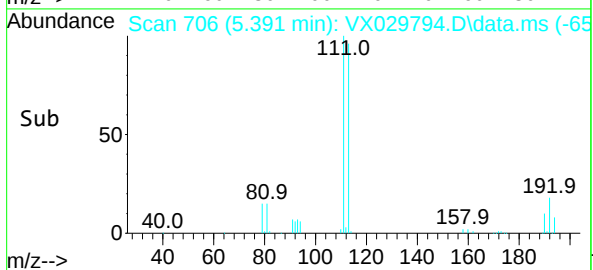
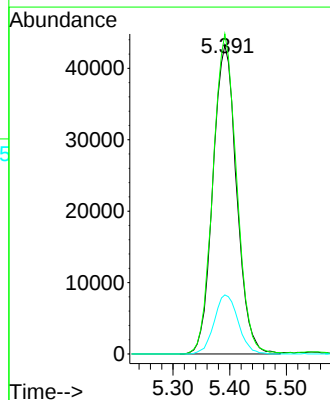
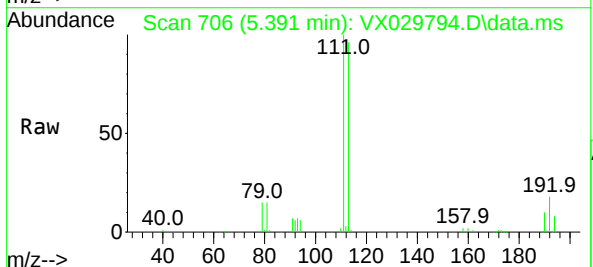


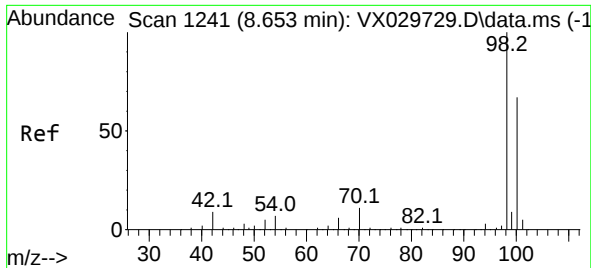

#50
Toluene-d8
Concen: 47.027 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07




Instrument :
MSVOA_X
ClientSampleId :
TB01-20220613


Tgt Ion: 98 Resp: 485680
Ion Ratio Lower Upper
98 100
100 67.0 52.6 78.8

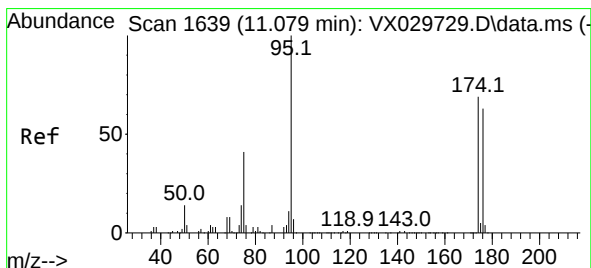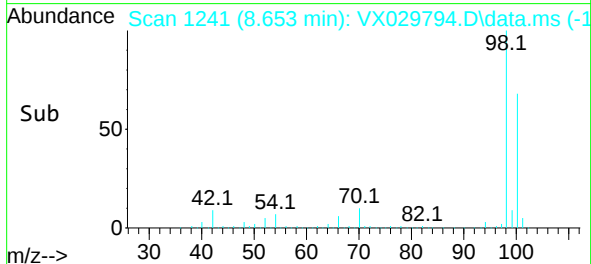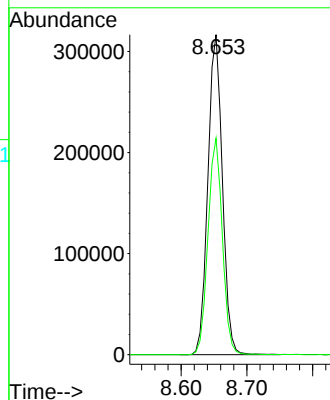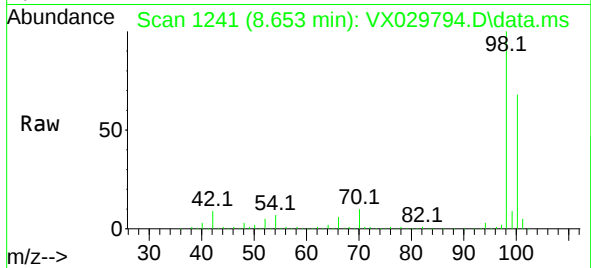

#62
4-Bromofluorobenzene
Concen: 44.542 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07

Tgt Ion: 95 Resp: 173478
Ion Ratio Lower Upper
95 100
174 74.1 0.0 163.0
176 73.3 0.0 155.0


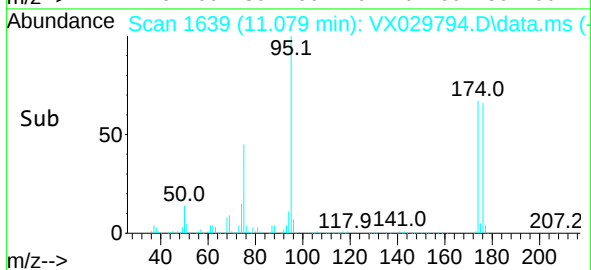
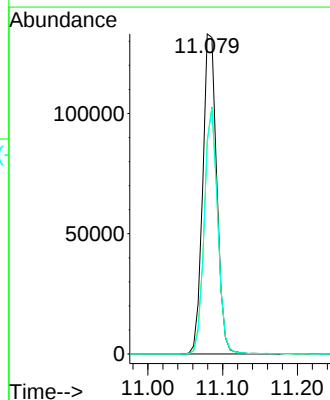
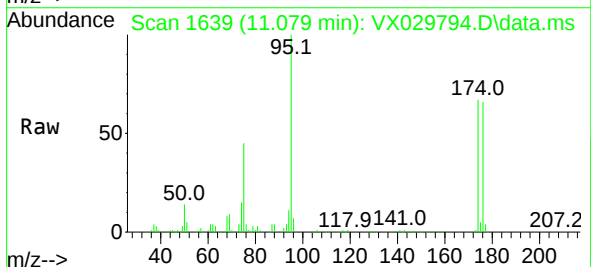


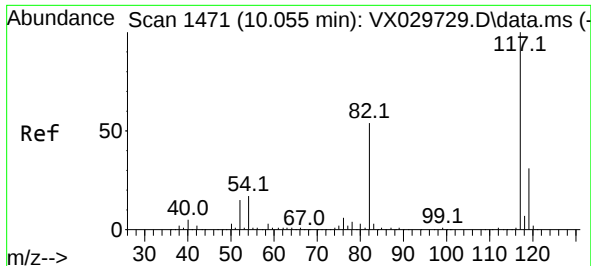

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07

Instrument :
MSVOA_X
ClientSampleId :
TB01-20220613

Tgt Ion:117 Resp: 374603
Ion Ratio Lower Upper
117 100
82 54.6 41.8 62.8
119 33.1 24.8 37.2

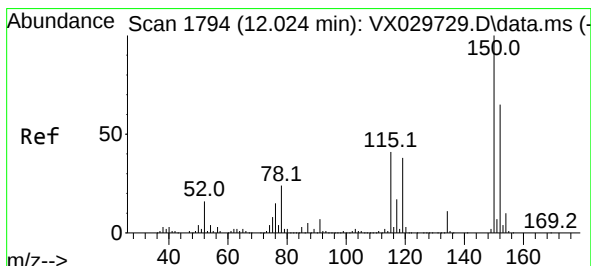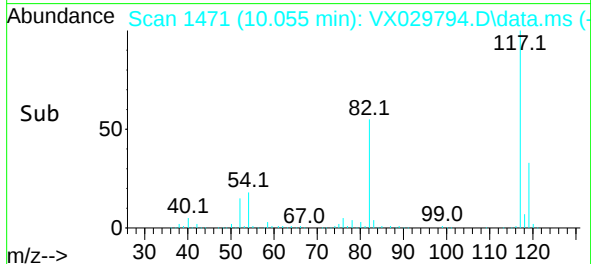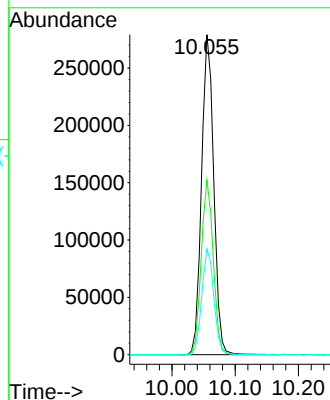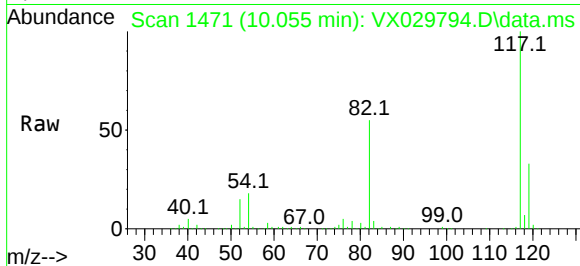

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX029794.D
Acq: 25 Jun 2022 03:07

Tgt Ion:152 Resp: 162812
Ion Ratio Lower Upper
152 100
115 62.8 37.5 112.7
150 158.4 0.0 338.2

