

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029801.D
 Acq On : 25 Jun 2022 05:50
 Operator : JC/MD
 Sample : N3386-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE117D2-20220615

Quant Time: Jun 25 09:05:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	262887	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	437159	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	380006	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	162740	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	141607	40.693	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	81.380%
35) Dibromofluoromethane	5.391	113	128095	44.963	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.920%
50) Toluene-d8	8.653	98	486357	46.731	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	93.460%
62) 4-Bromofluorobenzene	11.085	95	173644	44.242	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029801.D
Acq On : 25 Jun 2022 05:50
Operator : JC/MD
Sample : N3386-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20220615

Quant Time: Jun 25 09:05:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




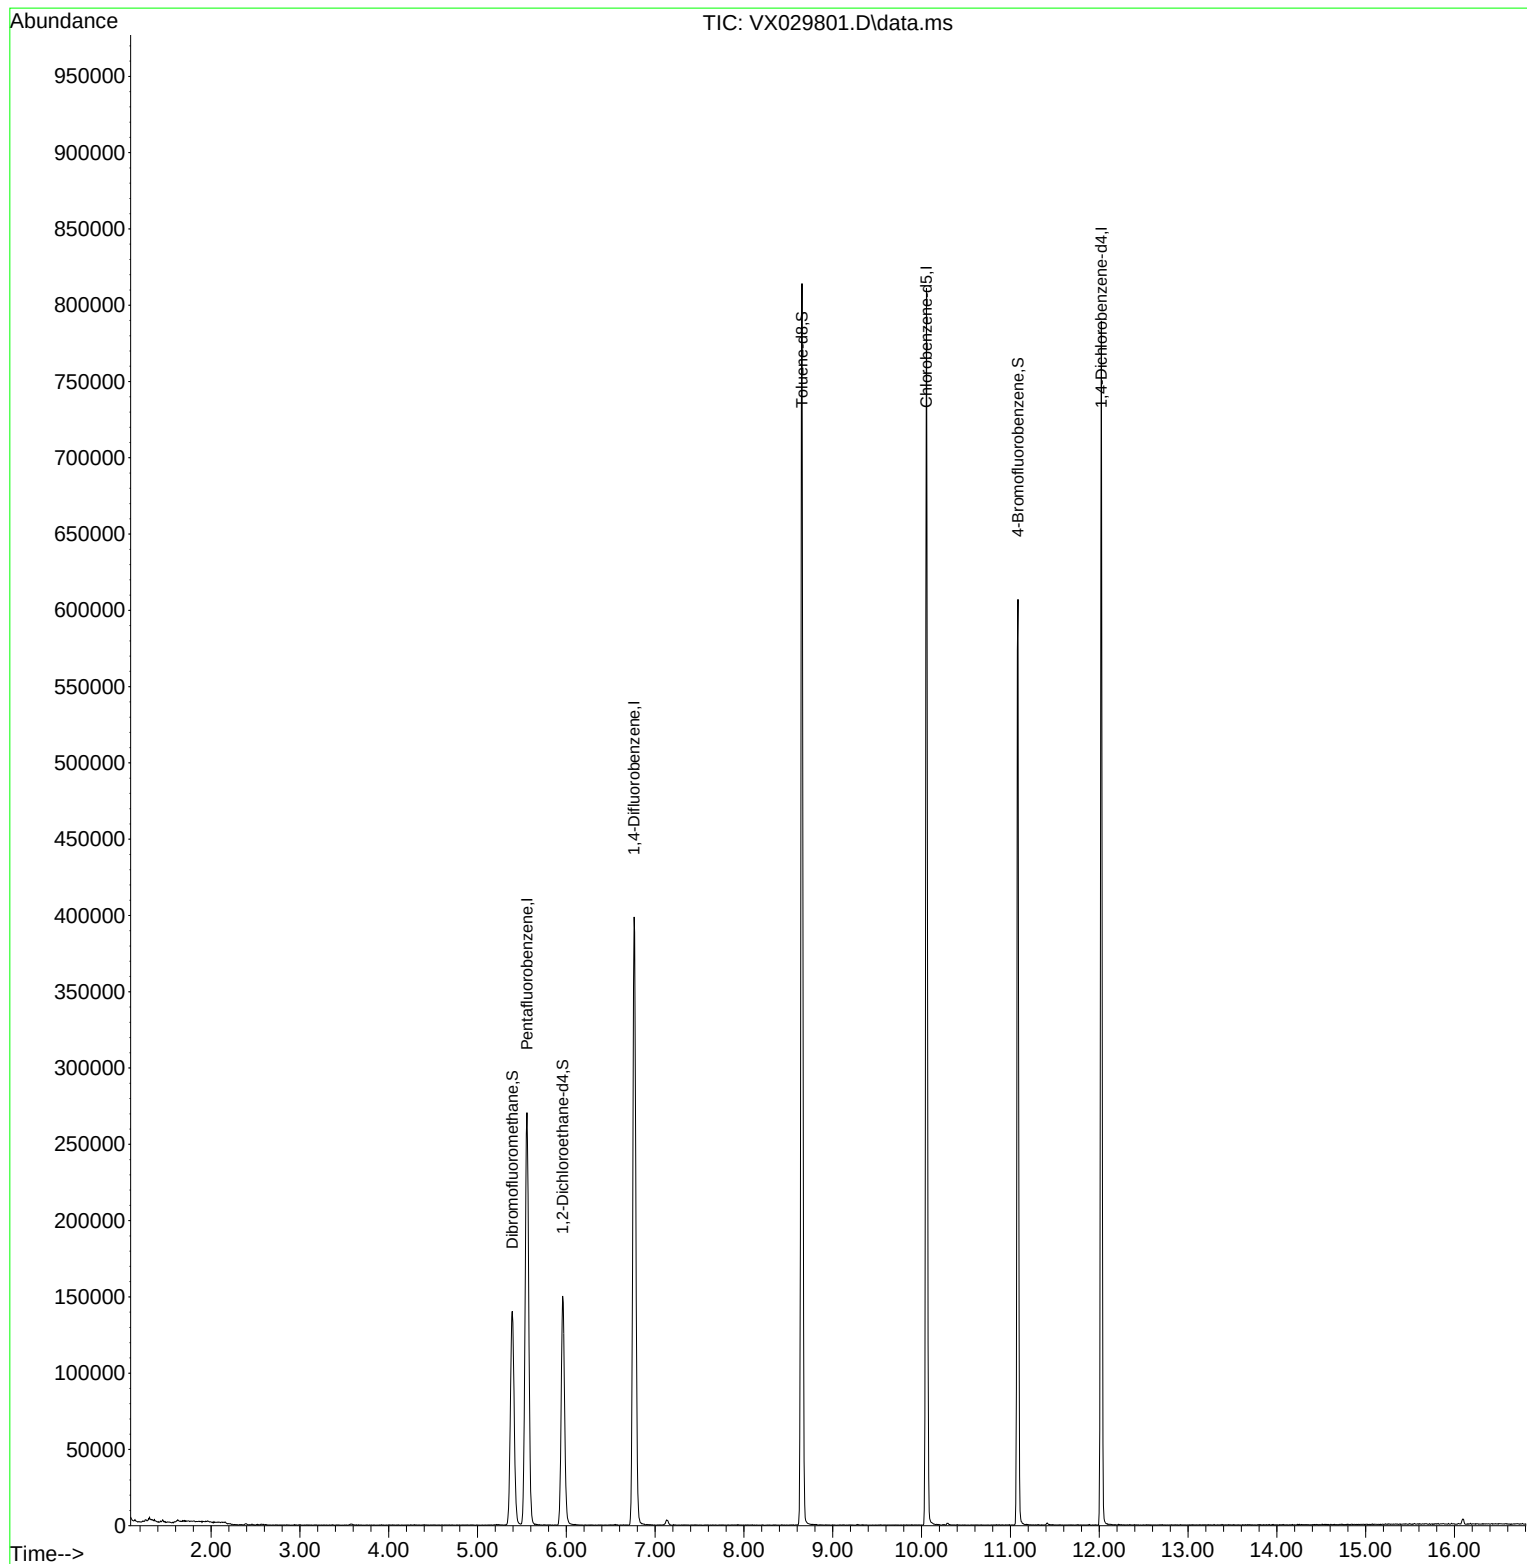


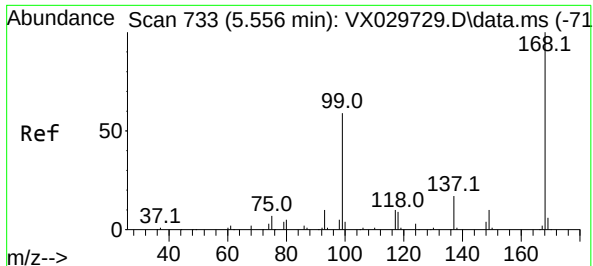

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 719
Delta R.T. -0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50




Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20220615


Tgt Ion:168 Resp: 262887
Ion Ratio Lower Upper
168 100
99 60.4 41.7 62.5

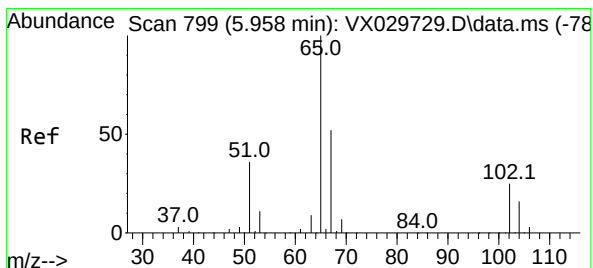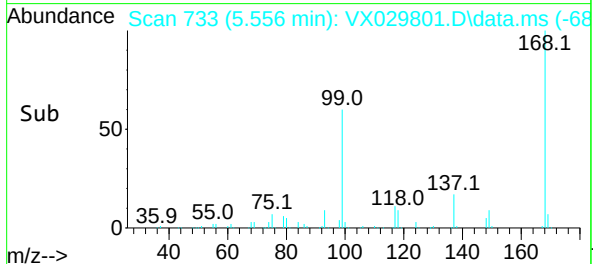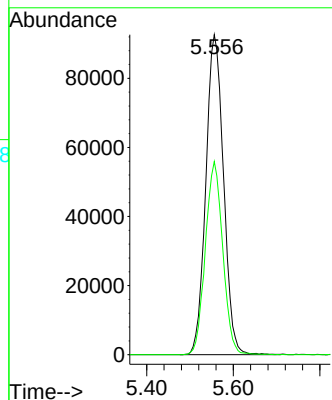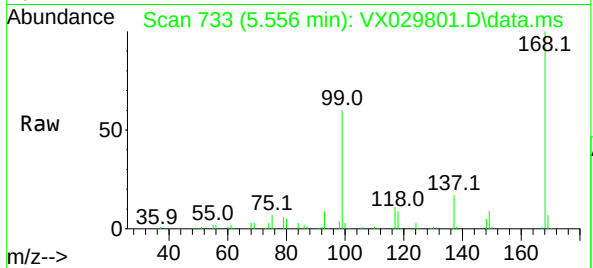

#33
1,2-Dichloroethane-d4
Concen: 40.693 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50

Tgt Ion: 65 Resp: 141607
Ion Ratio Lower Upper
65 100
67 53.0 0.0 107.4


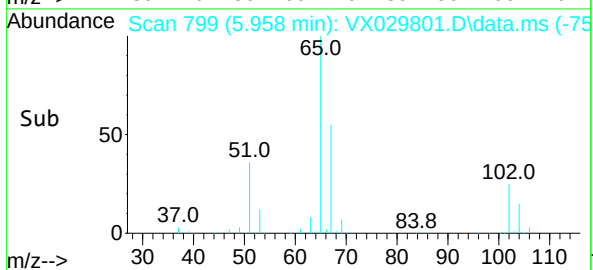
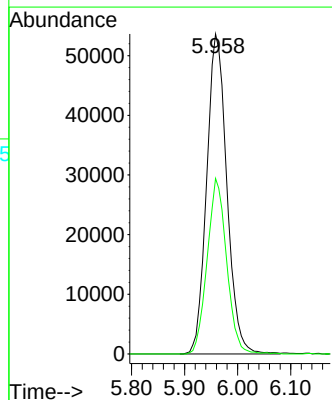
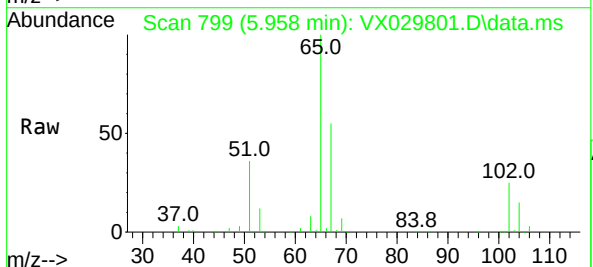


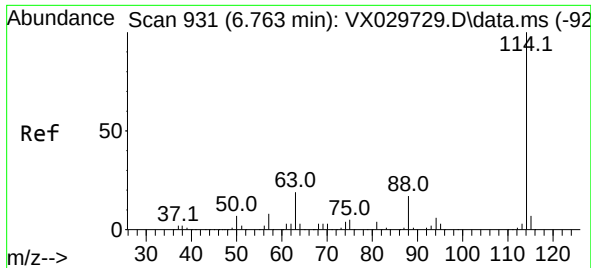

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50




Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20220615


Tgt Ion:114 Resp: 437159
Ion Ratio Lower Upper
114 100
63 17.8 0.0 36.8
88 16.4 0.0 32.4

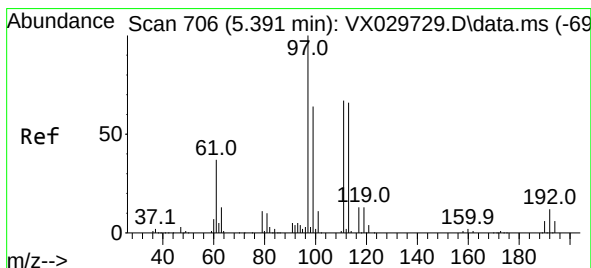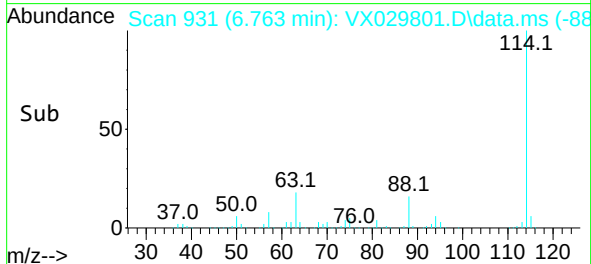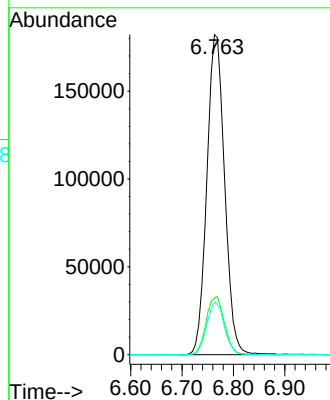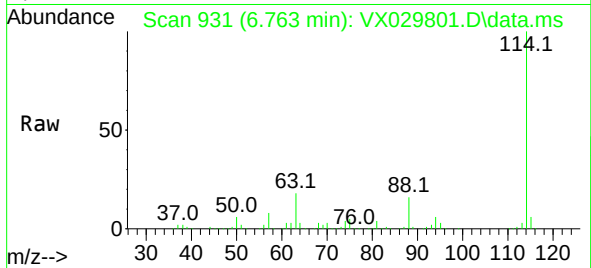

#35
Dibromofluoromethane
Concen: 44.963 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50

Tgt Ion:113 Resp: 128095
Ion Ratio Lower Upper
113 100
111 102.0 82.8 124.2
192 19.2 16.9 25.3


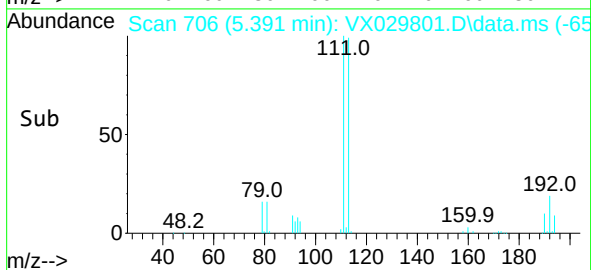
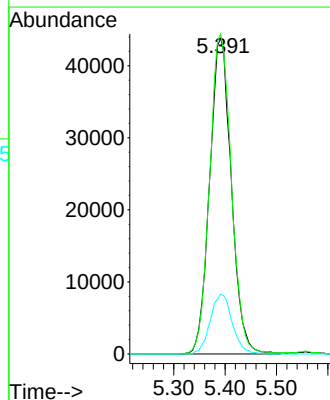
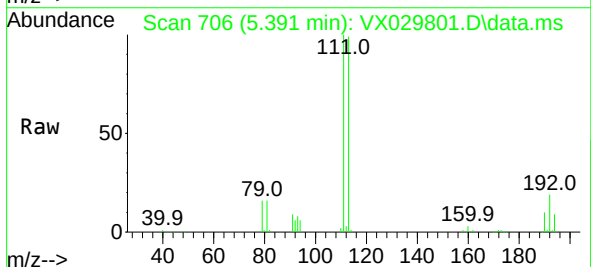


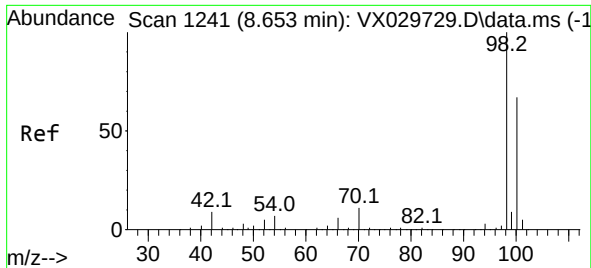

#50
Toluene-d8
Concen: 46.731 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50




Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20220615


Tgt Ion: 98 Resp: 486357
Ion Ratio Lower Upper
98 100
100 67.7 52.6 78.8

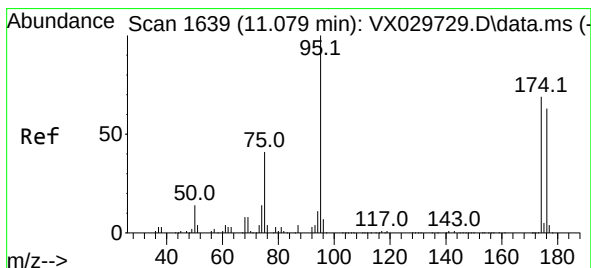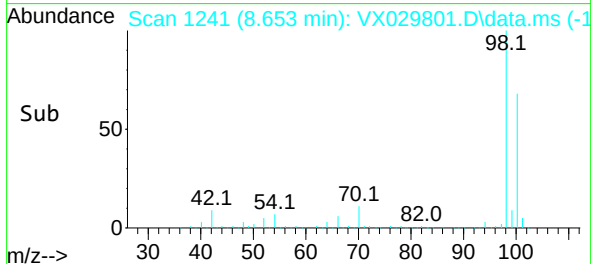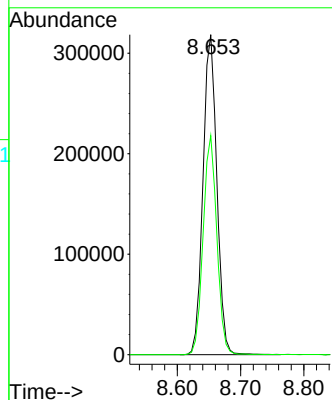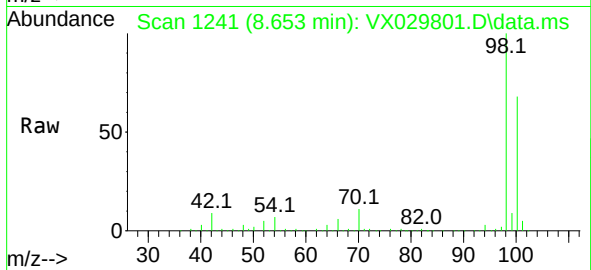

#62
4-Bromofluorobenzene
Concen: 44.242 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50

Tgt Ion: 95 Resp: 173644
Ion Ratio Lower Upper
95 100
174 76.0 0.0 163.0
176 72.3 0.0 155.0


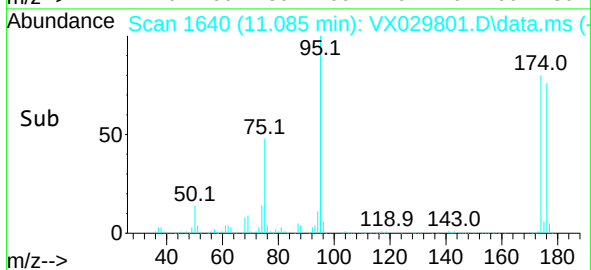
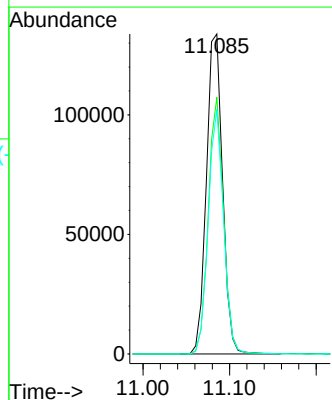
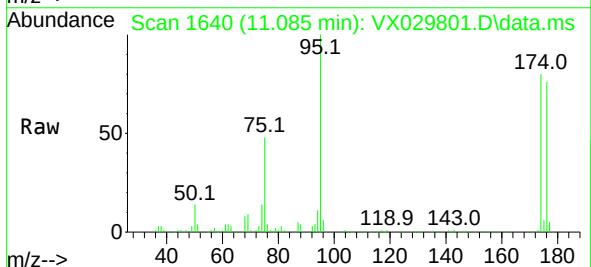


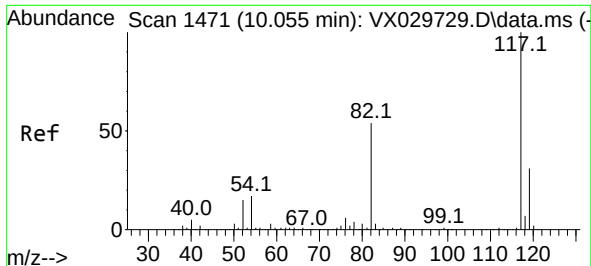

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20220615

Tgt Ion:117 Resp: 380006
Ion Ratio Lower Upper
117 100
82 54.5 41.8 62.8
119 32.1 24.8 37.2

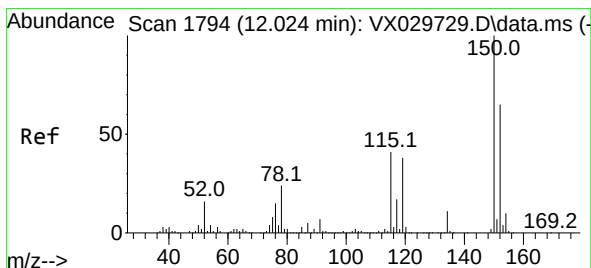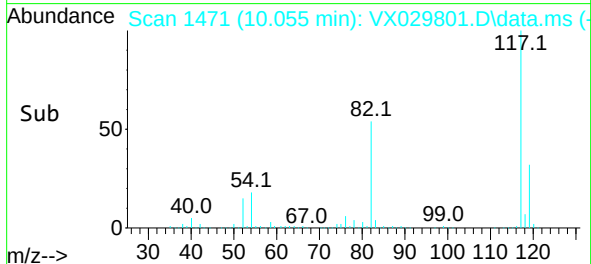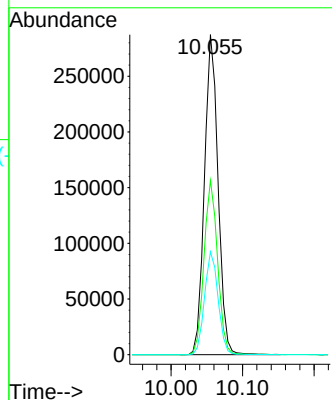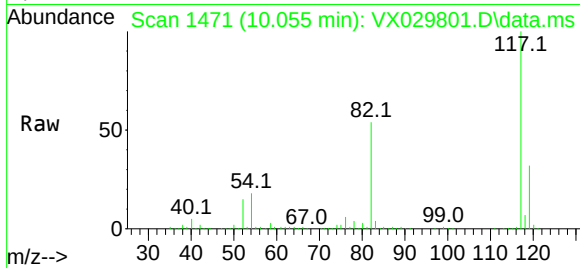

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029801.D
Acq: 25 Jun 2022 05:50

Tgt Ion:152 Resp: 162740
Ion Ratio Lower Upper
152 100
115 62.3 37.5 112.7
150 158.7 0.0 338.2

