

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029778.D
 Acq On : 24 Jun 2022 16:19
 Operator : JC/MD
 Sample : N3354-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-64

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	43	rBV	47398	175849	14.32%	2.593%
2	2.380	206	212	223	rBV	30579	50199	4.09%	0.740%
3	2.538	230	238	247	rBV2	14714	32663	2.66%	0.482%
4	5.391	694	706	721	rBV2	139353	408258	33.24%	6.019%
5	5.556	722	733	747	rVB	265148	753322	61.34%	11.107%
6	5.958	789	799	814	rBV	148009	392732	31.98%	5.790%
7	6.763	921	931	949	rBV	387405	938465	76.42%	13.836%
8	8.653	1234	1241	1249	rBV	810769	1228092	100.00%	18.106%
9	8.726	1249	1253	1260	rVB	11174	17307	1.41%	0.255%
10	10.055	1465	1471	1486	rBV	795539	1054384	85.86%	15.545%
11	11.085	1634	1640	1651	rBV	592997	774746	63.09%	11.422%
12	12.024	1789	1794	1804	rVB	768874	956649	77.90%	14.104%




Sum of corrected areas: 6782666

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029778.D
Acq On : 24 Jun 2022 16:19
Operator : JC/MD
Sample : N3354-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

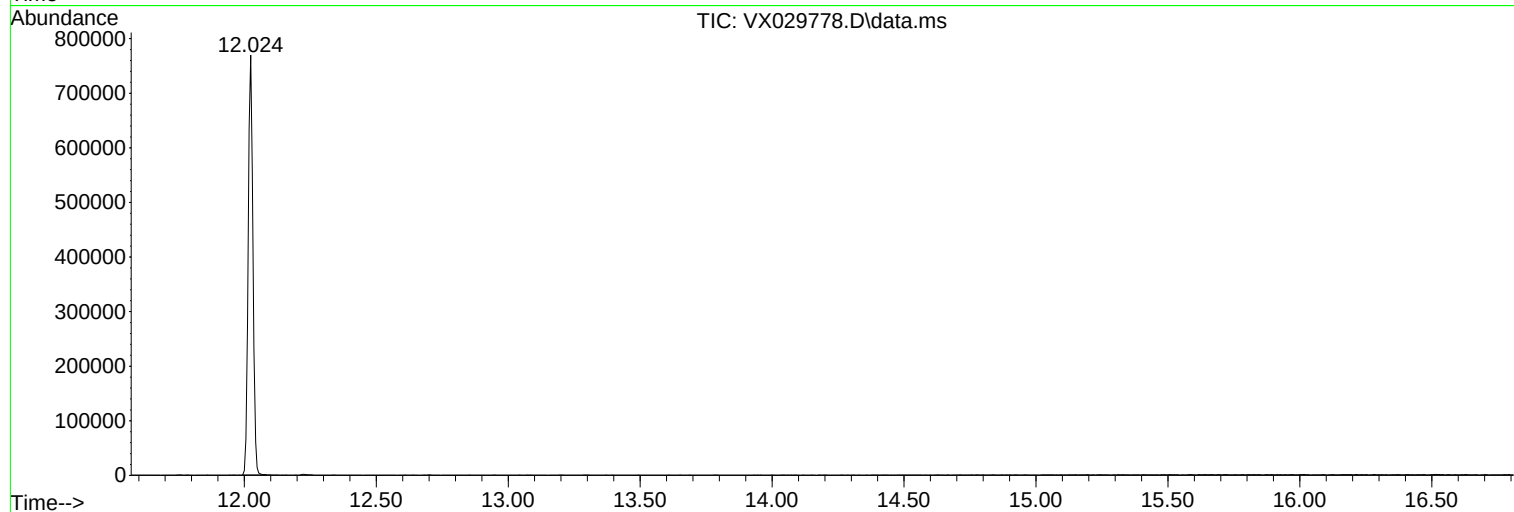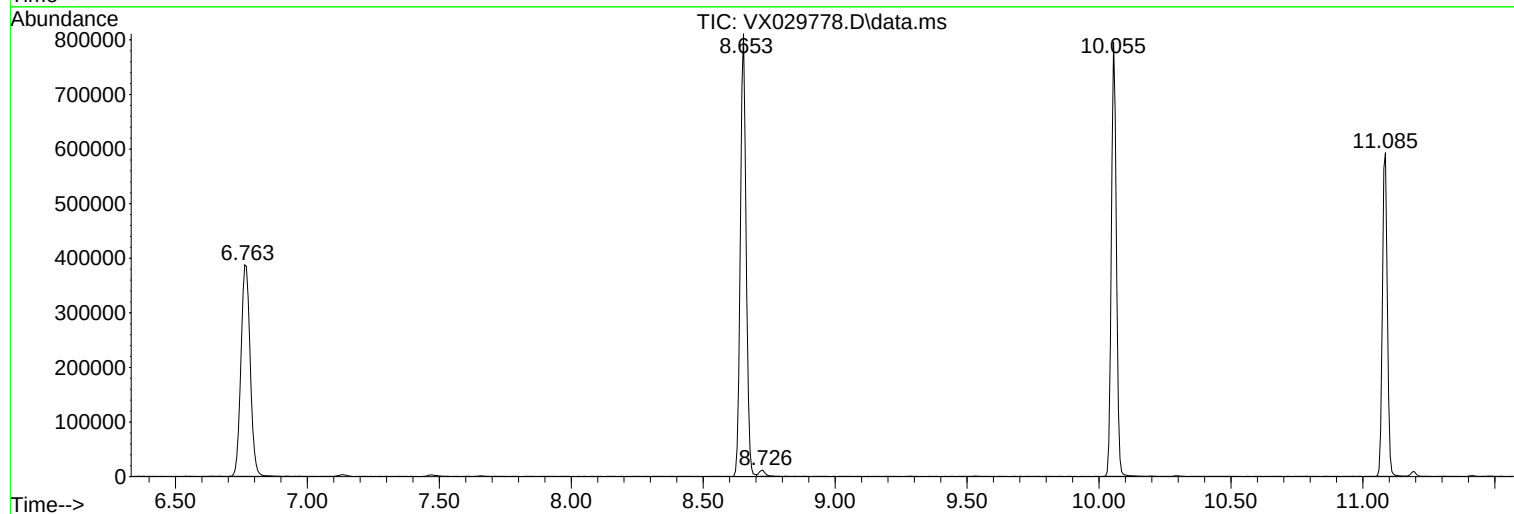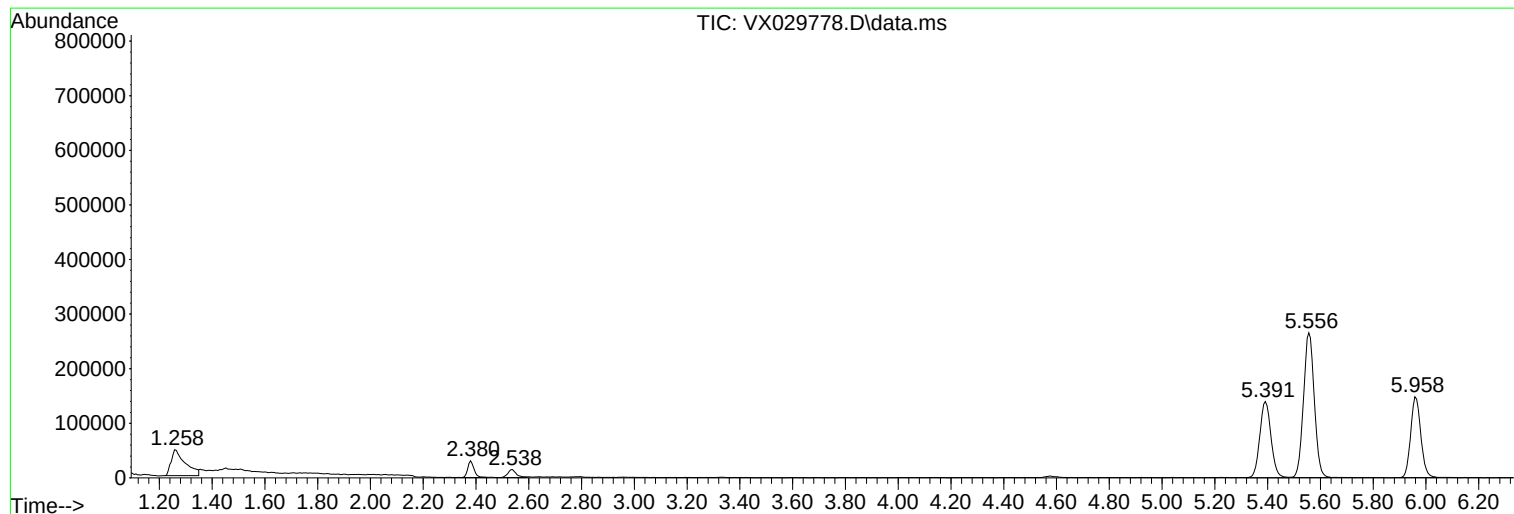

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029778.D
Acq On : 24 Jun 2022 16:19
Operator : JC/MD
Sample : N3354-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-64










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.258	11.67 ug/l	175849	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

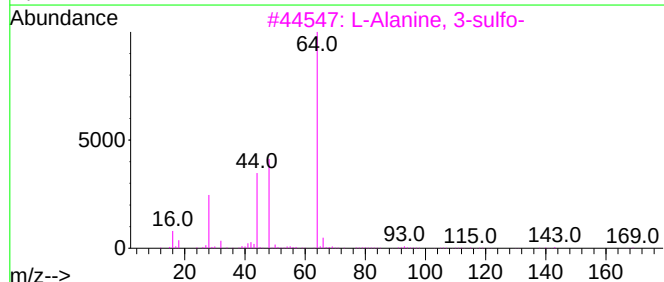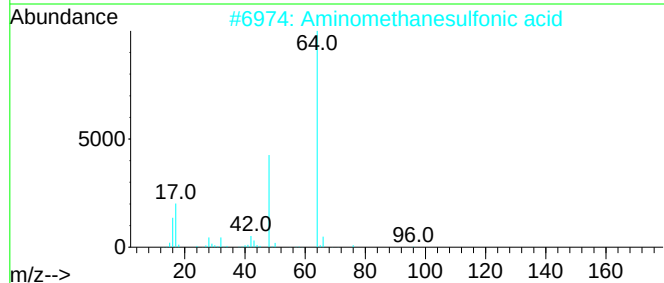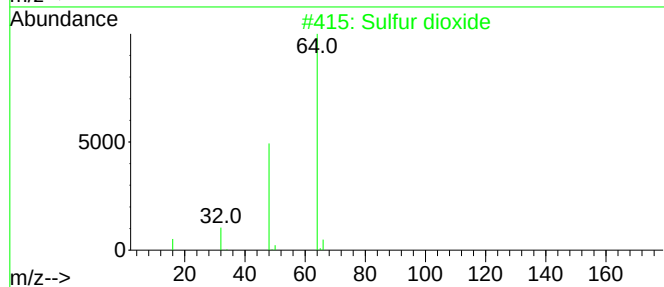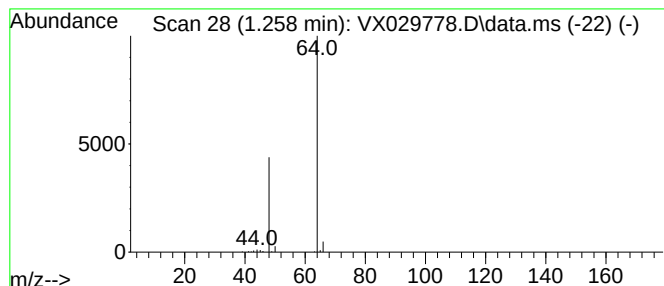

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029778.D
Acq On : 24 Jun 2022 16:19
Operator : JC/MD
Sample : N3354-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.258	11.7	ug/l	175849	1	5.556	753322	50.0