

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029779.D
 Acq On : 24 Jun 2022 16:43
 Operator : JC/MD
 Sample : N3202-06DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-28DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	38	rBV	93402	140874	1.29%	0.186%
2	2.959	298	307	321	rVB2	177016	398342	3.65%	0.525%
3	3.117	323	333	346	rVB	330247	762400	6.98%	1.005%
4	5.391	694	706	715	rBV	134490	393885	3.61%	0.519%
5	5.556	724	733	753	rVB2	251649	729948	6.68%	0.962%
6	5.958	789	799	805	rBV2	143895	372799	3.41%	0.491%
7	6.044	805	813	826	rVB	348131	912101	8.35%	1.202%
8	6.233	827	844	855	rBV3	255104	776176	7.11%	1.023%
9	6.763	922	931	944	rBV	376438	913709	8.37%	1.204%
10	8.427	1198	1204	1211	rVB	70776	120470	1.10%	0.159%
11	8.507	1211	1217	1224	rBV	126397	207125	1.90%	0.273%
12	8.653	1234	1241	1246	rBV	767409	1186790	10.87%	1.564%
13	8.720	1246	1252	1262	rVB	2730902	4218727	38.63%	5.558%
14	8.842	1268	1272	1282	rVB	138473	216580	1.98%	0.285%
15	9.458	1365	1373	1384	rVV2	278588	483379	4.43%	0.637%
16	10.055	1460	1471	1476	rBV	789939	1245898	11.41%	1.642%
17	10.147	1482	1486	1490	rVB	140032	161816	1.48%	0.213%
18	10.195	1490	1494	1500	rBV	547417	754415	6.91%	0.994%
19	10.305	1506	1512	1518	rVB	8108150	10920813	100.00%	14.389%
20	10.646	1562	1568	1578	rVB	7819515	10032659	91.87%	13.219%
21	10.793	1582	1592	1598	rBV3	57337	128954	1.18%	0.170%
22	11.085	1635	1640	1645	rBV	595726	764056	7.00%	1.007%
23	11.171	1649	1654	1660	rVB3	109709	186924	1.71%	0.246%
24	11.274	1667	1671	1674	rBV	86284	113761	1.04%	0.150%
25	11.384	1681	1689	1696	rBV	2866457	4685726	42.91%	6.174%
26	11.451	1696	1700	1706	rVB	3525992	4411466	40.40%	5.812%
27	11.616	1721	1727	1734	rBV	3209380	3931033	36.00%	5.179%
28	11.756	1745	1750	1755	rVB	4555993	5548194	50.80%	7.310%
29	11.976	1781	1786	1789	rBV	127925	159446	1.46%	0.210%
30	12.024	1789	1794	1799	rVB	778223	955638	8.75%	1.259%
31	12.091	1799	1805	1812	rBV	4153448	5234984	47.94%	6.897%
32	12.244	1824	1830	1838	rBV2	1844982	2579476	23.62%	3.399%
33	12.323	1838	1843	1849	rVV	855854	1078673	9.88%	1.421%
34	12.408	1853	1857	1862	rVV2	142140	190185	1.74%	0.251%
35	12.463	1862	1866	1871	rVB	216847	262718	2.41%	0.346%
36	12.530	1872	1877	1879	rBV	410120	507517	4.65%	0.669%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029779.D
 Acq On : 24 Jun 2022 16:43
 Operator : JC/MD
 Sample : N3202-06DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-28DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

37	12.555	1879	1881	1886	rVB	378094	413262	3.78%	0.545%
38	12.616	1886	1891	1894	rBV	994191	1176296	10.77%	1.550%
39	12.646	1894	1896	1900	rVV	137393	152007	1.39%	0.200%
40	12.701	1900	1905	1912	rVB2	634776	894670	8.19%	1.179%
41	12.847	1925	1929	1935	rVB	354334	437099	4.00%	0.576%
42	12.920	1935	1941	1945	rBV	696509	889623	8.15%	1.172%
43	12.963	1945	1948	1954	rVB	1109723	1272024	11.65%	1.676%
44	13.048	1954	1962	1964	rBV3	64609	119712	1.10%	0.158%
45	13.170	1978	1982	1986	rVB	408084	450474	4.12%	0.594%
46	13.292	1997	2002	2007	rVB2	1409396	1859223	17.02%	2.450%
47	13.347	2007	2011	2019	rVB4	83642	148315	1.36%	0.195%
48	13.426	2019	2024	2030	rVB	225808	287941	2.64%	0.379%
49	13.548	2040	2044	2046	rVV	121604	162369	1.49%	0.214%
50	13.585	2046	2050	2056	rVV2	151258	275544	2.52%	0.363%
51	13.646	2056	2060	2061	rVV	83219	112499	1.03%	0.148%
52	13.664	2061	2063	2068	rVB2	159327	207680	1.90%	0.274%
53	13.774	2075	2081	2088	rBV	468411	625135	5.72%	0.824%
54	14.079	2126	2131	2135	rBV	95371	123750	1.13%	0.163%
55	14.213	2148	2153	2159	rBV	92748	153694	1.41%	0.203%
56	14.640	2219	2223	2228	rVB	186728	230116	2.11%	0.303%
57	14.780	2240	2246	2254	rBV	165915	217873	2.00%	0.287%




Sum of corrected areas: 75896963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029779.D
Acq On : 24 Jun 2022 16:43
Operator : JC/MD
Sample : N3202-06DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

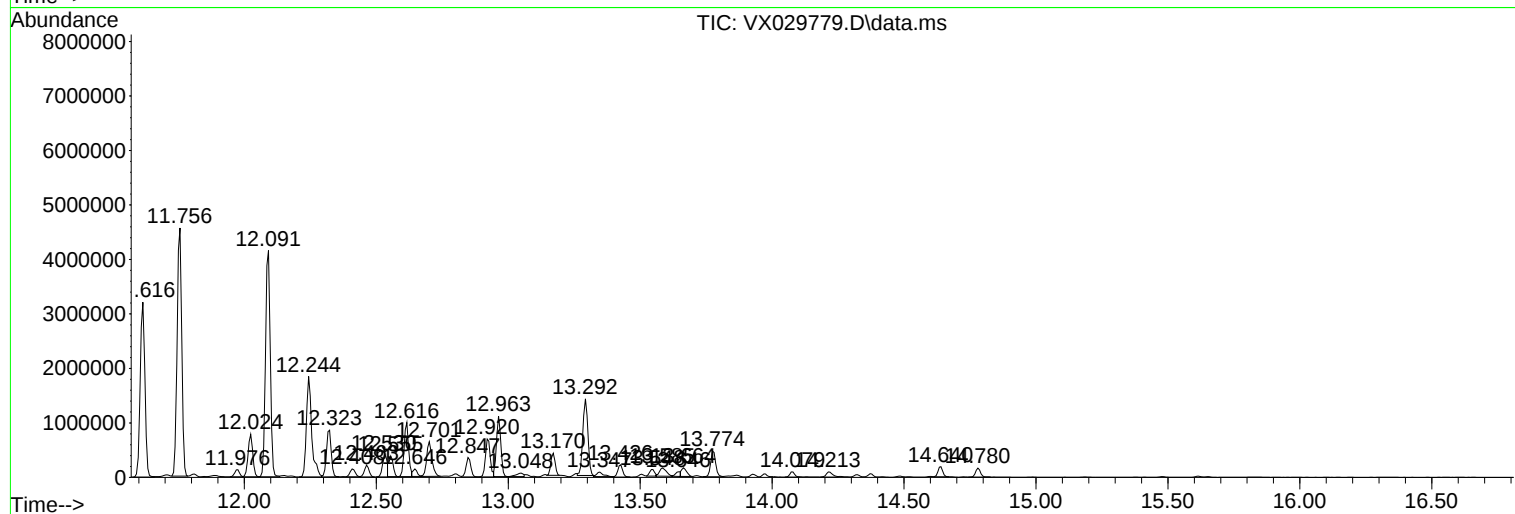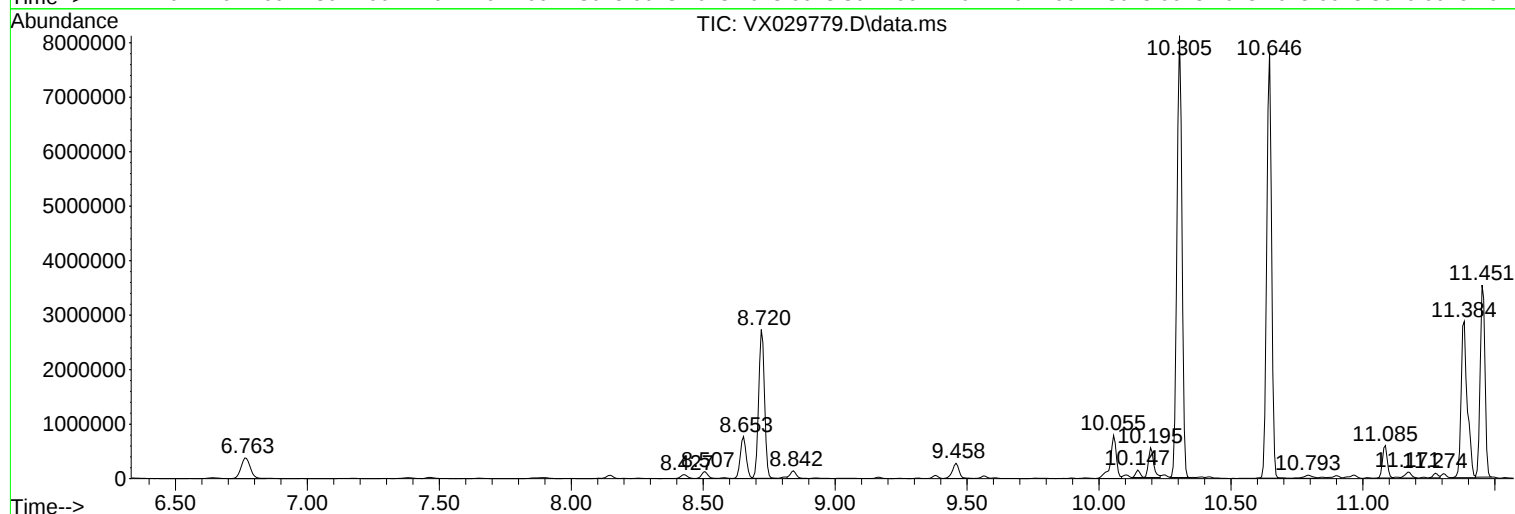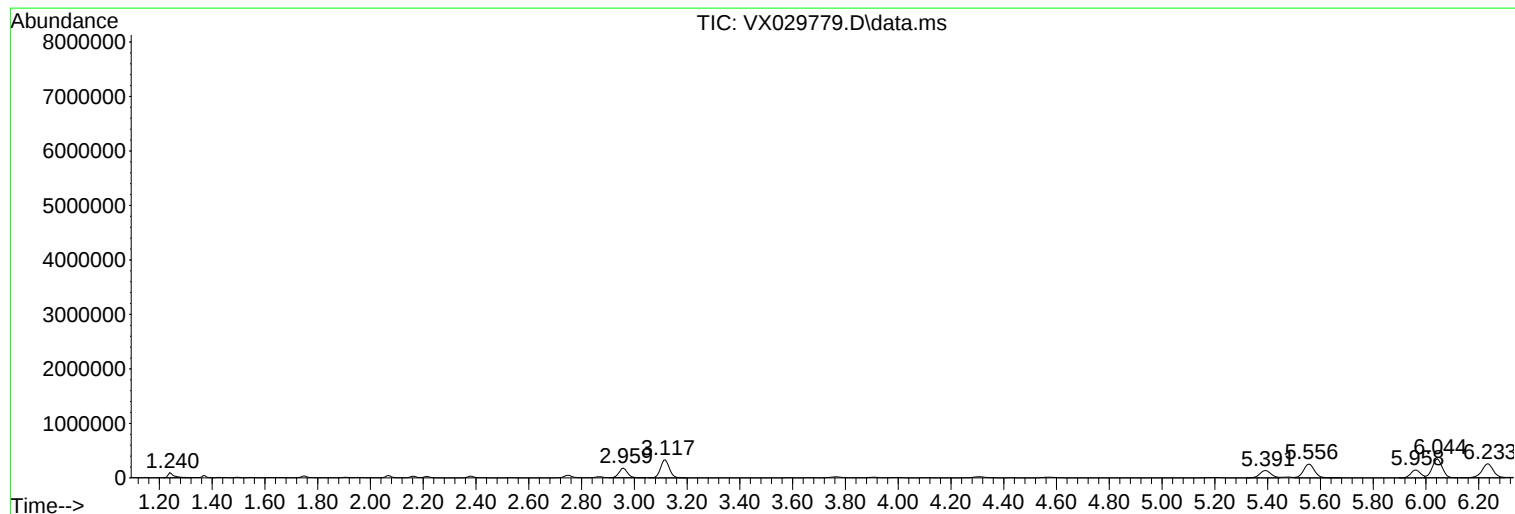

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029779.D
Acq On : 24 Jun 2022 16:43
Operator : JC/MD
Sample : N3202-06DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029779.D
Acq On : 24 Jun 2022 16:43
Operator : JC/MD
Sample : N3202-06DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------