

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029780.D
 Acq On : 24 Jun 2022 17:06
 Operator : JC/MD
 Sample : N3202-10DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-22DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	22	29	44	rBV	26067	79475	6.88%	1.103%
2	2.965	296	308	321	rBV3	40421	134477	11.64%	1.867%
3	3.117	323	333	348	rVB	141696	330633	28.62%	4.590%
4	4.580	563	573	586	rBV2	6226	20810	1.80%	0.289%
5	5.391	694	706	721	rBV	131204	382957	33.15%	5.316%
6	5.556	721	733	748	rVB	257256	712362	61.66%	9.889%
7	5.964	788	800	809	rBV	142878	383194	33.17%	5.320%
8	6.044	809	813	822	rVB3	8866	21628	1.87%	0.300%
9	6.251	837	847	857	rBV3	10767	30402	2.63%	0.422%
10	6.763	920	931	949	rBV	372126	896200	77.58%	12.441%
11	8.653	1234	1241	1249	rBV	751088	1155253	100.00%	16.038%
12	8.726	1249	1253	1263	rVB	9561	17376	1.50%	0.241%
13	8.848	1268	1273	1281	rVB	10369	16655	1.44%	0.231%
14	10.055	1466	1471	1478	rBV	728199	974068	84.32%	13.522%
15	10.195	1490	1494	1500	rBV	31888	42781	3.70%	0.594%
16	10.305	1507	1512	1518	rBV	88533	120899	10.47%	1.678%
17	10.646	1562	1568	1576	rBV	30254	41423	3.59%	0.575%
18	11.085	1634	1640	1650	rBV	569074	715651	61.95%	9.935%
19	11.384	1684	1689	1690	rBV	12053	14172	1.23%	0.197%
20	11.402	1690	1692	1697	rVV	12943	15376	1.33%	0.213%
21	11.457	1697	1701	1708	rVB	19251	25811	2.23%	0.358%
22	11.616	1722	1727	1732	rVB	21327	27927	2.42%	0.388%
23	11.756	1745	1750	1755	rBV	56820	69636	6.03%	0.967%
24	12.024	1789	1794	1801	rBV	719415	870231	75.33%	12.081%
25	12.091	1801	1805	1812	rVB	30485	38532	3.34%	0.535%
26	12.244	1825	1830	1838	rVB	20354	27891	2.41%	0.387%
27	13.292	1994	2002	2009	rBV2	10486	14742	1.28%	0.205%
28	13.780	2077	2082	2088	rVB	16800	22780	1.97%	0.316%




Sum of corrected areas: 7203342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029780.D
Acq On : 24 Jun 2022 17:06
Operator : JC/MD
Sample : N3202-10DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

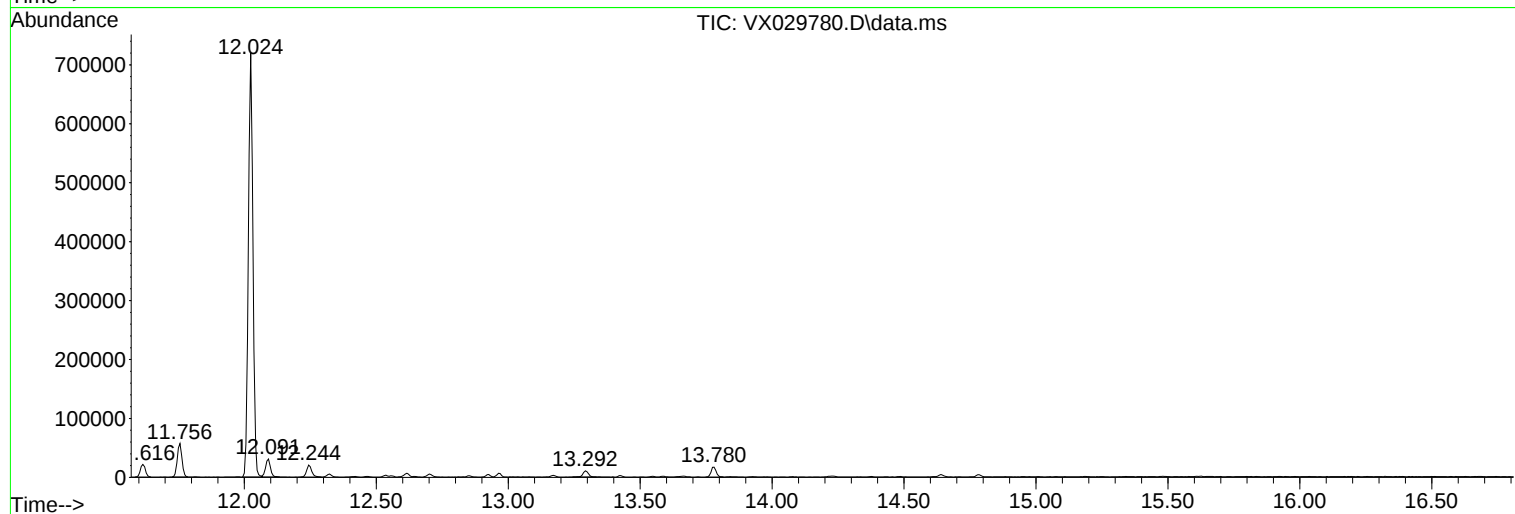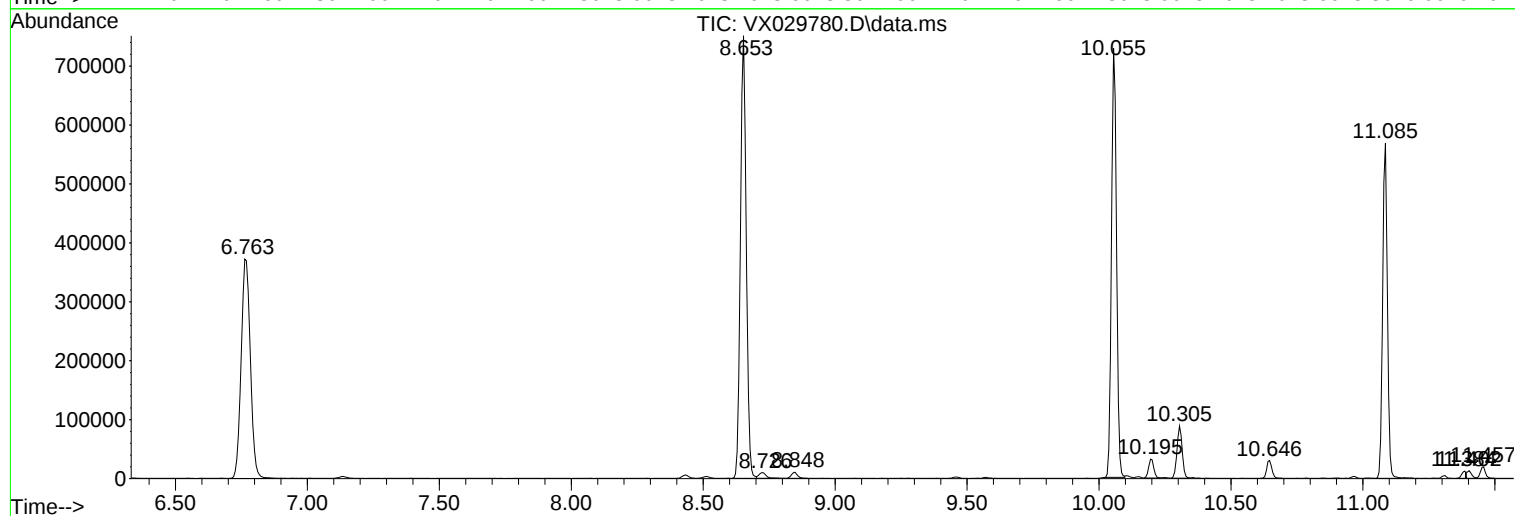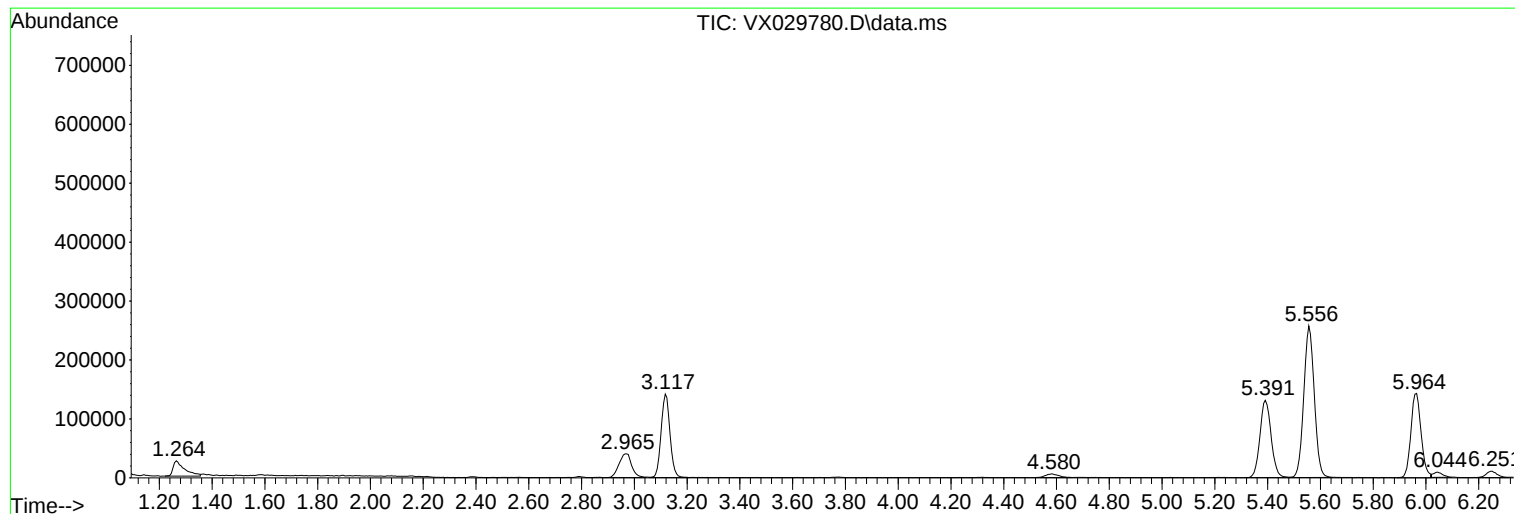

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029780.D
Acq On : 24 Jun 2022 17:06
Operator : JC/MD
Sample : N3202-10DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029780.D
Acq On : 24 Jun 2022 17:06
Operator : JC/MD
Sample : N3202-10DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------