

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029784.D
 Acq On : 24 Jun 2022 18:40
 Operator : JC/MD
 Sample : N3473-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-MW17411-TB-20220621

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	25	32	39	rBV4	7462	22109	1.96%	0.377%
2	2.105	159	167	179	rVB	7997	26866	2.38%	0.458%
3	2.386	207	213	223	rBV	38826	66814	5.93%	1.138%
4	5.391	695	706	720	rBV	128398	371892	32.99%	6.333%
5	5.556	722	733	749	rVB	246320	687551	60.98%	11.709%
6	5.964	790	800	814	rBV	132164	358858	31.83%	6.111%
7	6.763	921	931	945	rBV	355902	857828	76.09%	14.609%
8	8.653	1234	1241	1249	rBV	726350	1127434	100.00%	19.200%
9	10.055	1465	1471	1485	rBV	693827	938495	83.24%	15.982%
10	11.085	1634	1640	1655	rVB	519934	659527	58.50%	11.232%
11	12.024	1789	1794	1803	rBV	632194	754648	66.94%	12.852%




Sum of corrected areas: 5872022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029784.D
Acq On : 24 Jun 2022 18:40
Operator : JC/MD
Sample : N3473-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-MW17411-TB-20220621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

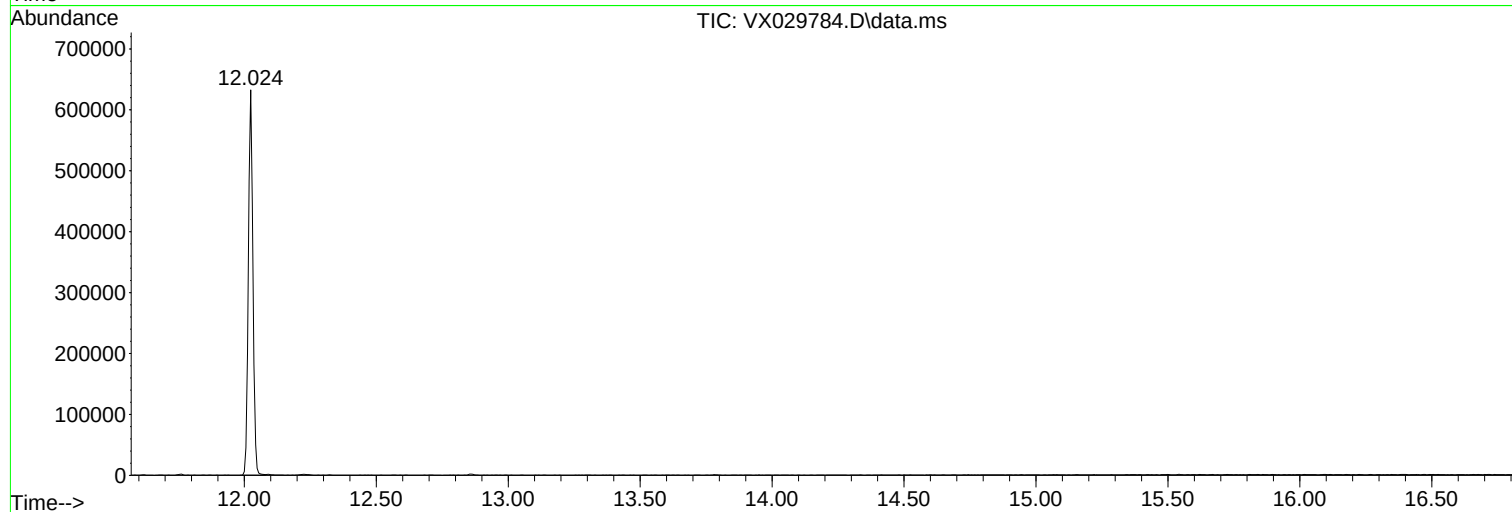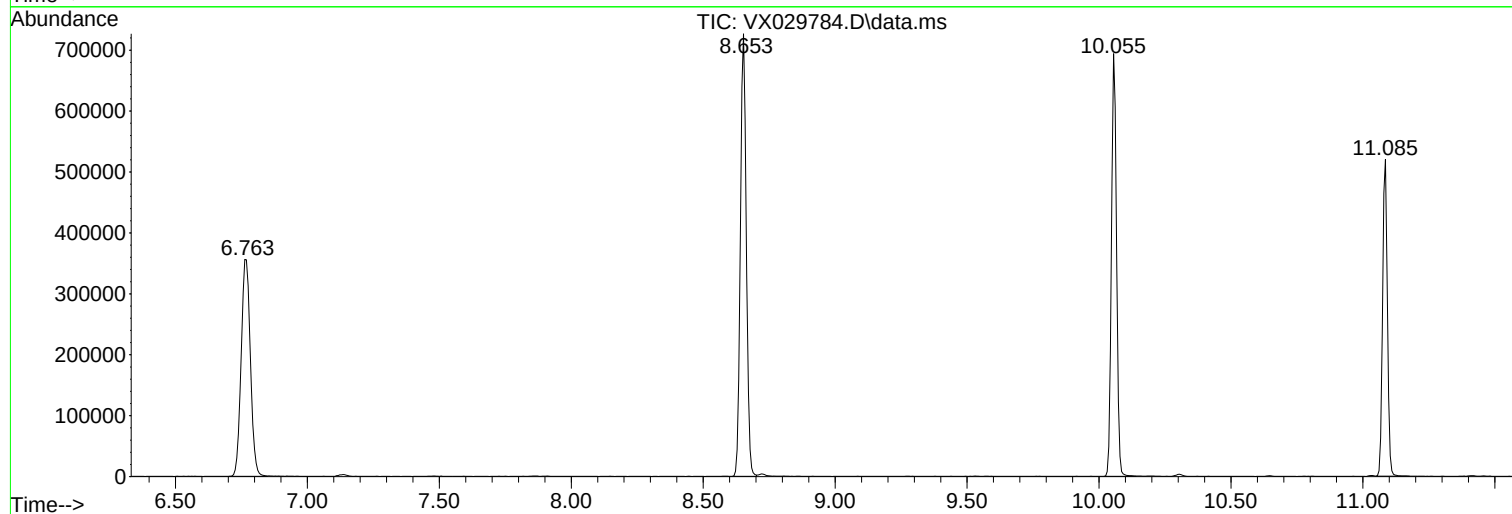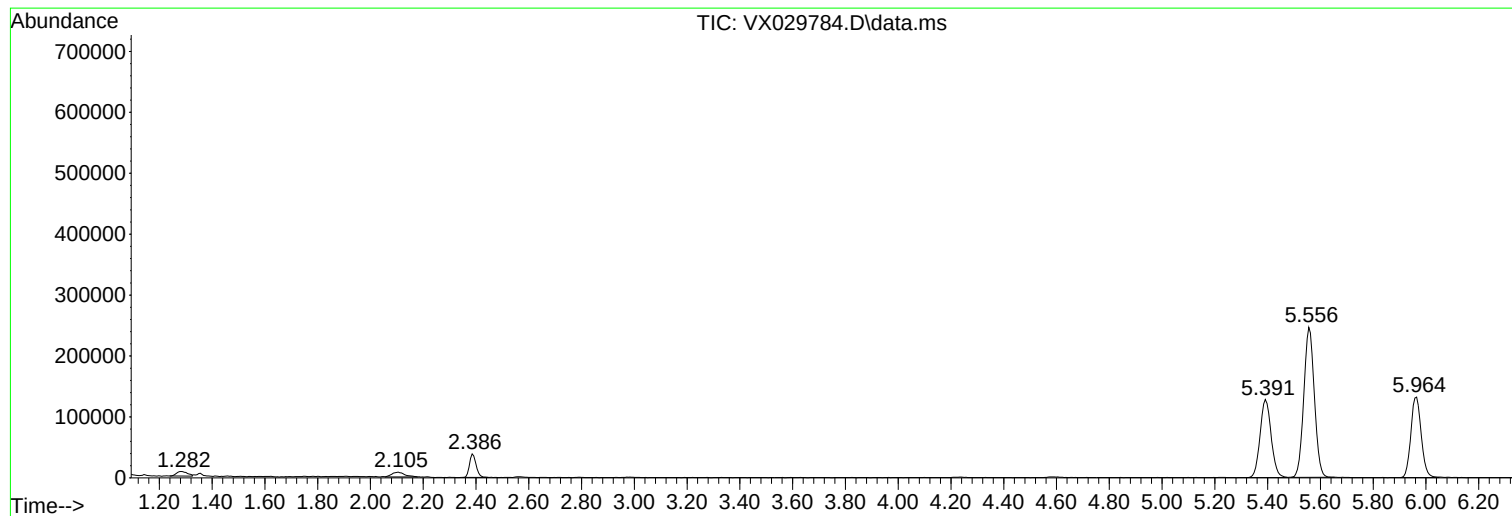

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029784.D
Acq On : 24 Jun 2022 18:40
Operator : JC/MD
Sample : N3473-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-MW17411-TB-20220621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029784.D
Acq On : 24 Jun 2022 18:40
Operator : JC/MD
Sample : N3473-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-MW17411-TB-20220621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------