

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029789.D
 Acq On : 25 Jun 2022 00:47
 Operator : JC/MD
 Sample : VX0624WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0624WBL02

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	27	34	43	rBV7	4154	10592	1.06%	0.205%
2	2.947	298	305	317	rVB2	13184	30878	3.08%	0.598%
3	4.580	563	573	584	rBV	4866	16017	1.60%	0.310%
4	5.391	693	706	719	rBV	114240	331220	33.08%	6.413%
5	5.556	722	733	748	rVB	185861	527107	52.65%	10.205%
6	5.958	789	799	811	rBV	114259	304609	30.42%	5.897%
7	6.763	921	931	945	rBV	311151	734281	73.34%	14.216%
8	8.653	1232	1241	1250	rBV	624038	1001202	100.00%	19.384%
9	10.055	1465	1471	1487	rBV	634599	844398	84.34%	16.348%
10	11.085	1634	1640	1649	rBV	475403	618558	61.78%	11.976%
11	12.024	1789	1794	1803	rBV	608508	746240	74.53%	14.448%




Sum of corrected areas: 5165102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029789.D
Acq On : 25 Jun 2022 00:47
Operator : JC/MD
Sample : VX0624WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0624WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

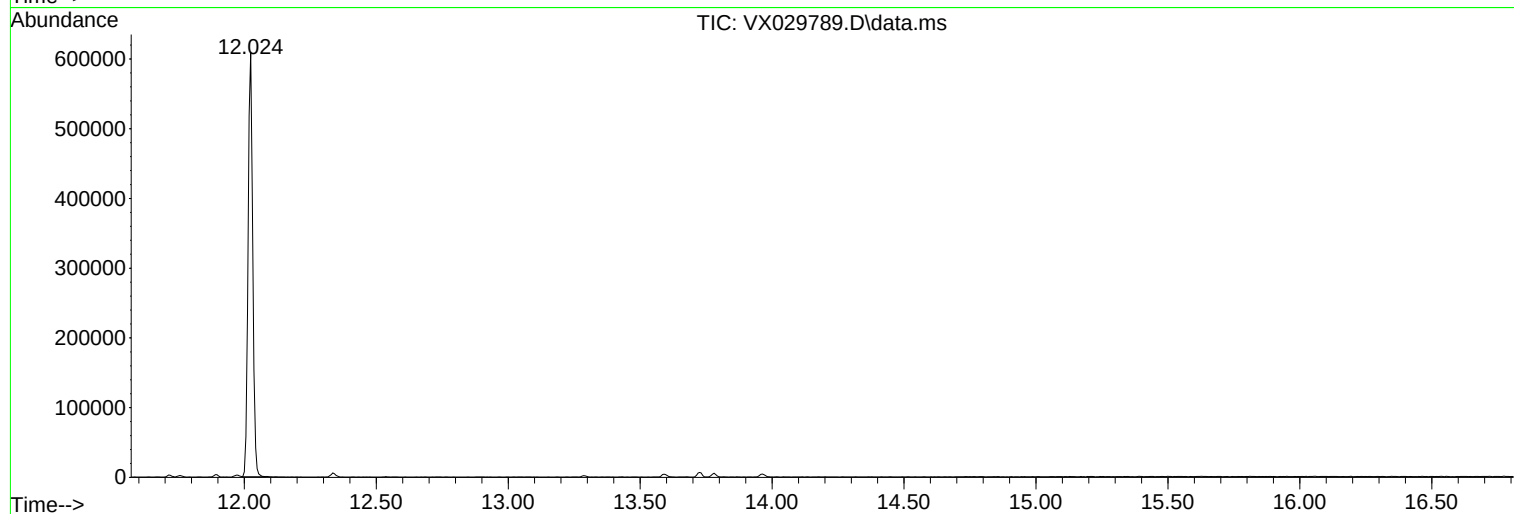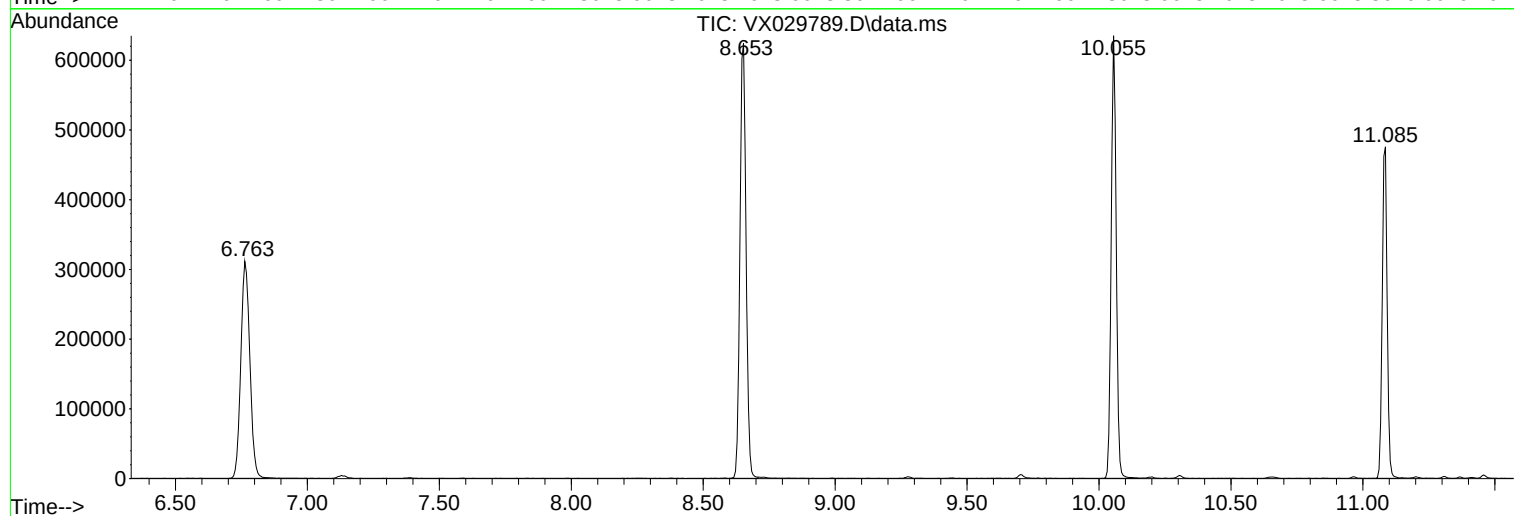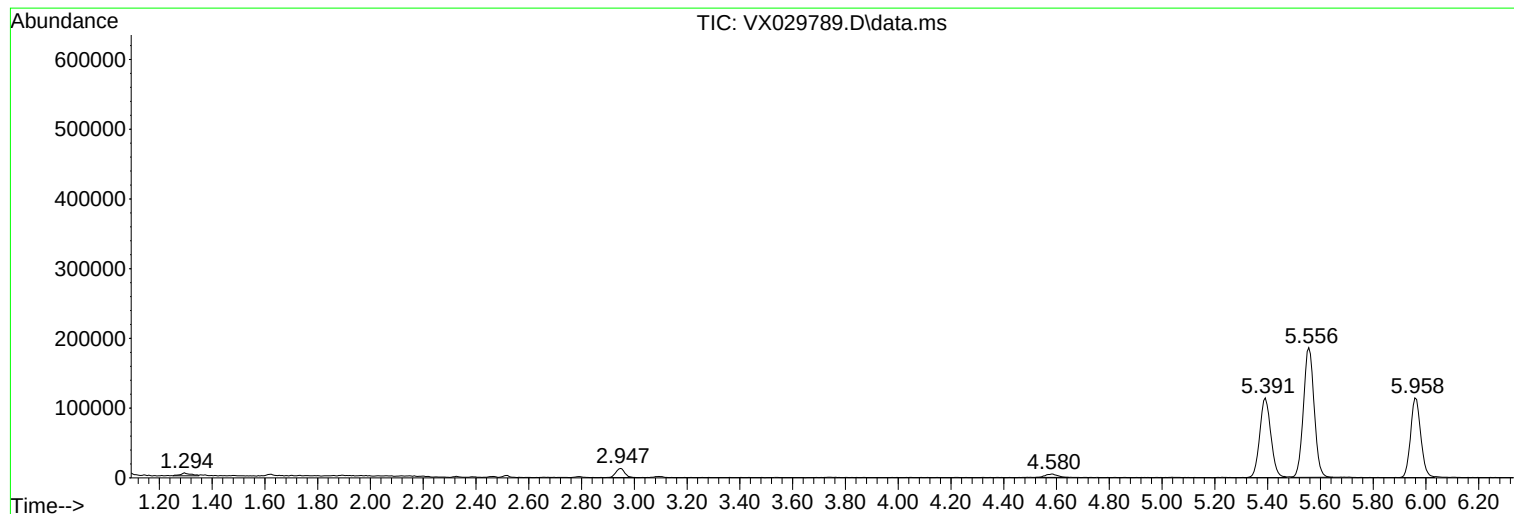

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029789.D
Acq On : 25 Jun 2022 00:47
Operator : JC/MD
Sample : VX0624WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0624WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029789.D
Acq On : 25 Jun 2022 00:47
Operator : JC/MD
Sample : VX0624WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0624WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------